

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
 Data File : PL075965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2022 03:50
 Operator : AR\AJ
 Sample : PB145757BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 05:22:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.636	10443102	25946073	13.808	13.680
28)	SA Decachlor...	11.634	10.376	8320303	17278865	13.222	11.250
Target Compounds							
5)	MB Aldrin	0.000	6.497	0	181089	N.D.	0.088 #
7)	B delta-BHC	7.122f	6.399	1038732	295634	1.330	0.131 #
10)	B gamma-Chl...	8.379	0.000	612749	0	0.788	N.D. #
11)	B alpha-Chl...	0.000	7.381f	0	343636	N.D.	0.180 #
13)	MA Dieldrin	0.000	7.723f	0	853689	N.D.	0.474 #
14)	MA Endrin	0.000	8.062f	0	2295646	N.D.	1.511 #
15)	B Endosulfa...	9.302	0.000	208355	0	0.328	N.D. #
17)	MA 4,4'-DDT	9.538f	0.000	1839511	0	3.013	N.D. #
21)	B Endrin ke...	10.184f	0.000	1181008	0	1.639	N.D. #
22)	Mirex	10.660f	0.000	390071	0	0.725	N.D. #
25)	Chlordane-3	8.379	0.000	612749	0	6.026	N.D. #
26)	Chlordane-4	0.000	7.381f	0	343636	N.D.	1.823 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
Data File : PL075965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2022 03:50
Operator : AR\AJ
Sample : PB145757BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 05:22:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

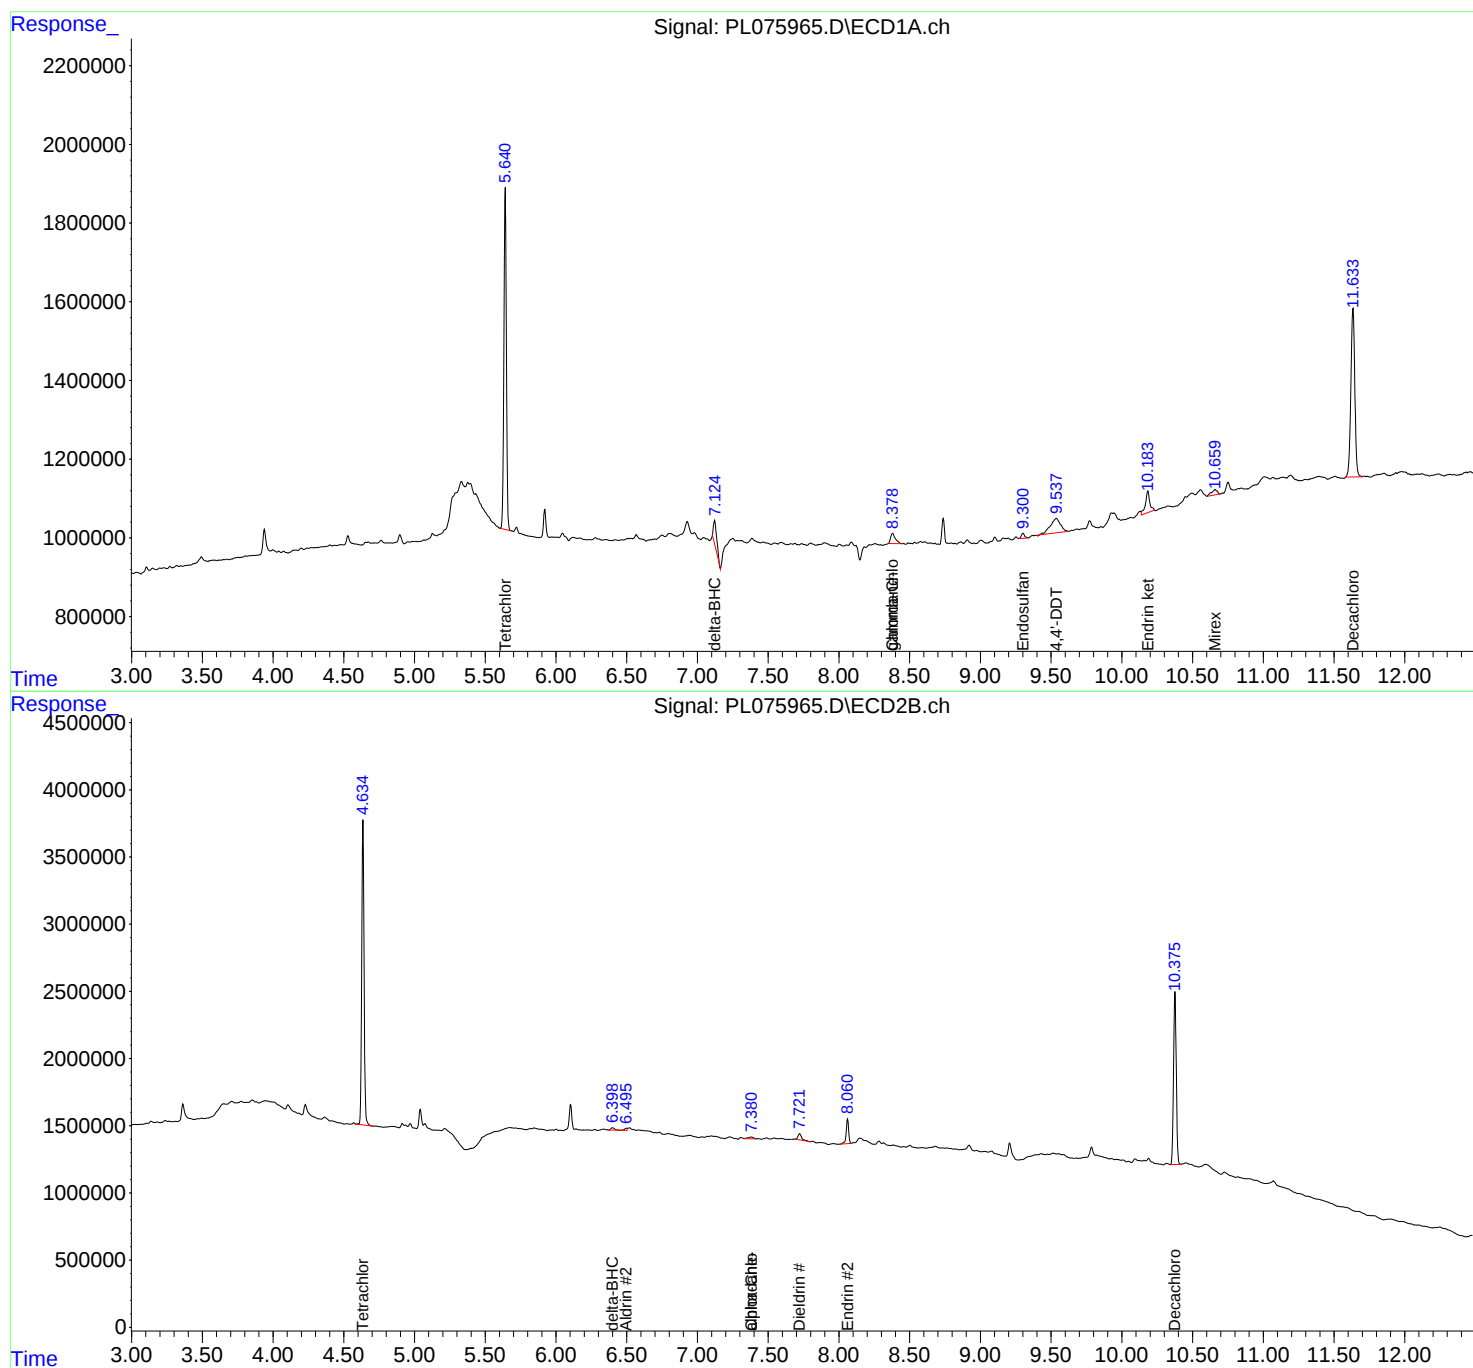


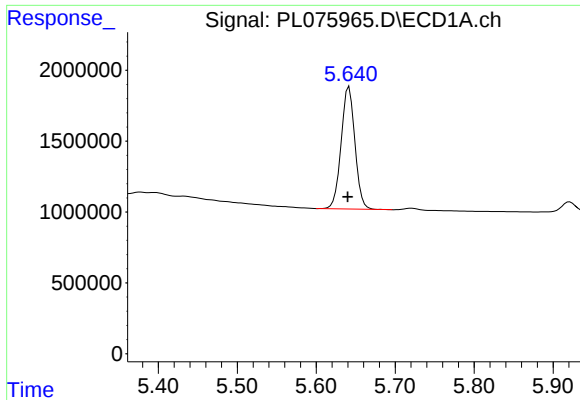

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.002 min
Response: 10443102
Conc: 13.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

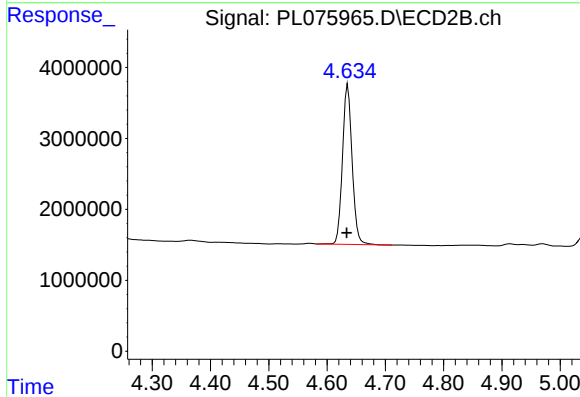


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: 0.002 min
Response: 25946073
Conc: 13.68 ng/ml

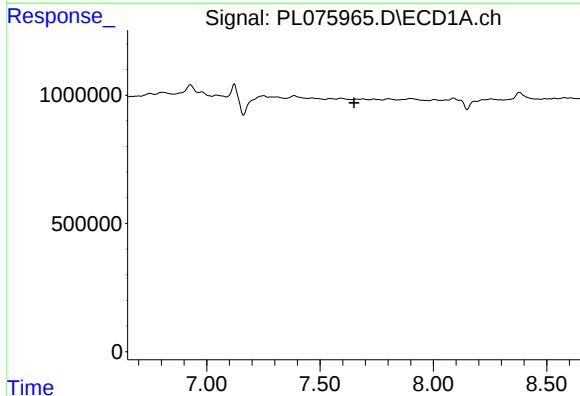


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.651 min
Response: 0
Conc: N.D.

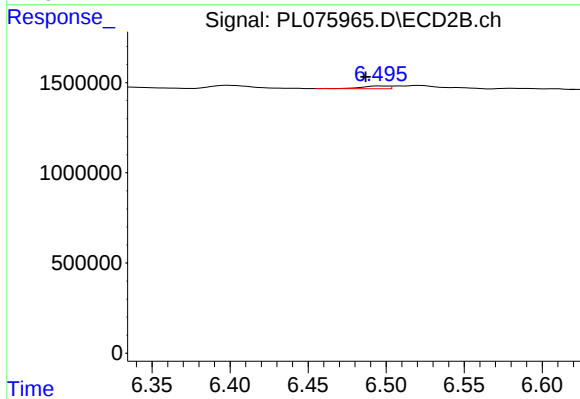

#5 Aldrin


R.T.: 6.497 min
Delta R.T.: 0.010 min
Response: 181089
Conc: 0.09 ng/ml

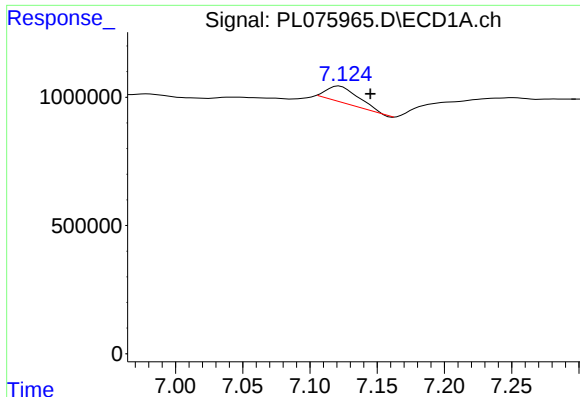

#7 delta-BHC


R.T.: 7.122 min
Delta R.T.: -0.023 min
Response: 1038732
Conc: 1.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

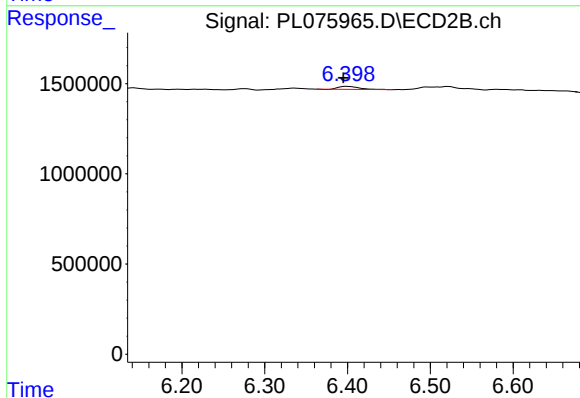


#7 delta-BHC

R.T.: 6.399 min
Delta R.T.: 0.004 min
Response: 295634
Conc: 0.13 ng/ml

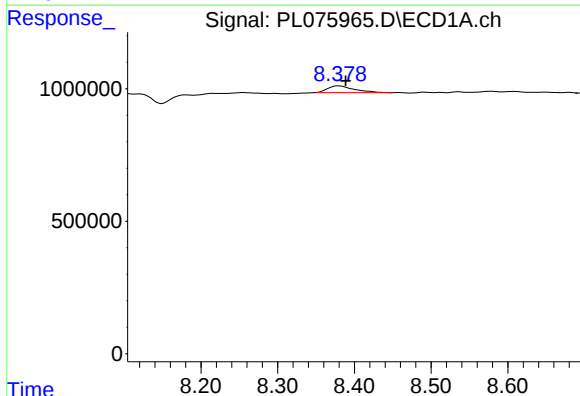


#10 gamma-Chlordane

R.T.: 8.379 min
Delta R.T.: -0.009 min
Response: 612749
Conc: 0.79 ng/ml

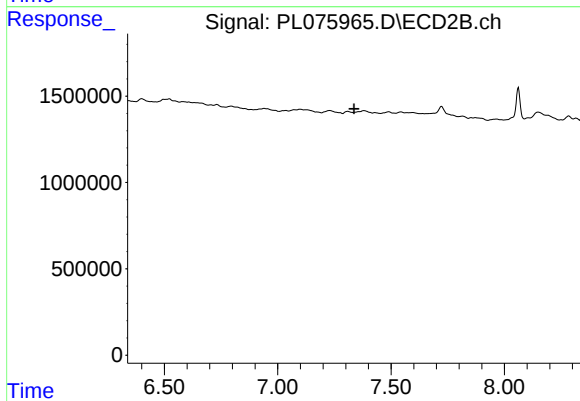

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.337 min
Response: 0
Conc: N.D.

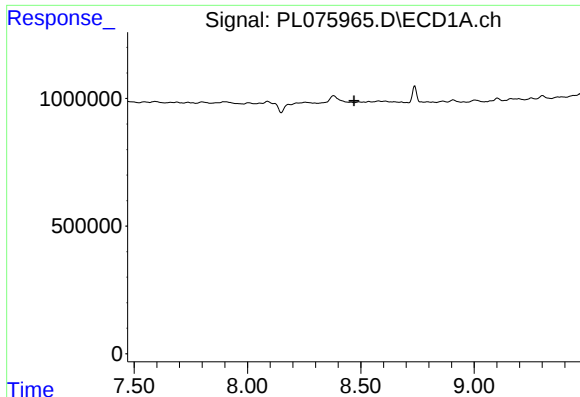

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

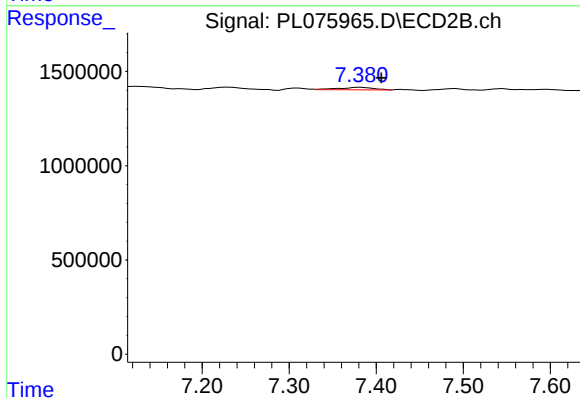


#11 alpha-Chlordane

R.T.: 7.381 min
Delta R.T.: -0.025 min
Response: 343636
Conc: 0.18 ng/ml

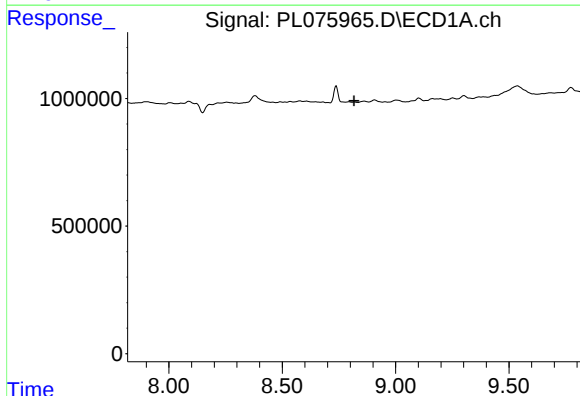


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.817 min
Response: 0
Conc: N.D.

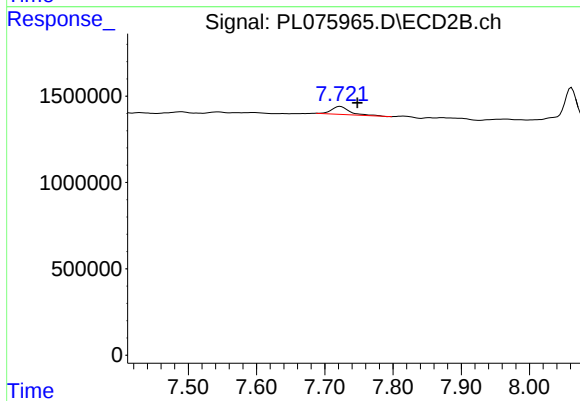

#13 Dieldrin


R.T.: 7.723 min
Delta R.T.: -0.025 min
Response: 853689
Conc: 0.47 ng/ml

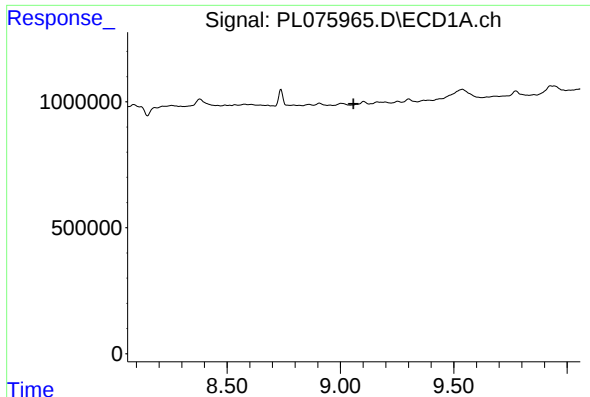

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

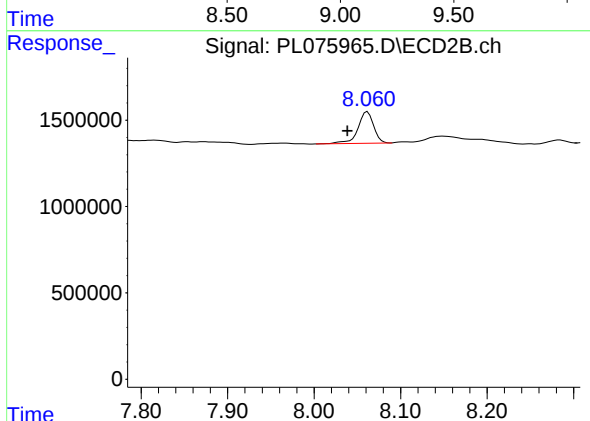


#14 Endrin

R.T.: 8.062 min
Delta R.T.: 0.023 min
Response: 2295646
Conc: 1.51 ng/ml

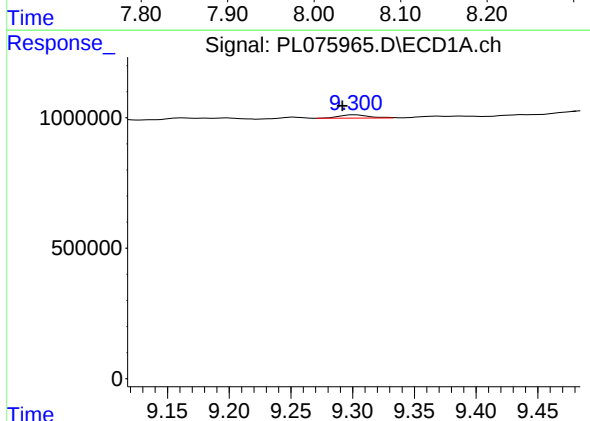


#15 Endosulfan II

R.T.: 9.302 min
Delta R.T.: 0.010 min
Response: 208355
Conc: 0.33 ng/ml

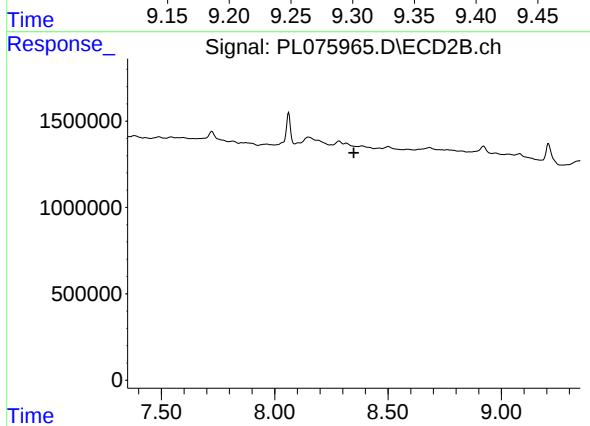

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.349 min
Response: 0
Conc: N.D.

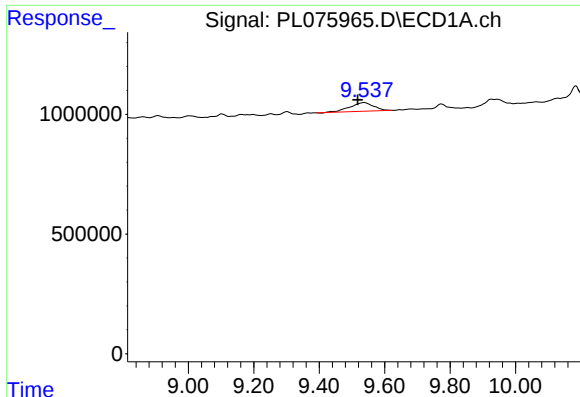

#17 4,4'-DDT


R.T.: 9.538 min
Delta R.T.: 0.020 min
Response: 1839511
Conc: 3.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

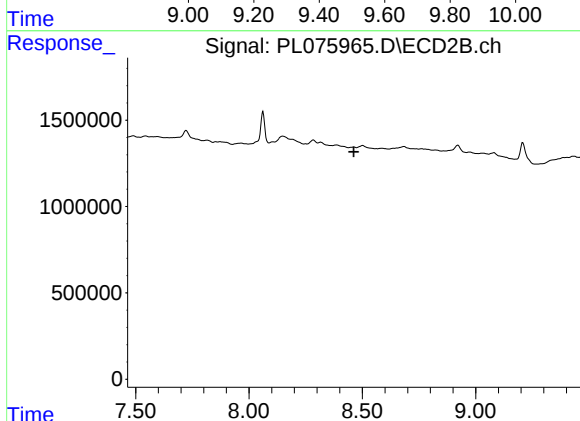


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.462 min
Response: 0
Conc: N.D.

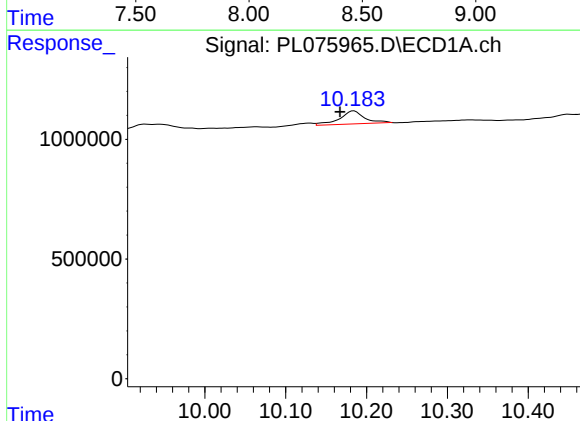


#21 Endrin ketone

R.T.: 10.184 min
Delta R.T.: 0.017 min
Response: 1181008
Conc: 1.64 ng/ml

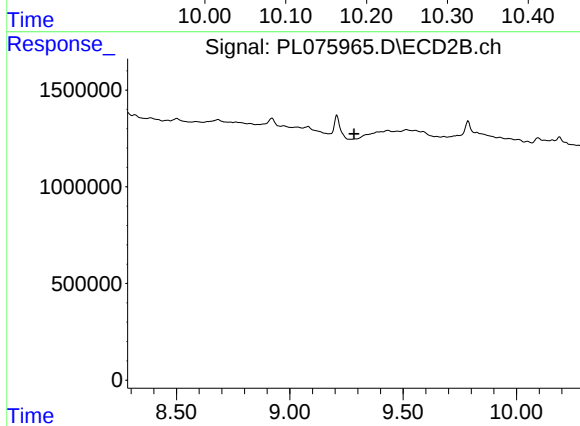

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

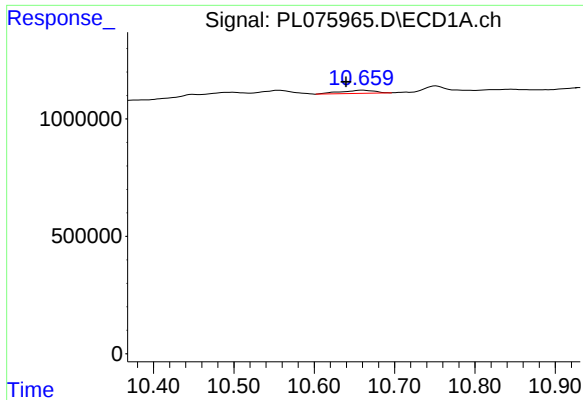

#22 Mirex


R.T.: 10.660 min
Delta R.T.: 0.021 min
Response: 390071
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

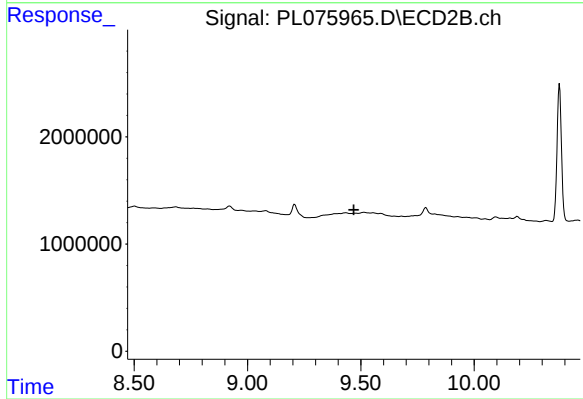


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.470 min
Response: 0
Conc: N.D.

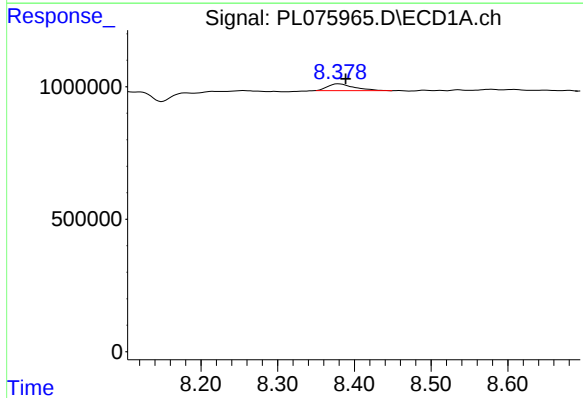


#25 Chlordane-3

R.T.: 8.379 min
Delta R.T.: -0.010 min
Response: 612749
Conc: 6.03 ng/ml

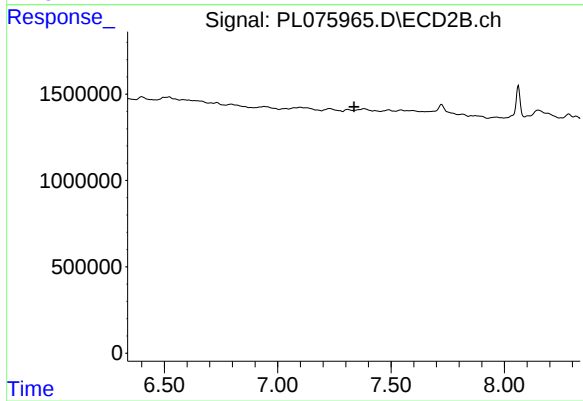

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.337 min
Response: 0
Conc: N.D.

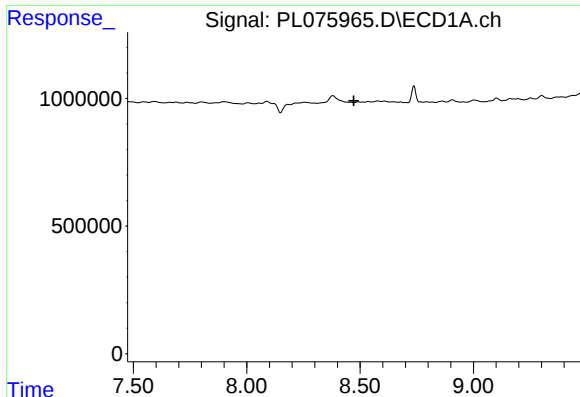

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

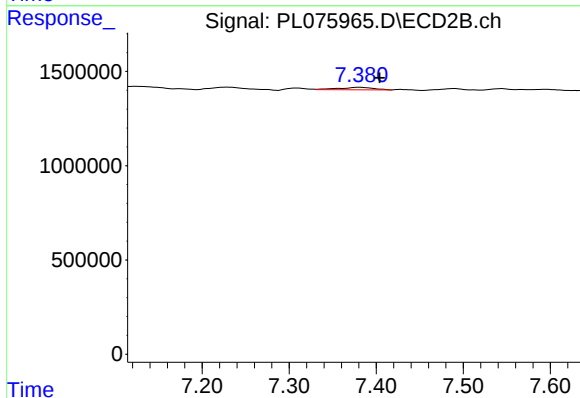


#26 Chlordane-4

R.T.: 7.381 min
Delta R.T.: -0.023 min
Response: 343636
Conc: 1.82 ng/ml

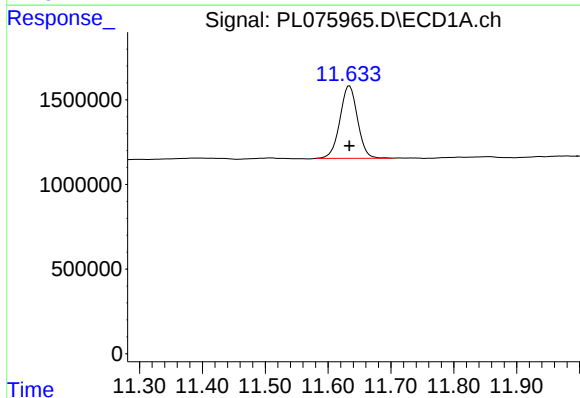

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: 0.000 min
Response: 8320303
Conc: 13.22 ng/ml

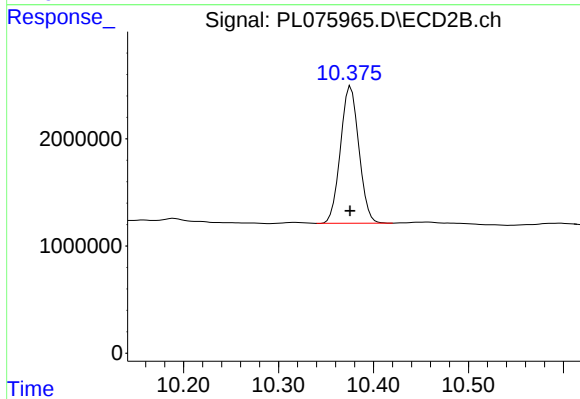

#28 Decachlorobiphenyl

R.T.: 10.376 min
Delta R.T.: 0.000 min
Response: 17278865
Conc: 11.25 ng/ml