

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
 Data File : PL075967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2022 04:23
 Operator : AR\AJ
 Sample : PB145718TB
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 05:23:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.636	13275296	32206698	17.552	16.981
28)	SA Decachlor...	11.634	10.376	10770476	22475490	17.116	14.634
Target Compounds							
7)	B delta-BHC	7.122f	6.399	1089603	217210	1.395	0.096 #
8)	B Heptachlo...	8.120	0.000	1830284	0	2.299	N.D. #
10)	B gamma-Chl...	8.380	7.311f	409725	268854	0.527	0.140 #
11)	B alpha-Chl...	0.000	7.384f	0	378813	N.D.	0.198 #
14)	MA Endrin	0.000	8.062f	0	33163718	N.D.	21.823 #
15)	B Endosulfa...	9.306	8.349	364968	668834	0.575	0.442
21)	B Endrin ke...	10.184f	0.000	692287	0	0.960	N.D. #
22)	Mirex	10.666f	0.000	660987	0	1.229	N.D. #
25)	Chlordane-3	8.380	7.311f	409725	268854	4.029	1.524 #
26)	Chlordane-4	0.000	7.384f	0	378813	N.D.	2.009 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
Data File : PL075967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2022 04:23
Operator : AR\AJ
Sample : PB145718TB
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 05:23:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

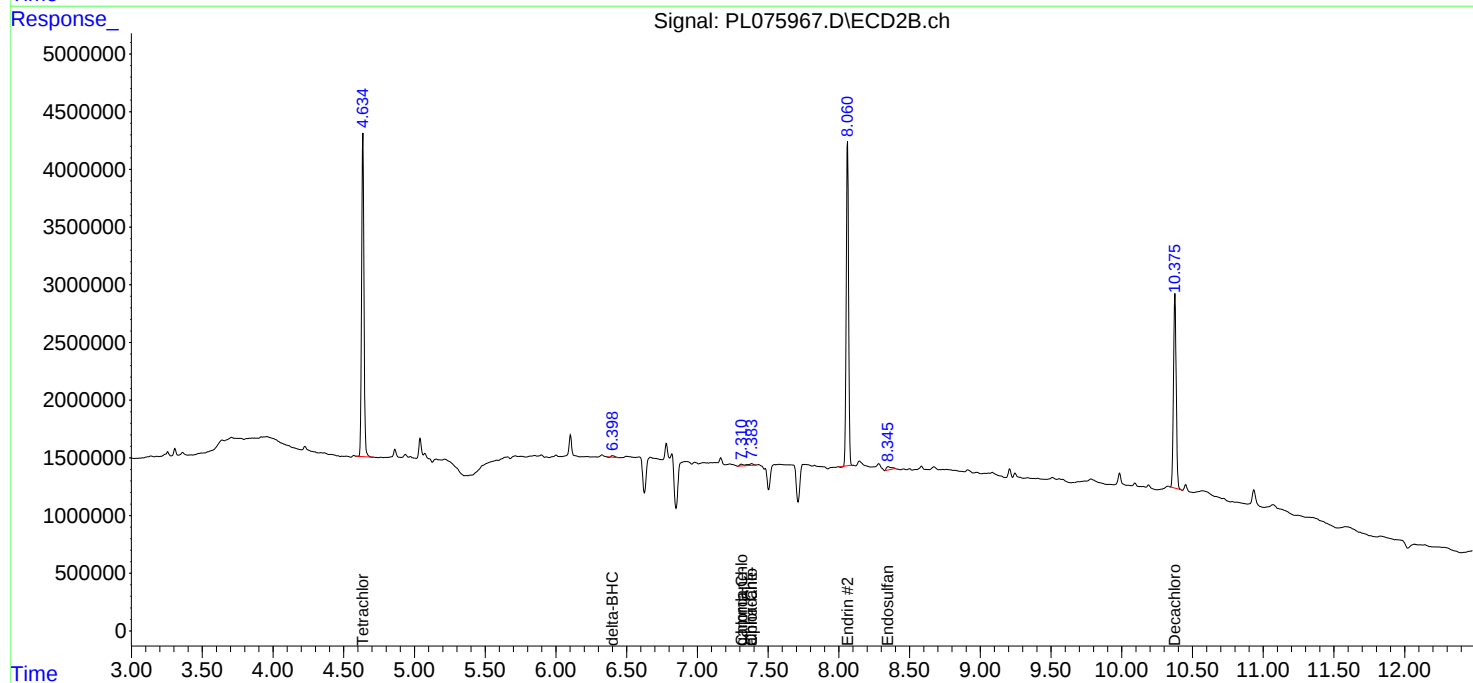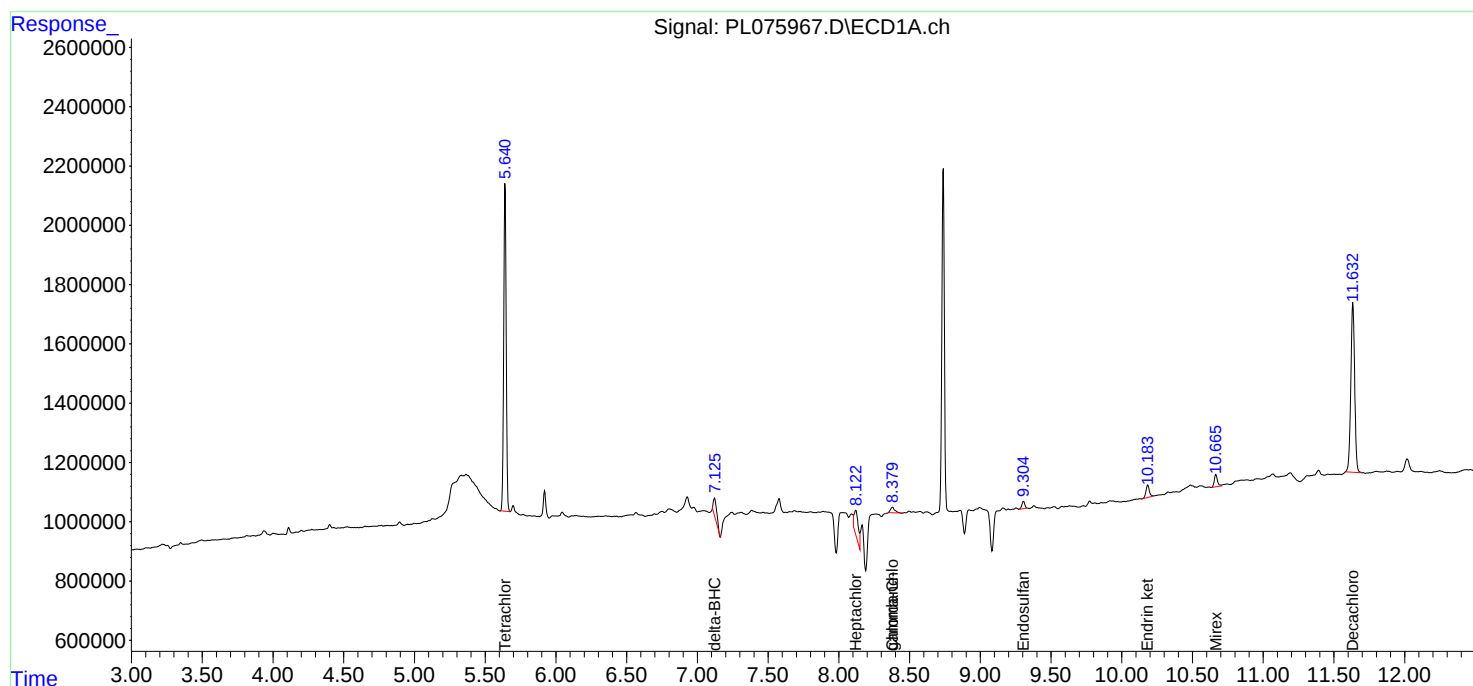


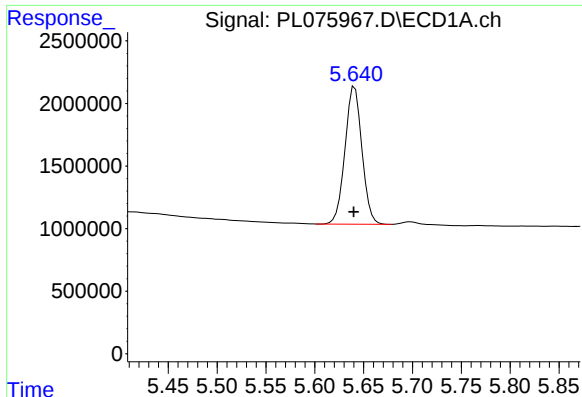

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 13275296
Conc: 17.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

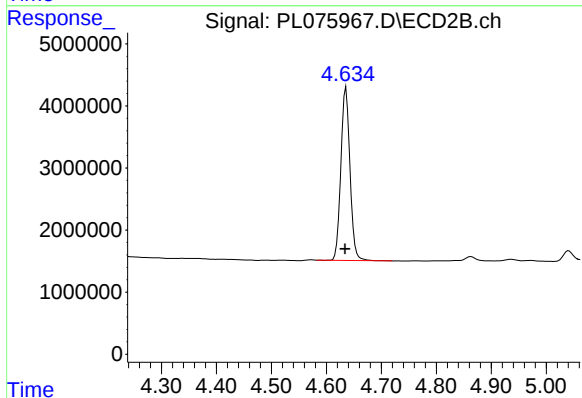


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: 0.002 min
Response: 32206698
Conc: 16.98 ng/ml

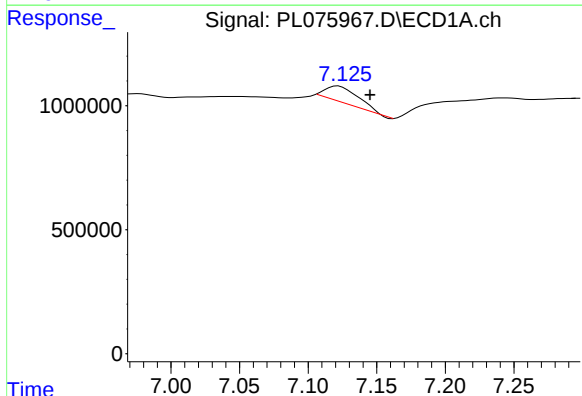


#7 delta-BHC

R.T.: 7.122 min
Delta R.T.: -0.023 min
Response: 1089603
Conc: 1.40 ng/ml

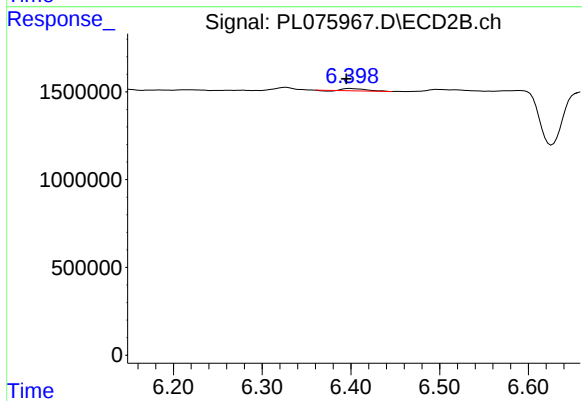

#7 delta-BHC


R.T.: 6.399 min
Delta R.T.: 0.004 min
Response: 217210
Conc: 0.10 ng/ml

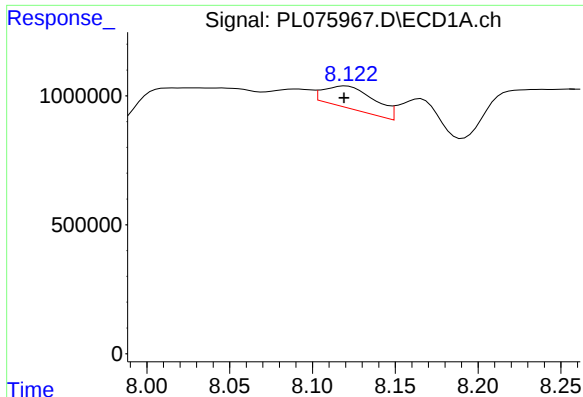

#8 Heptachlor epoxide


R.T.: 8.120 min
Delta R.T.: 0.001 min
Response: 1830284
Conc: 2.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

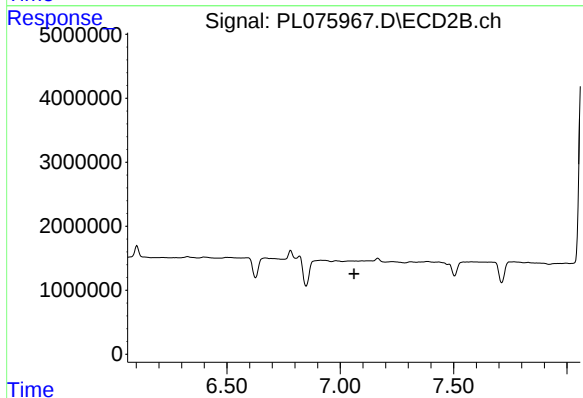


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.061 min
Response: 0
Conc: N.D.

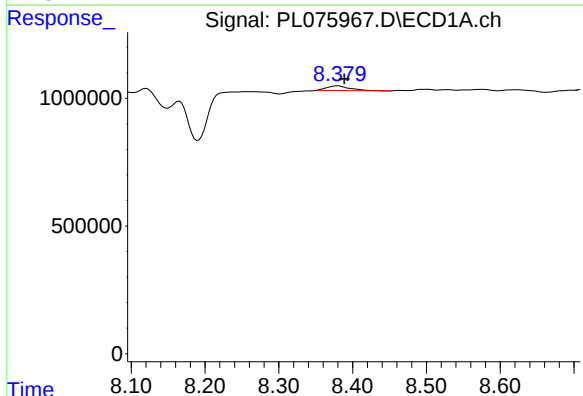


#10 gamma-Chlordane

R.T.: 8.380 min
Delta R.T.: -0.009 min
Response: 409725
Conc: 0.53 ng/ml

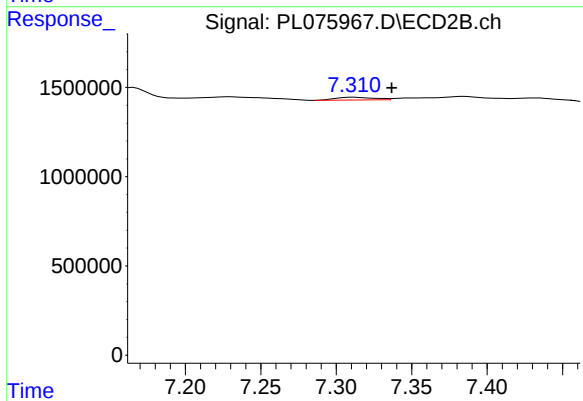

#10 gamma-Chlordane


R.T.: 7.311 min
Delta R.T.: -0.026 min
Response: 268854
Conc: 0.14 ng/ml

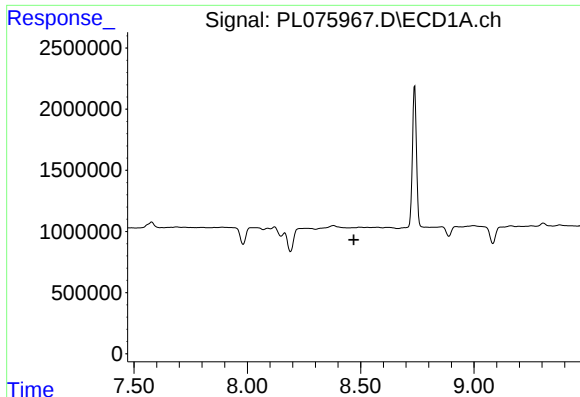

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

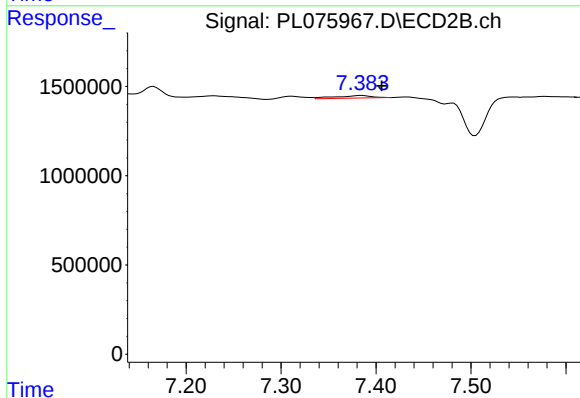


#11 alpha-Chlordane

R.T.: 7.384 min
Delta R.T.: -0.022 min
Response: 378813
Conc: 0.20 ng/ml

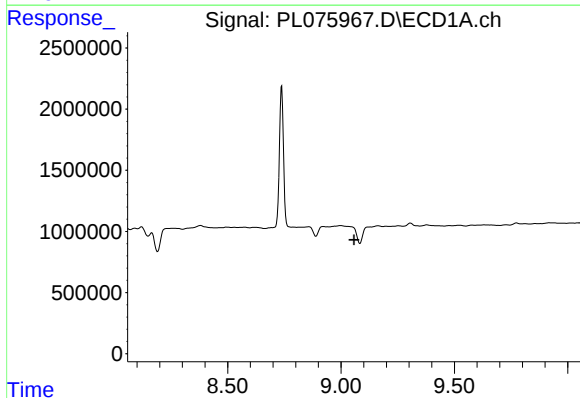


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

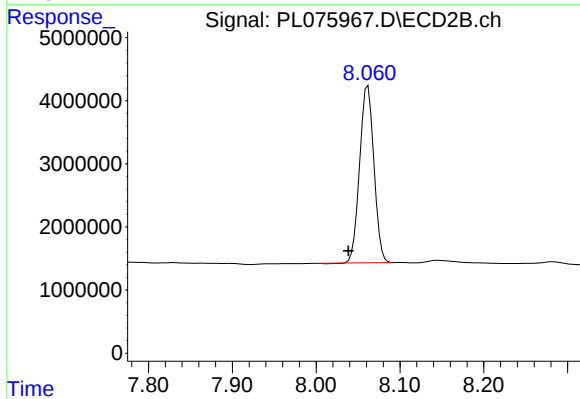

#14 Endrin


R.T.: 8.062 min
Delta R.T.: 0.023 min
Response: 33163718
Conc: 21.82 ng/ml

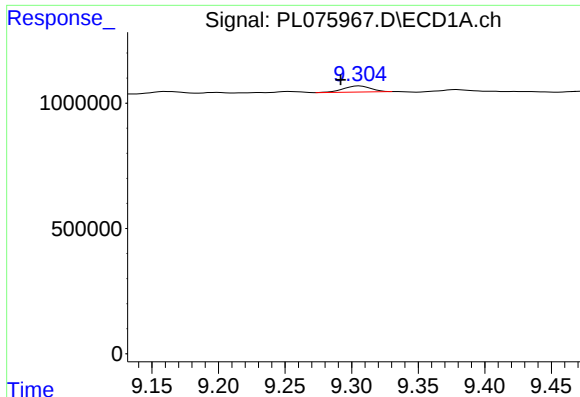

#15 Endosulfan II


R.T.: 9.306 min
Delta R.T.: 0.014 min
Response: 364968
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

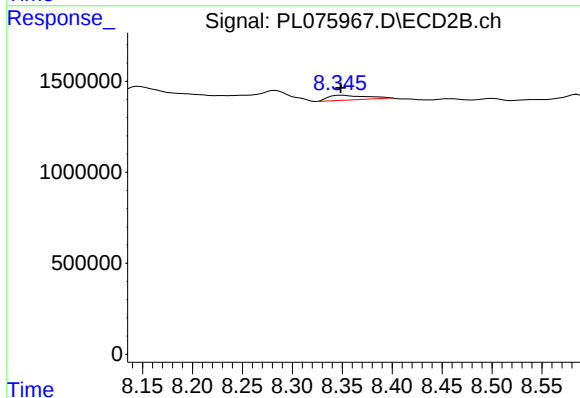


#15 Endosulfan II

R.T.: 8.349 min
Delta R.T.: 0.000 min
Response: 668834
Conc: 0.44 ng/ml

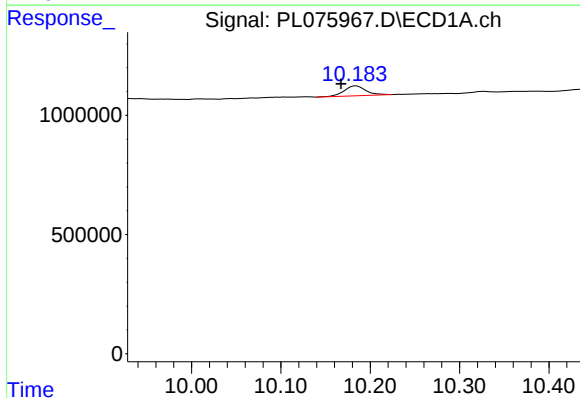


#21 Endrin ketone

R.T.: 10.184 min
Delta R.T.: 0.017 min
Response: 692287
Conc: 0.96 ng/ml

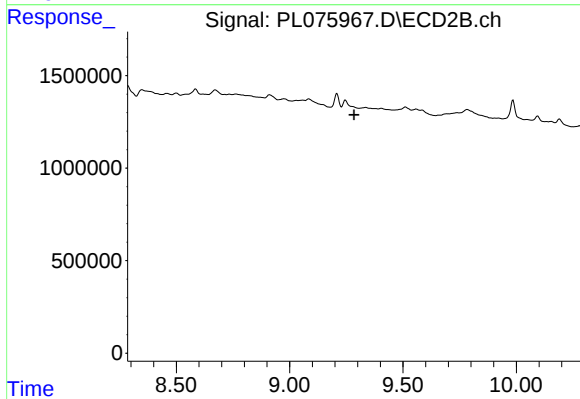

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

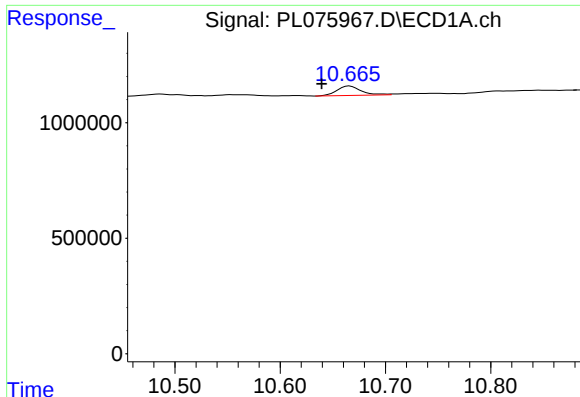

#22 Mirex


R.T.: 10.666 min
Delta R.T.: 0.026 min
Response: 660987
Conc: 1.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

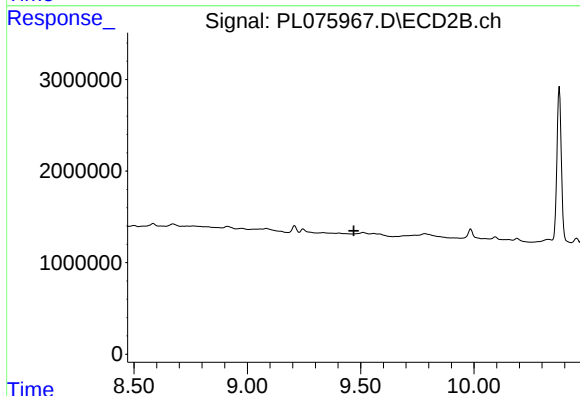


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.470 min
Response: 0
Conc: N.D.

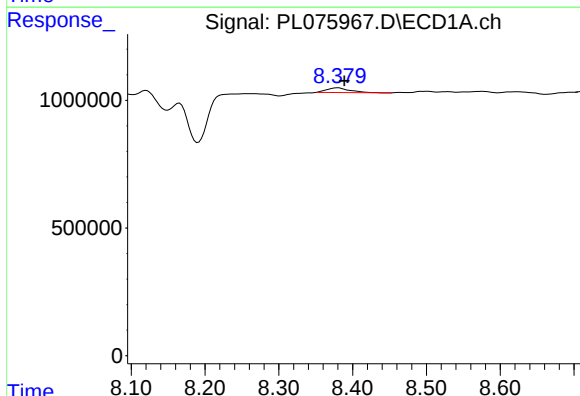


#25 Chlordane-3

R.T.: 8.380 min
Delta R.T.: -0.009 min
Response: 409725
Conc: 4.03 ng/ml

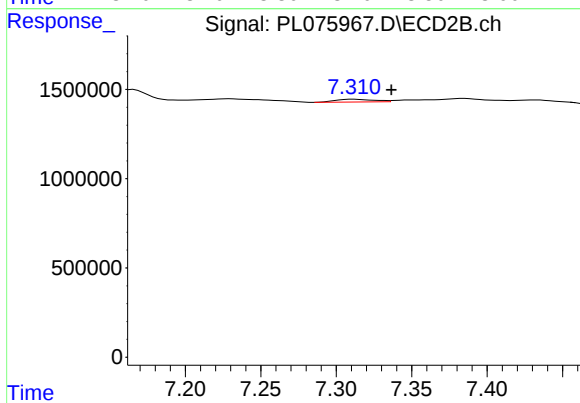

#25 Chlordane-3


R.T.: 7.311 min
Delta R.T.: -0.025 min
Response: 268854
Conc: 1.52 ng/ml

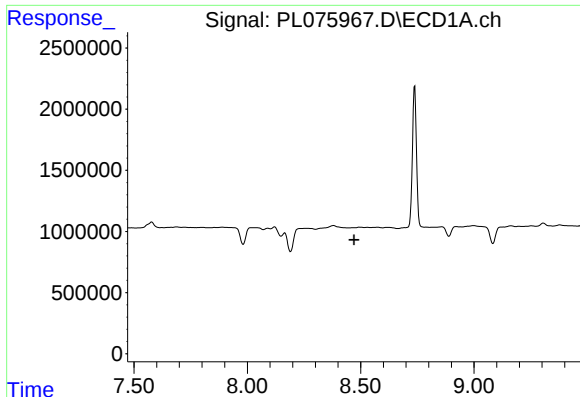

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

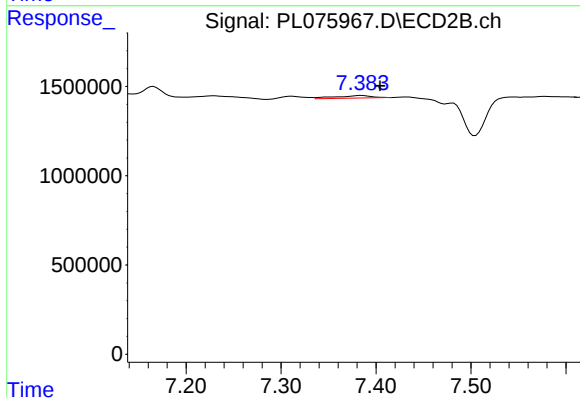


#26 Chlordane-4

R.T.: 7.384 min
Delta R.T.: -0.020 min
Response: 378813
Conc: 2.01 ng/ml

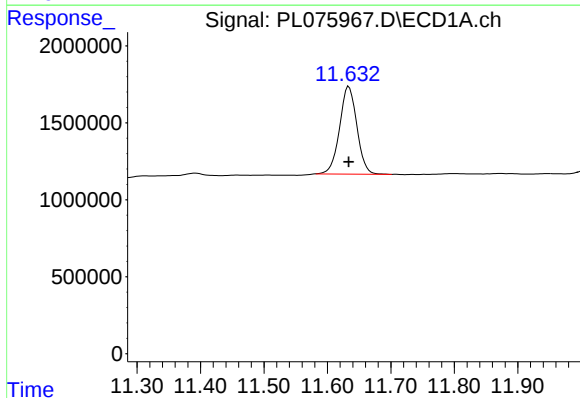

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: 0.000 min
Response: 10770476
Conc: 17.12 ng/ml

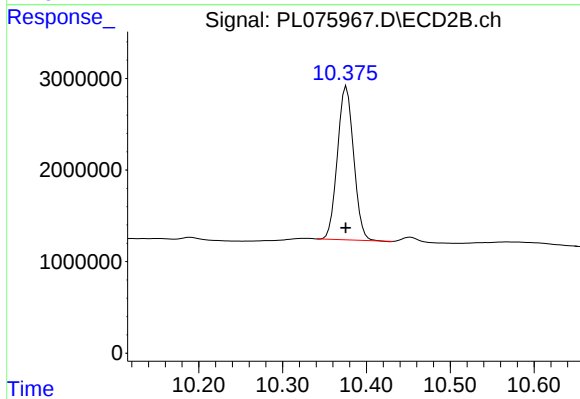

#28 Decachlorobiphenyl

R.T.: 10.376 min
Delta R.T.: 0.000 min
Response: 22475490
Conc: 14.63 ng/ml