

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
 Data File : PL075935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2022 19:36
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:40:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 01:37:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.634	72204892	211.5E6	99.424	98.972
28)	SA Decachlor...	11.633	10.375	54728885	134.8E6	96.204	95.884
Target Compounds							
23)	Chlordane-1	7.034	5.953	25276019	55198542	989.109	986.332
24)	Chlordane-2	7.627	6.639	29646917	63626247	973.438	966.014
25)	Chlordane-3	8.389	7.337	104.7E6	179.9E6	1005.273	1000.858
26)	Chlordane-4	8.472	7.404	126.1E6	188.8E6	996.241	994.818
27)	Chlordane-5	9.365	8.116	21750976	46762911	994.771	979.394



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
Data File : PL075935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2022 19:36
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:40:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 01:37:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

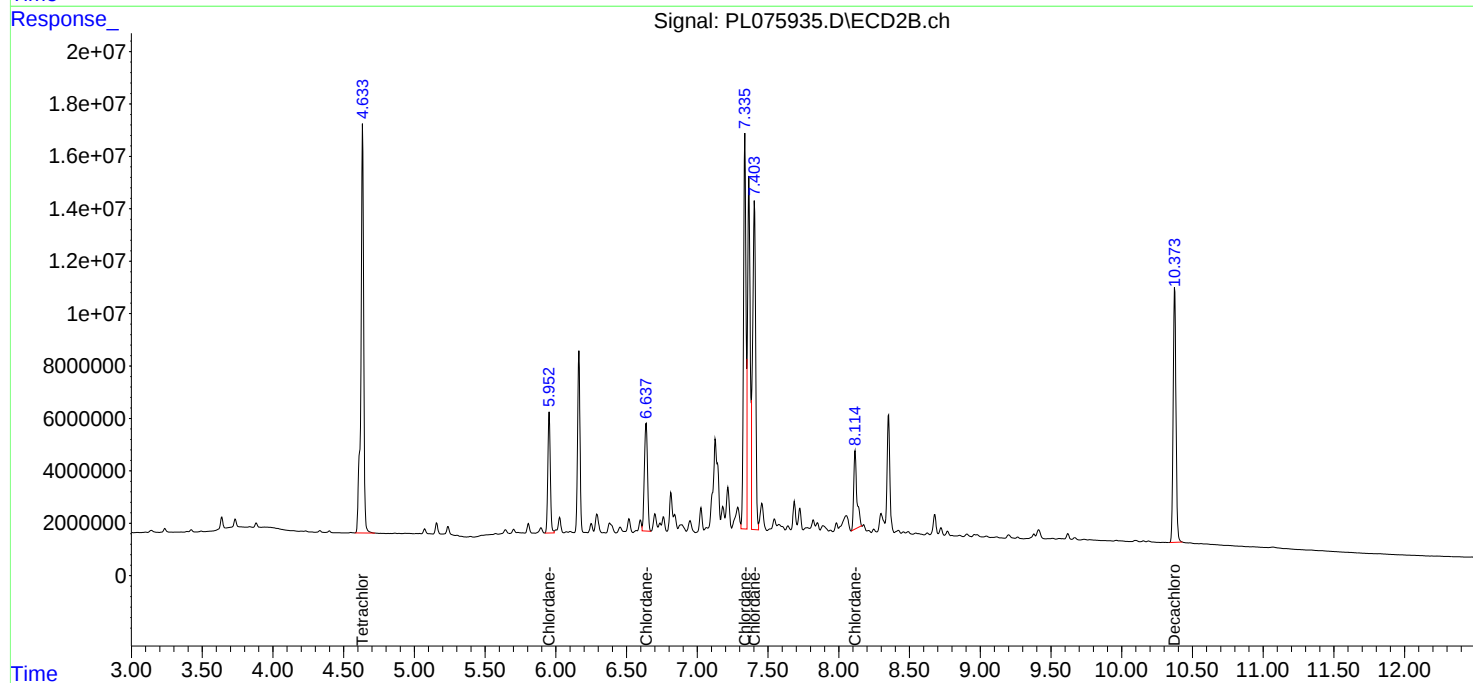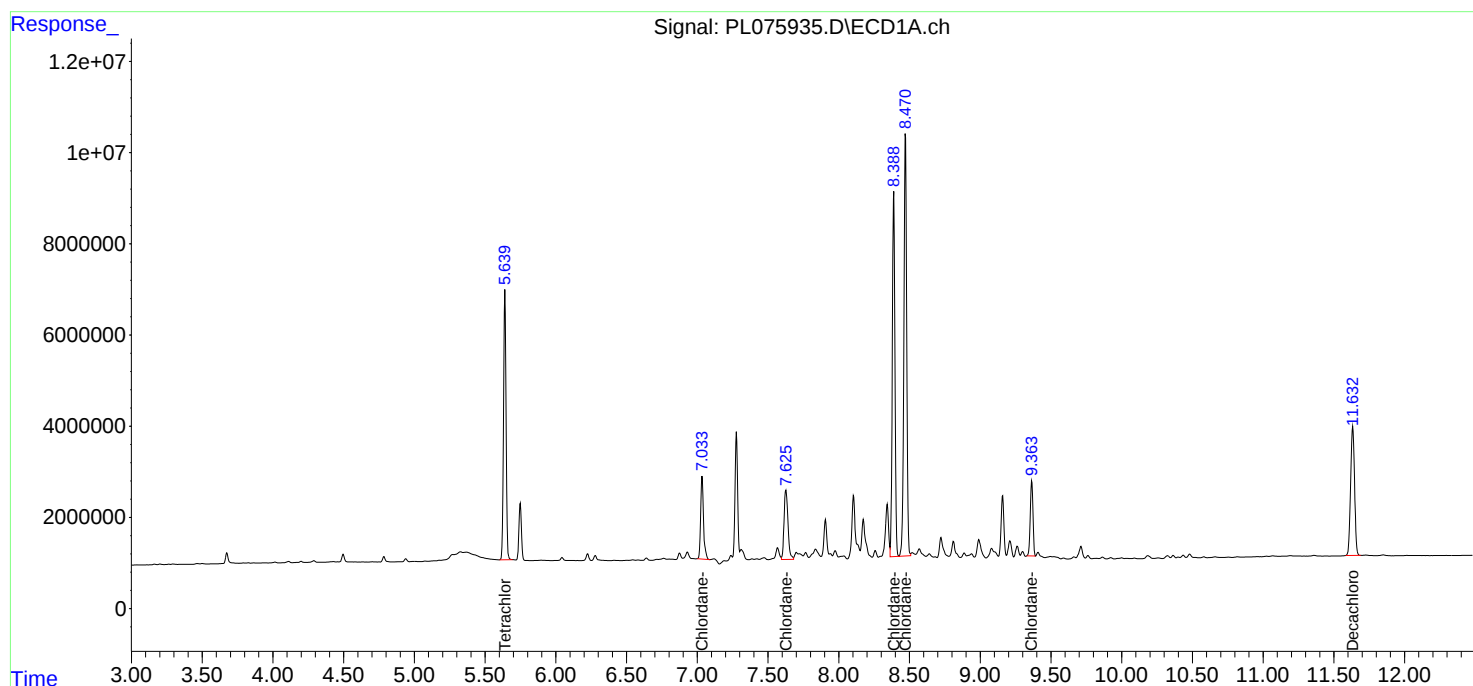


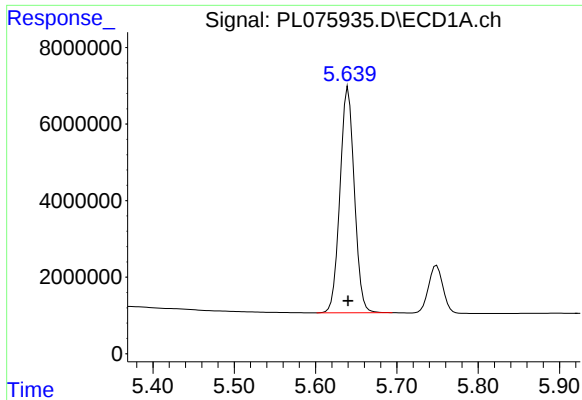

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 72204892
Conc: 99.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

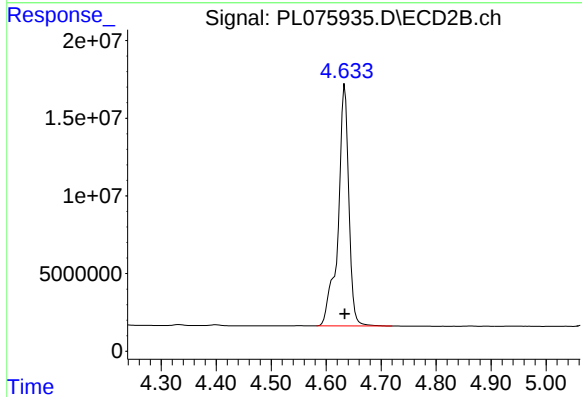


#1 Tetrachloro-m-xylene

R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 211486838
Conc: 98.97 ng/ml

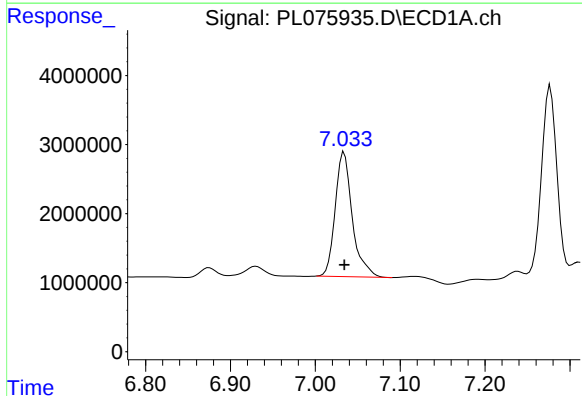


#23 Chlordane-1

R.T.: 7.034 min
Delta R.T.: 0.000 min
Response: 25276019
Conc: 989.11 ng/ml

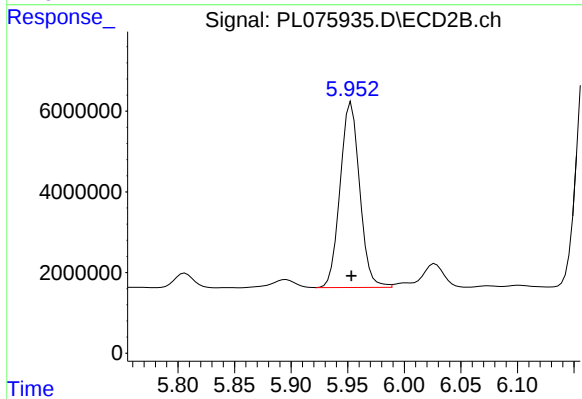

#23 Chlordane-1


R.T.: 5.953 min
Delta R.T.: 0.000 min
Response: 55198542
Conc: 986.33 ng/ml

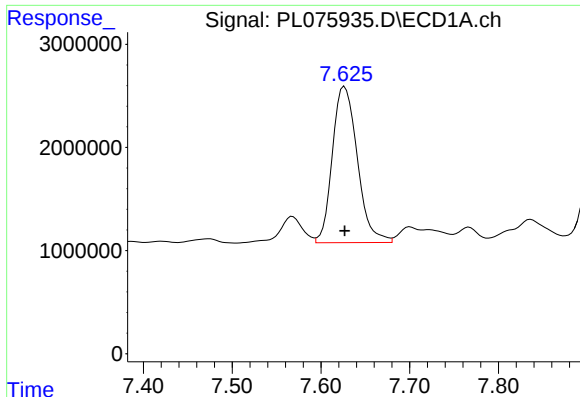

#24 Chlordane-2


R.T.: 7.627 min
Delta R.T.: 0.000 min
Response: 29646917
Conc: 973.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

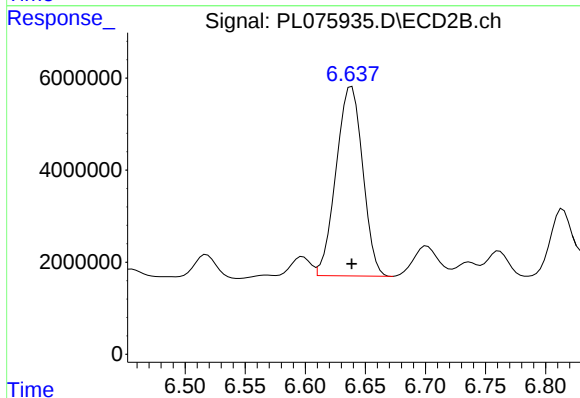


#24 Chlordane-2

R.T.: 6.639 min
Delta R.T.: 0.000 min
Response: 63626247
Conc: 966.01 ng/ml

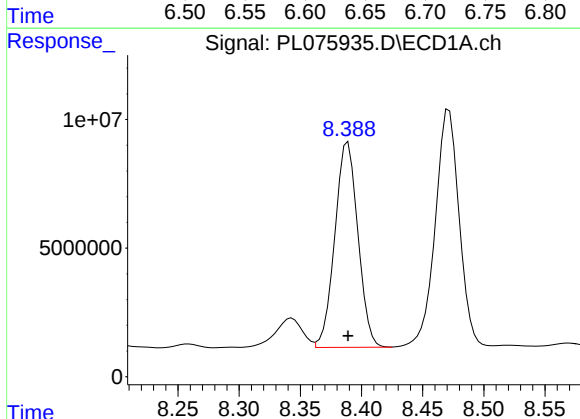


#25 Chlordane-3

R.T.: 8.389 min
Delta R.T.: 0.000 min
Response: 104702962
Conc: 1005.27 ng/ml

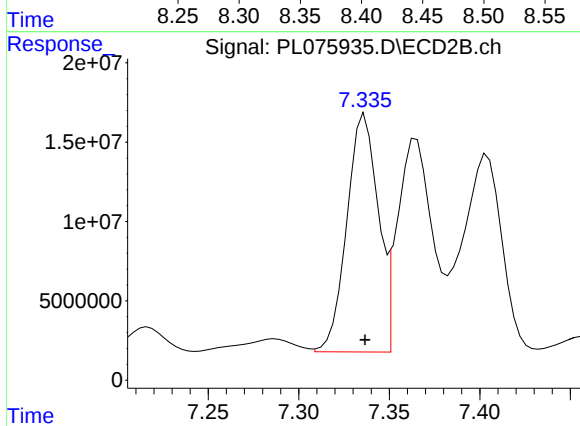

#25 Chlordane-3


R.T.: 7.337 min
Delta R.T.: 0.000 min
Response: 179877214
Conc: 1000.86 ng/ml

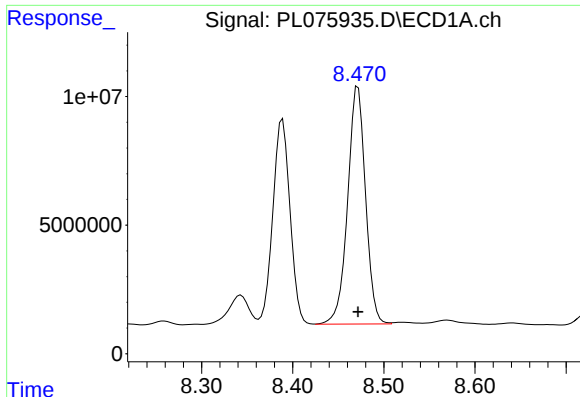

#26 Chlordane-4


R.T.: 8.472 min
Delta R.T.: 0.000 min
Response: 126102228
Conc: 996.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

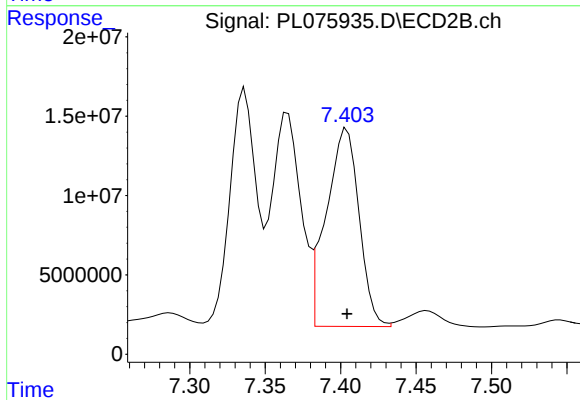


#26 Chlordane-4

R.T.: 7.404 min
Delta R.T.: 0.000 min
Response: 188812955
Conc: 994.82 ng/ml

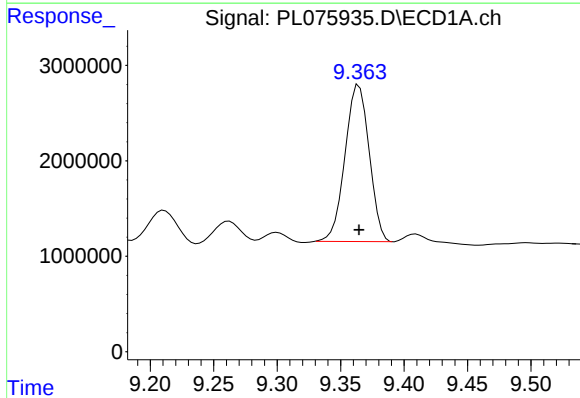


#27 Chlordane-5

R.T.: 9.365 min
Delta R.T.: 0.000 min
Response: 21750976
Conc: 994.77 ng/ml

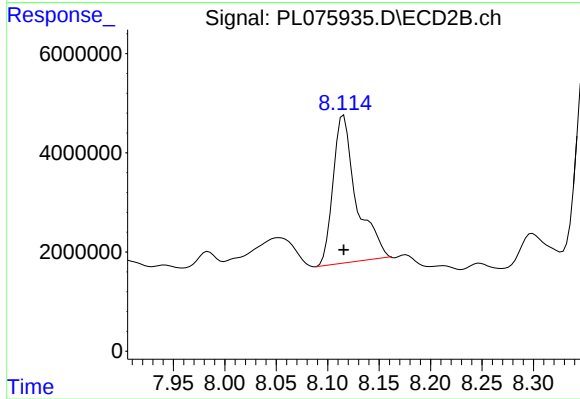

#27 Chlordane-5


R.T.: 8.116 min
Delta R.T.: 0.000 min
Response: 46762911
Conc: 979.39 ng/ml

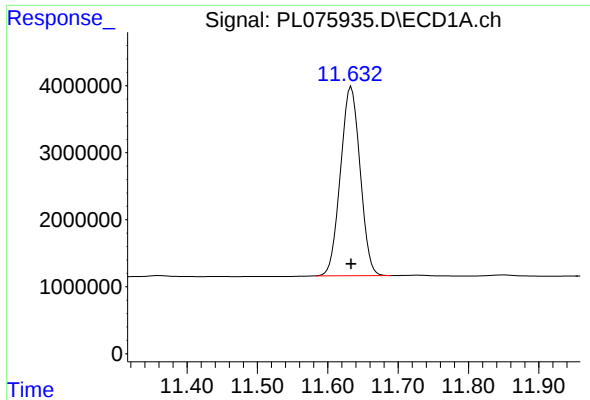

#28 Decachlorobiphenyl

R.T.: 11.633 min
Delta R.T.: 0.000 min
Response: 54728885
Conc: 96.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

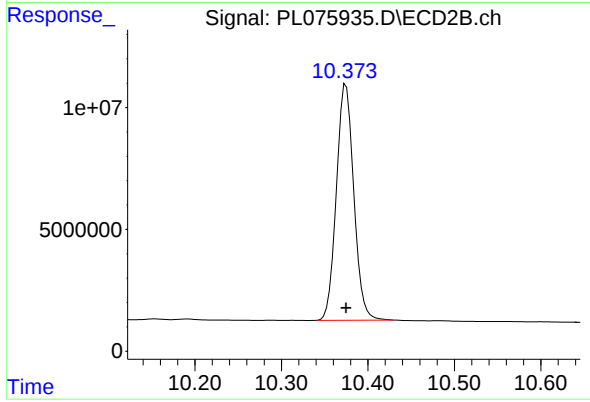

#28 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: 0.000 min
Response: 134828924
Conc: 95.88 ng/ml