

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
 Data File : PL075936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2022 19:52
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:43:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 01:37:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.634	53767112	157.8E6	74.354	74.215
28)	SA Decachlor...	11.634	10.375	42193140	103.1E6	74.444	73.889
Target Compounds							
23)	Chlordane-1	7.035	5.953	18978574	41206311	745.101	740.816
24)	Chlordane-2	7.628	6.639	22580415	48297180	744.254	738.769
25)	Chlordane-3	8.389	7.337	77243223	132.7E6	744.397	742.097
26)	Chlordane-4	8.472	7.405	94024607	139.5E6	745.197	739.926
27)	Chlordane-5	9.365	8.116	16190070	35074194	743.603	739.654



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
Data File : PL075936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2022 19:52
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:43:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 01:37:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

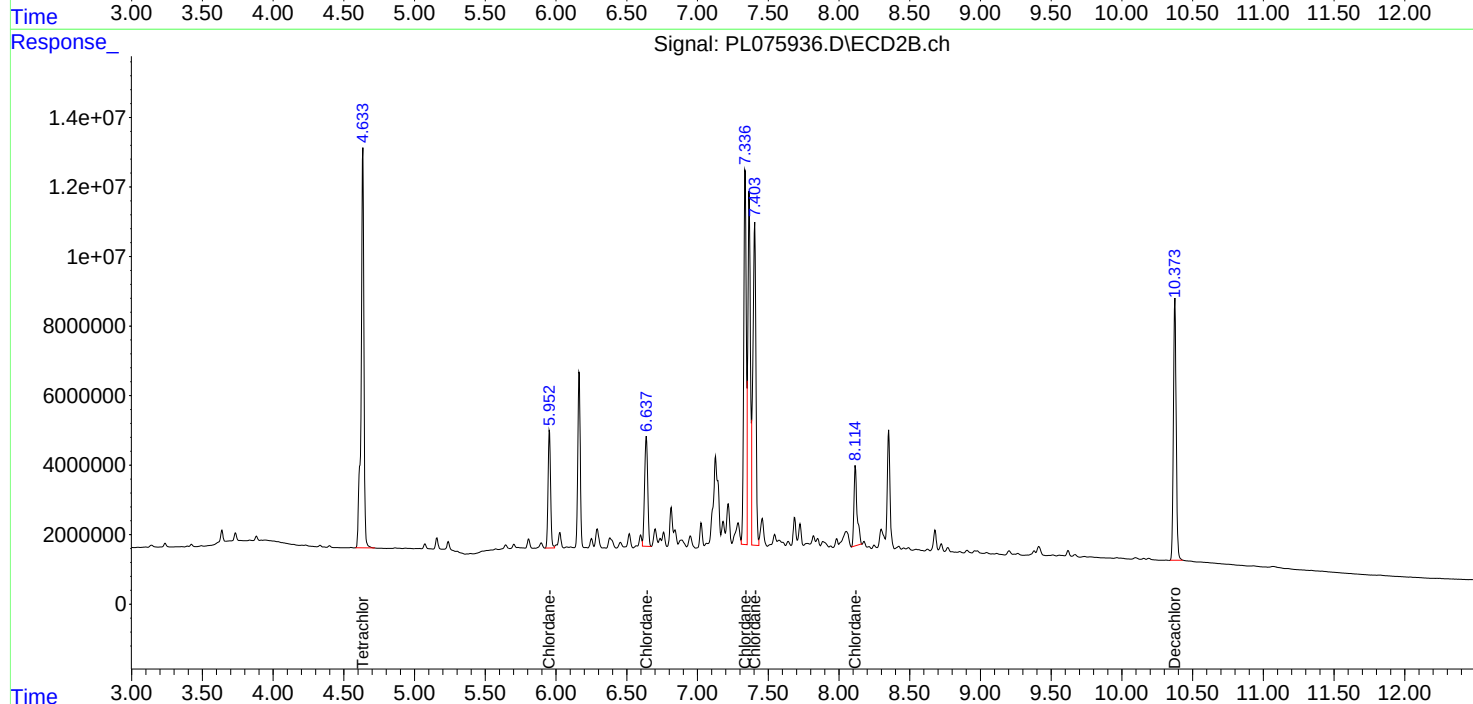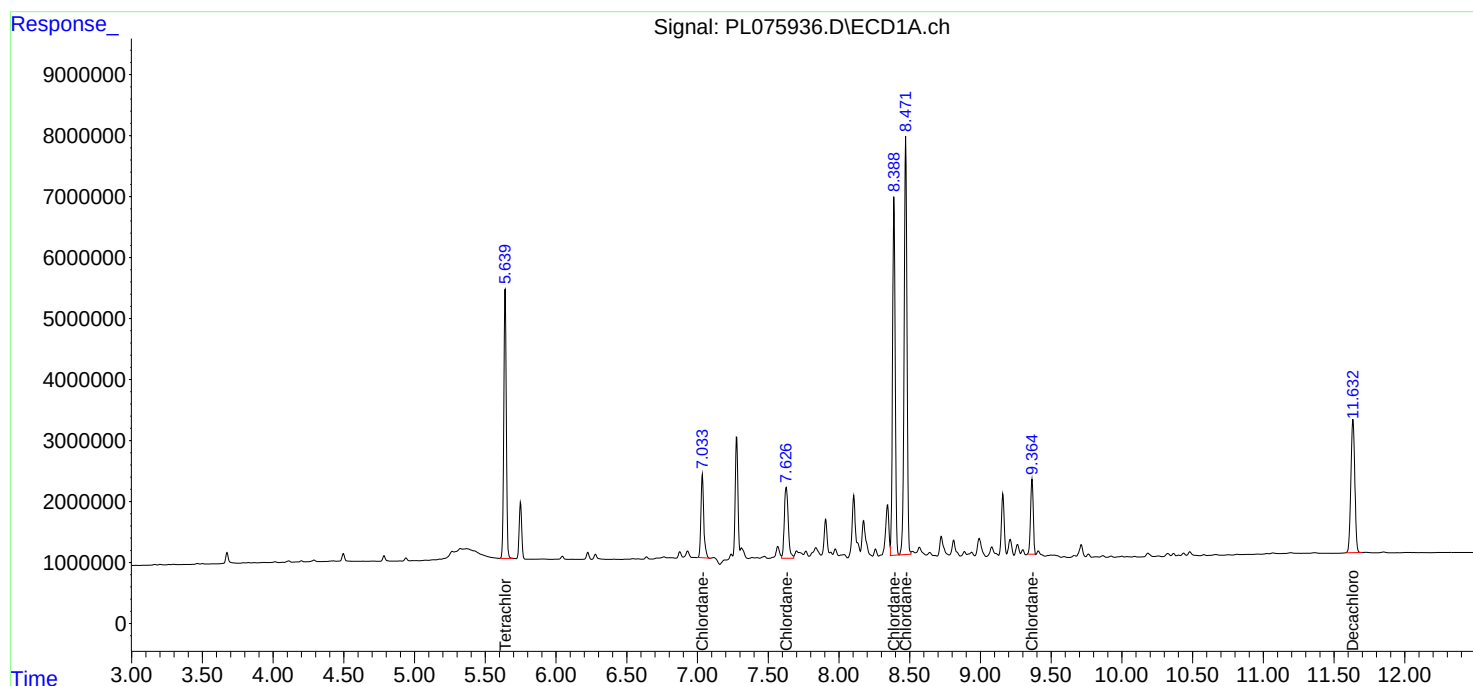


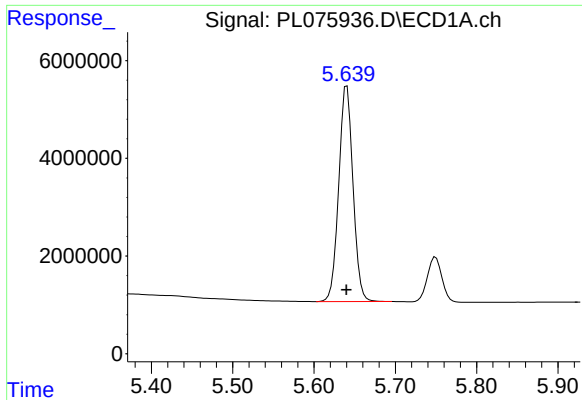

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 53767112
Conc: 74.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

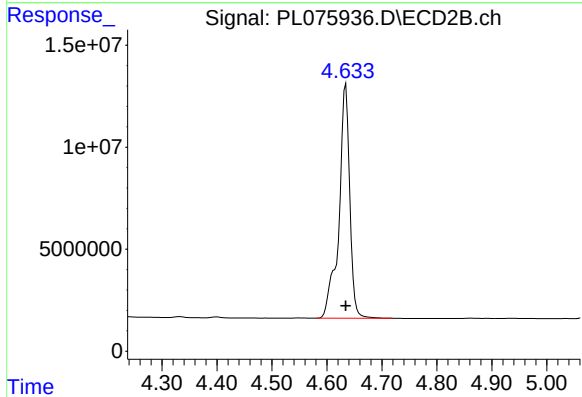


#1 Tetrachloro-m-xylene

R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 157761575
Conc: 74.22 ng/ml

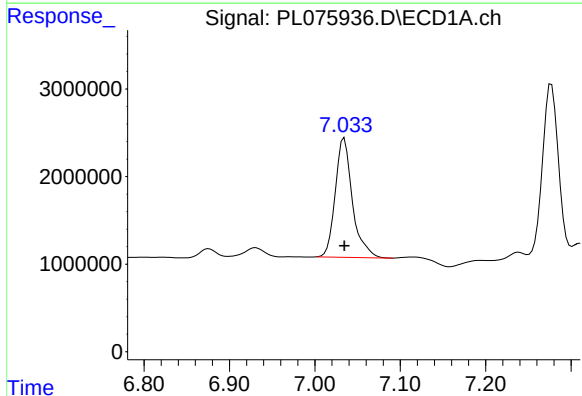


#23 Chlordane-1

R.T.: 7.035 min
Delta R.T.: 0.000 min
Response: 18978574
Conc: 745.10 ng/ml

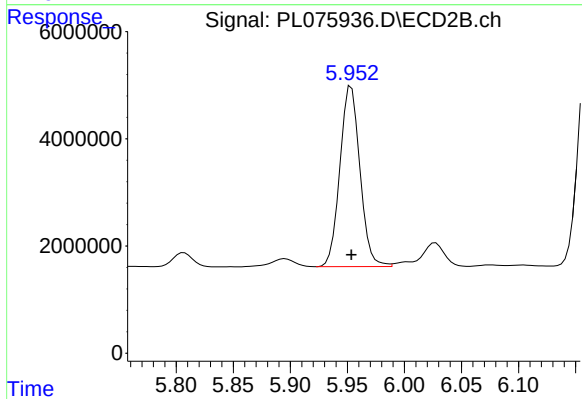

#23 Chlordane-1


R.T.: 5.953 min
Delta R.T.: 0.000 min
Response: 41206311
Conc: 740.82 ng/ml

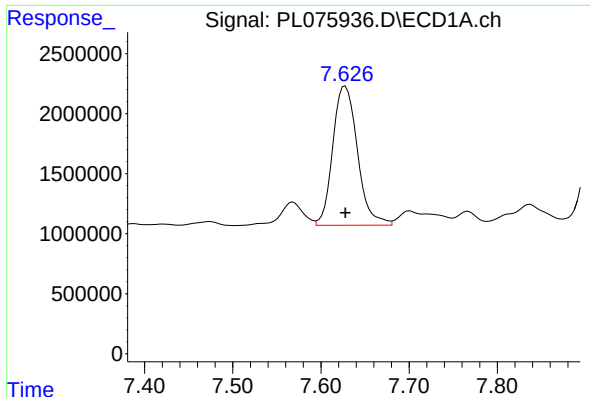

#24 Chlordane-2


R.T.: 7.628 min
Delta R.T.: 0.000 min
Response: 22580415
Conc: 744.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

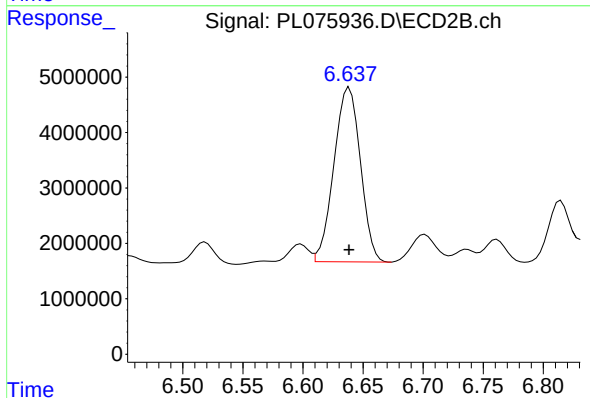


#24 Chlordane-2

R.T.: 6.639 min
Delta R.T.: 0.000 min
Response: 48297180
Conc: 738.77 ng/ml

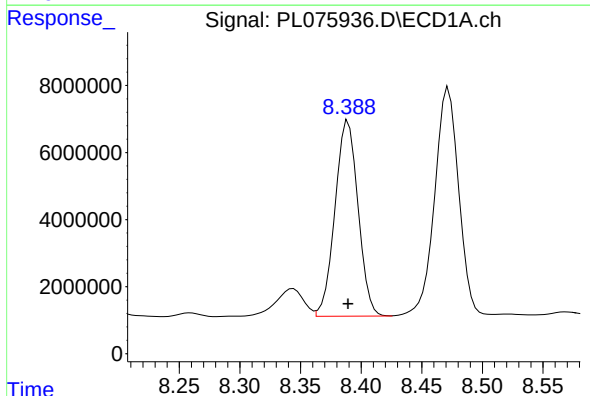


#25 Chlordane-3

R.T.: 8.389 min
Delta R.T.: 0.000 min
Response: 77243223
Conc: 744.40 ng/ml

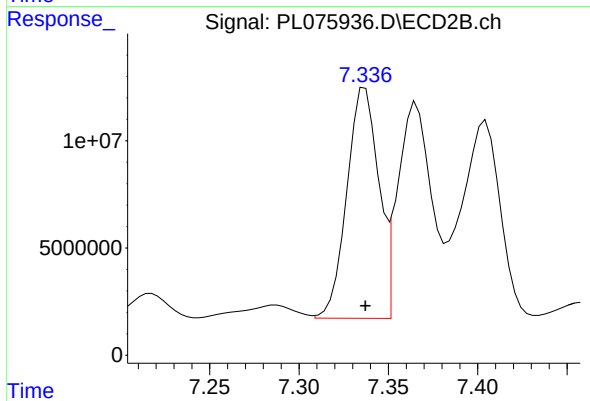

#25 Chlordane-3


R.T.: 7.337 min
Delta R.T.: 0.000 min
Response: 132672912
Conc: 742.10 ng/ml

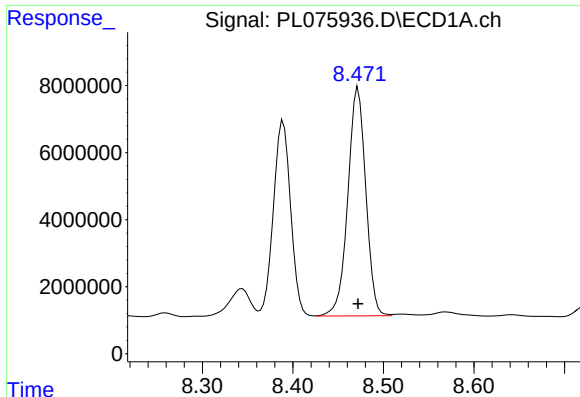

#26 Chlordane-4


R.T.: 8.472 min
Delta R.T.: 0.000 min
Response: 94024607
Conc: 745.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

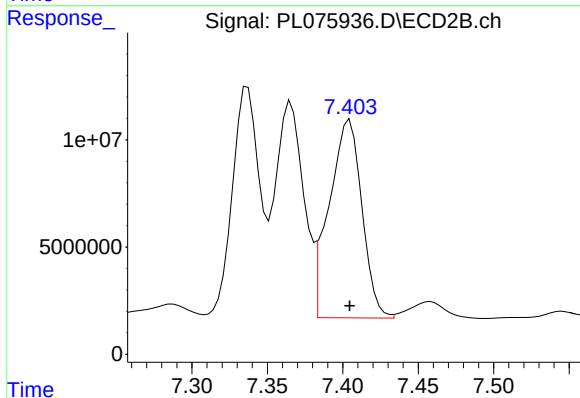


#26 Chlordane-4

R.T.: 7.405 min
Delta R.T.: 0.000 min
Response: 139498628
Conc: 739.93 ng/ml

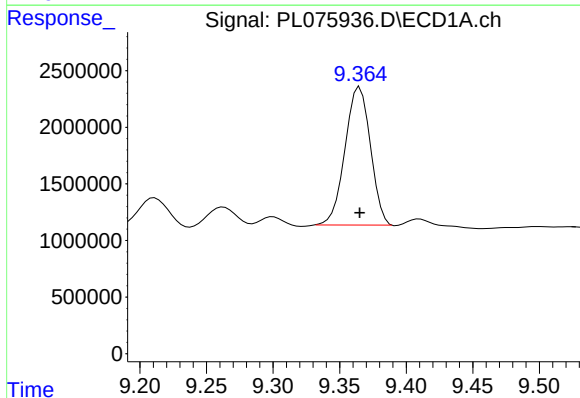


#27 Chlordane-5

R.T.: 9.365 min
Delta R.T.: 0.000 min
Response: 16190070
Conc: 743.60 ng/ml

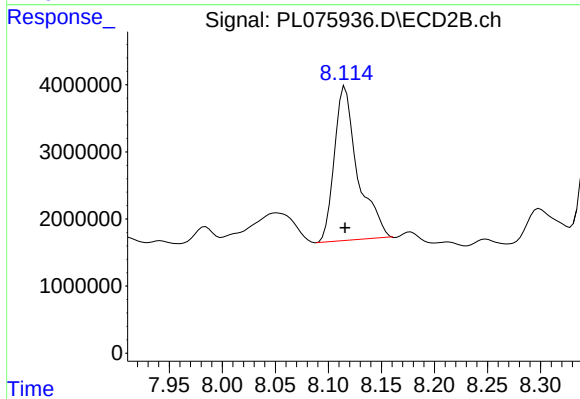

#27 Chlordane-5


R.T.: 8.116 min
Delta R.T.: 0.000 min
Response: 35074194
Conc: 739.65 ng/ml

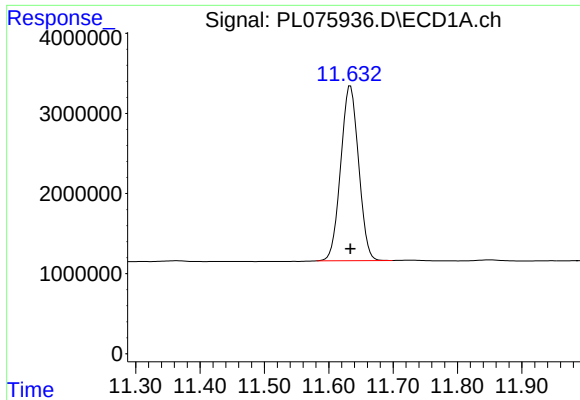

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: 0.000 min
Response: 42193140
Conc: 74.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

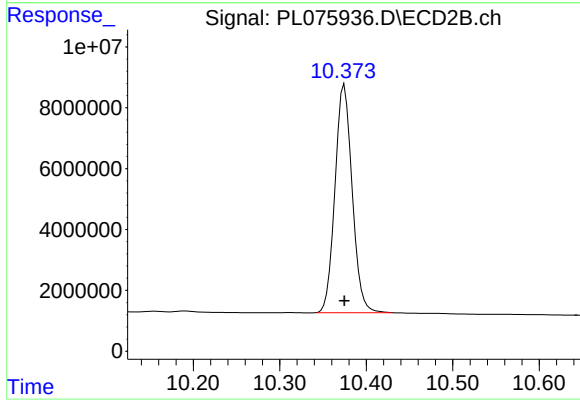

#28 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: 0.000 min
Response: 103136375
Conc: 73.89 ng/ml