

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
 Data File : PL075937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2022 20:09
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:38:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 01:37:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.634	36520963	107.9E6	50.000	50.000
28)	SA Decachlor...	11.634	10.375	29523754	73201904	50.000	50.000
Target Compounds							
23)	Chlordane-1	7.033	5.953	12916312	28364160	500.000	500.000
24)	Chlordane-2	7.628	6.639	15632434	34051612	500.000	500.000
25)	Chlordane-3	8.389	7.337	51802301	89784476	500.000	500.000
26)	Chlordane-4	8.472	7.404	63526979	95390030	500.000	500.000
27)	Chlordane-5	9.365	8.116	10989831	24365333	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
Data File : PL075937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2022 20:09
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:38:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 01:37:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

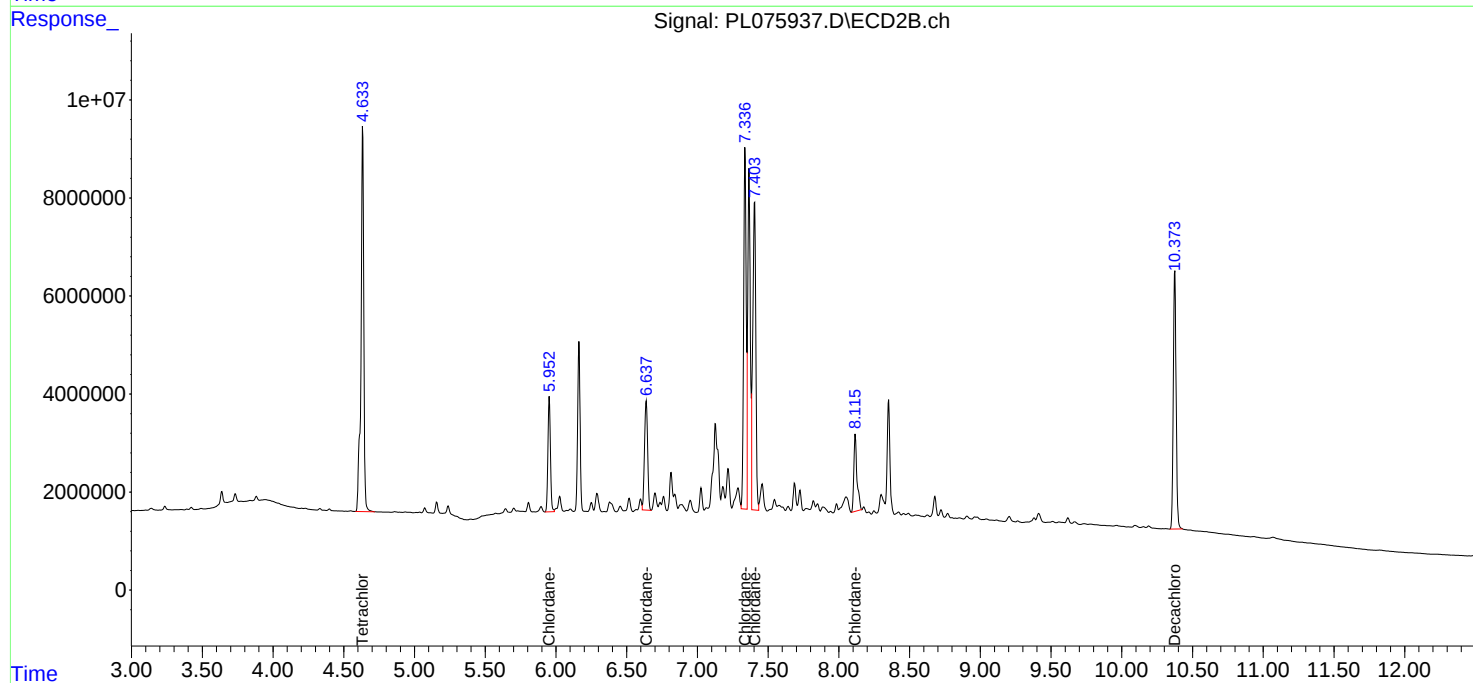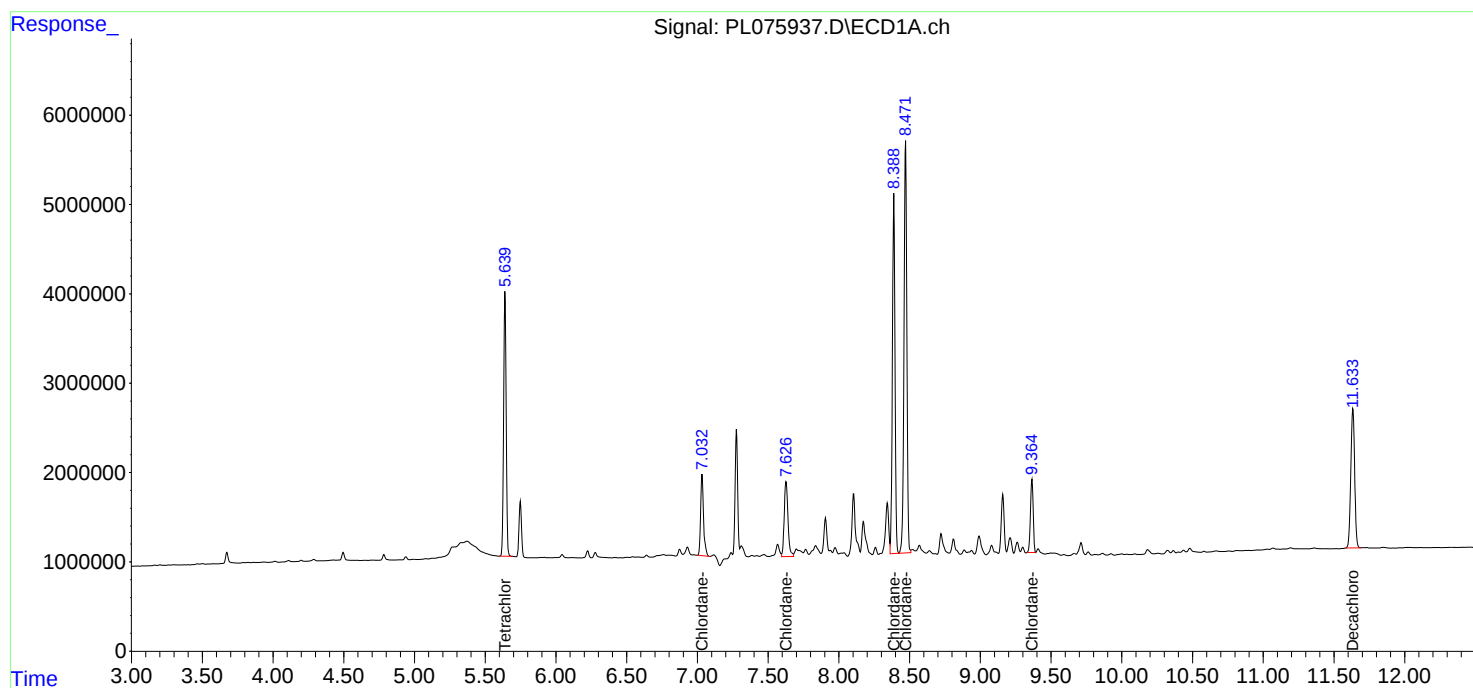


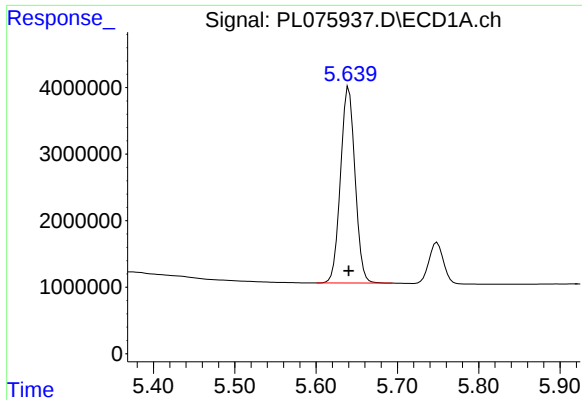

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 36520963
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

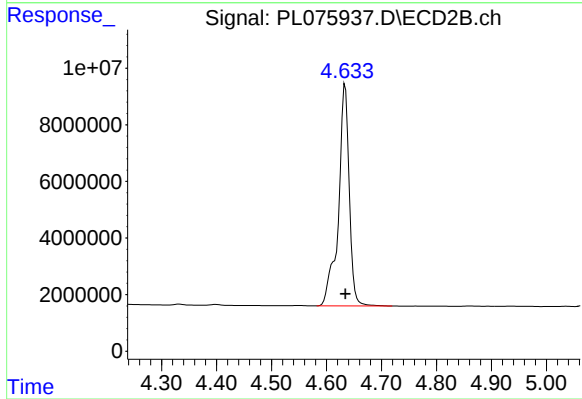


#1 Tetrachloro-m-xylene

R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 107940942
Conc: 50.00 ng/ml

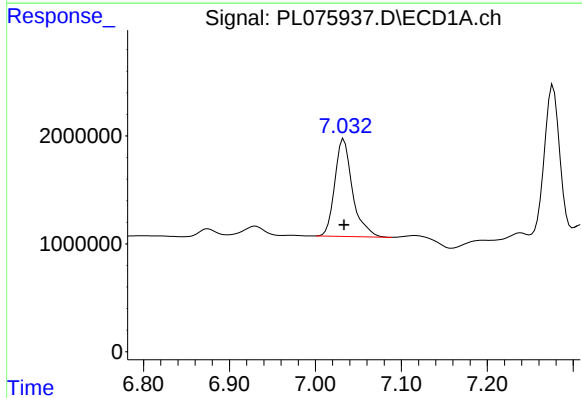


#23 Chlordane-1

R.T.: 7.033 min
Delta R.T.: 0.000 min
Response: 12916312
Conc: 500.00 ng/ml

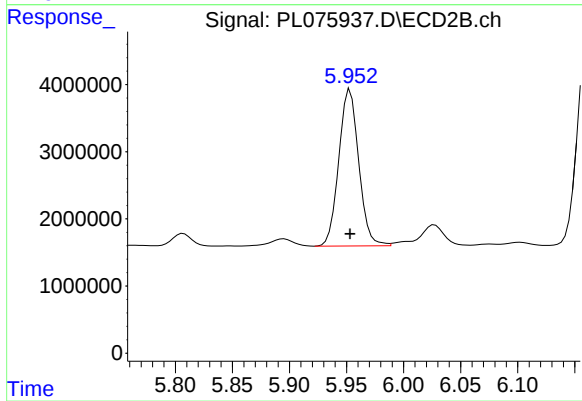

#23 Chlordane-1


R.T.: 5.953 min
Delta R.T.: 0.000 min
Response: 28364160
Conc: 500.00 ng/ml

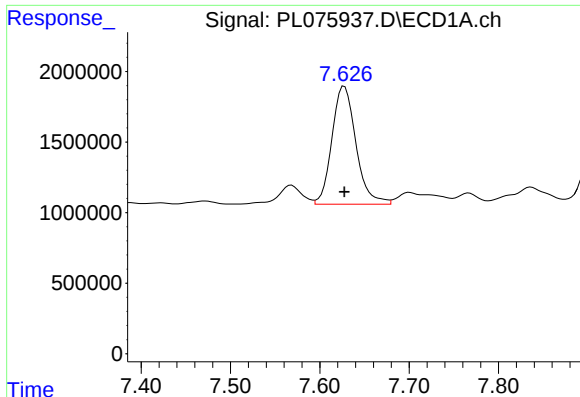

#24 Chlordane-2


R.T.: 7.628 min
Delta R.T.: 0.000 min
Response: 15632434
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

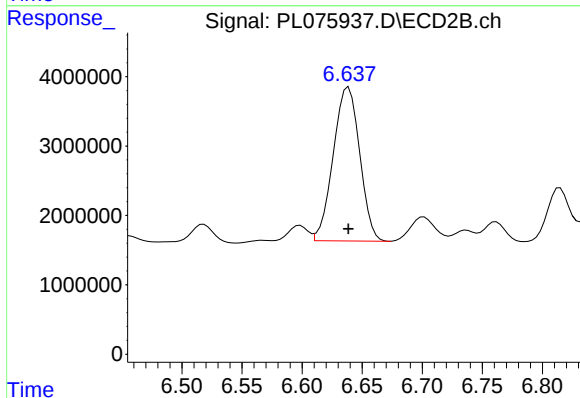


#24 Chlordane-2

R.T.: 6.639 min
Delta R.T.: 0.000 min
Response: 34051612
Conc: 500.00 ng/ml

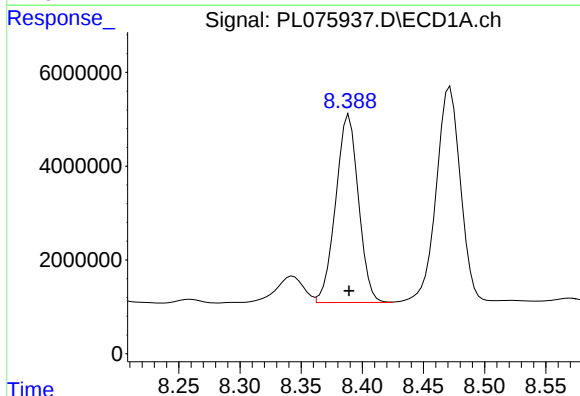


#25 Chlordane-3

R.T.: 8.389 min
Delta R.T.: 0.000 min
Response: 51802301
Conc: 500.00 ng/ml

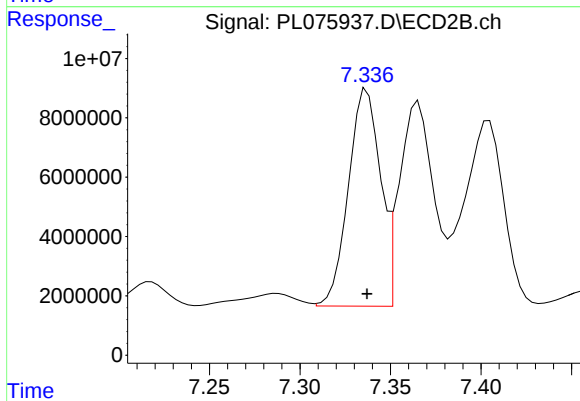

#25 Chlordane-3


R.T.: 7.337 min
Delta R.T.: 0.000 min
Response: 89784476
Conc: 500.00 ng/ml

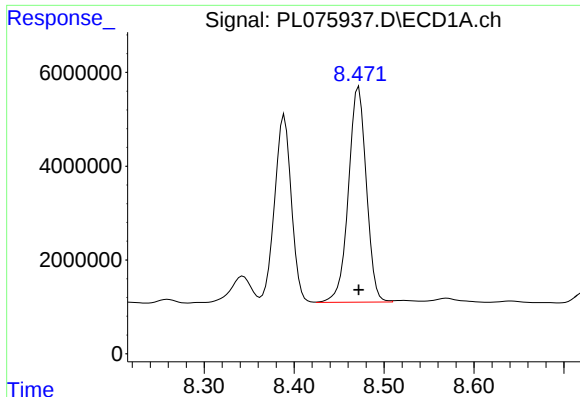

#26 Chlordane-4


R.T.: 8.472 min
Delta R.T.: 0.000 min
Response: 63526979
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

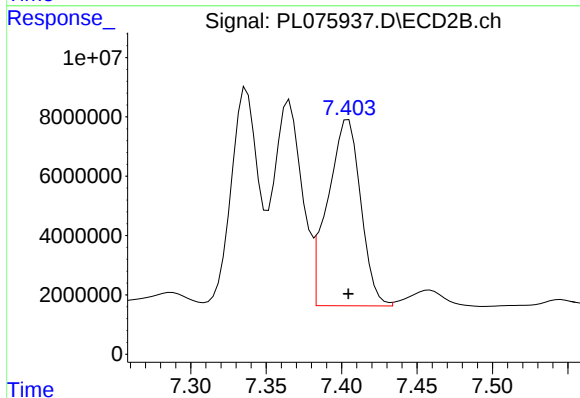


#26 Chlordane-4

R.T.: 7.404 min
Delta R.T.: 0.000 min
Response: 95390030
Conc: 500.00 ng/ml

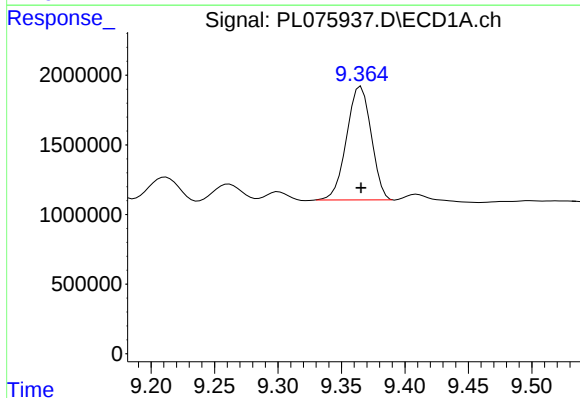


#27 Chlordane-5

R.T.: 9.365 min
Delta R.T.: 0.000 min
Response: 10989831
Conc: 500.00 ng/ml

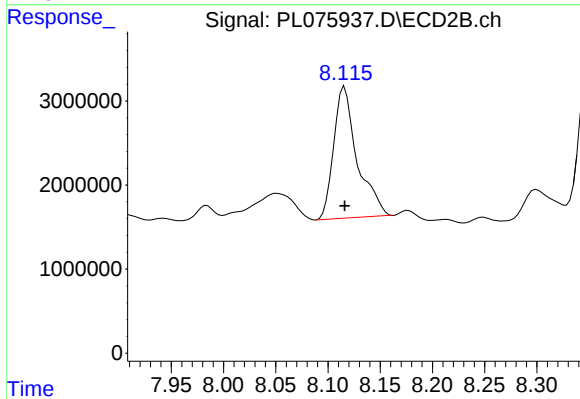

#27 Chlordane-5


R.T.: 8.116 min
Delta R.T.: 0.000 min
Response: 24365333
Conc: 500.00 ng/ml

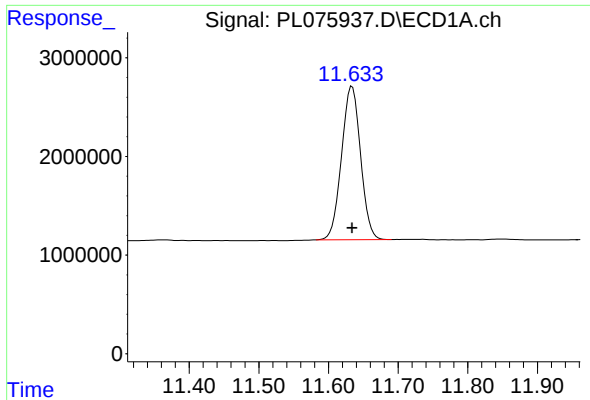

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: 0.000 min
Response: 29523754
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

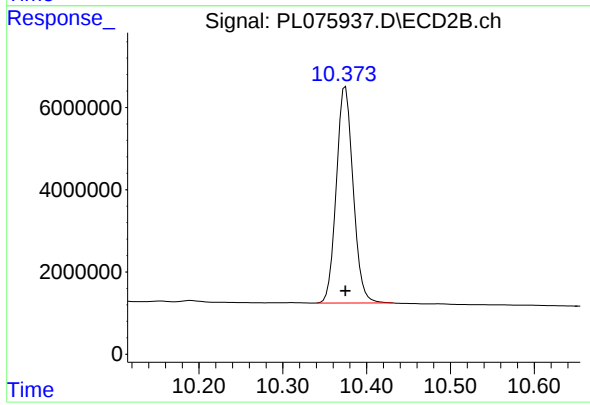

#28 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: 0.000 min
Response: 73201904
Conc: 50.00 ng/ml