

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
 Data File : PL075946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2022 22:37
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL062322

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:50:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 01:49:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.635	38699470	113.1E6	54.611	53.662
28)	SA Decachlor...	11.633	10.374	31198770	76968116	52.603	52.456
Target Compounds							
23)	Chlordane-1	7.034	5.954	13715355	29974803	541.927	535.379
24)	Chlordane-2	7.628	6.639	16458439	35710113	542.552	513.553
25)	Chlordane-3	8.389	7.338	54999115	95095521	540.850	539.202
26)	Chlordane-4	8.472	7.405	67386239	101.0E6	541.258	535.751
27)	Chlordane-5	9.365	8.116	11726997	25752449	549.594	562.855



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
Data File : PL075946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2022 22:37
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL062322

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:50:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 01:49:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

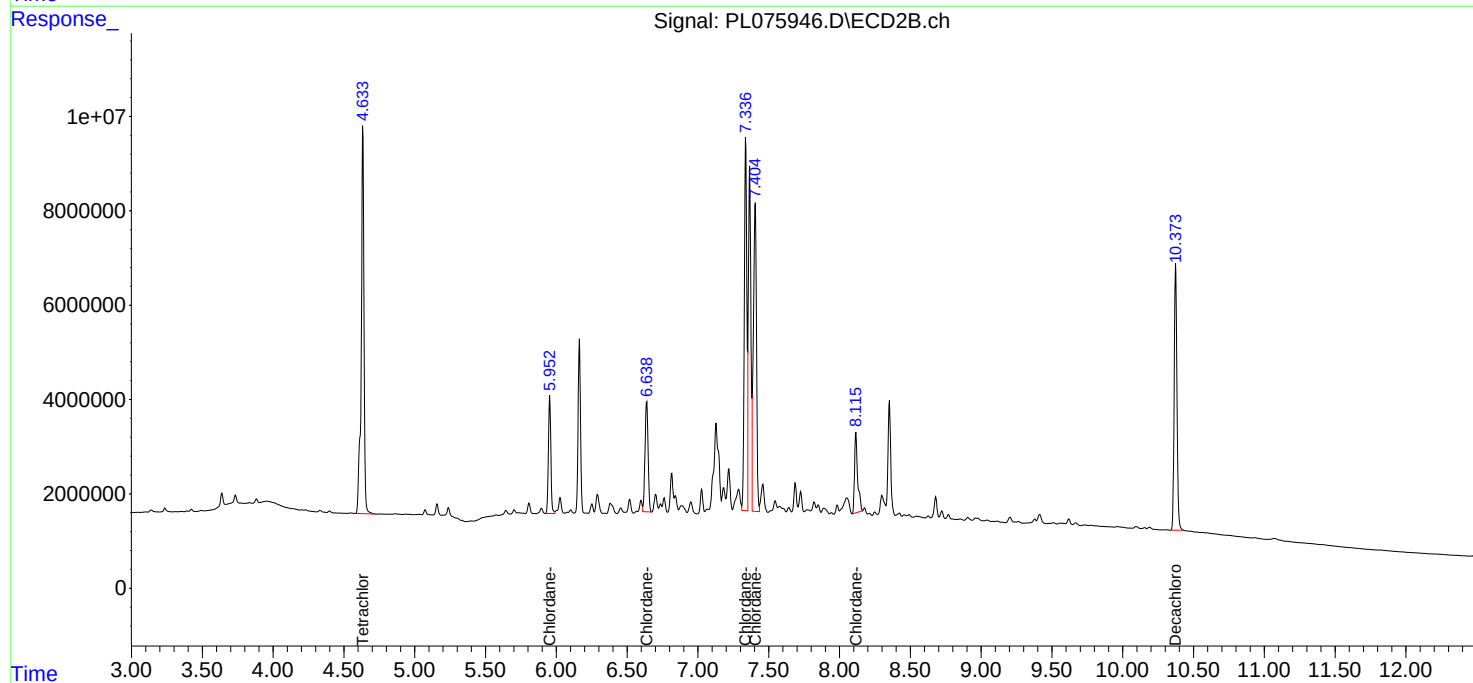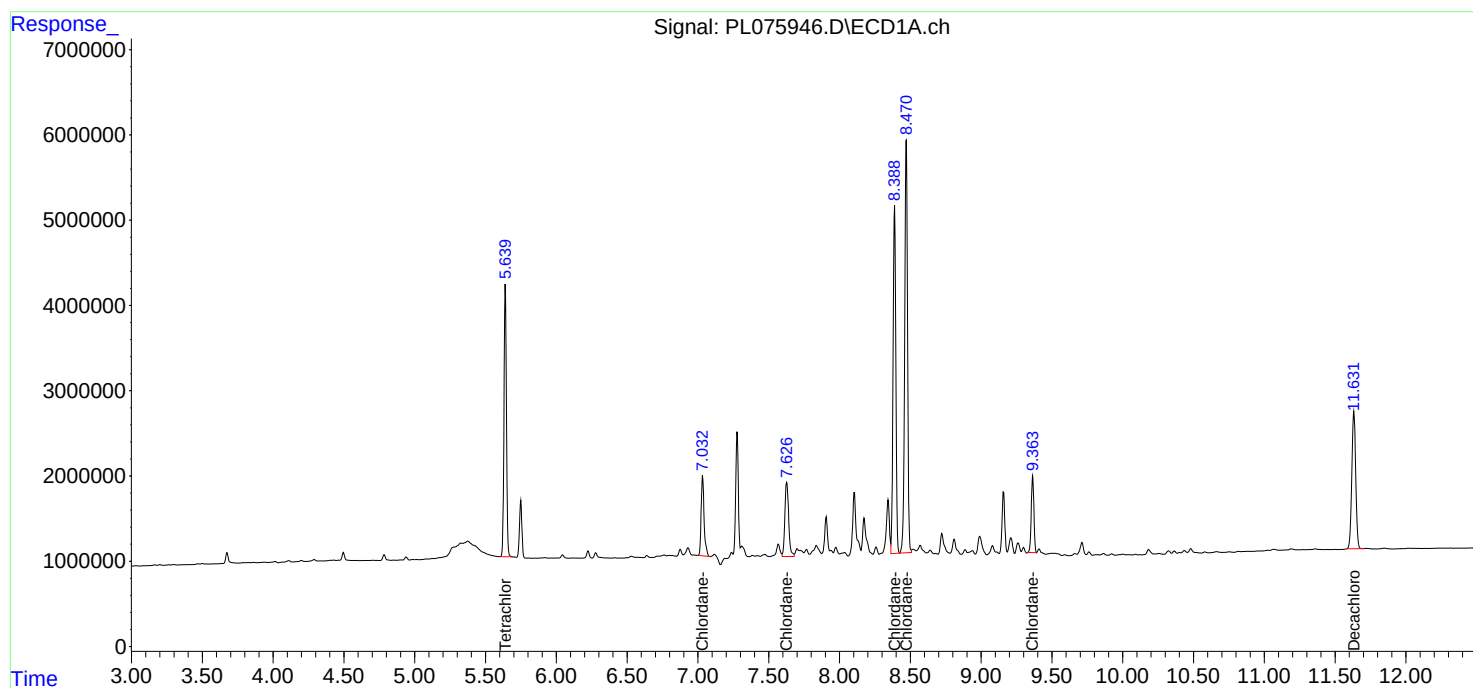


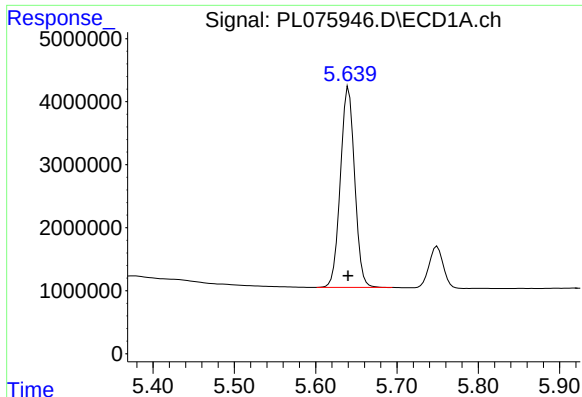

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 38699470
Conc: 54.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL062322

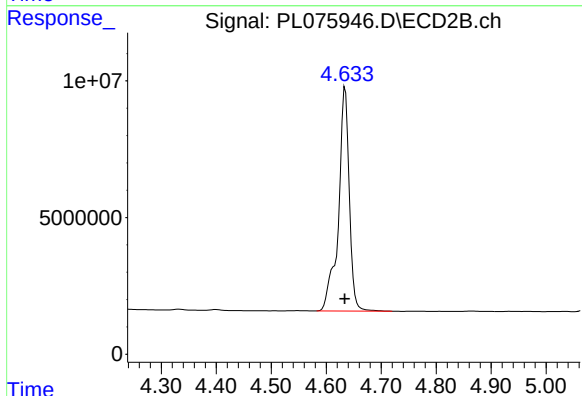


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: 0.000 min
Response: 113090490
Conc: 53.66 ng/ml

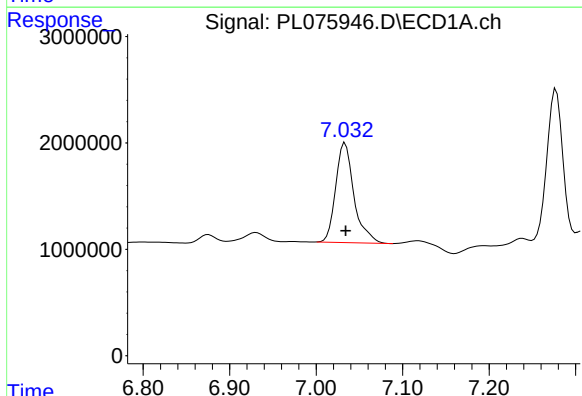


#23 Chlordane-1

R.T.: 7.034 min
Delta R.T.: 0.000 min
Response: 13715355
Conc: 541.93 ng/ml

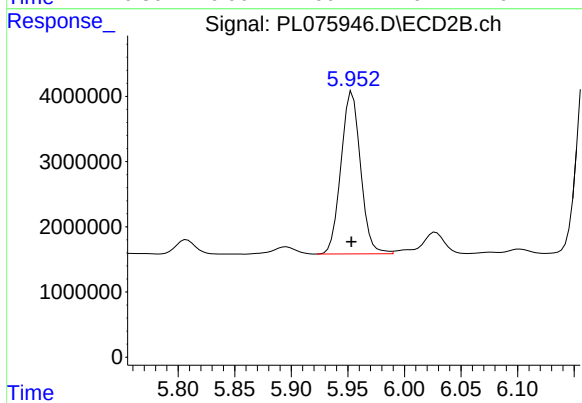

#23 Chlordane-1


R.T.: 5.954 min
Delta R.T.: 0.000 min
Response: 29974803
Conc: 535.38 ng/ml

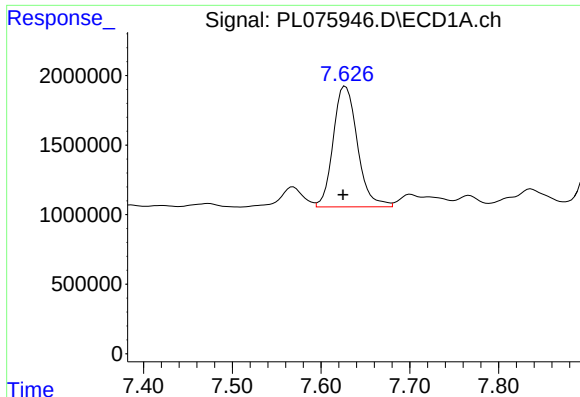

#24 Chlordane-2


R.T.: 7.628 min
Delta R.T.: 0.003 min
Response: 16458439
Conc: 542.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL062322

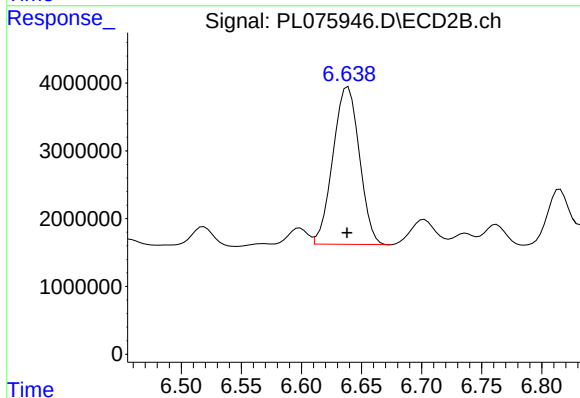


#24 Chlordane-2

R.T.: 6.639 min
Delta R.T.: 0.000 min
Response: 35710113
Conc: 513.55 ng/ml

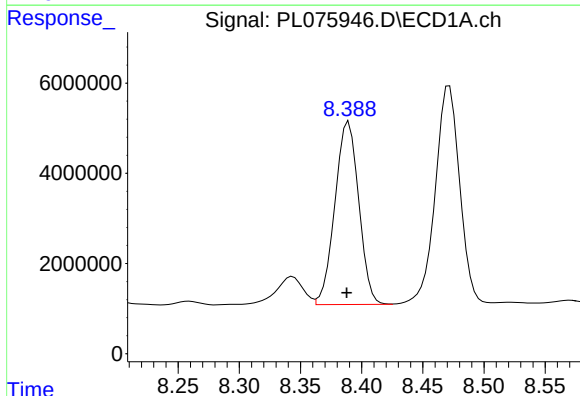


#25 Chlordane-3

R.T.: 8.389 min
Delta R.T.: 0.002 min
Response: 54999115
Conc: 540.85 ng/ml

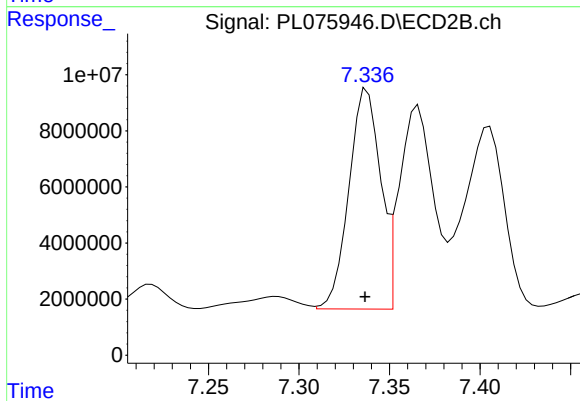

#25 Chlordane-3


R.T.: 7.338 min
Delta R.T.: 0.001 min
Response: 95095521
Conc: 539.20 ng/ml

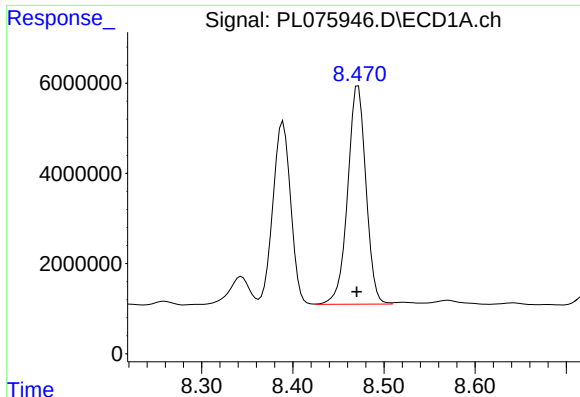

#26 Chlordane-4


R.T.: 8.472 min
Delta R.T.: 0.002 min
Response: 67386239
Conc: 541.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL062322

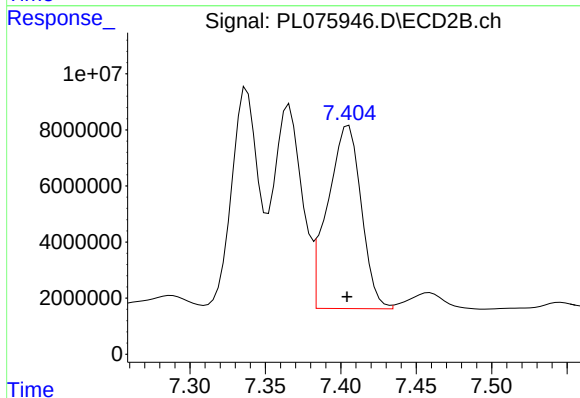


#26 Chlordane-4

R.T.: 7.405 min
Delta R.T.: 0.001 min
Response: 100999307
Conc: 535.75 ng/ml

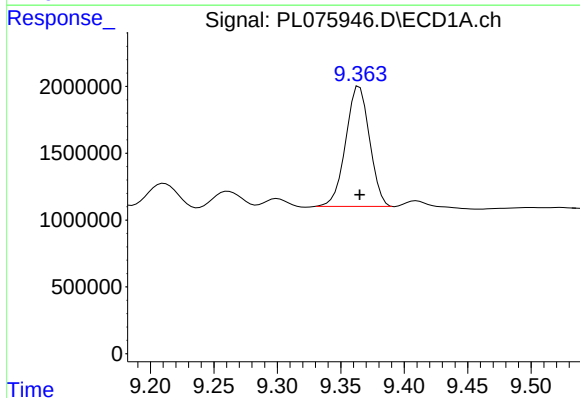


#27 Chlordane-5

R.T.: 9.365 min
Delta R.T.: 0.000 min
Response: 11726997
Conc: 549.59 ng/ml

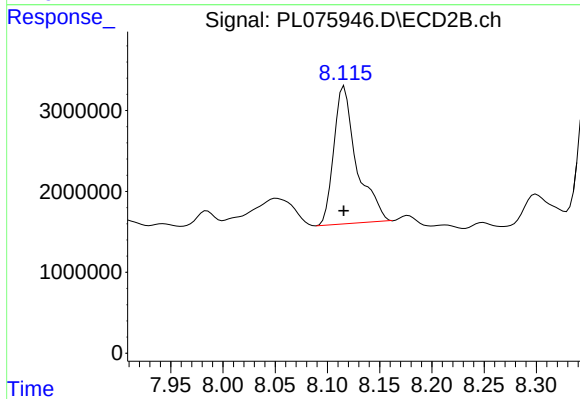

#27 Chlordane-5


R.T.: 8.116 min
Delta R.T.: 0.000 min
Response: 25752449
Conc: 562.85 ng/ml

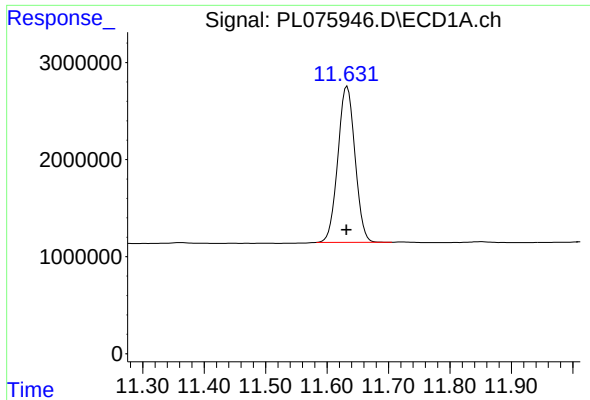

#28 Decachlorobiphenyl

R.T.: 11.633 min
Delta R.T.: 0.001 min
Response: 31198770
Conc: 52.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL062322

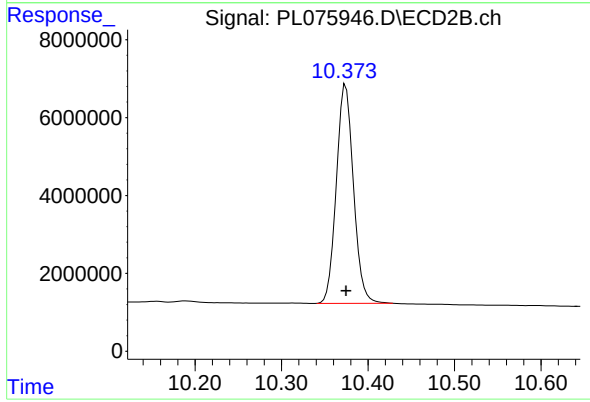

#28 Decachlorobiphenyl

R.T.: 10.374 min
Delta R.T.: 0.000 min
Response: 76968116
Conc: 52.46 ng/ml