

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
 Data File : PL075953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2022 00:33
 Operator : AR\AJ
 Sample : N3422-01 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-14A-1A-12

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/27/2022
 Supervised By :Ankita Jodhani 06/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 05:15:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.639	4.635	1194585	2305408	1.579m	1.216
28) SA Decachlor...	11.630	10.378	2114163	3633810	3.360m	2.366 #
Target Compounds						
16) A 4,4'-DDD	9.196	8.200	357092	817867	0.630m	0.590

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
Data File : PL075953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2022 00:33
Operator : AR\AJ
Sample : N3422-01 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-14A-1A-12


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/27/2022
Supervised By : Ankita Jodhani 06/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 05:15:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

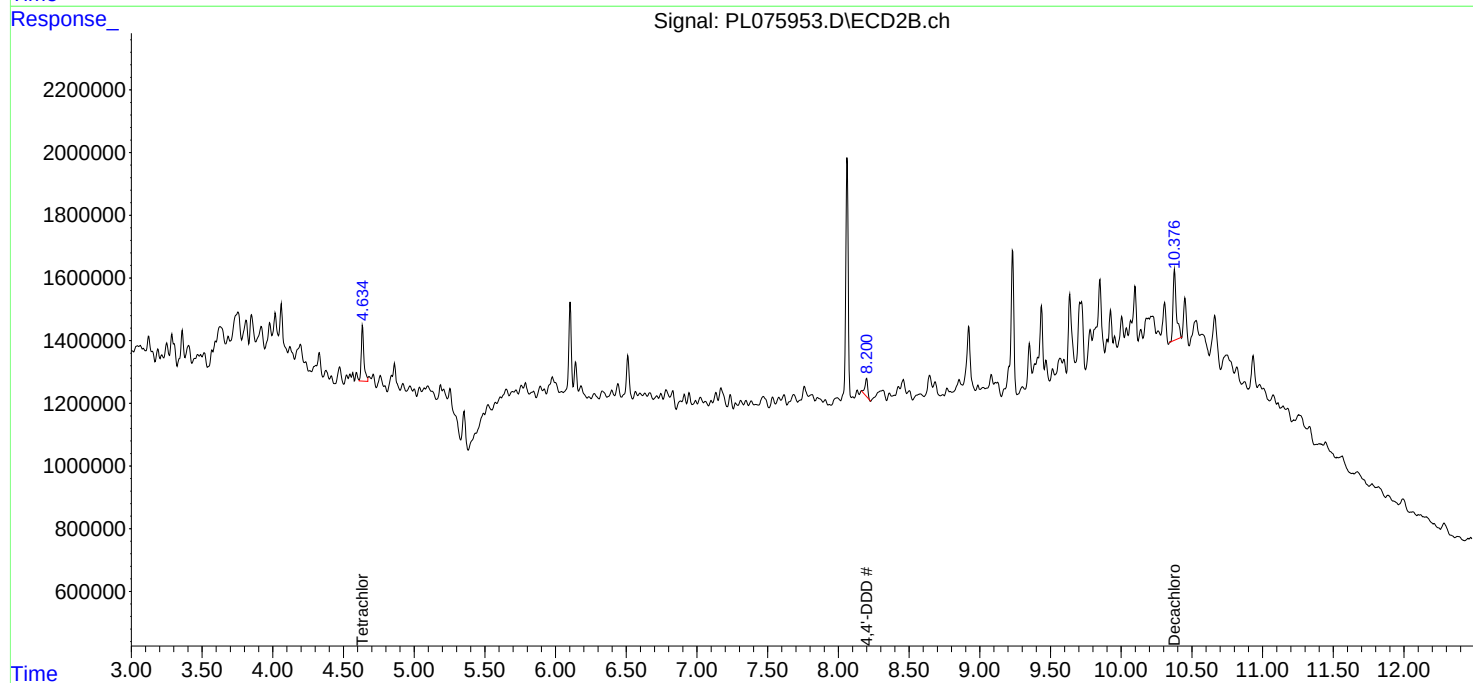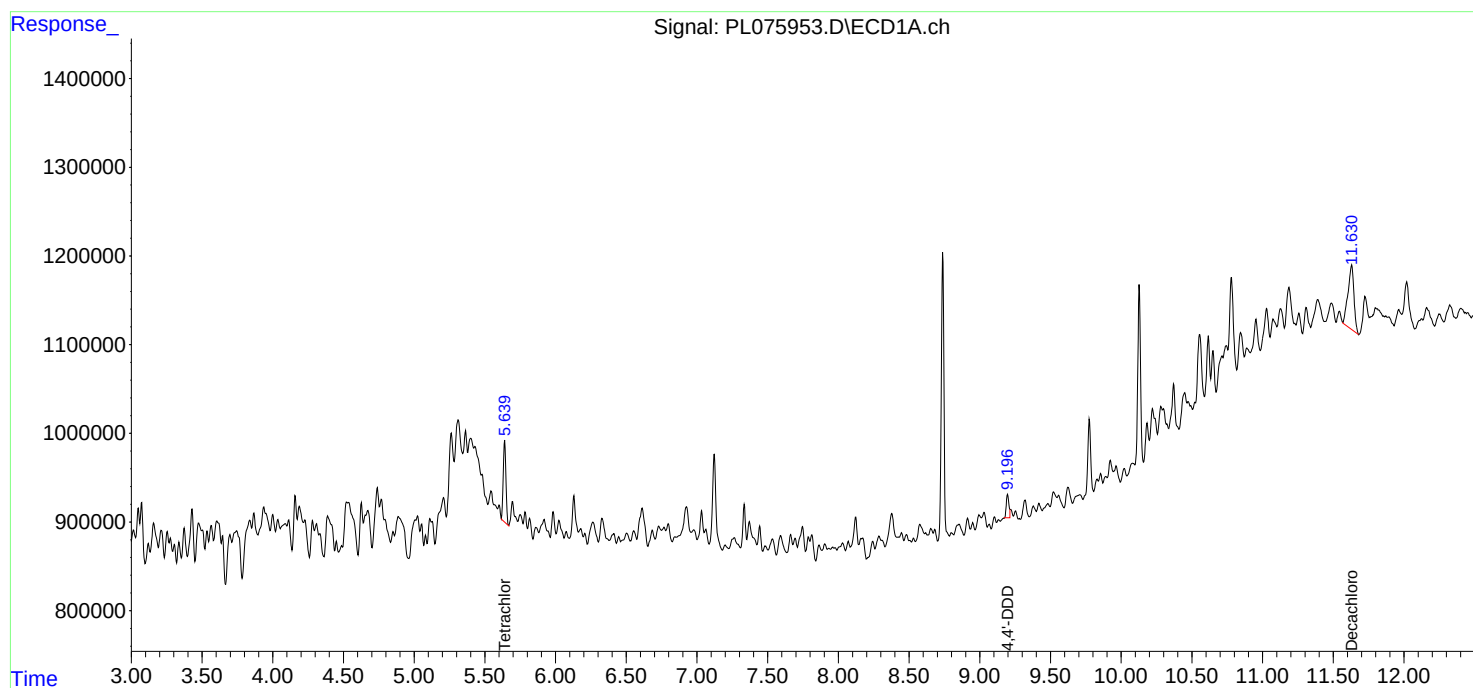

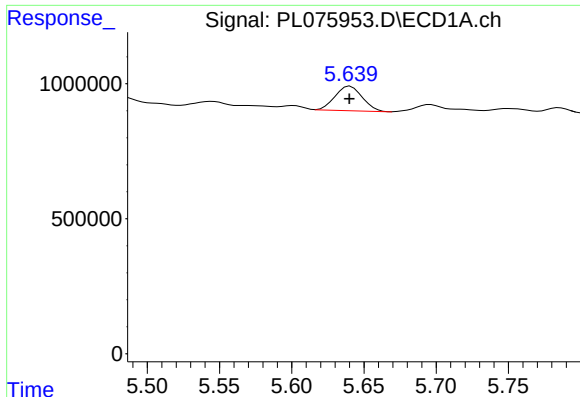


#1 Tetrachloro-m-xylene

R.T.: 5.639 min
Delta R.T.: 0.000 min
Response: 1194585
Conc: 1.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-14A-1A-12


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/27/2022
Supervised By :Ankita Jodhani 06/27/2022

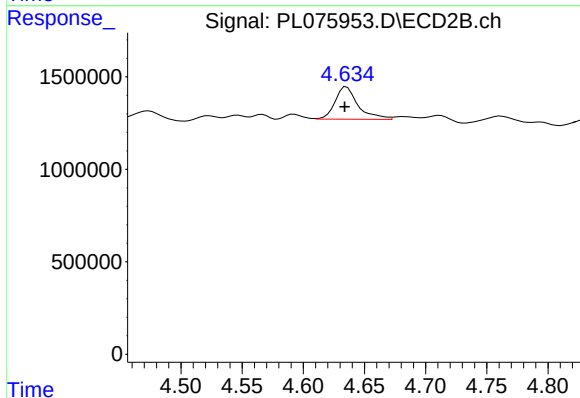


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: 0.002 min
Response: 2305408
Conc: 1.22 ng/ml

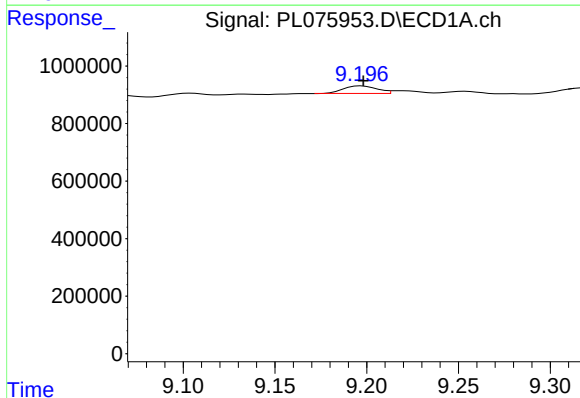


#16 4,4'-DDD

R.T.: 9.196 min
Delta R.T.: -0.002 min
Response: 357092
Conc: 0.63 ng/ml m

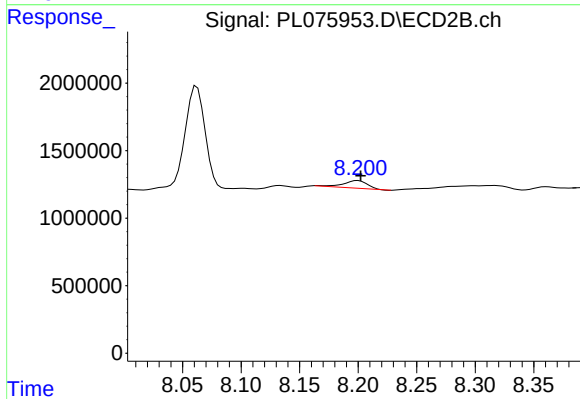

#16 4,4'-DDD

R.T.: 8.200 min
Delta R.T.: -0.002 min
Response: 817867
Conc: 0.59 ng/ml

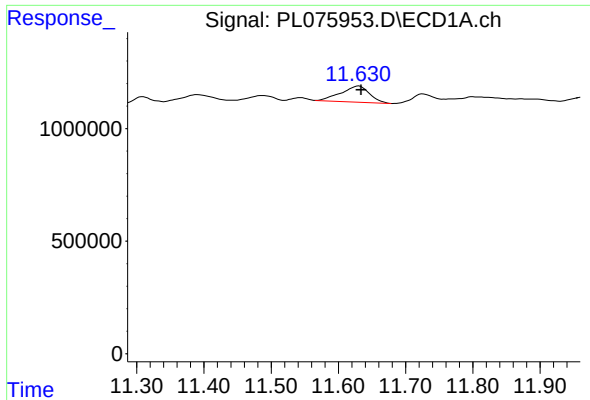


#28 Decachlorobiphenyl

R.T.: 11.630 min
Delta R.T.: -0.004 min
Response: 2114163
Conc: 3.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-14A-1A-12

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/27/2022
Supervised By :Ankita Jodhani 06/27/2022

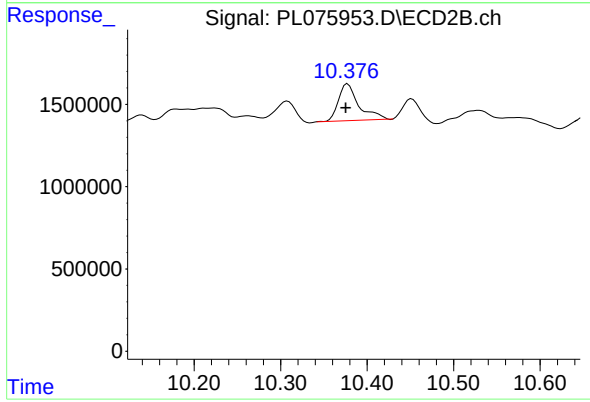

#28 Decachlorobiphenyl

R.T.: 10.378 min
Delta R.T.: 0.002 min
Response: 3633810
Conc: 2.37 ng/ml