

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
 Data File : PL075956.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2022 01:22
 Operator : AR\AJ
 Sample : N3428-01 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-01-062122

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/24/2022
 Supervised By : Ankita Jodhani 06/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 05:16:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.635	1482757	3936851	1.960m	2.076
28)	SA Decachlor...	11.633	10.375	2657047	3477295	4.222m	2.264 #
Target Compounds							
10)	B gamma-Chl...	8.384	7.336	1435660	686562	1.847	0.357m#
11)	B alpha-Chl...	8.473	7.404	356447	695347	0.459	0.363m
13)	MA Dieldrin	8.818	7.757	231826	2947671	0.316	1.638 #
17)	MA 4,4'-DDT	9.522	8.461	491511	959015	0.805m	0.648m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
Data File : PL075956.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2022 01:22
Operator : AR\AJ
Sample : N3428-01 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CL-01-062122


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/24/2022
Supervised By :Ankita Jodhani 06/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 05:16:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

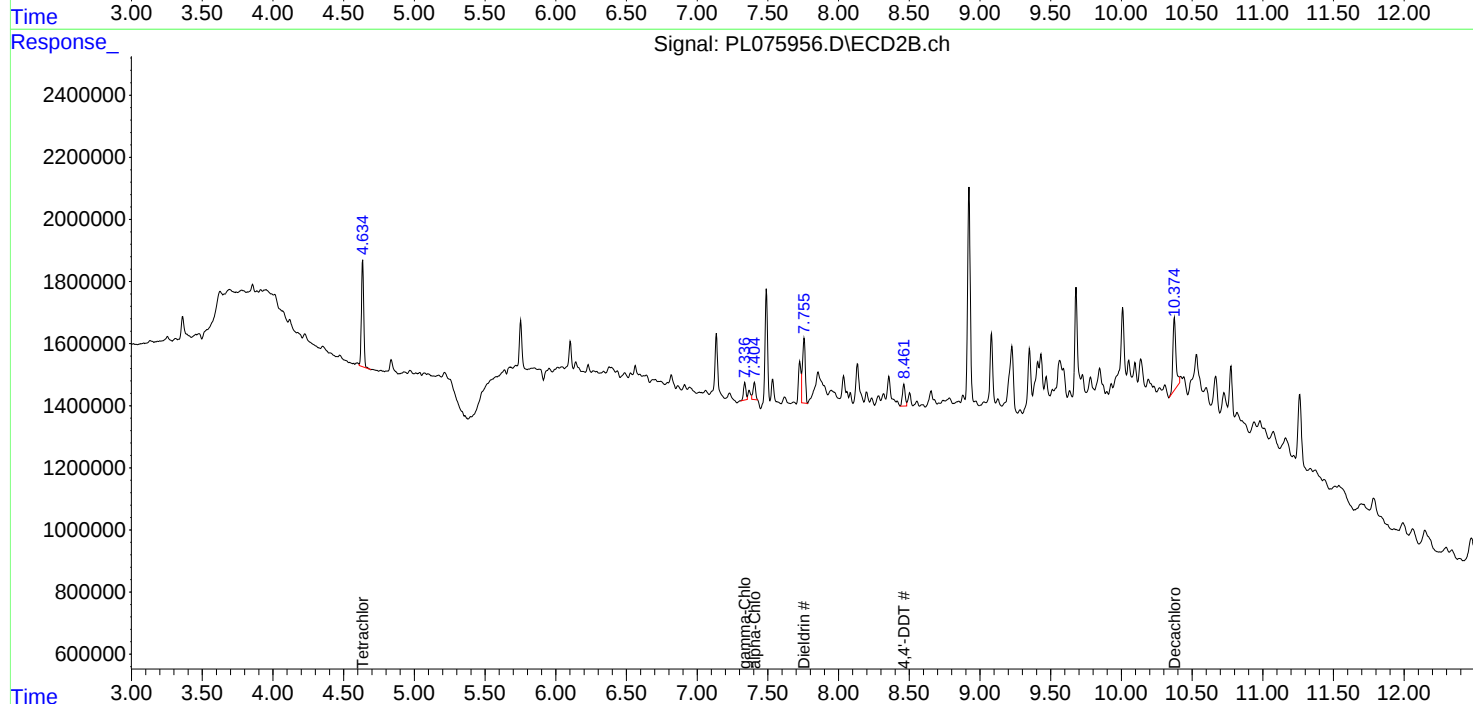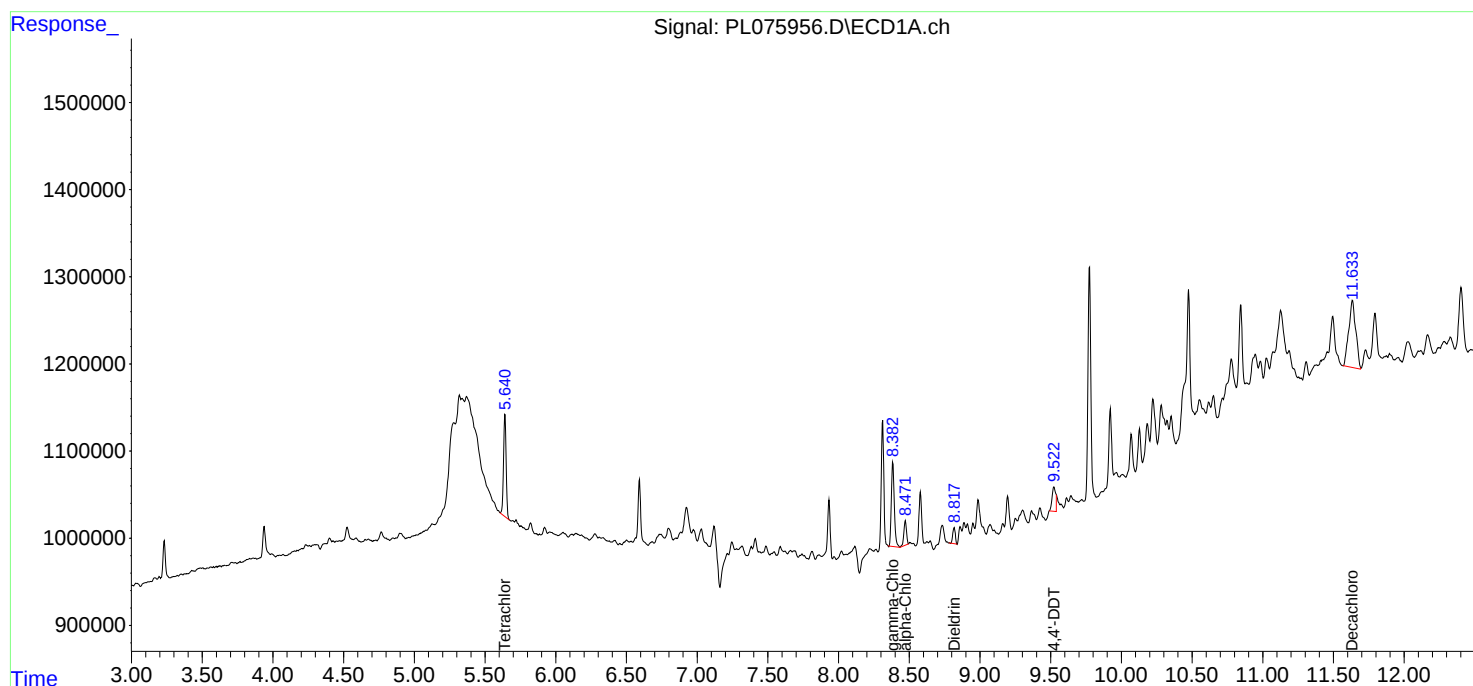

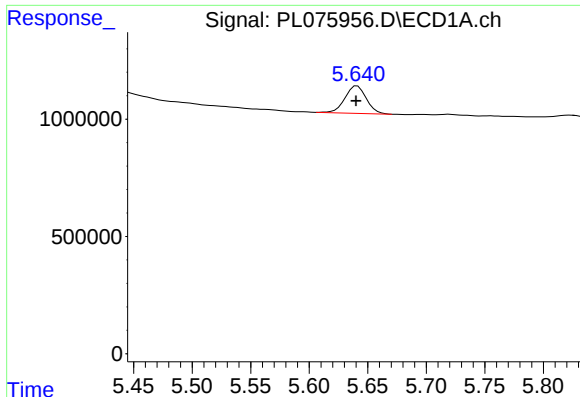


#1 Tetrachloro-m-xylene

R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 1482757
Conc: 1.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-062122


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/24/2022
Supervised By :Ankita Jodhani 06/24/2022

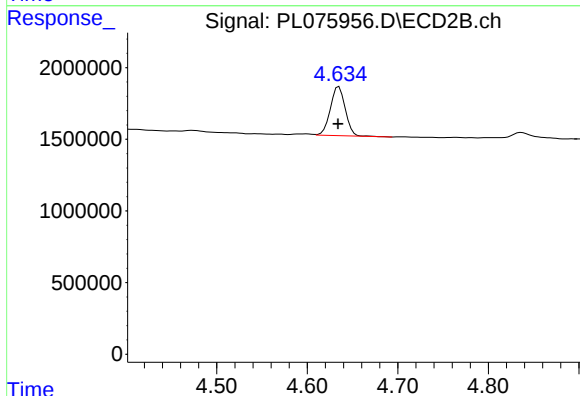


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: 0.001 min
Response: 3936851
Conc: 2.08 ng/ml

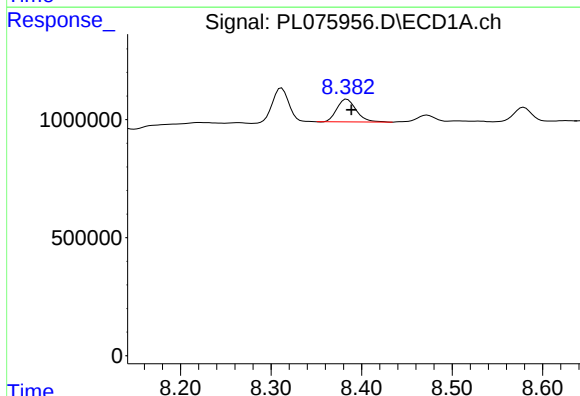


#10 gamma-Chlordane

R.T.: 8.384 min
Delta R.T.: -0.005 min
Response: 1435660
Conc: 1.85 ng/ml

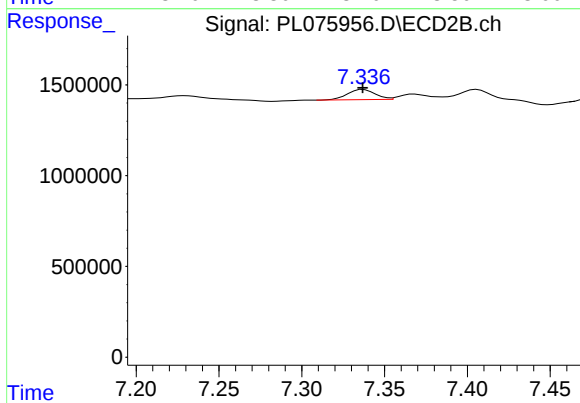

#10 gamma-Chlordane

R.T.: 7.336 min
Delta R.T.: -0.001 min
Response: 686562
Conc: 0.36 ng/ml m

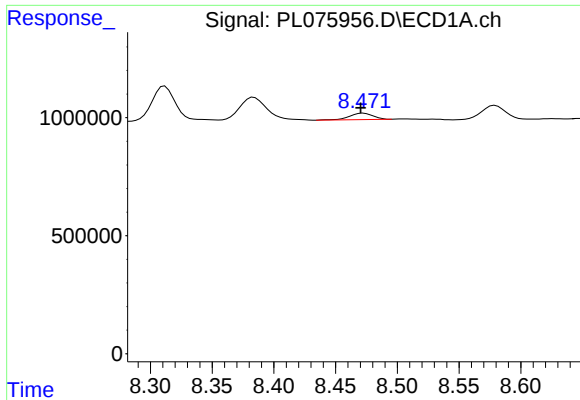


#11 alpha-Chlordane

R.T.: 8.473 min
Delta R.T.: 0.002 min
Response: 356447
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-062122


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/24/2022
Supervised By :Ankita Jodhani 06/24/2022

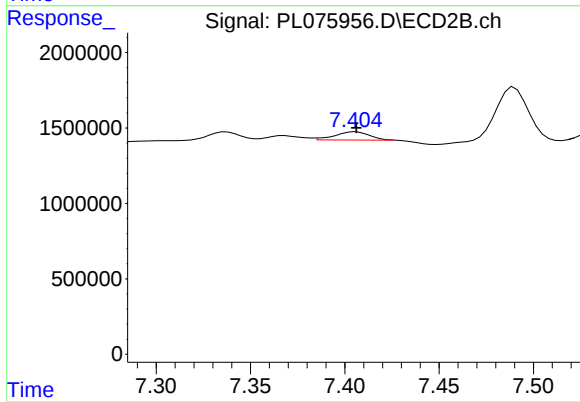


#11 alpha-Chlordane

R.T.: 7.404 min
Delta R.T.: -0.002 min
Response: 695347
Conc: 0.36 ng/ml m

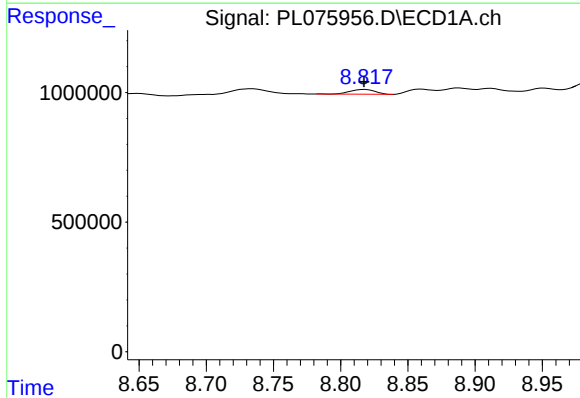


#13 Dieldrin

R.T.: 8.818 min
Delta R.T.: 0.000 min
Response: 231826
Conc: 0.32 ng/ml

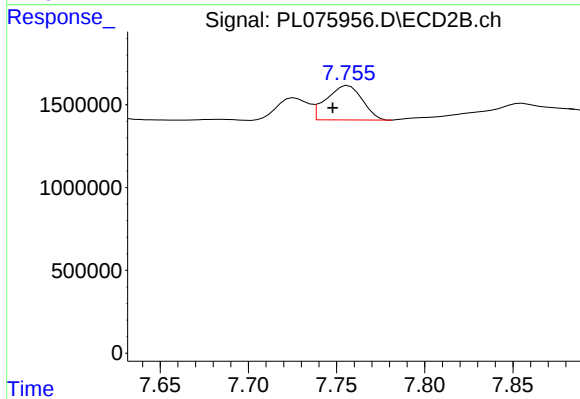

#13 Dieldrin

R.T.: 7.757 min
Delta R.T.: 0.009 min
Response: 2947671
Conc: 1.64 ng/ml

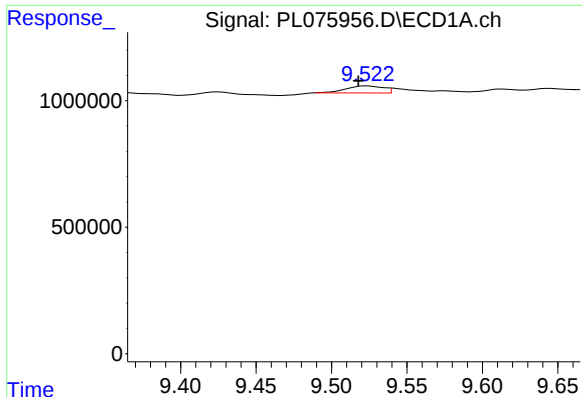


#17 4,4'-DDT

R.T.: 9.522 min
Delta R.T.: 0.004 min
Response: 491511
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-062122


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/24/2022
Supervised By :Ankita Jodhani 06/24/2022

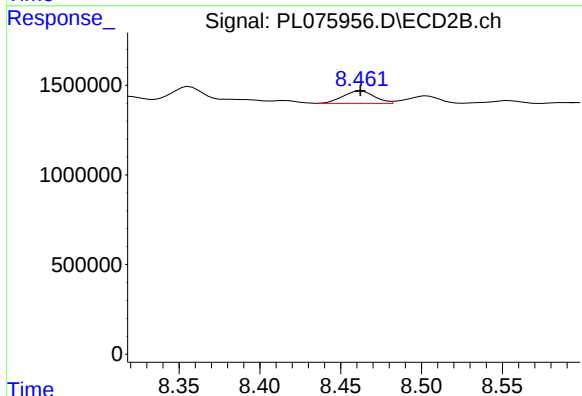


#17 4,4'-DDT

R.T.: 8.461 min
Delta R.T.: 0.000 min
Response: 959015
Conc: 0.65 ng/ml m

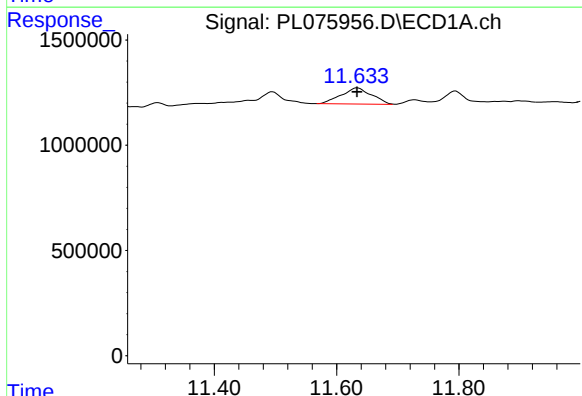

#28 Decachlorobiphenyl

R.T.: 11.633 min
Delta R.T.: 0.000 min
Response: 2657047
Conc: 4.22 ng/ml m

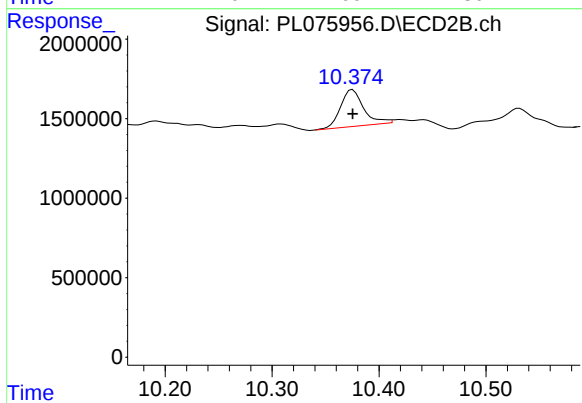

#28 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: 0.000 min
Response: 3477295
Conc: 2.26 ng/ml