

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062325\
 Data File : PL096146.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2025 14:21
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 14:32:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062325.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 23 14:31:56 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.880	79033190	135.9E6	25.582	25.355
28)	SA Decachlor...	9.111	8.062	62382294	128.1E6	26.268	25.667
Target Compounds							
23)	Chlordane-1	4.736	3.897	49478389	52657895	258.172	252.524
24)	Chlordane-2	5.263	4.478	50820202	59861394	261.261	256.500
25)	Chlordane-3	5.969	5.114	189.9E6	176.7E6	247.872	243.297
26)	Chlordane-4	6.053	5.178	225.8E6	158.9E6	249.707	248.927
27)	Chlordane-5	6.894	6.076	40903466	67588979	256.034	249.520



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062325\
Data File : PL096146.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2025 14:21
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 14:32:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062325.M
Quant Title : GC Extractables
QLast Update : Mon Jun 23 14:31:56 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

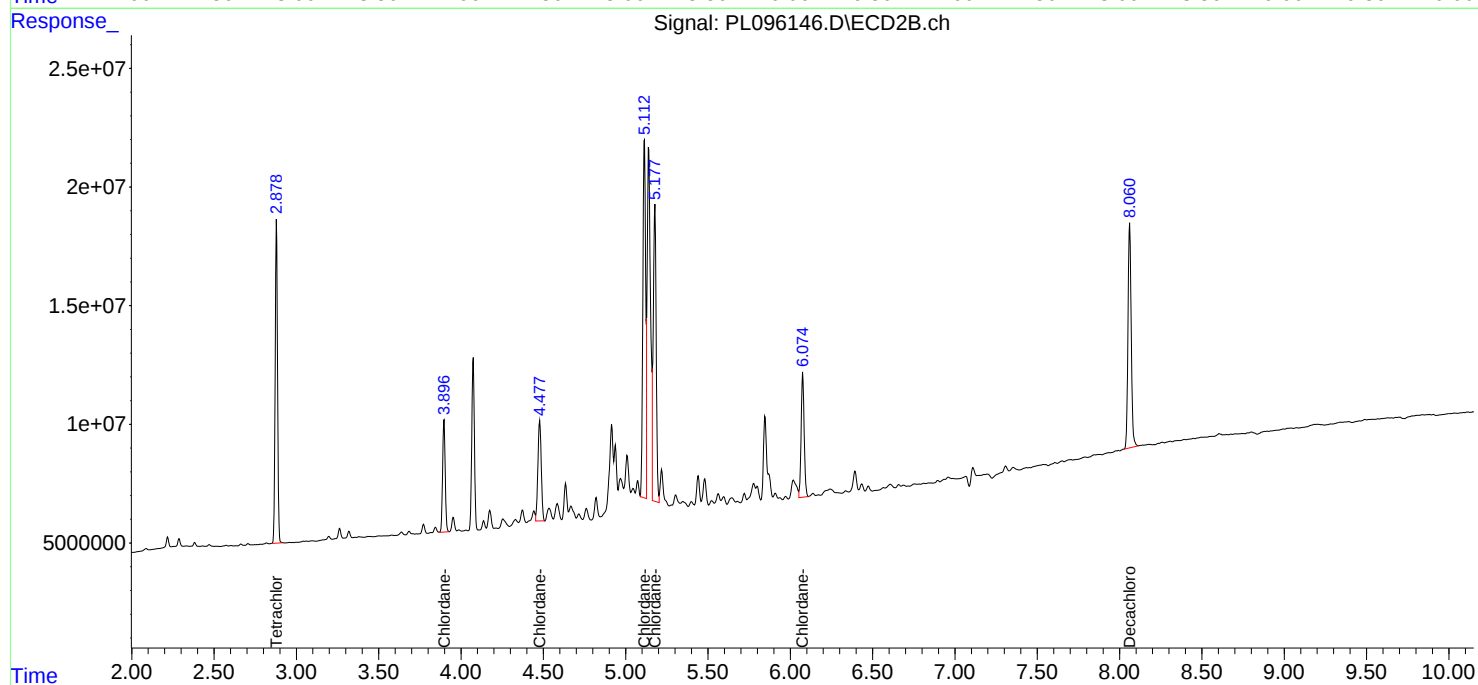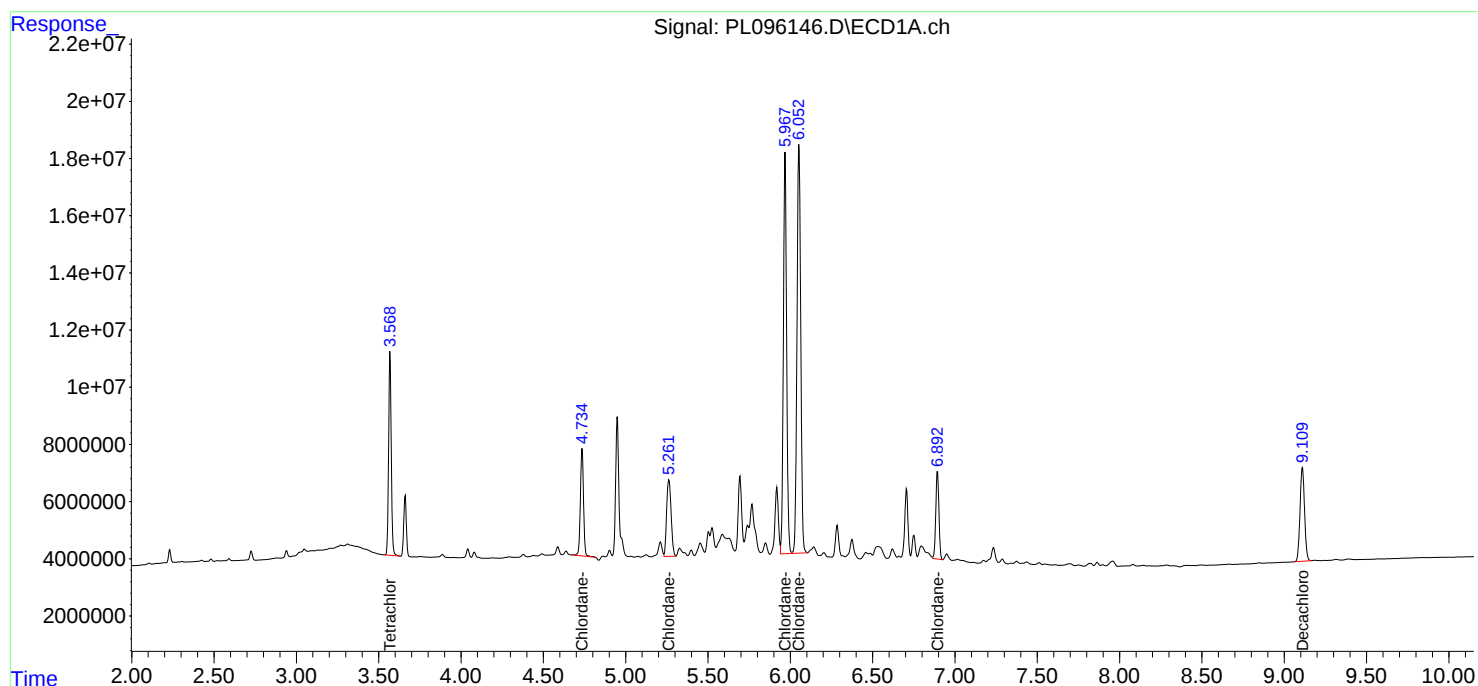


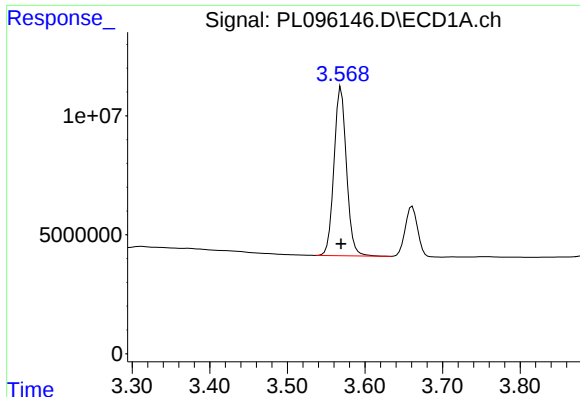

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 79033190
Conc: 25.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

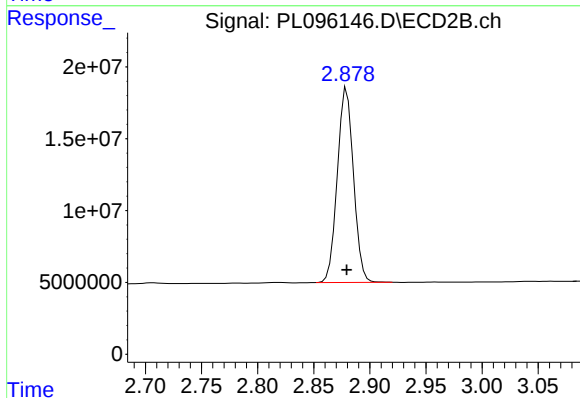


#1 Tetrachloro-m-xylene

R.T.: 2.880 min
Delta R.T.: 0.000 min
Response: 135920208
Conc: 25.35 ng/ml

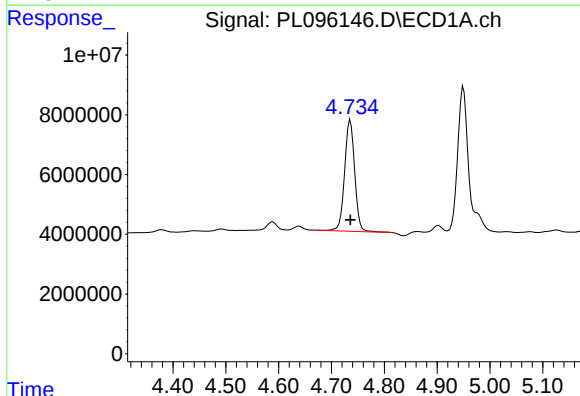


#23 Chlordane-1

R.T.: 4.736 min
Delta R.T.: 0.000 min
Response: 49478389
Conc: 258.17 ng/ml

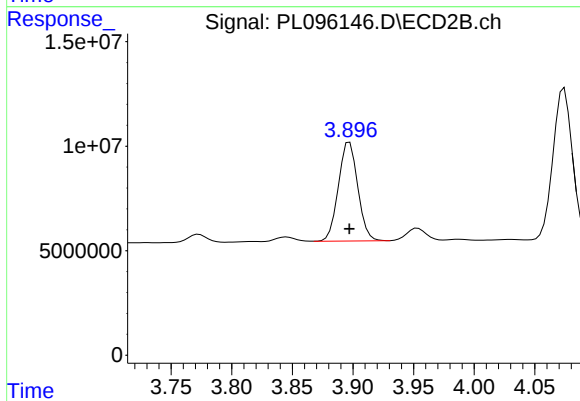

#23 Chlordane-1


R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 52657895
Conc: 252.52 ng/ml

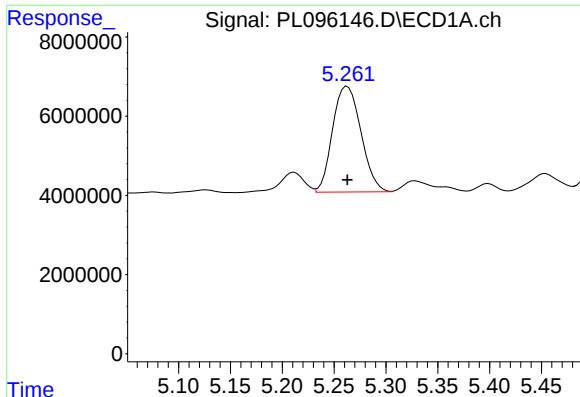

#24 Chlordane-2


R.T.: 5.263 min
Delta R.T.: 0.000 min
Response: 50820202
Conc: 261.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

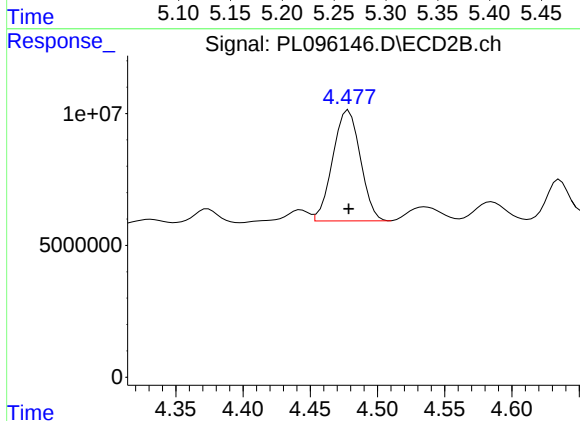


#24 Chlordane-2

R.T.: 4.478 min
Delta R.T.: 0.000 min
Response: 59861394
Conc: 256.50 ng/ml

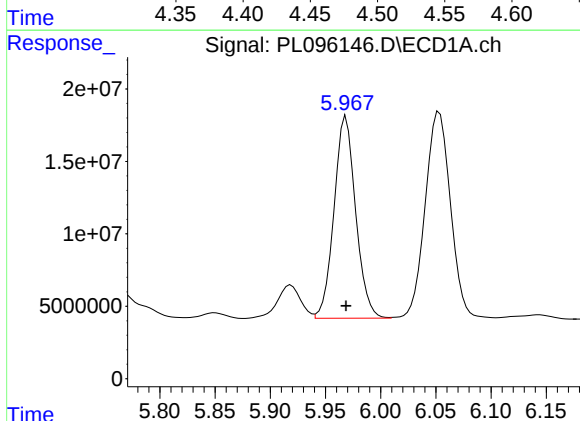


#25 Chlordane-3

R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 189900195
Conc: 247.87 ng/ml

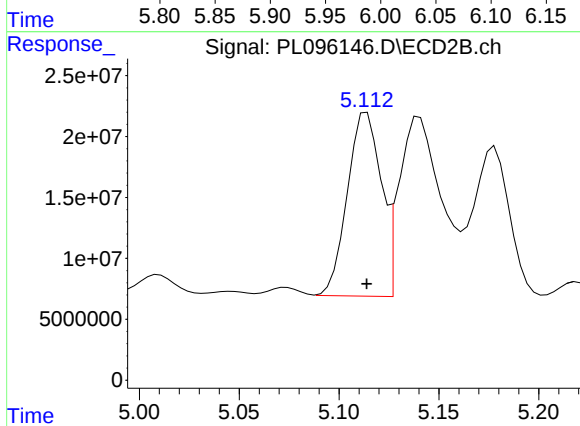

#25 Chlordane-3


R.T.: 5.114 min
Delta R.T.: 0.000 min
Response: 176688926
Conc: 243.30 ng/ml

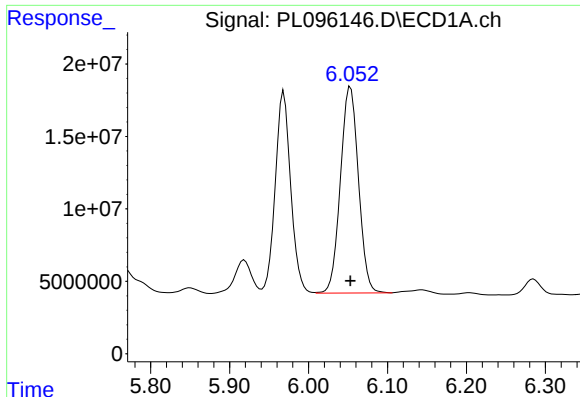

#26 Chlordane-4


R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 225829811
Conc: 249.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

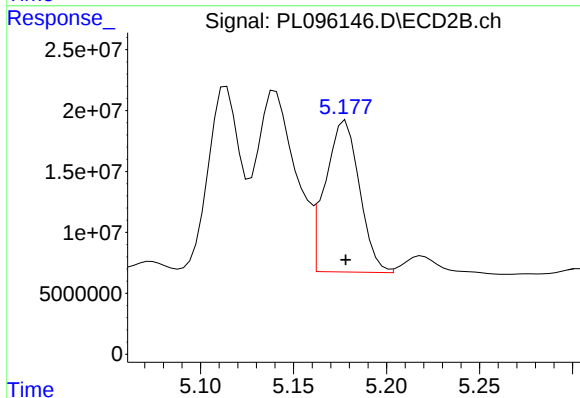


#26 Chlordane-4

R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 158861994
Conc: 248.93 ng/ml

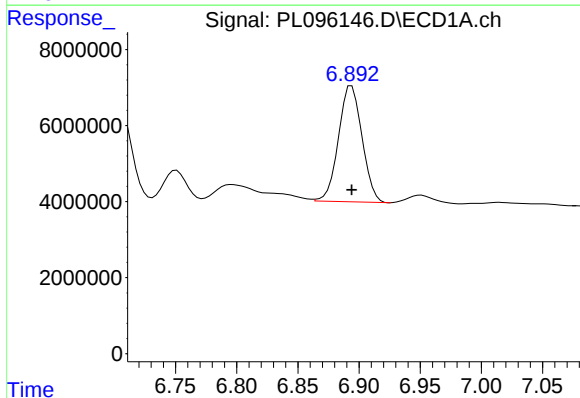


#27 Chlordane-5

R.T.: 6.894 min
Delta R.T.: 0.000 min
Response: 40903466
Conc: 256.03 ng/ml

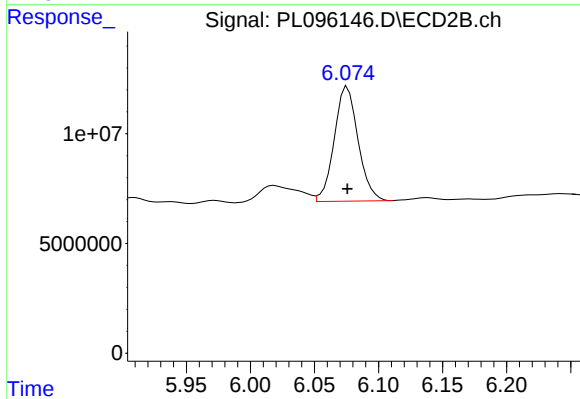

#27 Chlordane-5


R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 67588979
Conc: 249.52 ng/ml

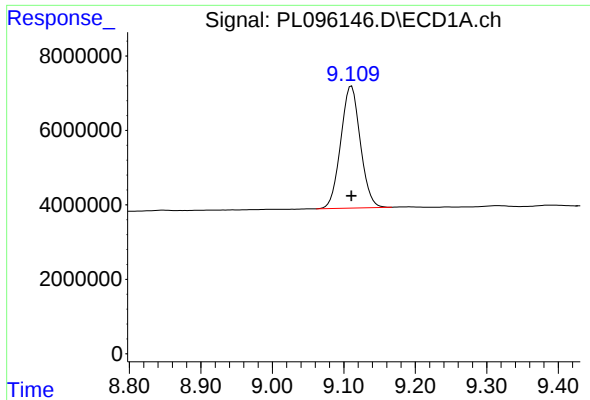

#28 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 62382294
Conc: 26.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

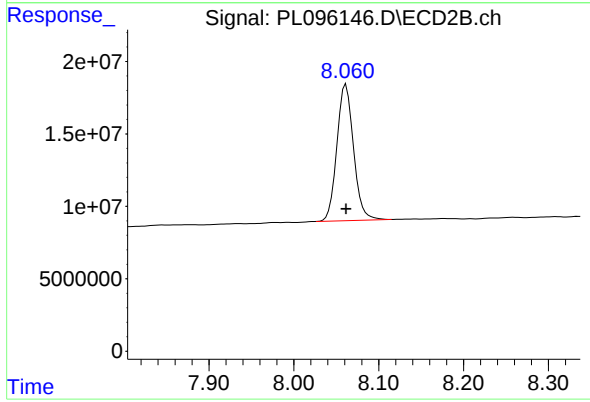

#28 Decachlorobiphenyl

R.T.: 8.062 min
Delta R.T.: 0.000 min
Response: 128082973
Conc: 25.67 ng/ml