

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062325\
 Data File : PL096145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2025 14:07
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 14:19:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062325.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 23 14:18:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.880	155.5E6	269.4E6	50.000	50.000
28)	SA Decachlor...	9.111	8.062	120.6E6	253.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.736	3.897	96848330	105.2E6	500.000	500.000
24)	Chlordane-2	5.264	4.478	98202553	117.6E6	500.000	500.000
25)	Chlordane-3	5.969	5.114	386.9E6	366.3E6	500.000	500.000
26)	Chlordane-4	6.054	5.178	456.3E6	320.5E6	500.000	500.000
27)	Chlordane-5	6.895	6.076	80803072	136.7E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062325\
Data File : PL096145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2025 14:07
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 14:19:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062325.M
Quant Title : GC Extractables
QLast Update : Mon Jun 23 14:18:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

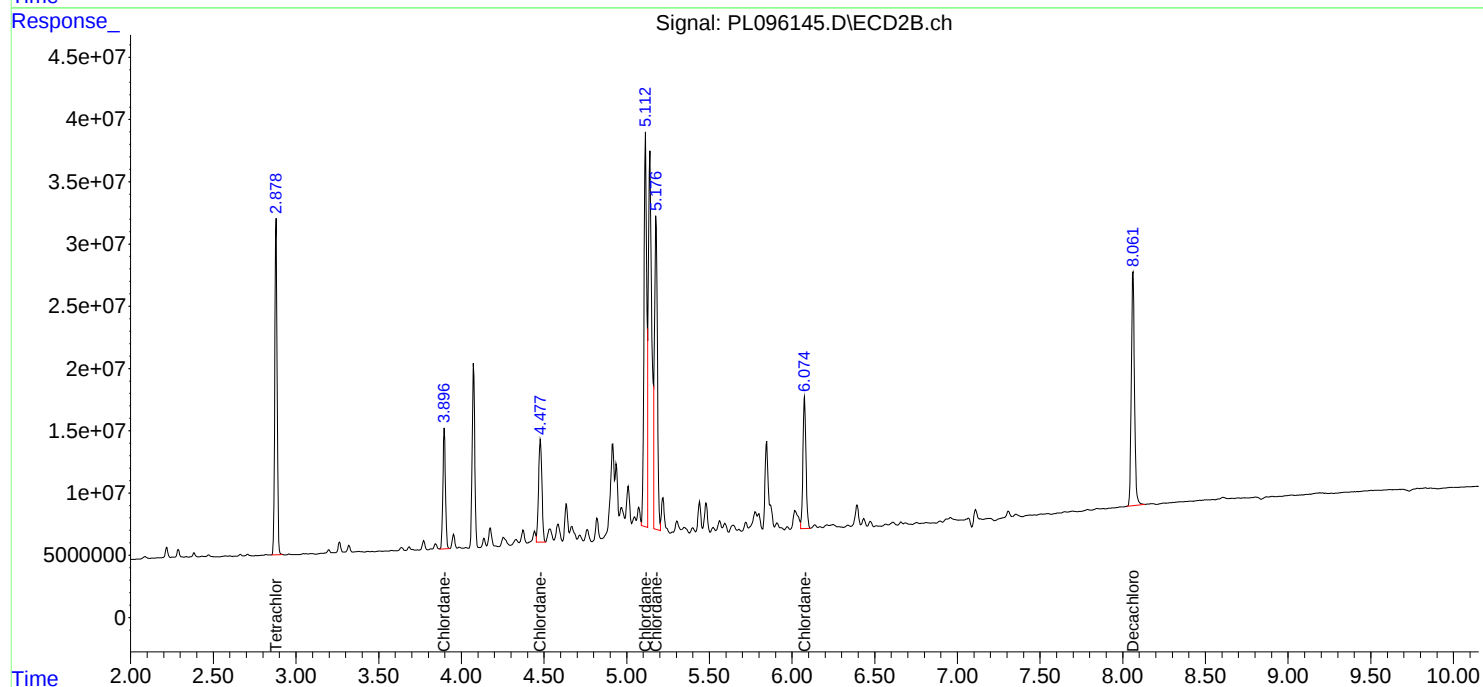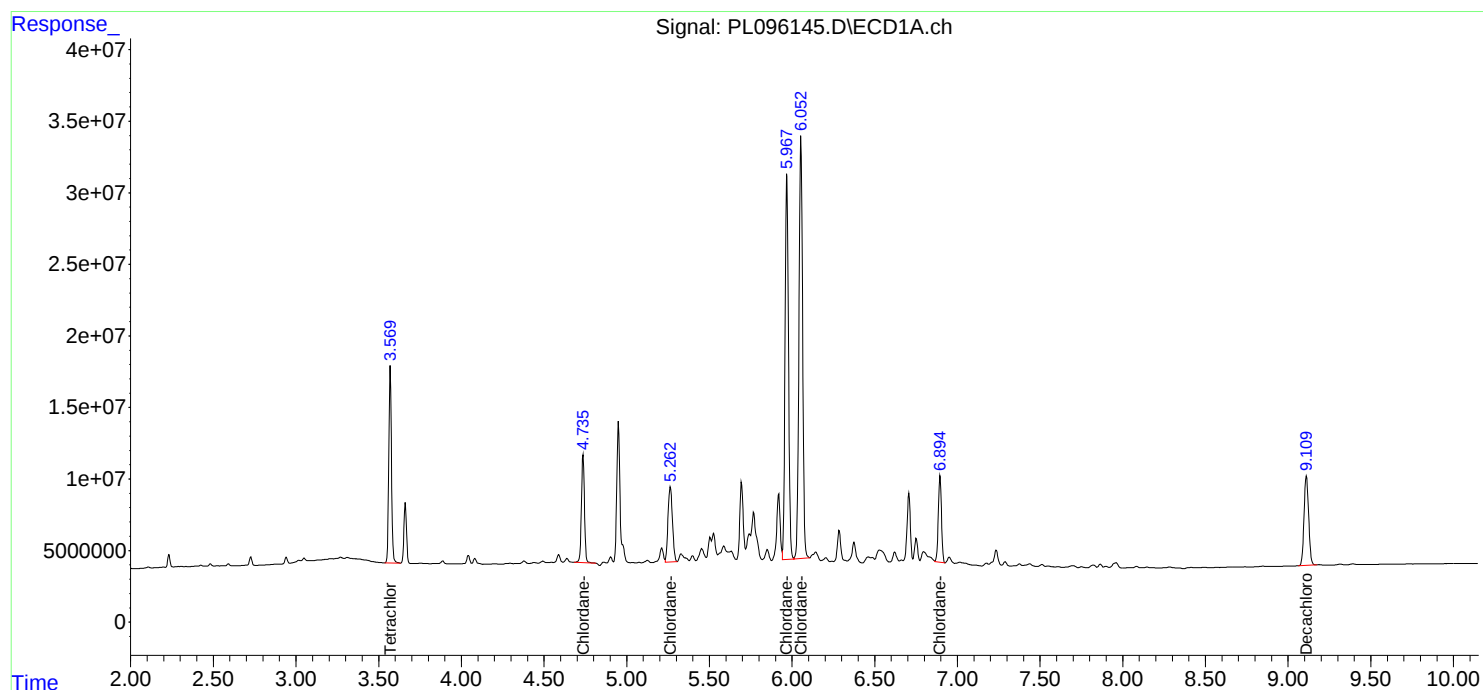


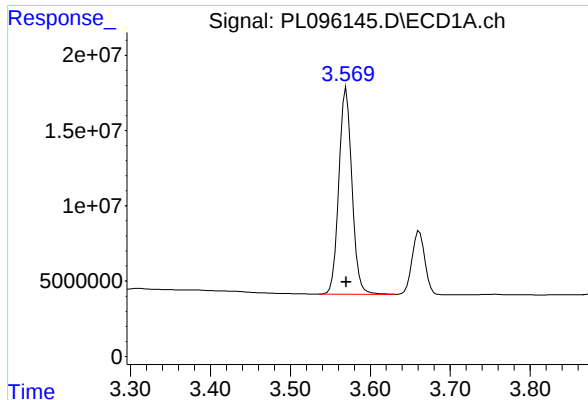

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 155542660
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

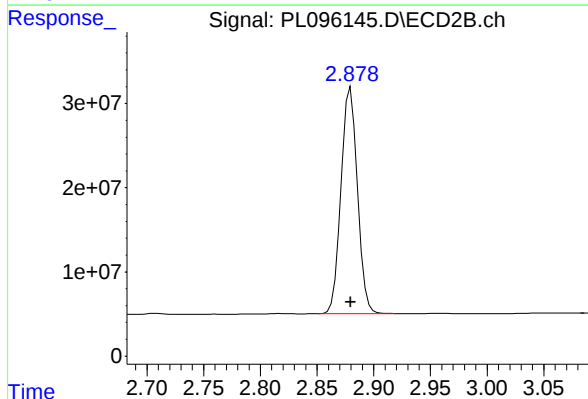


#1 Tetrachloro-m-xylene

R.T.: 2.880 min
Delta R.T.: 0.000 min
Response: 269379361
Conc: 50.00 ng/ml

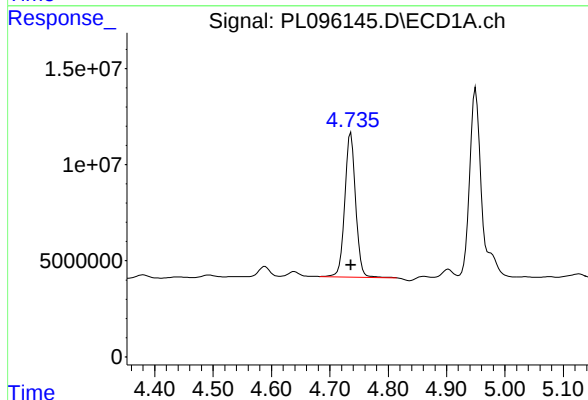


#23 Chlordane-1

R.T.: 4.736 min
Delta R.T.: 0.000 min
Response: 96848330
Conc: 500.00 ng/ml

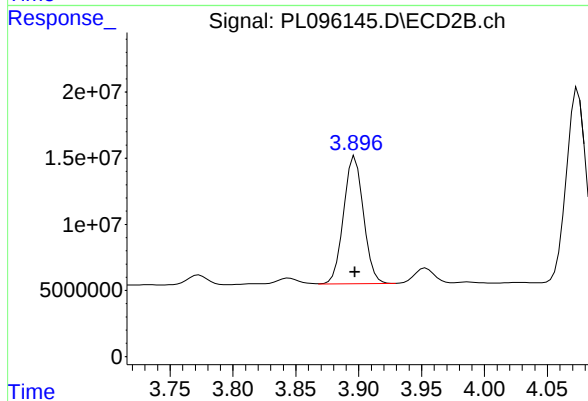

#23 Chlordane-1


R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 105236672
Conc: 500.00 ng/ml

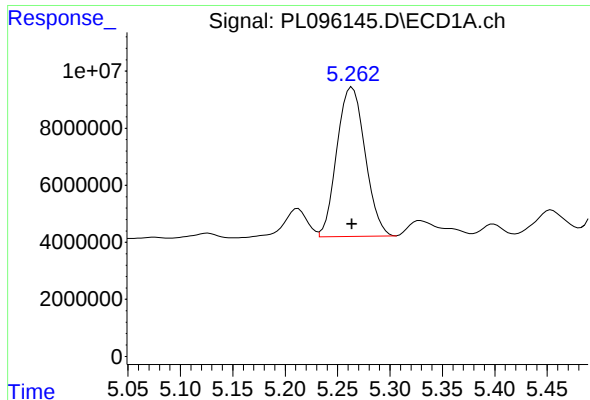

#24 Chlordane-2


R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 98202553
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

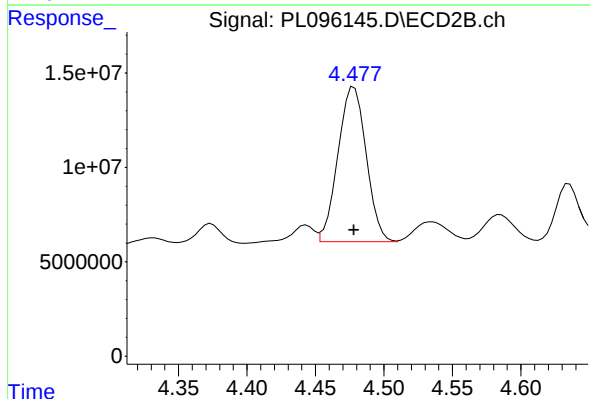


#24 Chlordane-2

R.T.: 4.478 min
Delta R.T.: 0.000 min
Response: 117573101
Conc: 500.00 ng/ml

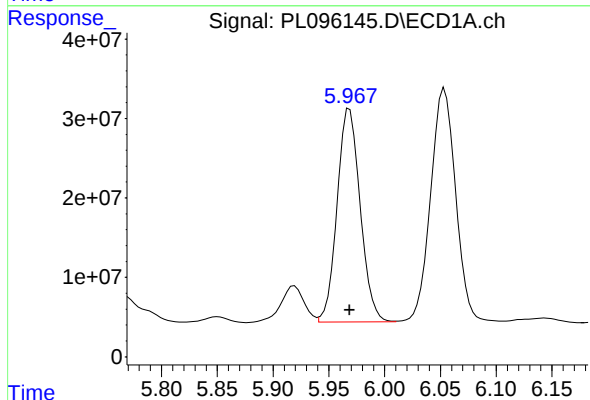


#25 Chlordane-3

R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 386867932
Conc: 500.00 ng/ml

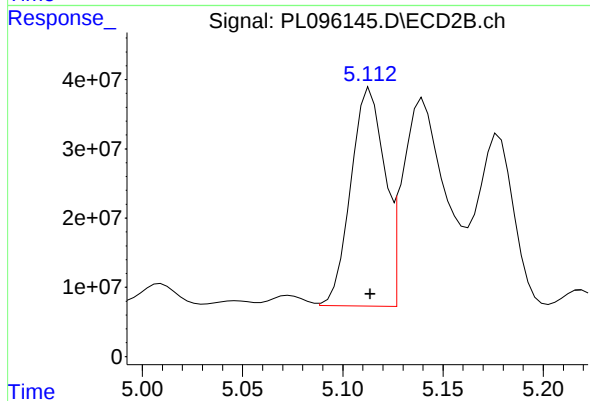

#25 Chlordane-3


R.T.: 5.114 min
Delta R.T.: 0.000 min
Response: 366324097
Conc: 500.00 ng/ml

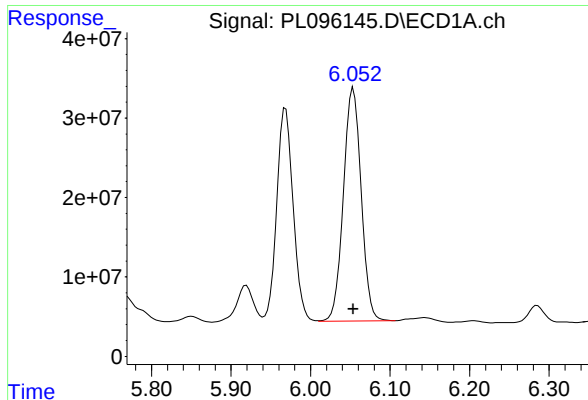

#26 Chlordane-4


R.T.: 6.054 min
Delta R.T.: 0.000 min
Response: 456260187
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

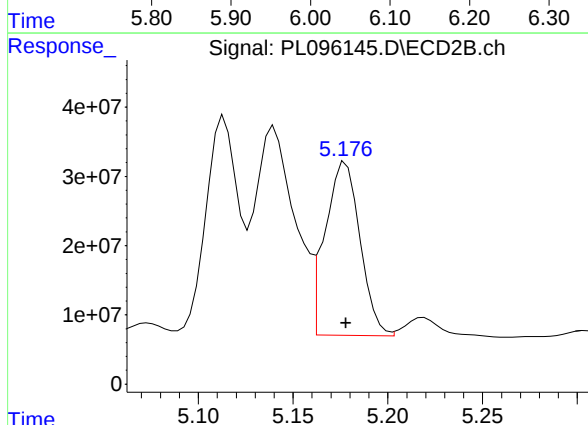


#26 Chlordane-4

R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 320459367
Conc: 500.00 ng/ml

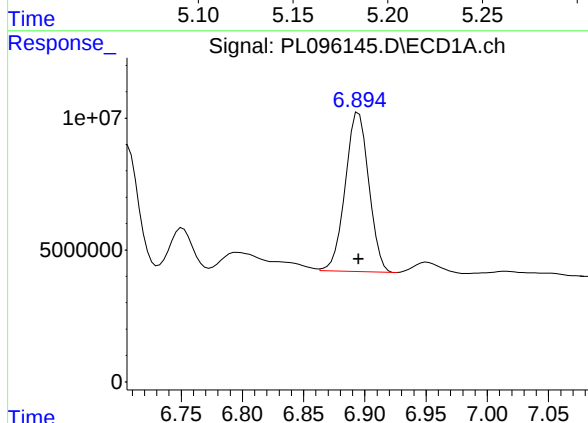


#27 Chlordane-5

R.T.: 6.895 min
Delta R.T.: 0.000 min
Response: 80803072
Conc: 500.00 ng/ml

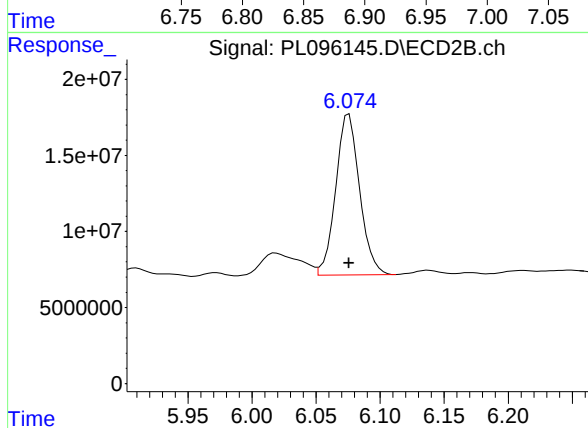

#27 Chlordane-5


R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 136728380
Conc: 500.00 ng/ml

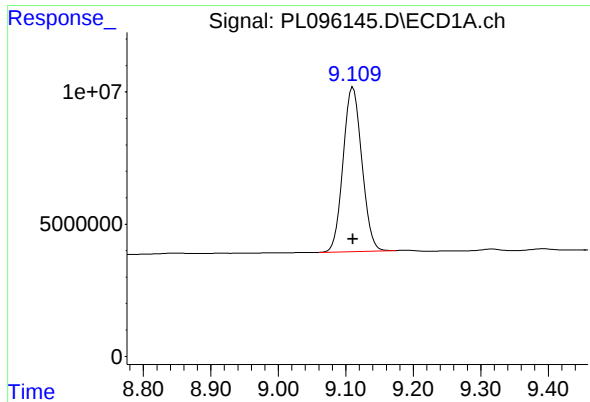

#28 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 120630363
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

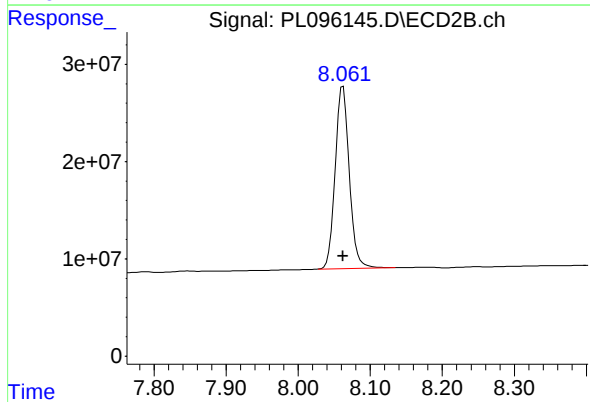

#28 Decachlorobiphenyl

R.T.: 8.062 min
Delta R.T.: 0.000 min
Response: 253460844
Conc: 50.00 ng/ml