

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062419\
 Data File : PL049798.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2019 14:27
 Operator : SM\AJ
 Sample : K3482-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:04:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	3.934	248.5E6	65120154	22.032	21.269
28)	SA Decachlor...	7.988	8.970	213.4E6	64305334	16.797	19.155
Target Compounds							
3)	MA gamma-BHC...	0.000	4.588f	0	6731363	N.D.	1.623 #
9)	A Endosulfan I	5.346f	0.000	101.0E6	0	6.526	N.D. #
10)	B gamma-Chl...	0.000	6.023	0	15785789	N.D.	4.236 #
13)	MA Dieldrin	5.565	0.000	85502609	0	5.133	N.D. #
16)	A 4,4'-DDD	0.000	6.750	0	10807696	N.D.	4.134 #
25)	Chlordane-3	0.000	6.023	0	15785789	N.D.	31.722 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062419\
Data File : PL049798.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2019 14:27
Operator : SM\AJ
Sample : K3482-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:04:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

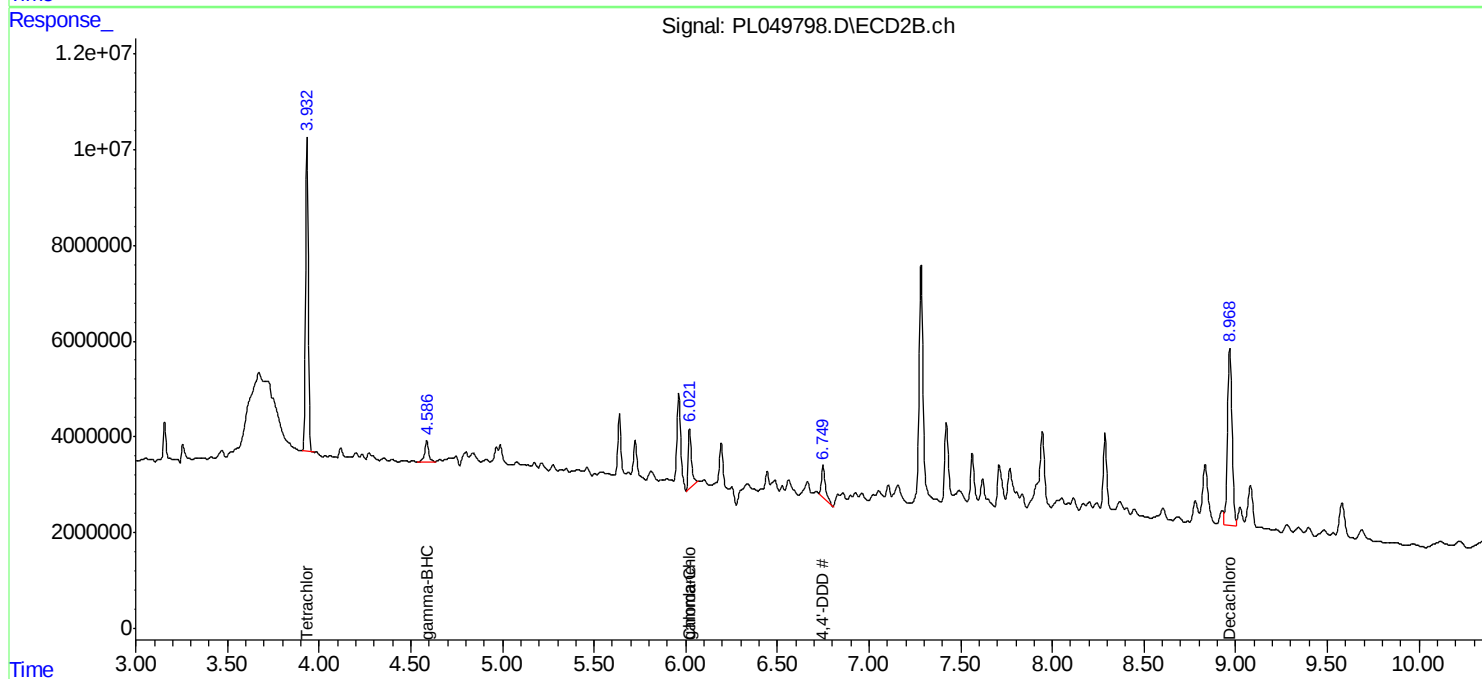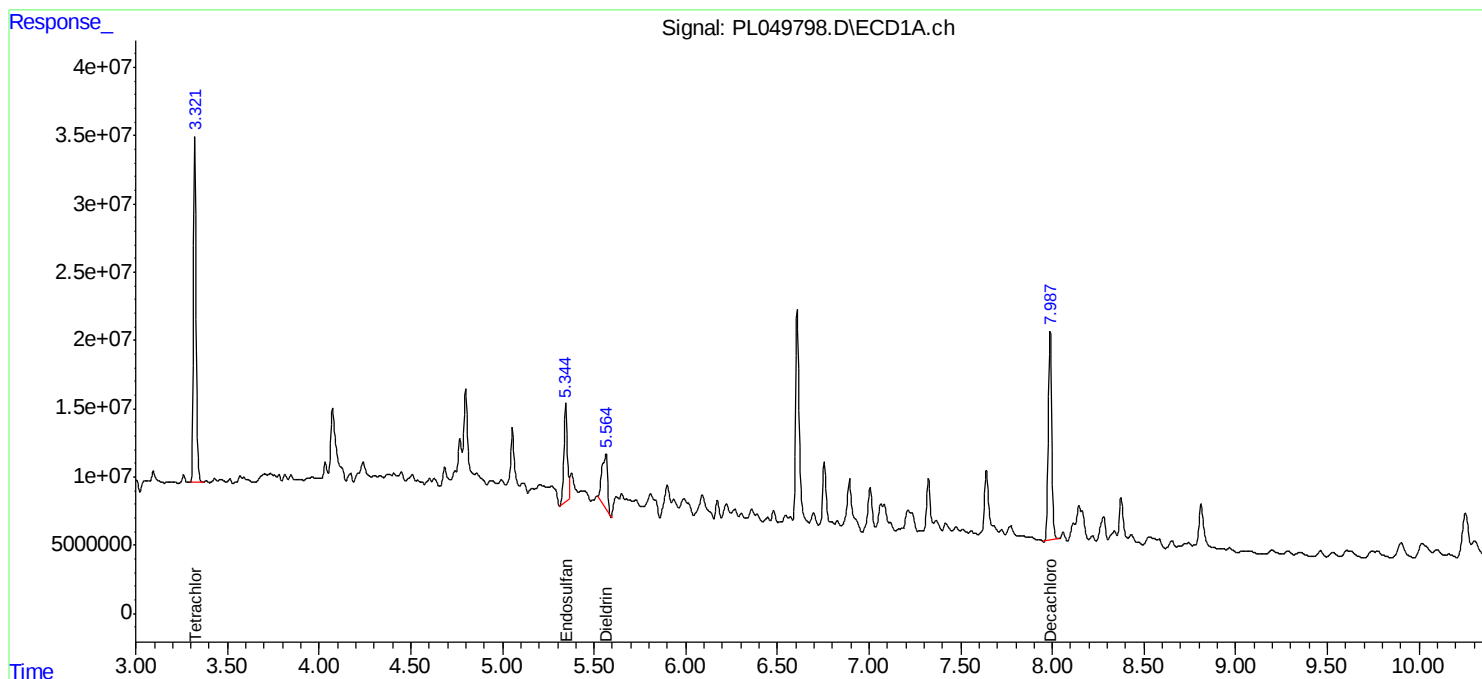


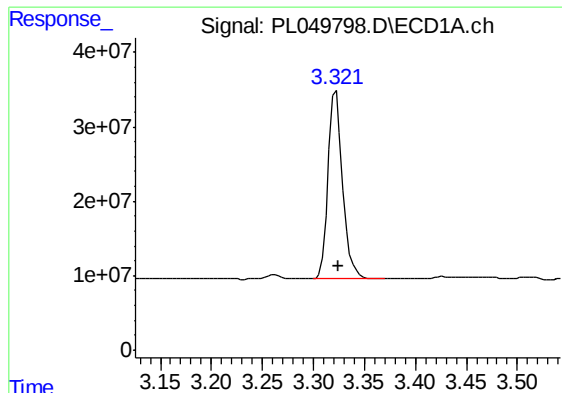

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 248473988
Conc: 22.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

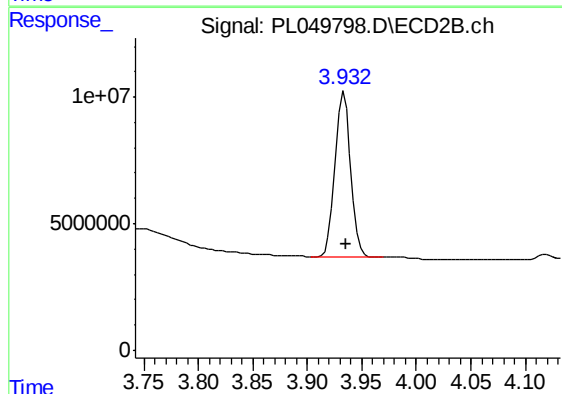


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.001 min
Response: 65120154
Conc: 21.27 ng/ml

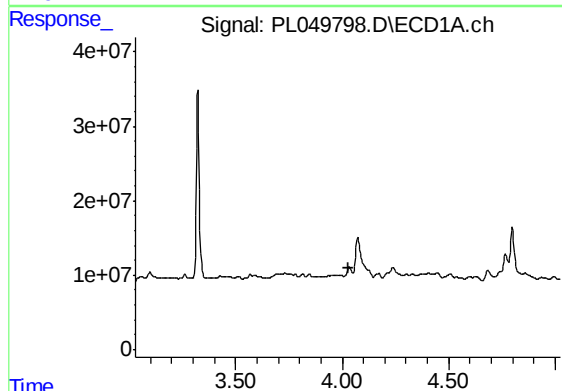


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.028 min
Response: 0
Conc: N.D.

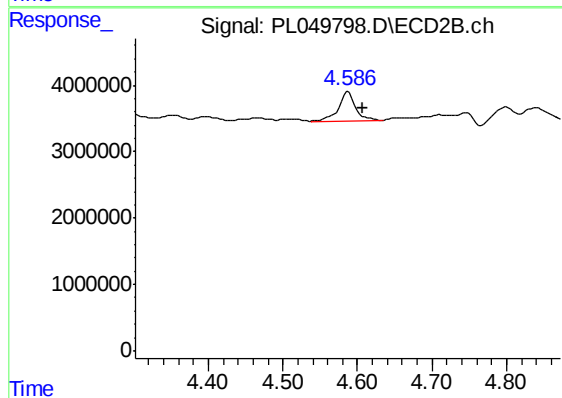

#3 gamma-BHC (Lindane)


R.T.: 4.588 min
Delta R.T.: -0.020 min
Response: 6731363
Conc: 1.62 ng/ml

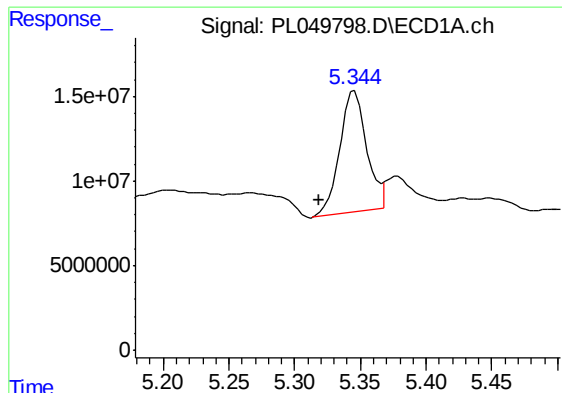

#9 Endosulfan I


R.T.: 5.346 min
Delta R.T.: 0.027 min
Response: 100978909
Conc: 6.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

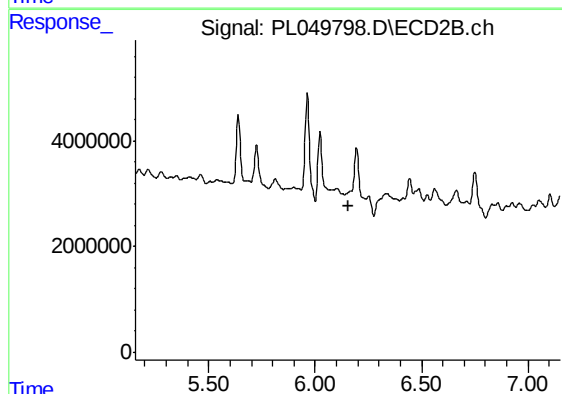


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

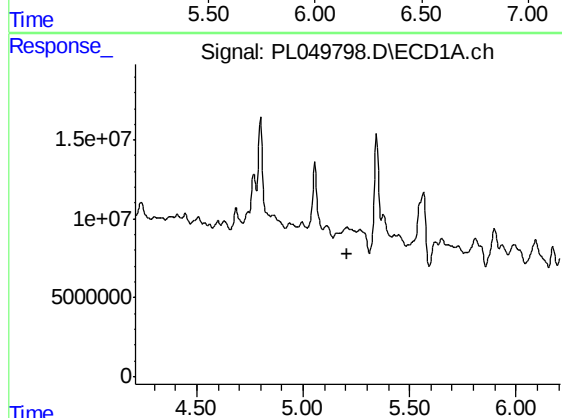


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.210 min
Response: 0
Conc: N.D.

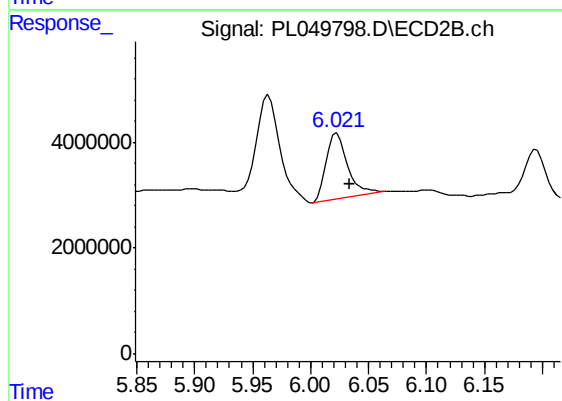

#10 gamma-Chlordane


R.T.: 6.023 min
Delta R.T.: -0.011 min
Response: 15785789
Conc: 4.24 ng/ml

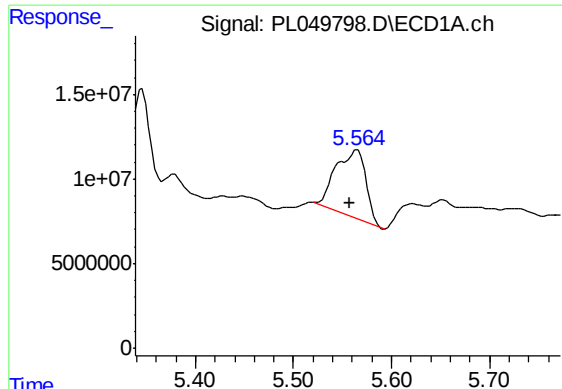

#13 Dieldrin


R.T.: 5.565 min
Delta R.T.: 0.007 min
Response: 85502609
Conc: 5.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

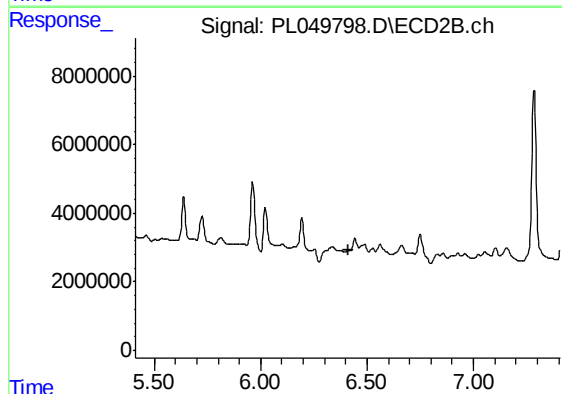


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.412 min
Response: 0
Conc: N.D.

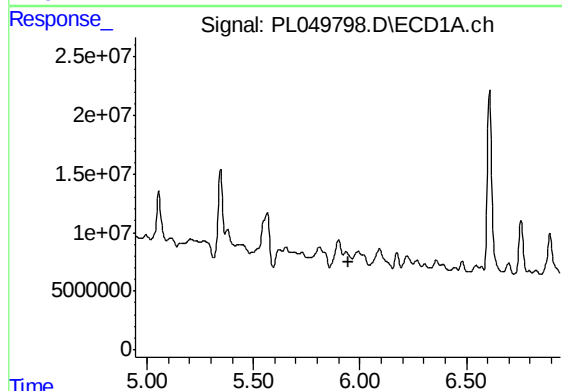


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.945 min
Response: 0
Conc: N.D.

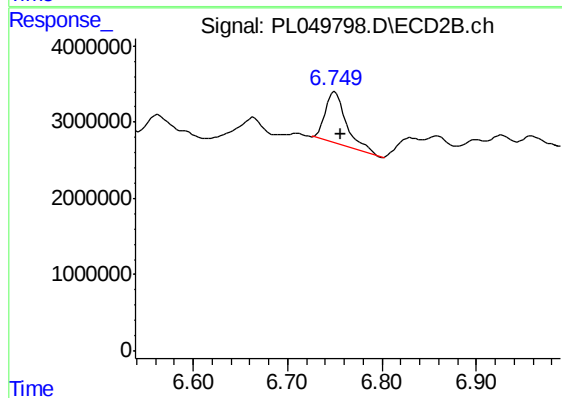

#16 4,4'-DDD


R.T.: 6.750 min
Delta R.T.: -0.007 min
Response: 10807696
Conc: 4.13 ng/ml

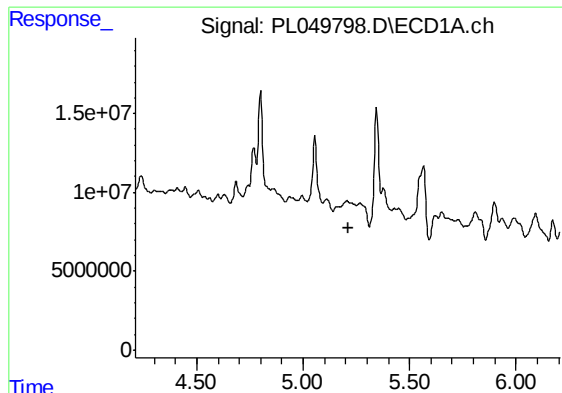

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.211 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-2

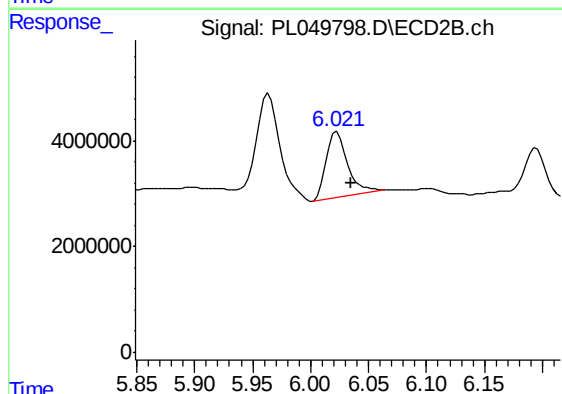


#25 Chlordane-3

R.T.: 6.023 min
Delta R.T.: -0.012 min
Response: 15785789
Conc: 31.72 ng/ml

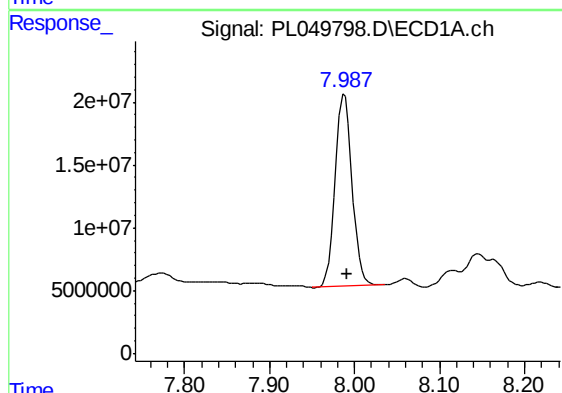

#28 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: -0.004 min
Response: 213425586
Conc: 16.80 ng/ml

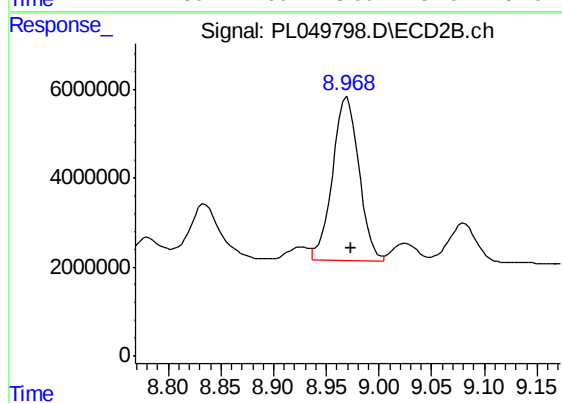

#28 Decachlorobiphenyl

R.T.: 8.970 min
Delta R.T.: -0.003 min
Response: 64305334
Conc: 19.16 ng/ml