

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062420\
 Data File : PL059477.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2020 18:38
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 19:03:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 22 14:09:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.518	4.072	28947729	42173746	16.108	16.340
28)	SA Decachlor...	8.289	9.185	27837194	38112778	16.348	16.646
Target Compounds							
2)	A alpha-BHC	3.963	0.000	869442	0	0.337	N.D. #
4)	MA Heptachlor	0.000	5.264	0	822373	N.D.	0.254 #
5)	MB Aldrin	0.000	5.574	0	1121884	N.D.	0.364 #
7)	B delta-BHC	0.000	5.113f	0	1213898	N.D.	0.436 #
8)	B Heptachlo...	0.000	5.948	0	759084	N.D.	0.302 #
15)	B Endosulfa...	0.000	7.009	0	737275	N.D.	0.291 #
17)	MA 4,4'-DDT	0.000	7.220	0	45463	N.D.	0.020 #
18)	B Endrin al...	0.000	7.158f	0	127806	N.D.	0.058 #
22)	Mirex	7.423	0.000	184969	0	0.131	N.D. #
23)	Chlordane-1	4.421f	0.000	604547	0	10.624	N.D. #
24)	Chlordane-2	0.000	5.574f	0	1121884	N.D.	10.221 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062420\
Data File : PL059477.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2020 18:38
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 19:03:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
Quant Title : GC Extractables
QLast Update : Mon Jun 22 14:09:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

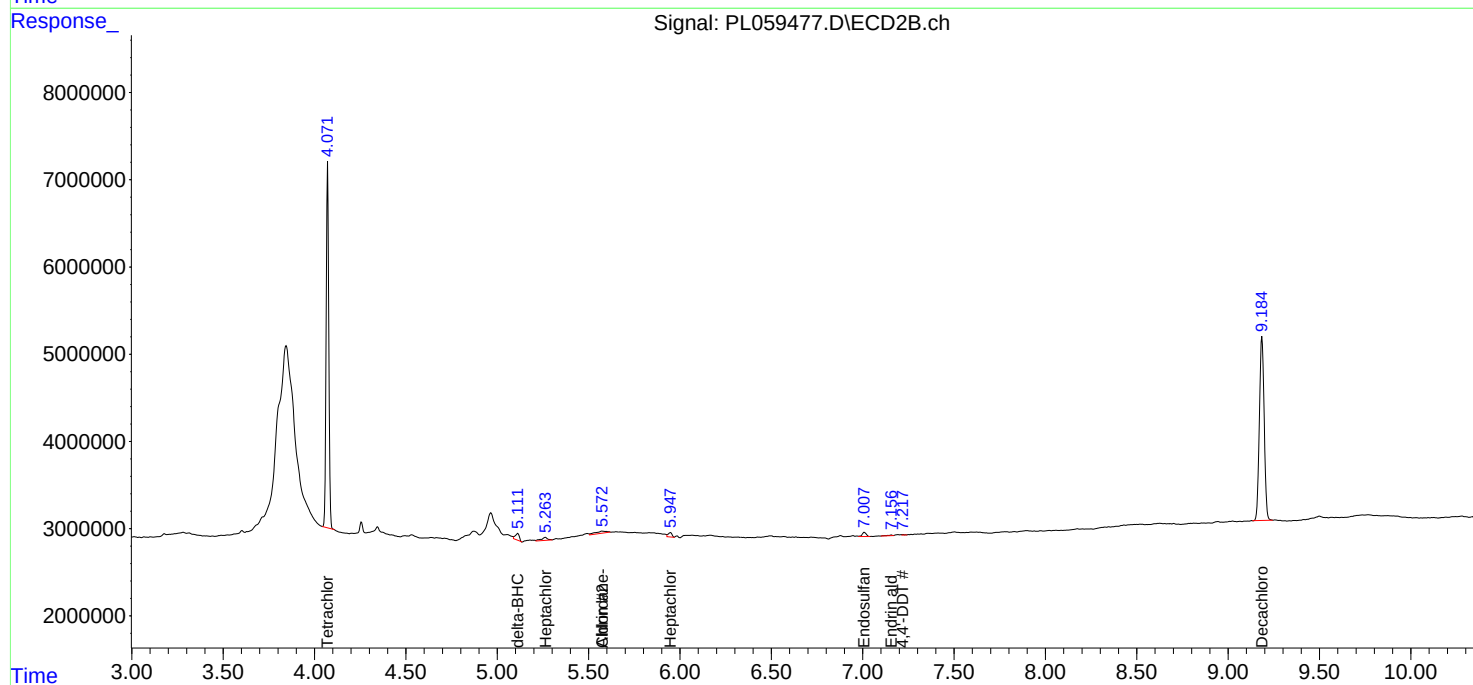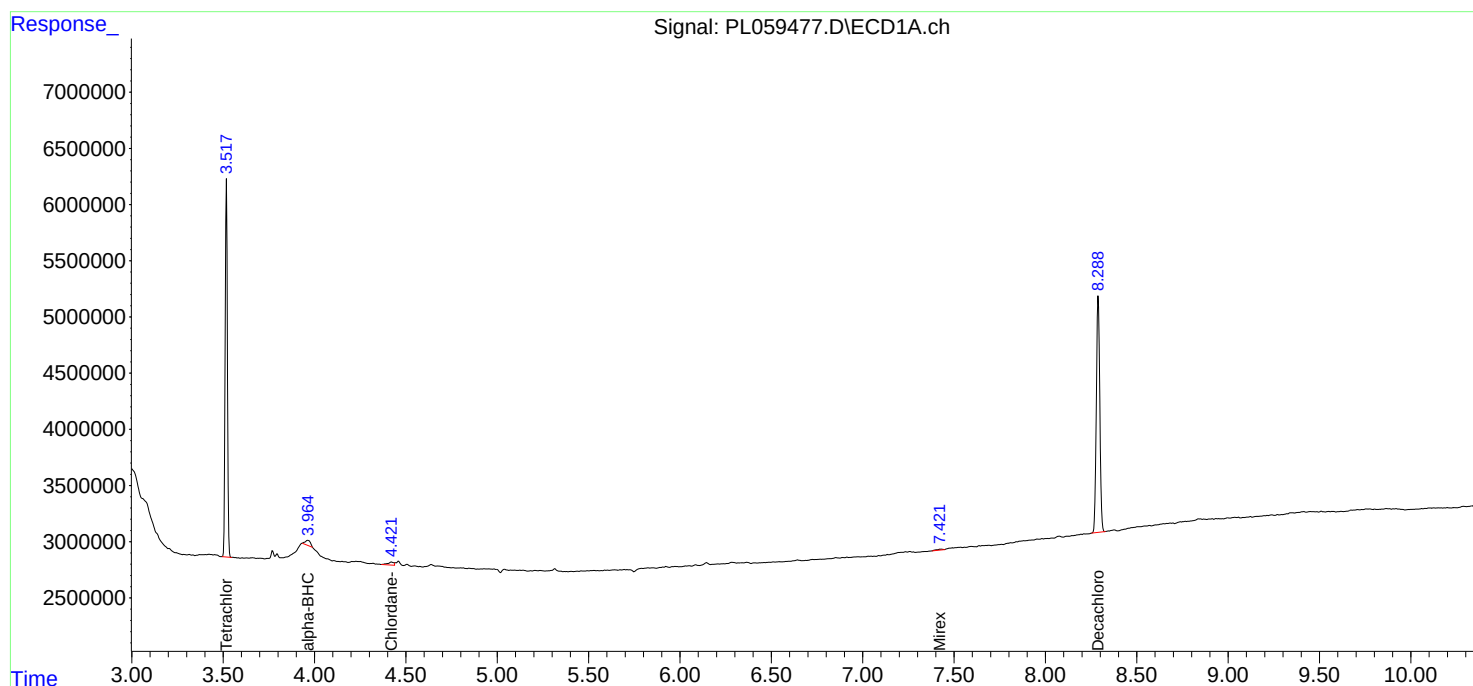


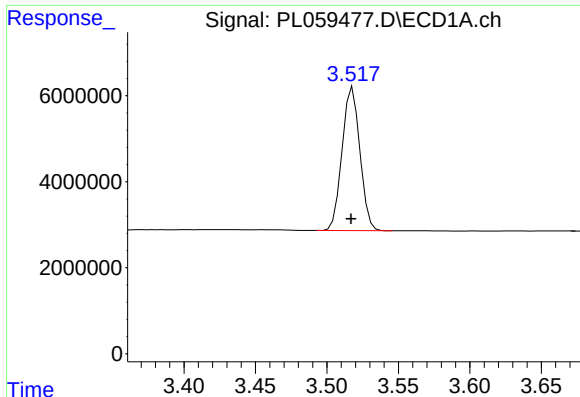

#1 Tetrachloro-m-xylene


R.T.: 3.518 min
Delta R.T.: 0.001 min
Response: 28947729
Conc: 16.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

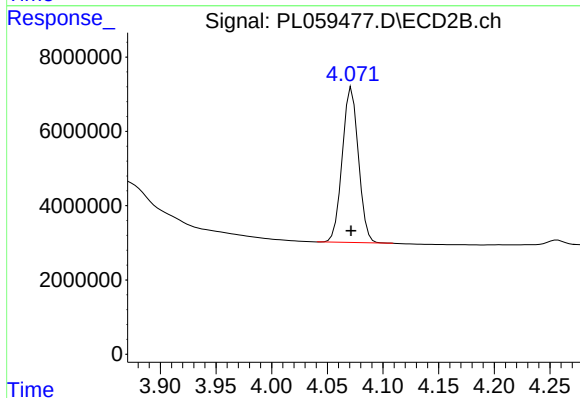


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 42173746
Conc: 16.34 ng/ml

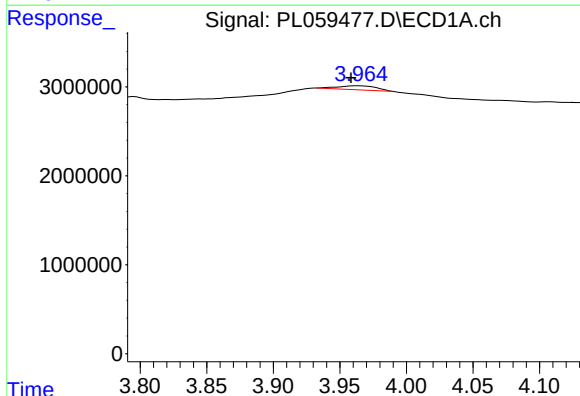


#2 alpha-BHC

R.T.: 3.963 min
Delta R.T.: 0.005 min
Response: 869442
Conc: 0.34 ng/ml

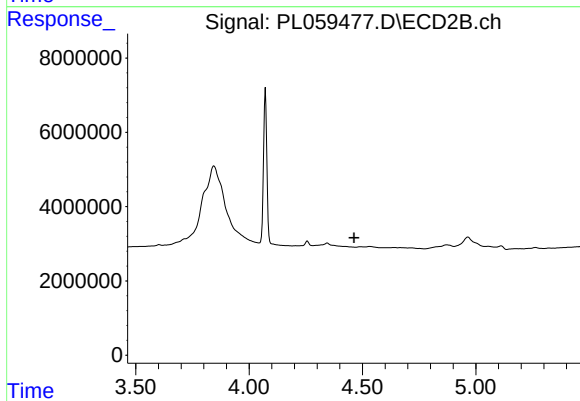

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.463 min
Response: 0
Conc: N.D.

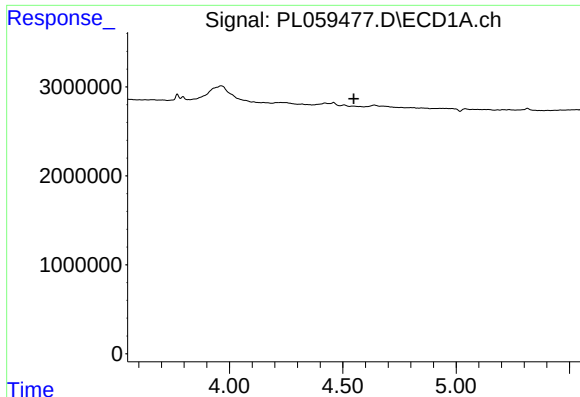

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

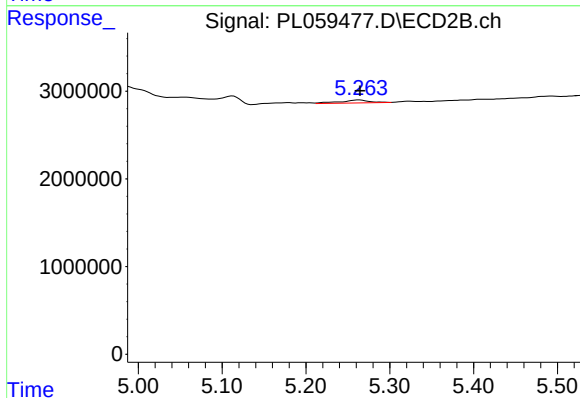


#4 Heptachlor

R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 822373
Conc: 0.25 ng/ml

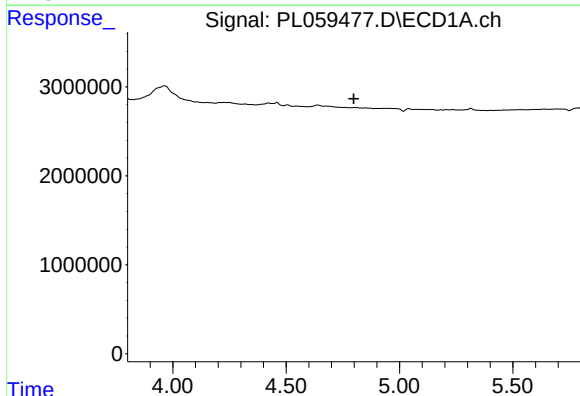


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.799 min
Response: 0
Conc: N.D.

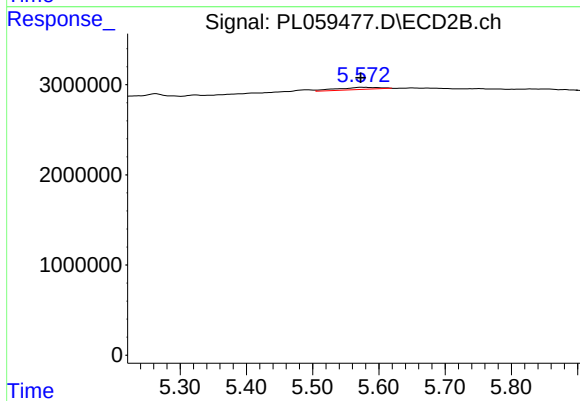

#5 Aldrin


R.T.: 5.574 min
Delta R.T.: 0.001 min
Response: 1121884
Conc: 0.36 ng/ml

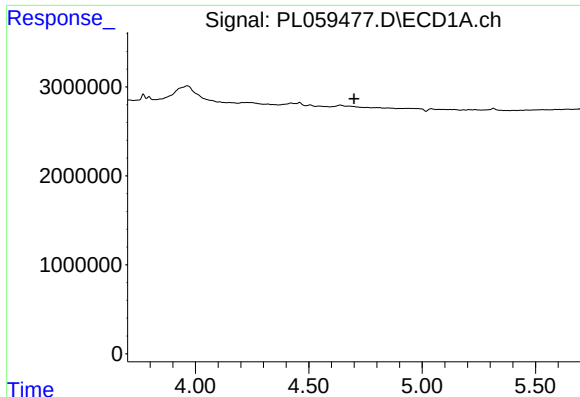

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.700 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

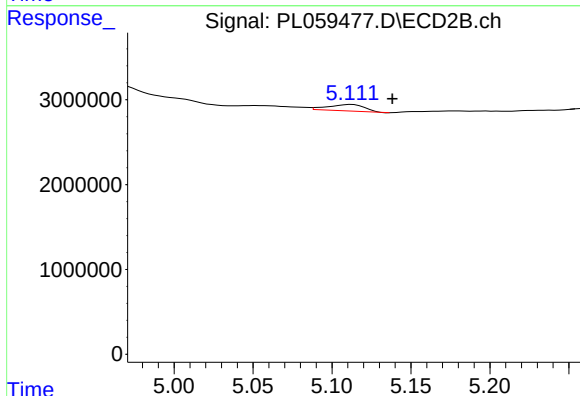


#7 delta-BHC

R.T.: 5.113 min
Delta R.T.: -0.026 min
Response: 1213898
Conc: 0.44 ng/ml

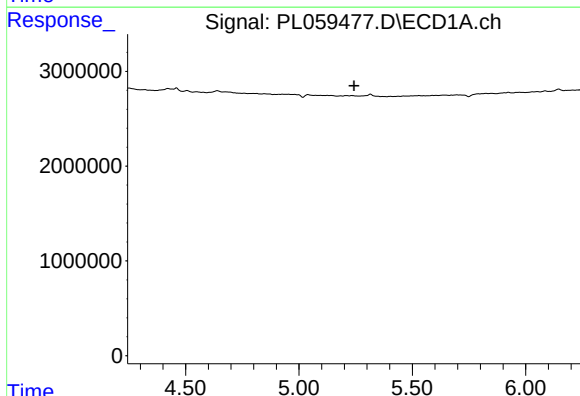


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.243 min
Response: 0
Conc: N.D.

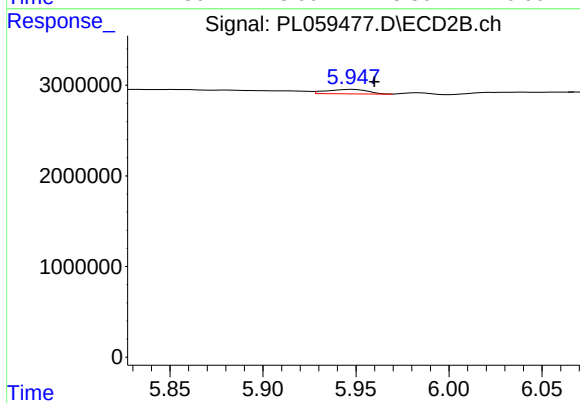

#8 Heptachlor epoxide


R.T.: 5.948 min
Delta R.T.: -0.012 min
Response: 759084
Conc: 0.30 ng/ml

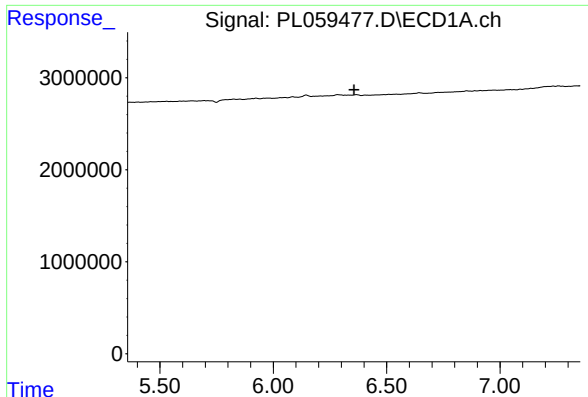

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

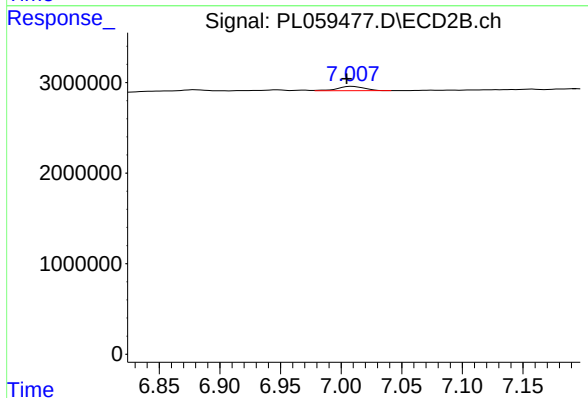


#15 Endosulfan II

R.T.: 7.009 min
Delta R.T.: 0.004 min
Response: 737275
Conc: 0.29 ng/ml

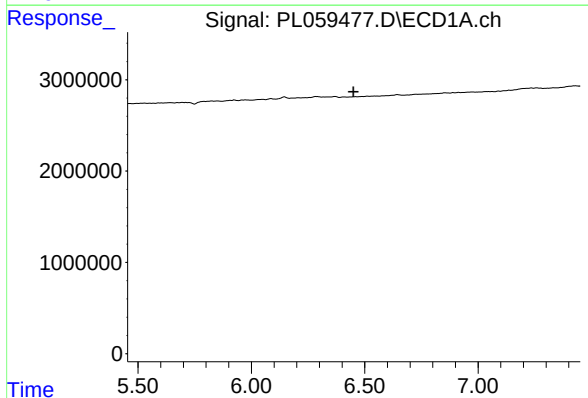


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

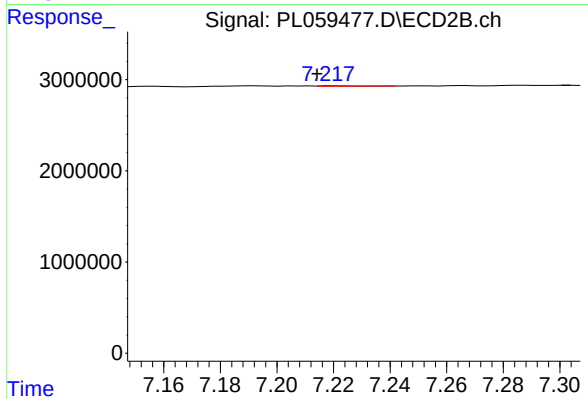

#17 4,4'-DDT


R.T.: 7.220 min
Delta R.T.: 0.006 min
Response: 45463
Conc: 0.02 ng/ml

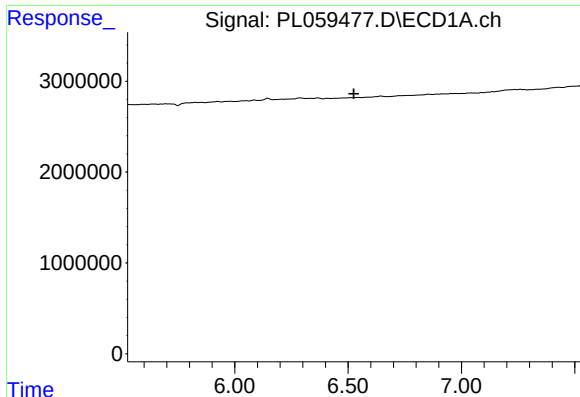

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

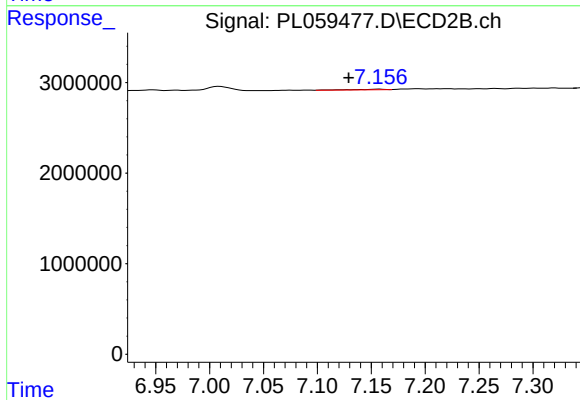


#18 Endrin aldehyde

R.T.: 7.158 min
Delta R.T.: 0.029 min
Response: 127806
Conc: 0.06 ng/ml

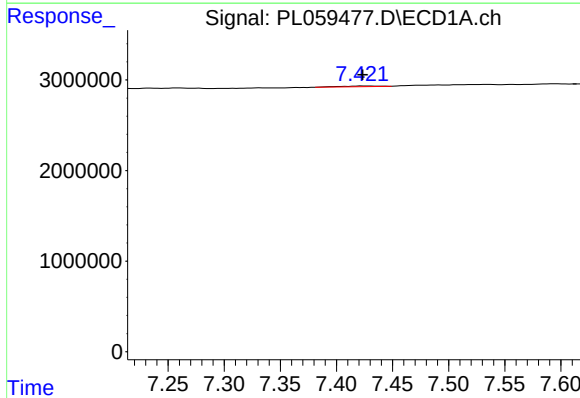


#22 Mirex

R.T.: 7.423 min
Delta R.T.: 0.000 min
Response: 184969
Conc: 0.13 ng/ml

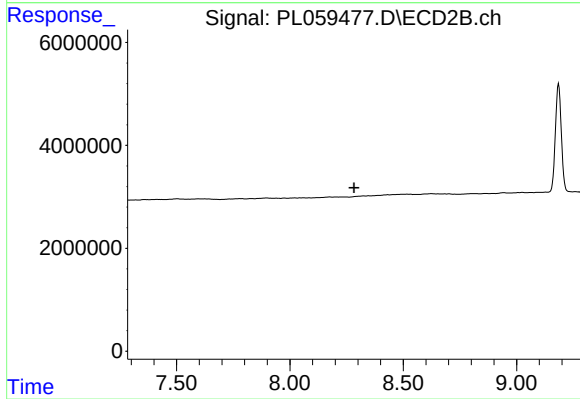

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

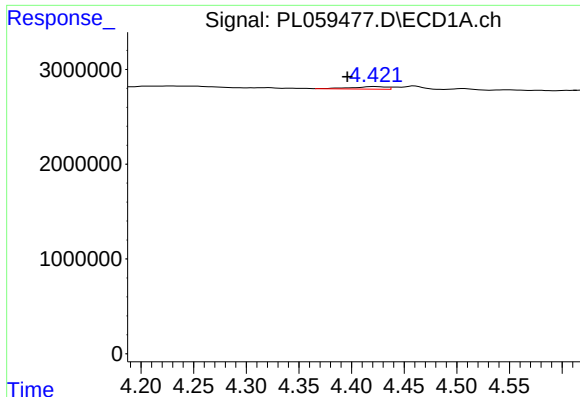

#23 Chlordane-1


R.T.: 4.421 min
Delta R.T.: 0.025 min
Response: 604547
Conc: 10.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

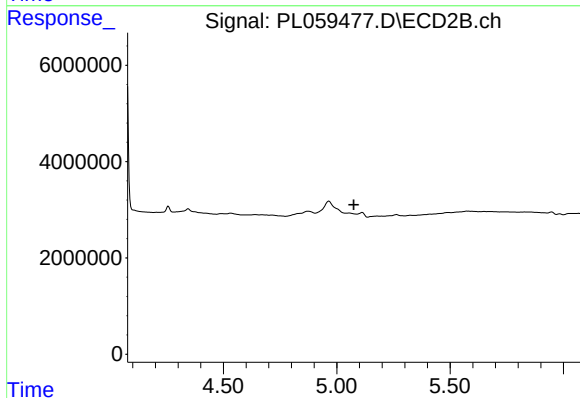


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.075 min
Response: 0
Conc: N.D.

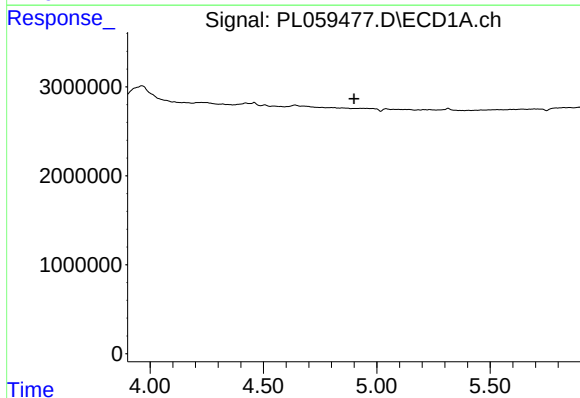


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.900 min
Response: 0
Conc: N.D.

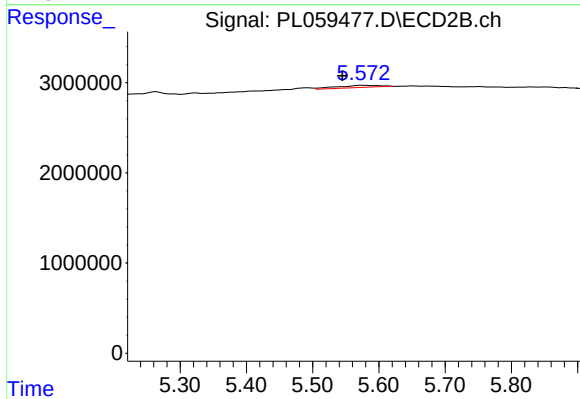

#24 Chlordane-2


R.T.: 5.574 min
Delta R.T.: 0.029 min
Response: 1121884
Conc: 10.22 ng/ml

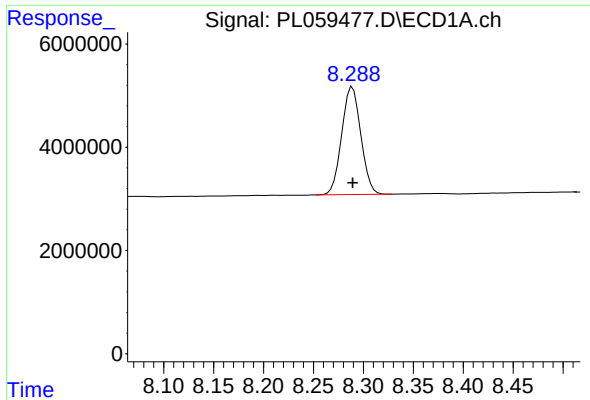

#28 Decachlorobiphenyl

R.T.: 8.289 min
Delta R.T.: 0.000 min
Response: 27837194
Conc: 16.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

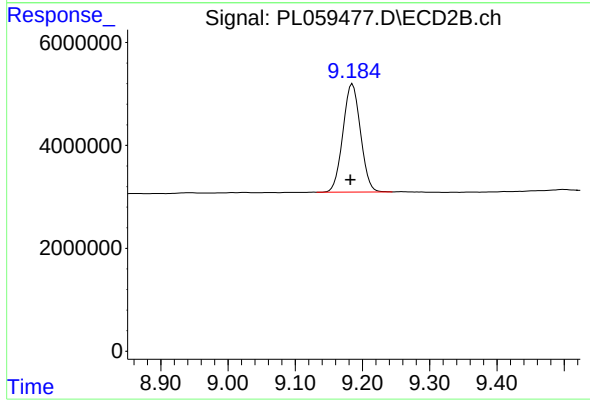

#28 Decachlorobiphenyl

R.T.: 9.185 min
Delta R.T.: 0.003 min
Response: 38112778
Conc: 16.65 ng/ml