

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062420\
 Data File : PL059486.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2020 20:45
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:12:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 22 14:09:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.518	4.072	29532019	43003417	16.433	16.662
28)	SA Decachlor...	8.290	9.185	24629104	34592683	14.464	15.109
Target Compounds							
2)	A alpha-BHC	3.968	0.000	1141543	0	0.442	N.D. #
4)	MA Heptachlor	0.000	5.263	0	620377	N.D.	0.192 #
7)	B delta-BHC	0.000	5.112f	0	996054	N.D.	0.358 #
8)	B Heptachlo...	0.000	5.952	0	1597854	N.D.	0.637 #
14)	MA Endrin	6.086	0.000	179972	0	0.118	N.D. #
15)	B Endosulfa...	6.362	7.010	128258	588773	0.083	0.232 #
23)	Chlordane-1	4.424f	0.000	452070	0	7.944	N.D. #
27)	Chlordane-5	6.362	0.000	128258	0	2.285	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062420\
Data File : PL059486.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2020 20:45
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:12:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
Quant Title : GC Extractables
QLast Update : Mon Jun 22 14:09:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

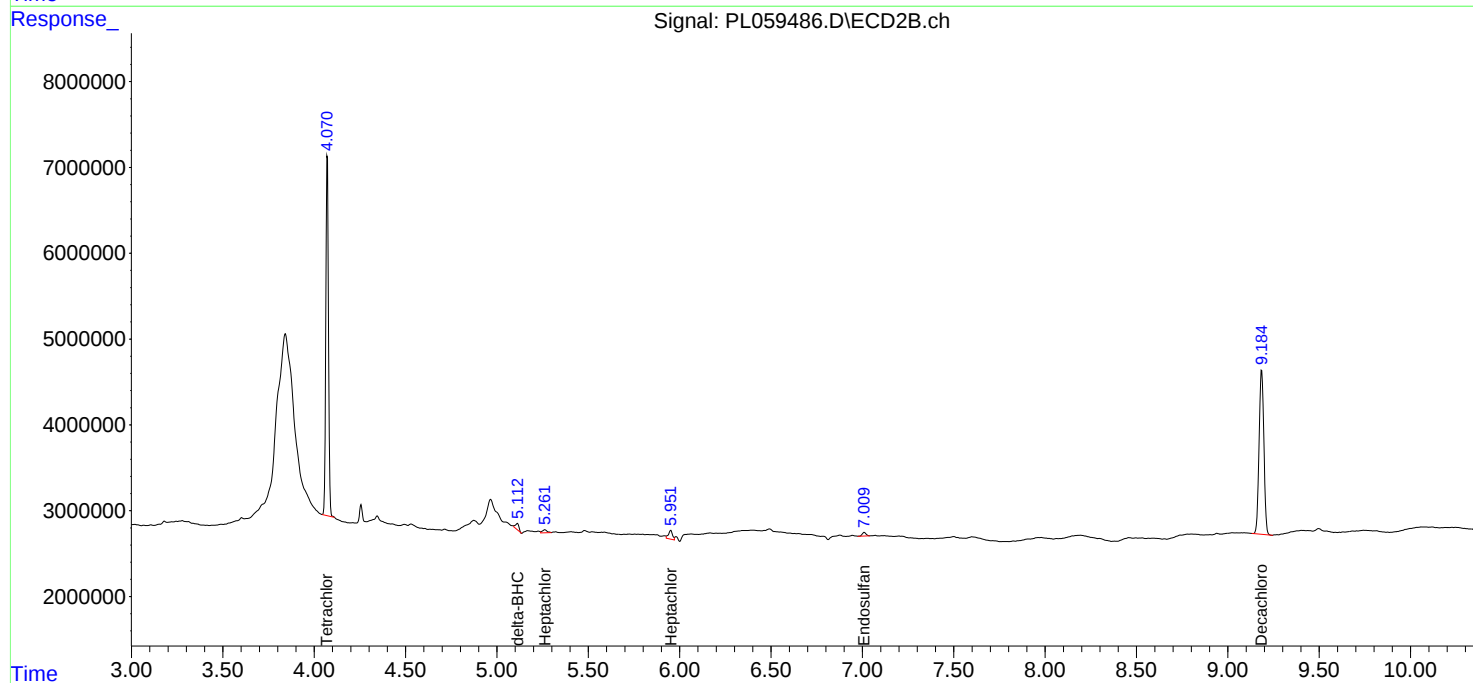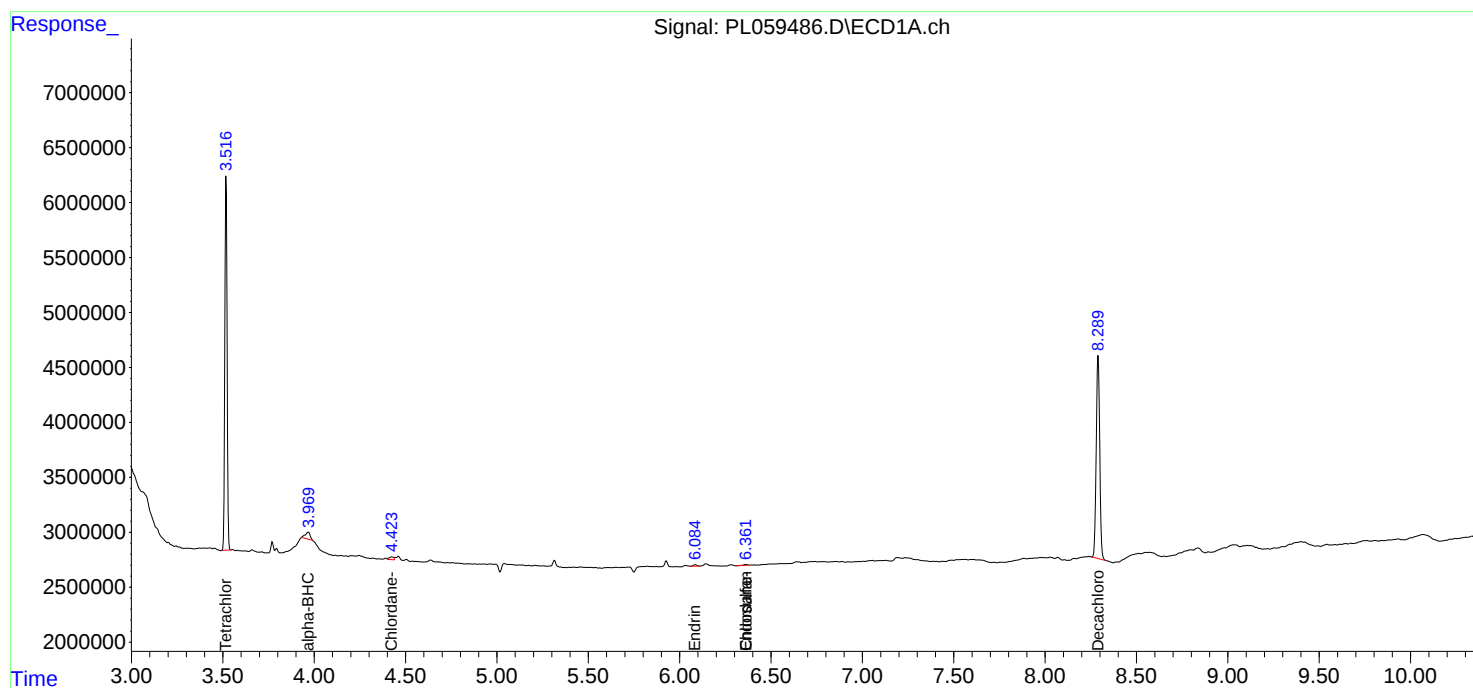


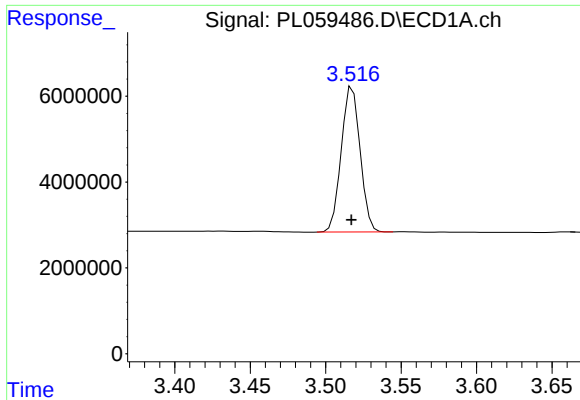

#1 Tetrachloro-m-xylene


R.T.: 3.518 min
Delta R.T.: 0.000 min
Response: 29532019
Conc: 16.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

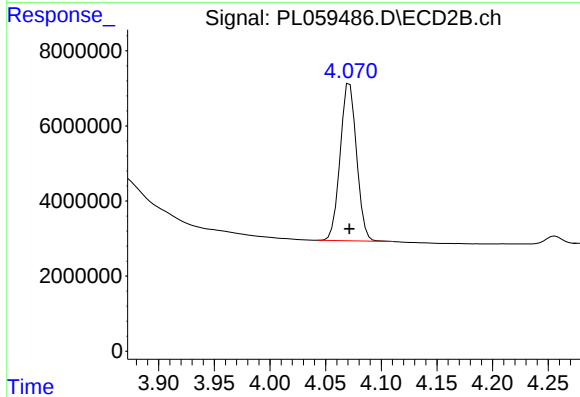


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 43003417
Conc: 16.66 ng/ml

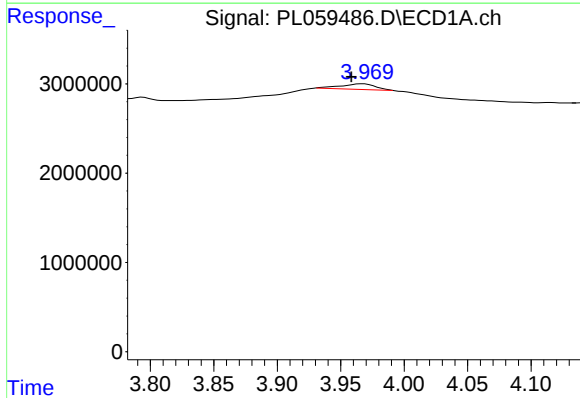


#2 alpha-BHC

R.T.: 3.968 min
Delta R.T.: 0.009 min
Response: 1141543
Conc: 0.44 ng/ml

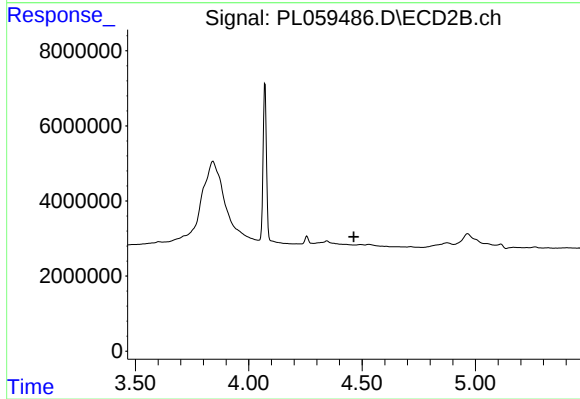

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.463 min
Response: 0
Conc: N.D.

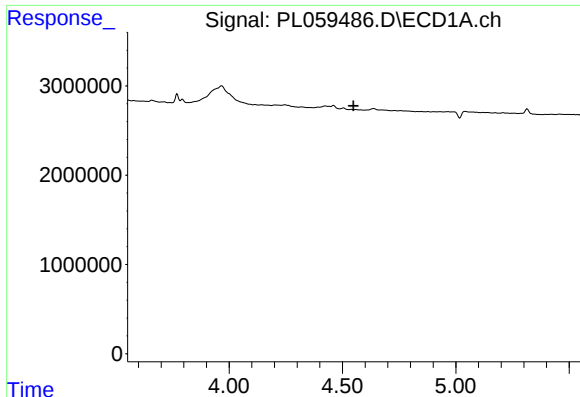

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

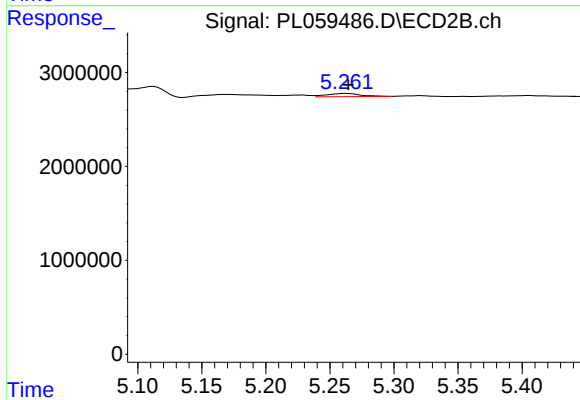


#4 Heptachlor

R.T.: 5.263 min
Delta R.T.: -0.002 min
Response: 620377
Conc: 0.19 ng/ml

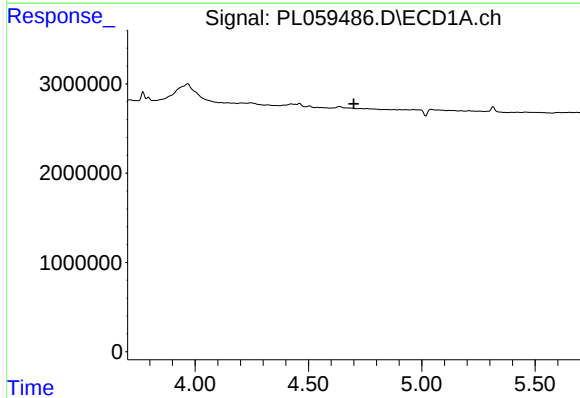


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.700 min
Response: 0
Conc: N.D.

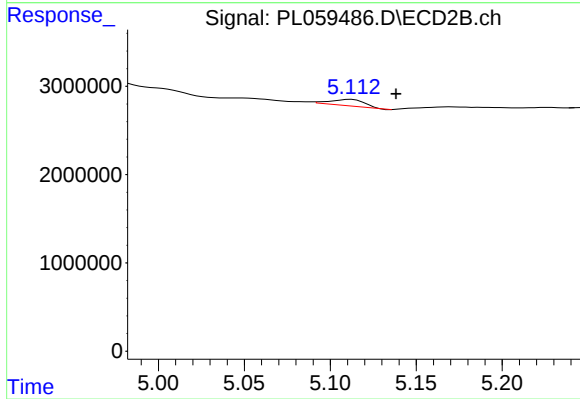

#7 delta-BHC


R.T.: 5.112 min
Delta R.T.: -0.026 min
Response: 996054
Conc: 0.36 ng/ml

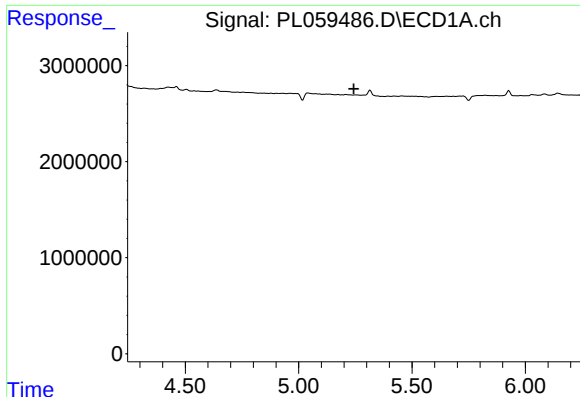

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.243 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

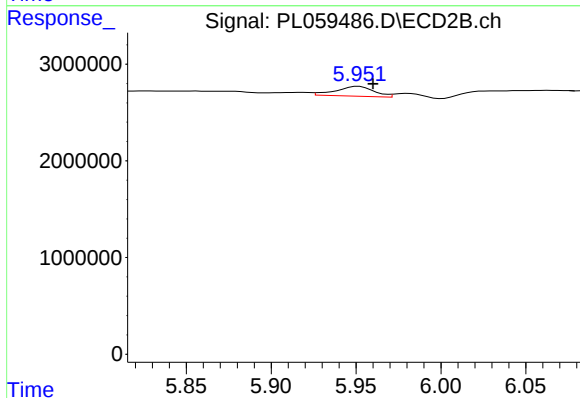


#8 Heptachlor epoxide

R.T.: 5.952 min
Delta R.T.: -0.008 min
Response: 1597854
Conc: 0.64 ng/ml

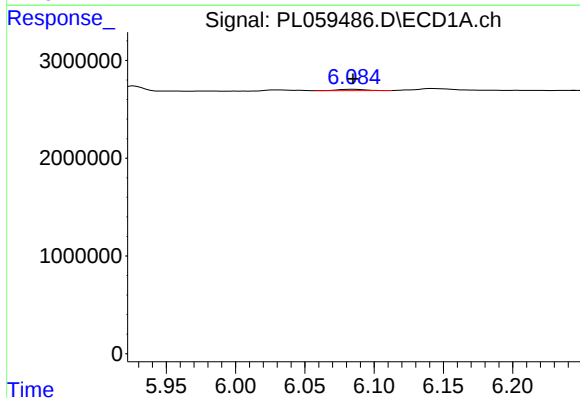


#14 Endrin

R.T.: 6.086 min
Delta R.T.: 0.000 min
Response: 179972
Conc: 0.12 ng/ml

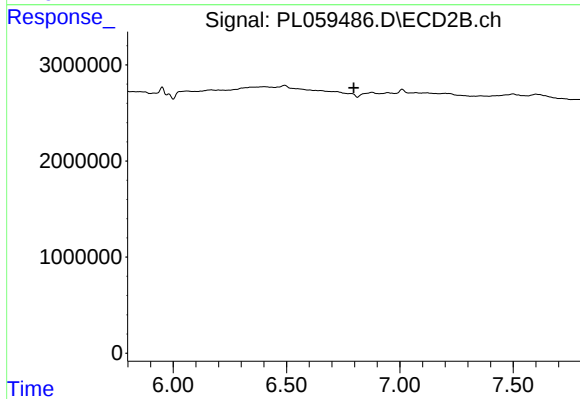

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.796 min
Response: 0
Conc: N.D.

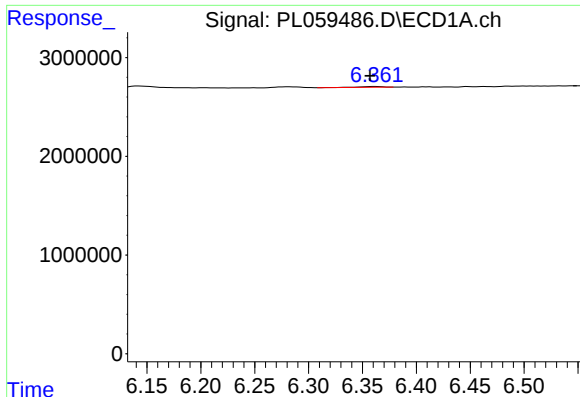

#15 Endosulfan II


R.T.: 6.362 min
Delta R.T.: 0.005 min
Response: 128258
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

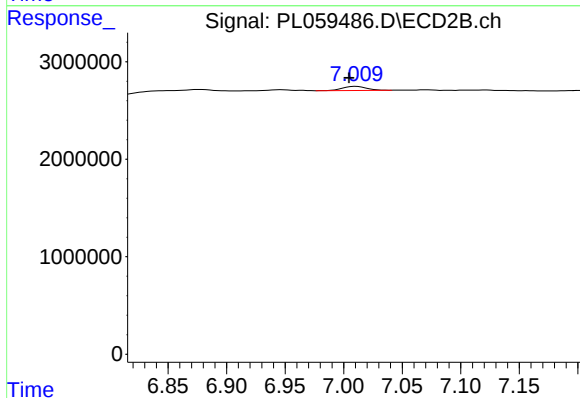


#15 Endosulfan II

R.T.: 7.010 min
Delta R.T.: 0.006 min
Response: 588773
Conc: 0.23 ng/ml

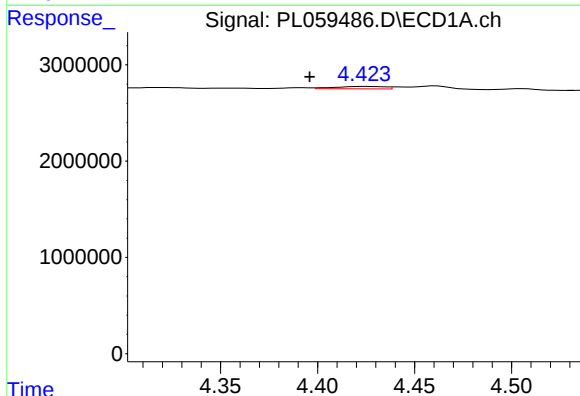


#23 Chlordane-1

R.T.: 4.424 min
Delta R.T.: 0.028 min
Response: 452070
Conc: 7.94 ng/ml

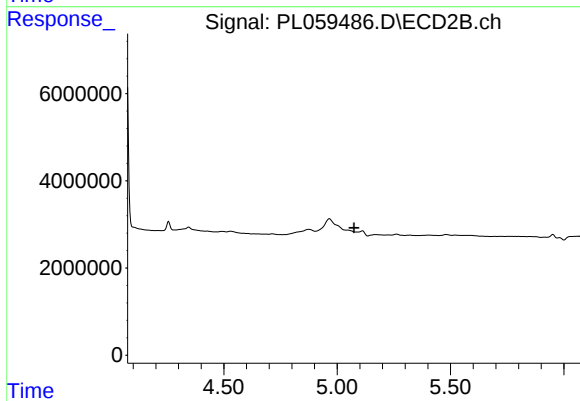

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.075 min
Response: 0
Conc: N.D.

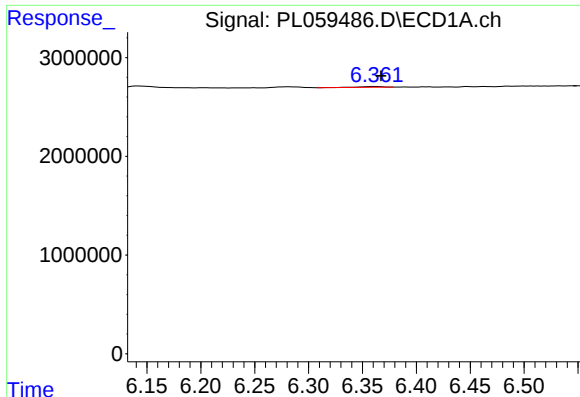

#27 Chlordane-5


R.T.: 6.362 min
Delta R.T.: -0.005 min
Response: 128258
Conc: 2.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

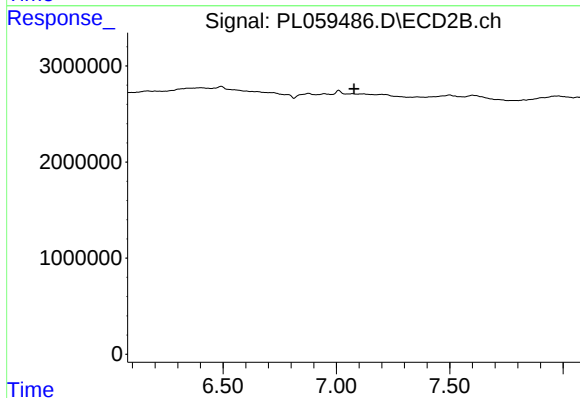


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

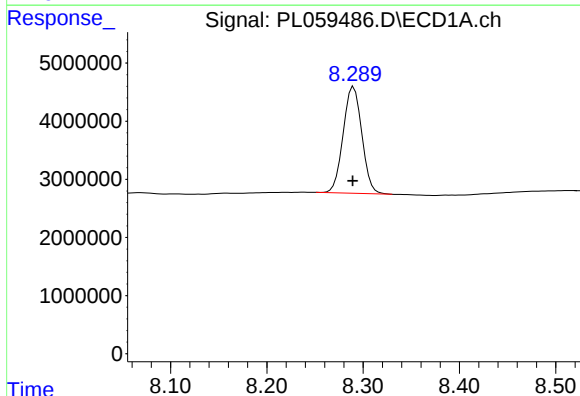

#28 Decachlorobiphenyl

R.T.: 8.290 min
Delta R.T.: 0.001 min
Response: 24629104
Conc: 14.46 ng/ml

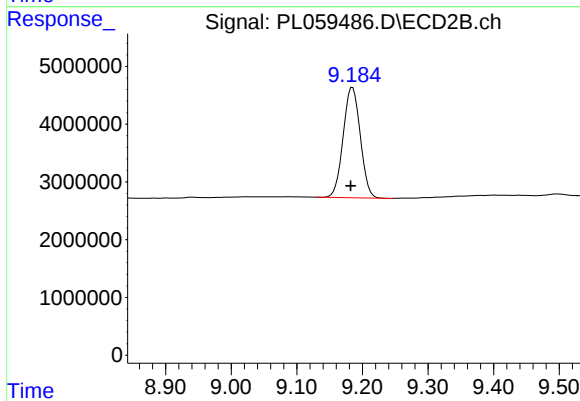

#28 Decachlorobiphenyl

R.T.: 9.185 min
Delta R.T.: 0.003 min
Response: 34592683
Conc: 15.11 ng/ml