

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062420\
 Data File : PL059473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2020 17:41
 Operator : AJ\MA
 Sample : L3089-02MS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RB47184-RTMS

Manual Integrations
 APPROVED

Ankita
 6/25/2020 1:29:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 18:42:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 22 14:09:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.518	4.072	39942813	58401564	22.226	22.628
28)	SA Decachlor...	8.290	9.185	36380485	49747039	21.365	21.727
Target Compounds							
2)	A alpha-BHC	3.959	4.464	161.5E6	238.2E6	62.559	69.924m
3)	MA gamma-BHC...	4.244	4.753	142.8E6	218.9E6	62.626	69.939
4)	MA Heptachlor	4.550	5.267	132.2E6	207.1E6	61.972	63.942
5)	MB Aldrin	4.800	5.575	114.4E6	189.8E6	64.294	61.628
6)	B beta-BHC	4.494	4.921	57166010	89911998	60.029	66.109
7)	B delta-BHC	4.700	5.141	128.3E6	170.8E6	62.883	61.400
8)	B Heptachlo...	5.244	5.963	105.6E6	158.6E6	70.258	63.199
9)	A Endosulfan I	5.584	6.322	96582048	156.0E6	65.650	57.471
10)	B gamma-Chl...	5.471	6.197	102.9E6	172.7E6	67.064	58.957
11)	B alpha-Chl...	5.530	6.271	102.6E6	171.3E6	66.005	58.176
12)	B 4,4'-DDE	5.693	6.426	95469592	147.2E6	65.702	54.508
13)	MA Dieldrin	5.828	6.580	102.3E6	164.6E6	64.816	58.462
14)	MA Endrin	6.086	6.799	95418570	148.3E6	62.800	60.054
15)	B Endosulfa...	6.358	7.007	95340267	151.3E6	61.739	59.663
16)	A 4,4'-DDD	6.210	6.917	82543710	136.7E6	63.254	61.438
17)	MA 4,4'-DDT	6.451	7.218	85085964	138.2E6	64.530	60.786
18)	B Endrin al...	6.526	7.132	80868598	131.6E6	61.187	60.013
19)	B Endosulfa...	6.739	7.355	92349325	144.6E6	60.826	59.753
20)	A Methoxychlor	6.997	7.675	47910602	77224139	59.117	58.174
21)	B Endrin ke...	7.231	7.829	106.2E6	155.1E6	60.931	60.055
22)	Mirex	7.424	8.286	82849348	115.7E6	58.671	58.598

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062420\
Data File : PL059473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2020 17:41
Operator : AJ\MA
Sample : L3089-02MS
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RB47184-RTMS


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 18:42:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
Quant Title : GC Extractables
QLast Update : Mon Jun 22 14:09:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

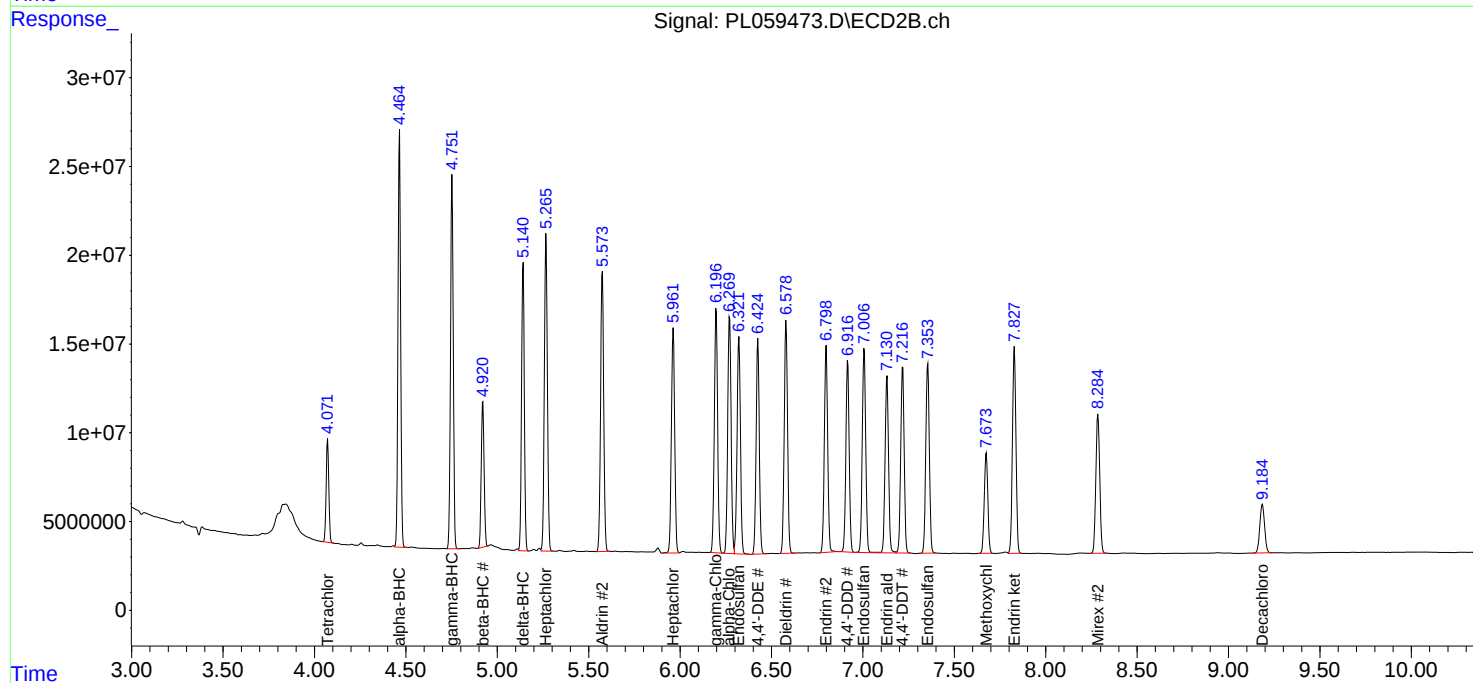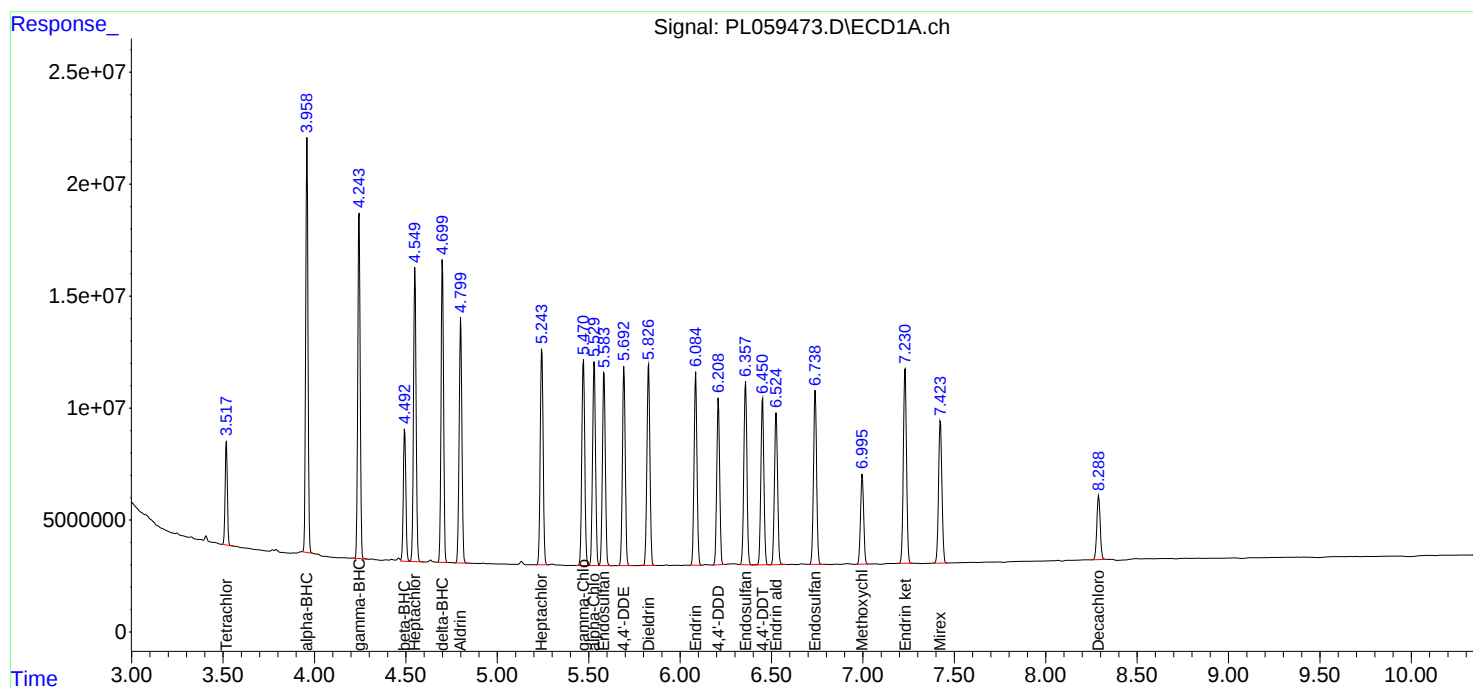

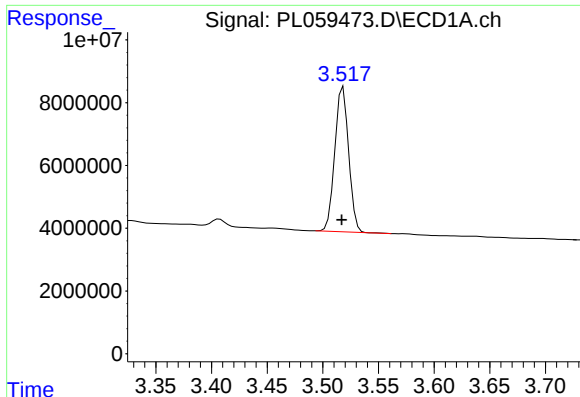


#1 Tetrachloro-m-xylene

R.T.: 3.518 min
Delta R.T.: 0.001 min
Response: 39942813
Conc: 22.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
RB47184-RTMS


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:27 PM

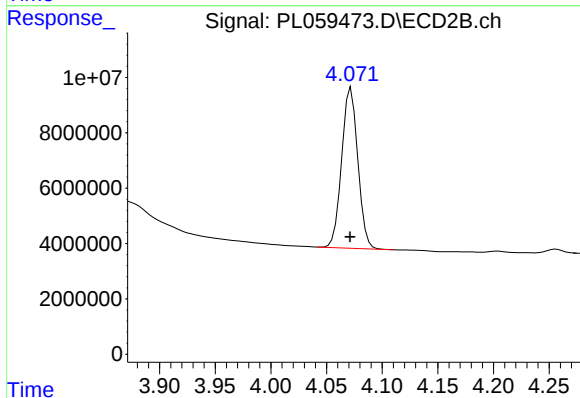


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 58401564
Conc: 22.63 ng/ml

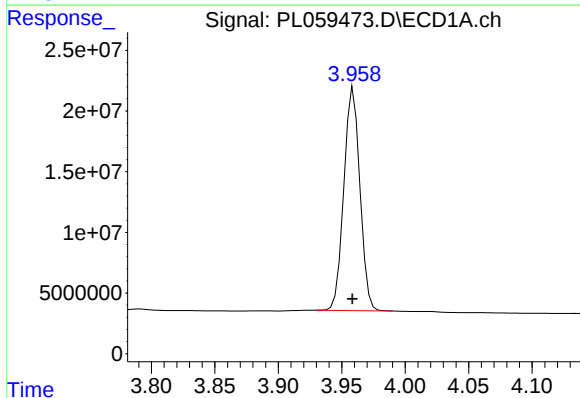


#2 alpha-BHC

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 161469539
Conc: 62.56 ng/ml

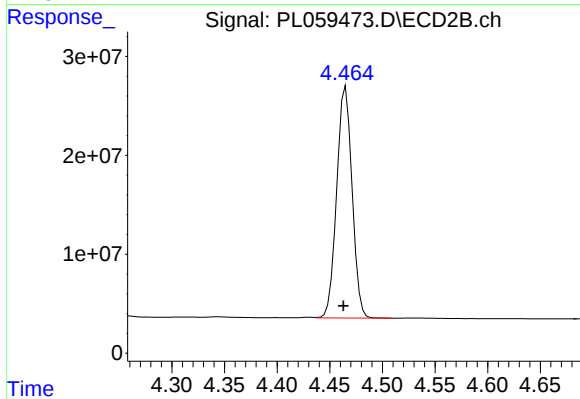

#2 alpha-BHC

R.T.: 4.464 min
Delta R.T.: 0.000 min
Response: 238201049
Conc: 69.92 ng/ml m

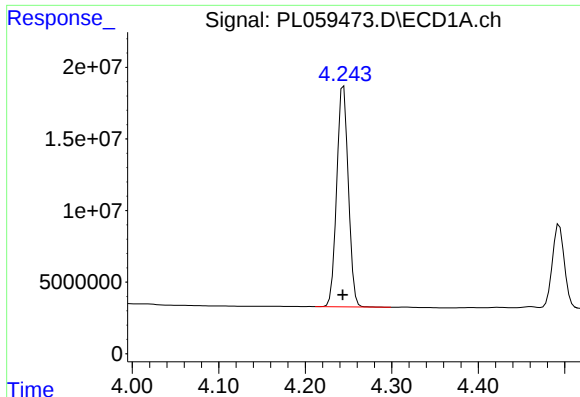


#3 gamma-BHC (Lindane)

R.T.: 4.244 min
Delta R.T.: 0.001 min
Response: 142823959
Conc: 62.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
RB47184-RTMS


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:27 PM

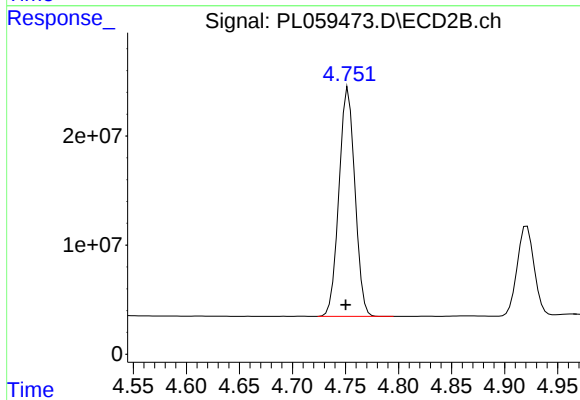


#3 gamma-BHC (Lindane)

R.T.: 4.753 min
Delta R.T.: 0.002 min
Response: 218903477
Conc: 69.94 ng/ml

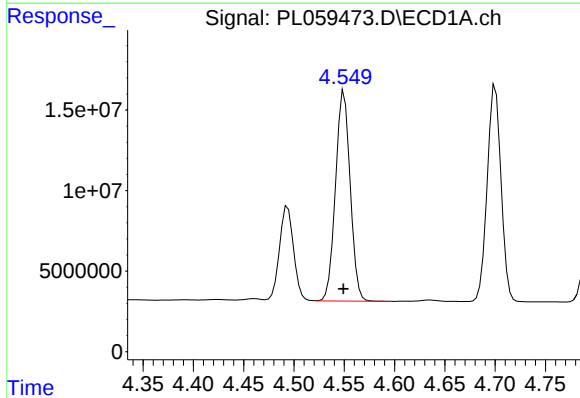


#4 Heptachlor

R.T.: 4.550 min
Delta R.T.: 0.000 min
Response: 132155425
Conc: 61.97 ng/ml

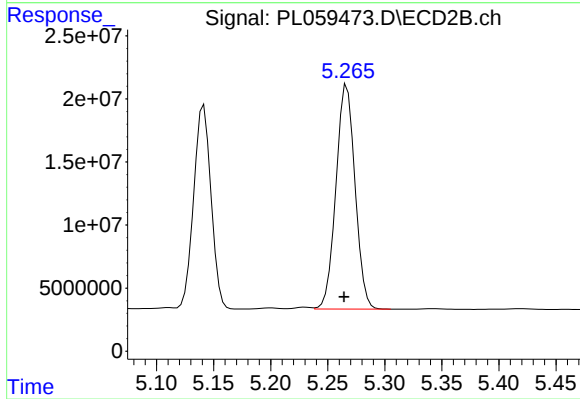

#4 Heptachlor

R.T.: 5.267 min
Delta R.T.: 0.002 min
Response: 207098962
Conc: 63.94 ng/ml

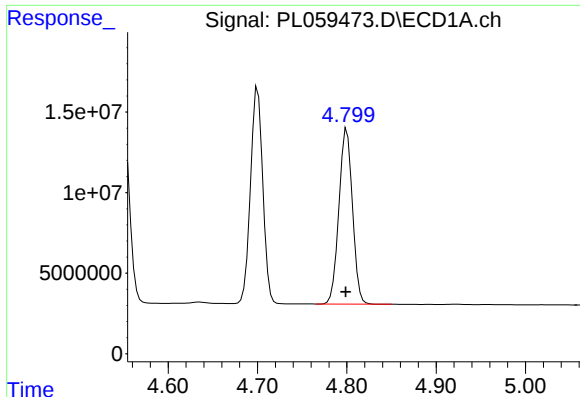


#5 Aldrin

R.T.: 4.800 min
Delta R.T.: 0.001 min
Response: 114410556
Conc: 64.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
RB47184-RTMS


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:27 PM

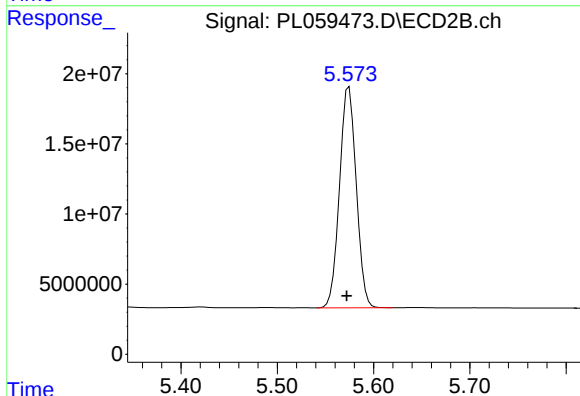


#5 Aldrin

R.T.: 5.575 min
Delta R.T.: 0.002 min
Response: 189791595
Conc: 61.63 ng/ml

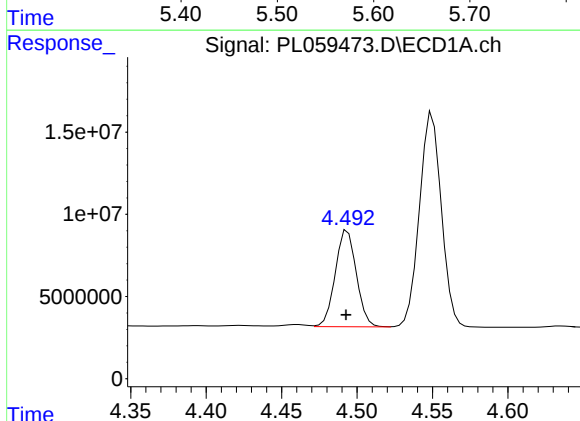


#6 beta-BHC

R.T.: 4.494 min
Delta R.T.: 0.000 min
Response: 57166010
Conc: 60.03 ng/ml

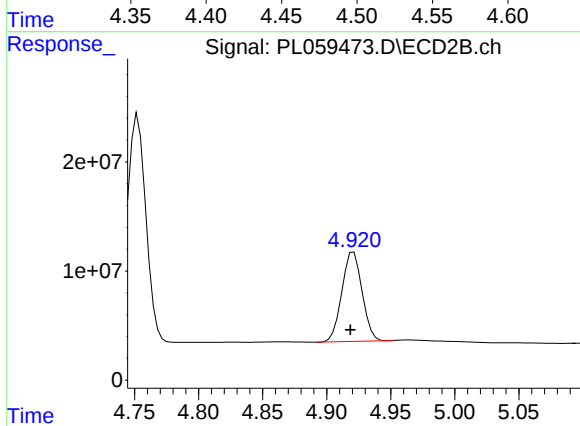

#6 beta-BHC

R.T.: 4.921 min
Delta R.T.: 0.002 min
Response: 89911998
Conc: 66.11 ng/ml

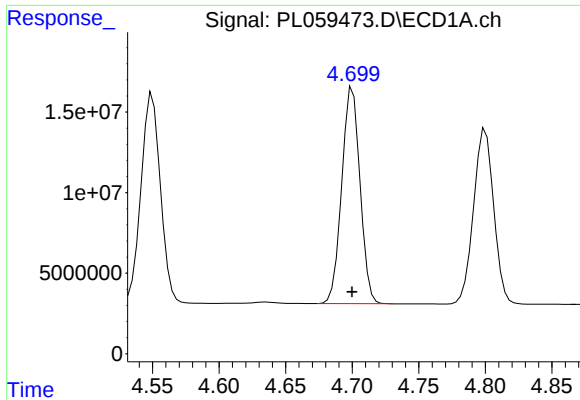


#7 delta-BHC

R.T.: 4.700 min
Delta R.T.: 0.000 min
Response: 128259067
Conc: 62.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
RB47184-RTMS


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:27 PM

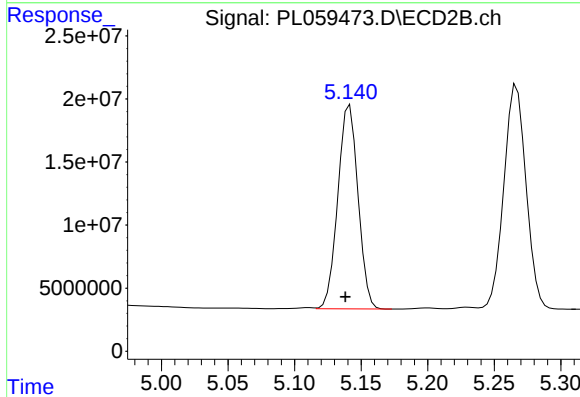


#7 delta-BHC

R.T.: 5.141 min
Delta R.T.: 0.003 min
Response: 170834501
Conc: 61.40 ng/ml

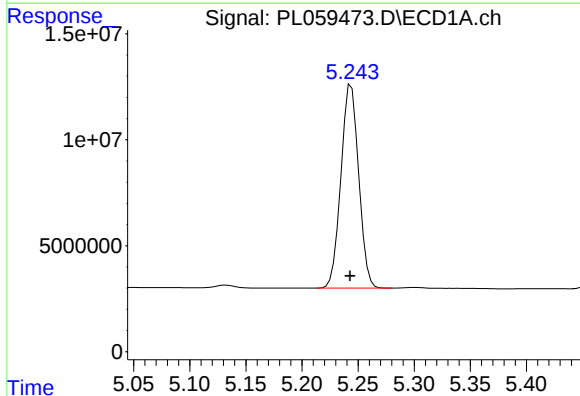


#8 Heptachlor epoxide

R.T.: 5.244 min
Delta R.T.: 0.001 min
Response: 105612351
Conc: 70.26 ng/ml

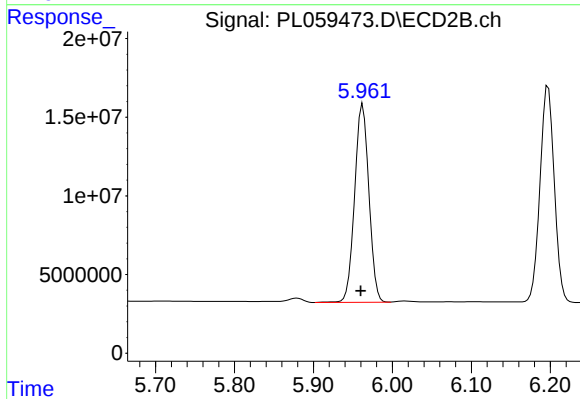

#8 Heptachlor epoxide

R.T.: 5.963 min
Delta R.T.: 0.003 min
Response: 158613266
Conc: 63.20 ng/ml

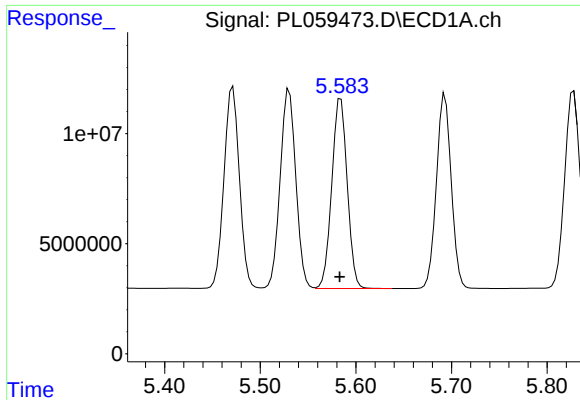


#9 Endosulfan I

R.T.: 5.584 min
Delta R.T.: 0.001 min
Response: 96582048
Conc: 65.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
RB47184-RTMS


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:27 PM

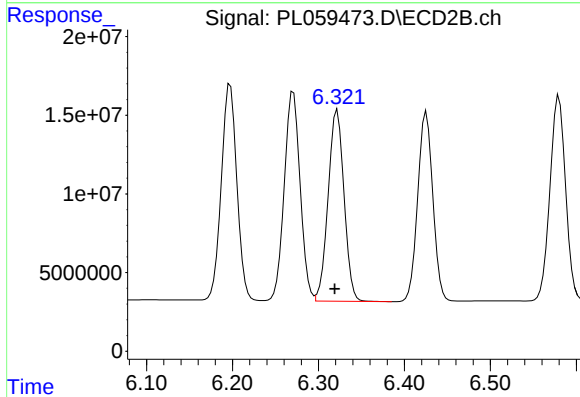


#9 Endosulfan I

R.T.: 6.322 min
Delta R.T.: 0.003 min
Response: 155977376
Conc: 57.47 ng/ml

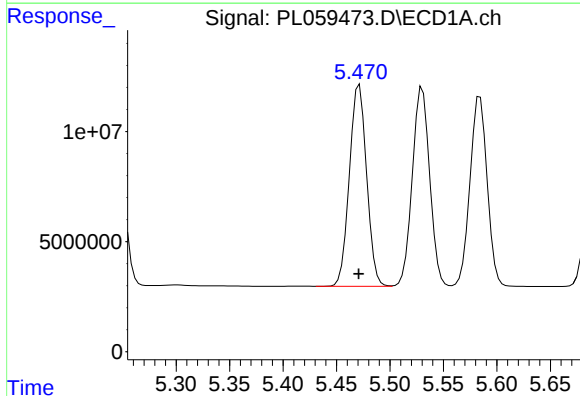


#10 gamma-Chlordane

R.T.: 5.471 min
Delta R.T.: 0.000 min
Response: 102859479
Conc: 67.06 ng/ml

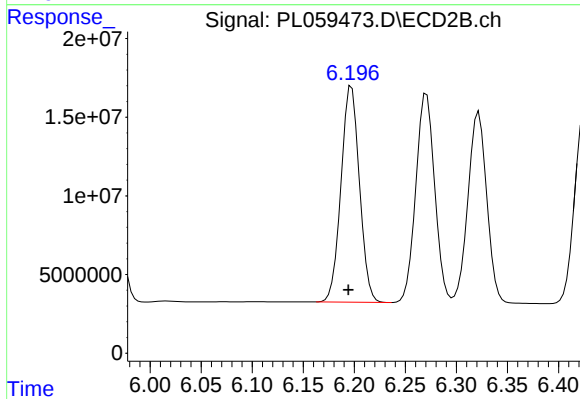

#10 gamma-Chlordane

R.T.: 6.197 min
Delta R.T.: 0.003 min
Response: 172691583
Conc: 58.96 ng/ml

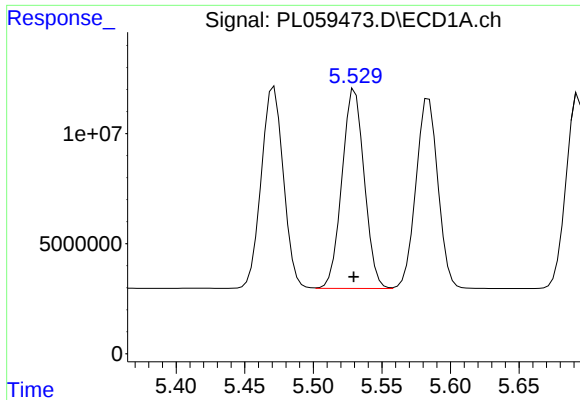


#11 alpha-Chlordane

R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 102574833
Conc: 66.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
RB47184-RTMS


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:27 PM

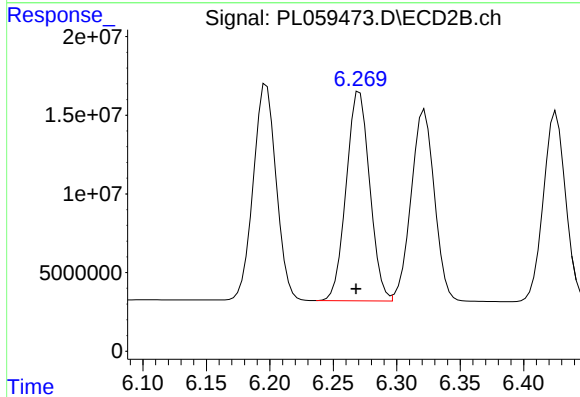


#11 alpha-Chlordane

R.T.: 6.271 min
Delta R.T.: 0.003 min
Response: 171315237
Conc: 58.18 ng/ml

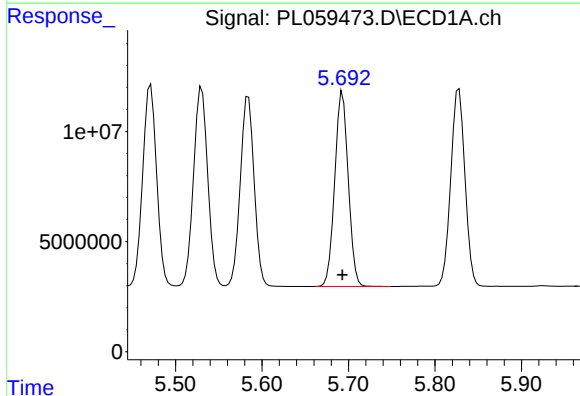


#12 4,4'-DDE

R.T.: 5.693 min
Delta R.T.: 0.000 min
Response: 95469592
Conc: 65.70 ng/ml

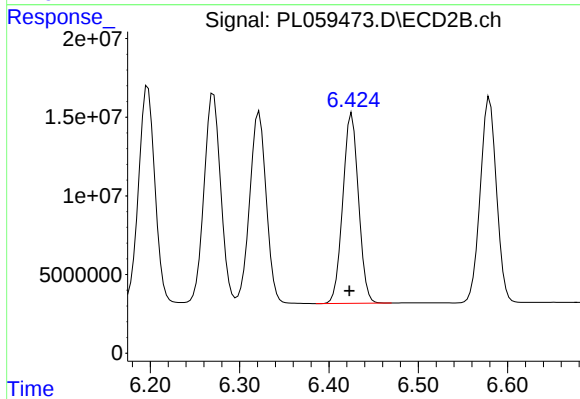

#12 4,4'-DDE

R.T.: 6.426 min
Delta R.T.: 0.003 min
Response: 147208909
Conc: 54.51 ng/ml

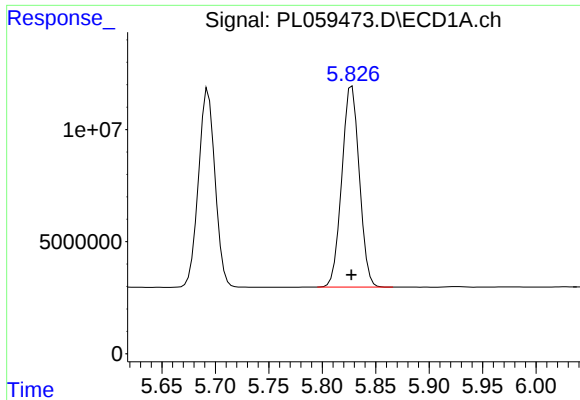


#13 Dieldrin

R.T.: 5.828 min
Delta R.T.: 0.000 min
Response: 102251861
Conc: 64.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
RB47184-RTMS


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:27 PM

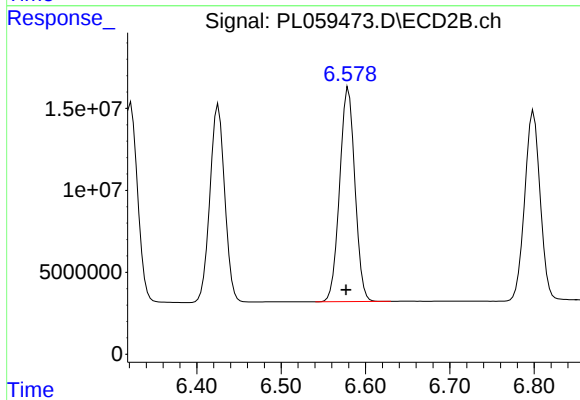


#13 Dieldrin

R.T.: 6.580 min
Delta R.T.: 0.003 min
Response: 164583360
Conc: 58.46 ng/ml

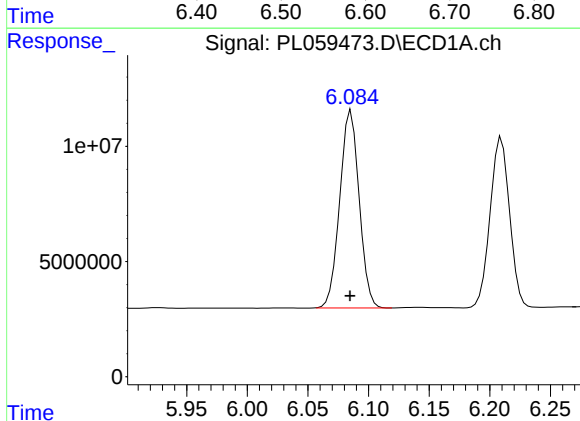


#14 Endrin

R.T.: 6.086 min
Delta R.T.: 0.000 min
Response: 95418570
Conc: 62.80 ng/ml

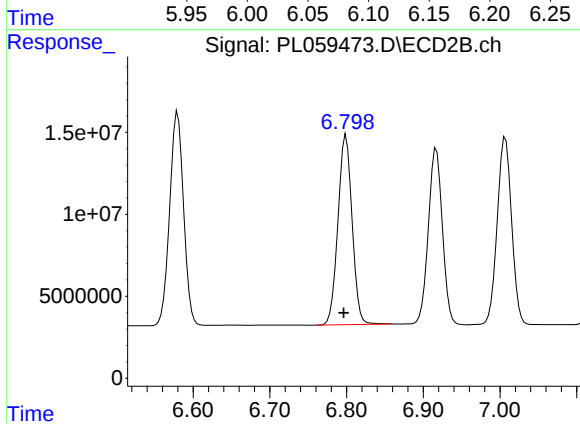

#14 Endrin

R.T.: 6.799 min
Delta R.T.: 0.003 min
Response: 148348858
Conc: 60.05 ng/ml

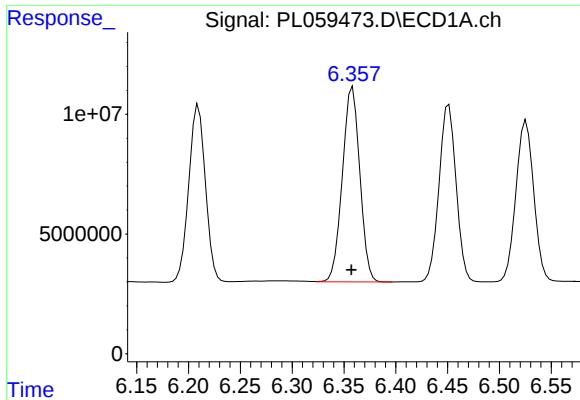


#15 Endosulfan II

R.T.: 6.358 min
Delta R.T.: 0.001 min
Response: 95340267
Conc: 61.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
RB47184-RTMS


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:27 PM

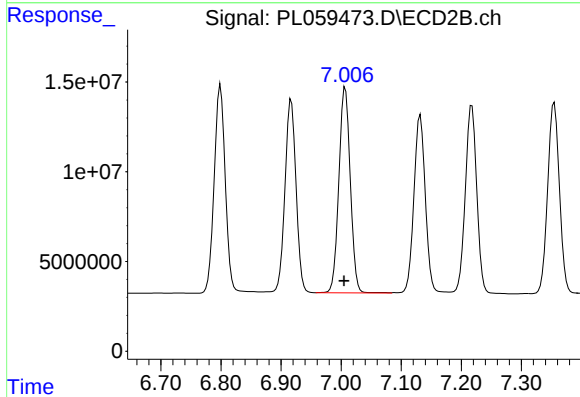


#15 Endosulfan II

R.T.: 7.007 min
Delta R.T.: 0.002 min
Response: 151297621
Conc: 59.66 ng/ml

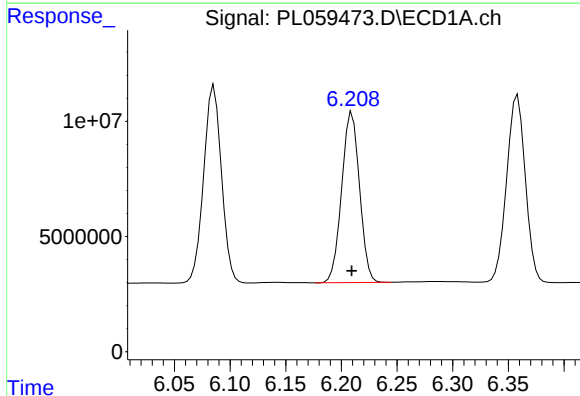


#16 4,4'-DDD

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 82543710
Conc: 63.25 ng/ml

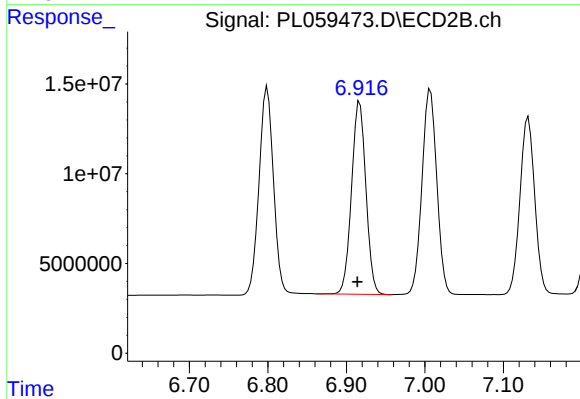

#16 4,4'-DDD

R.T.: 6.917 min
Delta R.T.: 0.003 min
Response: 136706663
Conc: 61.44 ng/ml

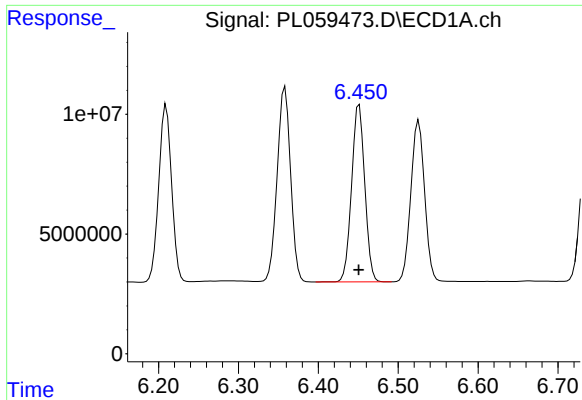


#17 4,4'-DDT

R.T.: 6.451 min
Delta R.T.: 0.000 min
Response: 85085964
Conc: 64.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
RB47184-RTMS


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:27 PM

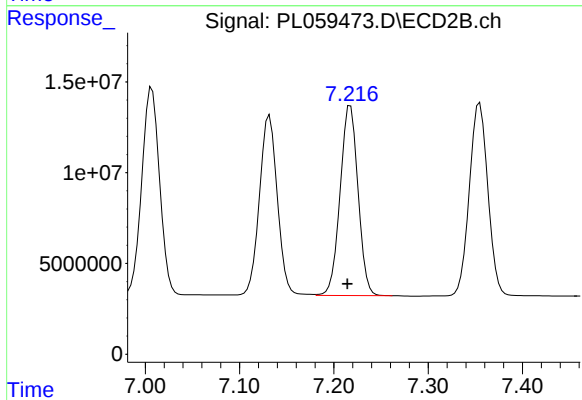


#17 4,4'-DDT

R.T.: 7.218 min
Delta R.T.: 0.003 min
Response: 138167563
Conc: 60.79 ng/ml

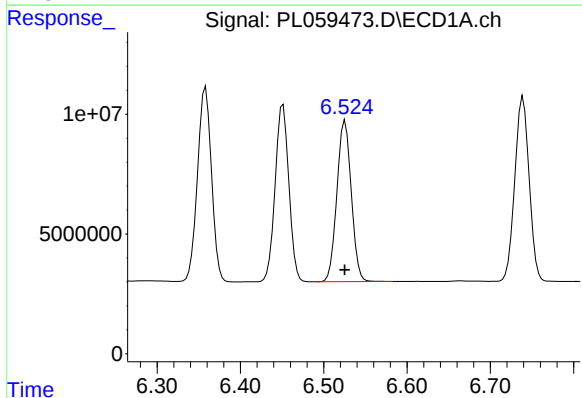


#18 Endrin aldehyde

R.T.: 6.526 min
Delta R.T.: 0.000 min
Response: 80868598
Conc: 61.19 ng/ml

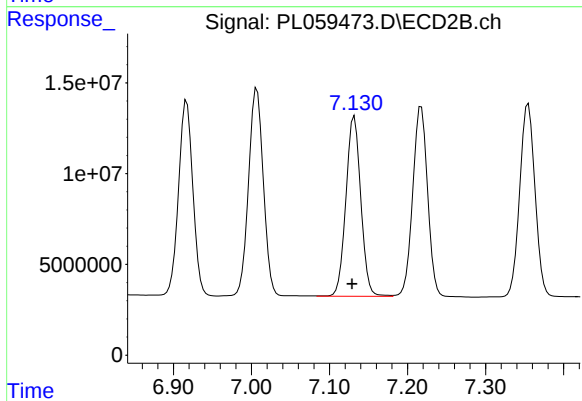

#18 Endrin aldehyde

R.T.: 7.132 min
Delta R.T.: 0.003 min
Response: 131628208
Conc: 60.01 ng/ml

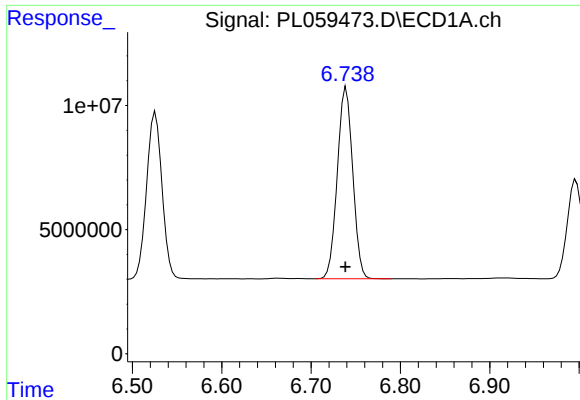


#19 Endosulfan Sulfate

R.T.: 6.739 min
Delta R.T.: 0.000 min
Response: 92349325
Conc: 60.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
RB47184-RTMS


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:27 PM

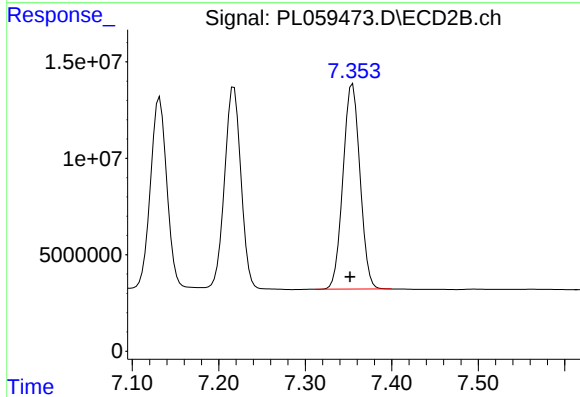


#19 Endosulfan Sulfate

R.T.: 7.355 min
Delta R.T.: 0.003 min
Response: 144626197
Conc: 59.75 ng/ml

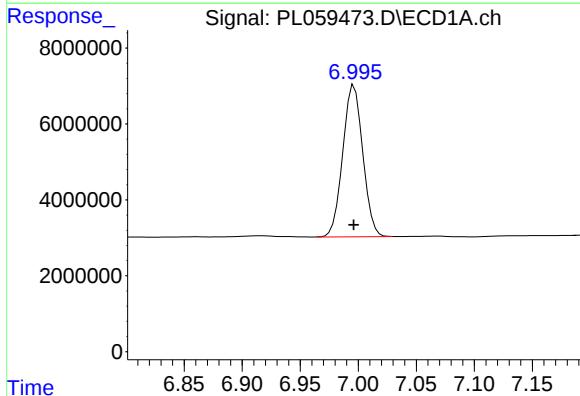


#20 Methoxychlor

R.T.: 6.997 min
Delta R.T.: 0.000 min
Response: 47910602
Conc: 59.12 ng/ml

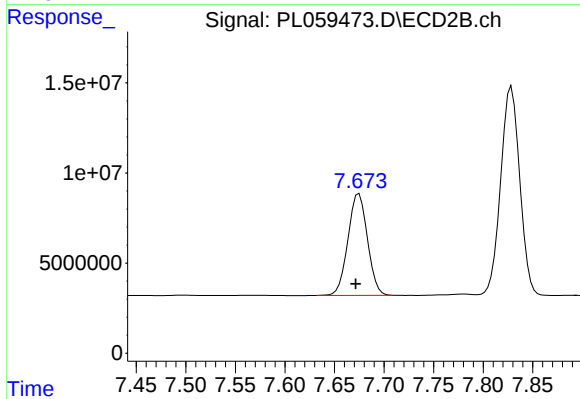

#20 Methoxychlor

R.T.: 7.675 min
Delta R.T.: 0.003 min
Response: 77224139
Conc: 58.17 ng/ml

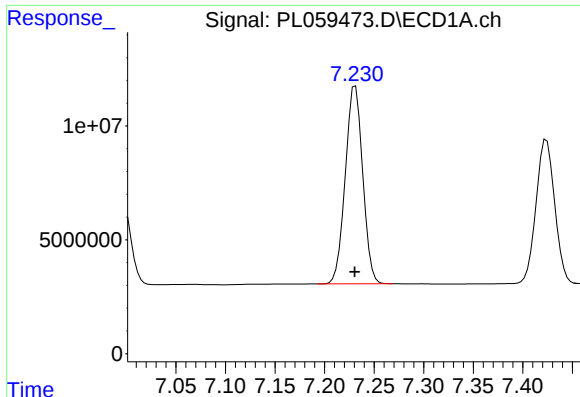


#21 Endrin ketone

R.T.: 7.231 min
Delta R.T.: 0.000 min
Response: 106235131
Conc: 60.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
RB47184-RTMS


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:27 PM

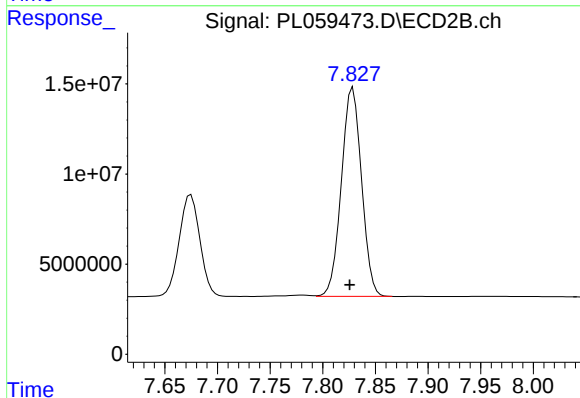


#21 Endrin ketone

R.T.: 7.829 min
Delta R.T.: 0.003 min
Response: 155130426
Conc: 60.05 ng/ml

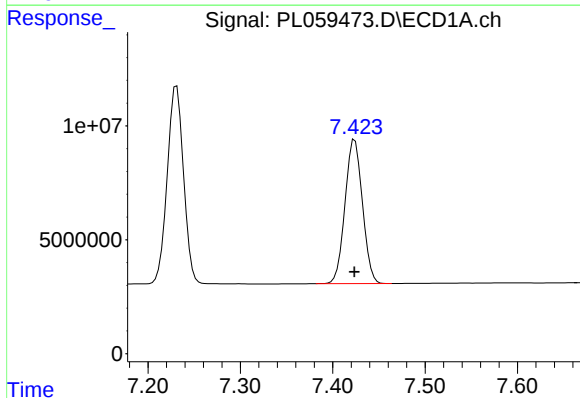


#22 Mirex

R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 82849348
Conc: 58.67 ng/ml

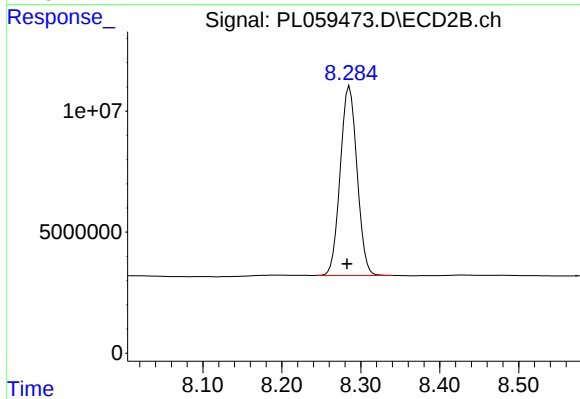

#22 Mirex

R.T.: 8.286 min
Delta R.T.: 0.003 min
Response: 115739196
Conc: 58.60 ng/ml

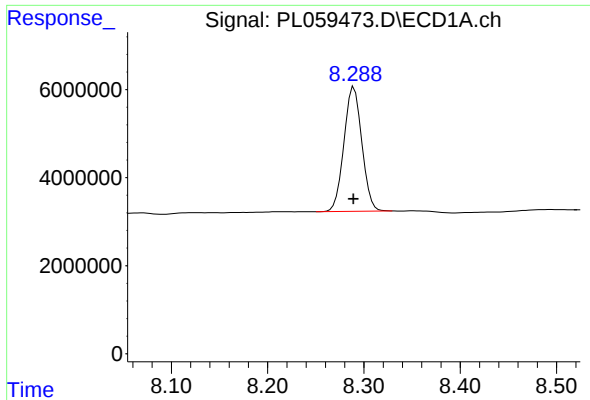


#28 Decachlorobiphenyl

R.T.: 8.290 min
Delta R.T.: 0.000 min
Response: 36380485
Conc: 21.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
RB47184-RTMS

Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:27 PM

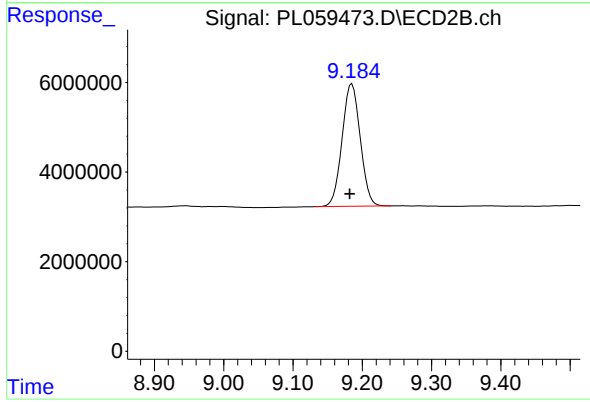

#28 Decachlorobiphenyl

R.T.: 9.185 min
Delta R.T.: 0.003 min
Response: 49747039
Conc: 21.73 ng/ml