

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062420\
 Data File : PL059485.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2020 20:31
 Operator : AJ\MA
 Sample : L3089-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RB47185-RT

Manual Integrations
 APPROVED

Ankita
 6/25/2020 1:29:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:12:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 22 14:09:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.518	4.072	23013408	33653896	12.806	13.039
28)	SA Decachlor...	8.289	9.185	15734703	21622239	9.240	9.444
Target Compounds							
12)	B 4,4'-DDE	5.693	6.422	669175	1370877	0.461	0.508m
17)	MA 4,4'-DDT	6.450	7.215	637183	966469	0.483	0.425m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062420\
Data File : PL059485.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2020 20:31
Operator : AJ\MA
Sample : L3089-07
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RB47185-RT


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:12:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
Quant Title : GC Extractables
QLast Update : Mon Jun 22 14:09:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

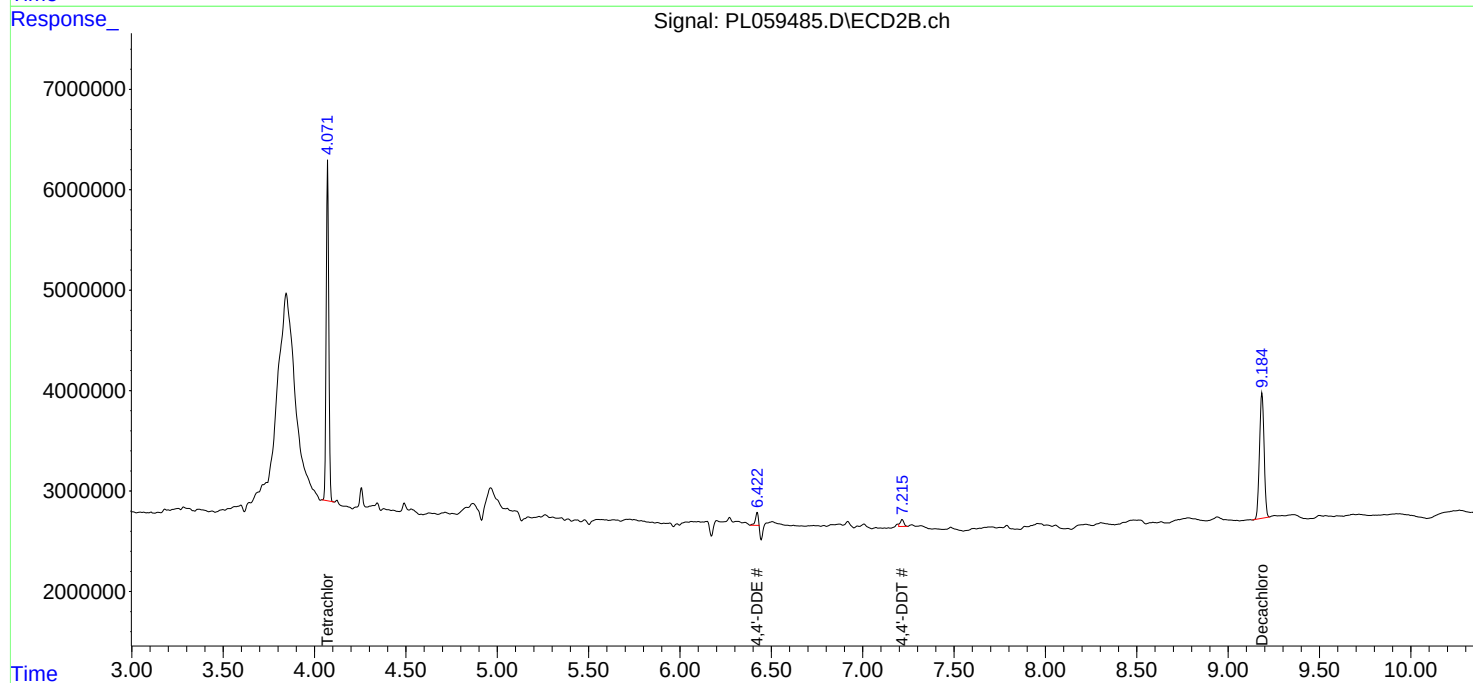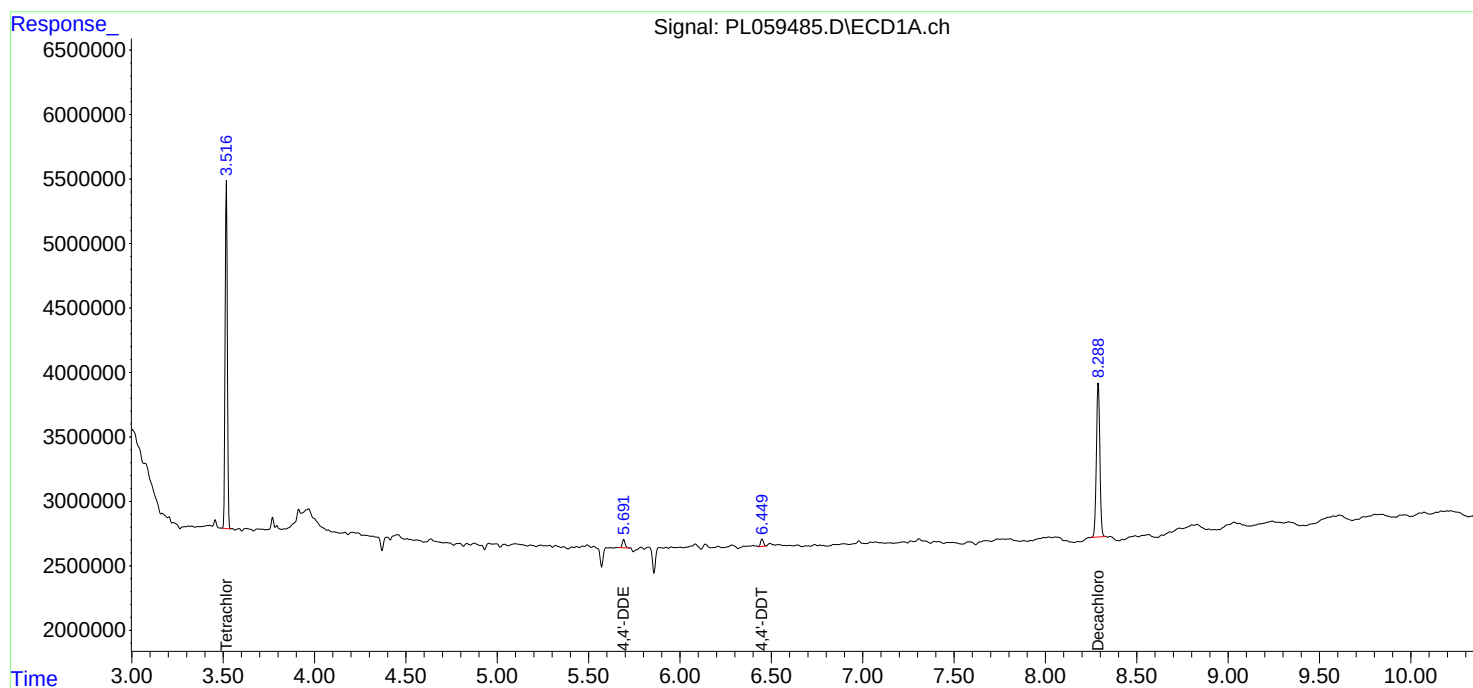

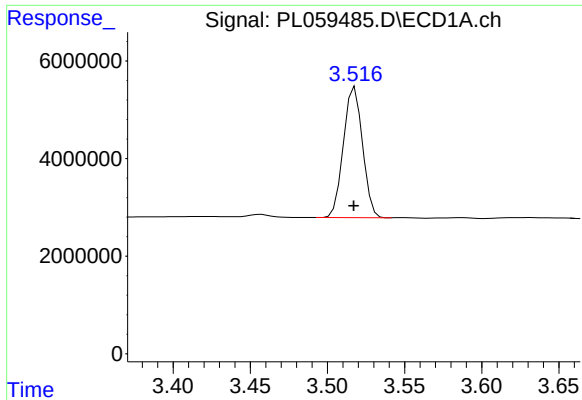


#1 Tetrachloro-m-xylene

R.T.: 3.518 min
Delta R.T.: 0.000 min
Response: 23013408
Conc: 12.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
RB47185-RT


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:55 PM

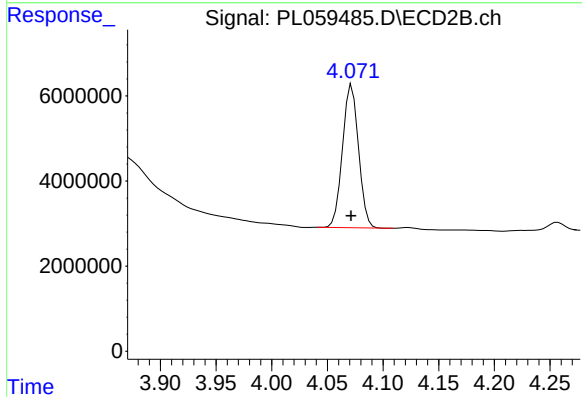


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 33653896
Conc: 13.04 ng/ml

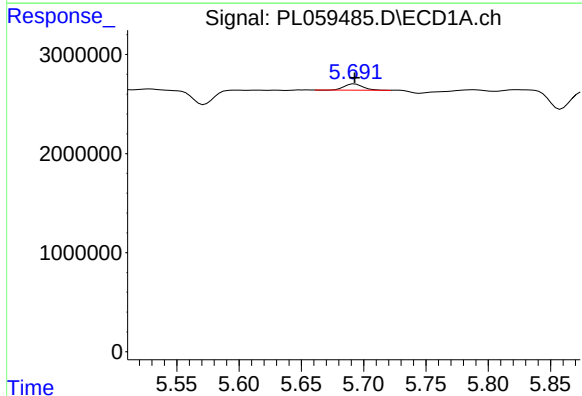


#12 4,4'-DDE

R.T.: 5.693 min
Delta R.T.: 0.000 min
Response: 669175
Conc: 0.46 ng/ml

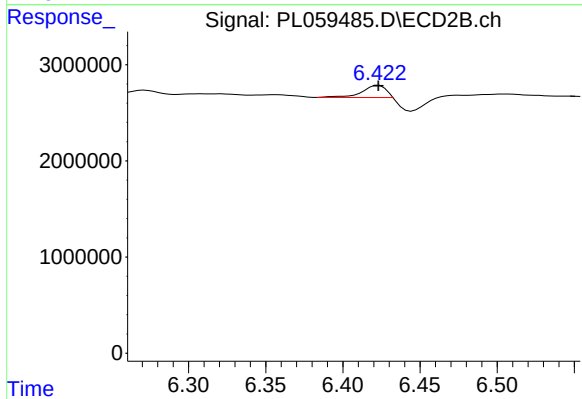

#12 4,4'-DDE

R.T.: 6.422 min
Delta R.T.: -0.001 min
Response: 1370877
Conc: 0.51 ng/ml m

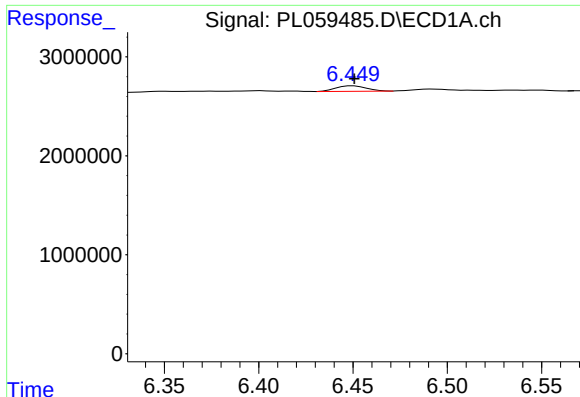


#17 4,4'-DDT

R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 637183
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
RB47185-RT


Manual Integrations
APPROVED

Ankita
6/25/2020 1:29:55 PM

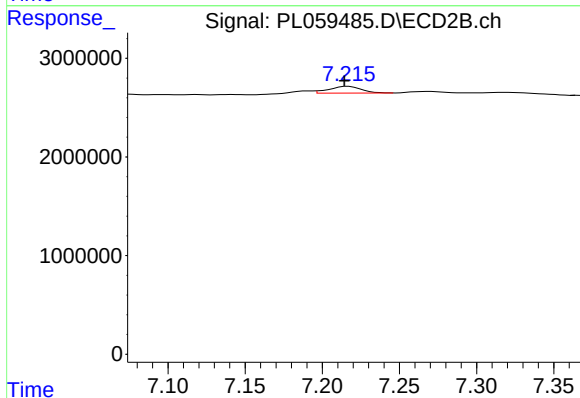


#17 4,4'-DDT

R.T.: 7.215 min
Delta R.T.: 0.001 min
Response: 966469
Conc: 0.43 ng/ml m

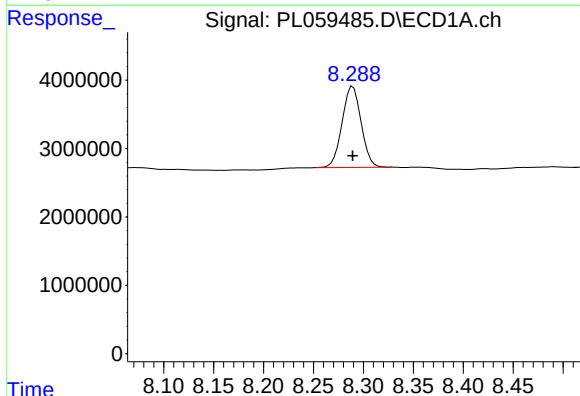

#28 Decachlorobiphenyl

R.T.: 8.289 min
Delta R.T.: 0.000 min
Response: 15734703
Conc: 9.24 ng/ml

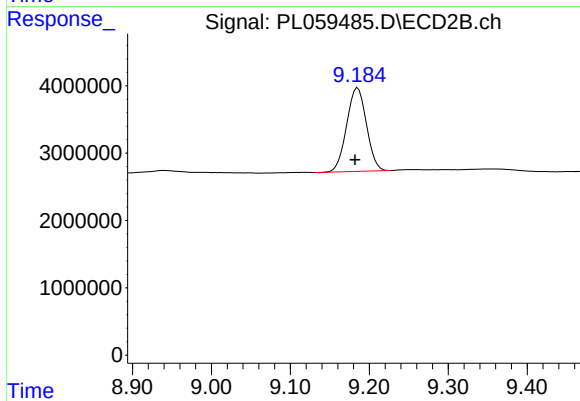

#28 Decachlorobiphenyl

R.T.: 9.185 min
Delta R.T.: 0.003 min
Response: 21622239
Conc: 9.44 ng/ml