

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062421\
 Data File : PL067785.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2021 17:40
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:23:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.477	5.527	10218564	19082547	18.586	20.242
28)	SA Decachlor...	10.216	11.421	13927284	20541848	19.652	20.623
Target Compounds							
2)	A alpha-BHC	5.163f	0.000	243777	0	0.331	N.D. #
4)	MA Heptachlor	5.985f	0.000	533162	0	0.707	N.D. #
6)	B beta-BHC	5.985	0.000	533162	0	1.490	N.D. #
15)	B Endosulfa...	0.000	9.178f	0	792543	N.D.	0.994 #
16)	A 4,4'-DDD	8.028f	0.000	153455	0	0.264	N.D. #
24)	Chlordane-2	6.483	0.000	290149	0	10.835	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062421\
Data File : PL067785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2021 17:40
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:23:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

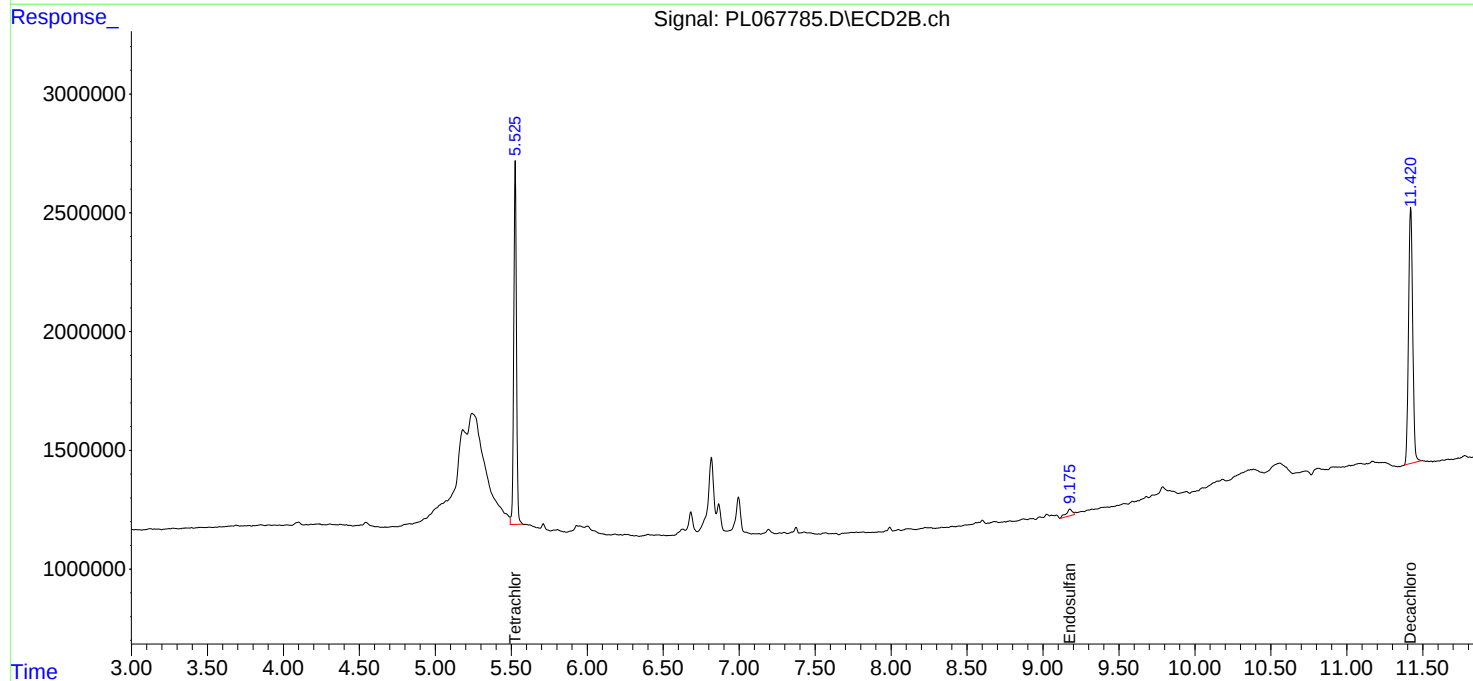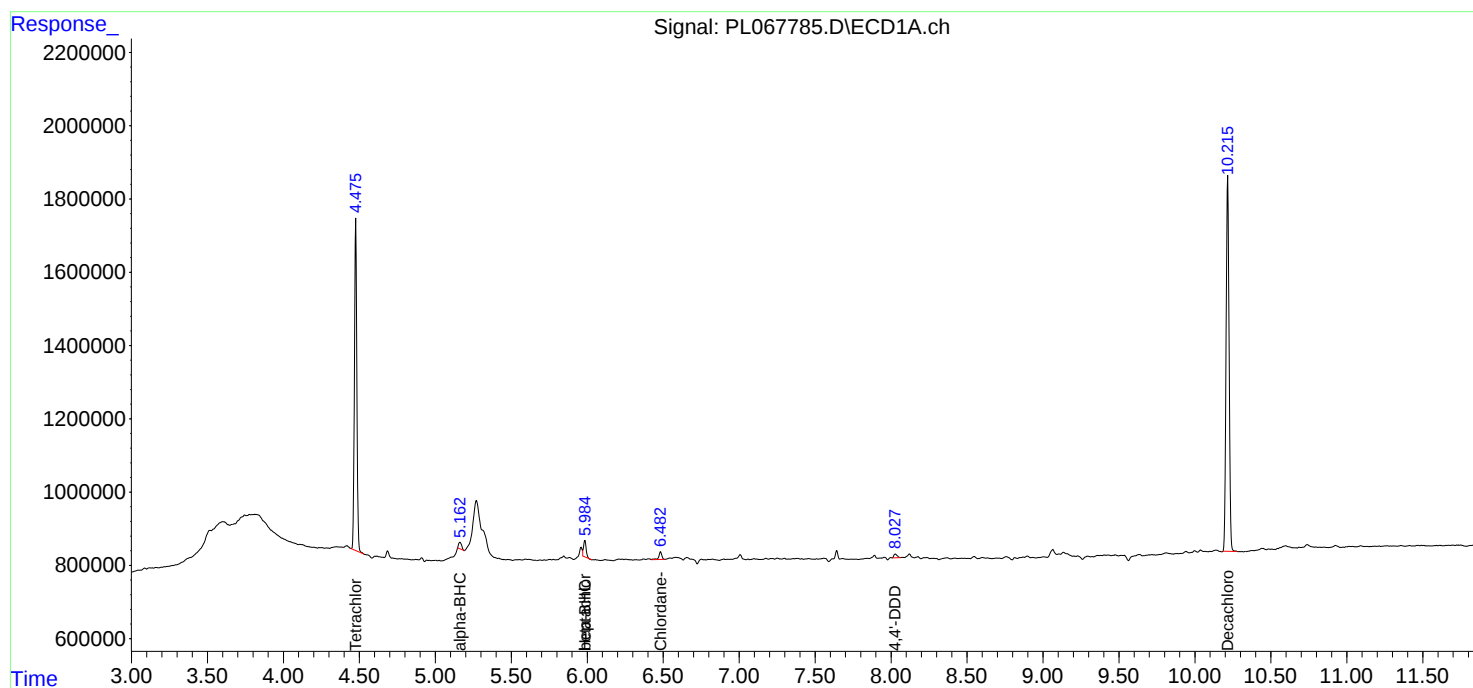


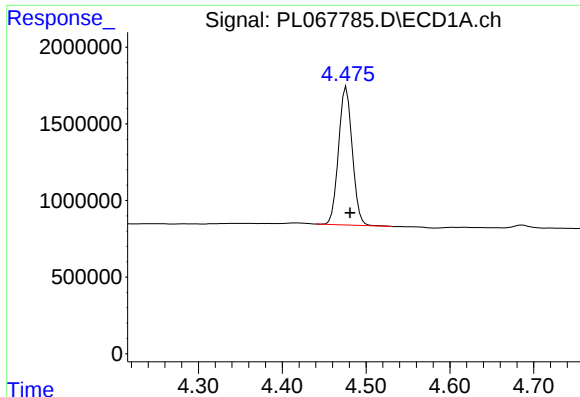

#1 Tetrachloro-m-xylene


R.T.: 4.477 min
Delta R.T.: -0.004 min
Response: 10218564
Conc: 18.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

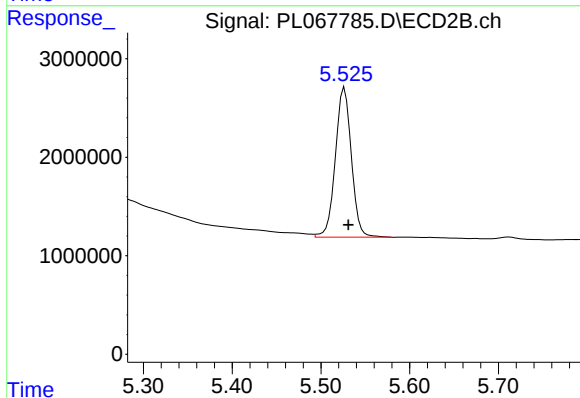


#1 Tetrachloro-m-xylene

R.T.: 5.527 min
Delta R.T.: -0.004 min
Response: 19082547
Conc: 20.24 ng/ml

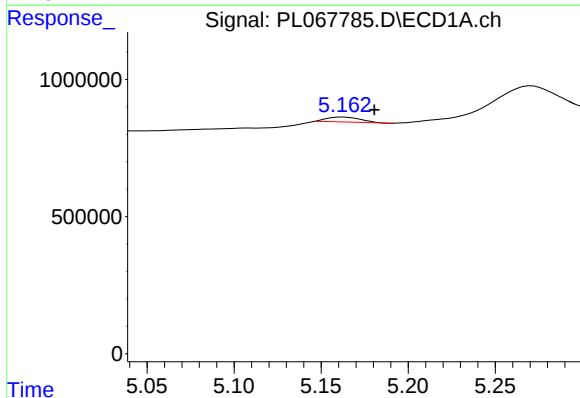


#2 alpha-BHC

R.T.: 5.163 min
Delta R.T.: -0.018 min
Response: 243777
Conc: 0.33 ng/ml

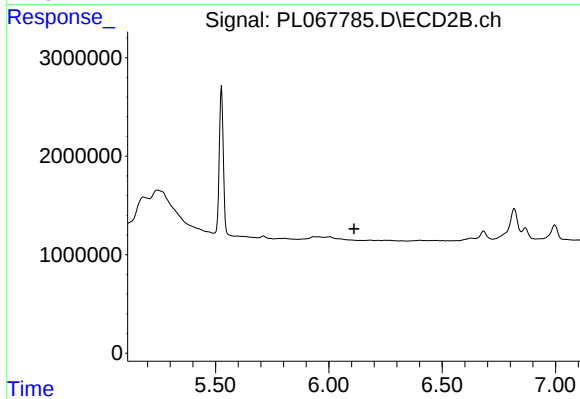

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

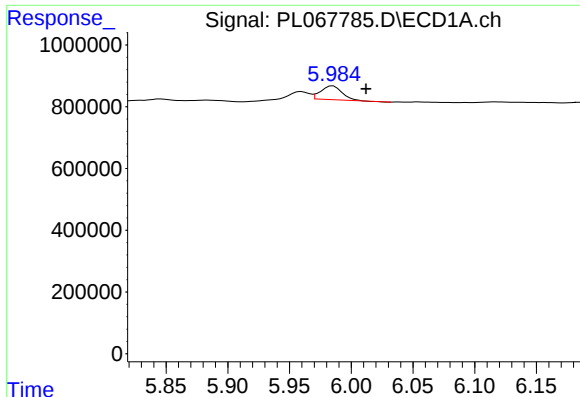

#4 Heptachlor


R.T.: 5.985 min
Delta R.T.: -0.027 min
Response: 533162
Conc: 0.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

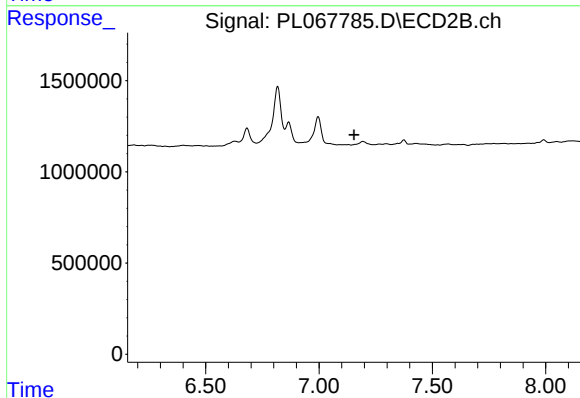


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

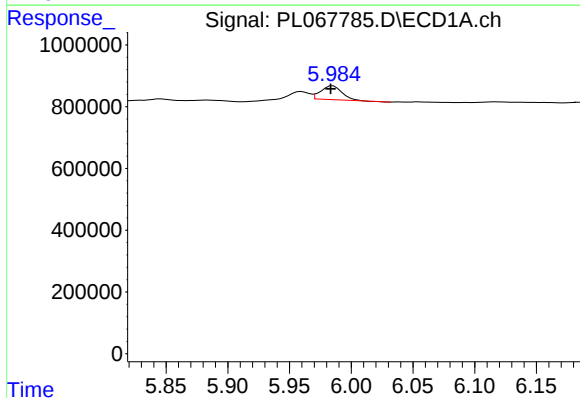


#6 beta-BHC

R.T.: 5.985 min
Delta R.T.: 0.002 min
Response: 533162
Conc: 1.49 ng/ml

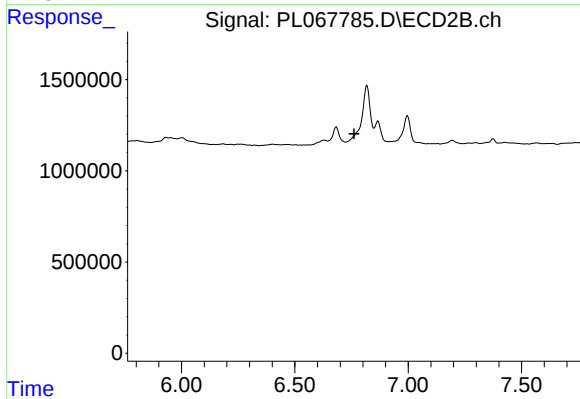

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

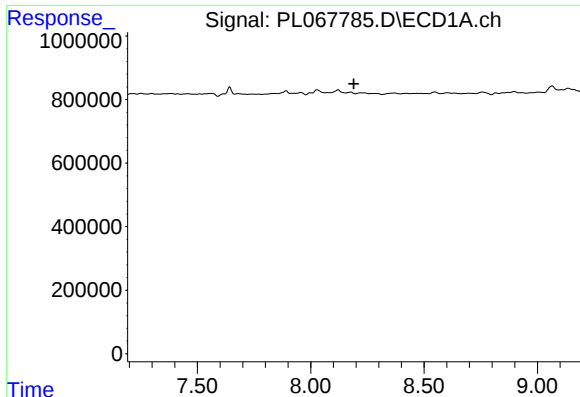

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

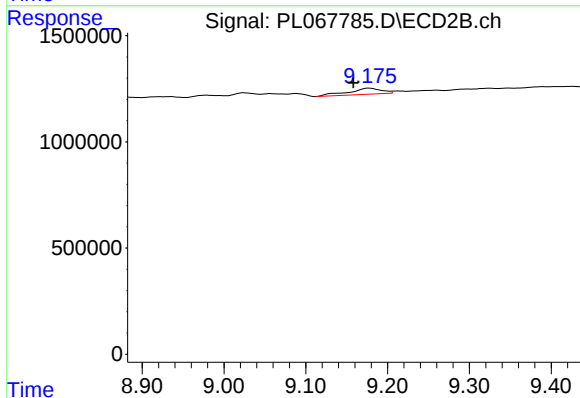


#15 Endosulfan II

R.T.: 9.178 min
Delta R.T.: 0.019 min
Response: 792543
Conc: 0.99 ng/ml

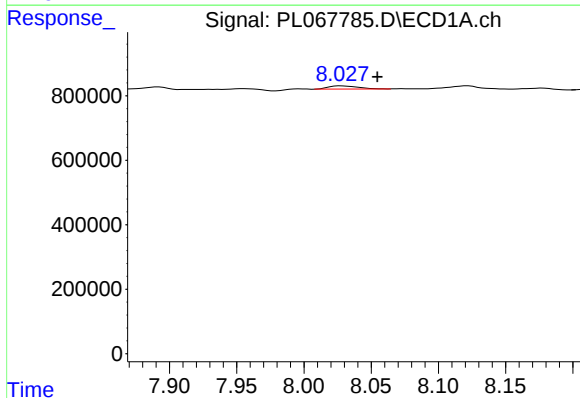


#16 4,4'-DDD

R.T.: 8.028 min
Delta R.T.: -0.027 min
Response: 153455
Conc: 0.26 ng/ml

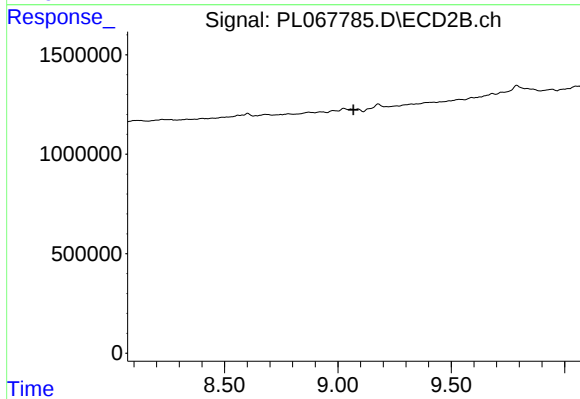

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 9.069 min
Response: 0
Conc: N.D.

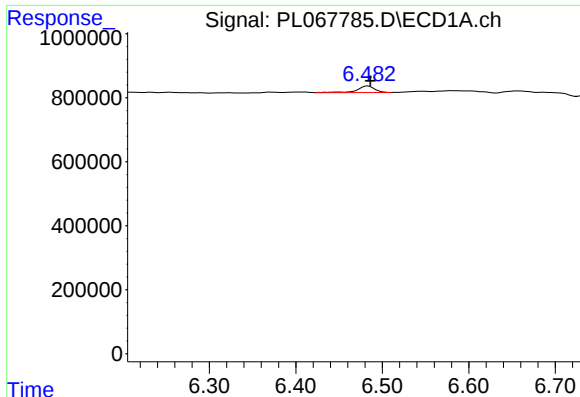

#24 Chlordane-2


R.T.: 6.483 min
Delta R.T.: -0.003 min
Response: 290149
Conc: 10.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

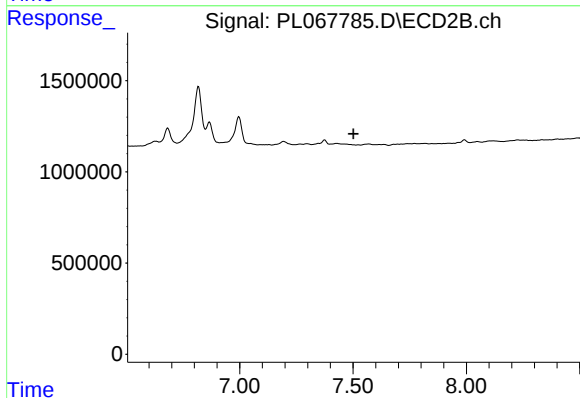


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

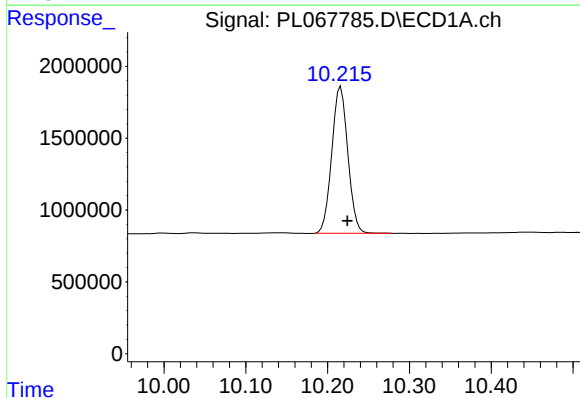

#28 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: -0.008 min
Response: 13927284
Conc: 19.65 ng/ml

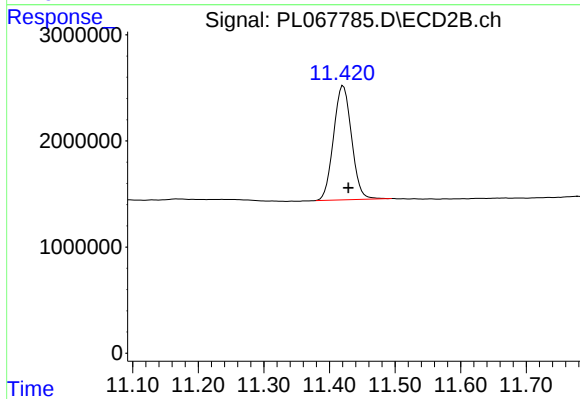

#28 Decachlorobiphenyl

R.T.: 11.421 min
Delta R.T.: -0.008 min
Response: 20541848
Conc: 20.62 ng/ml