

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062421\
 Data File : PL067773.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2021 11:43
 Operator : AR\AJ
 Sample : M2764-03RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PHC-250EM-002RE

Manual Integrations
 APPROVED

Ankita
 6/25/2021 9:49:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:19:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.483	5.526	6577689	10827881	11.964m	11.486
28)	SA Decachlor...	10.221	11.423	29210013	41414403	41.217	41.578

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062421\
Data File : PL067773.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2021 11:43
Operator : AR\AJ
Sample : M2764-03RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PHC-250EM-002RE


Manual Integrations
APPROVED

Ankita
6/25/2021 9:49:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:19:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

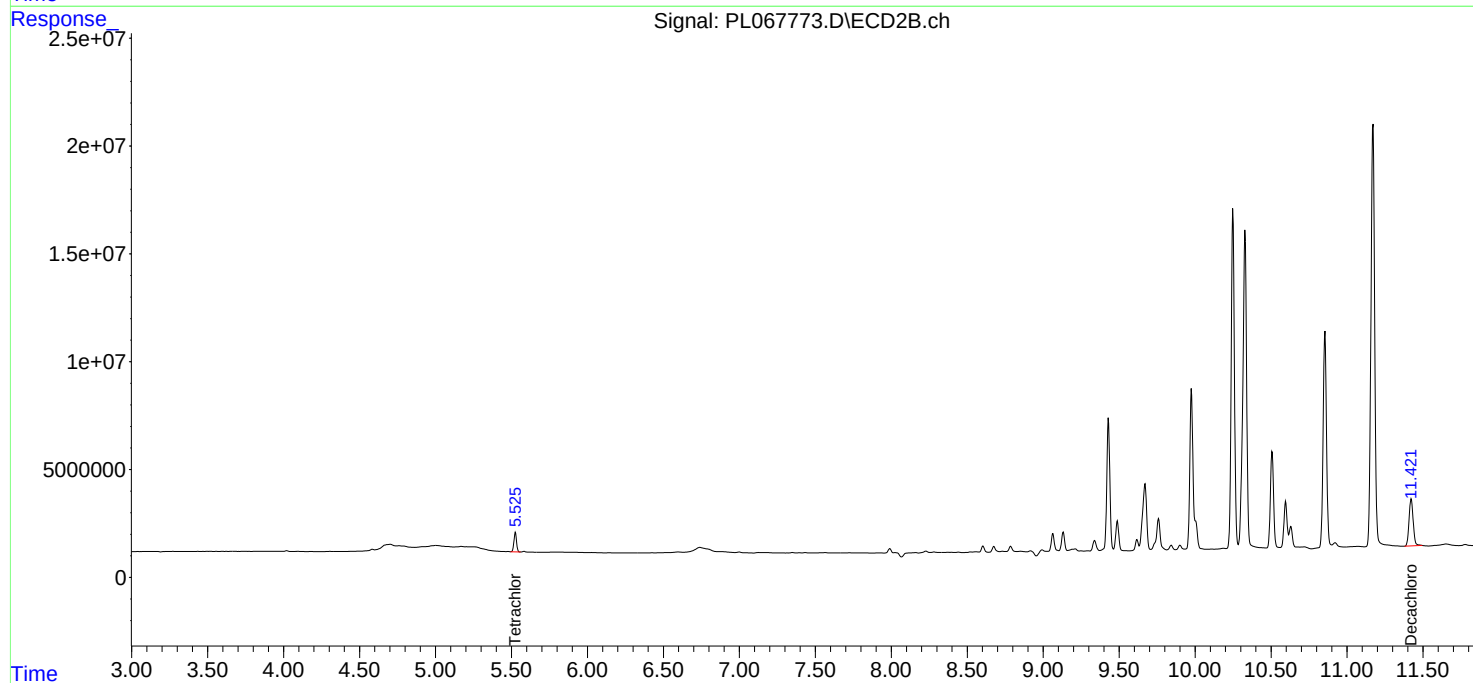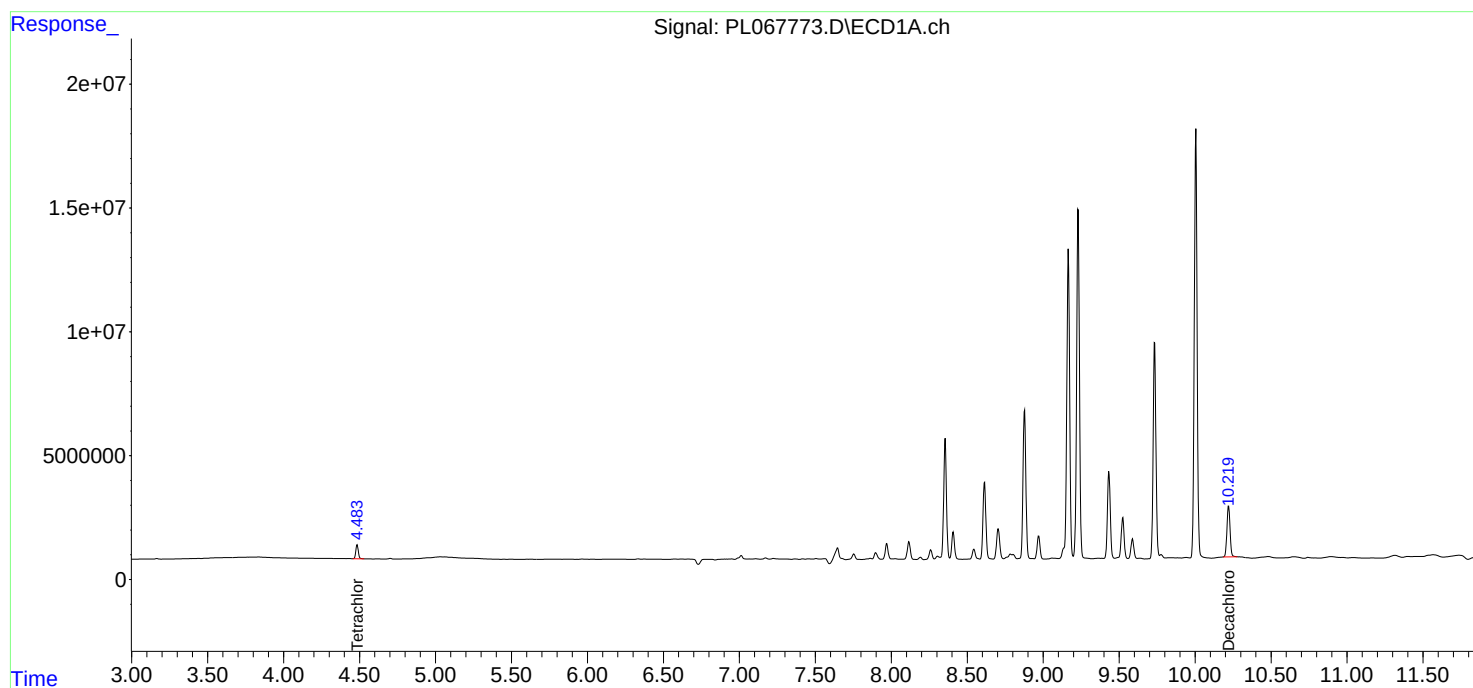

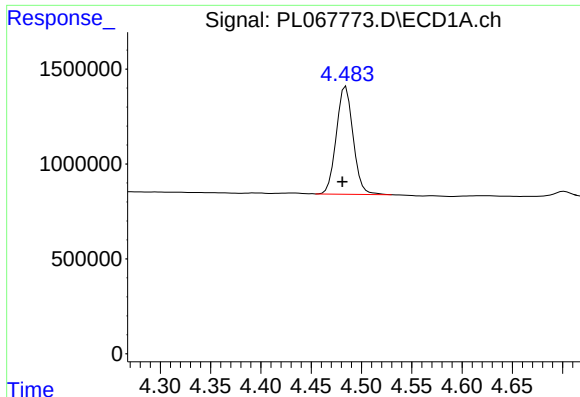

#1 Tetrachloro-m-xylene

R.T.: 4.483 min

Delta R.T.: 0.002 min


Response: 6577689

Conc: 11.96 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PHC-250EM-002RE

Manual Integrations
APPROVED

Ankita
6/25/2021 9:49:24 AM

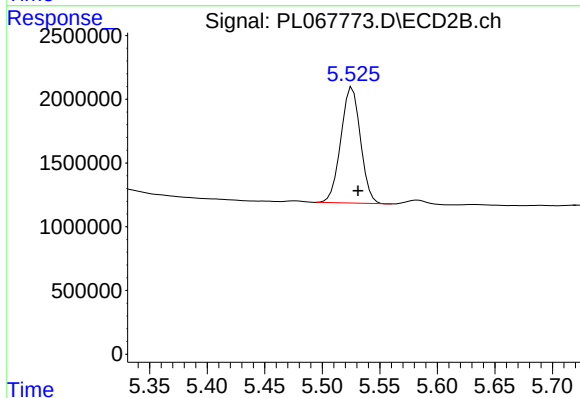


#1 Tetrachloro-m-xylene

R.T.: 5.526 min

Delta R.T.: -0.005 min

Response: 10827881

Conc: 11.49 ng/ml

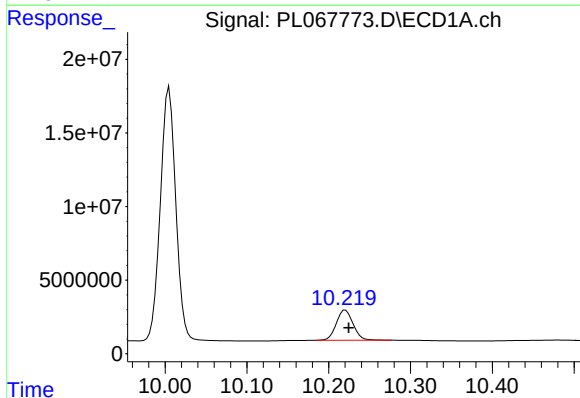


#28 Decachlorobiphenyl

R.T.: 10.221 min

Delta R.T.: -0.004 min

Response: 29210013

Conc: 41.22 ng/ml

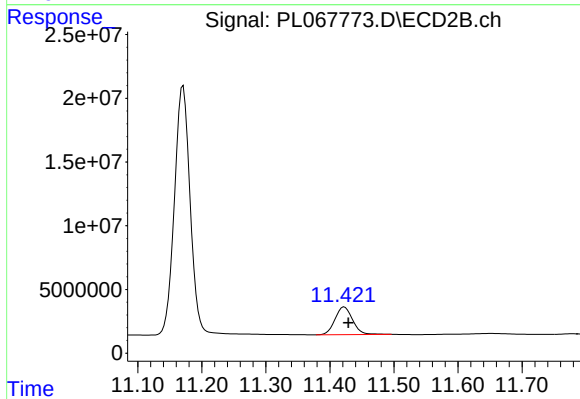

#28 Decachlorobiphenyl

R.T.: 11.423 min

Delta R.T.: -0.006 min

Response: 41414403

Conc: 41.58 ng/ml