

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062421\
 Data File : PL067778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2021 15:44
 Operator : AR\AJ
 Sample : M2819-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-062321

Manual Integrations
 APPROVED

Ankita
 6/25/2021 9:49:26 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:21:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.484	5.523	6015548	10359244	10.942	10.989
28)	SA Decachlor...	10.224	11.426	9497863	13736640	13.402	13.791
Target Compounds							
10)	B gamma-Chl...	7.185	8.254	389866	512441	0.538m	0.508m
11)	B alpha-Chl...	7.252	8.337	689672	1313929	0.942m	1.301m#
15)	B Endosulfa...	8.190	9.165	275877	1200693	0.448	1.506 #
17)	MA 4,4'-DDT	8.311	9.380	297771	433479	0.512m	0.591m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062421\
Data File : PL067778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2021 15:44
Operator : AR\AJ
Sample : M2819-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CL-02-062321


Manual Integrations
APPROVED

Ankita
6/25/2021 9:49:26 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:21:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

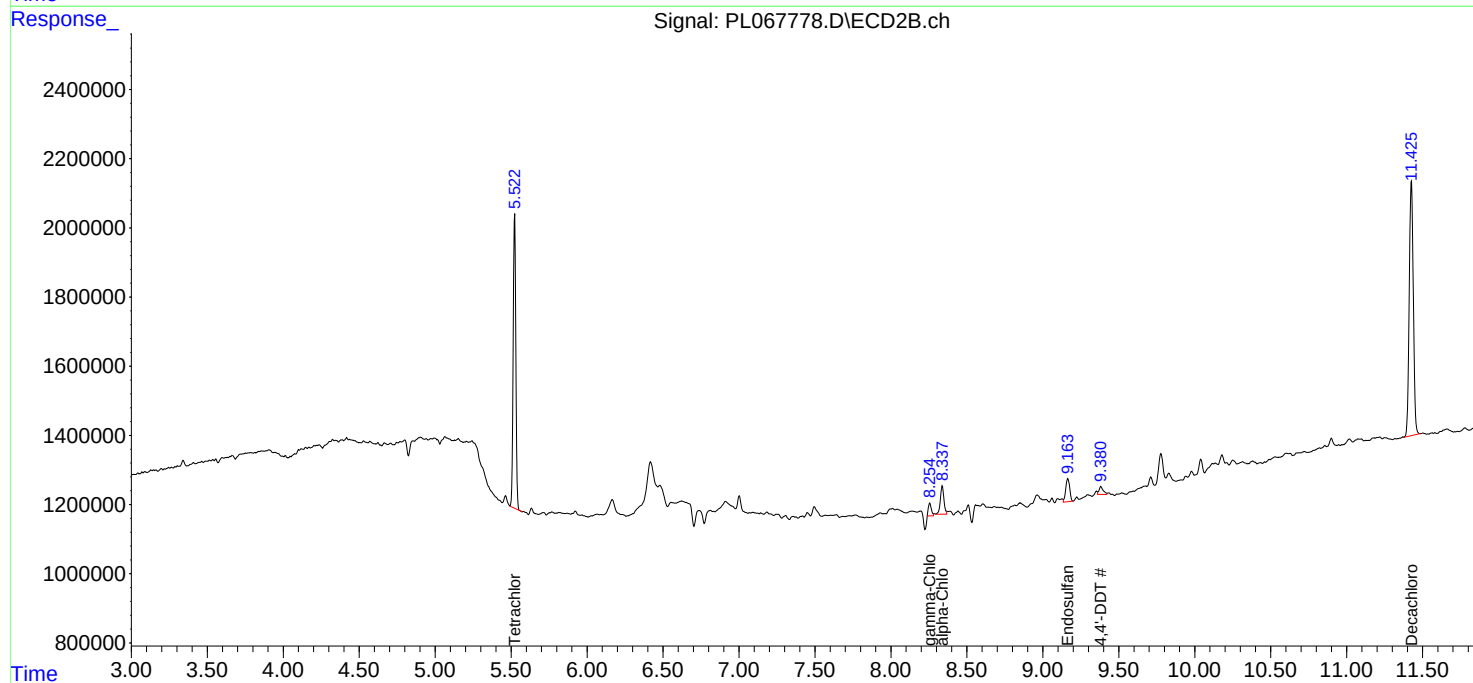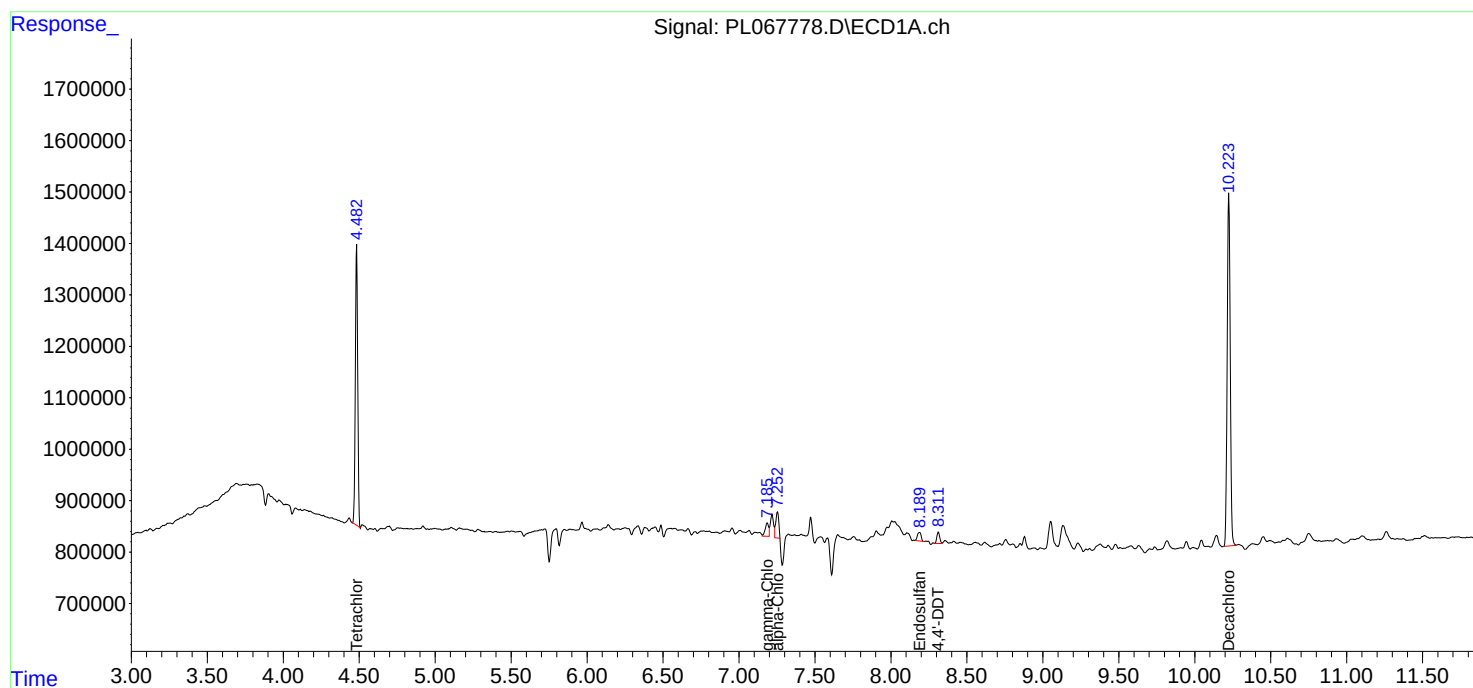

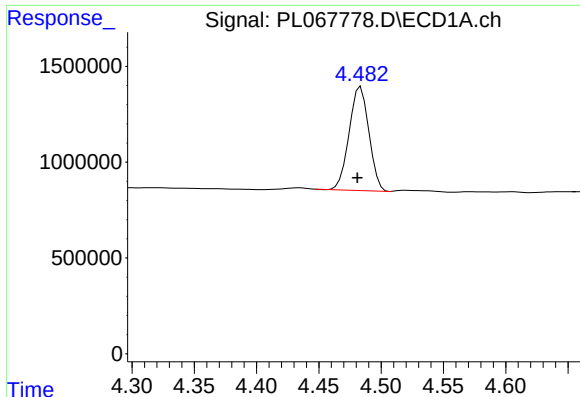


#1 Tetrachloro-m-xylene

R.T.: 4.484 min
Delta R.T.: 0.003 min
Response: 6015548
Conc: 10.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-062321


Manual Integrations
APPROVED

Ankita
6/25/2021 9:49:26 AM

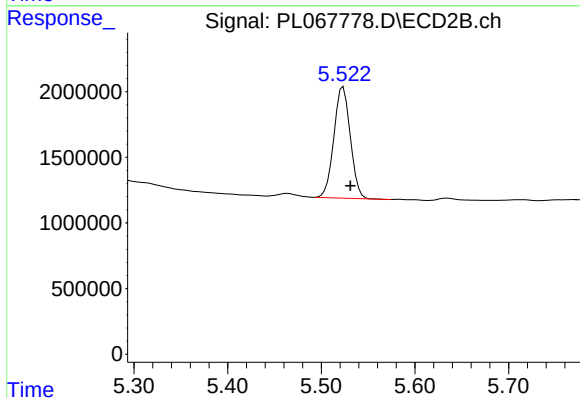


#1 Tetrachloro-m-xylene

R.T.: 5.523 min
Delta R.T.: -0.008 min
Response: 10359244
Conc: 10.99 ng/ml

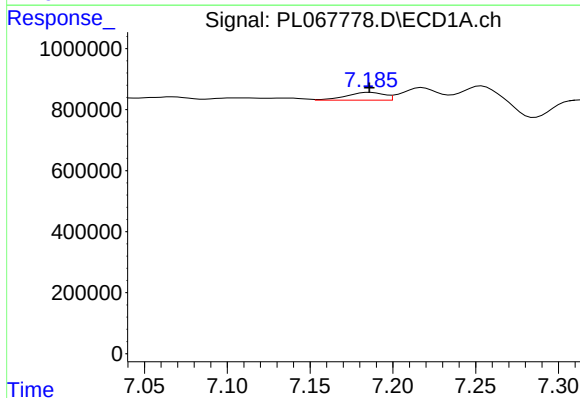


#10 gamma-Chlordane

R.T.: 7.185 min
Delta R.T.: 0.000 min
Response: 389866
Conc: 0.54 ng/ml m

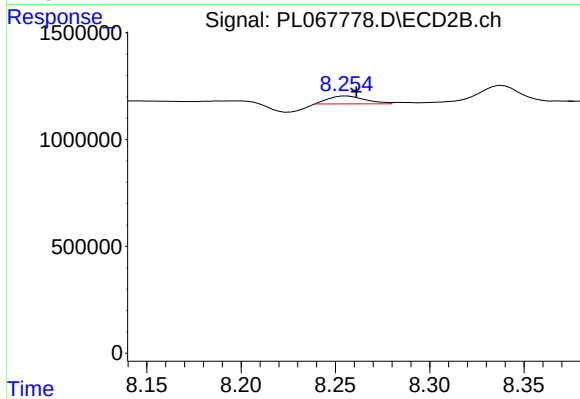

#10 gamma-Chlordane

R.T.: 8.254 min
Delta R.T.: -0.007 min
Response: 512441
Conc: 0.51 ng/ml m

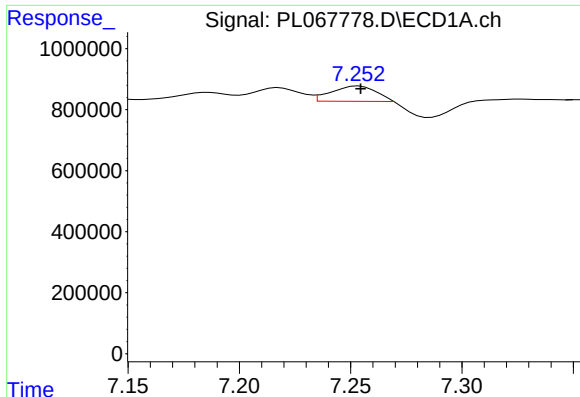


#11 alpha-Chlordane

R.T.: 7.252 min
Delta R.T.: -0.002 min
Response: 689672
Conc: 0.94 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CL-02-062321


Manual Integrations
APPROVED

Ankita
6/25/2021 9:49:26 AM

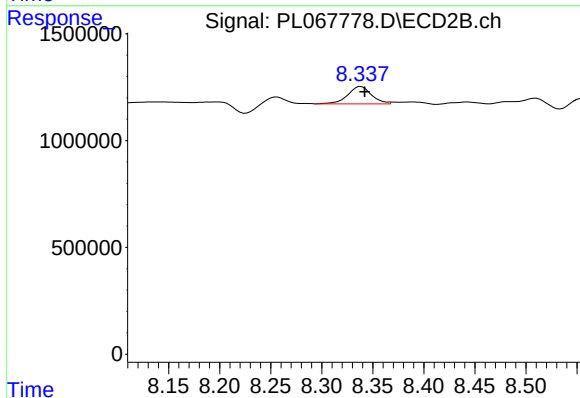


#11 alpha-Chlordane

R.T.: 8.337 min
Delta R.T.: -0.005 min
Response: 1313929
Conc: 1.30 ng/ml m

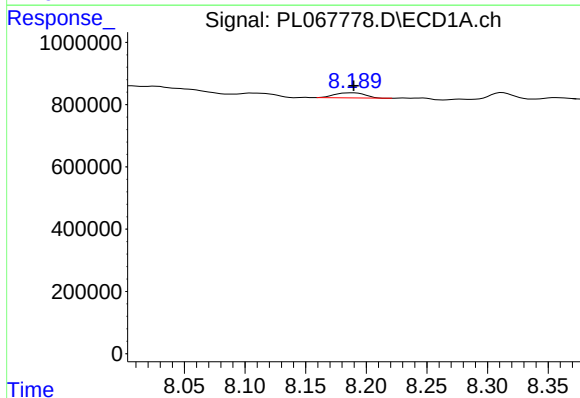


#15 Endosulfan II

R.T.: 8.190 min
Delta R.T.: 0.000 min
Response: 275877
Conc: 0.45 ng/ml

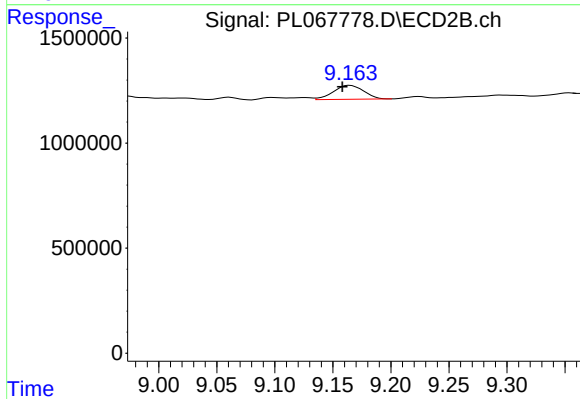

#15 Endosulfan II

R.T.: 9.165 min
Delta R.T.: 0.006 min
Response: 1200693
Conc: 1.51 ng/ml

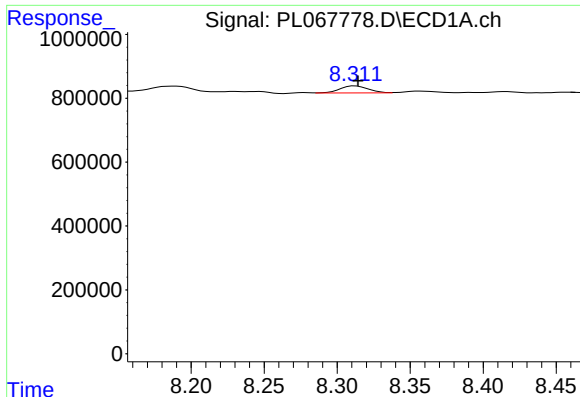


#17 4,4'-DDT

R.T.: 8.311 min
Delta R.T.: -0.003 min
Response: 297771
Conc: 0.51 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CL-02-062321


Manual Integrations
APPROVED

Ankita
6/25/2021 9:49:26 AM

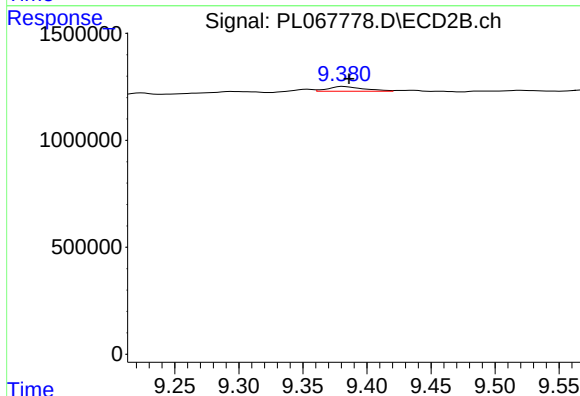


#17 4,4'-DDT

R.T.: 9.380 min
Delta R.T.: -0.006 min
Response: 433479
Conc: 0.59 ng/ml m

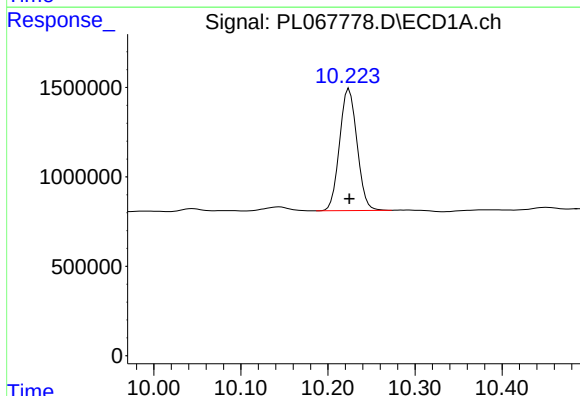

#28 Decachlorobiphenyl

R.T.: 10.224 min
Delta R.T.: 0.000 min
Response: 9497863
Conc: 13.40 ng/ml

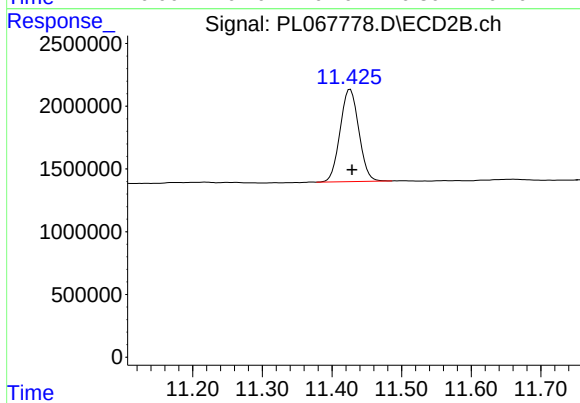

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.002 min
Response: 13736640
Conc: 13.79 ng/ml