

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062422\
 Data File : PL076002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2022 23:44
 Operator : AR\AJ
 Sample : PB145805BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 02:32:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.633	12100784	29868603	16.000	15.748
28)	SA Decachlor...	11.632	10.373	11302421	25852108	17.961	16.832
Target Compounds							
4)	MA Heptachlor	7.305f	0.000	259077	0	0.282	N.D. #
7)	B delta-BHC	0.000	6.399	0	202313	N.D.	0.090 #
10)	B gamma-Chl...	0.000	7.348	0	529698	N.D.	0.276 #
11)	B alpha-Chl...	0.000	7.380f	0	260111	N.D.	0.136 #
13)	MA Dieldrin	0.000	7.719f	0	245513	N.D.	0.136 #
14)	MA Endrin	0.000	8.059f	0	235449	N.D.	0.155 #
15)	B Endosulfa...	9.302	0.000	219995	0	0.347	N.D. #
21)	B Endrin ke...	10.182	0.000	700264	0	0.972	N.D. #
25)	Chlordane-3	0.000	7.348	0	529698	N.D.	3.003 #
26)	Chlordane-4	0.000	7.380f	0	260111	N.D.	1.380 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062422\
Data File : PL076002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2022 23:44
Operator : AR\AJ
Sample : PB145805BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 02:32:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

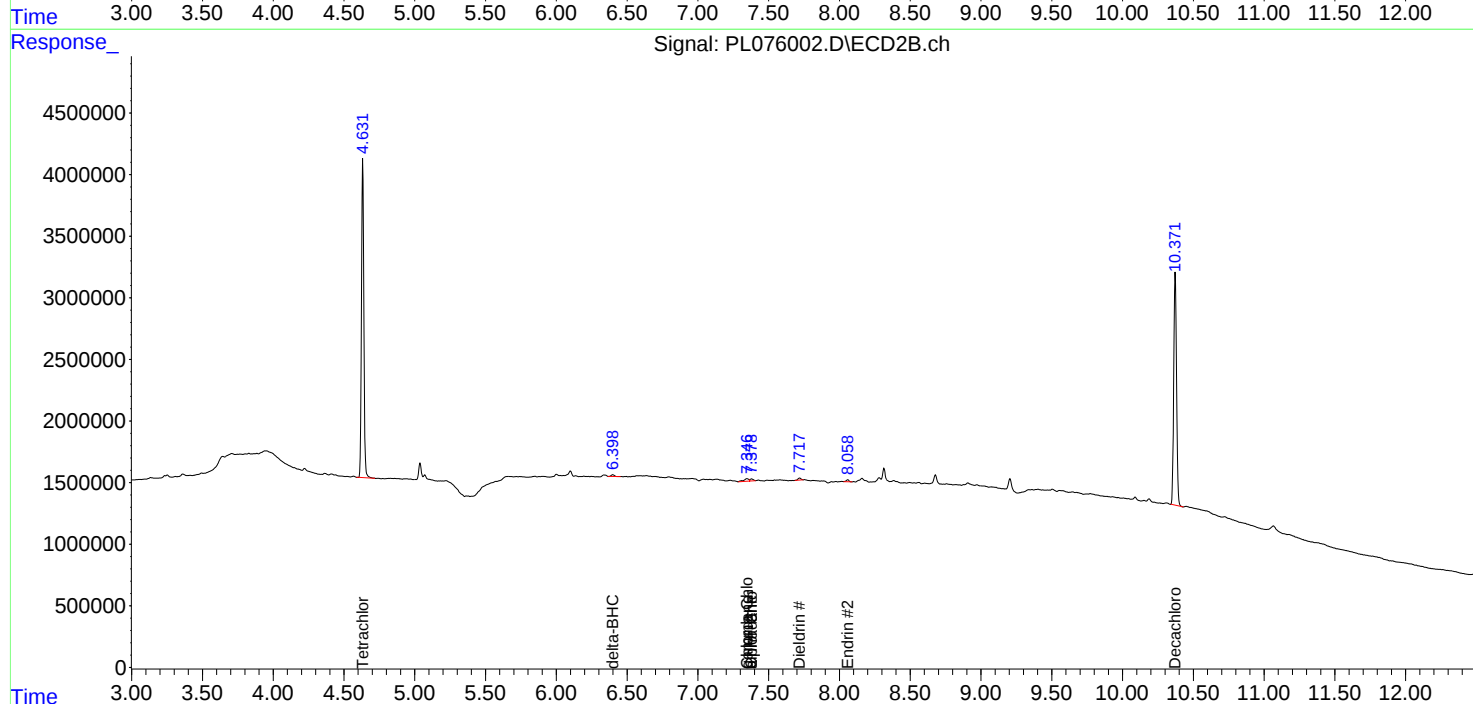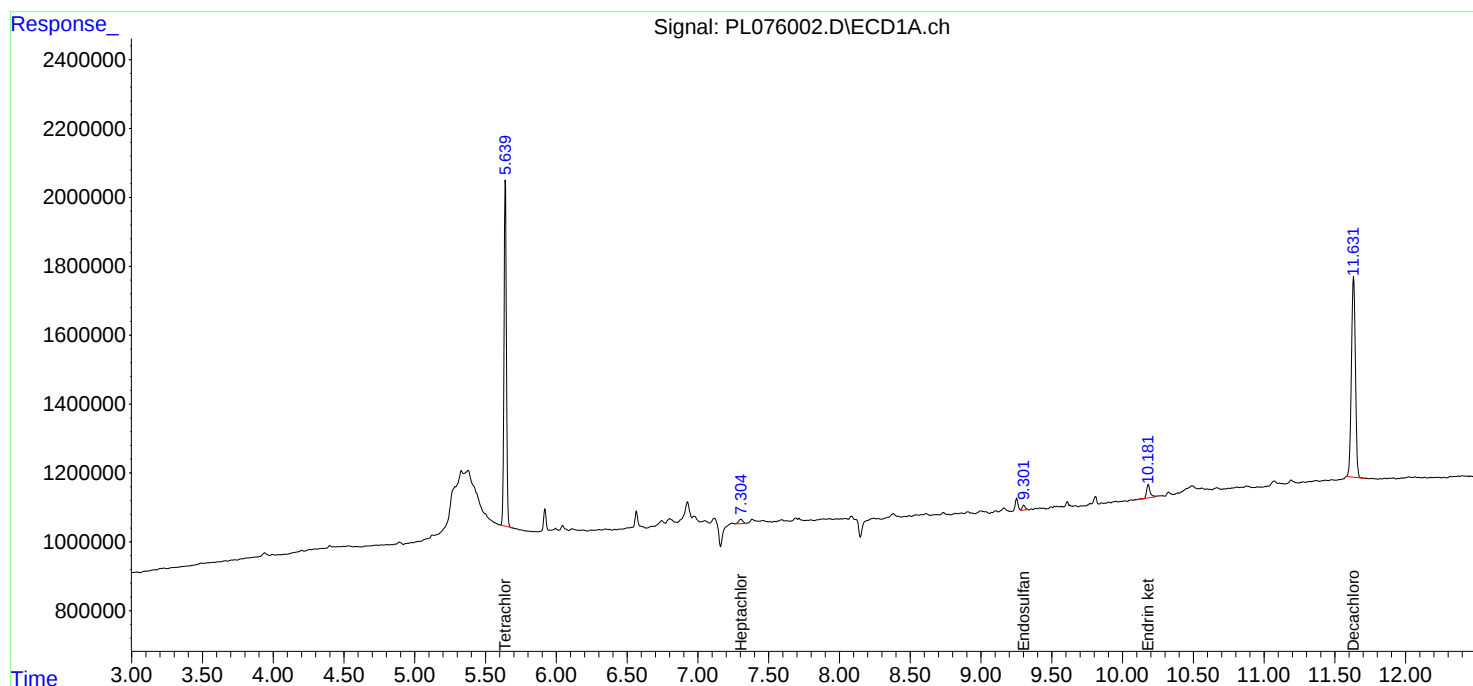


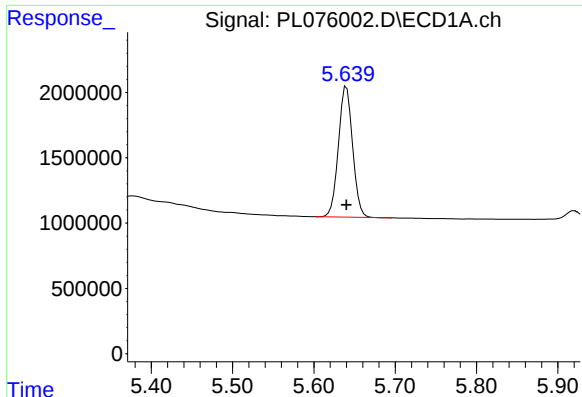

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 12100784
Conc: 16.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

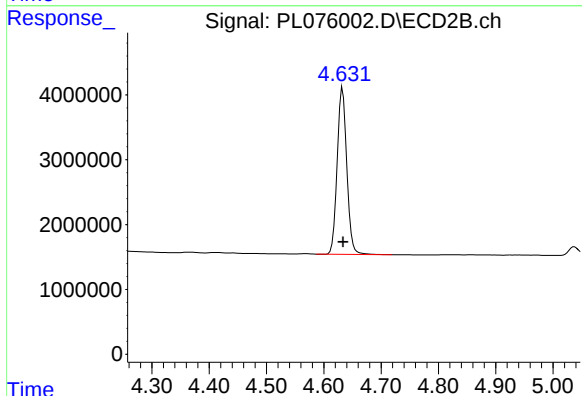


#1 Tetrachloro-m-xylene

R.T.: 4.633 min
Delta R.T.: -0.001 min
Response: 29868603
Conc: 15.75 ng/ml

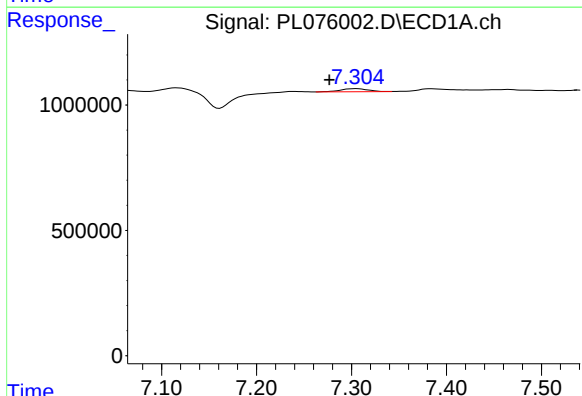


#4 Heptachlor

R.T.: 7.305 min
Delta R.T.: 0.028 min
Response: 259077
Conc: 0.28 ng/ml

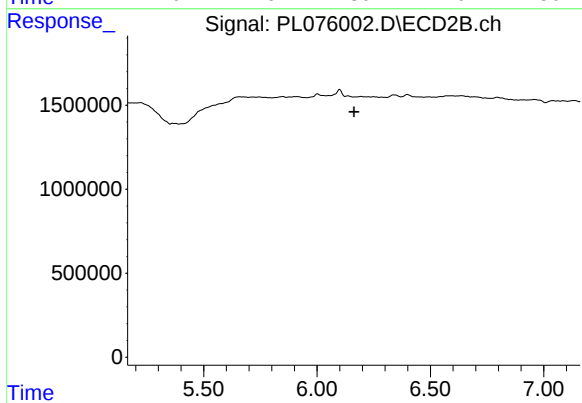

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 6.163 min
Response: 0
Conc: N.D.

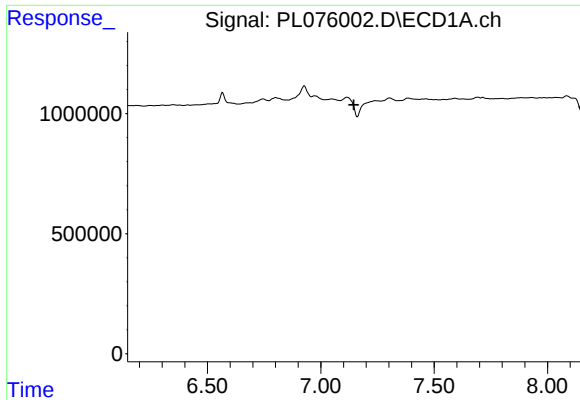

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

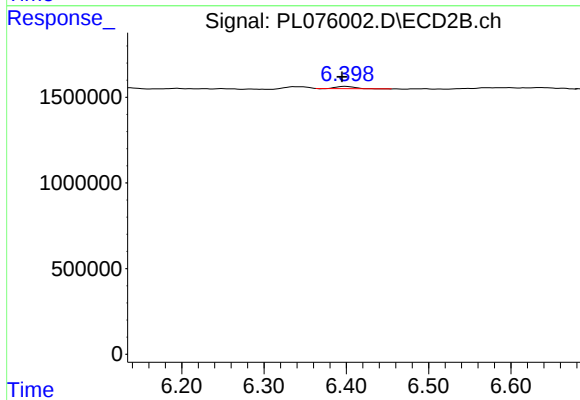


#7 delta-BHC

R.T.: 6.399 min
Delta R.T.: 0.004 min
Response: 202313
Conc: 0.09 ng/ml

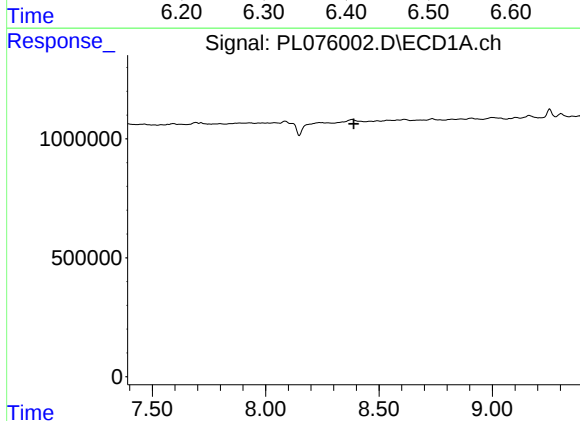


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 8.389 min
Response: 0
Conc: N.D.

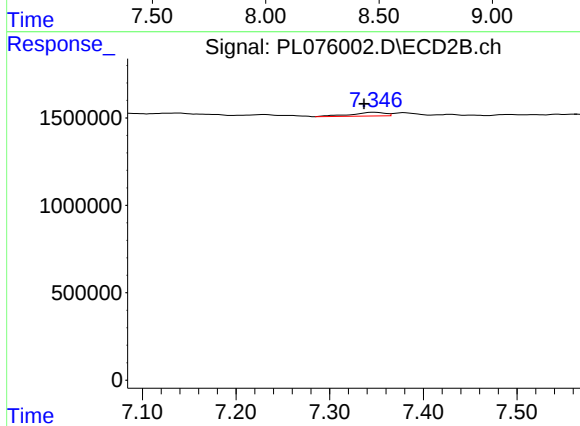

#10 gamma-Chlordane


R.T.: 7.348 min
Delta R.T.: 0.011 min
Response: 529698
Conc: 0.28 ng/ml

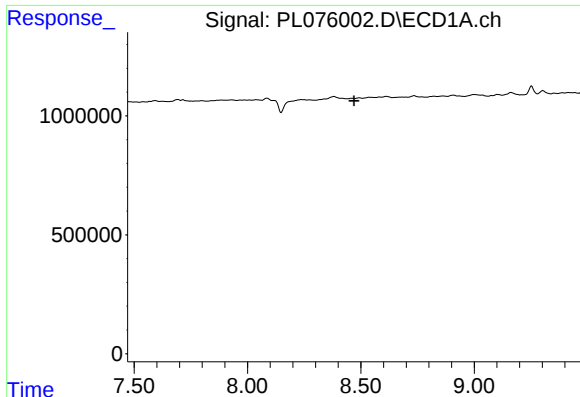

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

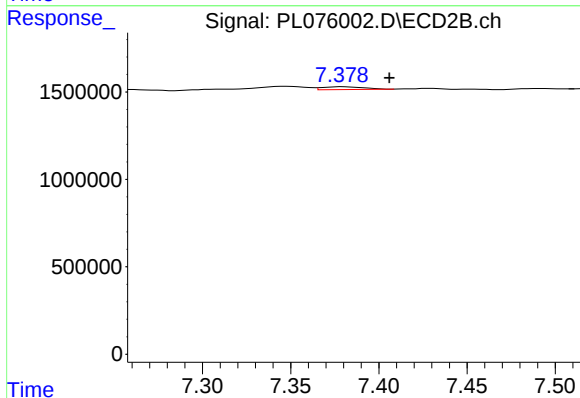


#11 alpha-Chlordane

R.T.: 7.380 min
Delta R.T.: -0.026 min
Response: 260111
Conc: 0.14 ng/ml

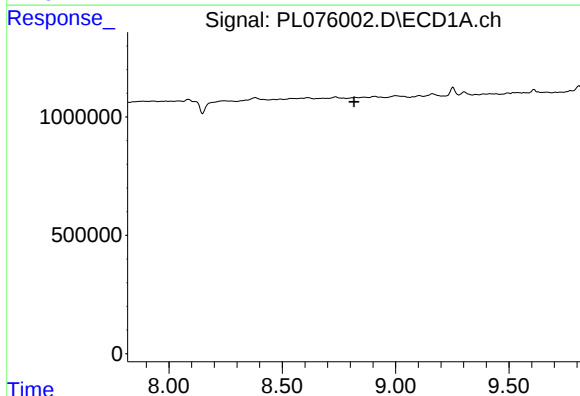


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.817 min
Response: 0
Conc: N.D.

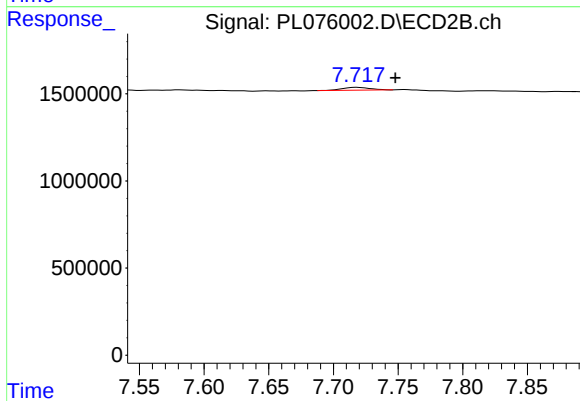

#13 Dieldrin


R.T.: 7.719 min
Delta R.T.: -0.029 min
Response: 245513
Conc: 0.14 ng/ml

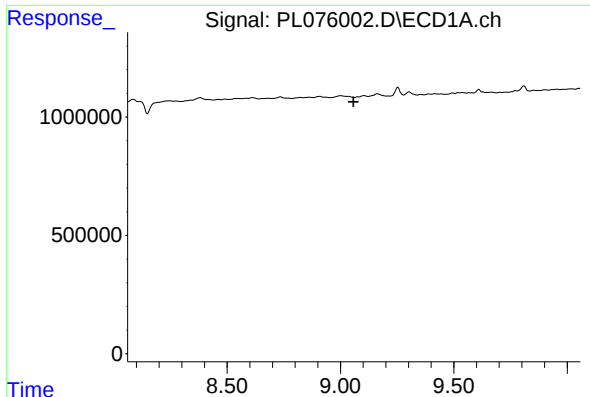

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

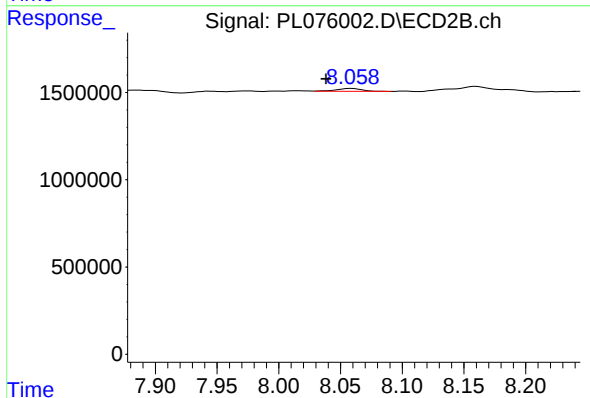


#14 Endrin

R.T.: 8.059 min
Delta R.T.: 0.021 min
Response: 235449
Conc: 0.15 ng/ml

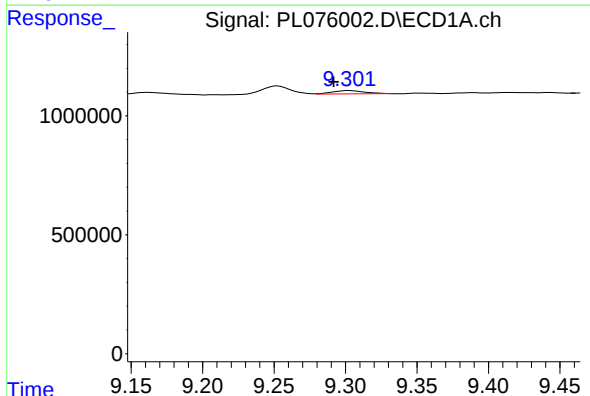


#15 Endosulfan II

R.T.: 9.302 min
Delta R.T.: 0.011 min
Response: 219995
Conc: 0.35 ng/ml

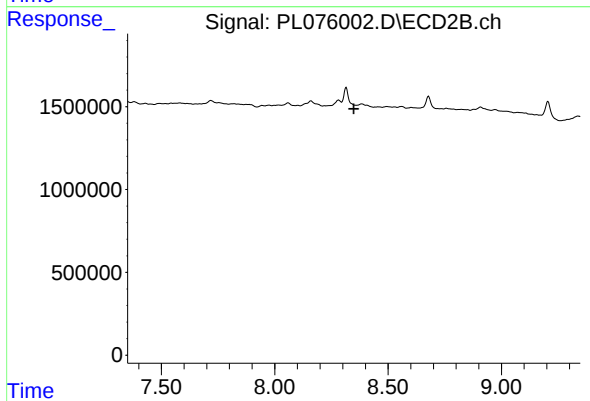

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.349 min
Response: 0
Conc: N.D.

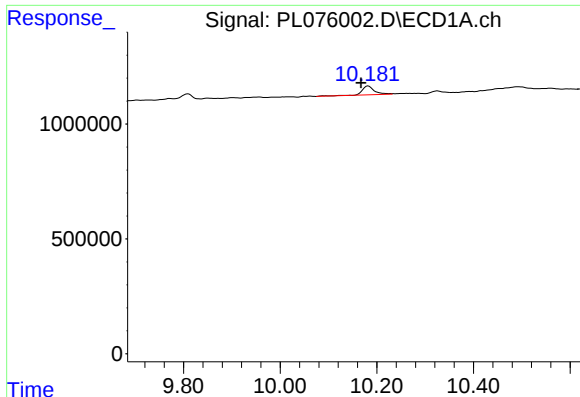

#21 Endrin ketone


R.T.: 10.182 min
Delta R.T.: 0.015 min
Response: 700264
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

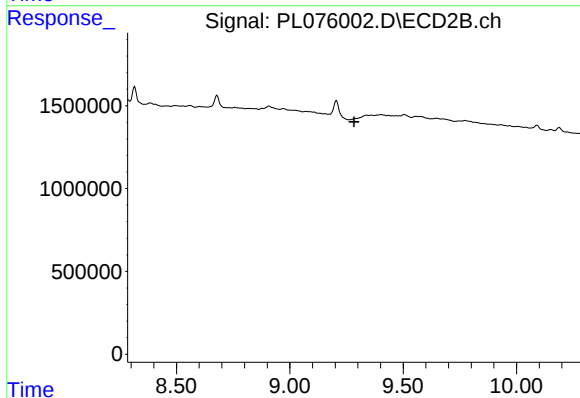


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

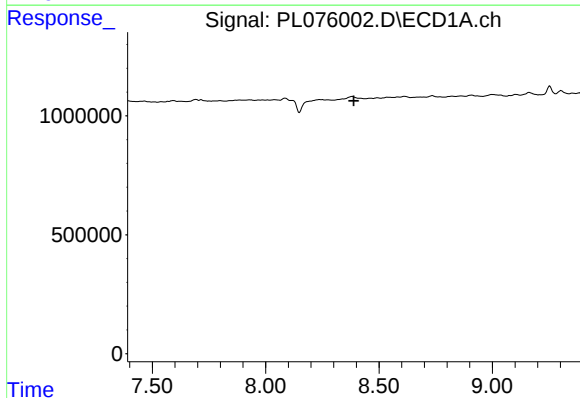


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.389 min
Response: 0
Conc: N.D.

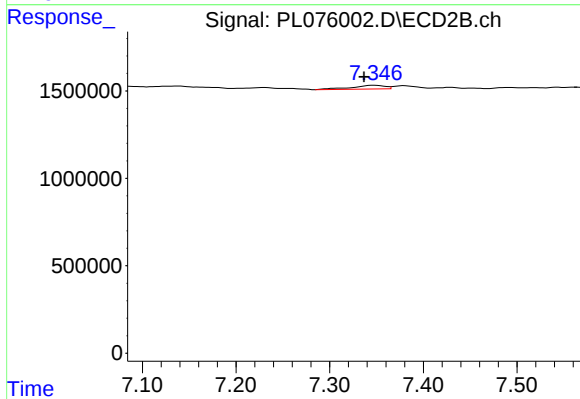

#25 Chlordane-3


R.T.: 7.348 min
Delta R.T.: 0.011 min
Response: 529698
Conc: 3.00 ng/ml

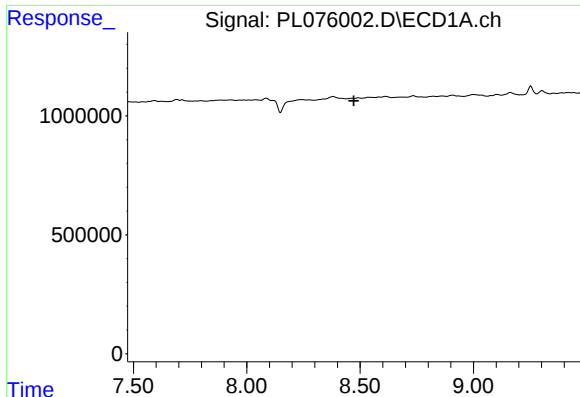

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

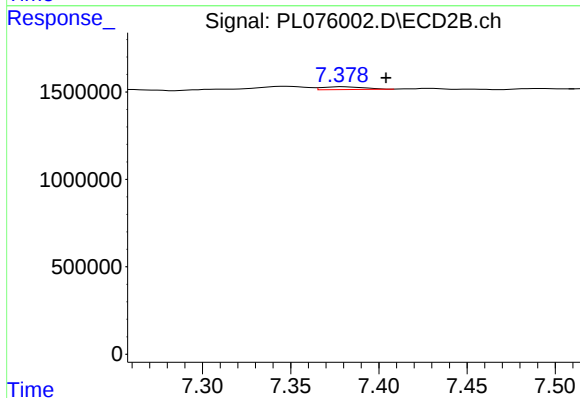


#26 Chlordane-4

R.T.: 7.380 min
Delta R.T.: -0.024 min
Response: 260111
Conc: 1.38 ng/ml

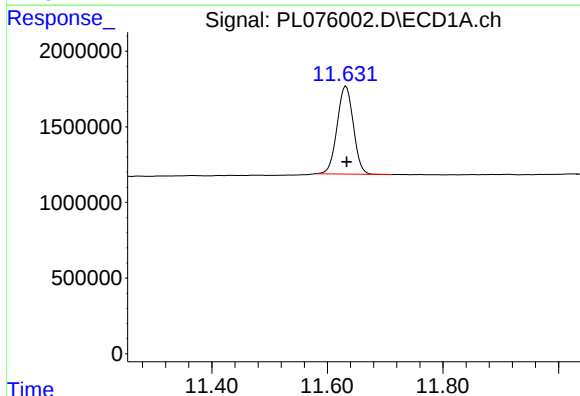

#28 Decachlorobiphenyl

R.T.: 11.632 min
Delta R.T.: -0.001 min
Response: 11302421
Conc: 17.96 ng/ml

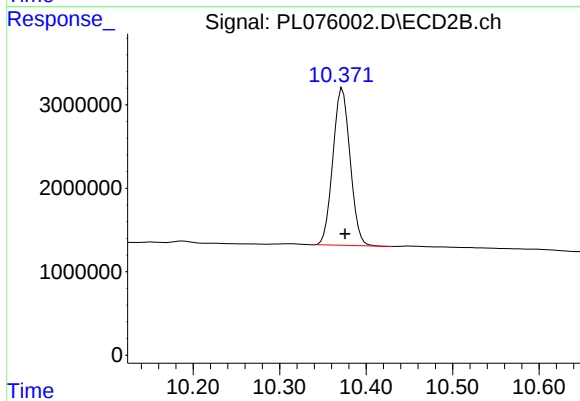

#28 Decachlorobiphenyl

R.T.: 10.373 min
Delta R.T.: -0.003 min
Response: 25852108
Conc: 16.83 ng/ml