

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062422\
 Data File : PL076022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2022 06:37
 Operator : AR\AJ
 Sample : N3455-10
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 02:29:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.633	13824545	33260332	18.279	17.537
28)	SA Decachlor...	11.632	10.373	9314275	21339796	14.802	13.894
Target Compounds							
2)	A alpha-BHC	6.195f	0.000	306703	0	0.311	N.D. #
5)	MB Aldrin	0.000	6.496	0	198074	N.D.	0.096 #
7)	B delta-BHC	7.122f	6.403	1380661	409093	1.768	0.181 #
10)	B gamma-Chl...	8.383	0.000	459326	0	0.591	N.D. #
13)	MA Dieldrin	0.000	7.722f	0	1047513	N.D.	0.582 #
14)	MA Endrin	0.000	8.059f	0	325085	N.D.	0.214 #
15)	B Endosulfa...	9.302	0.000	259380	0	0.409	N.D. #
16)	A 4,4'-DDD	9.197	8.195	221538	274552	0.391	0.198 #
17)	MA 4,4'-DDT	9.528	0.000	260460	0	0.427	N.D. #
21)	B Endrin ke...	10.183f	0.000	455878	0	0.632	N.D. #
25)	Chlordane-3	8.383	0.000	459326	0	4.517	N.D. #
27)	Chlordane-5	0.000	8.135f	0	363153	N.D.	7.937 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062422\
Data File : PL076022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2022 06:37
Operator : AR\AJ
Sample : N3455-10
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 02:29:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

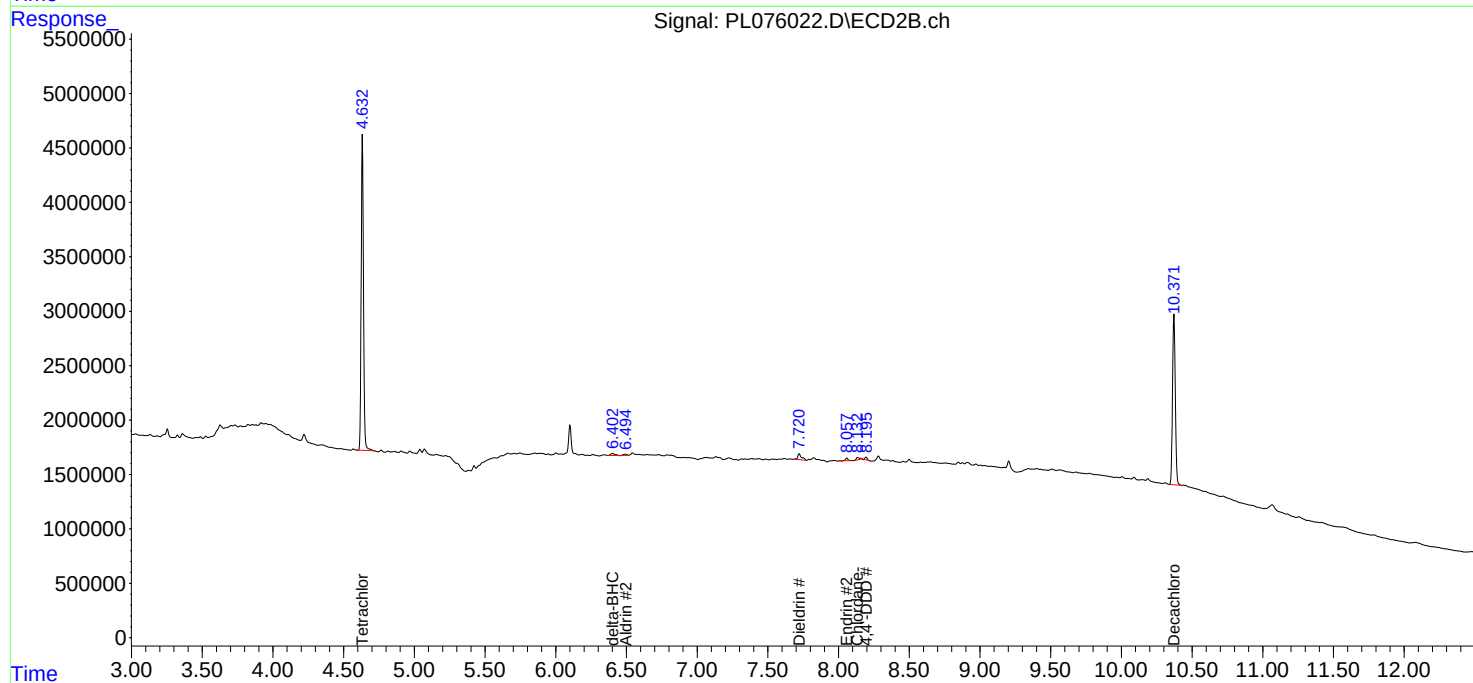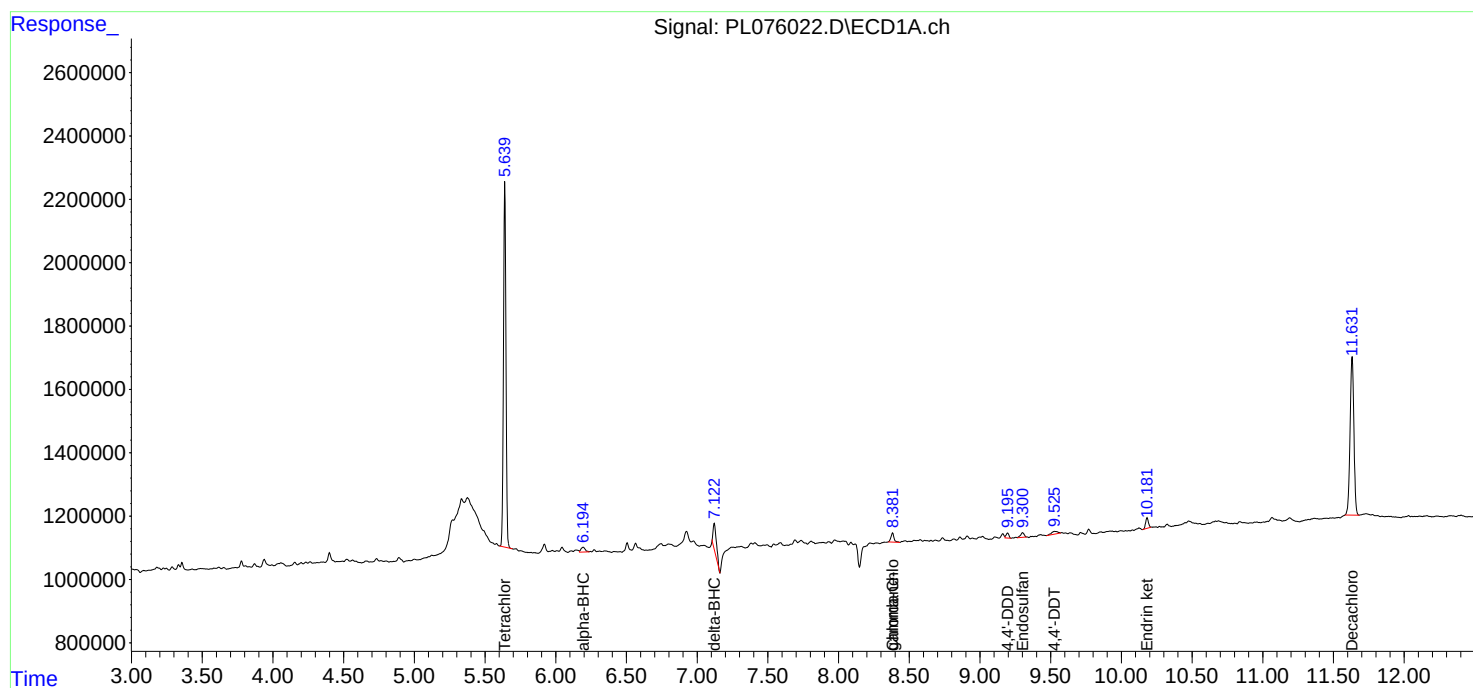


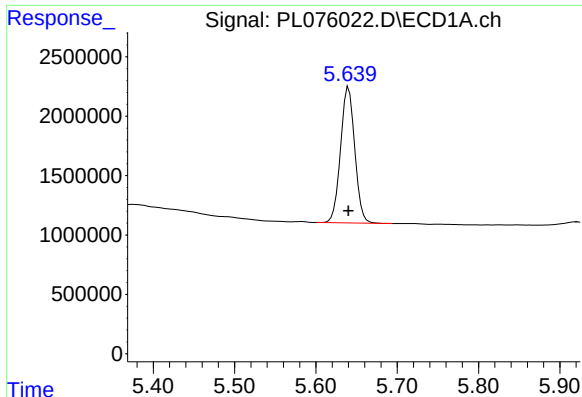

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 13824545
Conc: 18.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

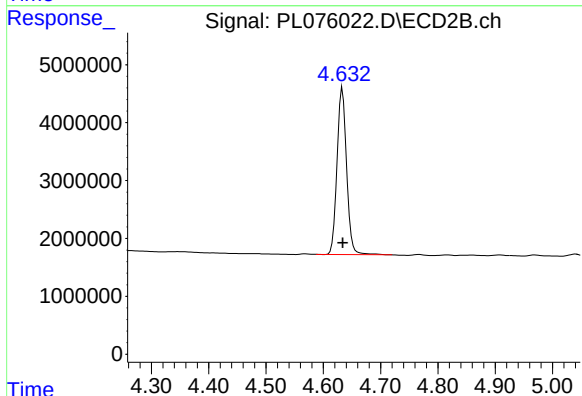


#1 Tetrachloro-m-xylene

R.T.: 4.633 min
Delta R.T.: 0.000 min
Response: 33260332
Conc: 17.54 ng/ml

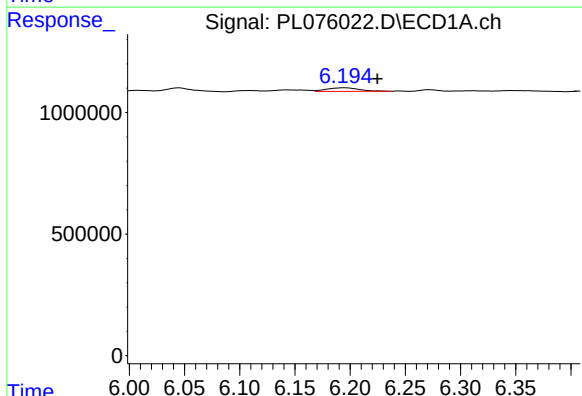


#2 alpha-BHC

R.T.: 6.195 min
Delta R.T.: -0.030 min
Response: 306703
Conc: 0.31 ng/ml

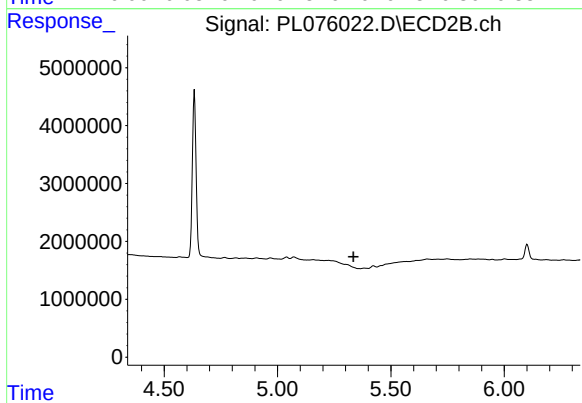

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

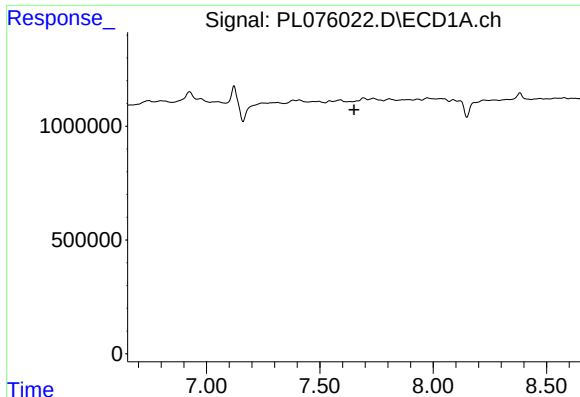

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 7.651 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

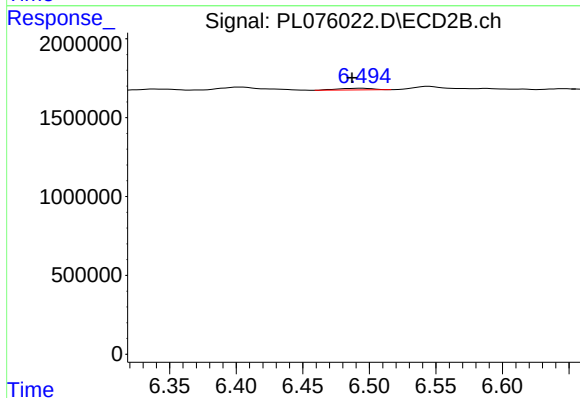


#5 Aldrin

R.T.: 6.496 min
Delta R.T.: 0.009 min
Response: 198074
Conc: 0.10 ng/ml

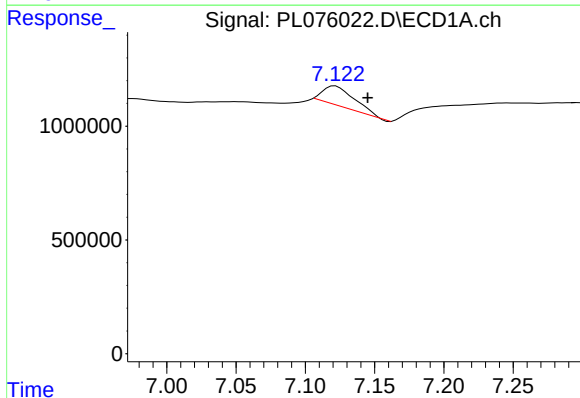


#7 delta-BHC

R.T.: 7.122 min
Delta R.T.: -0.023 min
Response: 1380661
Conc: 1.77 ng/ml

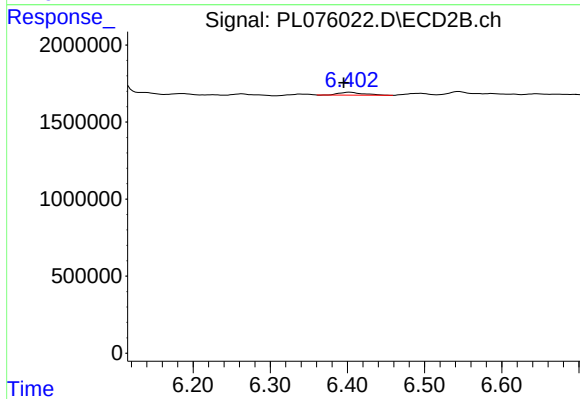

#7 delta-BHC


R.T.: 6.403 min
Delta R.T.: 0.008 min
Response: 409093
Conc: 0.18 ng/ml

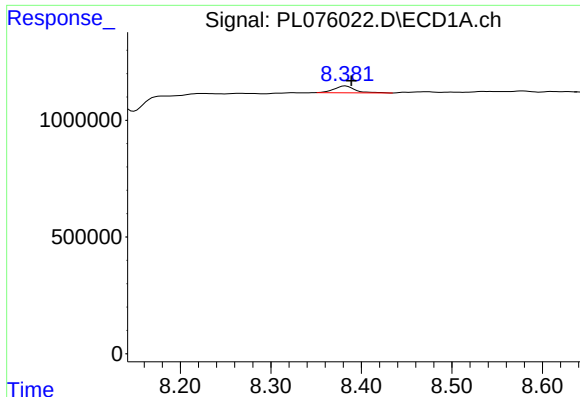

#10 gamma-Chlordane


R.T.: 8.383 min
Delta R.T.: -0.006 min
Response: 459326
Conc: 0.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

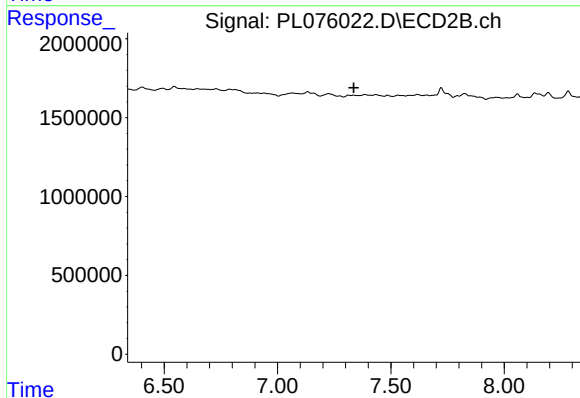


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.337 min
Response: 0
Conc: N.D.

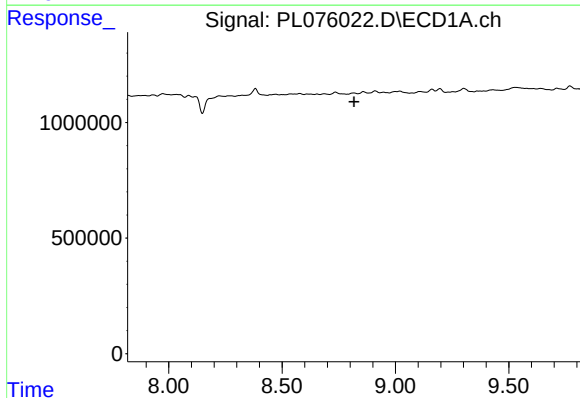


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.817 min
Response: 0
Conc: N.D.

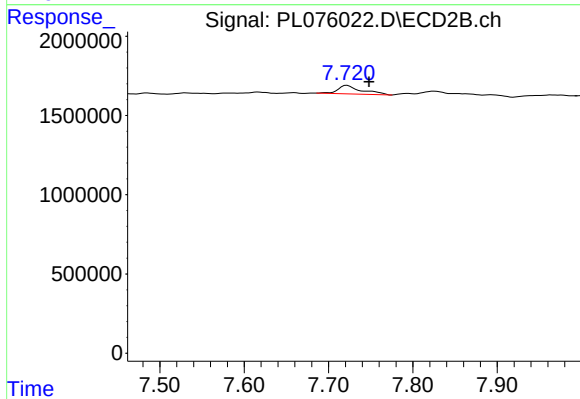

#13 Dieldrin


R.T.: 7.722 min
Delta R.T.: -0.026 min
Response: 1047513
Conc: 0.58 ng/ml

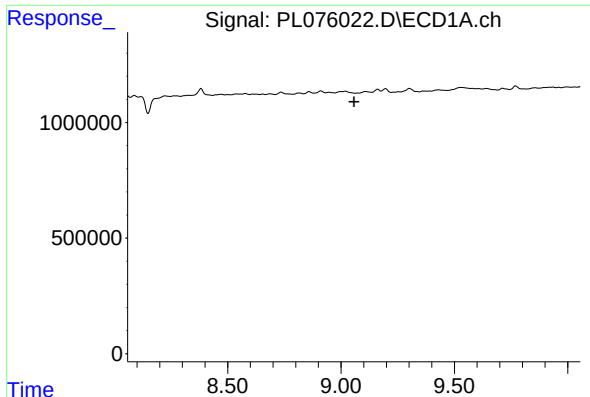

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

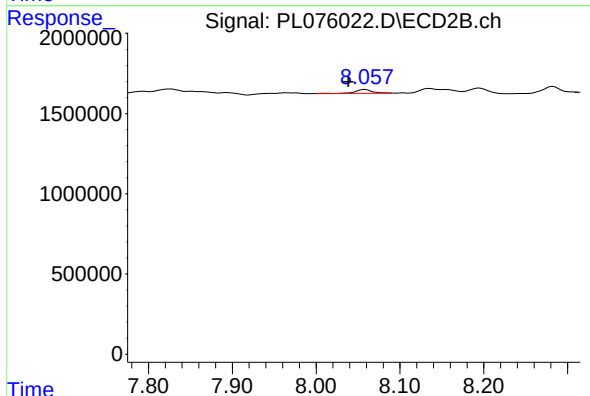


#14 Endrin

R.T.: 8.059 min
Delta R.T.: 0.020 min
Response: 325085
Conc: 0.21 ng/ml

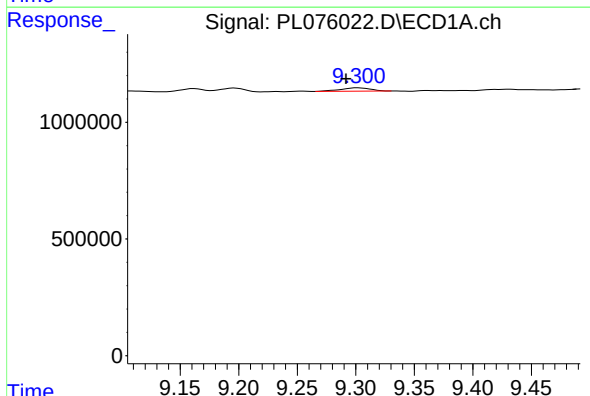


#15 Endosulfan II

R.T.: 9.302 min
Delta R.T.: 0.010 min
Response: 259380
Conc: 0.41 ng/ml

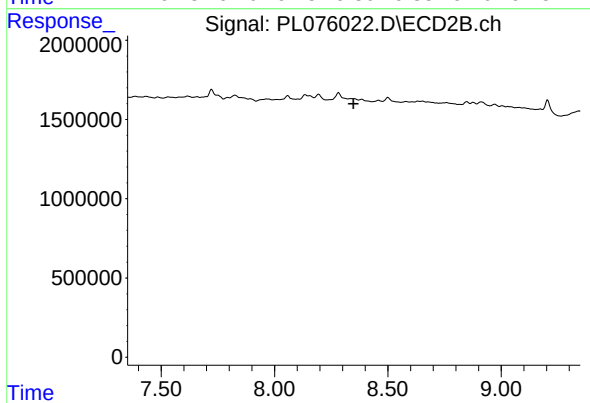

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.349 min
Response: 0
Conc: N.D.

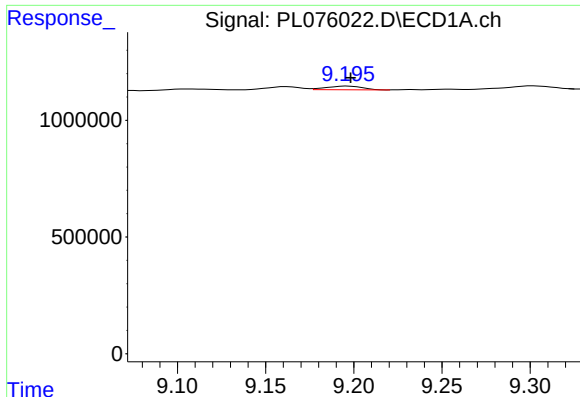

#16 4,4'-DDD


R.T.: 9.197 min
Delta R.T.: -0.002 min
Response: 221538
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

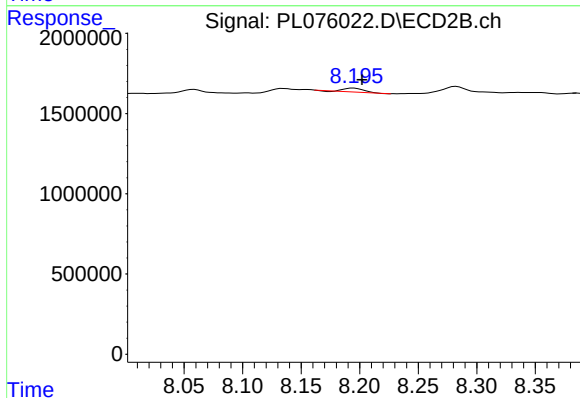


#16 4,4'-DDD

R.T.: 8.195 min
Delta R.T.: -0.007 min
Response: 274552
Conc: 0.20 ng/ml

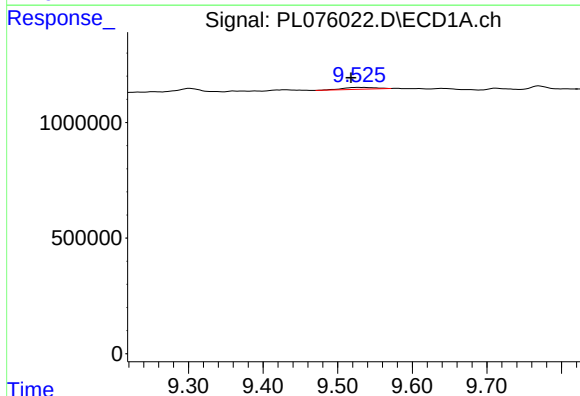


#17 4,4'-DDT

R.T.: 9.528 min
Delta R.T.: 0.010 min
Response: 260460
Conc: 0.43 ng/ml

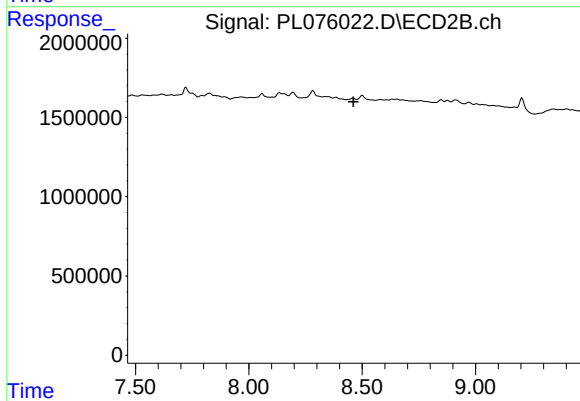

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.462 min
Response: 0
Conc: N.D.

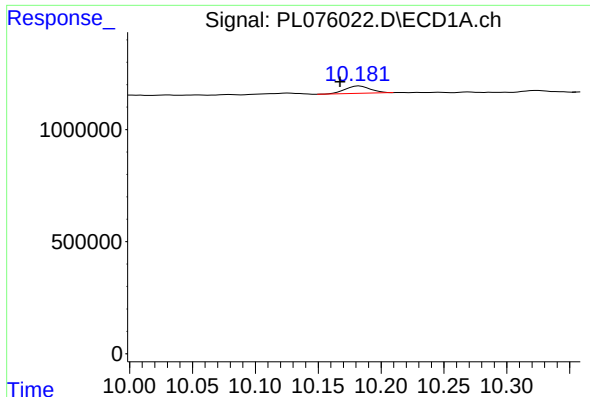

#21 Endrin ketone


R.T.: 10.183 min
Delta R.T.: 0.015 min
Response: 455878
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

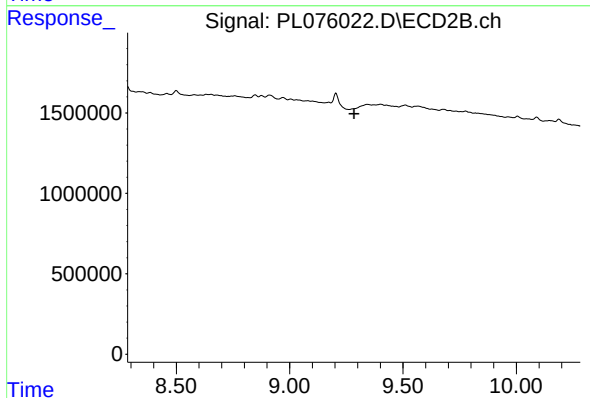


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

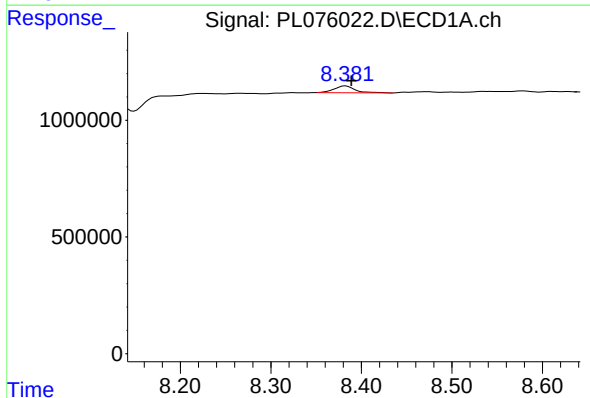


#25 Chlordane-3

R.T.: 8.383 min
Delta R.T.: -0.006 min
Response: 459326
Conc: 4.52 ng/ml

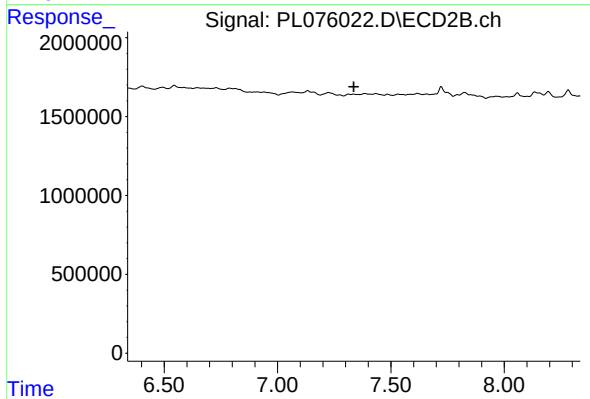

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.337 min
Response: 0
Conc: N.D.

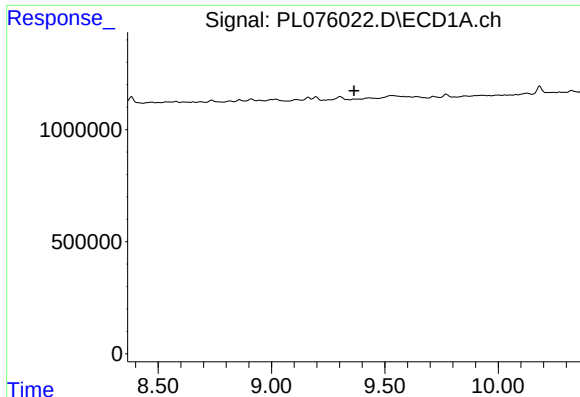

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.365 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

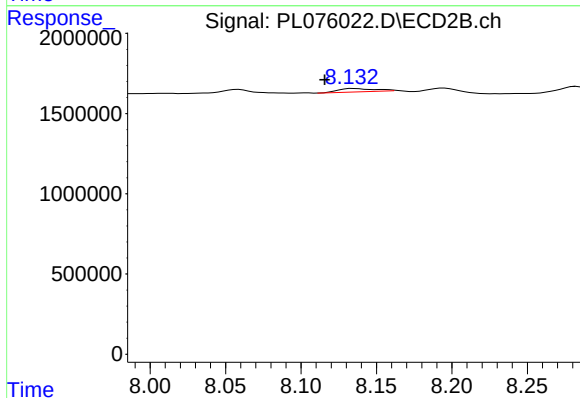


#27 Chlordane-5

R.T.: 8.135 min
Delta R.T.: 0.019 min
Response: 363153
Conc: 7.94 ng/ml

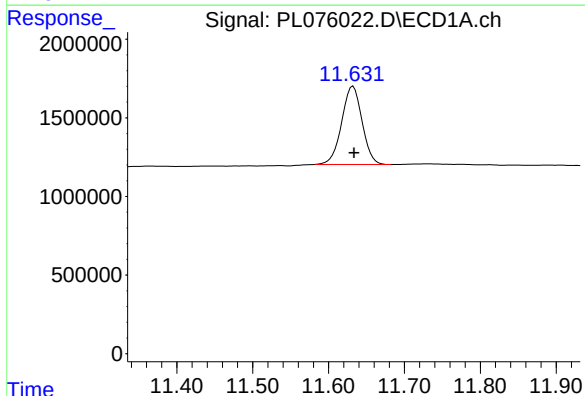

#28 Decachlorobiphenyl

R.T.: 11.632 min
Delta R.T.: -0.001 min
Response: 9314275
Conc: 14.80 ng/ml

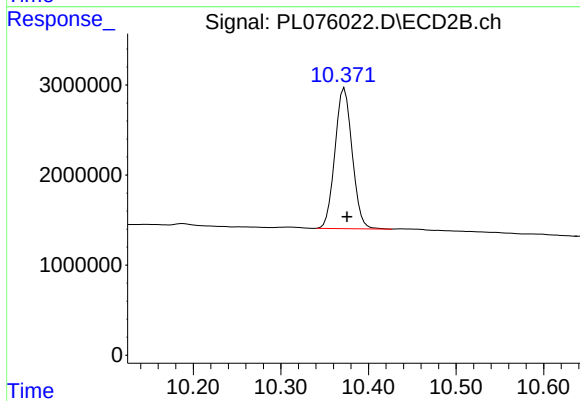

#28 Decachlorobiphenyl

R.T.: 10.373 min
Delta R.T.: -0.003 min
Response: 21339796
Conc: 13.89 ng/ml