

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062422\
 Data File : PL076028.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2022 08:16
 Operator : AR\AJ
 Sample : N3454-08 10X
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 02:31:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.639	4.633	453029	1461446	0.599	0.771 #
28)	SA Decachlor...	11.633	10.374	1102971	1642296	1.753	1.069 #
Target Compounds							
4)	MA Heptachlor	7.255f	0.000	172208	0	0.188	N.D. #
7)	B delta-BHC	7.120f	6.400	276720	171950	0.354	0.076 #
9)	A Endosulfan I	0.000	7.484f	0	244163	N.D.	0.139 #
10)	B gamma-Chl...	8.381	0.000	385094	0	0.495	N.D. #
13)	MA Dieldrin	0.000	7.721f	0	191713	N.D.	0.107 #
15)	B Endosulfa...	9.303	0.000	227326	0	0.358	N.D. #
16)	A 4,4'-DDD	9.195	0.000	257500	0	0.454	N.D. #
20)	A Methoxychlor	0.000	9.079f	0	1054743	N.D.	1.239 #
21)	B Endrin ke...	10.182	0.000	376226	0	0.522	N.D. #
23)	Chlordane-1	0.000	5.973f	0	468803	N.D.	8.373 #
24)	Chlordane-2	7.601f	0.000	277961	0	9.163	N.D. #
25)	Chlordane-3	8.381	0.000	385094	0	3.787	N.D. #
27)	Chlordane-5	0.000	8.135f	0	24831	N.D.	0.543 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062422\
Data File : PL076028.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2022 08:16
Operator : AR\AJ
Sample : N3454-08 10X
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 02:31:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

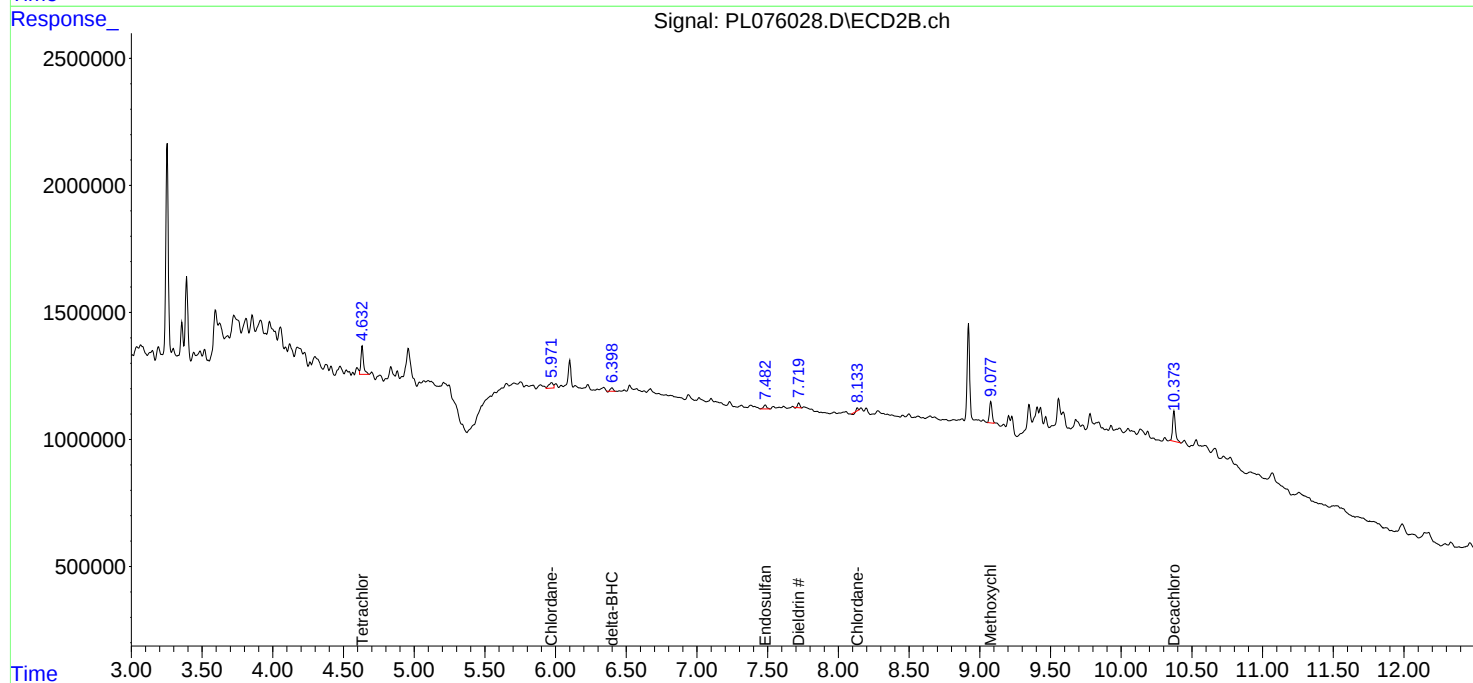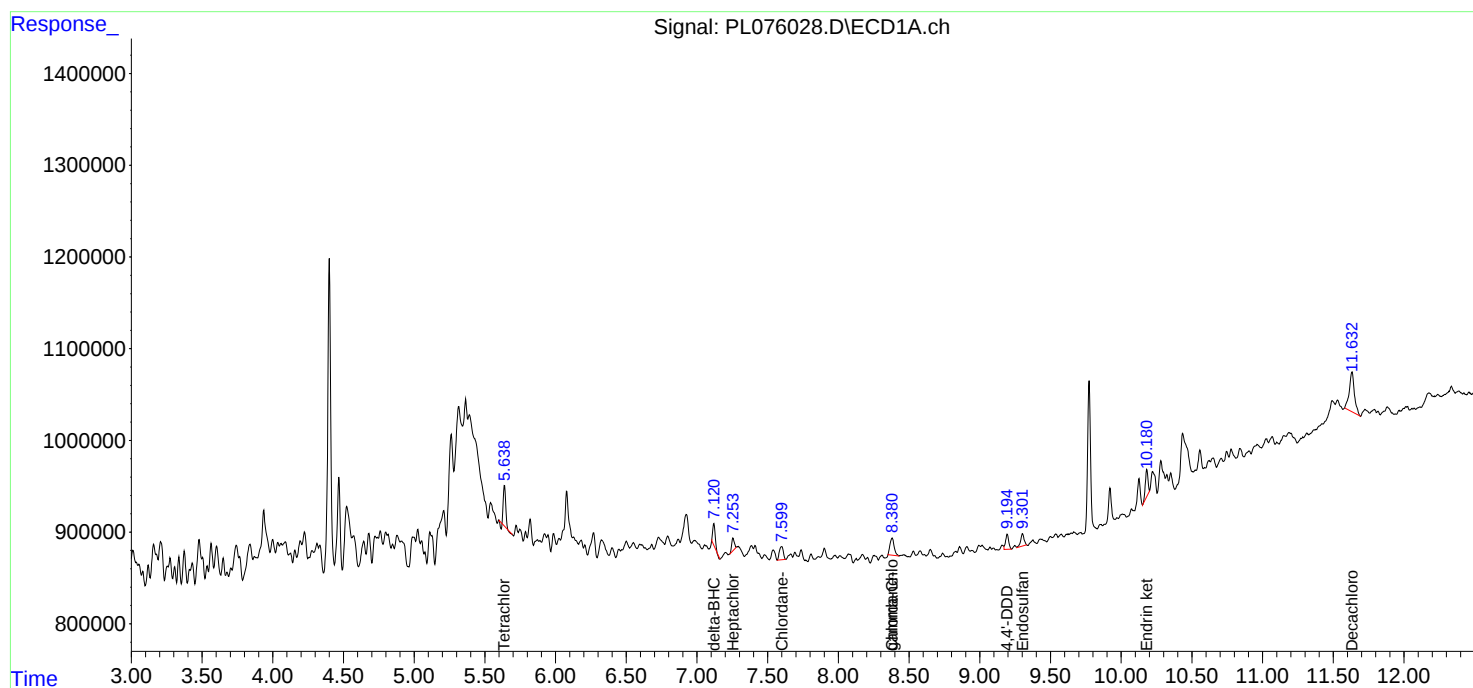


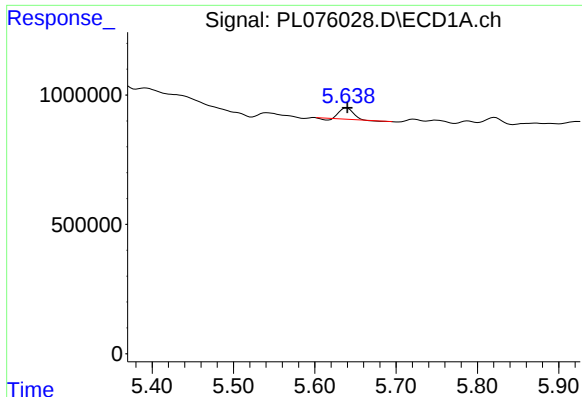

#1 Tetrachloro-m-xylene


R.T.: 5.639 min
Delta R.T.: 0.000 min
Response: 453029
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

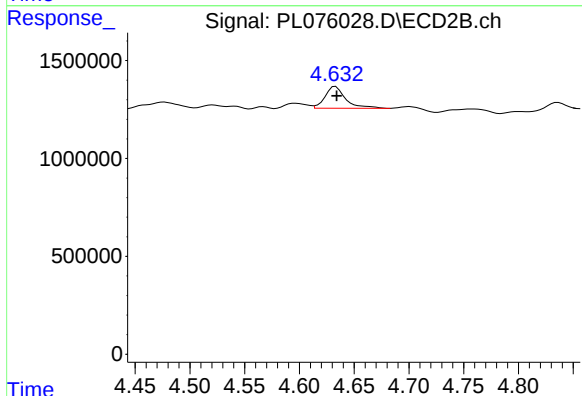


#1 Tetrachloro-m-xylene

R.T.: 4.633 min
Delta R.T.: 0.000 min
Response: 1461446
Conc: 0.77 ng/ml

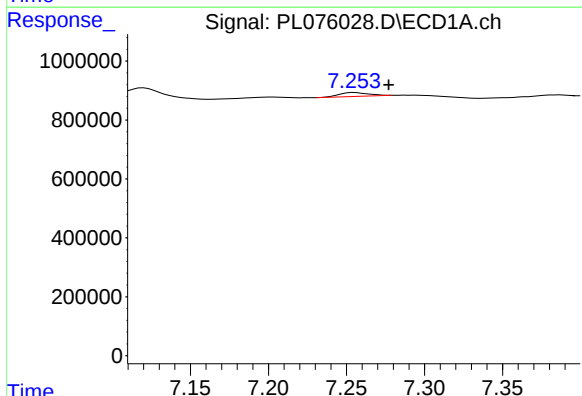


#4 Heptachlor

R.T.: 7.255 min
Delta R.T.: -0.022 min
Response: 172208
Conc: 0.19 ng/ml

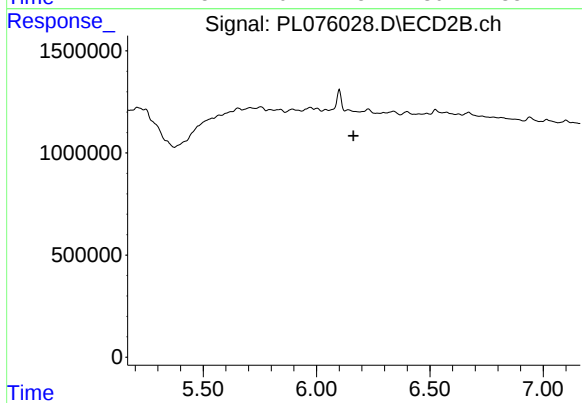

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 6.163 min
Response: 0
Conc: N.D.

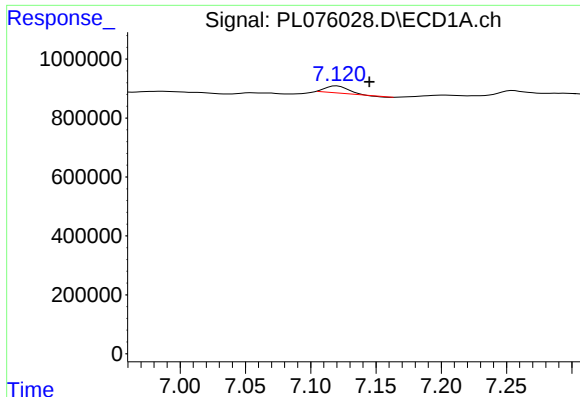

#7 delta-BHC


R.T.: 7.120 min
Delta R.T.: -0.025 min
Response: 276720
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

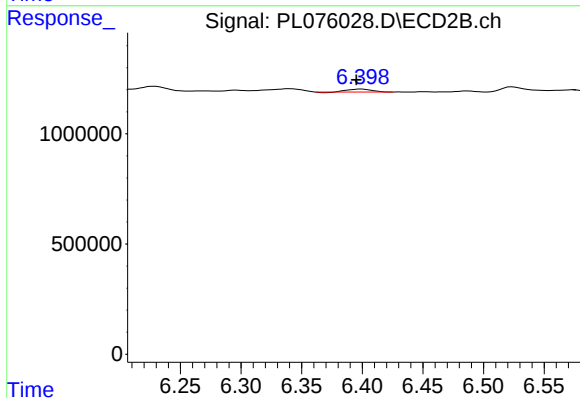


#7 delta-BHC

R.T.: 6.400 min
Delta R.T.: 0.005 min
Response: 171950
Conc: 0.08 ng/ml

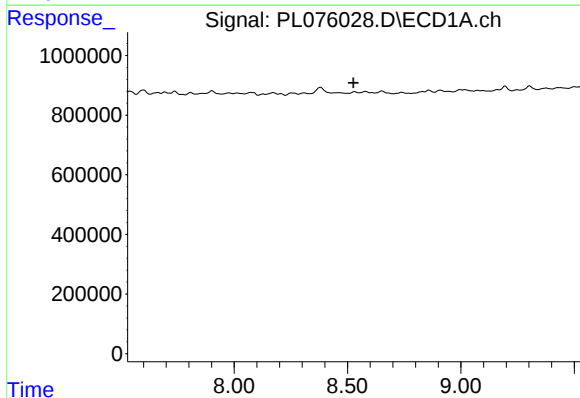


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.527 min
Response: 0
Conc: N.D.

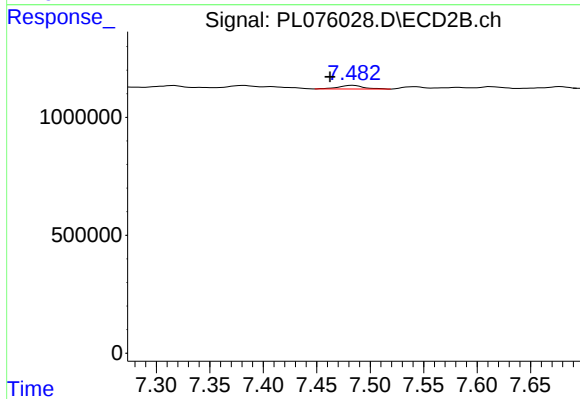

#9 Endosulfan I


R.T.: 7.484 min
Delta R.T.: 0.021 min
Response: 244163
Conc: 0.14 ng/ml

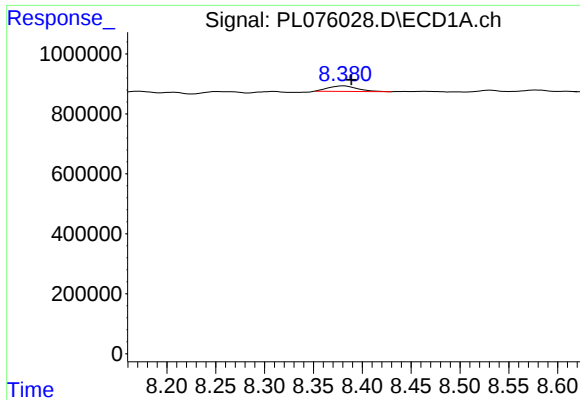

#10 gamma-Chlordane


R.T.: 8.381 min
Delta R.T.: -0.008 min
Response: 385094
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

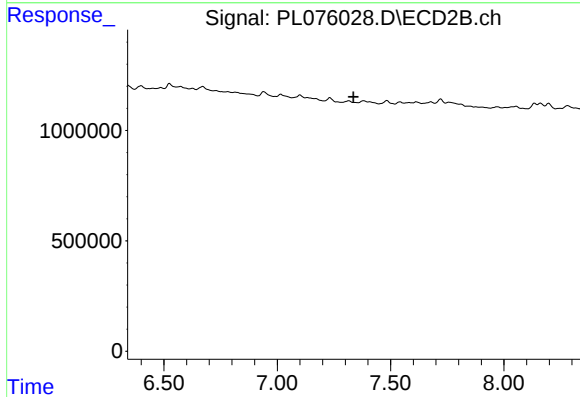


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.337 min
Response: 0
Conc: N.D.

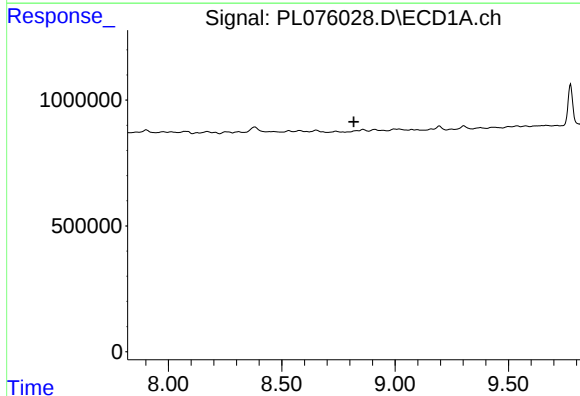


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.817 min
Response: 0
Conc: N.D.

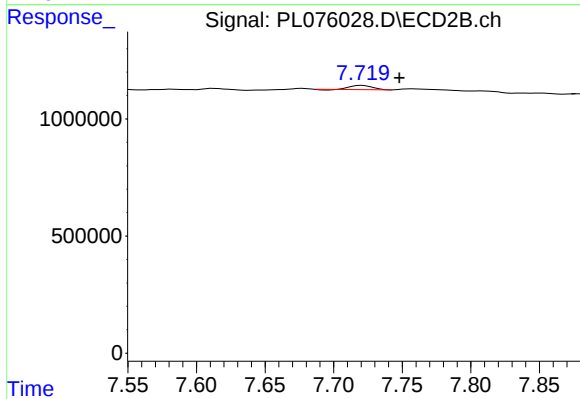

#13 Dieldrin


R.T.: 7.721 min
Delta R.T.: -0.027 min
Response: 191713
Conc: 0.11 ng/ml

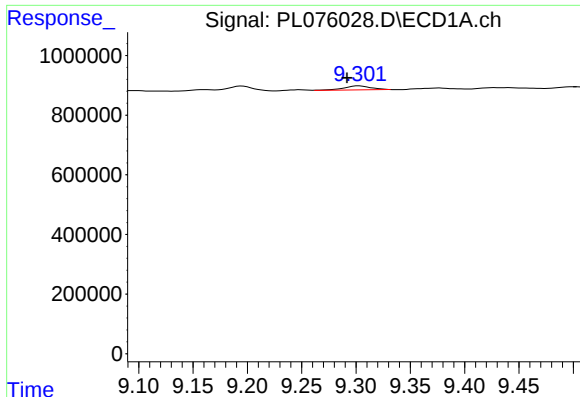

#15 Endosulfan II


R.T.: 9.303 min
Delta R.T.: 0.011 min
Response: 227326
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

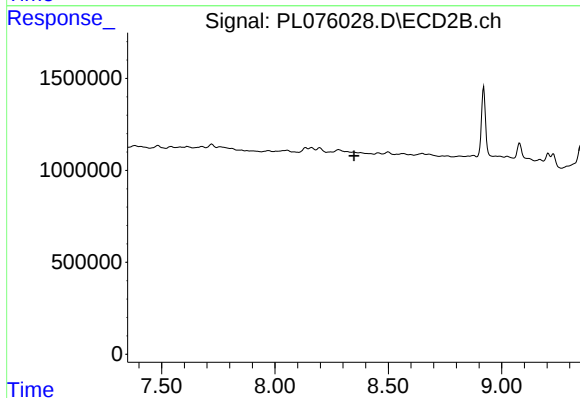


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

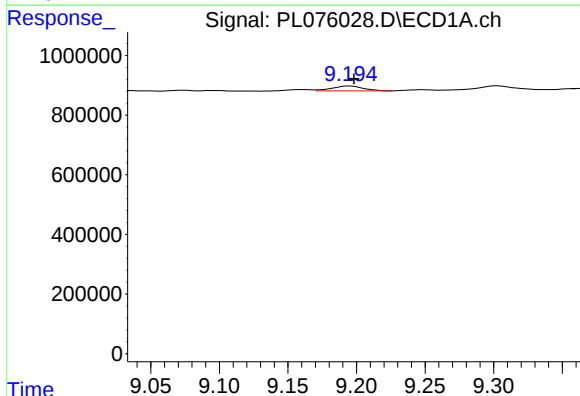


#16 4,4'-DDD

R.T.: 9.195 min
Delta R.T.: -0.003 min
Response: 257500
Conc: 0.45 ng/ml

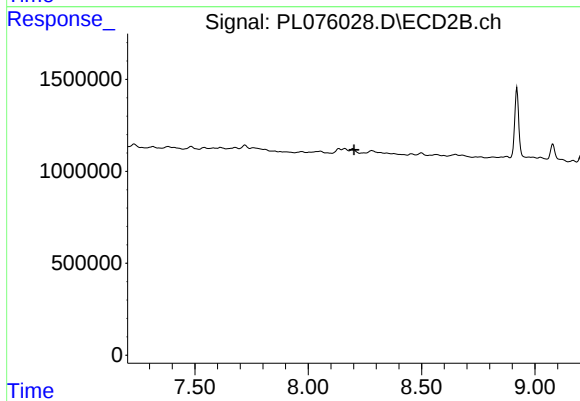

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 8.202 min
Response: 0
Conc: N.D.

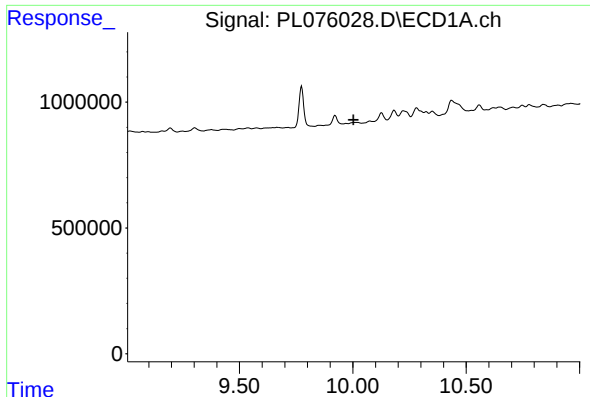

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 10.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

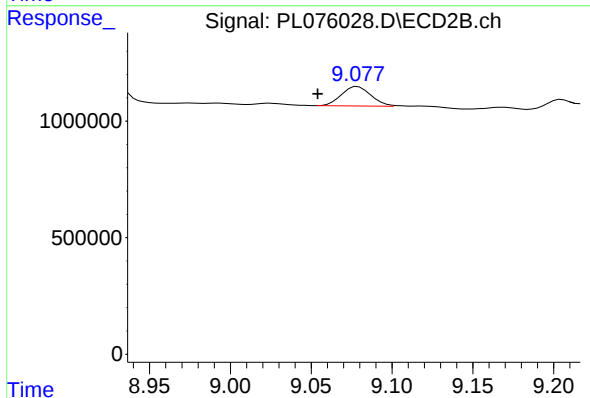


#20 Methoxychlor

R.T.: 9.079 min
Delta R.T.: 0.025 min
Response: 1054743
Conc: 1.24 ng/ml

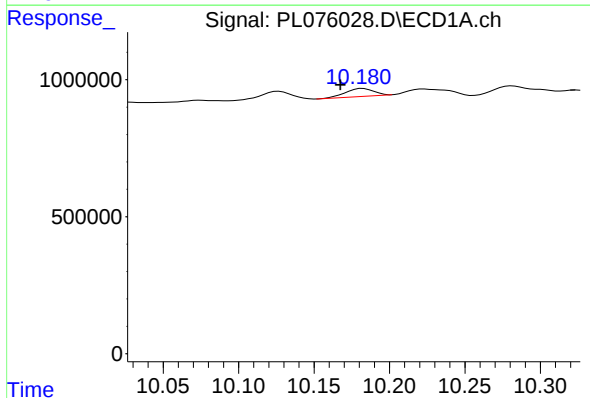


#21 Endrin ketone

R.T.: 10.182 min
Delta R.T.: 0.015 min
Response: 376226
Conc: 0.52 ng/ml

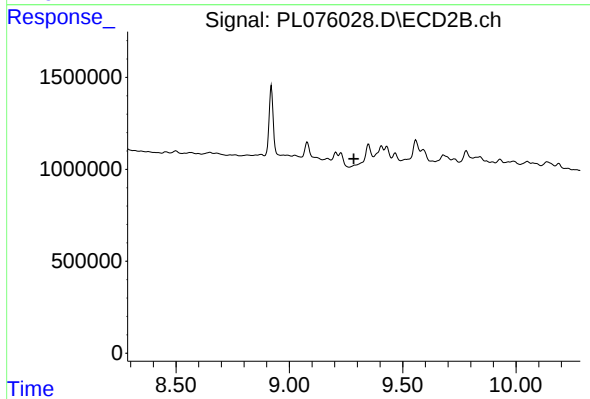

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.284 min
Response: 0
Conc: N.D.

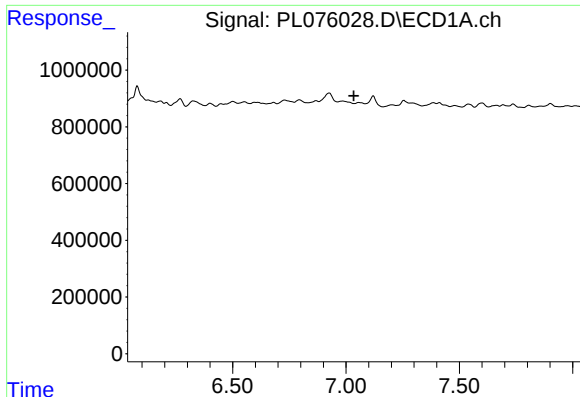

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 7.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

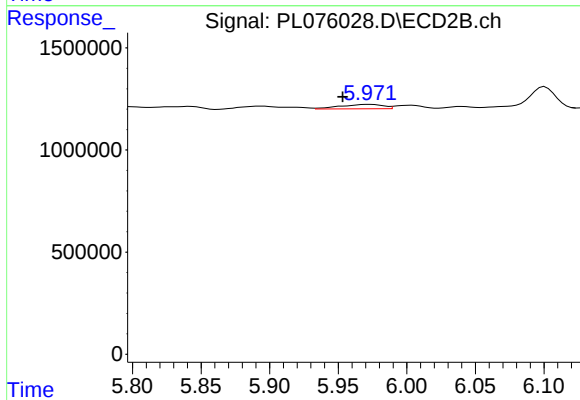


#23 Chlordane-1

R.T.: 5.973 min
Delta R.T.: 0.019 min
Response: 468803
Conc: 8.37 ng/ml

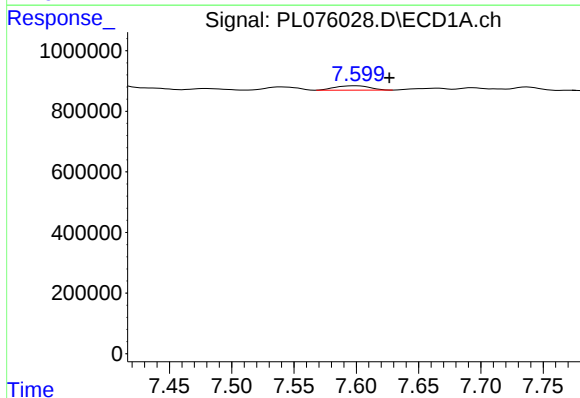


#24 Chlordane-2

R.T.: 7.601 min
Delta R.T.: -0.026 min
Response: 277961
Conc: 9.16 ng/ml

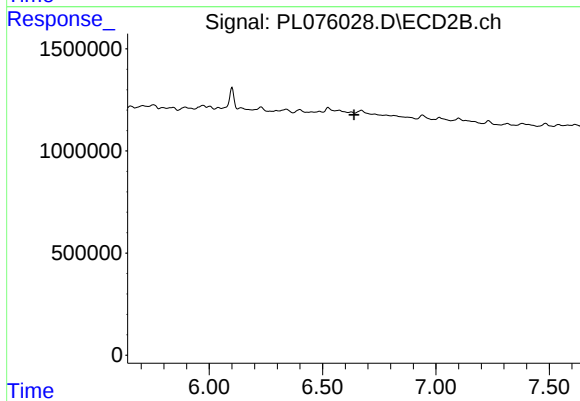

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.639 min
Response: 0
Conc: N.D.

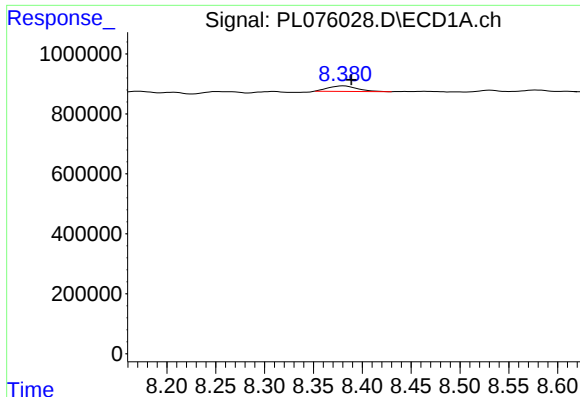

#25 Chlordane-3


R.T.: 8.381 min
Delta R.T.: -0.008 min
Response: 385094
Conc: 3.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

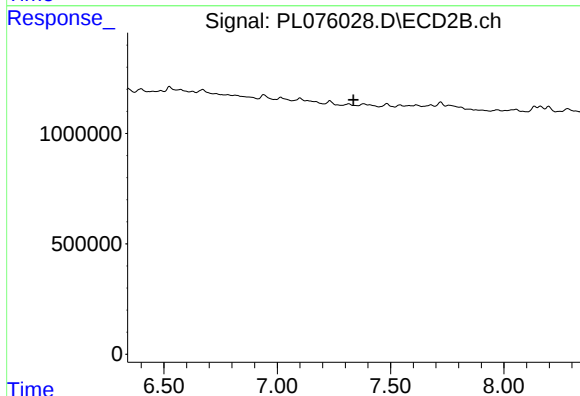


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.337 min
Response: 0
Conc: N.D.

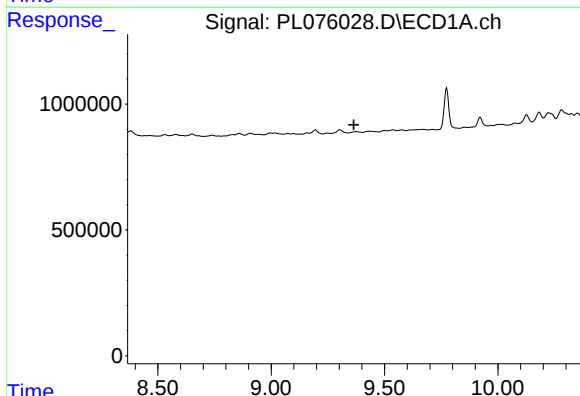


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.365 min
Response: 0
Conc: N.D.

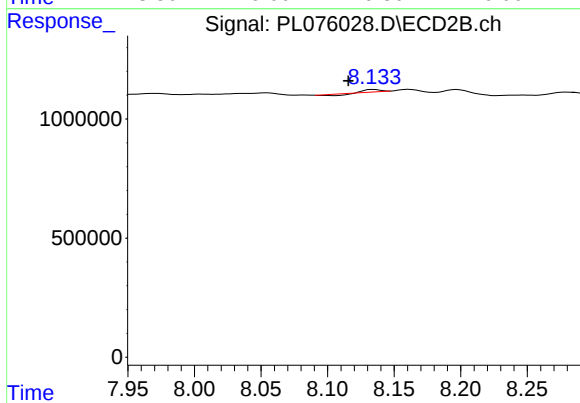

#27 Chlordane-5


R.T.: 8.135 min
Delta R.T.: 0.019 min
Response: 24831
Conc: 0.54 ng/ml

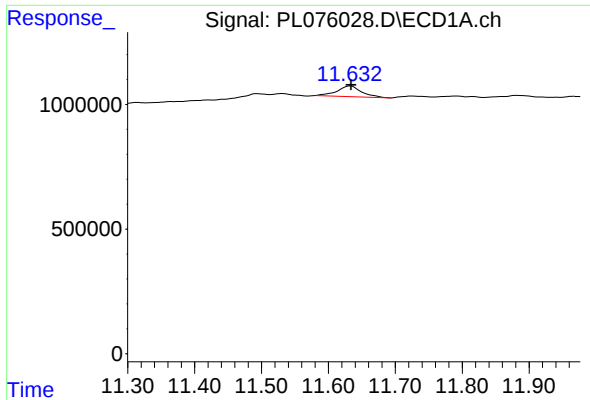

#28 Decachlorobiphenyl

R.T.: 11.633 min
Delta R.T.: 0.000 min
Response: 1102971
Conc: 1.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

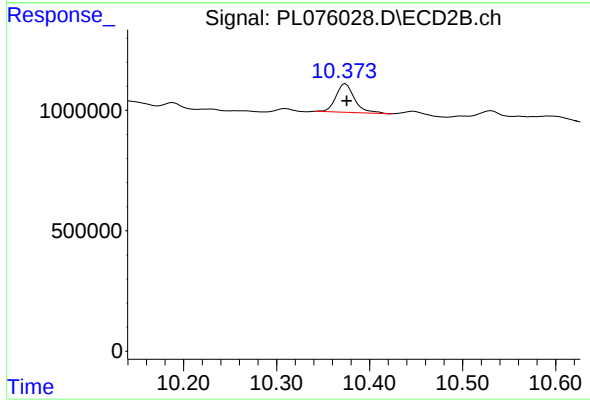

#28 Decachlorobiphenyl

R.T.: 10.374 min
Delta R.T.: -0.001 min
Response: 1642296
Conc: 1.07 ng/ml