

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062422\
 Data File : PL076023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2022 06:54
 Operator : AR\AJ
 Sample : N3455-16
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-EXC-2-3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/27/2022
 Supervised By : Ankita Jodhani 06/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 02:30:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.633	13155368	31469336	17.394	16.592
28)	SA Decachlor...	11.633	10.373	9339523	21389743	14.842	13.927
Target Compounds							
16)	A 4,4'-DDD	9.198	8.197	375812	763603	0.663	0.551m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062422\
Data File : PL076023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2022 06:54
Operator : AR\AJ
Sample : N3455-16
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SP-EXC-2-3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/27/2022
Supervised By : Ankita Jodhani 06/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 02:30:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

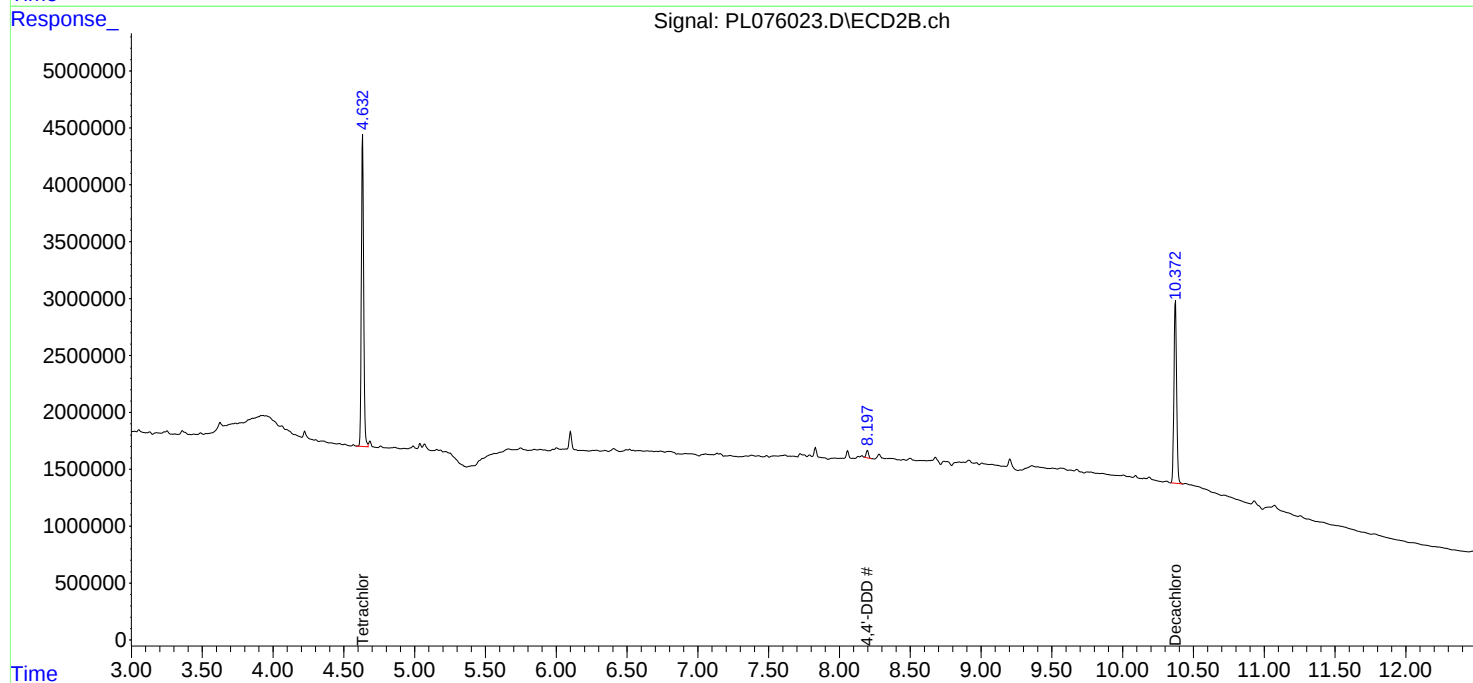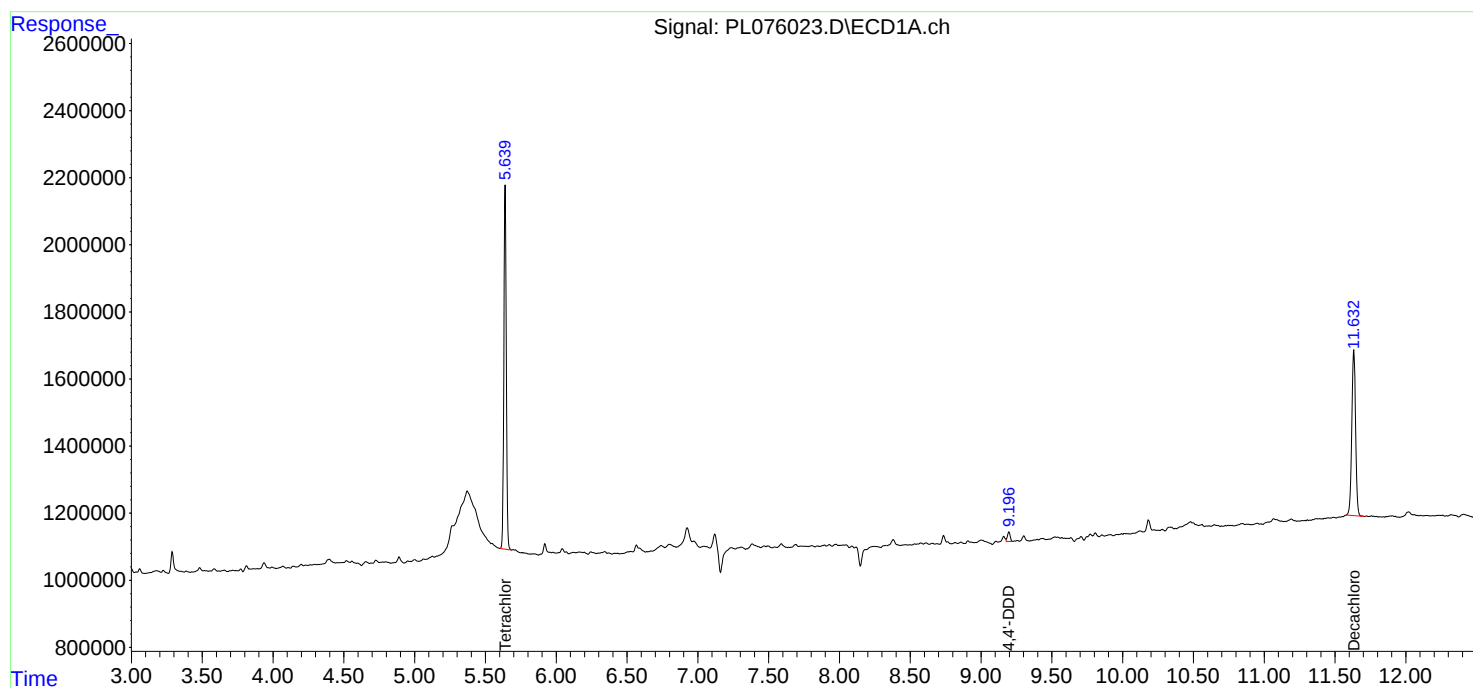

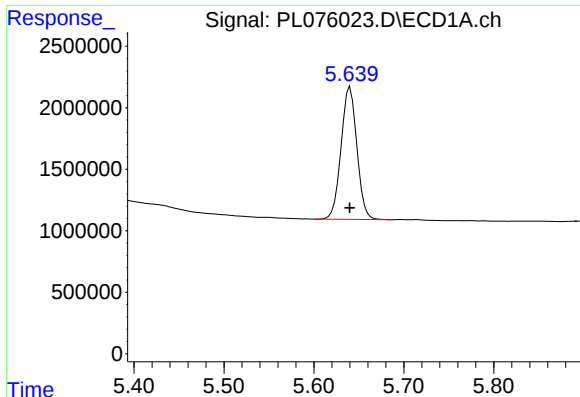


#1 Tetrachloro-m-xylene

R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 13155368
Conc: 17.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-EXC-2-3


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/27/2022
Supervised By :Ankita Jodhani 06/27/2022

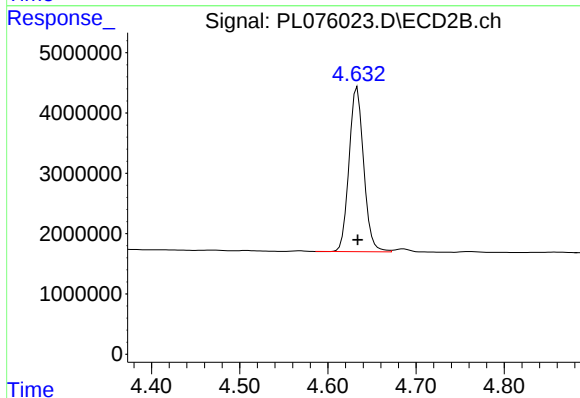


#1 Tetrachloro-m-xylene

R.T.: 4.633 min
Delta R.T.: 0.000 min
Response: 31469336
Conc: 16.59 ng/ml

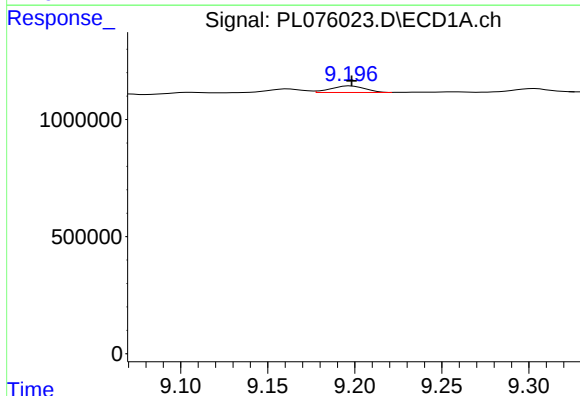


#16 4,4'-DDD

R.T.: 9.198 min
Delta R.T.: 0.000 min
Response: 375812
Conc: 0.66 ng/ml

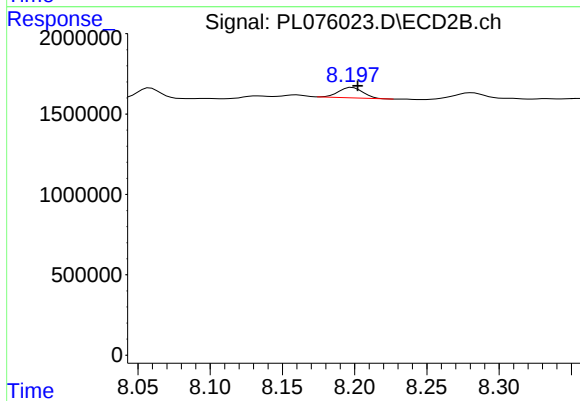

#16 4,4'-DDD

R.T.: 8.197 min
Delta R.T.: -0.005 min
Response: 763603
Conc: 0.55 ng/ml m

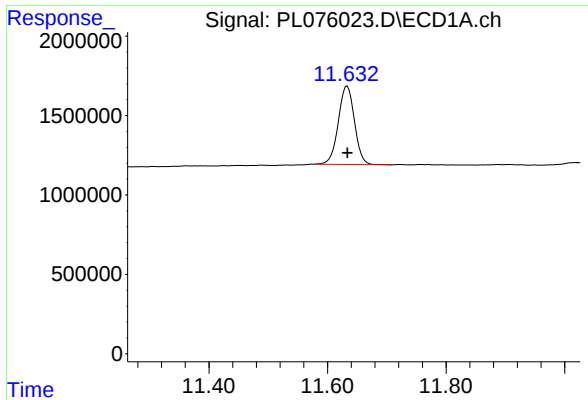


#28 Decachlorobiphenyl

R.T.: 11.633 min
Delta R.T.: 0.000 min
Response: 9339523
Conc: 14.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-EXC-2-3

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/27/2022
Supervised By :Ankita Jodhani 06/27/2022

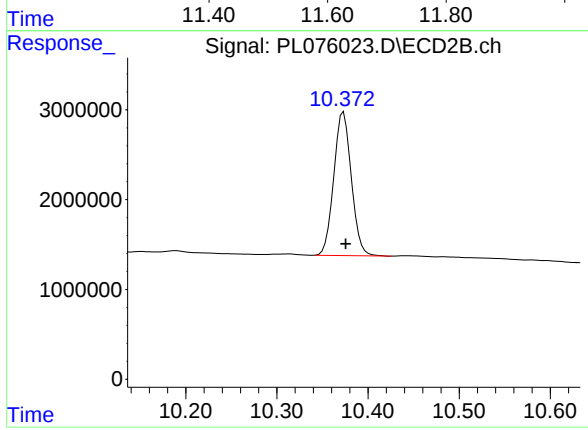

#28 Decachlorobiphenyl

R.T.: 10.373 min
Delta R.T.: -0.002 min
Response: 21389743
Conc: 13.93 ng/ml