

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062424\
 Data File : PL090305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2024 15:05
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:59:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062424.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 25 01:45:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.789	47947668	32407732	21.126	20.488
28)	SA Decachlor...	9.061	7.937	32282562	30626596	20.933	20.531
Target Compounds							
9)	A Endosulfan I	6.077	5.119	24876975	16038422	10.564	9.269
10)	B gamma-Chl...	5.947	4.999	28842704	18867818	11.415	9.845
12)	B 4,4'-DDE	6.199	5.252	46126102	32769969	21.130	19.782
13)	MA Dieldrin	6.352	5.384	51180482	35979443	20.934	19.507
19)	B Endosulfa...	7.164	6.355	42098374	31595910	21.254	20.205
20)	A Methoxychlor	7.505	6.633	94569310	80794597	91.767	96.845
21)	B Endrin ke...	7.649	6.861	45477342	35384609	20.966	19.762



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062424\
Data File : PL090305.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2024 15:05
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:59:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062424.M
Quant Title : GC Extractables
QLast Update : Tue Jun 25 01:45:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

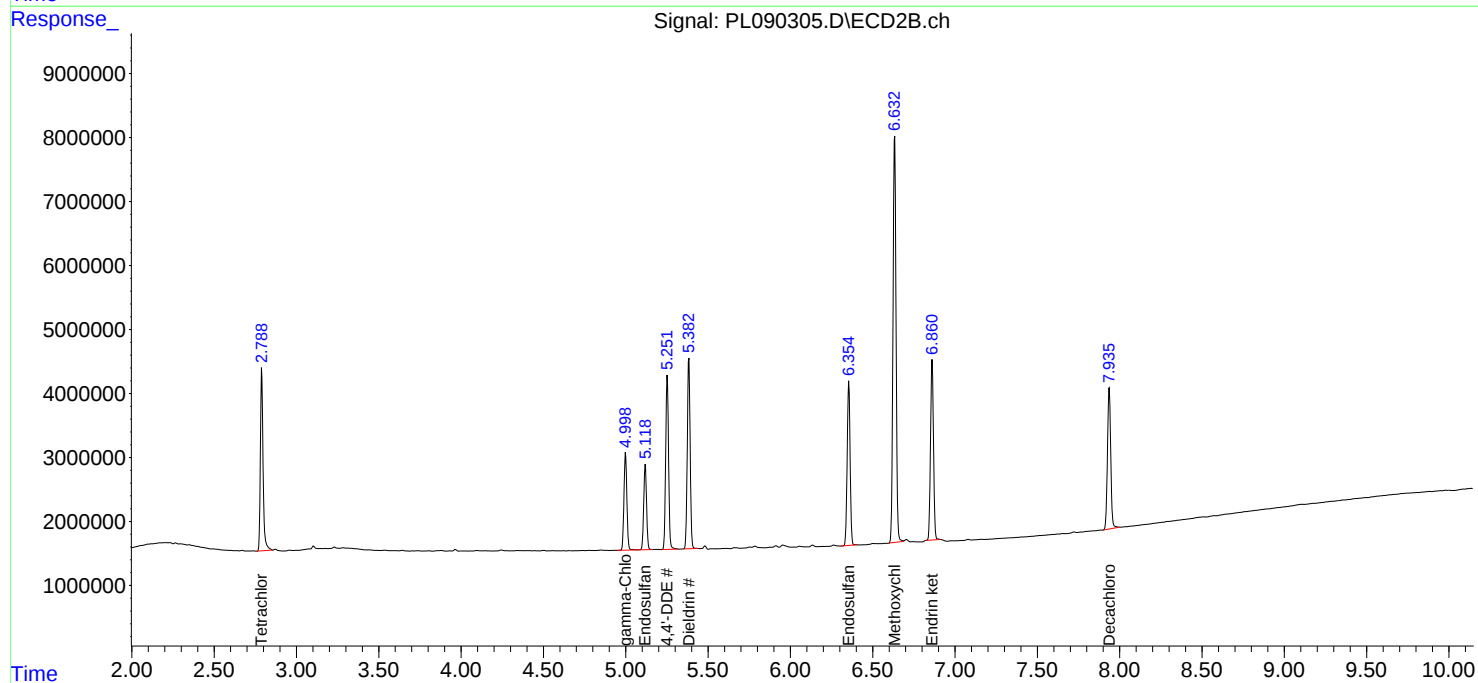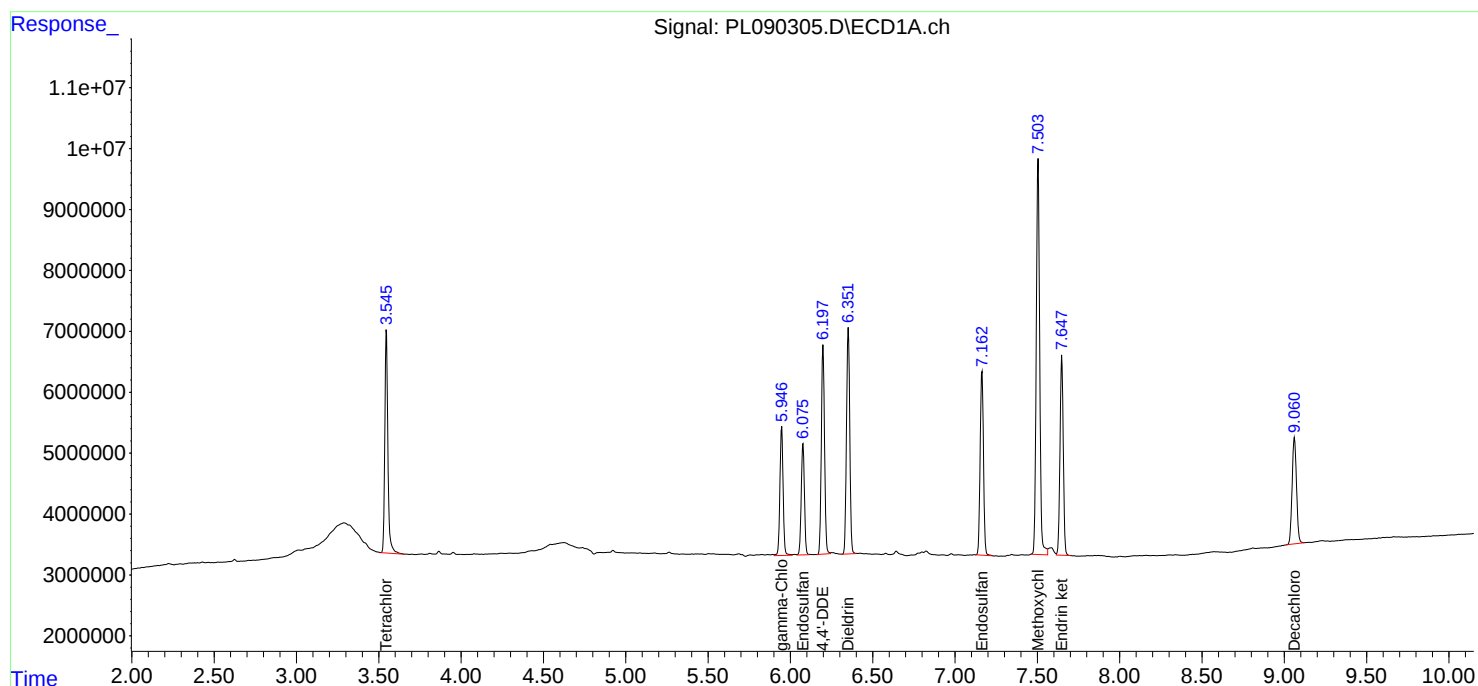


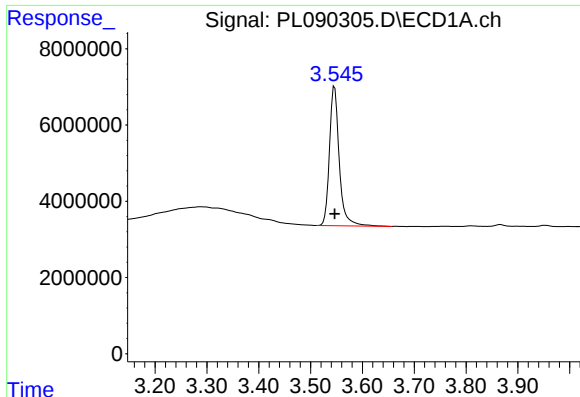

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 47947668
Conc: 21.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

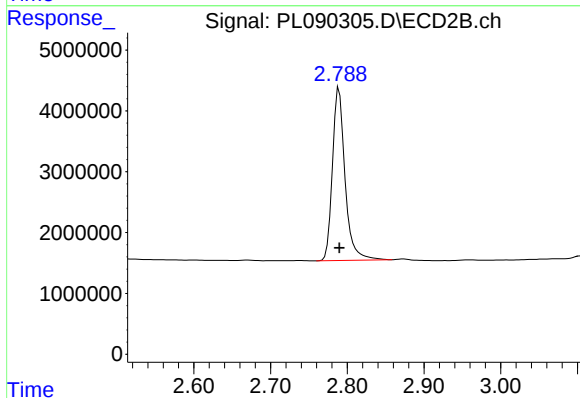


#1 Tetrachloro-m-xylene

R.T.: 2.789 min
Delta R.T.: 0.000 min
Response: 32407732
Conc: 20.49 ng/ml

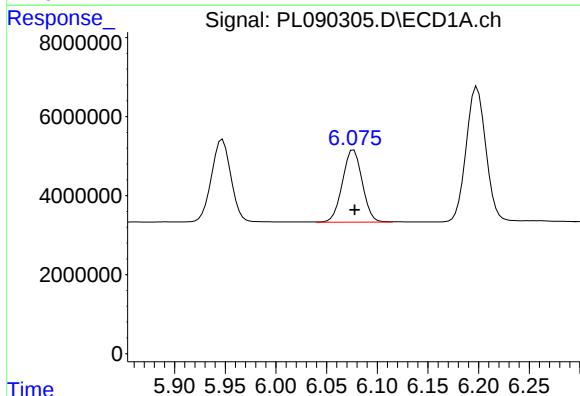


#9 Endosulfan I

R.T.: 6.077 min
Delta R.T.: -0.001 min
Response: 24876975
Conc: 10.56 ng/ml

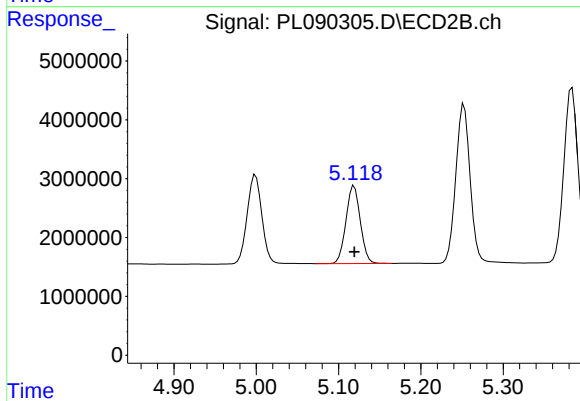

#9 Endosulfan I


R.T.: 5.119 min
Delta R.T.: 0.000 min
Response: 16038422
Conc: 9.27 ng/ml

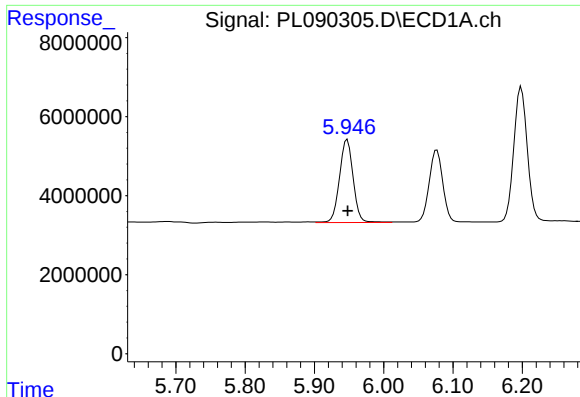

#10 gamma-Chlordane


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 28842704
Conc: 11.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

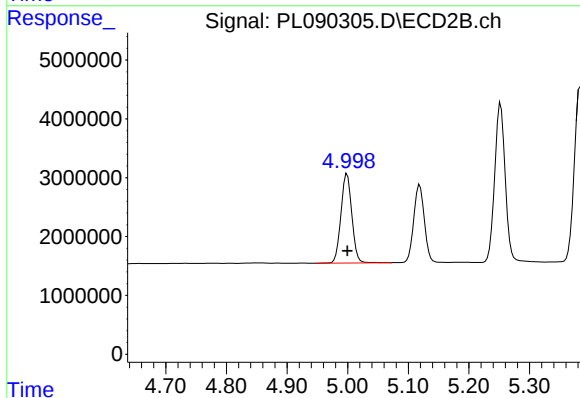


#10 gamma-Chlordane

R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 18867818
Conc: 9.84 ng/ml

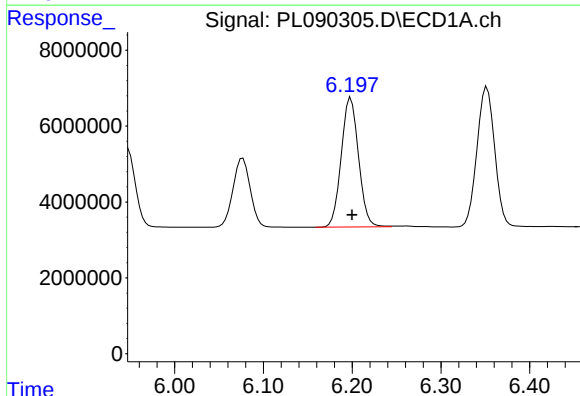


#12 4,4'-DDE

R.T.: 6.199 min
Delta R.T.: -0.001 min
Response: 46126102
Conc: 21.13 ng/ml

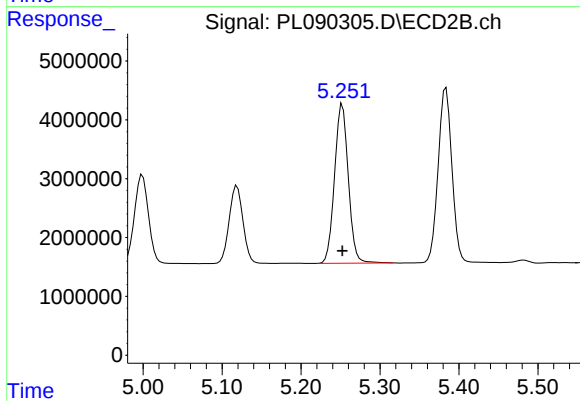

#12 4,4'-DDE


R.T.: 5.252 min
Delta R.T.: 0.000 min
Response: 32769969
Conc: 19.78 ng/ml

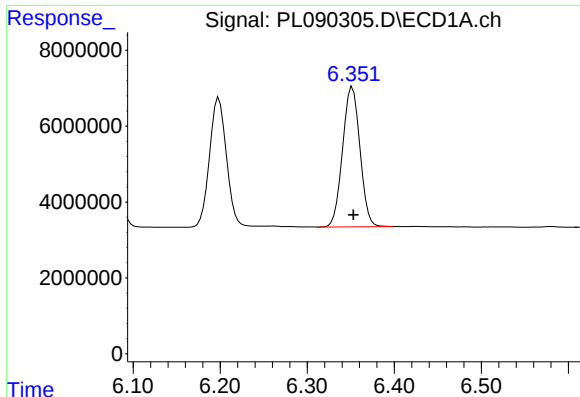

#13 Dieldrin


R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 51180482
Conc: 20.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

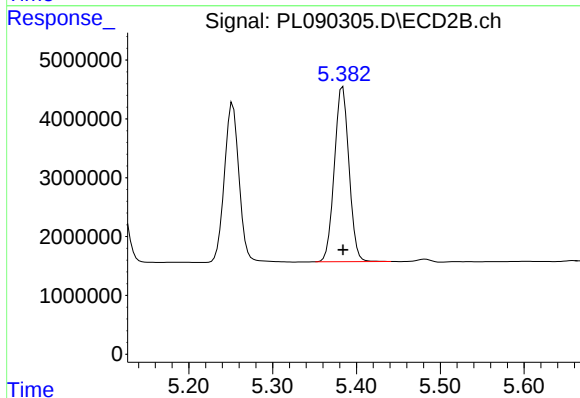


#13 Dieldrin

R.T.: 5.384 min
Delta R.T.: 0.000 min
Response: 35979443
Conc: 19.51 ng/ml

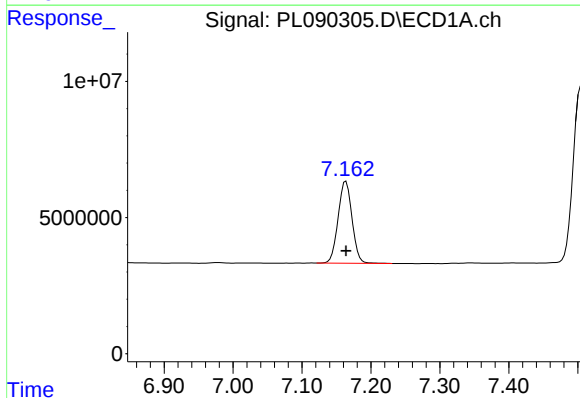


#19 Endosulfan Sulfate

R.T.: 7.164 min
Delta R.T.: 0.000 min
Response: 42098374
Conc: 21.25 ng/ml

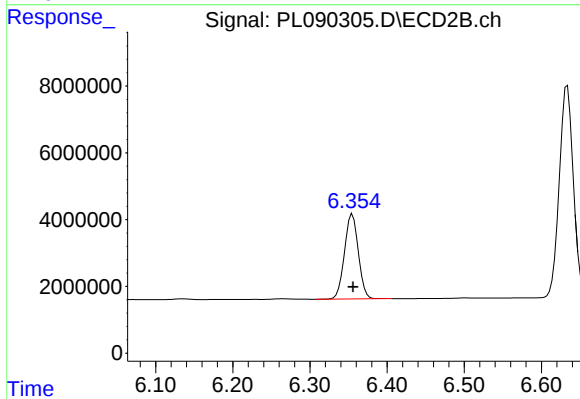

#19 Endosulfan Sulfate


R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 31595910
Conc: 20.21 ng/ml

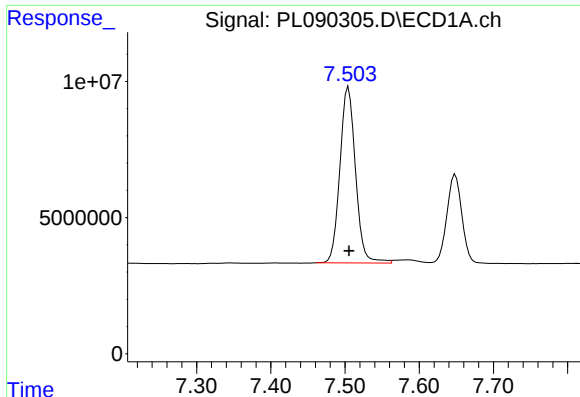

#20 Methoxychlor


R.T.: 7.505 min
Delta R.T.: 0.000 min
Response: 94569310
Conc: 91.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

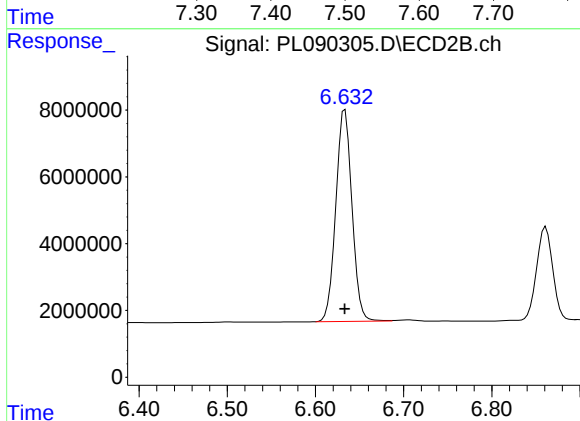


#20 Methoxychlor

R.T.: 6.633 min
Delta R.T.: 0.000 min
Response: 80794597
Conc: 96.84 ng/ml

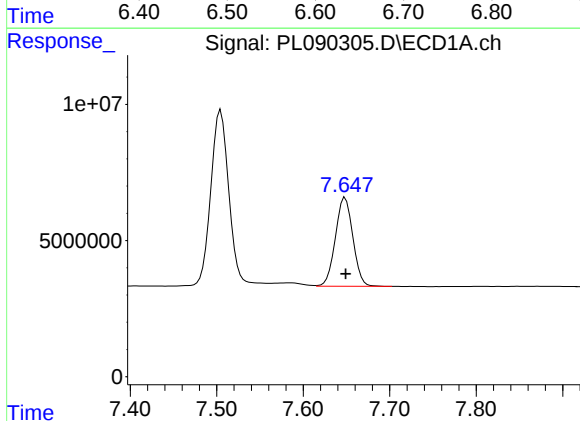


#21 Endrin ketone

R.T.: 7.649 min
Delta R.T.: 0.000 min
Response: 45477342
Conc: 20.97 ng/ml

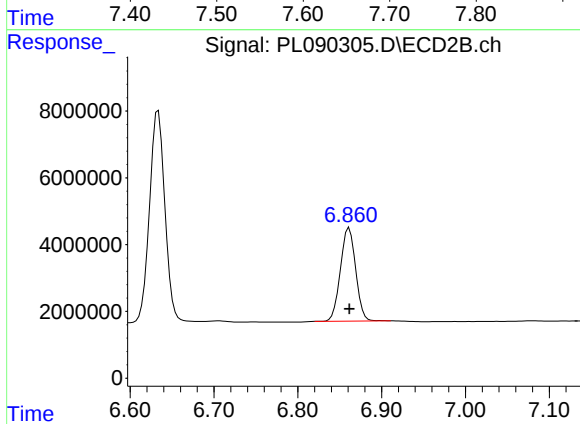

#21 Endrin ketone


R.T.: 6.861 min
Delta R.T.: 0.000 min
Response: 35384609
Conc: 19.76 ng/ml

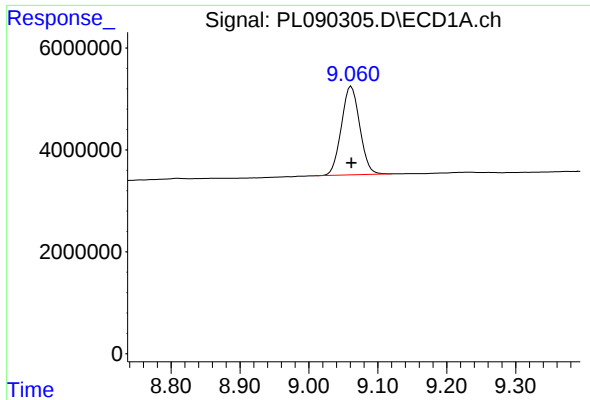

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 32282562
Conc: 20.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

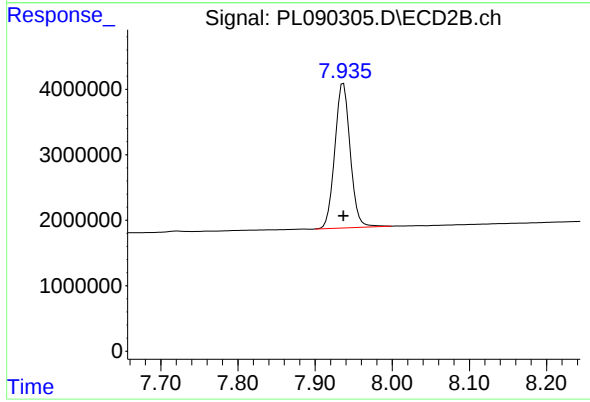

#28 Decachlorobiphenyl

R.T.: 7.937 min
Delta R.T.: 0.000 min
Response: 30626596
Conc: 20.53 ng/ml