

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062424\
 Data File : PL090313.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2024 18:41
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:28:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062424.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 25 01:25:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.789	106.1E6	91610830	50.000	50.000
28)	SA Decachlor...	9.060	7.935	73109382	73088788	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.708	3.791	46105431	28887817	500.000	500.000
24)	Chlordane-2	5.238	4.369	54344416	33180993	500.000	500.000
25)	Chlordane-3	5.947	4.999	168.6E6	96643725	500.000	500.000
26)	Chlordane-4	6.030	5.062	206.4E6	91659033	500.000	500.000
27)	Chlordane-5	6.878	5.728	42877949	28233315	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062424\
Data File : PL090313.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2024 18:41
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:28:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062424.M
Quant Title : GC Extractables
QLast Update : Tue Jun 25 01:25:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

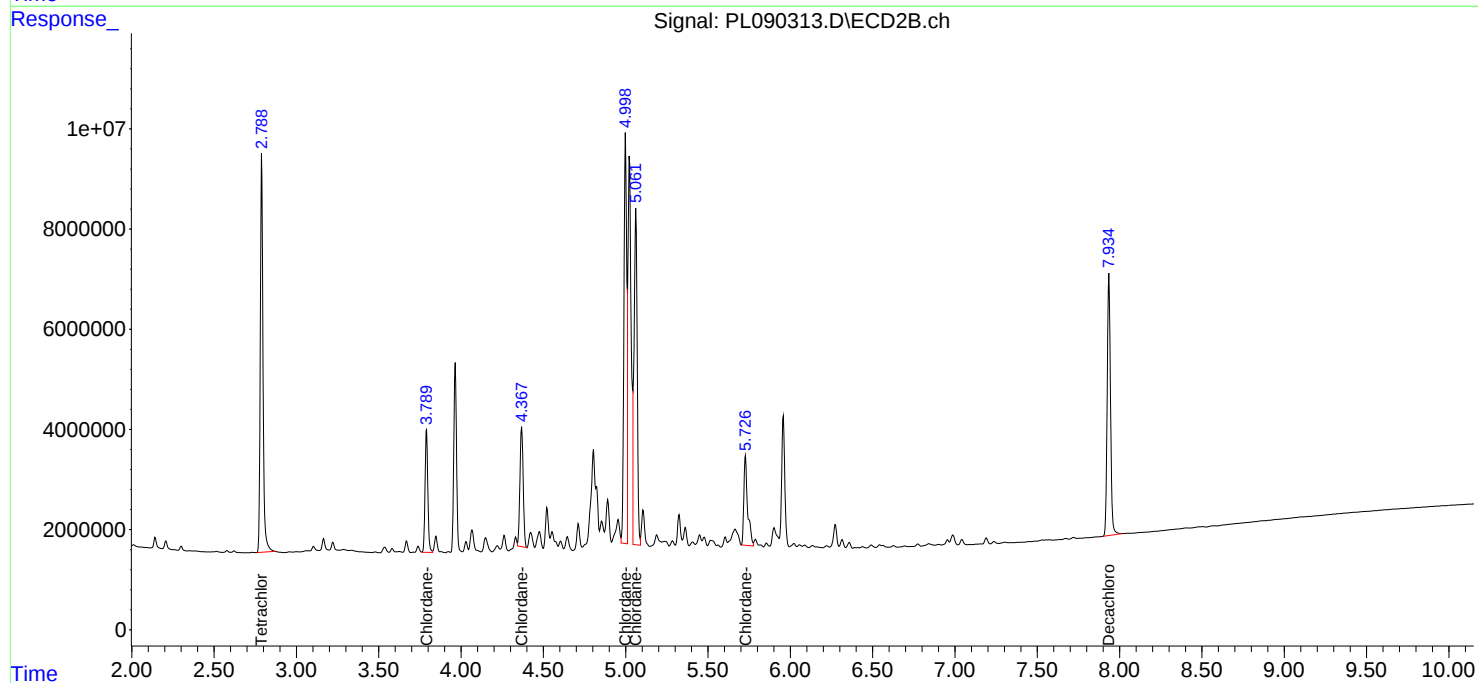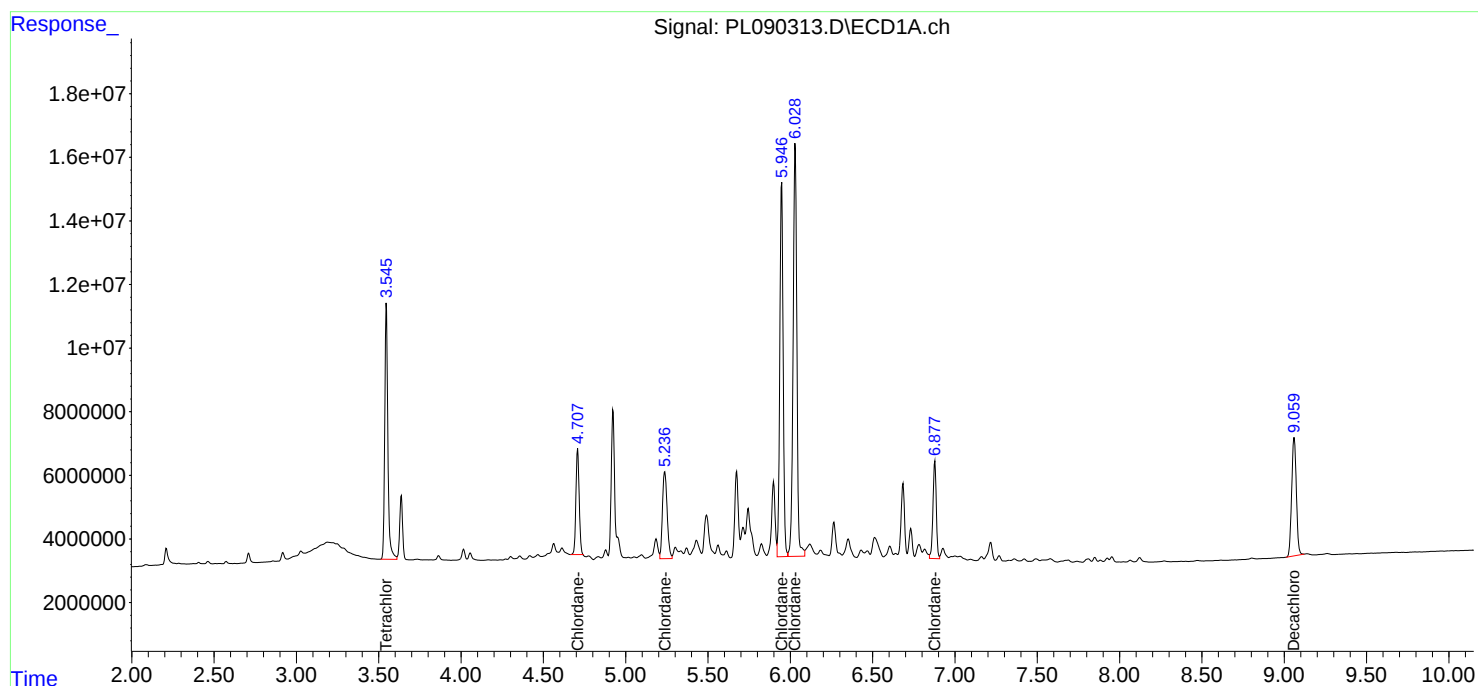


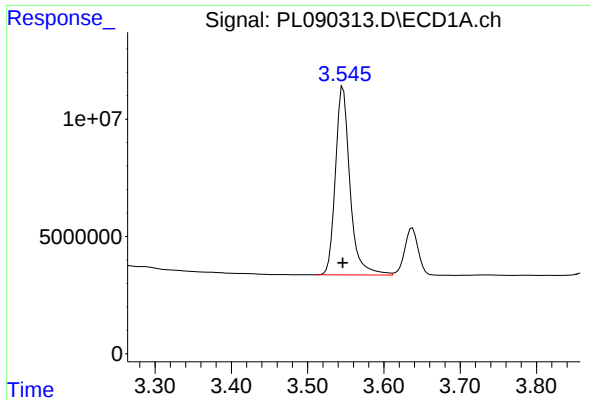

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 106052702
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

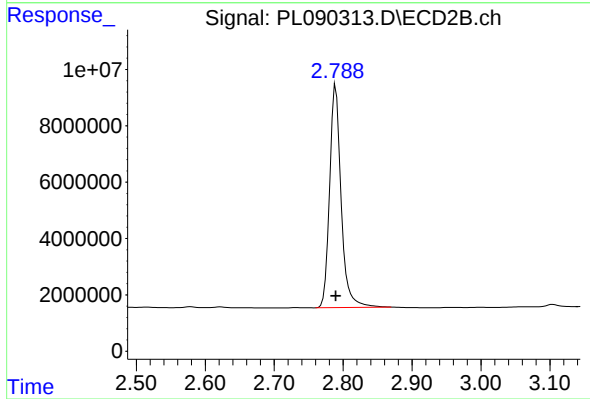


#1 Tetrachloro-m-xylene

R.T.: 2.789 min
Delta R.T.: 0.000 min
Response: 91610830
Conc: 50.00 ng/ml

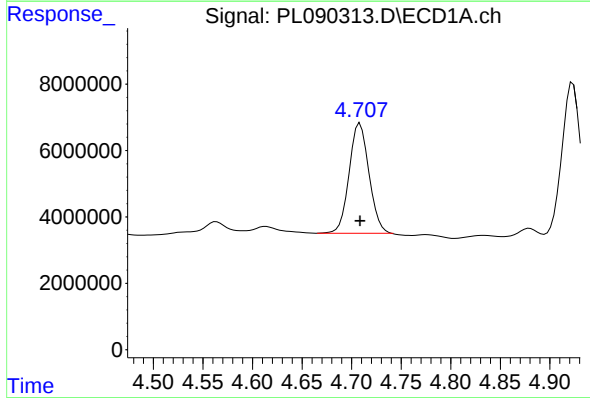


#23 Chlordane-1

R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 46105431
Conc: 500.00 ng/ml

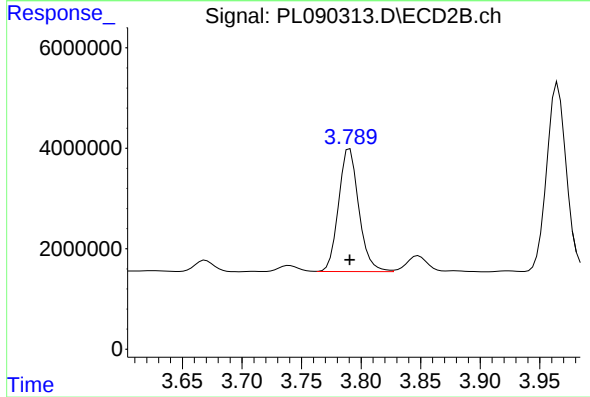

#23 Chlordane-1


R.T.: 3.791 min
Delta R.T.: 0.000 min
Response: 28887817
Conc: 500.00 ng/ml

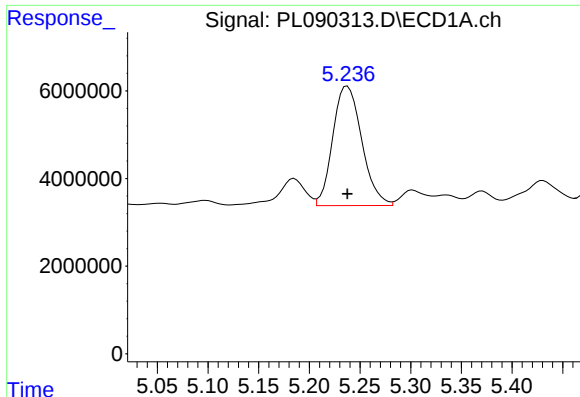

#24 Chlordane-2


R.T.: 5.238 min
Delta R.T.: 0.000 min
Response: 54344416
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

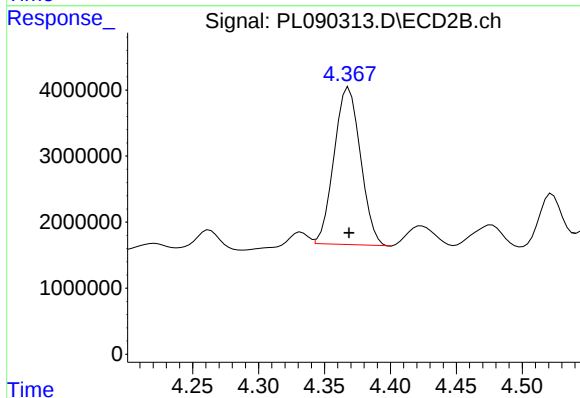


#24 Chlordane-2

R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 33180993
Conc: 500.00 ng/ml

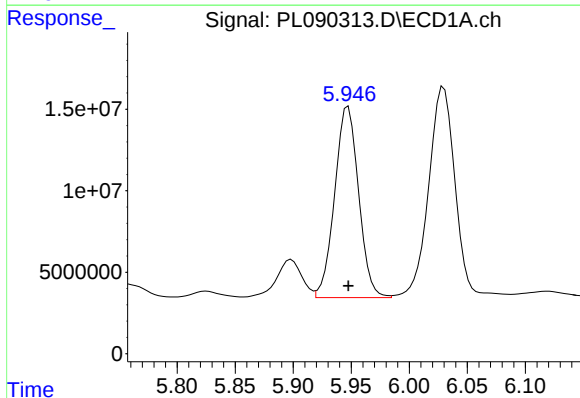


#25 Chlordane-3

R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 168570136
Conc: 500.00 ng/ml

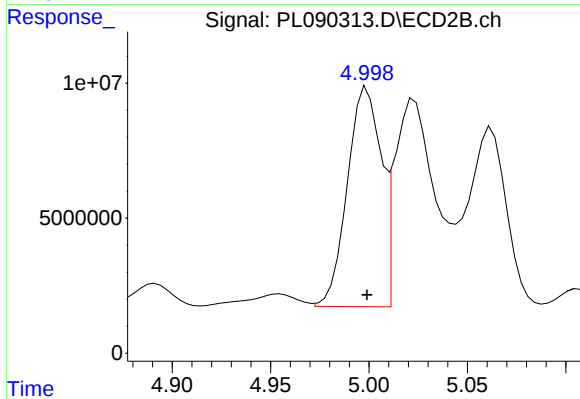

#25 Chlordane-3


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 96643725
Conc: 500.00 ng/ml

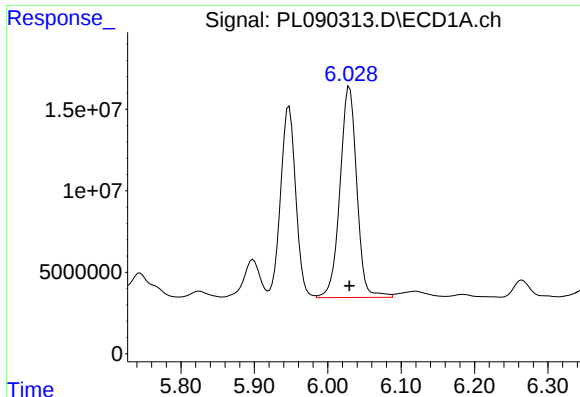

#26 Chlordane-4


R.T.: 6.030 min
Delta R.T.: 0.000 min
Response: 206388655
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

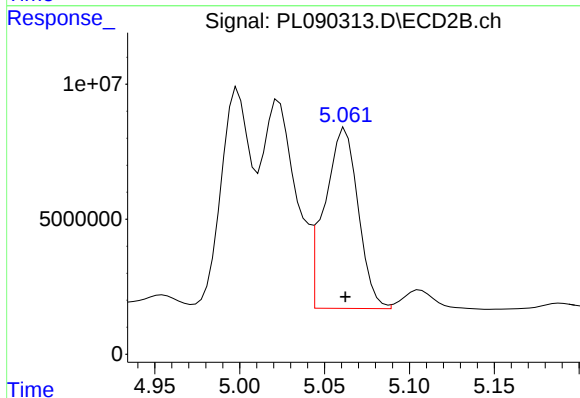


#26 Chlordane-4

R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 91659033
Conc: 500.00 ng/ml

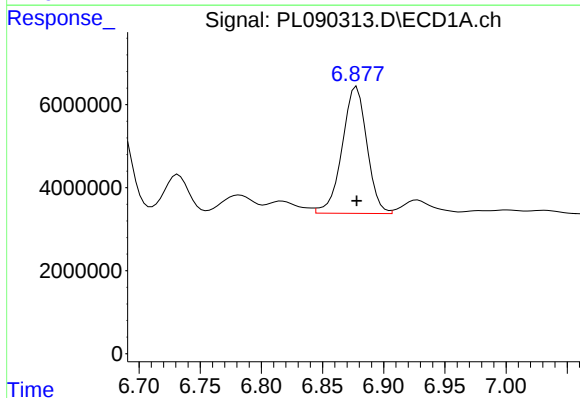


#27 Chlordane-5

R.T.: 6.878 min
Delta R.T.: 0.000 min
Response: 42877949
Conc: 500.00 ng/ml

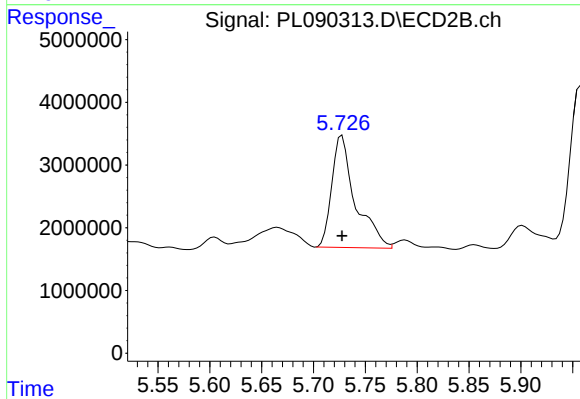

#27 Chlordane-5


R.T.: 5.728 min
Delta R.T.: 0.000 min
Response: 28233315
Conc: 500.00 ng/ml

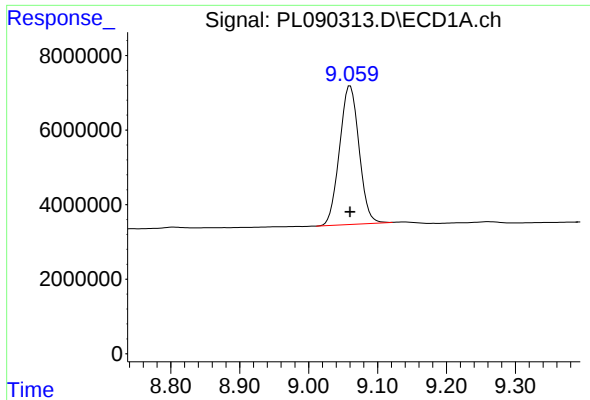

#28 Decachlorobiphenyl

R.T.: 9.060 min
Delta R.T.: 0.000 min
Response: 73109382
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

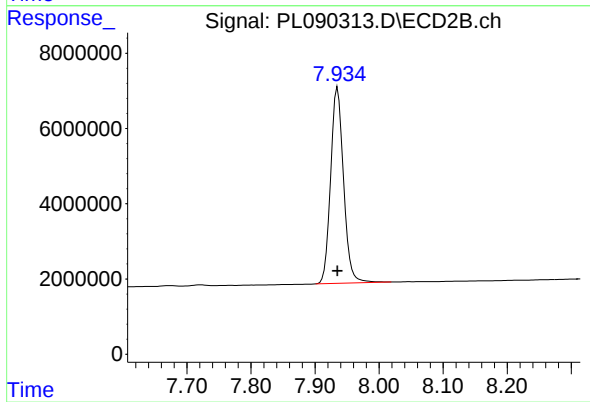

#28 Decachlorobiphenyl

R.T.: 7.935 min
Delta R.T.: 0.000 min
Response: 73088788
Conc: 50.00 ng/ml