

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062424\
 Data File : PL090314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2024 18:55
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:36:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062424.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 25 01:36:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.789	58512503	47741110	27.344	25.533
28)	SA Decachlor...	9.061	7.936	39706412	38669915	27.345	26.172
Target Compounds							
23)	Chlordane-1	4.708	3.791	25222188	15230300	270.203	258.510
24)	Chlordane-2	5.237	4.369	33671613	18010589	300.304	268.022
25)	Chlordane-3	5.947	4.999	91858506	49162377	267.238	247.306
26)	Chlordane-4	6.029	5.063	111.0E6	45987854	265.273	246.145
27)	Chlordane-5	6.877	5.729	23346898	15131098	271.747	263.018



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062424\
Data File : PL090314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2024 18:55
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:36:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062424.M
Quant Title : GC Extractables
QLast Update : Tue Jun 25 01:36:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

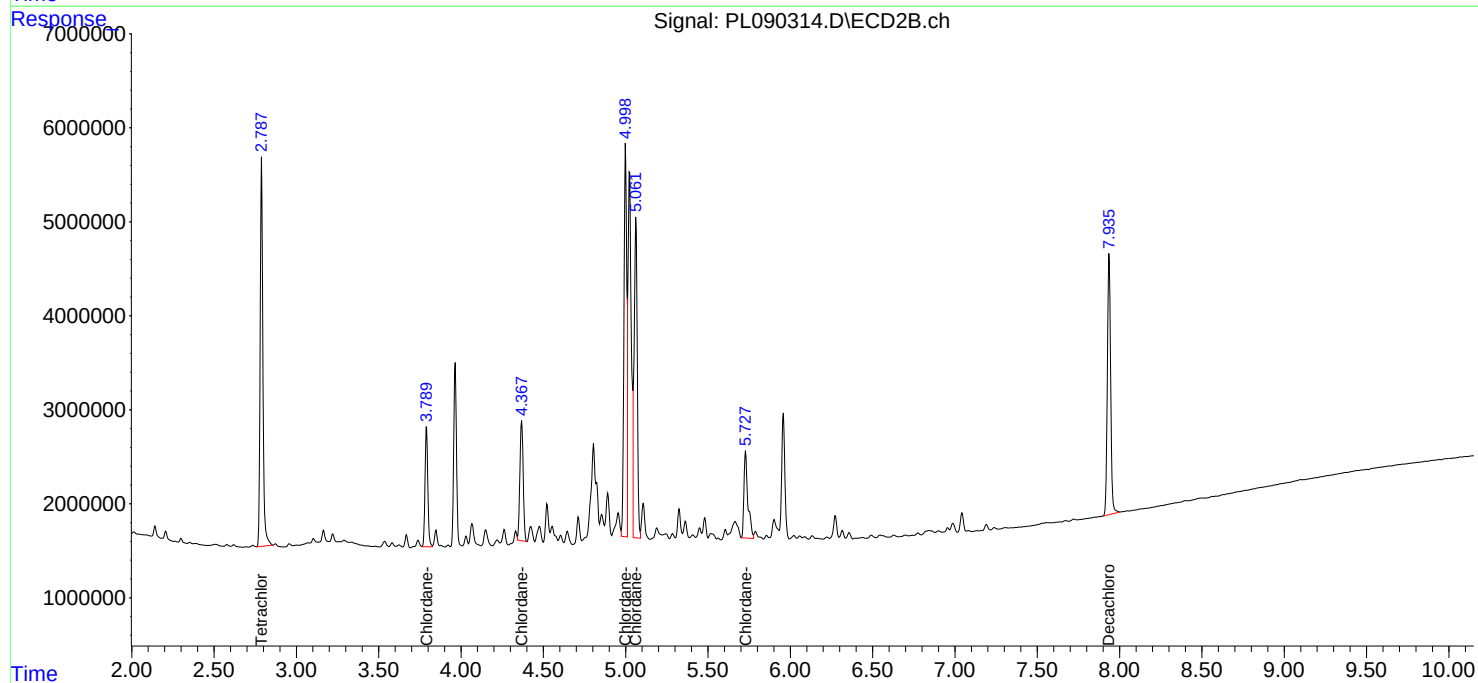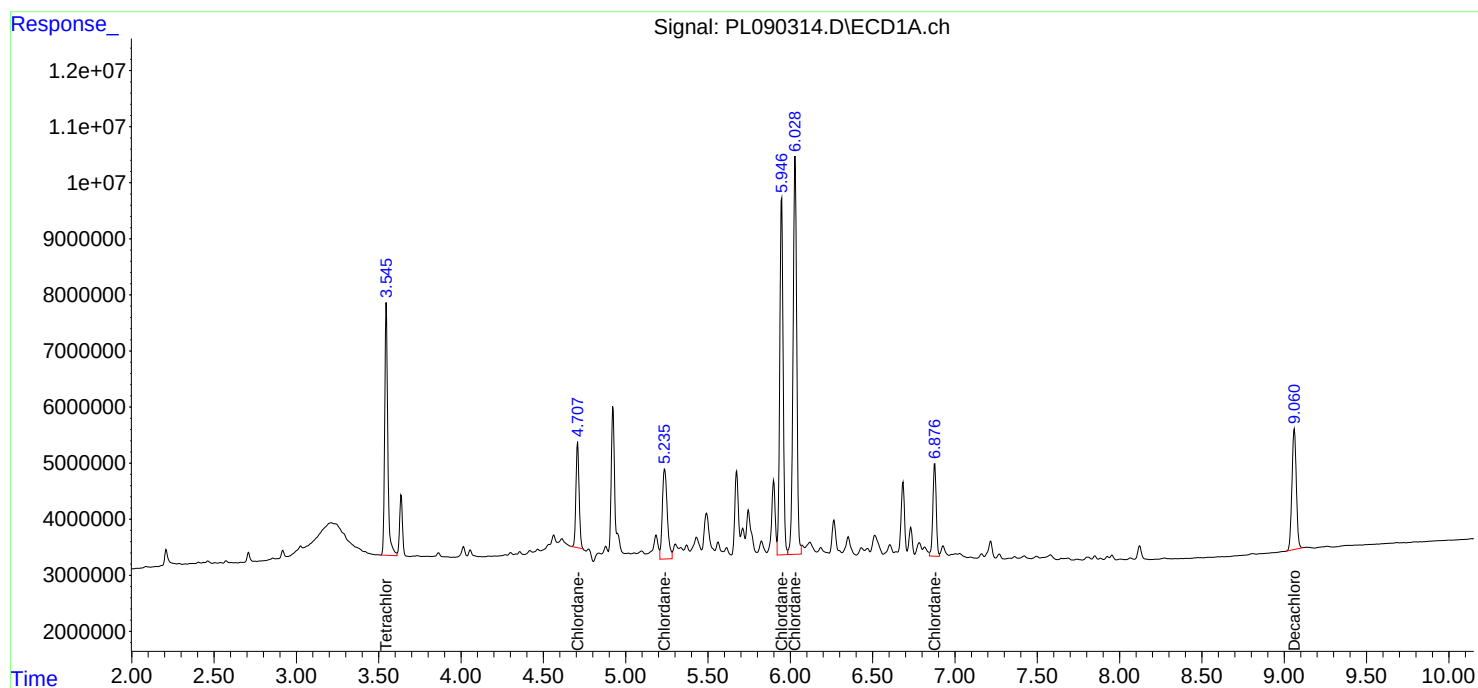


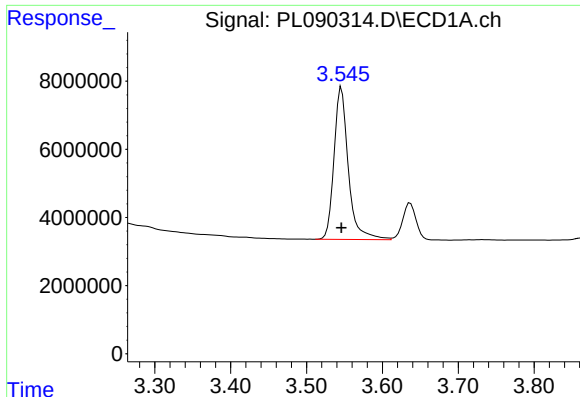

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 58512503
Conc: 27.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

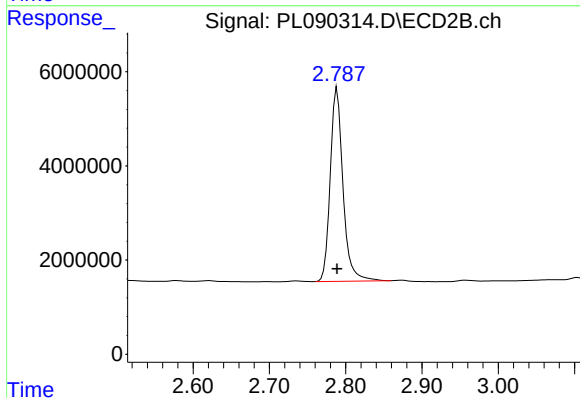


#1 Tetrachloro-m-xylene

R.T.: 2.789 min
Delta R.T.: 0.000 min
Response: 47741110
Conc: 25.53 ng/ml

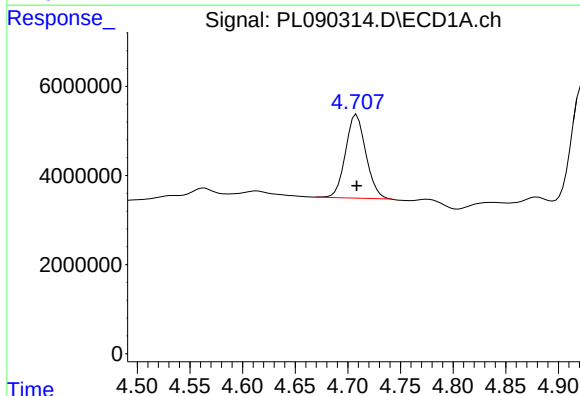


#23 Chlordane-1

R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 25222188
Conc: 270.20 ng/ml

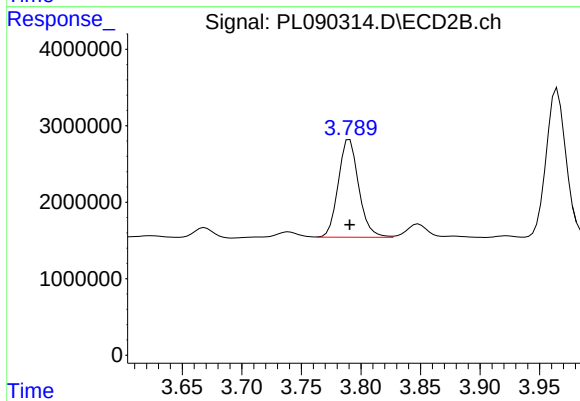

#23 Chlordane-1


R.T.: 3.791 min
Delta R.T.: 0.000 min
Response: 15230300
Conc: 258.51 ng/ml

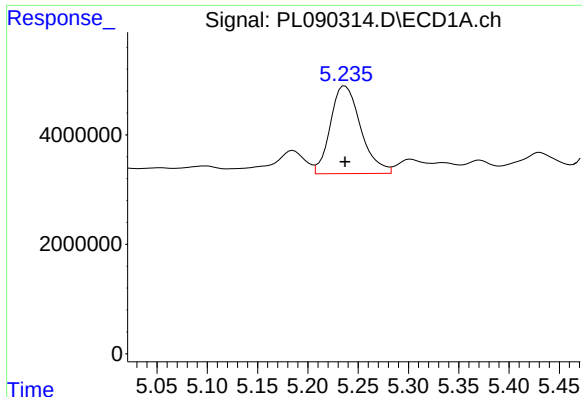

#24 Chlordane-2


R.T.: 5.237 min
Delta R.T.: 0.000 min
Response: 33671613
Conc: 300.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

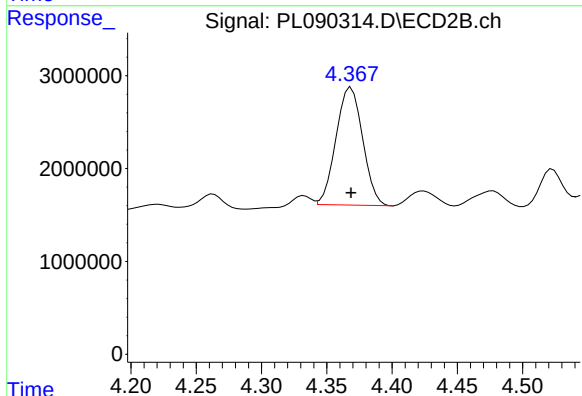


#24 Chlordane-2

R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 18010589
Conc: 268.02 ng/ml

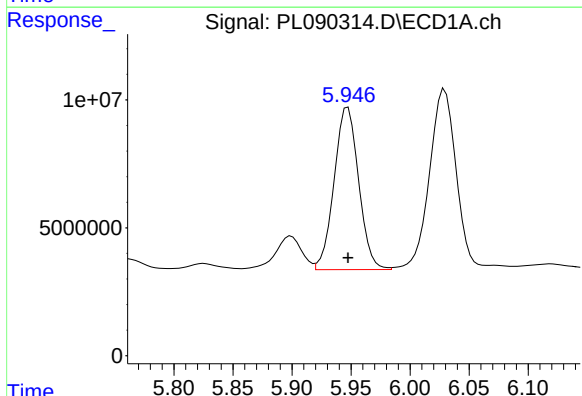


#25 Chlordane-3

R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 91858506
Conc: 267.24 ng/ml

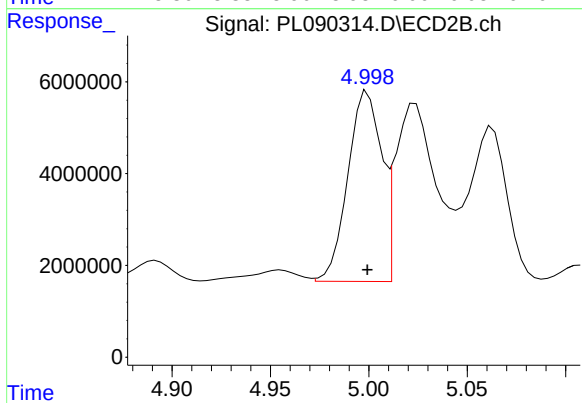

#25 Chlordane-3


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 49162377
Conc: 247.31 ng/ml

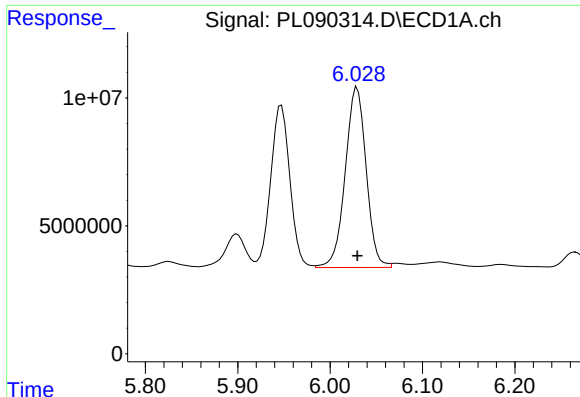

#26 Chlordane-4


R.T.: 6.029 min
Delta R.T.: 0.000 min
Response: 110971261
Conc: 265.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

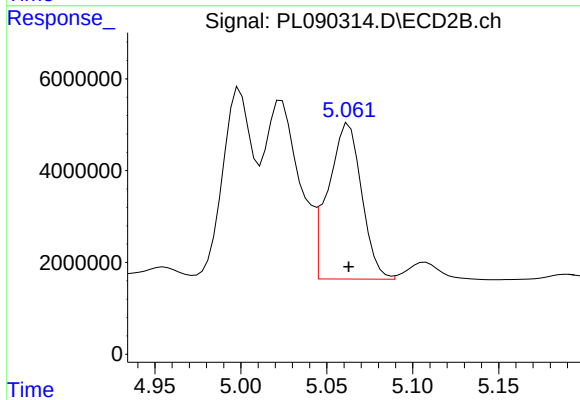


#26 Chlordane-4

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 45987854
Conc: 246.14 ng/ml

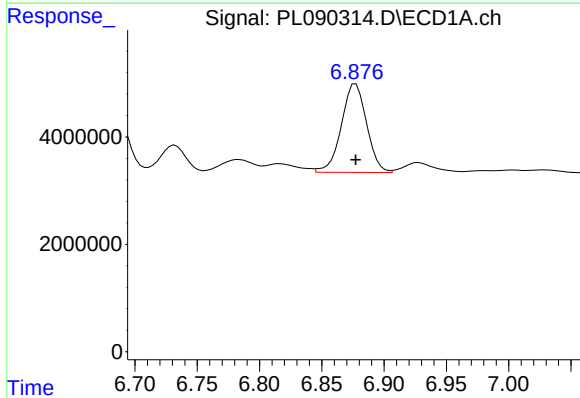


#27 Chlordane-5

R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 23346898
Conc: 271.75 ng/ml

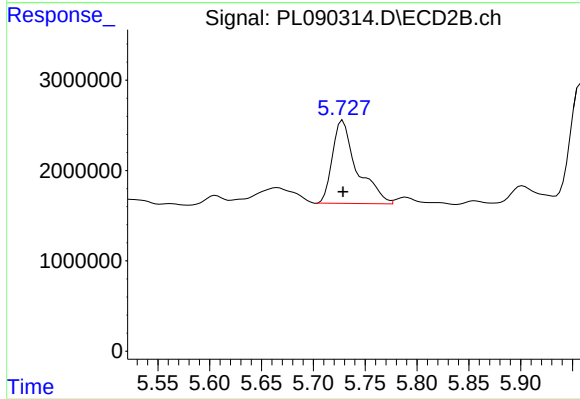

#27 Chlordane-5


R.T.: 5.729 min
Delta R.T.: 0.000 min
Response: 15131098
Conc: 263.02 ng/ml

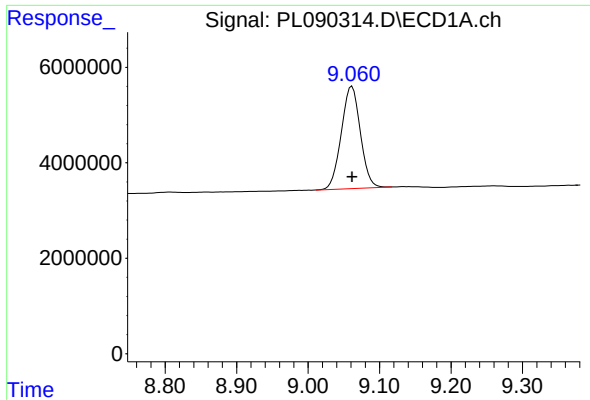

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 39706412
Conc: 27.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

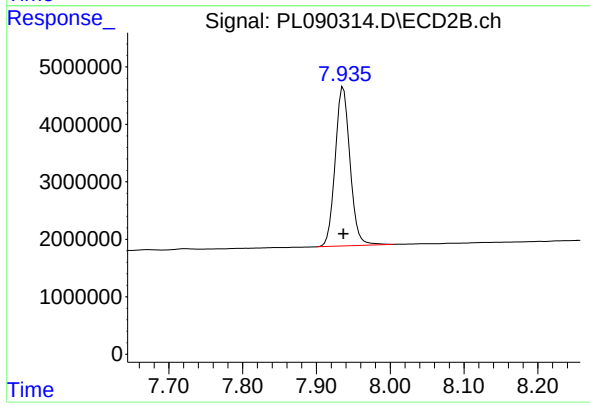

#28 Decachlorobiphenyl

R.T.: 7.936 min
Delta R.T.: 0.000 min
Response: 38669915
Conc: 26.17 ng/ml