

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062424\
 Data File : PL090322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2024 20:45
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL062424

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 11:03:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062424.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 25 11:02:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.789	113.0E6	97120419	50.656	50.667
28)	SA Decachlor...	9.062	7.936	76419735	76987961	49.054	49.864
Target Compounds							
23)	Chlordane-1	4.709	3.791	49006373	30776197	498.922	505.473
24)	Chlordane-2	5.237	4.369	57562983	35800250	485.276	506.614
25)	Chlordane-3	5.948	5.000	178.5E6	103.0E6	485.565	510.067
26)	Chlordane-4	6.029	5.063	218.4E6	97109079	489.639	508.638
27)	Chlordane-5	6.878	5.729	45283924	29945916	502.763	495.772



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062424\
Data File : PL090322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2024 20:45
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL062424

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 11:03:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062424.M
Quant Title : GC Extractables
QLast Update : Tue Jun 25 11:02:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

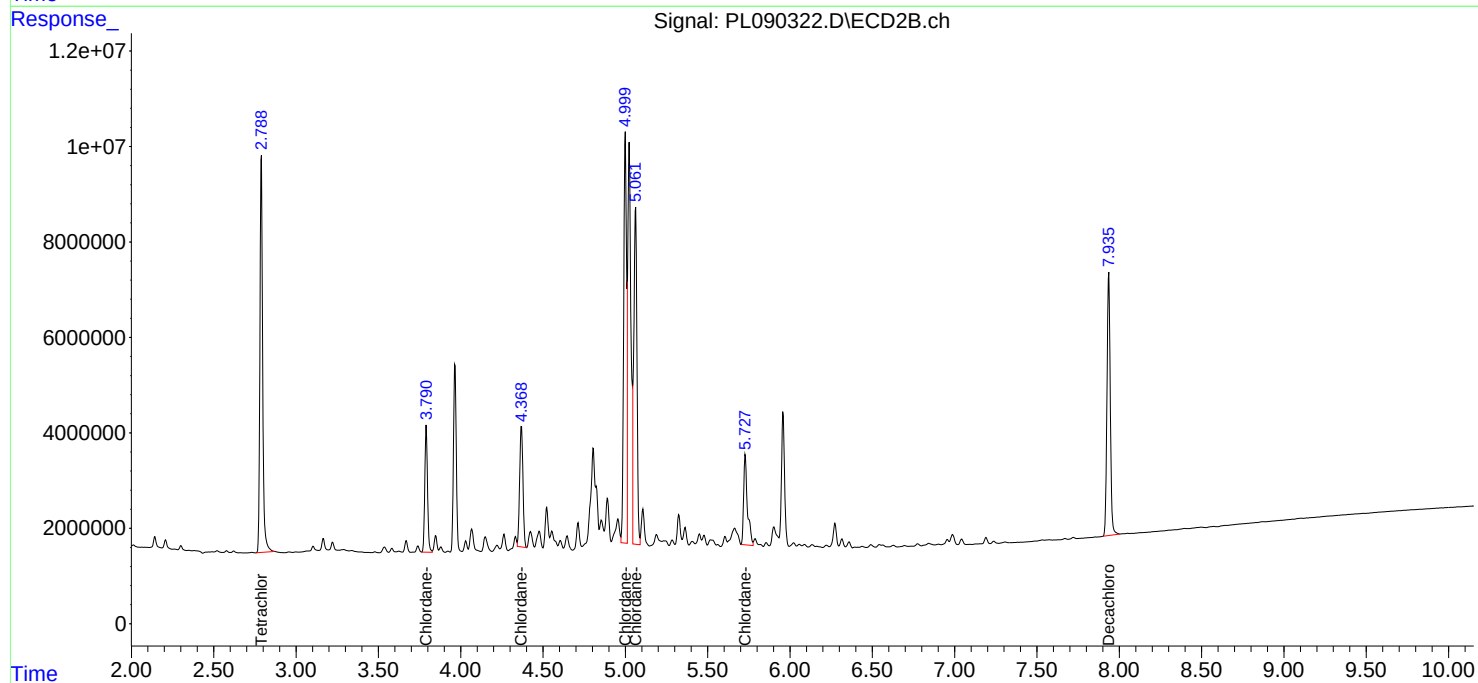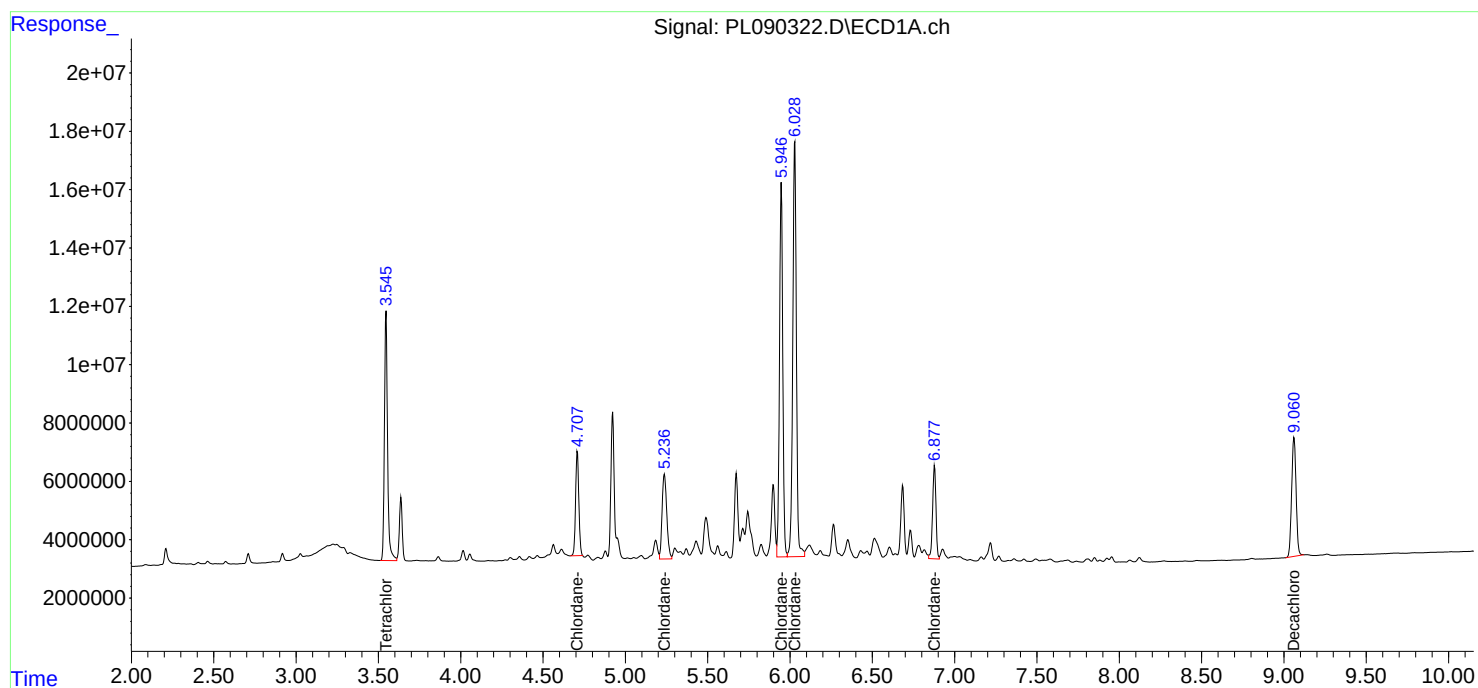


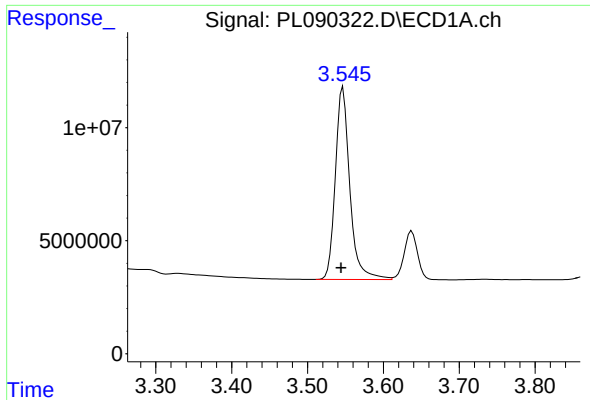

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.003 min
Response: 113023271
Conc: 50.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL062424

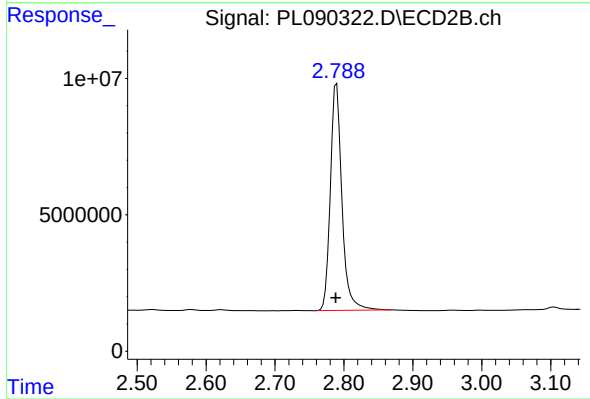


#1 Tetrachloro-m-xylene

R.T.: 2.789 min
Delta R.T.: 0.001 min
Response: 97120419
Conc: 50.67 ng/ml

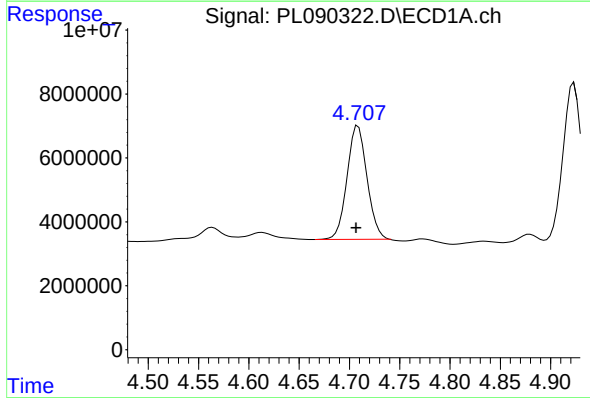


#23 Chlordane-1

R.T.: 4.709 min
Delta R.T.: 0.002 min
Response: 49006373
Conc: 498.92 ng/ml

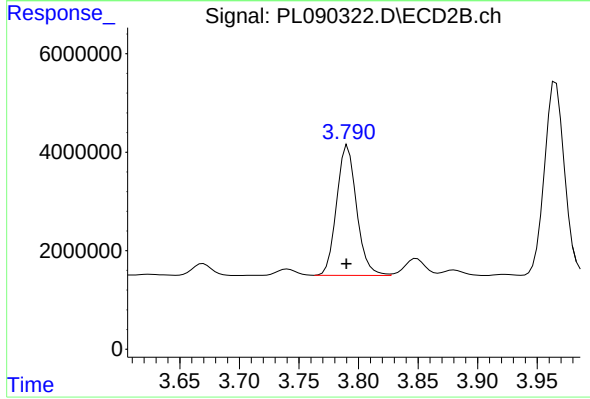

#23 Chlordane-1


R.T.: 3.791 min
Delta R.T.: 0.001 min
Response: 30776197
Conc: 505.47 ng/ml

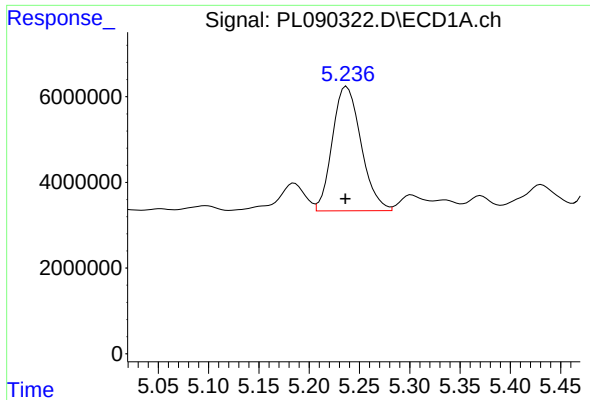

#24 Chlordane-2


R.T.: 5.237 min
Delta R.T.: 0.001 min
Response: 57562983
Conc: 485.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL062424

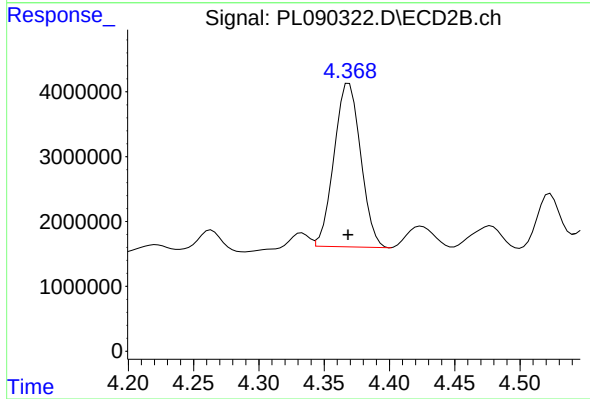


#24 Chlordane-2

R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 35800250
Conc: 506.61 ng/ml

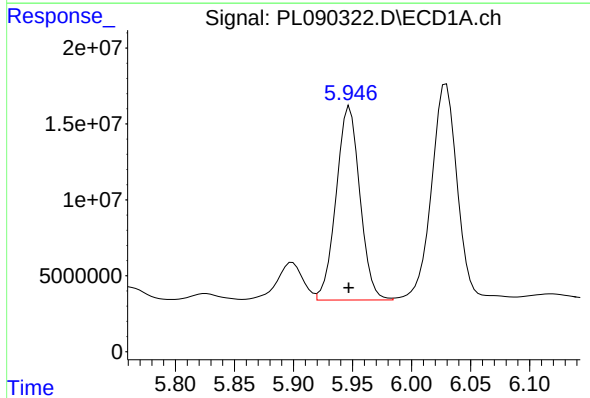


#25 Chlordane-3

R.T.: 5.948 min
Delta R.T.: 0.000 min
Response: 178522457
Conc: 485.57 ng/ml

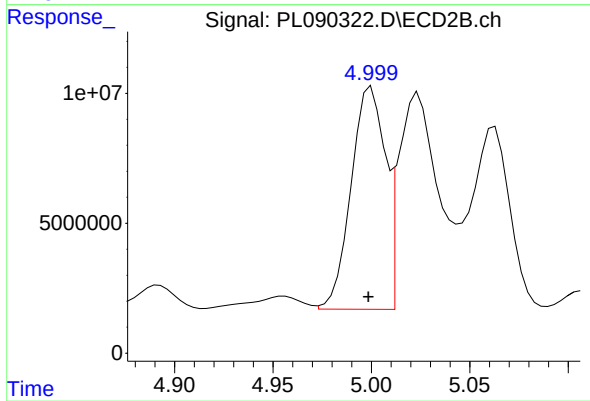

#25 Chlordane-3


R.T.: 5.000 min
Delta R.T.: 0.001 min
Response: 102987685
Conc: 510.07 ng/ml

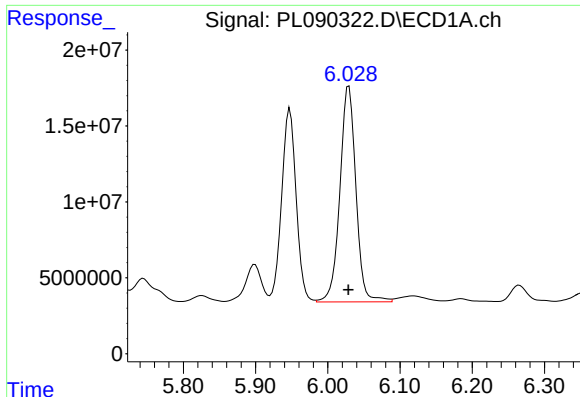

#26 Chlordane-4


R.T.: 6.029 min
Delta R.T.: 0.000 min
Response: 218432249
Conc: 489.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL062424

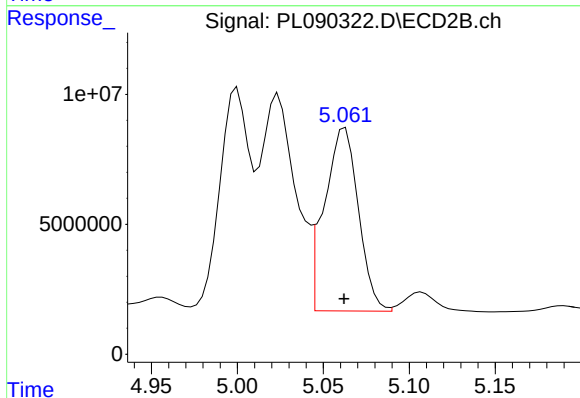


#26 Chlordane-4

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 97109079
Conc: 508.64 ng/ml

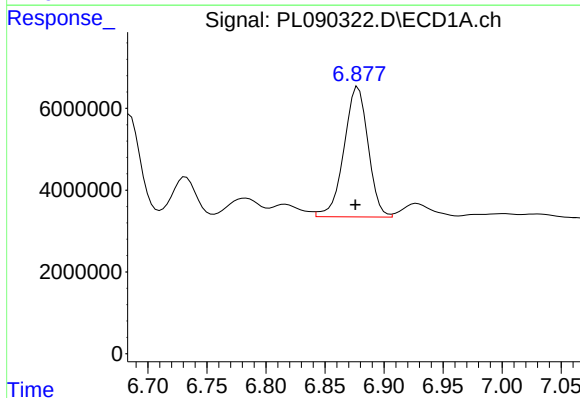


#27 Chlordane-5

R.T.: 6.878 min
Delta R.T.: 0.002 min
Response: 45283924
Conc: 502.76 ng/ml

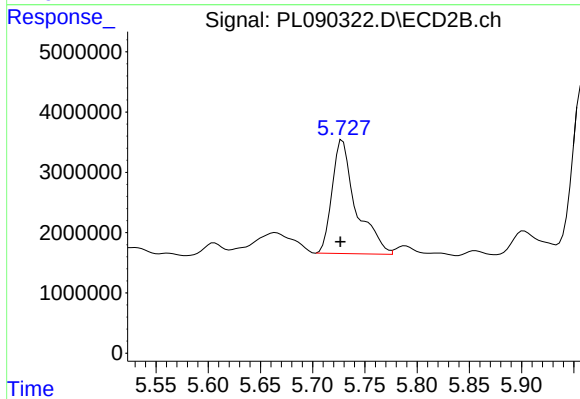

#27 Chlordane-5


R.T.: 5.729 min
Delta R.T.: 0.002 min
Response: 29945916
Conc: 495.77 ng/ml

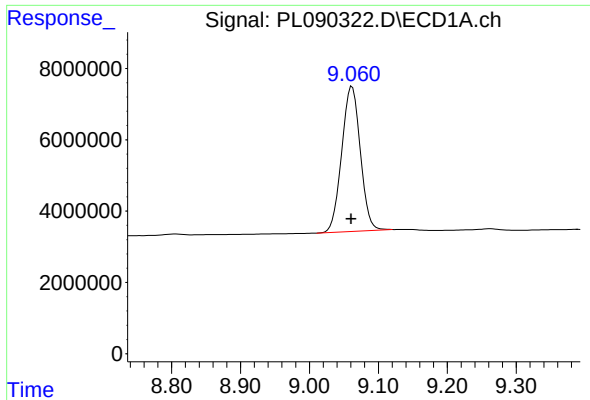

#28 Decachlorobiphenyl

R.T.: 9.062 min
Delta R.T.: 0.002 min
Response: 76419735
Conc: 49.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL062424

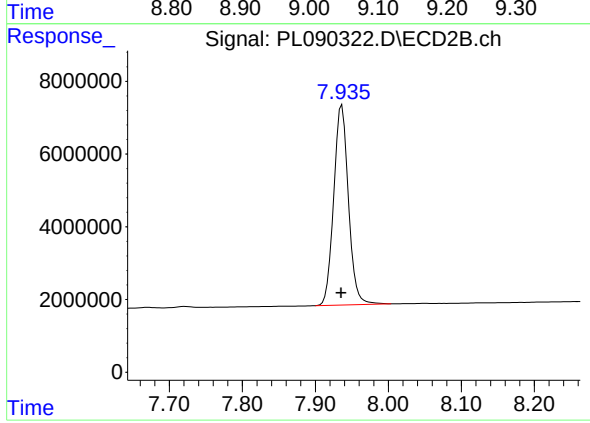

#28 Decachlorobiphenyl

R.T.: 7.936 min
Delta R.T.: 0.000 min
Response: 76987961
Conc: 49.86 ng/ml