

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062425\
 Data File : PL096156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2025 14:29
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 04:29:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062325.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 24 16:08:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	5.707	0.000	12953959	0	2.954	N.D. #
14) MA	Endrin	0.000	5.783	0	9666975	N.D.	1.769 #
24)	Chlordane-2	0.000	4.465	0	6282254	N.D.	26.678 #
25)	Chlordane-3	5.943f	0.000	1651624	0	2.144	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062425\
Data File : PL096156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2025 14:29
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 04:29:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062325.M
Quant Title : GC Extractables
QLast Update : Tue Jun 24 16:08:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

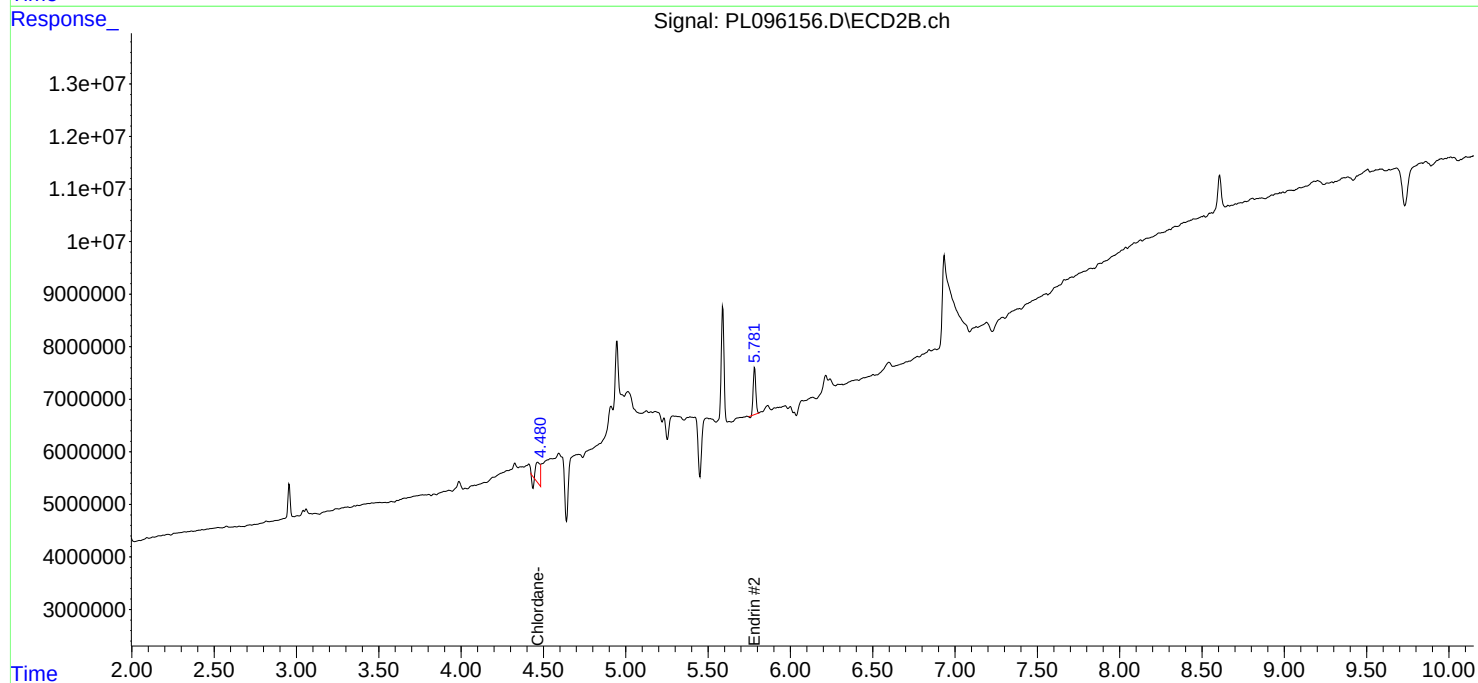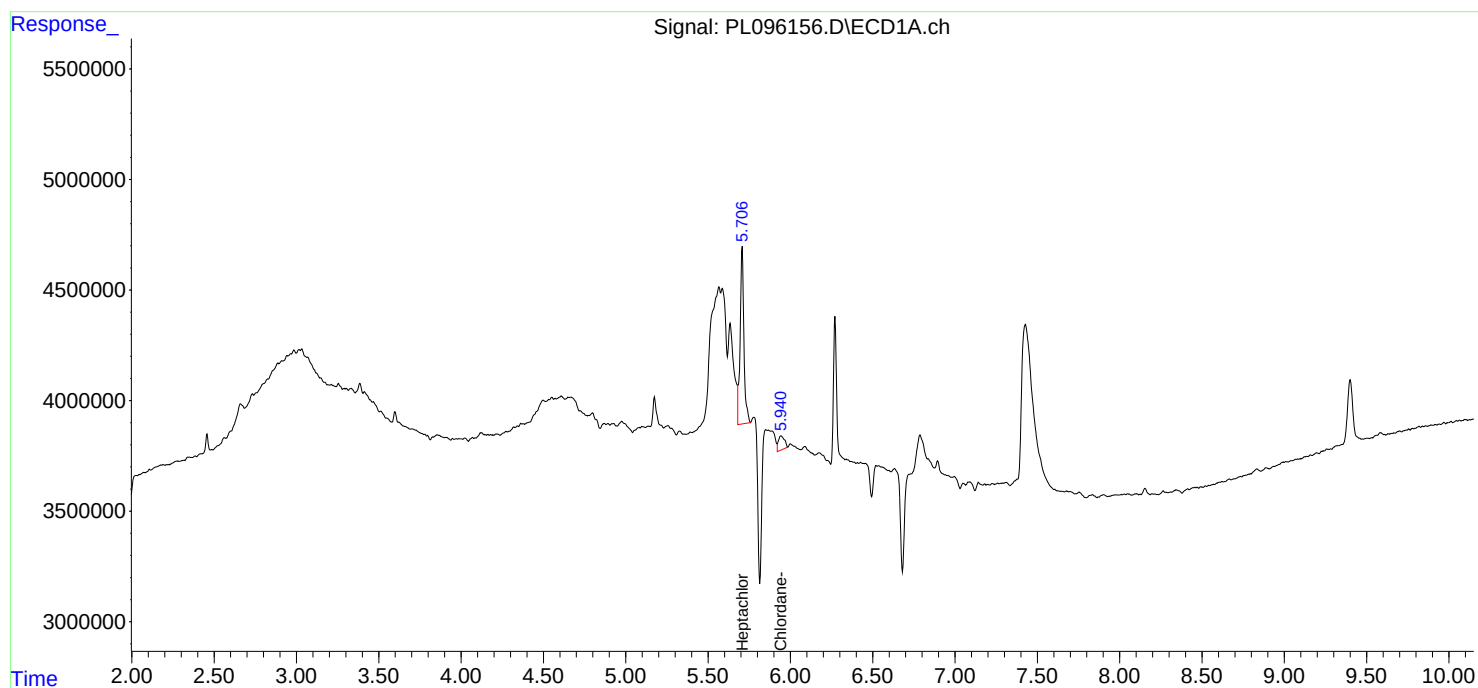


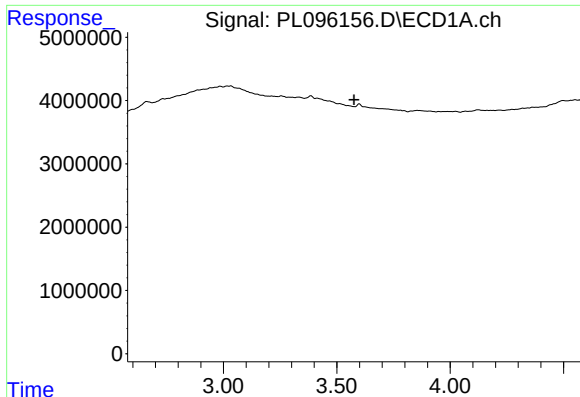

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

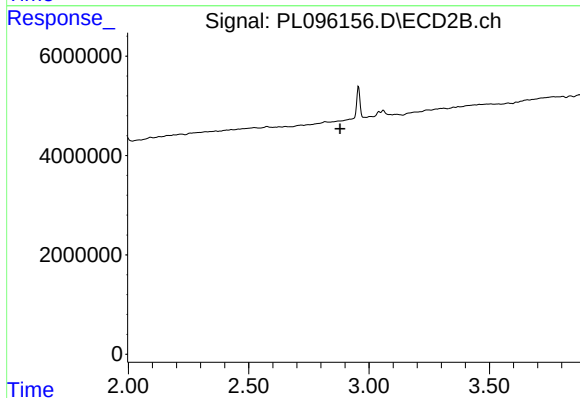


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.879 min
Response: 0
Conc: N.D.

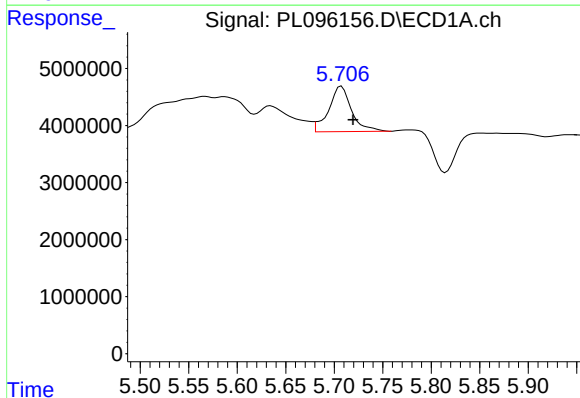


#8 Heptachlor epoxide

R.T.: 5.707 min
Delta R.T.: -0.012 min
Response: 12953959
Conc: 2.95 ng/ml

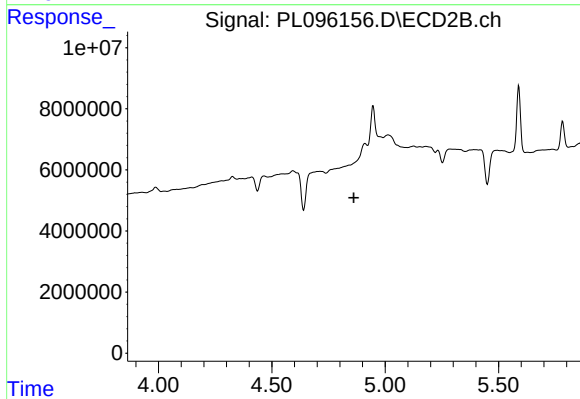

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.861 min
Response: 0
Conc: N.D.

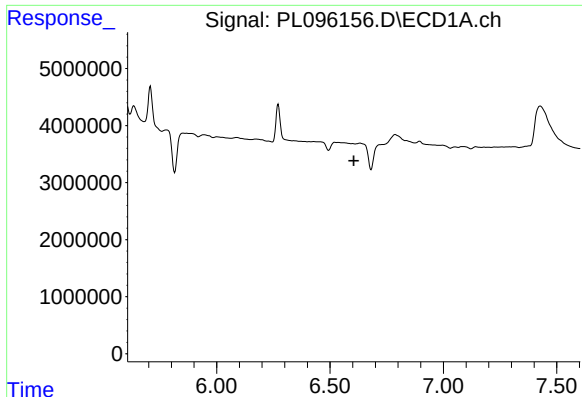

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.605 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

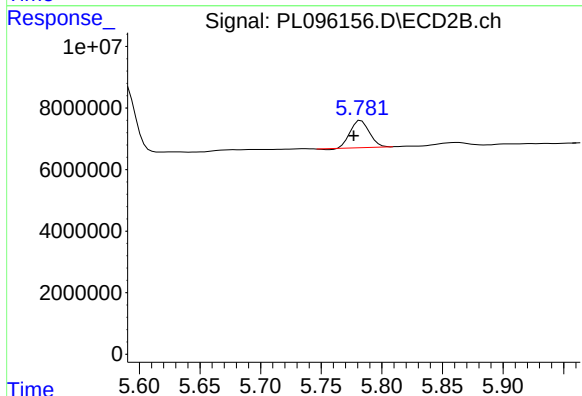


#14 Endrin

R.T.: 5.783 min
Delta R.T.: 0.006 min
Response: 9666975
Conc: 1.77 ng/ml

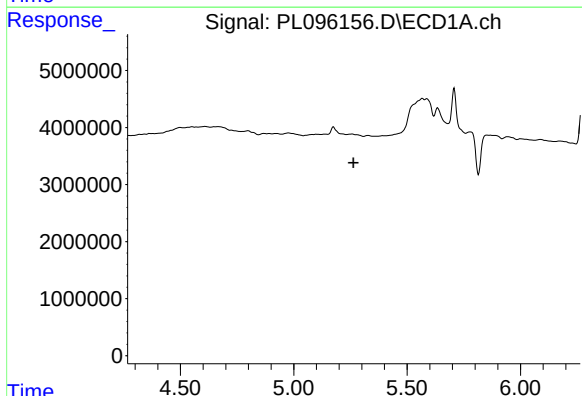


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.264 min
Response: 0
Conc: N.D.

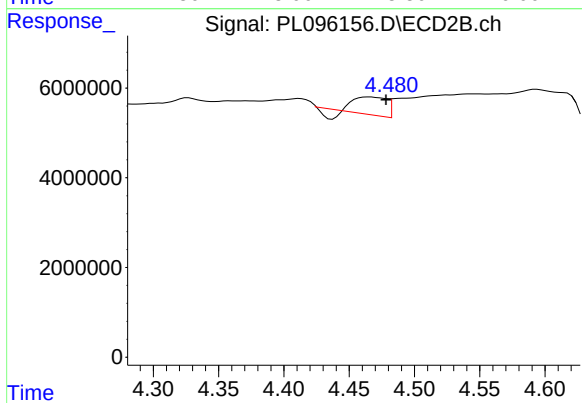

#24 Chlordane-2


R.T.: 4.465 min
Delta R.T.: -0.013 min
Response: 6282254
Conc: 26.68 ng/ml

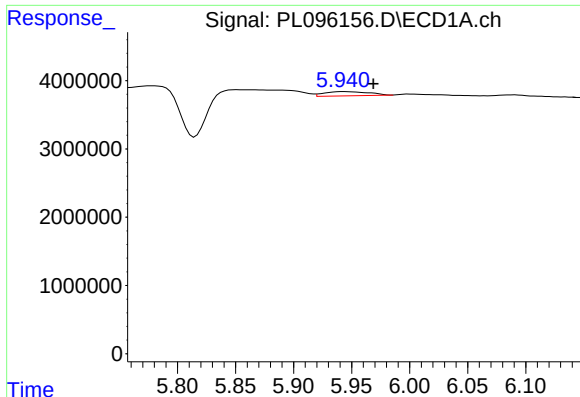

#25 Chlordane-3


R.T.: 5.943 min
Delta R.T.: -0.025 min
Response: 1651624
Conc: 2.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

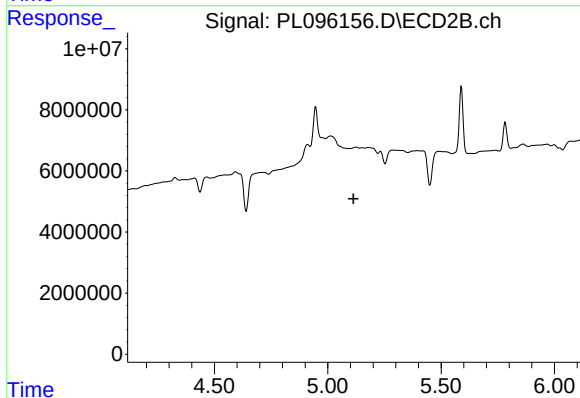


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

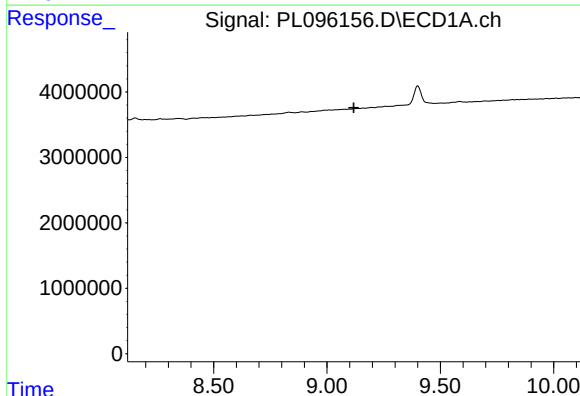

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.118 min
Response: 0
Conc: N.D.

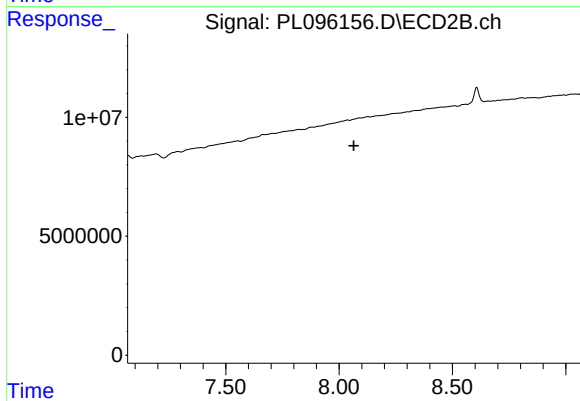

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.064 min
Response: 0
Conc: N.D.