

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062425\
 Data File : PL096160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2025 16:07
 Operator : AR\AJ
 Sample : PB168452BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB168452BL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/25/2025
 Supervised By :mohammad ahmed 06/26/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 04:57:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062325.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 24 16:08:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.577	2.879	59892513	74935797	17.399	17.079
28) SA Decachlor...	9.144f	8.065	51958774	98751351	19.490m	18.351

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062425\
Data File : PL096160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2025 16:07
Operator : AR\AJ
Sample : PB168452BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB168452BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/25/2025
Supervised By : mohammad ahmed 06/26/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 04:57:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062325.M
Quant Title : GC Extractables
QLast Update : Tue Jun 24 16:08:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

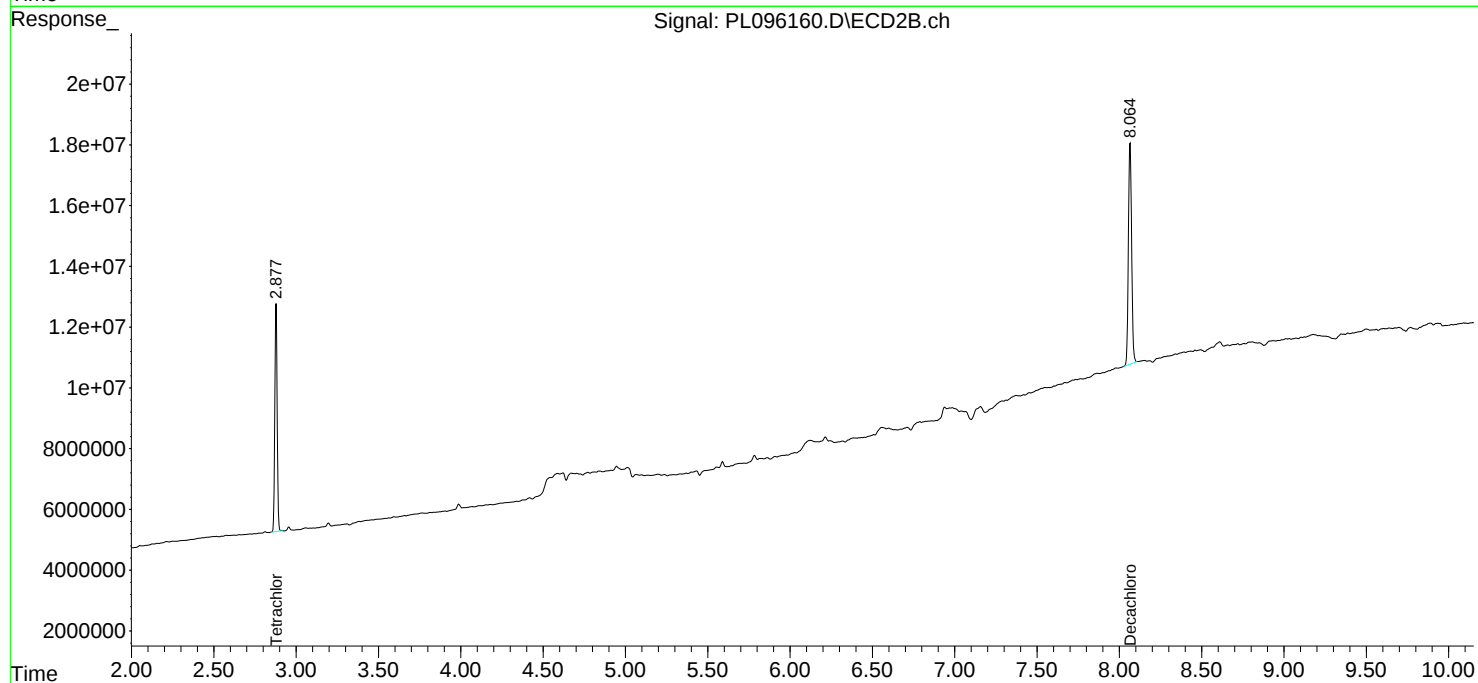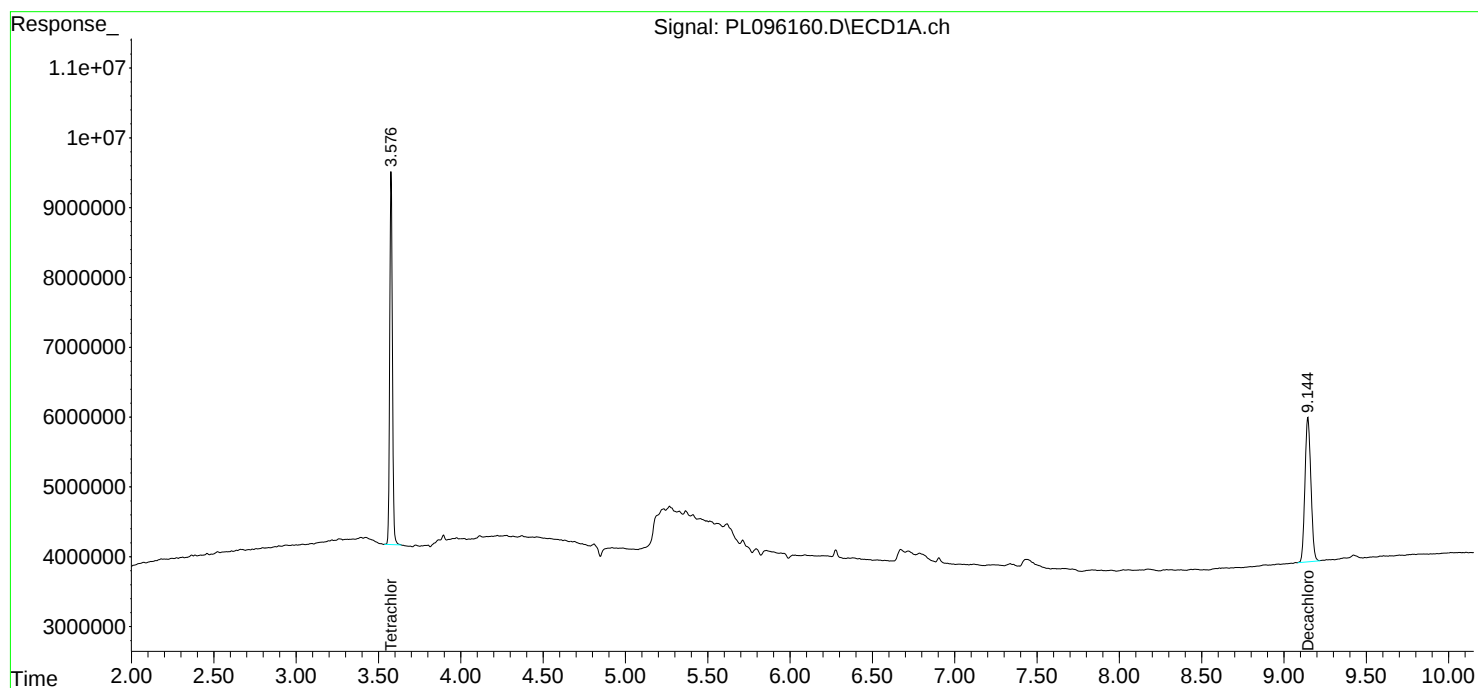

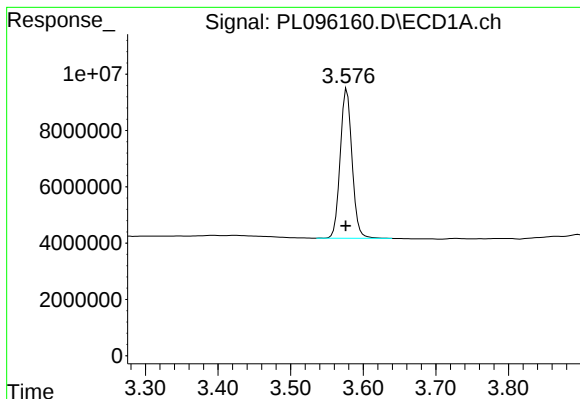


#1 Tetrachloro-m-xylene

R.T.: 3.577 min
Delta R.T.: 0.001 min
Response: 59892513
Conc: 17.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB168452BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/25/2025
Supervised By :mohammad ahmed 06/26/2025

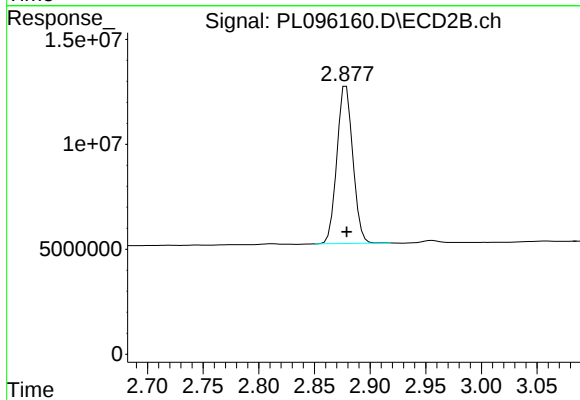


#1 Tetrachloro-m-xylene

R.T.: 2.879 min
Delta R.T.: 0.000 min
Response: 74935797
Conc: 17.08 ng/ml

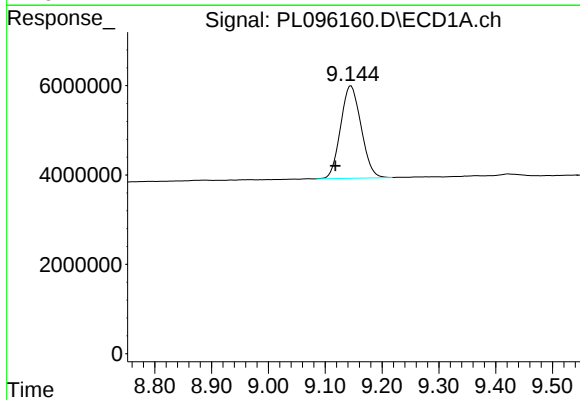

#28 Decachlorobiphenyl

R.T.: 9.144 min
Delta R.T.: 0.026 min
Response: 51958774
Conc: 19.49 ng/ml m

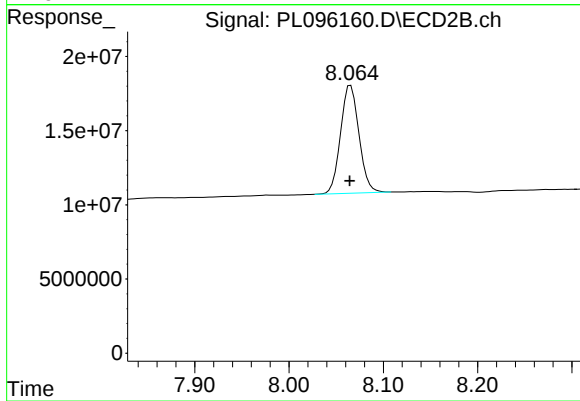

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 98751351
Conc: 18.35 ng/ml