

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
 Data File : PL037345.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2018 11:59
 Operator : UA\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 04:11:42 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	7.964f	0.000	1743756	0	0.289	N.D. #
Target Compounds							
2)	A alpha-BHC	3.718f	0.000	3995442	0	0.326	N.D. #
3)	MA gamma-BHC...	4.007f	0.000	2333827	0	0.226	N.D. #
4)	MA Heptachlor	4.360	0.000	2761134	0	0.270	N.D. #
5)	MB Aldrin	4.582	0.000	3494031	0	0.343	N.D. #
6)	B beta-BHC	4.267f	0.000	4127269	0	0.905	N.D. #
17)	MA 4,4'-DDT	6.211	0.000	8780785	0	1.360	N.D. #
18)	B Endrin al...	6.254	0.000	2221043	0	0.398	N.D. #
20)	A Methoxychlor	6.710f	0.000	4701598	0	1.383	N.D. #
21)	B Endrin ke...	6.929f	0.000	30656545	0	4.311	N.D. #
24)	Chlordane-2	4.611	0.000	1811368	0	5.088	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
Data File : PL037345.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2018 11:59
Operator : UA\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:11:42 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

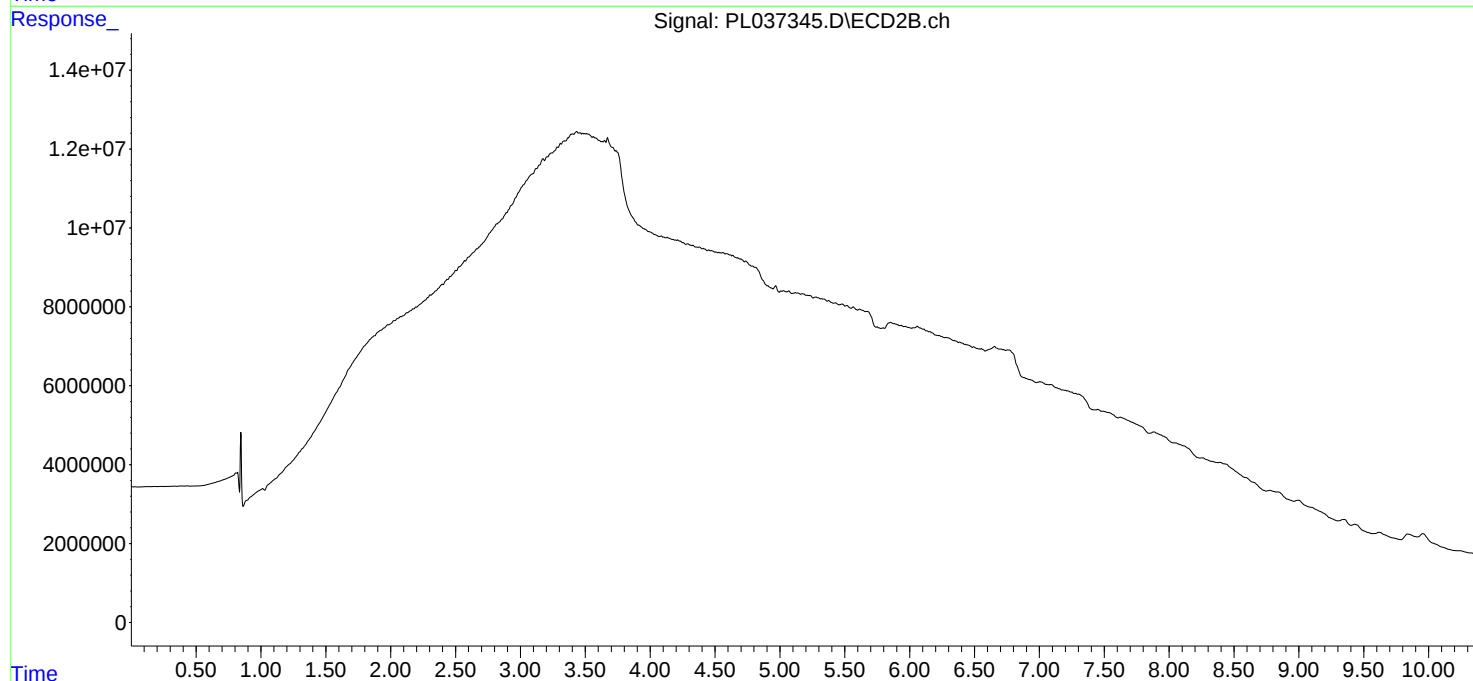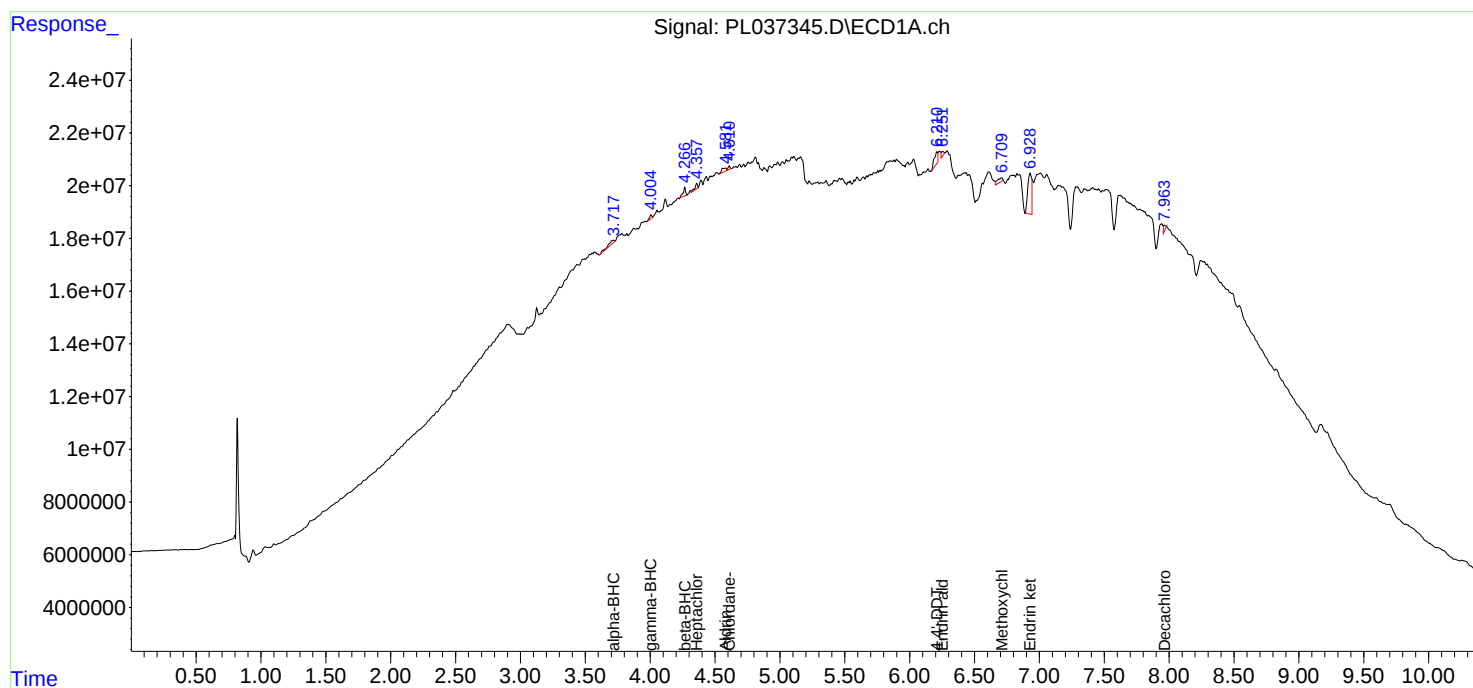


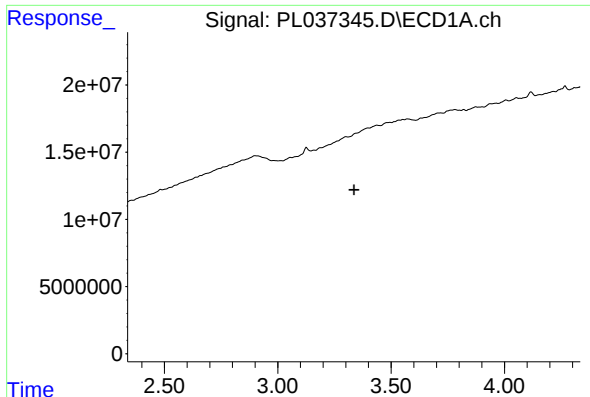

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

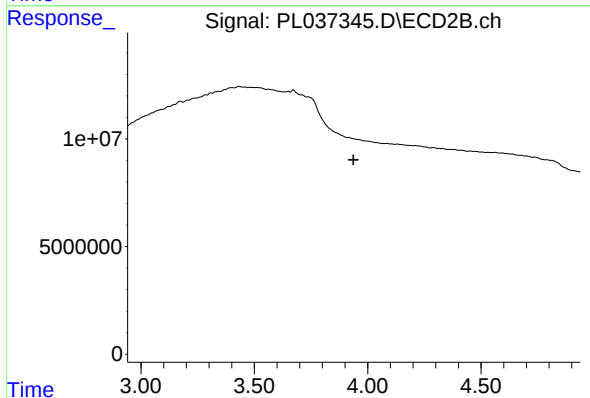


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.938 min
Response: 0
Conc: N.D.

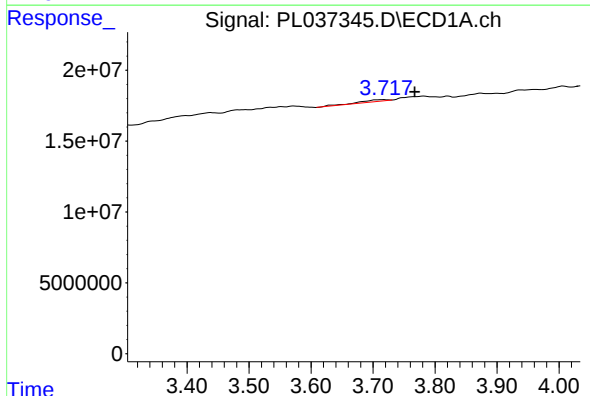


#2 alpha-BHC

R.T.: 3.718 min
Delta R.T.: -0.049 min
Response: 3995442
Conc: 0.33 ng/ml

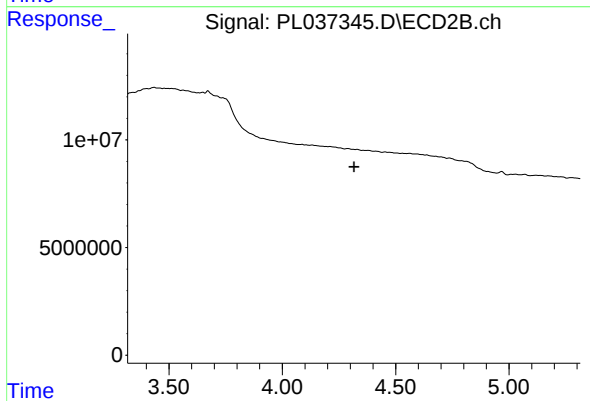

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

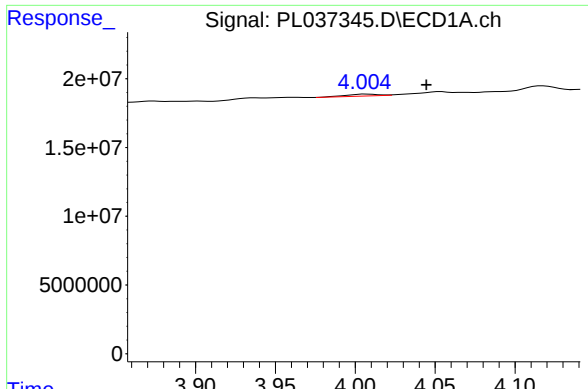

#3 gamma-BHC (Lindane)


R.T.: 4.007 min
Delta R.T.: -0.038 min
Response: 2333827
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

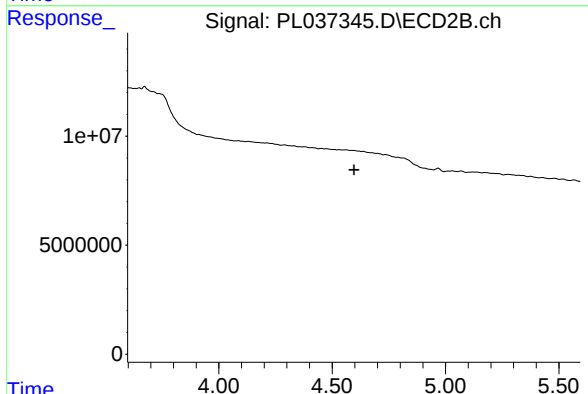


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.597 min
Response: 0
Conc: N.D.

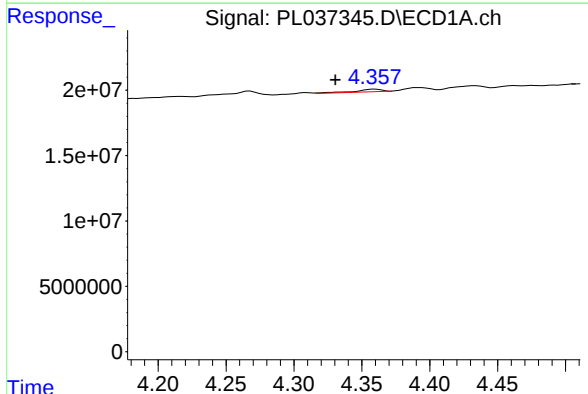


#4 Heptachlor

R.T.: 4.360 min
Delta R.T.: 0.029 min
Response: 2761134
Conc: 0.27 ng/ml

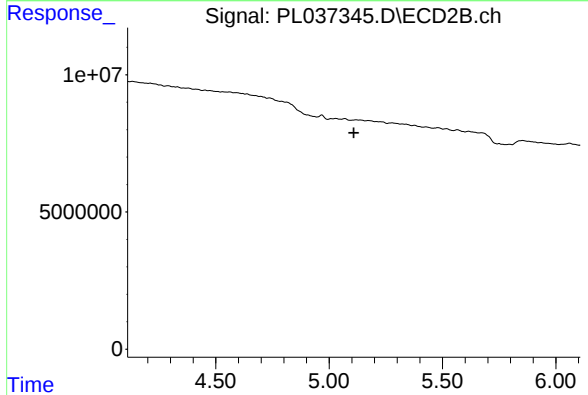

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.108 min
Response: 0
Conc: N.D.

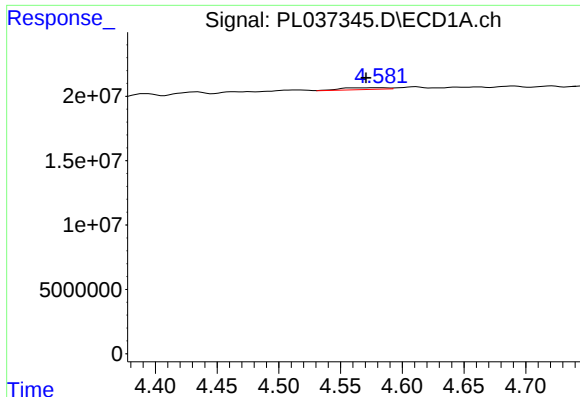

#5 Aldrin


R.T.: 4.582 min
Delta R.T.: 0.012 min
Response: 3494031
Conc: 0.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

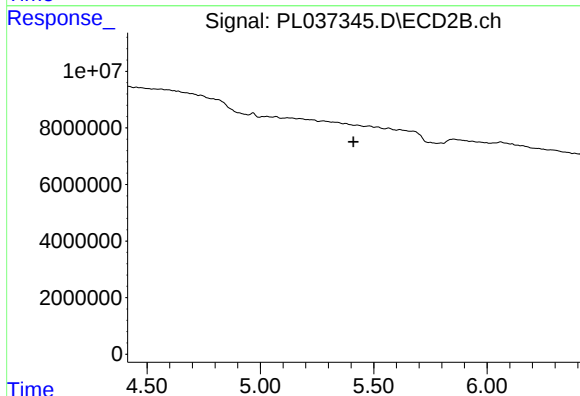


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.411 min
Response: 0
Conc: N.D.

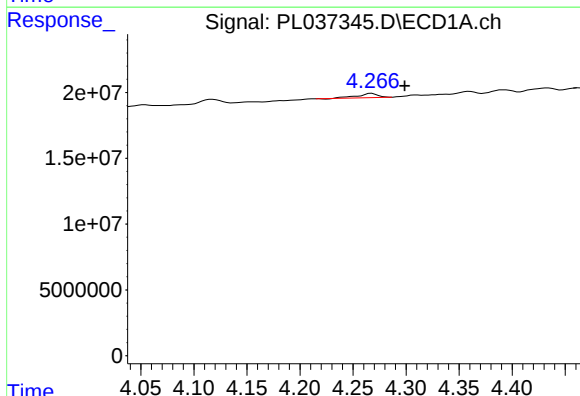


#6 beta-BHC

R.T.: 4.267 min
Delta R.T.: -0.031 min
Response: 4127269
Conc: 0.90 ng/ml

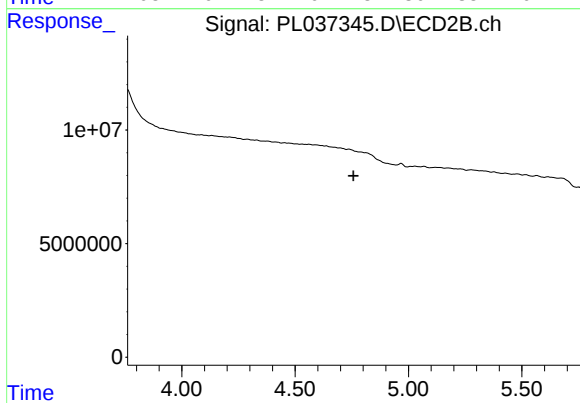

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

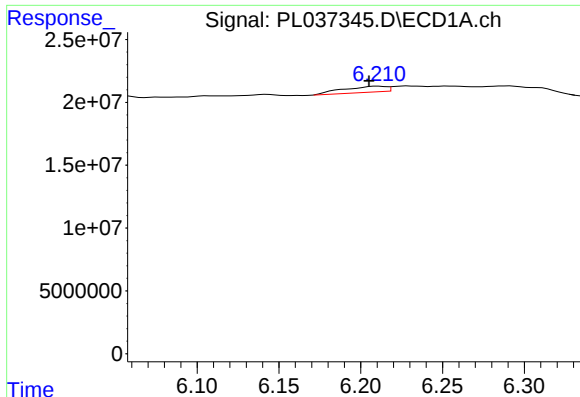

#17 4,4'-DDT


R.T.: 6.211 min
Delta R.T.: 0.006 min
Response: 8780785
Conc: 1.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

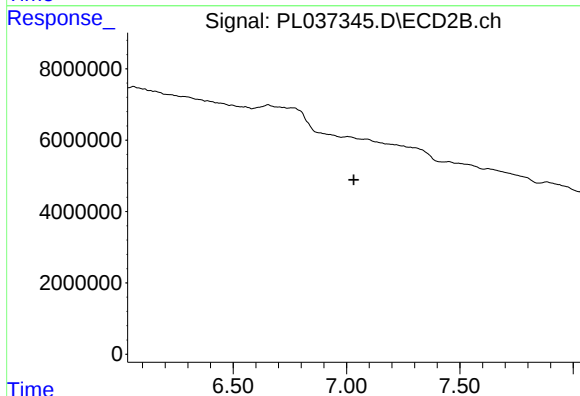


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.033 min
Response: 0
Conc: N.D.

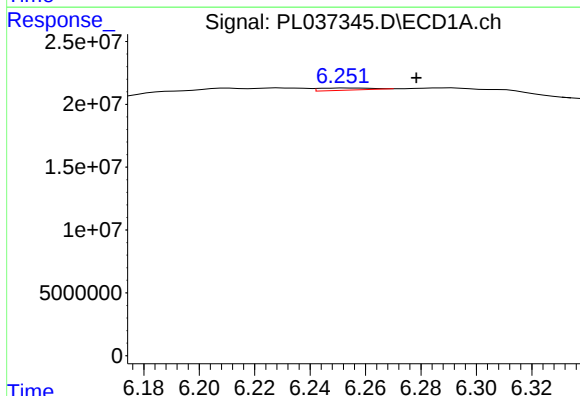


#18 Endrin aldehyde

R.T.: 6.254 min
Delta R.T.: -0.025 min
Response: 2221043
Conc: 0.40 ng/ml

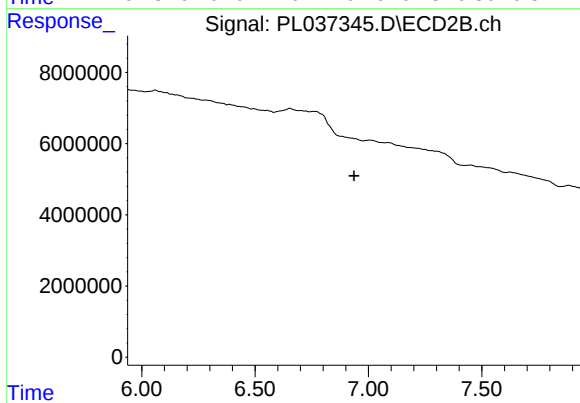

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.937 min
Response: 0
Conc: N.D.

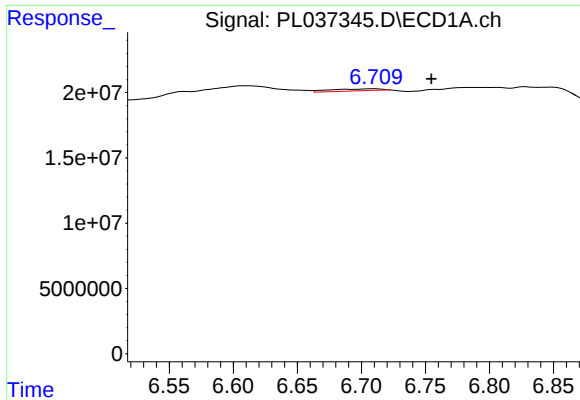

#20 Methoxychlor


R.T.: 6.710 min
Delta R.T.: -0.044 min
Response: 4701598
Conc: 1.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

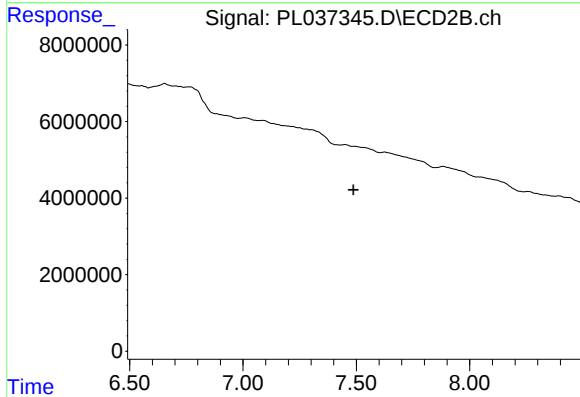


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.488 min
Response: 0
Conc: N.D.

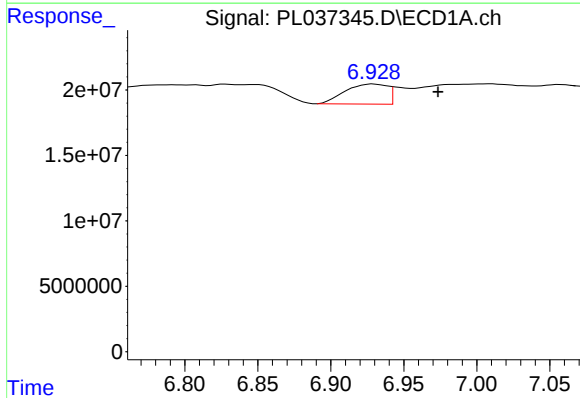


#21 Endrin ketone

R.T.: 6.929 min
Delta R.T.: -0.045 min
Response: 30656545
Conc: 4.31 ng/ml

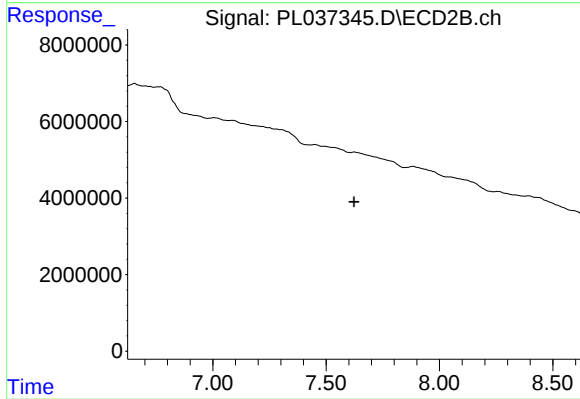

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.623 min
Response: 0
Conc: N.D.

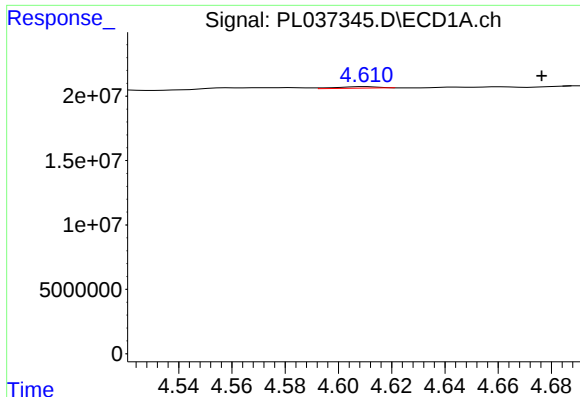

#24 Chlordane-2


R.T.: 4.611 min
Delta R.T.: -0.066 min
Response: 1811368
Conc: 5.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

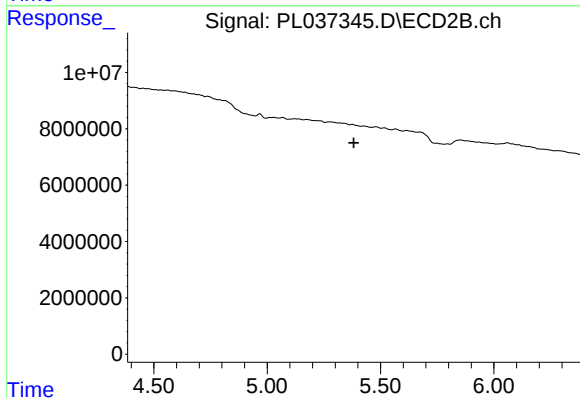


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.382 min
Response: 0
Conc: N.D.

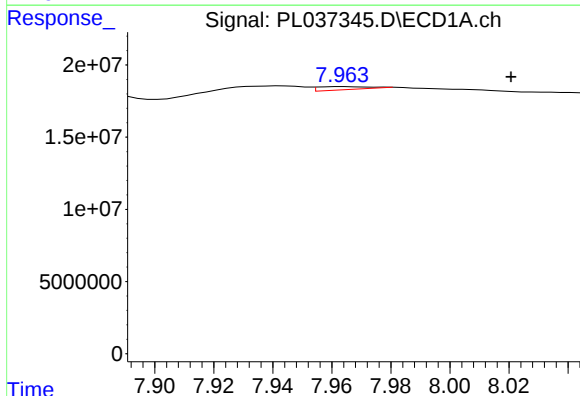

#28 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: -0.057 min
Response: 1743756
Conc: 0.29 ng/ml

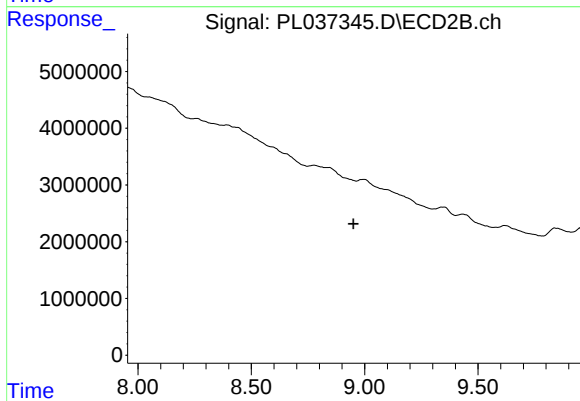

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.951 min
Response: 0
Conc: N.D.