

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
 Data File : PL037353.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2018 14:16
 Operator : UA\AJ
 Sample : J3241-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 04:14:33 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.936	77801703	21873444	9.835	7.906
28)	SA Decachlor...	8.018	8.947	47452868	17376465	7.864	8.759
Target Compounds							
2)	A alpha-BHC	3.781	0.000	2077359	0	0.170	N.D. #
6)	B beta-BHC	4.254f	0.000	16457026	0	3.608	N.D. #
10)	B gamma-Chl...	5.163f	0.000	17837053	0	1.904	N.D. #
16)	A 4,4'-DDD	5.963	0.000	9008908	0	1.372	N.D. #
23)	Chlordane-1	4.186	0.000	10971650	0	35.732	N.D. #
24)	Chlordane-2	4.708	0.000	13346781	0	37.491	N.D. #
25)	Chlordane-3	5.163	0.000	17837053	0	16.781	N.D. #
27)	Chlordane-5	5.963	0.000	9008908	0	68.840	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
Data File : PL037353.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2018 14:16
Operator : UA\AJ
Sample : J3241-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:14:33 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

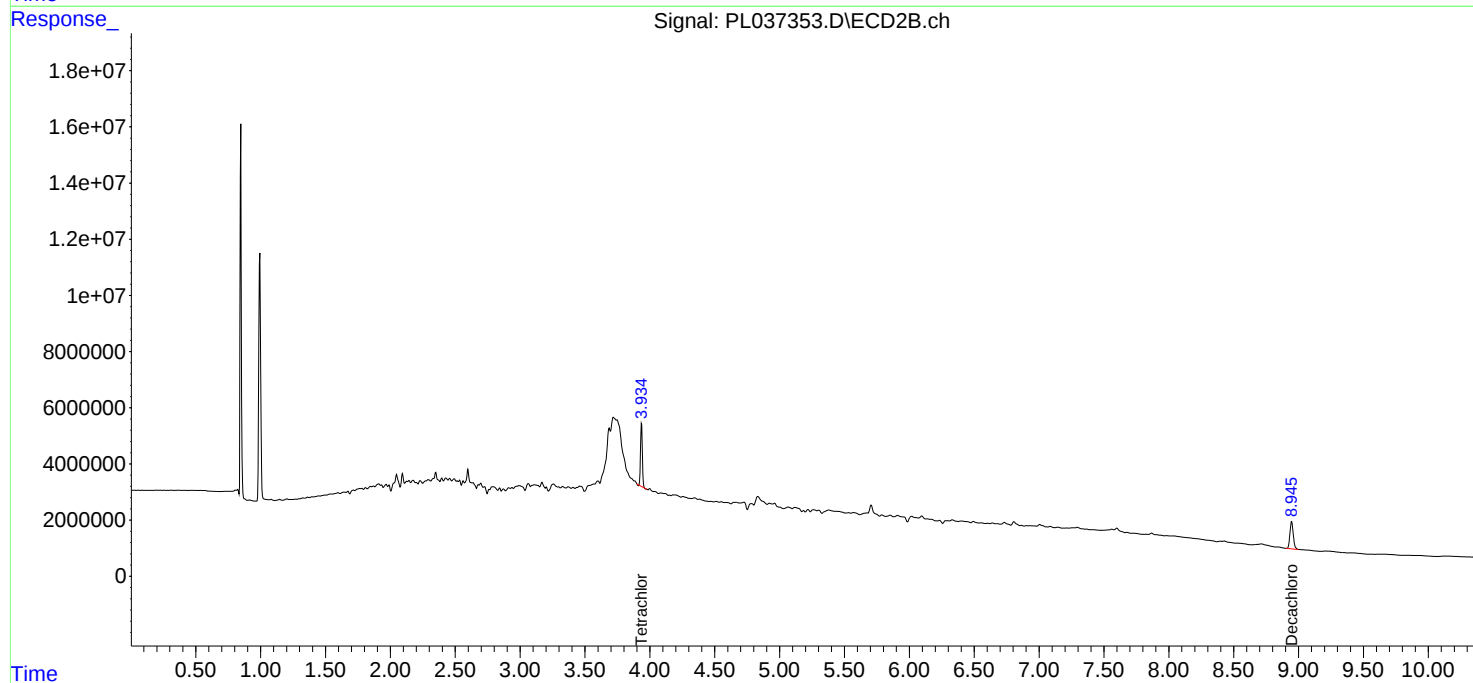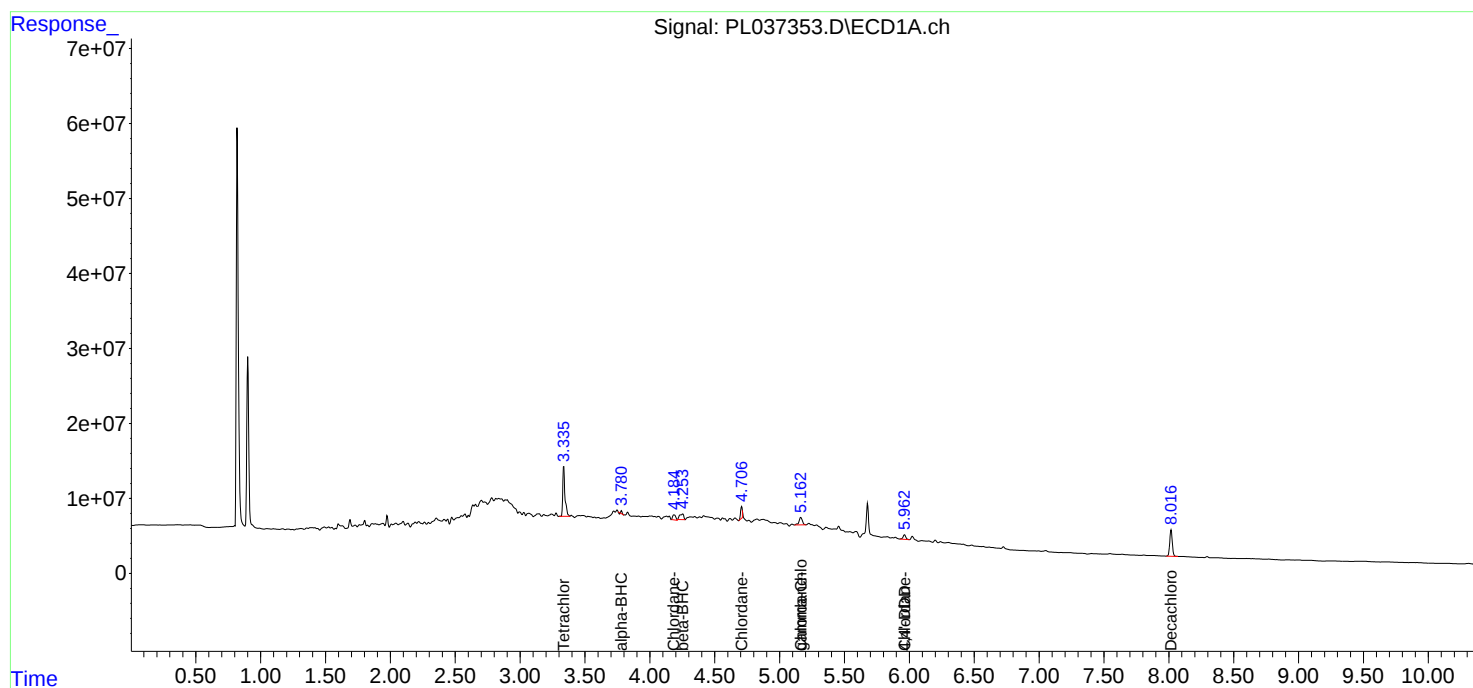


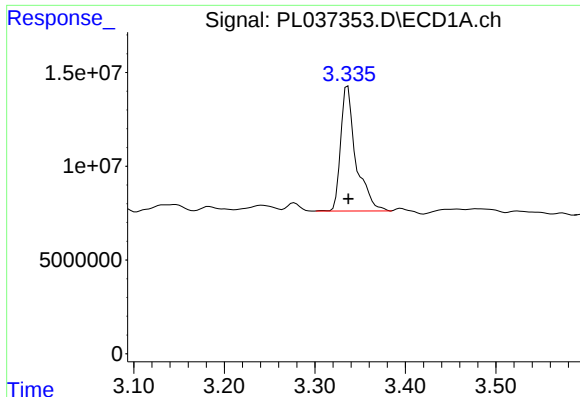

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 77801703
Conc: 9.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

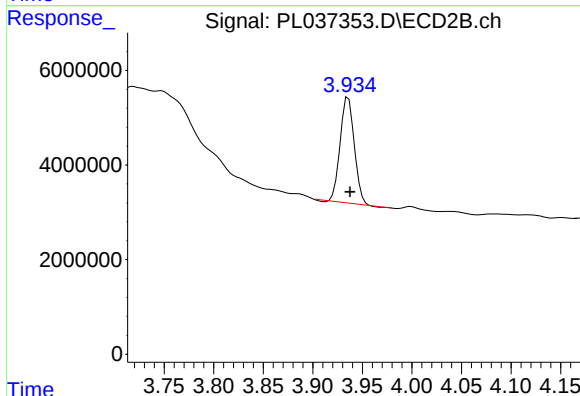


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 21873444
Conc: 7.91 ng/ml

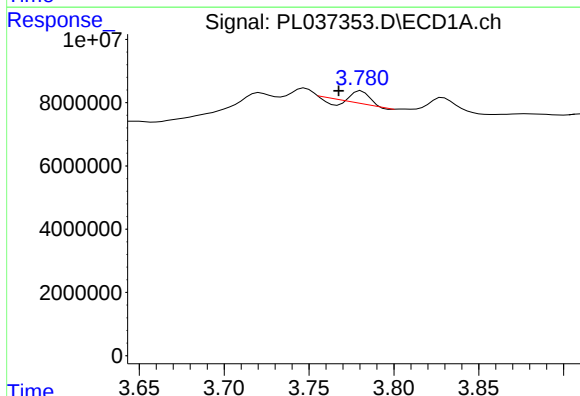


#2 alpha-BHC

R.T.: 3.781 min
Delta R.T.: 0.013 min
Response: 2077359
Conc: 0.17 ng/ml

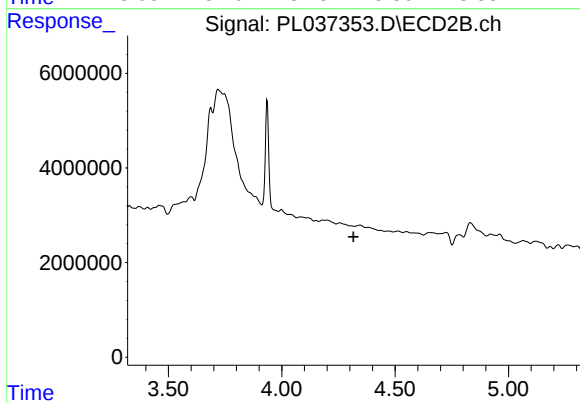

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

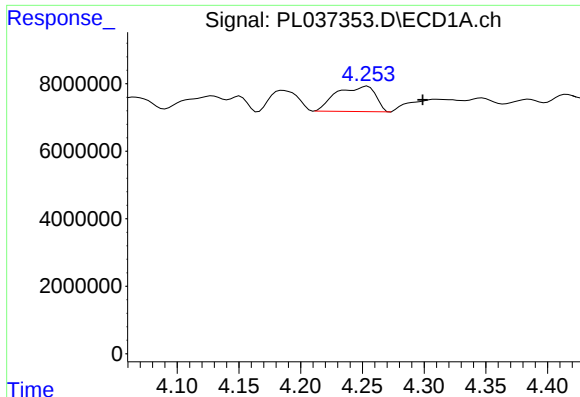

#6 beta-BHC


R.T.: 4.254 min
Delta R.T.: -0.045 min
Response: 16457026
Conc: 3.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

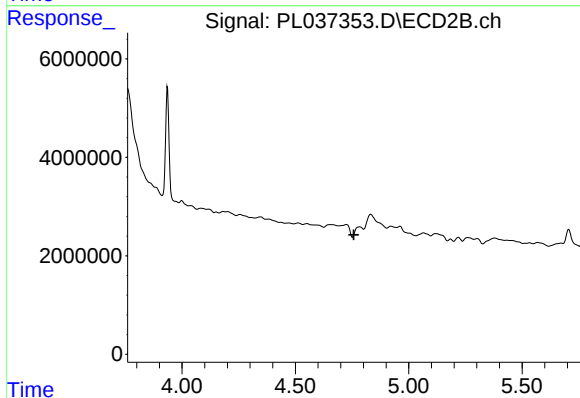


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

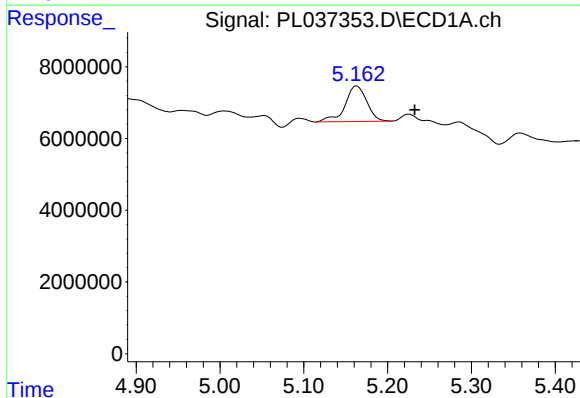


#10 gamma-Chlordane

R.T.: 5.163 min
Delta R.T.: -0.069 min
Response: 17837053
Conc: 1.90 ng/ml

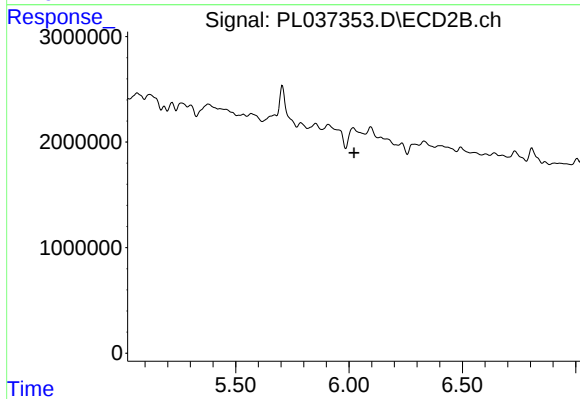

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

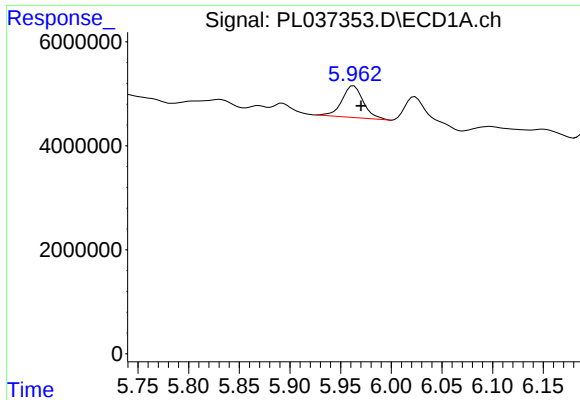

#16 4,4'-DDD


R.T.: 5.963 min
Delta R.T.: -0.007 min
Response: 9008908
Conc: 1.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

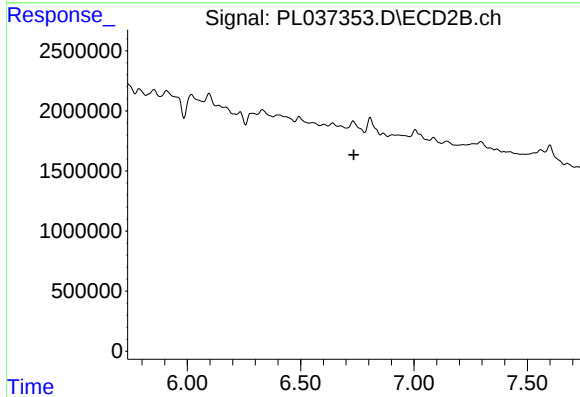


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.734 min
Response: 0
Conc: N.D.

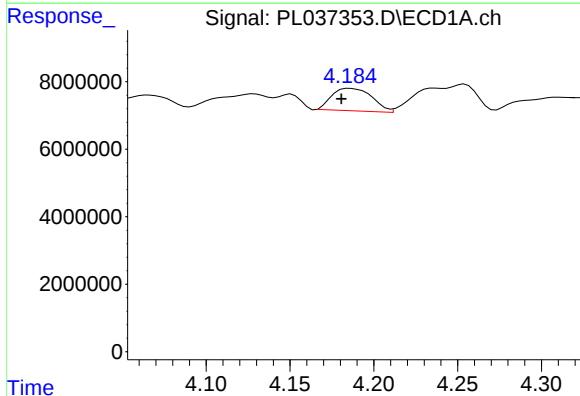


#23 Chlordane-1

R.T.: 4.186 min
Delta R.T.: 0.005 min
Response: 10971650
Conc: 35.73 ng/ml

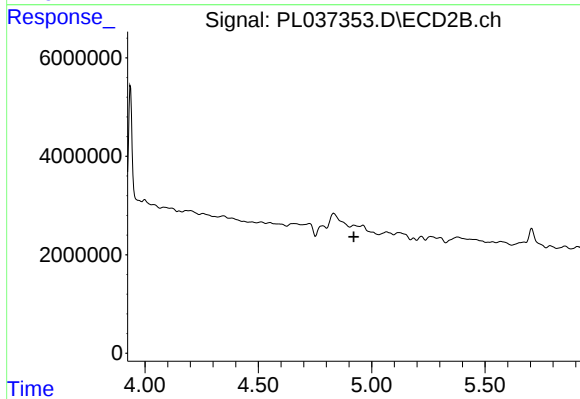

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

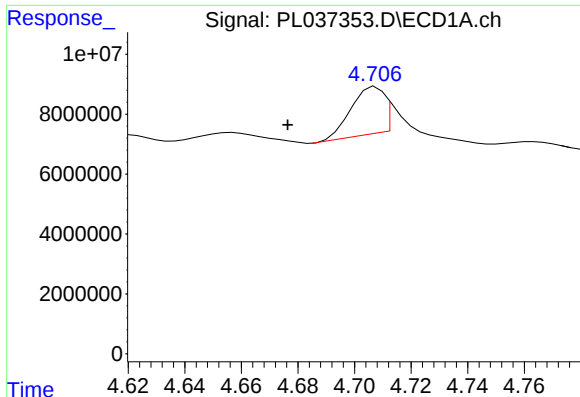

#24 Chlordane-2


R.T.: 4.708 min
Delta R.T.: 0.031 min
Response: 13346781
Conc: 37.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

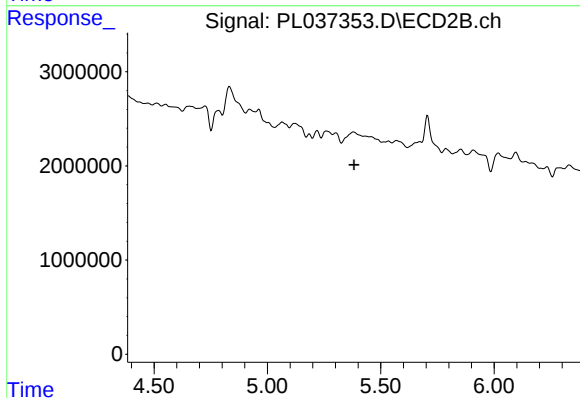


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.382 min
Response: 0
Conc: N.D.

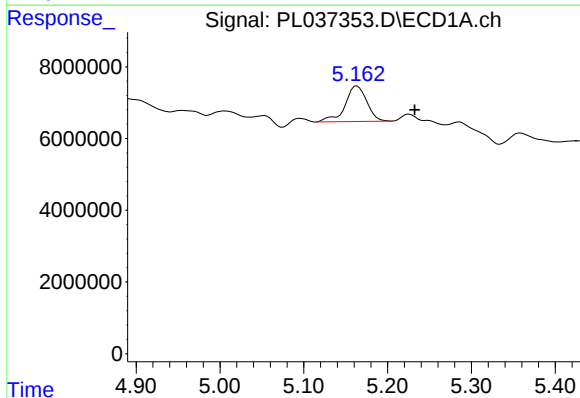


#25 Chlordane-3

R.T.: 5.163 min
Delta R.T.: -0.069 min
Response: 17837053
Conc: 16.78 ng/ml

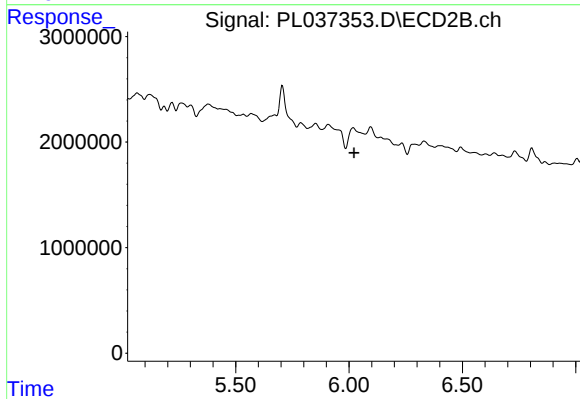

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

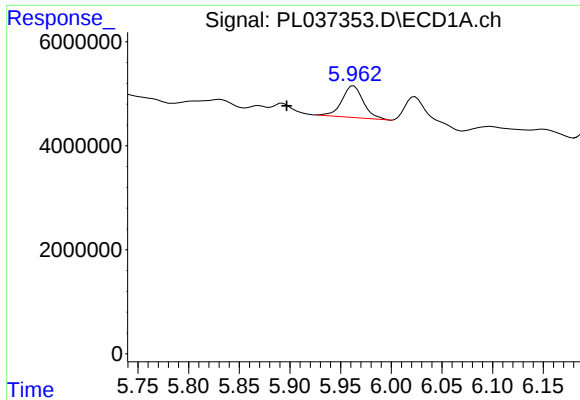

#27 Chlordane-5


R.T.: 5.963 min
Delta R.T.: 0.066 min
Response: 9008908
Conc: 68.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

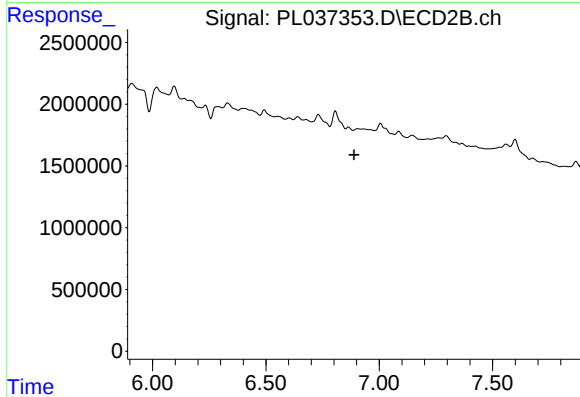


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.889 min
Response: 0
Conc: N.D.

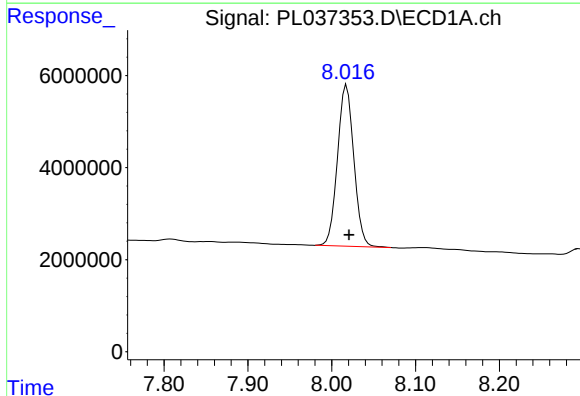

#28 Decachlorobiphenyl

R.T.: 8.018 min
Delta R.T.: -0.003 min
Response: 47452868
Conc: 7.86 ng/ml

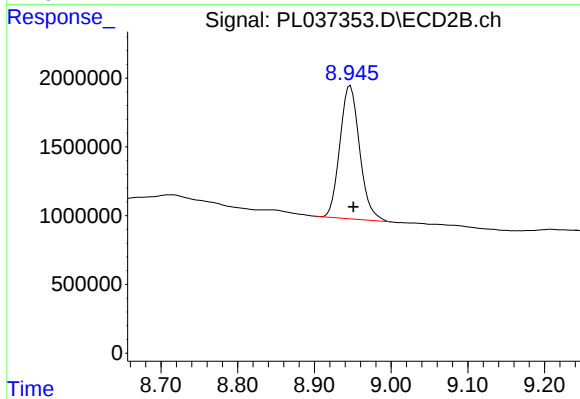

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 17376465
Conc: 8.76 ng/ml