

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
 Data File : PL037354.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2018 14:30
 Operator : UA\AJ
 Sample : J3241-17
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 04:15:06 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.936	74741766	23552504	9.449	8.513
28)	SA Decachlor...	8.018	8.948	47717260	17422862	7.908	8.782
Target Compounds							
6)	B beta-BHC	4.256f	0.000	16453241	0	3.607	N.D. #
10)	B gamma-Chl...	5.165f	0.000	13958849	0	1.490	N.D. #
23)	Chlordane-1	4.183	0.000	9059999	0	29.506	N.D. #
25)	Chlordane-3	5.165	0.000	13958849	0	13.133	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
Data File : PL037354.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2018 14:30
Operator : UA\AJ
Sample : J3241-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:15:06 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

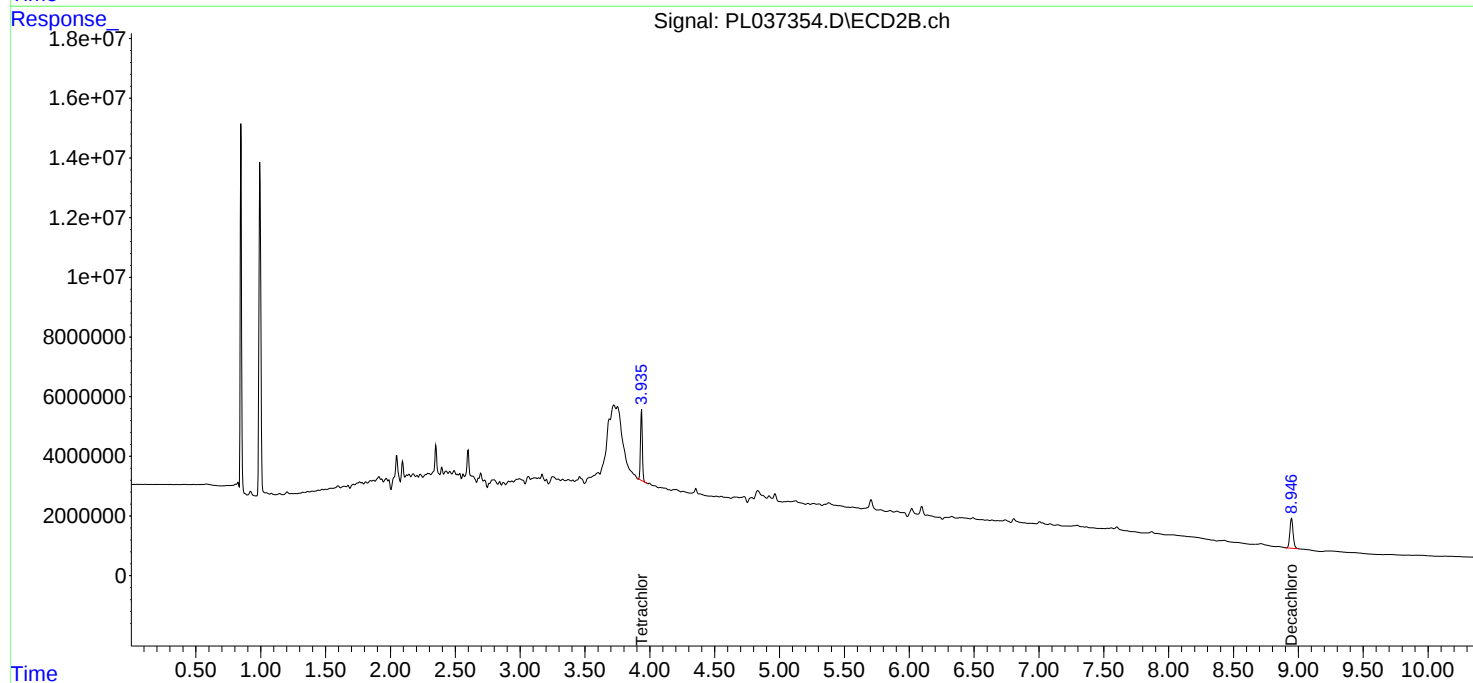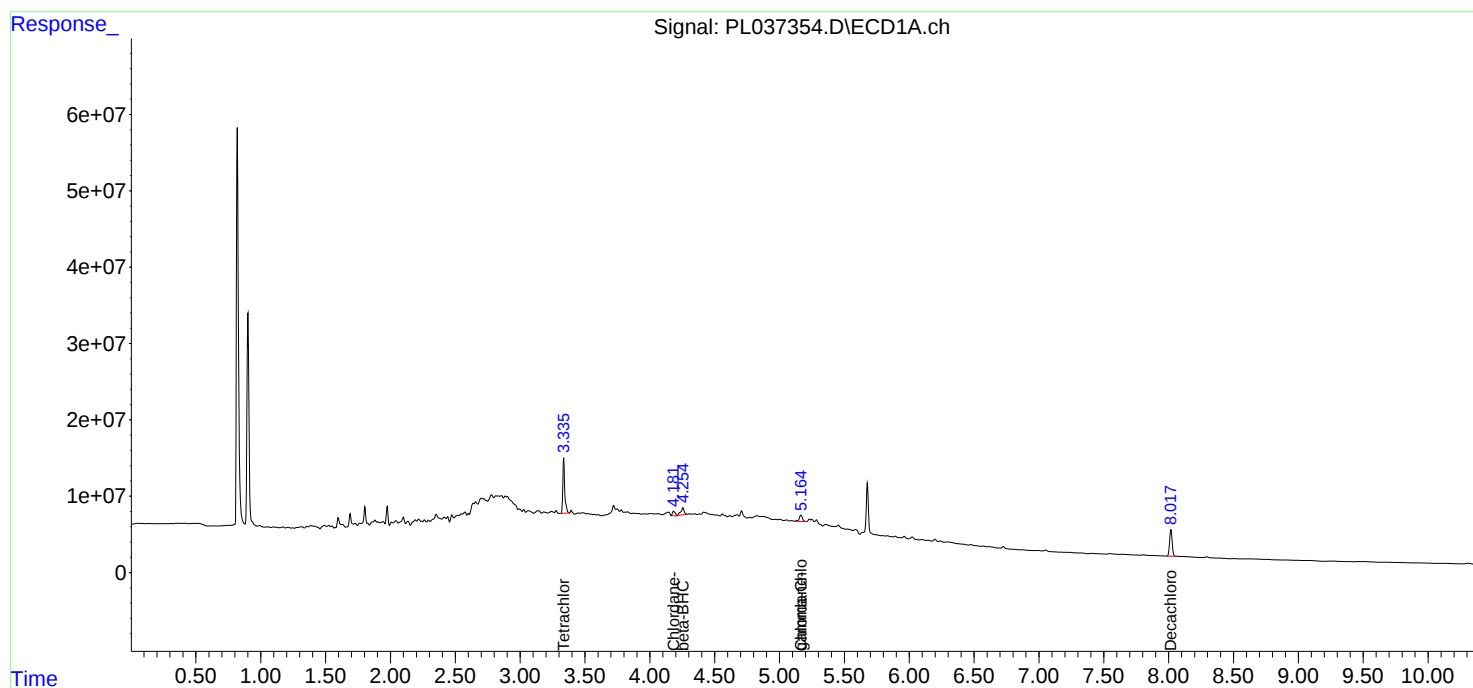


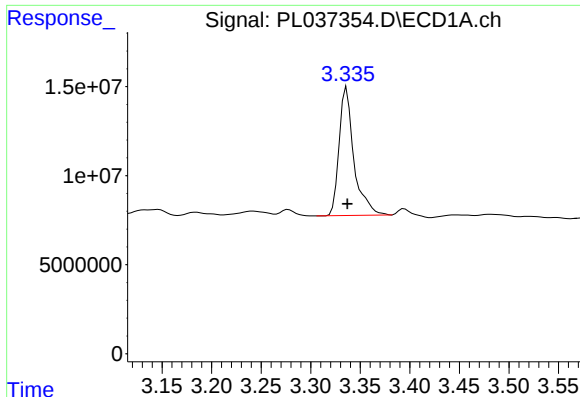

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 74741766
Conc: 9.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

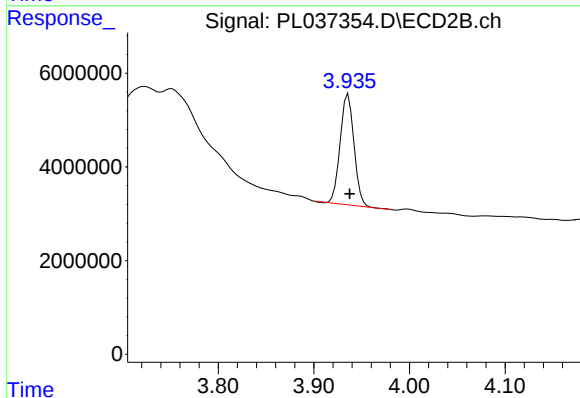


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 23552504
Conc: 8.51 ng/ml

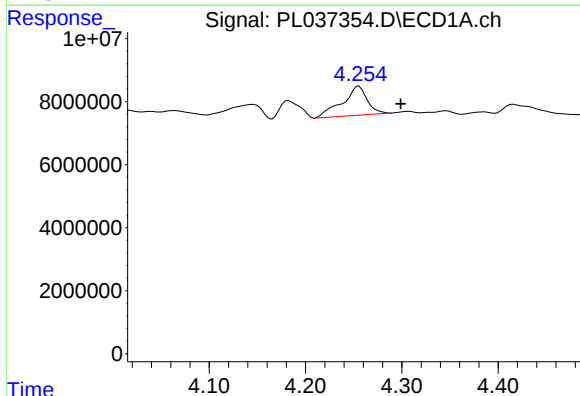


#6 beta-BHC

R.T.: 4.256 min
Delta R.T.: -0.043 min
Response: 16453241
Conc: 3.61 ng/ml

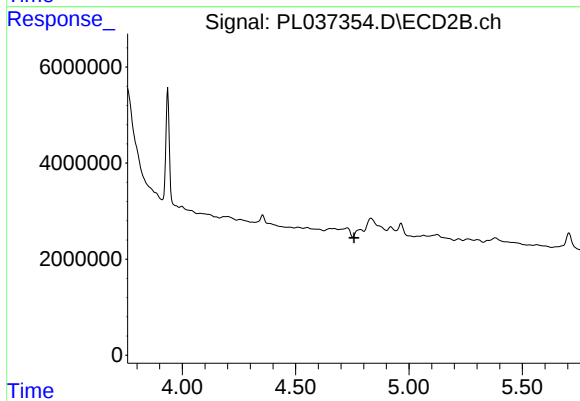

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

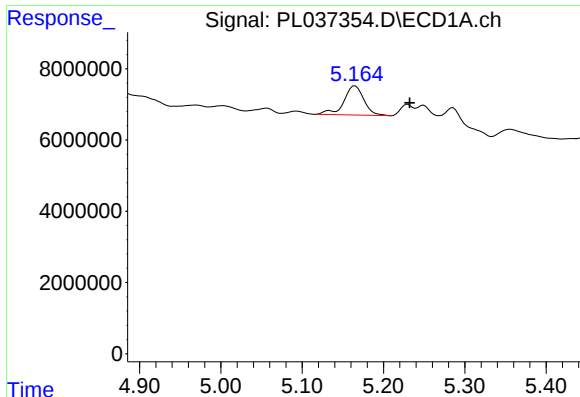

#10 gamma-Chlordane


R.T.: 5.165 min
Delta R.T.: -0.067 min
Response: 13958849
Conc: 1.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

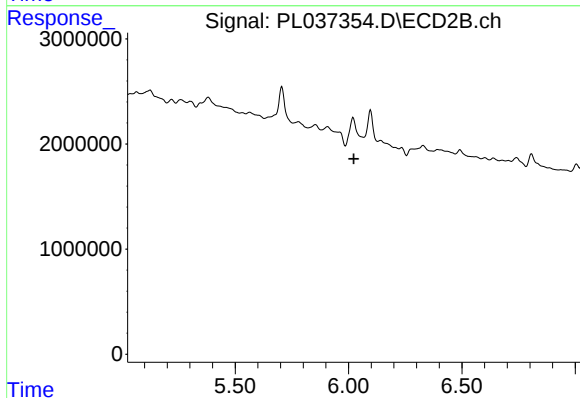


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

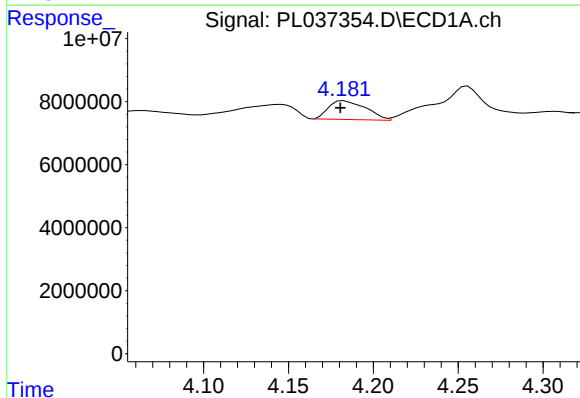


#23 Chlordane-1

R.T.: 4.183 min
Delta R.T.: 0.002 min
Response: 9059999
Conc: 29.51 ng/ml

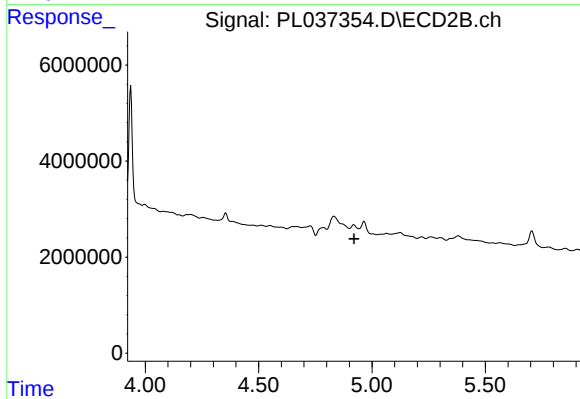

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

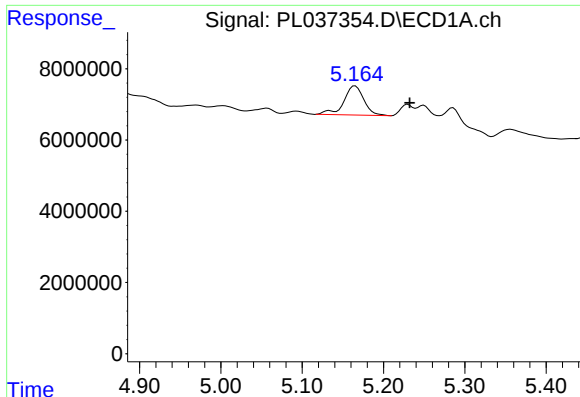

#25 Chlordane-3


R.T.: 5.165 min
Delta R.T.: -0.067 min
Response: 13958849
Conc: 13.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

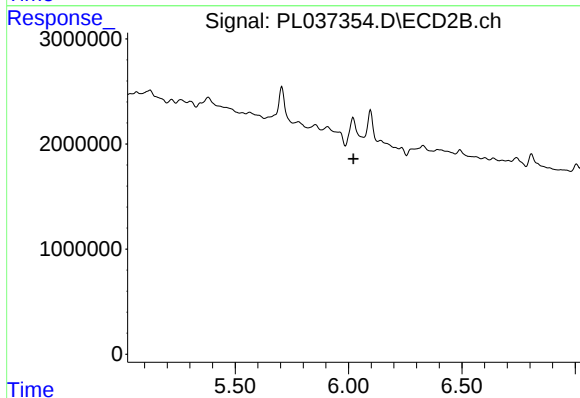


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

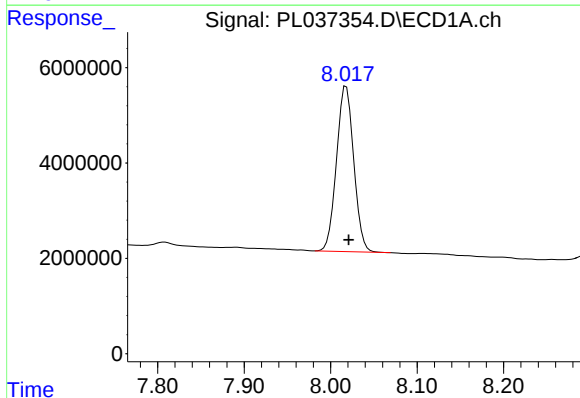

#28 Decachlorobiphenyl

R.T.: 8.018 min
Delta R.T.: -0.003 min
Response: 47717260
Conc: 7.91 ng/ml

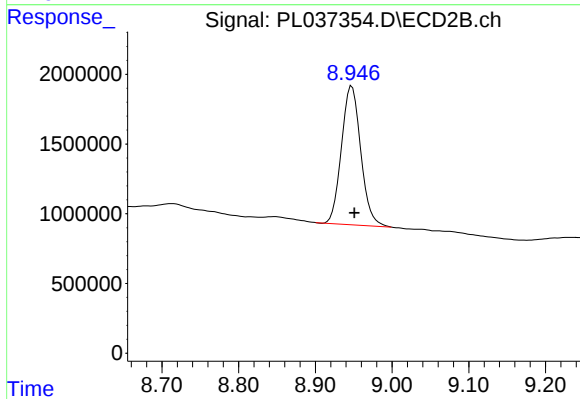

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 17422862
Conc: 8.78 ng/ml