

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
 Data File : PL037360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2018 15:55
 Operator : UA\AJ
 Sample : J3629-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 04:16:28 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	76953096	28398305	9.728	10.264
28)	SA Decachlor...	8.017	8.948	50213157	17437688	8.322	8.789
Target Compounds							
2)	A alpha-BHC	3.721f	0.000	9727850	0	0.795	N.D. #
6)	B beta-BHC	4.255f	0.000	8980573	0	1.969	N.D. #
10)	B gamma-Chl...	5.164f	0.000	14623211	0	1.561	N.D. #
23)	Chlordane-1	4.131	0.000	9997441	0	32.559	N.D. #
25)	Chlordane-3	5.164	0.000	14623211	0	13.758	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
Data File : PL037360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2018 15:55
Operator : UA\AJ
Sample : J3629-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:16:28 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

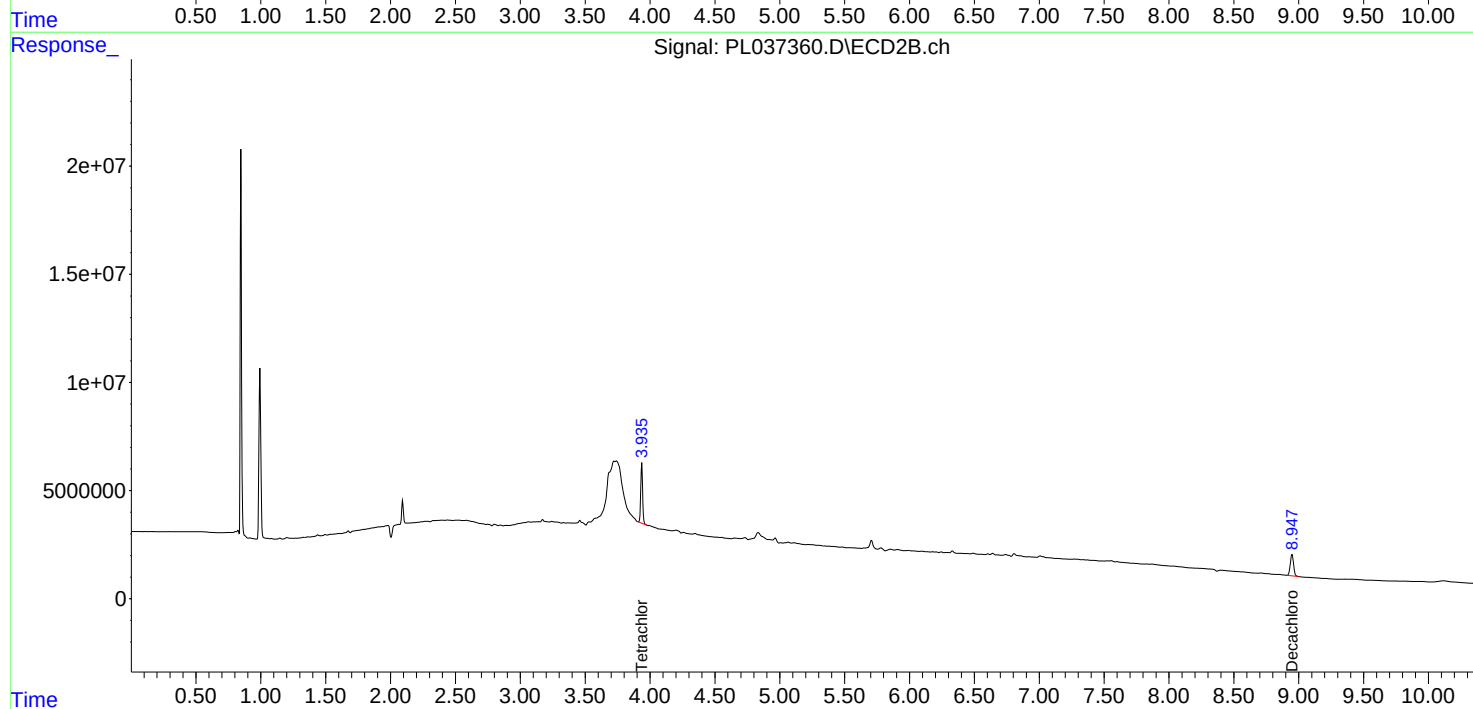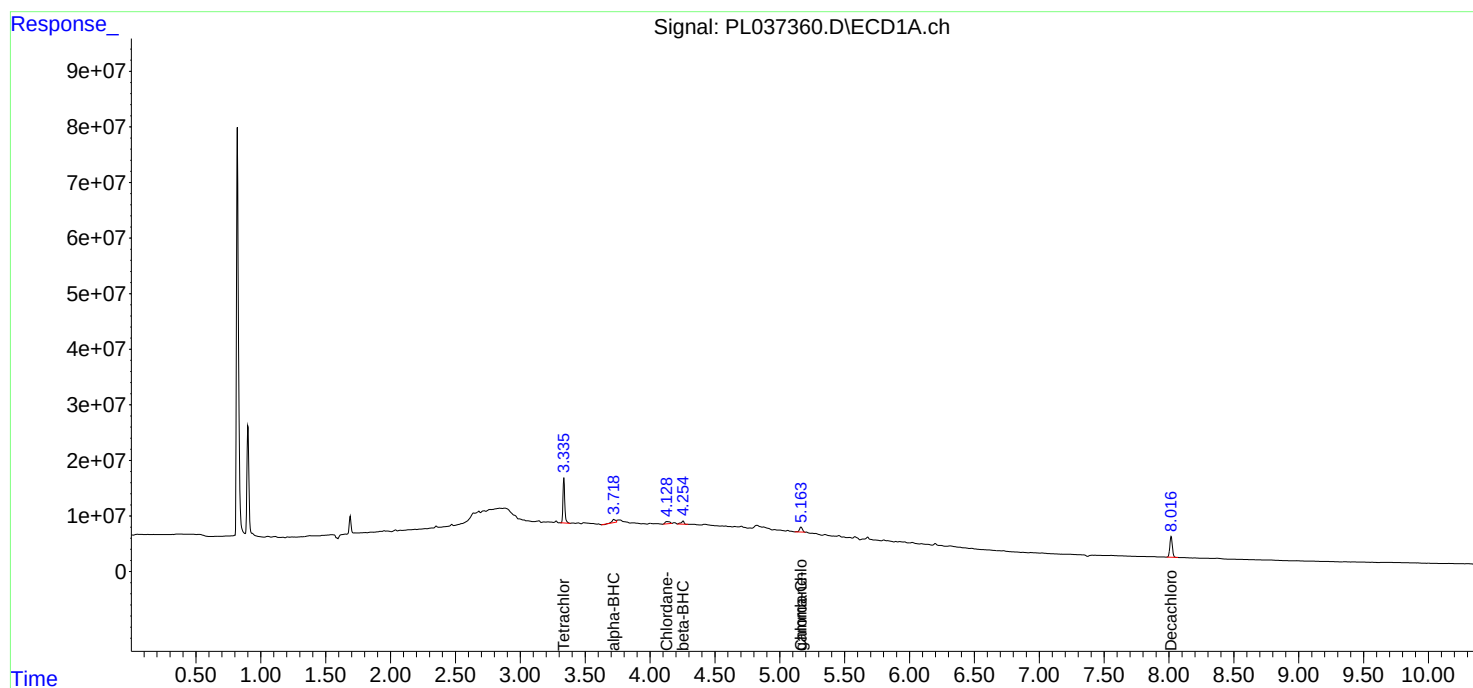


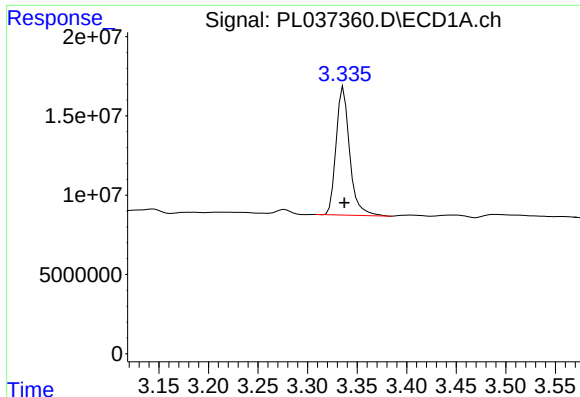

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 76953096
Conc: 9.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

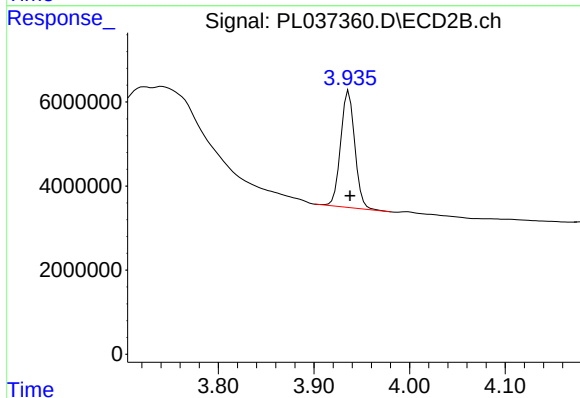


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.001 min
Response: 28398305
Conc: 10.26 ng/ml

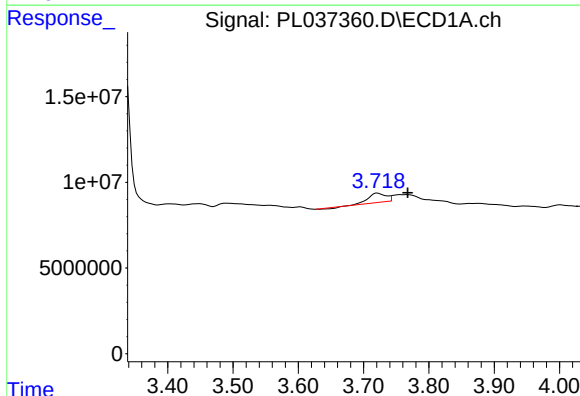


#2 alpha-BHC

R.T.: 3.721 min
Delta R.T.: -0.047 min
Response: 9727850
Conc: 0.79 ng/ml

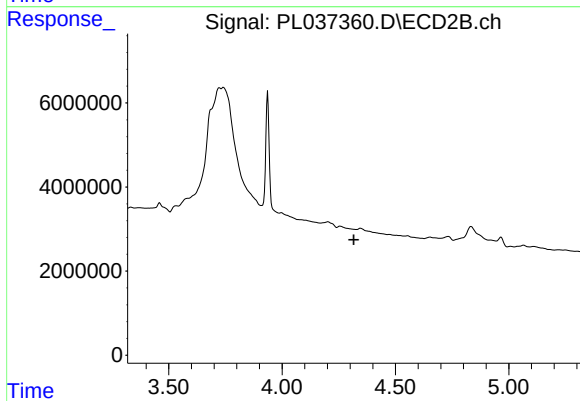

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

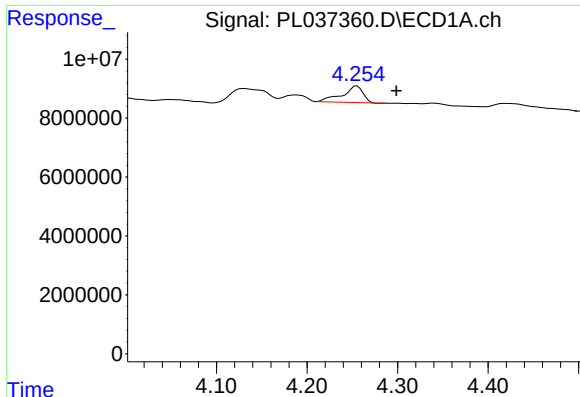

#6 beta-BHC


R.T.: 4.255 min
Delta R.T.: -0.044 min
Response: 8980573
Conc: 1.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

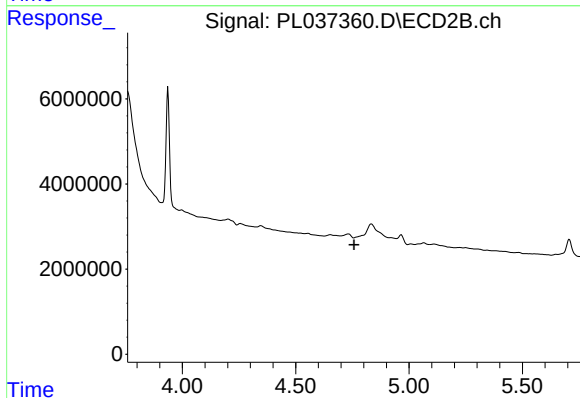


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

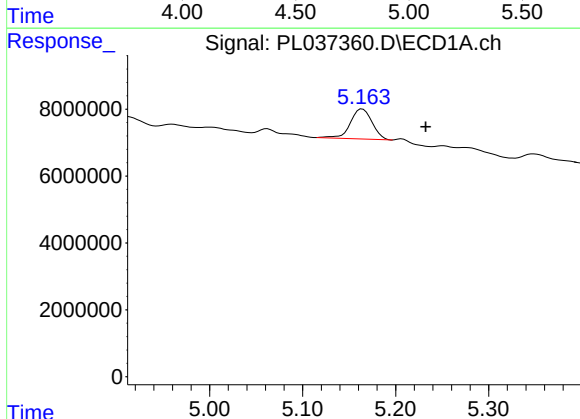


#10 gamma-Chlordane

R.T.: 5.164 min
Delta R.T.: -0.068 min
Response: 14623211
Conc: 1.56 ng/ml

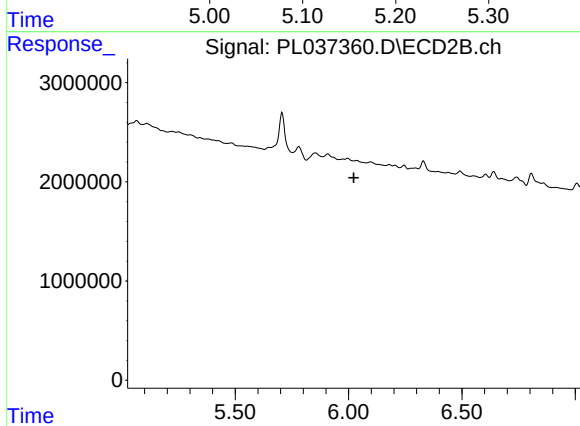

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

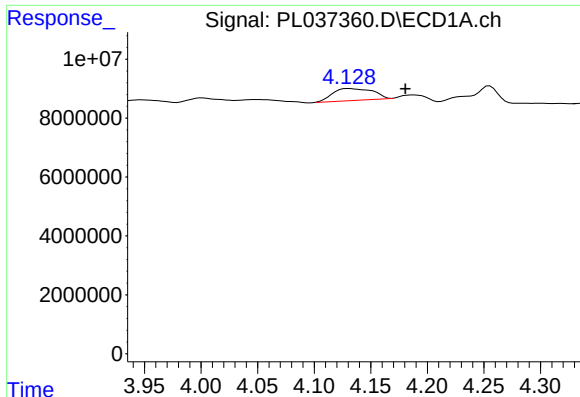

#23 Chlordane-1


R.T.: 4.131 min
Delta R.T.: -0.050 min
Response: 9997441
Conc: 32.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

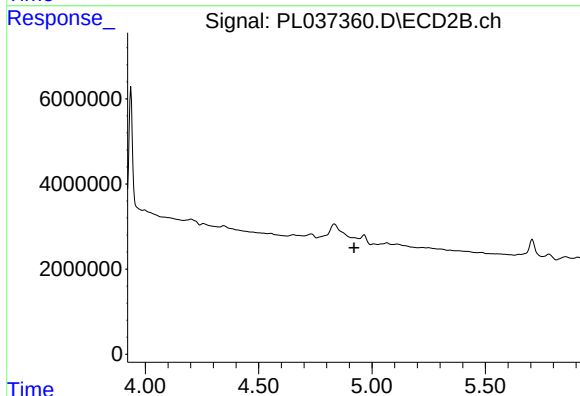


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

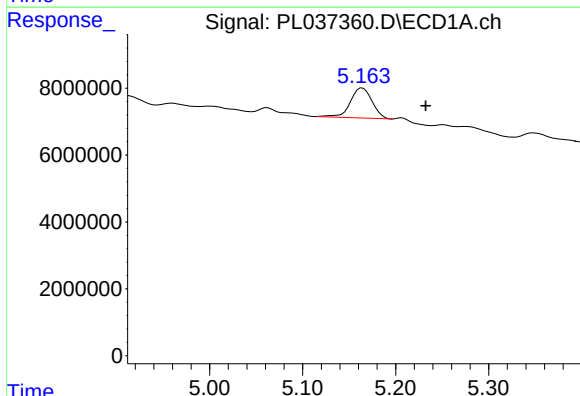


#25 Chlordane-3

R.T.: 5.164 min
Delta R.T.: -0.068 min
Response: 14623211
Conc: 13.76 ng/ml

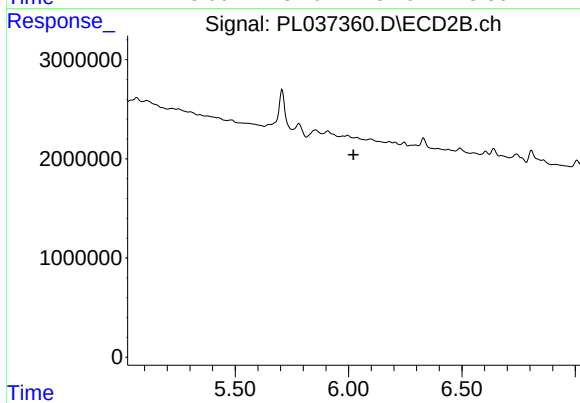

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

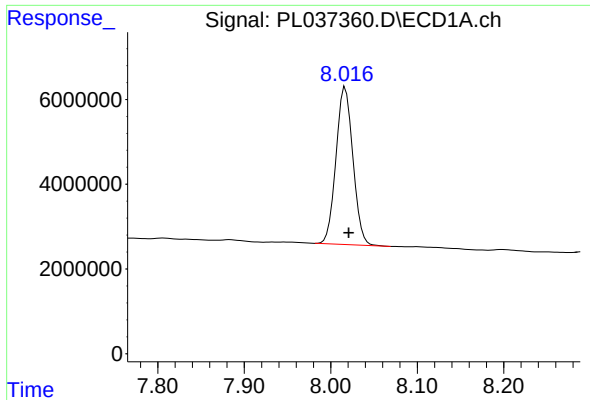

#28 Decachlorobiphenyl

R.T.: 8.017 min
Delta R.T.: -0.004 min
Response: 50213157
Conc: 8.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

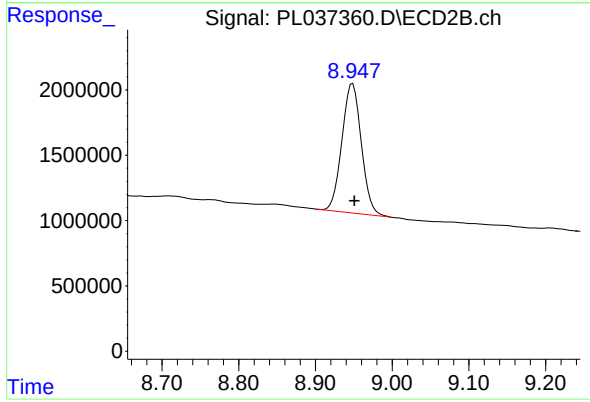

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.002 min
Response: 17437688
Conc: 8.79 ng/ml