

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
 Data File : PL037361.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2018 16:09
 Operator : UA\AJ
 Sample : J3629-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 04:16:39 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.936	136.1E6	50173353	17.208	18.135
28)	SA Decachlor...	8.017	8.948	73635971	25448192	12.203	12.827
Target Compounds							
2)	A alpha-BHC	3.722f	0.000	2627578	0	0.215	N.D. #
4)	MA Heptachlor	4.261f	0.000	8468720	0	0.827	N.D. #
6)	B beta-BHC	4.261f	0.000	8468720	0	1.857	N.D. #
10)	B gamma-Chl...	5.165f	0.000	11879902	0	1.268	N.D. #
12)	B 4,4'-DDE	5.456	0.000	14826942	0	1.679	N.D. #
16)	A 4,4'-DDD	5.909f	0.000	1330106	0	0.203	N.D. #
17)	MA 4,4'-DDT	6.202	7.030	18582408	6217924	2.878	2.936
23)	Chlordane-1	4.113	0.000	23535591	0	76.650	N.D. #
25)	Chlordane-3	5.165	0.000	11879902	0	11.177	N.D. #
27)	Chlordane-5	5.909	0.000	1330106	0	10.164	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
Data File : PL037361.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2018 16:09
Operator : UA\AJ
Sample : J3629-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:16:39 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

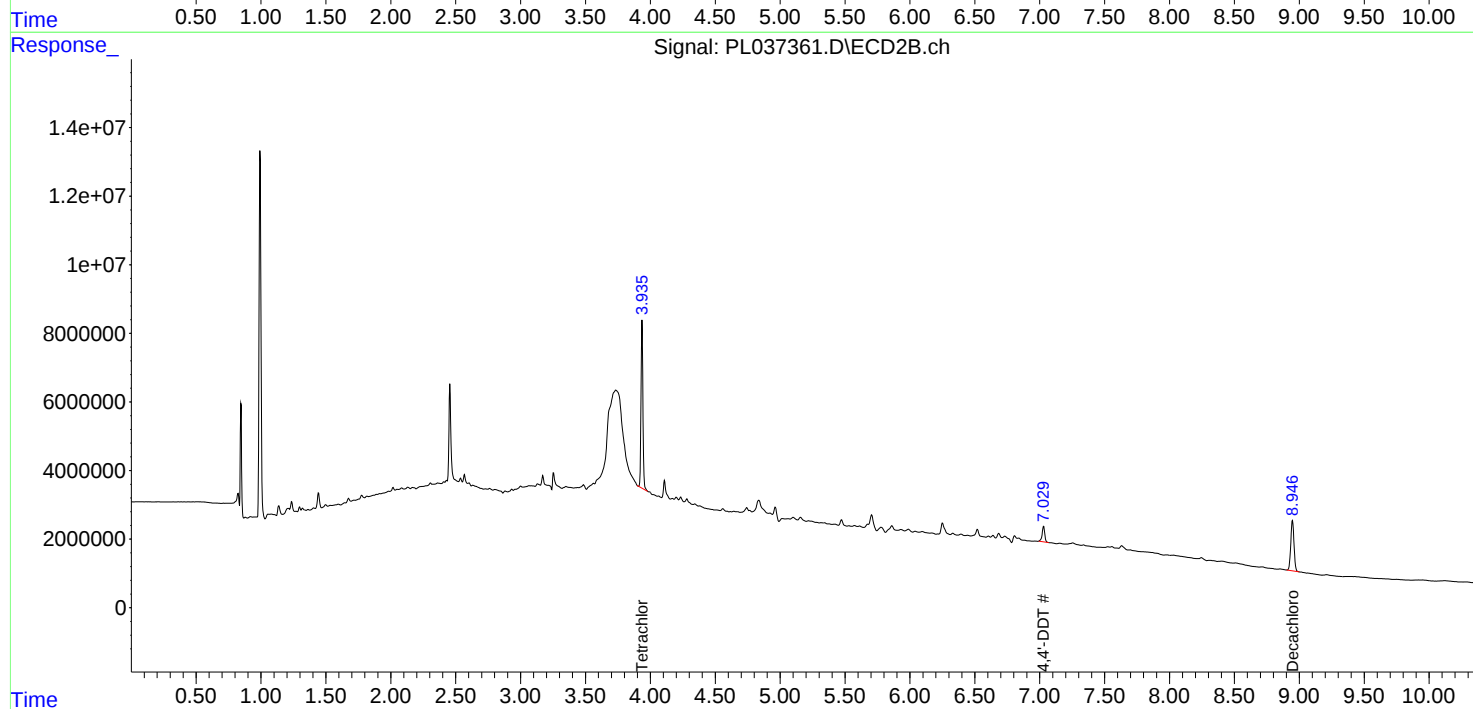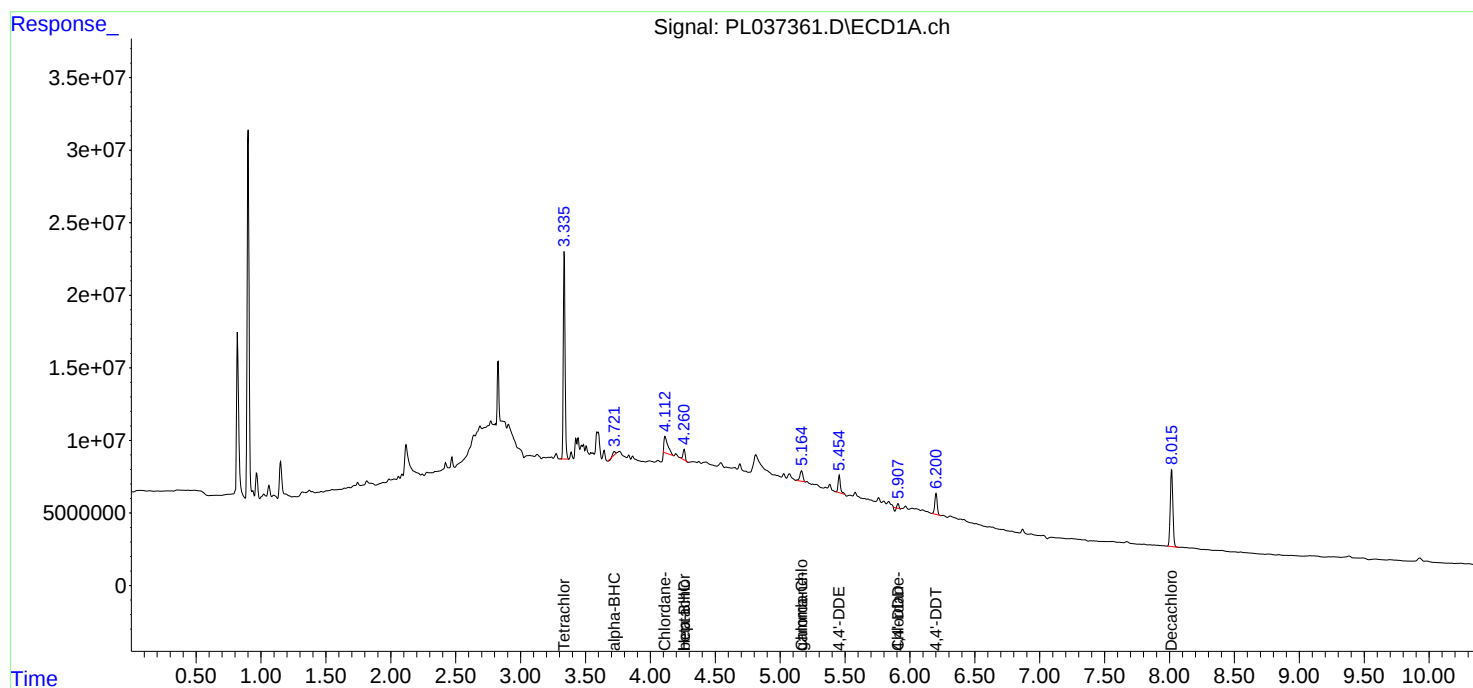


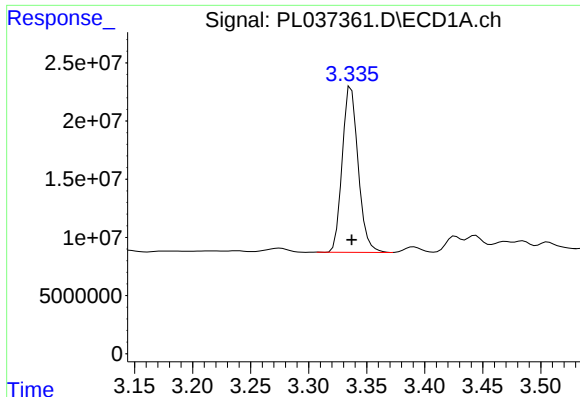

#1 Tetrachloro-m-xylene


R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 136123148
Conc: 17.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

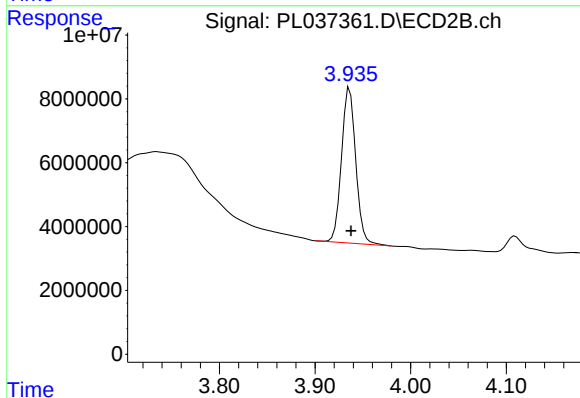


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.001 min
Response: 50173353
Conc: 18.13 ng/ml

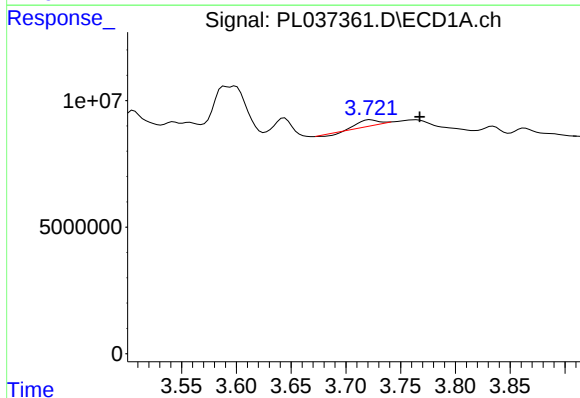


#2 alpha-BHC

R.T.: 3.722 min
Delta R.T.: -0.045 min
Response: 2627578
Conc: 0.21 ng/ml

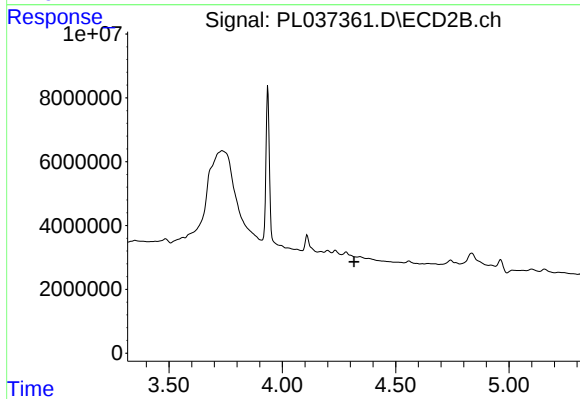

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

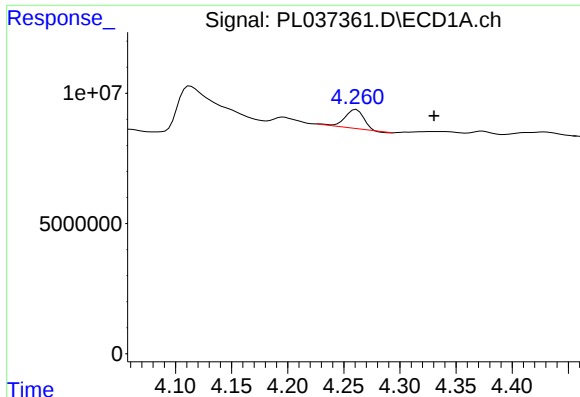

#4 Heptachlor


R.T.: 4.261 min
Delta R.T.: -0.069 min
Response: 8468720
Conc: 0.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

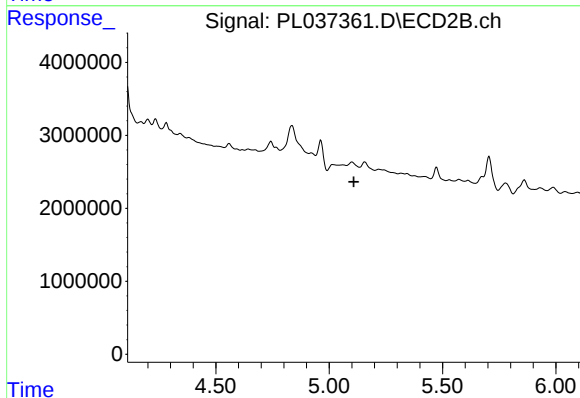


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.108 min
Response: 0
Conc: N.D.

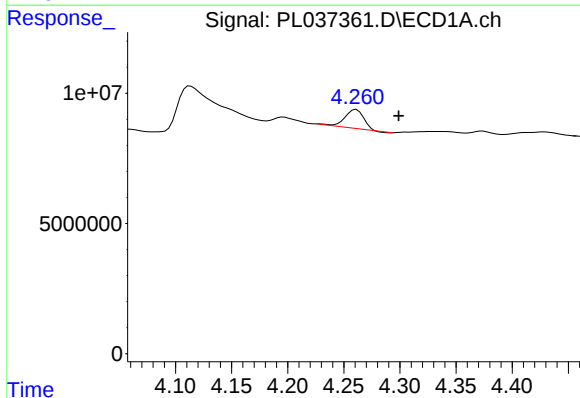


#6 beta-BHC

R.T.: 4.261 min
Delta R.T.: -0.038 min
Response: 8468720
Conc: 1.86 ng/ml

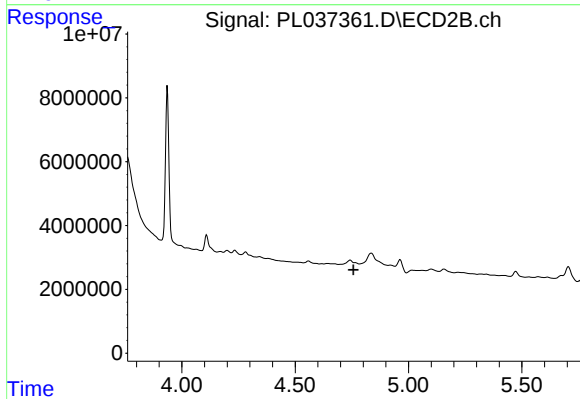

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

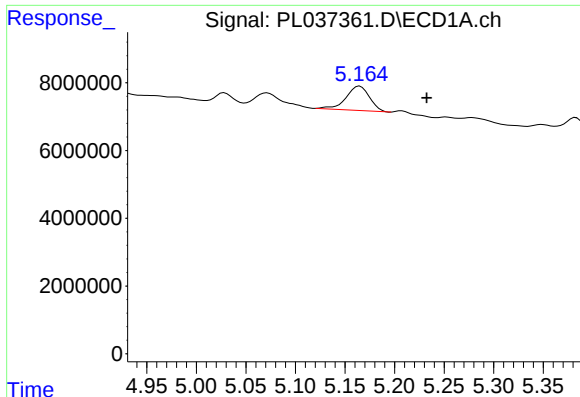

#10 gamma-Chlordane


R.T.: 5.165 min
Delta R.T.: -0.068 min
Response: 11879902
Conc: 1.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

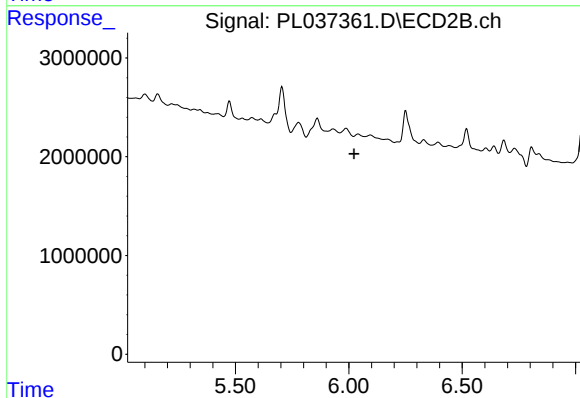


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

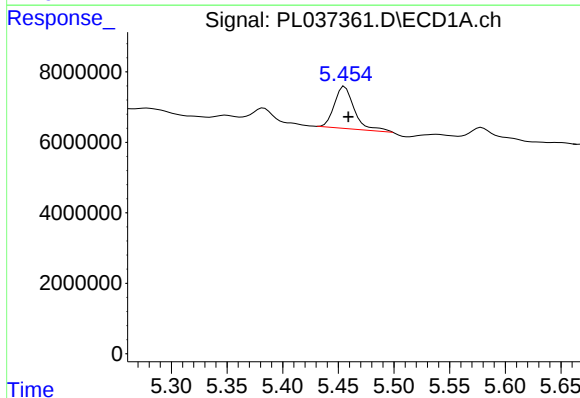


#12 4,4'-DDE

R.T.: 5.456 min
Delta R.T.: -0.003 min
Response: 14826942
Conc: 1.68 ng/ml

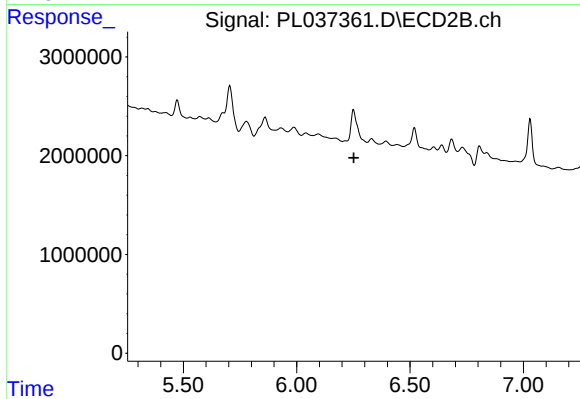

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.252 min
Response: 0
Conc: N.D.

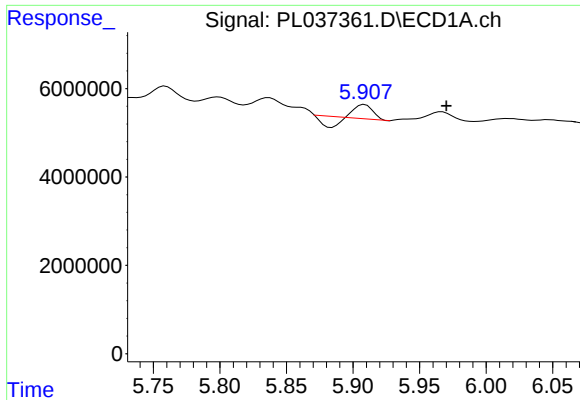

#16 4,4'-DDD


R.T.: 5.909 min
Delta R.T.: -0.061 min
Response: 1330106
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

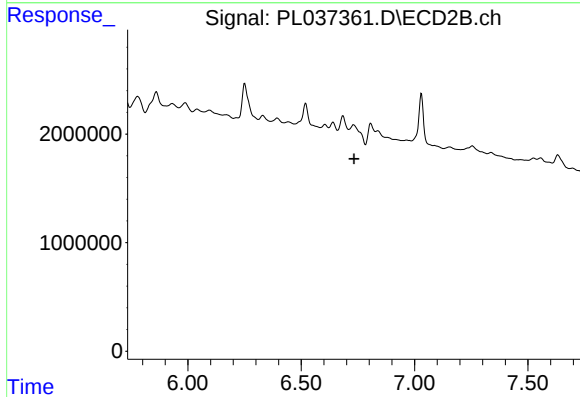


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.734 min
Response: 0
Conc: N.D.

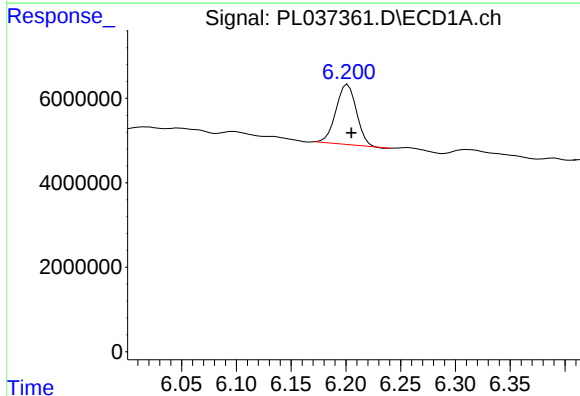


#17 4,4'-DDT

R.T.: 6.202 min
Delta R.T.: -0.003 min
Response: 18582408
Conc: 2.88 ng/ml

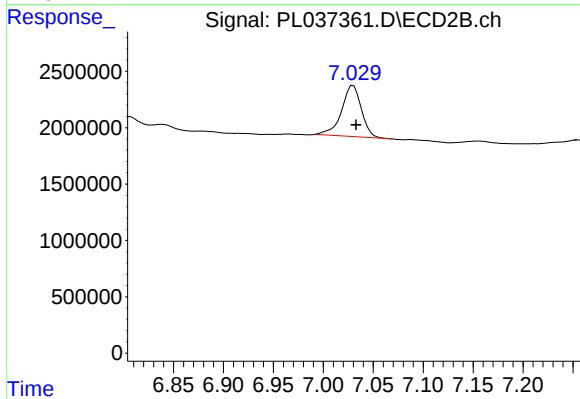

#17 4,4'-DDT


R.T.: 7.030 min
Delta R.T.: -0.003 min
Response: 6217924
Conc: 2.94 ng/ml

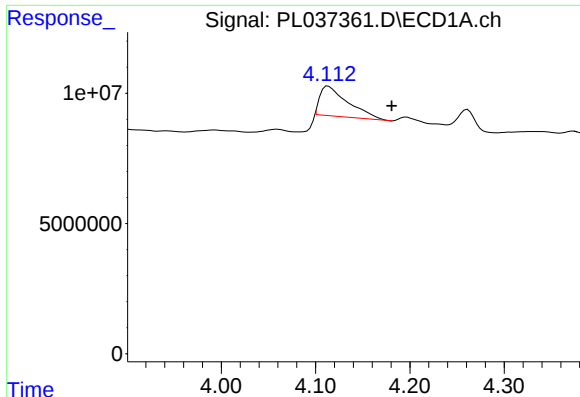

#23 Chlordane-1


R.T.: 4.113 min
Delta R.T.: -0.067 min
Response: 23535591
Conc: 76.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

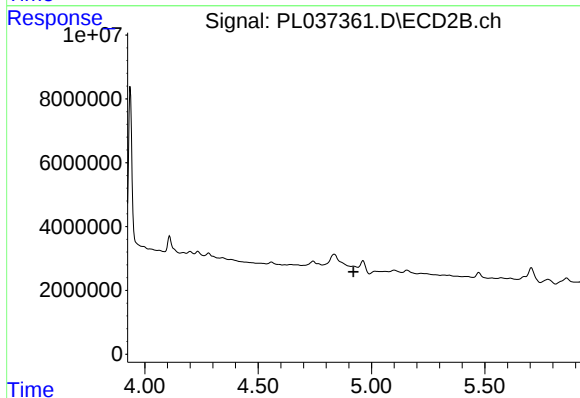


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

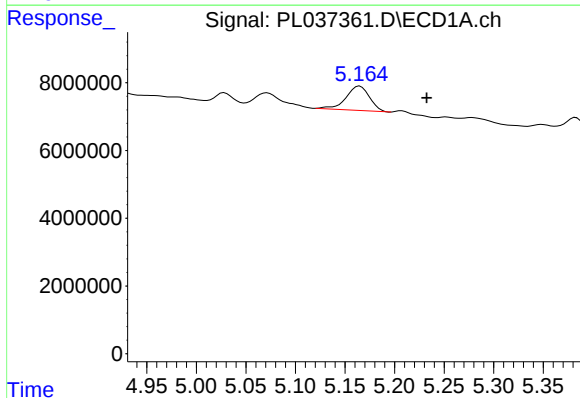


#25 Chlordane-3

R.T.: 5.165 min
Delta R.T.: -0.067 min
Response: 11879902
Conc: 11.18 ng/ml

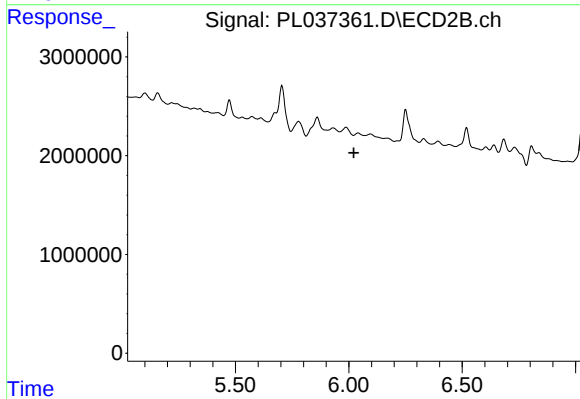

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

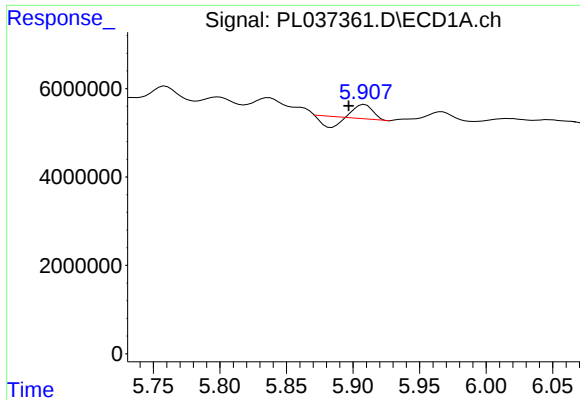

#27 Chlordane-5


R.T.: 5.909 min
Delta R.T.: 0.012 min
Response: 1330106
Conc: 10.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

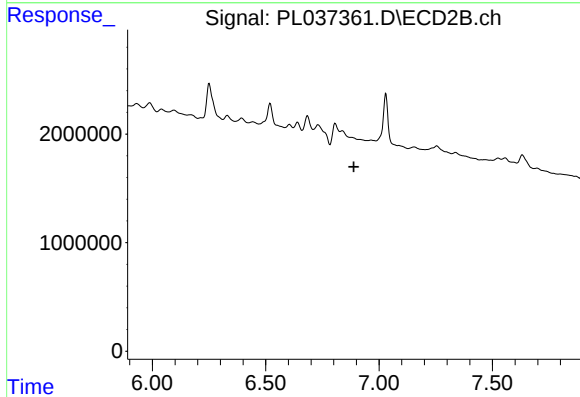


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.889 min
Response: 0
Conc: N.D.

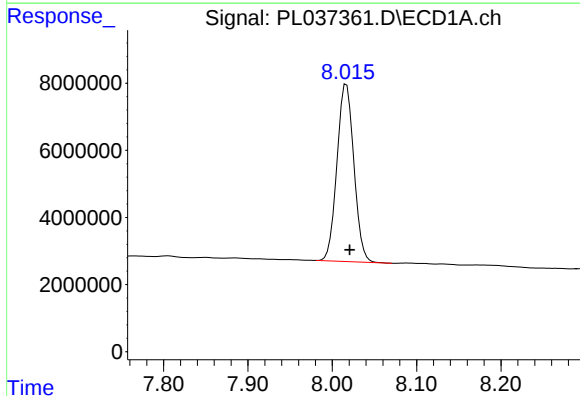

#28 Decachlorobiphenyl

R.T.: 8.017 min
Delta R.T.: -0.004 min
Response: 73635971
Conc: 12.20 ng/ml

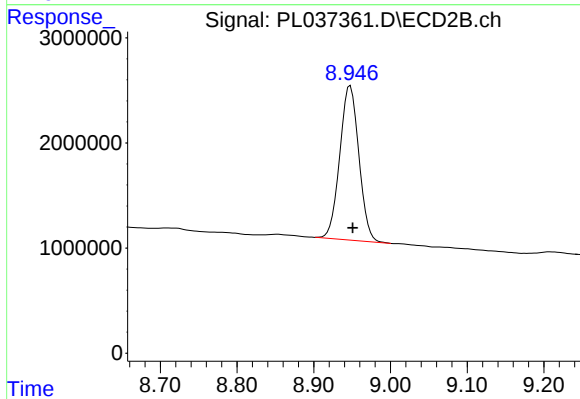

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 25448192
Conc: 12.83 ng/ml