

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
 Data File : PL037396.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2018 00:20
 Operator : UA\AJ
 Sample : J3570-10
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 04:28:01 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.936	153.1E6	55860348	19.355	20.190
28)	SA Decachlor...	8.016	8.947	123.8E6	39744444	20.525	20.033
Target Compounds							
4)	MA Heptachlor	4.315	0.000	39023261	0	3.809	N.D. #
6)	B beta-BHC	4.315	0.000	39023261	0	8.556	N.D. #
7)	B delta-BHC	4.472	0.000	7576601	0	0.716	N.D. #
10)	B gamma-Chl...	5.259	0.000	18388217	0	1.963	N.D. #
11)	B alpha-Chl...	5.259	0.000	18388217	0	2.025	N.D. #
15)	B Endosulfa...	6.048f	0.000	63472873	0	8.632	N.D. #
16)	A 4,4'-DDD	5.935f	6.686f	6739457	4797710	1.026	2.337 #
20)	A Methoxychlor	6.759	0.000	54157694	0	15.933	N.D. #
25)	Chlordane-3	5.259	0.000	18388217	0	17.300	N.D. #
26)	Chlordane-4	5.259	0.000	18388217	0	19.085	N.D. #
27)	Chlordane-5	5.935	0.000	6739457	0	51.498	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
Data File : PL037396.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2018 00:20
Operator : UA\AJ
Sample : J3570-10
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:28:01 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

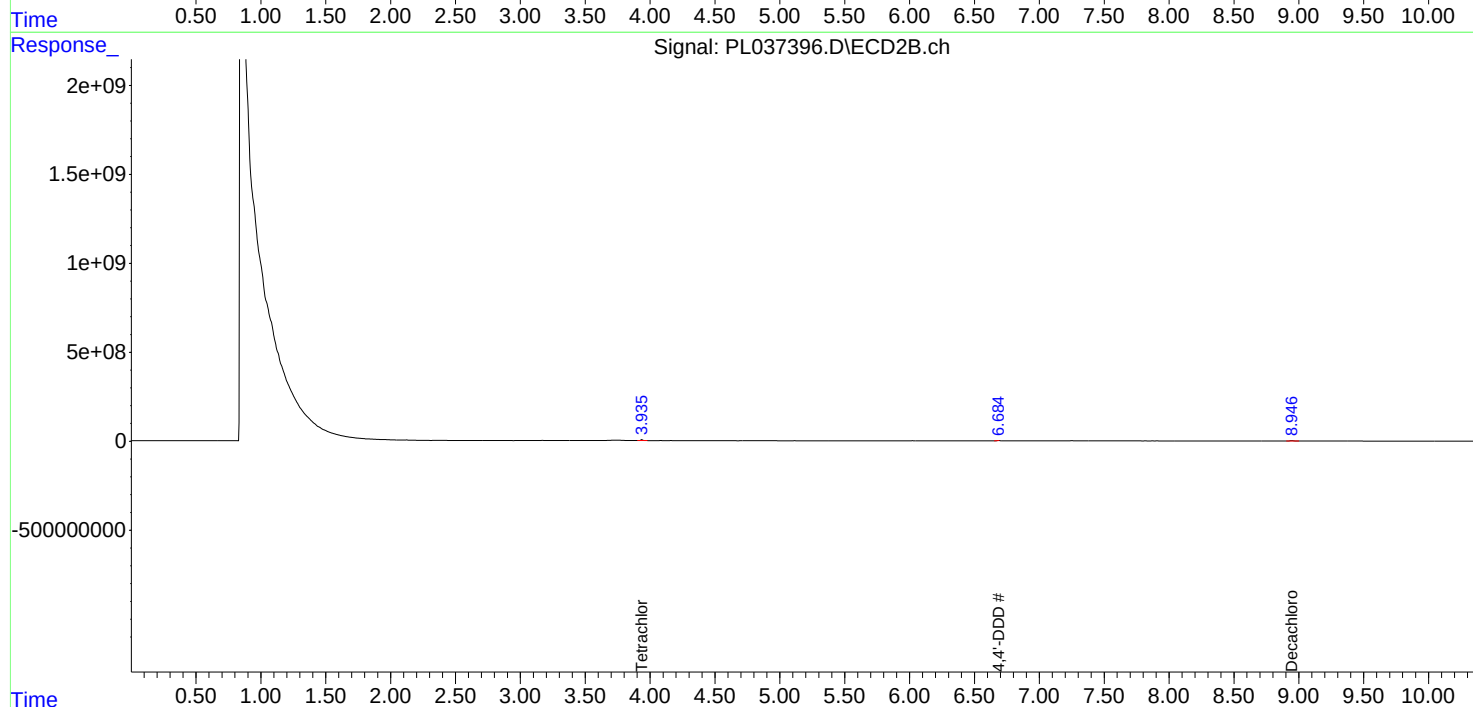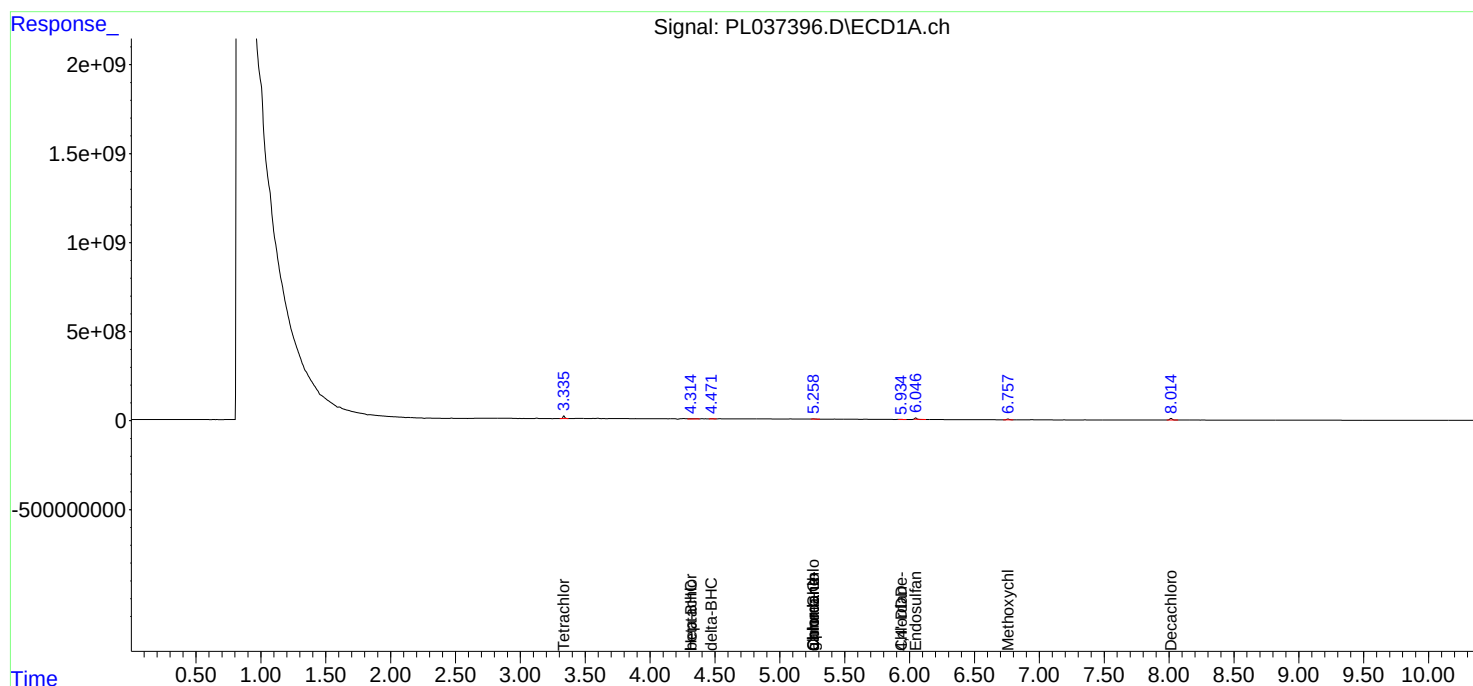


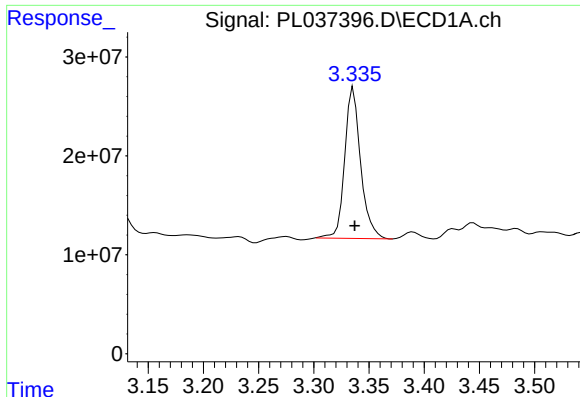

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: -0.001 min
Response: 153101006
Conc: 19.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

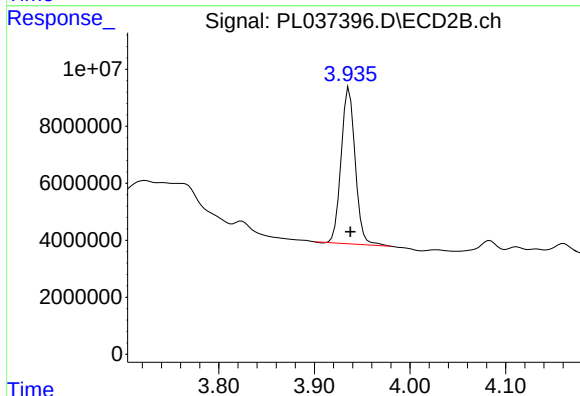


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.001 min
Response: 55860348
Conc: 20.19 ng/ml

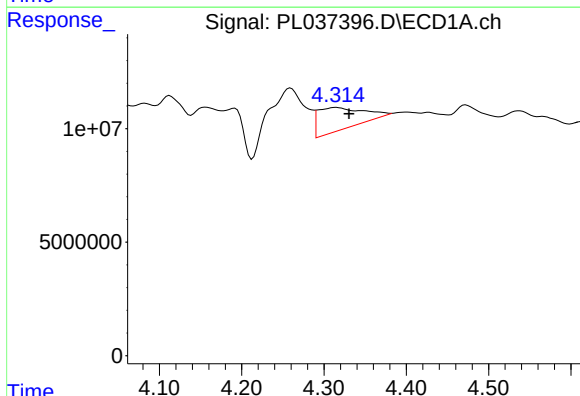


#4 Heptachlor

R.T.: 4.315 min
Delta R.T.: -0.015 min
Response: 39023261
Conc: 3.81 ng/ml

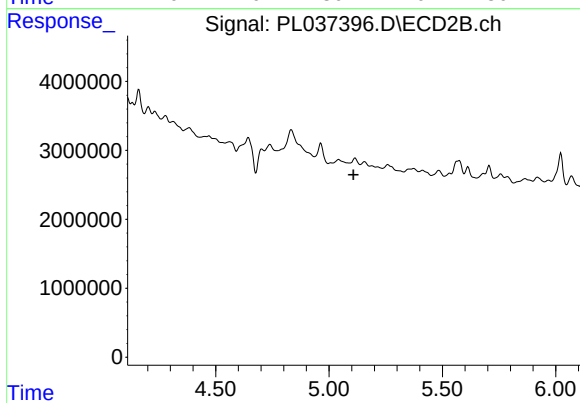

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.108 min
Response: 0
Conc: N.D.

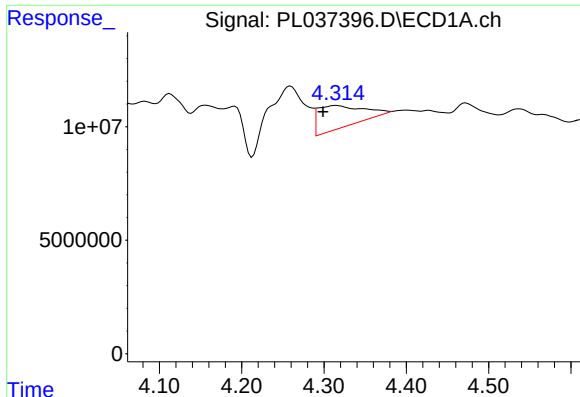

#6 beta-BHC


R.T.: 4.315 min
Delta R.T.: 0.016 min
Response: 39023261
Conc: 8.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

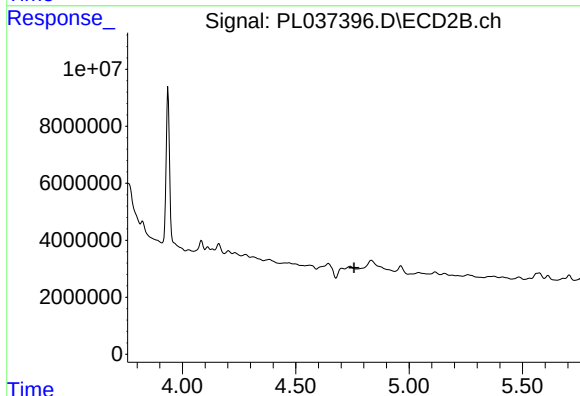


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

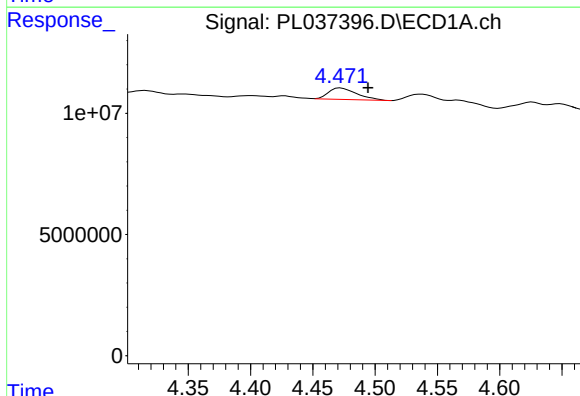


#7 delta-BHC

R.T.: 4.472 min
Delta R.T.: -0.022 min
Response: 7576601
Conc: 0.72 ng/ml

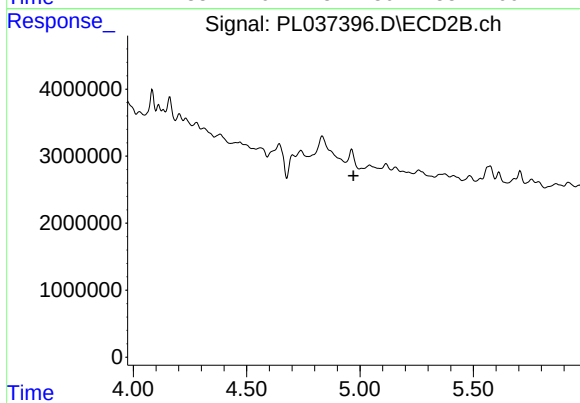

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.972 min
Response: 0
Conc: N.D.

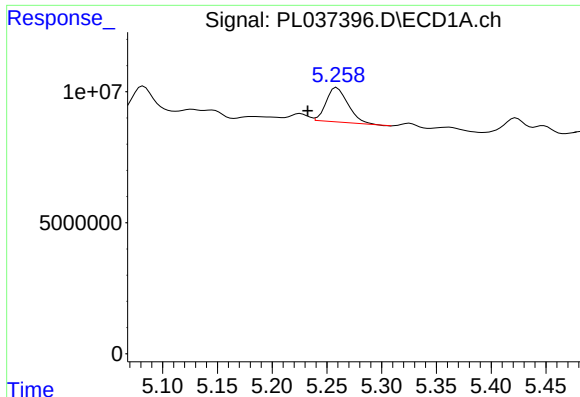

#10 gamma-Chlordane


R.T.: 5.259 min
Delta R.T.: 0.027 min
Response: 18388217
Conc: 1.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

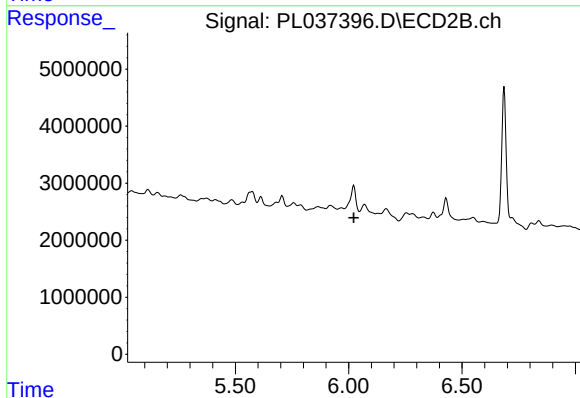


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

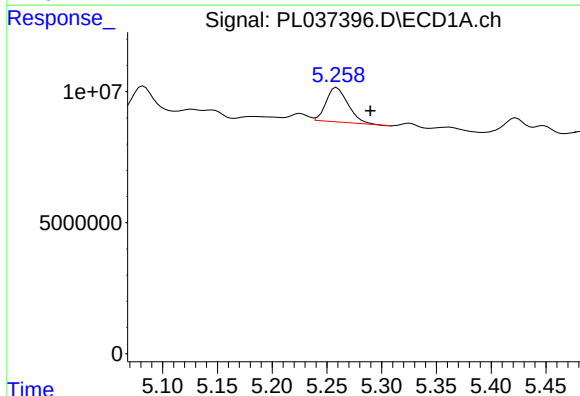


#11 alpha-Chlordane

R.T.: 5.259 min
Delta R.T.: -0.031 min
Response: 18388217
Conc: 2.02 ng/ml

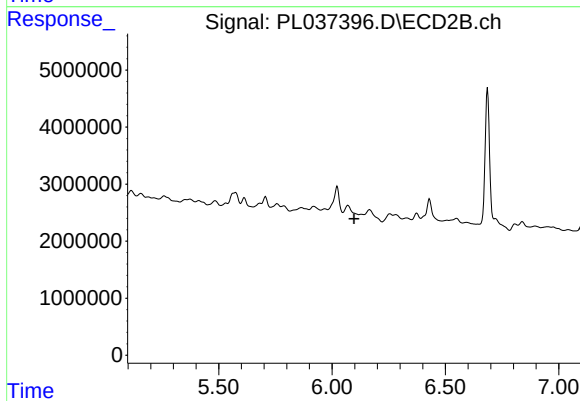

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.097 min
Response: 0
Conc: N.D.

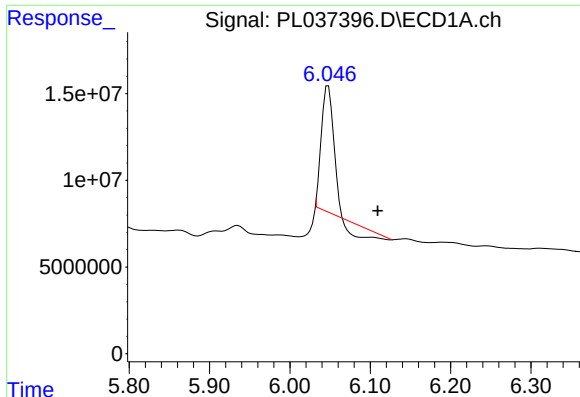

#15 Endosulfan II


R.T.: 6.048 min
Delta R.T.: -0.062 min
Response: 63472873
Conc: 8.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

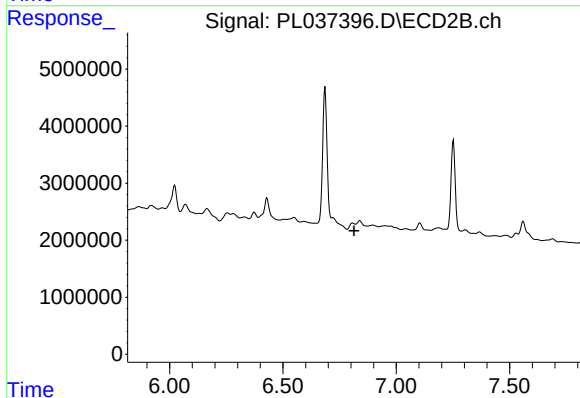


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.814 min
Response: 0
Conc: N.D.

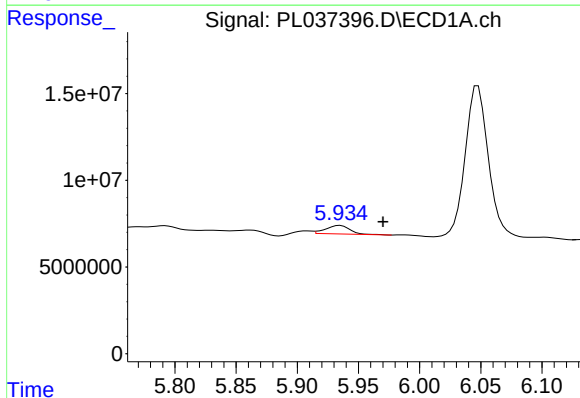


#16 4,4'-DDD

R.T.: 5.935 min
Delta R.T.: -0.035 min
Response: 6739457
Conc: 1.03 ng/ml

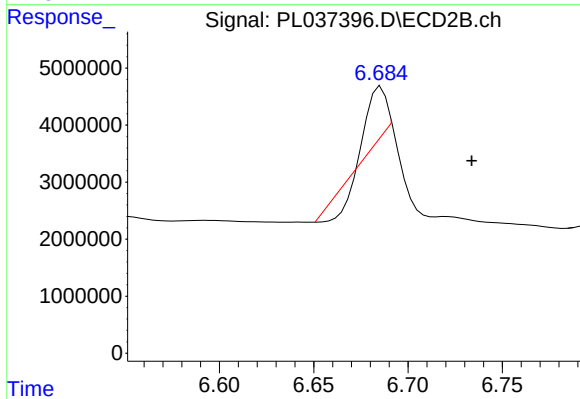

#16 4,4'-DDD


R.T.: 6.686 min
Delta R.T.: -0.048 min
Response: 4797710
Conc: 2.34 ng/ml

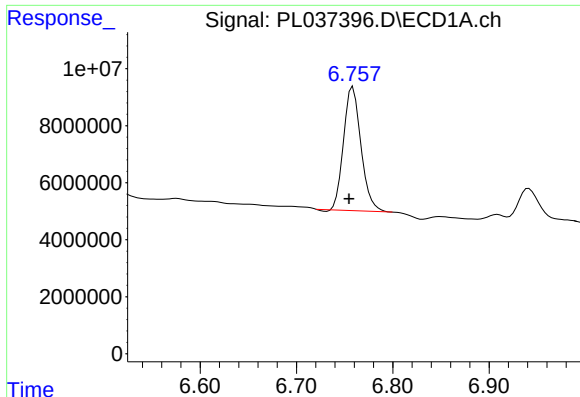

#20 Methoxychlor


R.T.: 6.759 min
Delta R.T.: 0.004 min
Response: 54157694
Conc: 15.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

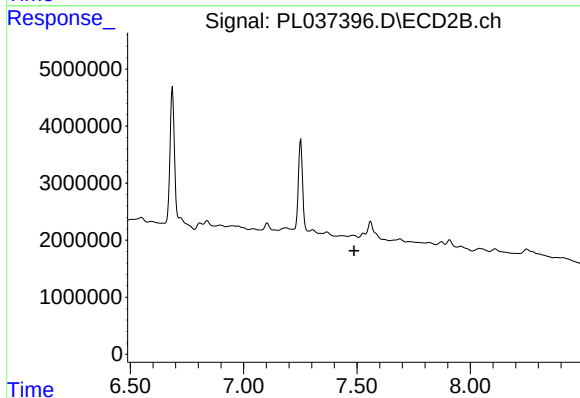


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.488 min
Response: 0
Conc: N.D.

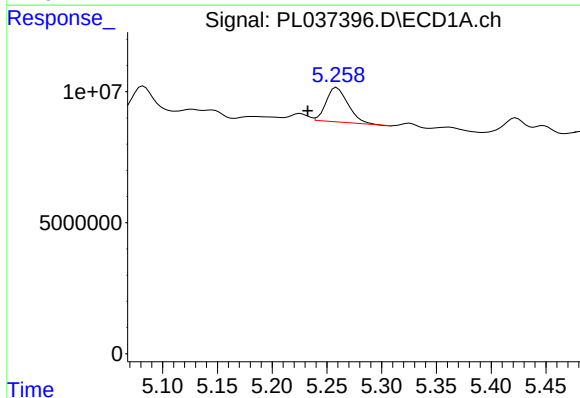


#25 Chlordane-3

R.T.: 5.259 min
Delta R.T.: 0.027 min
Response: 18388217
Conc: 17.30 ng/ml

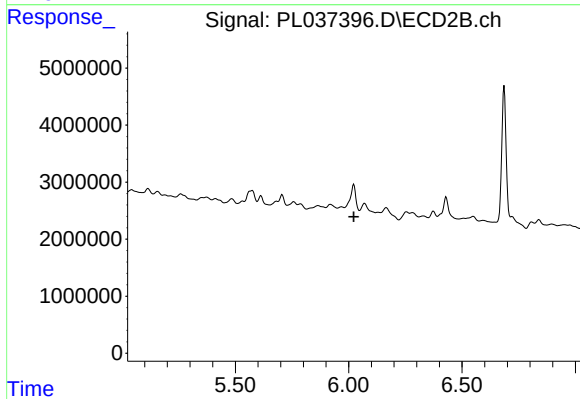

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

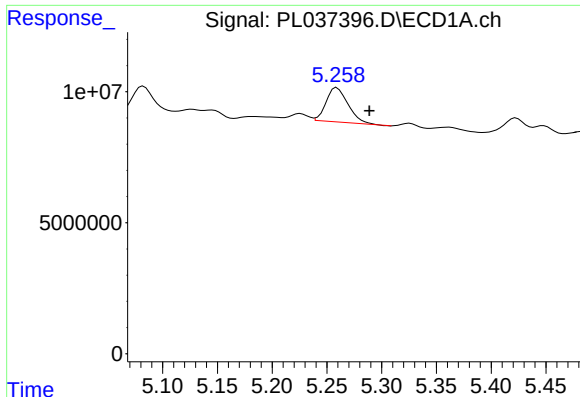

#26 Chlordane-4


R.T.: 5.259 min
Delta R.T.: -0.030 min
Response: 18388217
Conc: 19.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

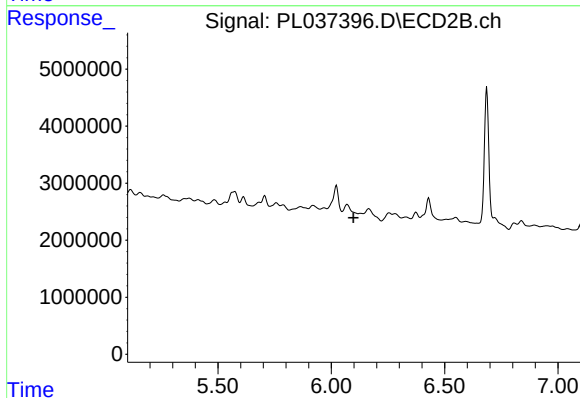


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

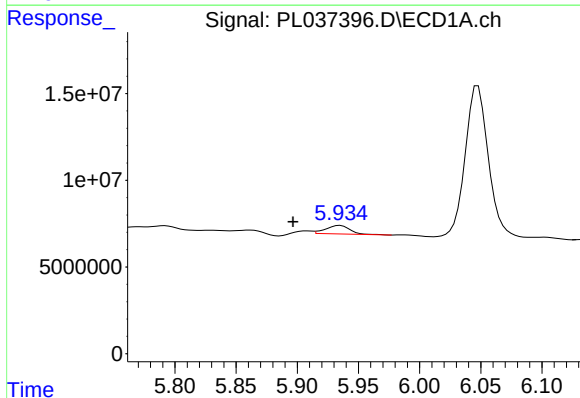


#27 Chlordane-5

R.T.: 5.935 min
Delta R.T.: 0.038 min
Response: 6739457
Conc: 51.50 ng/ml

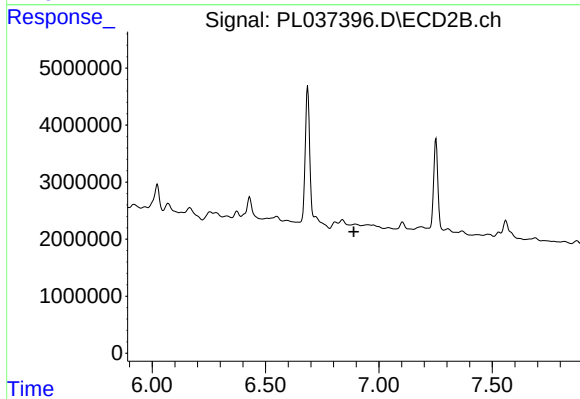

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.889 min
Response: 0
Conc: N.D.

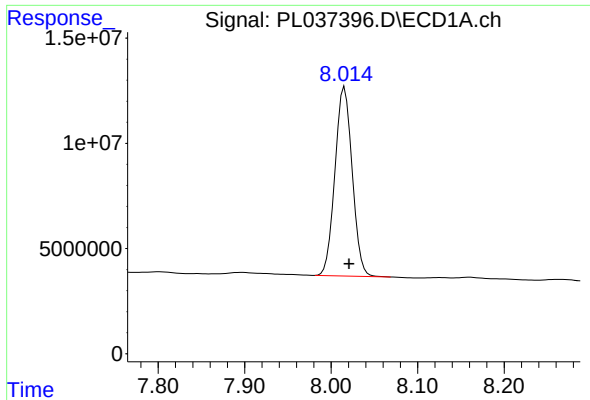

#28 Decachlorobiphenyl

R.T.: 8.016 min
Delta R.T.: -0.005 min
Response: 123846463
Conc: 20.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

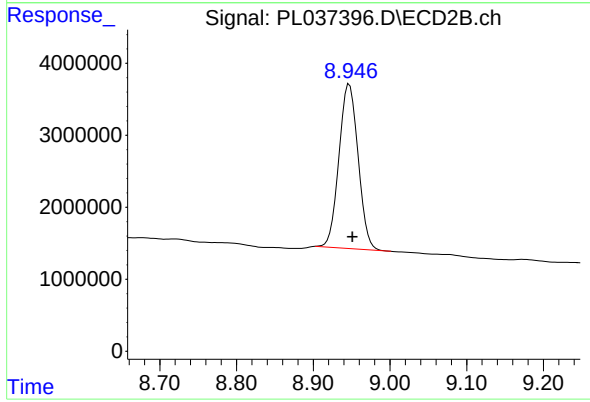

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 39744444
Conc: 20.03 ng/ml