

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
 Data File : PL037406.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2018 02:54
 Operator : UA\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 04:31:53 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.937	123.6E6	35292605	15.620	12.756
28)	SA Decachlor...	8.016	8.948	77319117	29870452	12.814	15.056
Target Compounds							
6)	B beta-BHC	4.255f	0.000	6176739	0	1.354	N.D. #
8)	B Heptachlo...	0.000	5.781	0	11334389	N.D.	3.976 #
10)	B gamma-Chl...	5.165f	0.000	11757362	0	1.255	N.D. #
14)	MA Endrin	5.850	0.000	9988077	0	1.268	N.D. #
21)	B Endrin ke...	6.936f	0.000	137.8E6	0	19.384	N.D. #
24)	Chlordane-2	0.000	5.316	0	10203873	N.D.	80.631 #
25)	Chlordane-3	5.165	0.000	11757362	0	11.061	N.D. #
27)	Chlordane-5	5.850	0.000	9988077	0	76.322	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
Data File : PL037406.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2018 02:54
Operator : UA\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:31:53 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

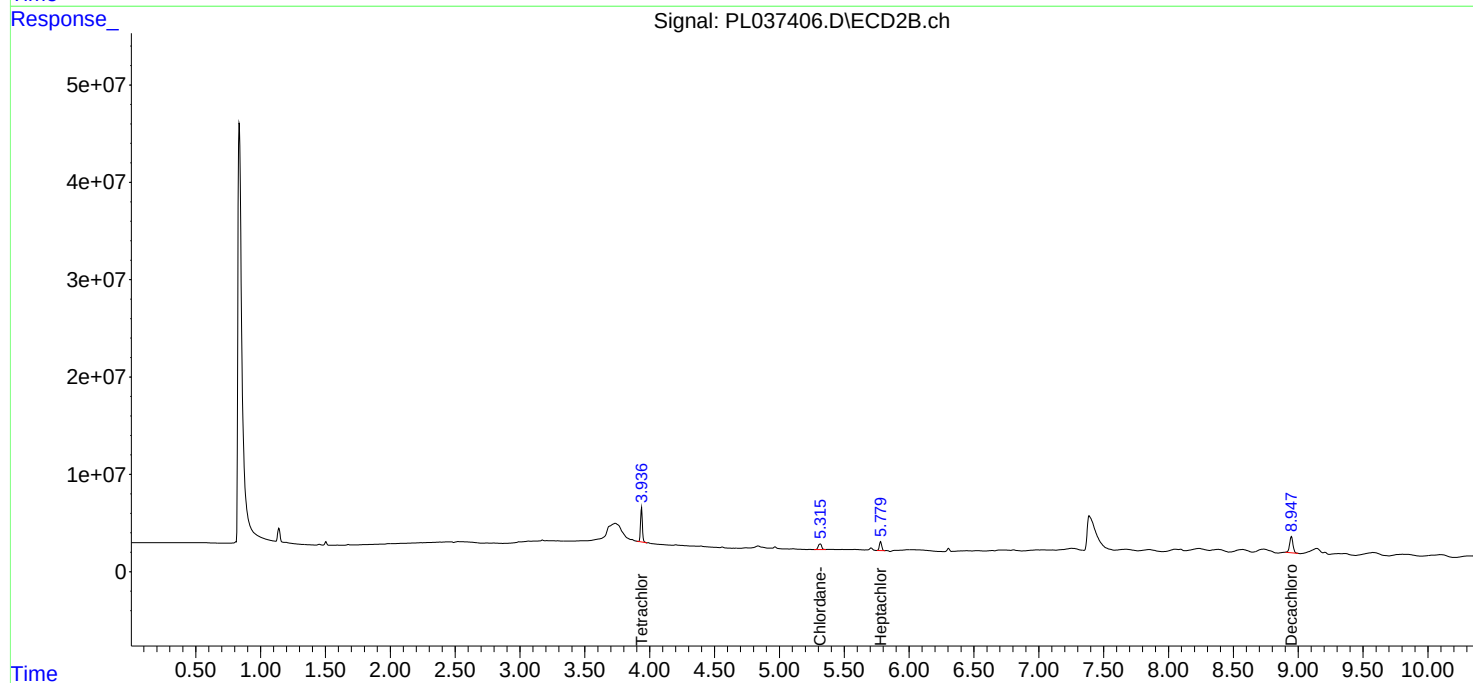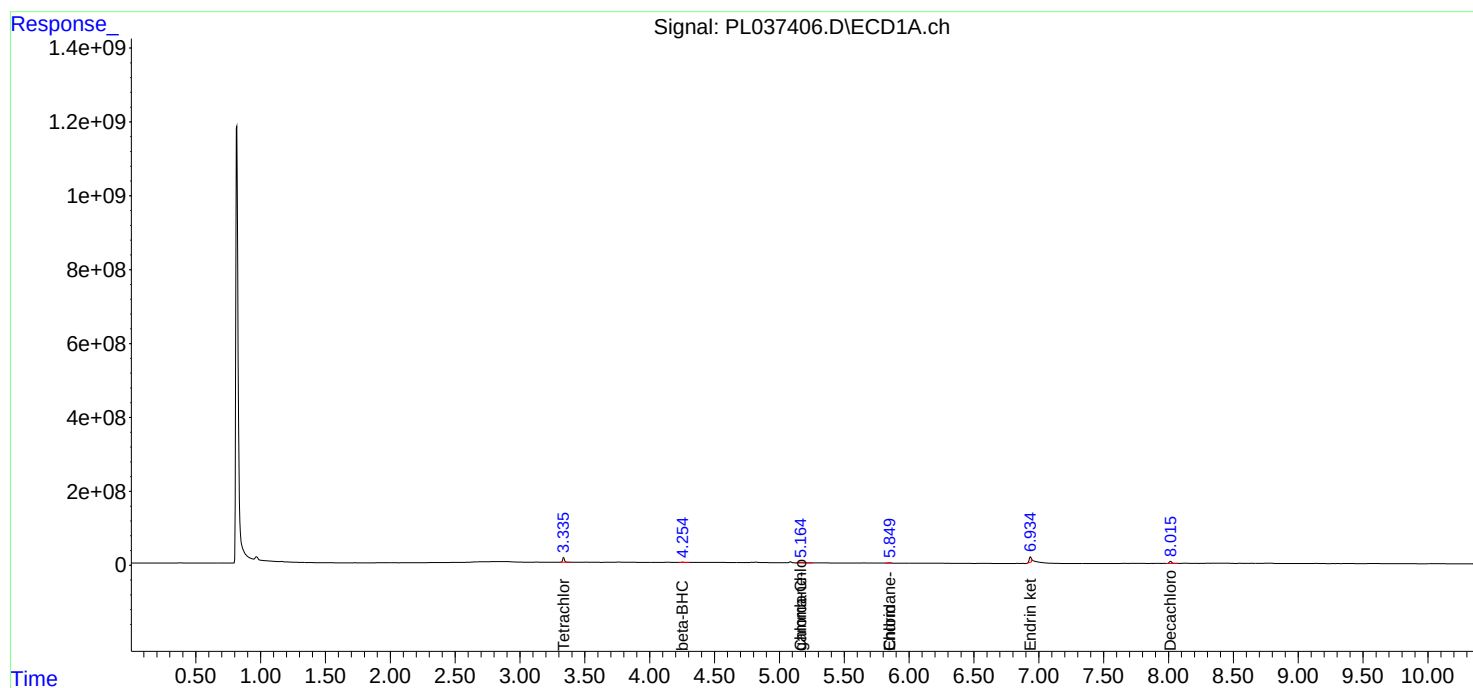


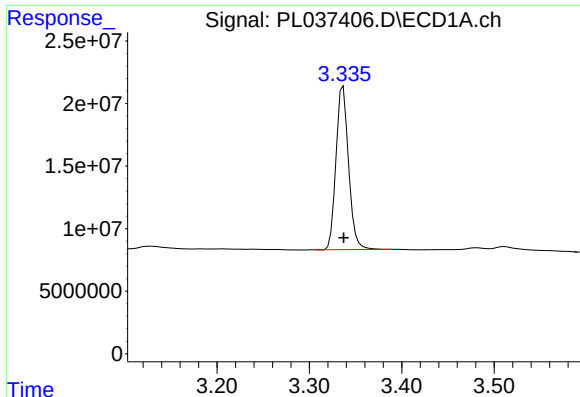

#1 Tetrachloro-m-xylene


R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 123560283
Conc: 15.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

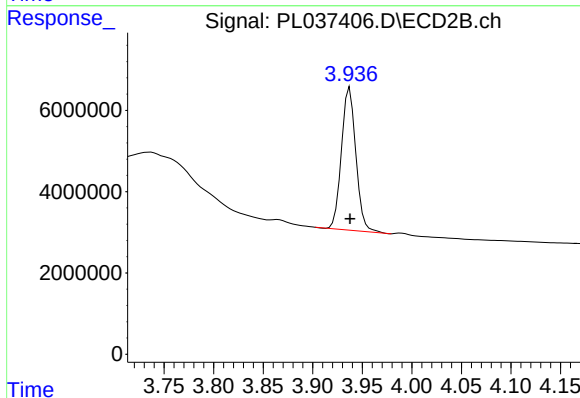


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 35292605
Conc: 12.76 ng/ml

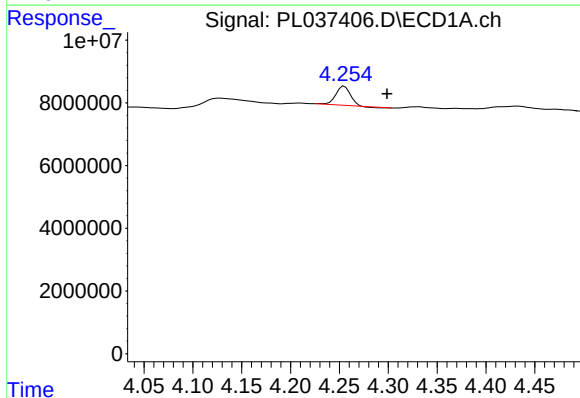


#6 beta-BHC

R.T.: 4.255 min
Delta R.T.: -0.044 min
Response: 6176739
Conc: 1.35 ng/ml

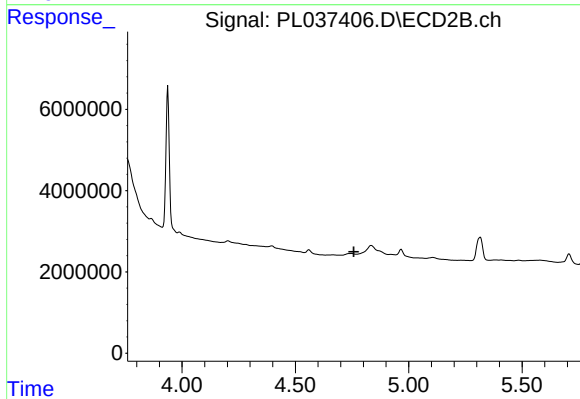

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

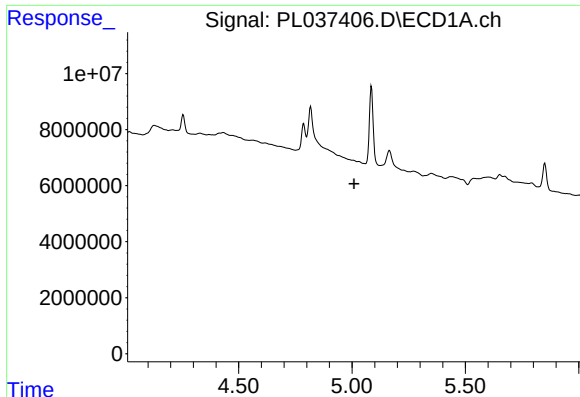

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.010 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

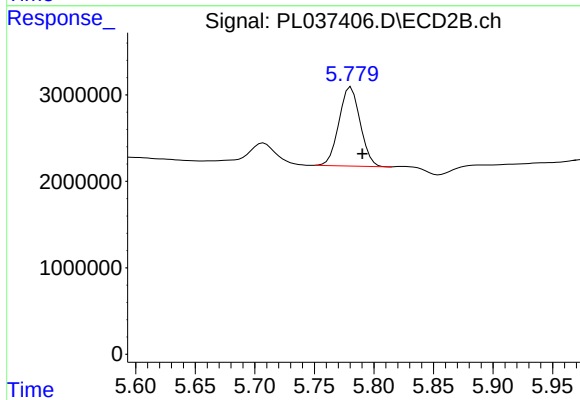


#8 Heptachlor epoxide

R.T.: 5.781 min
Delta R.T.: -0.010 min
Response: 11334389
Conc: 3.98 ng/ml

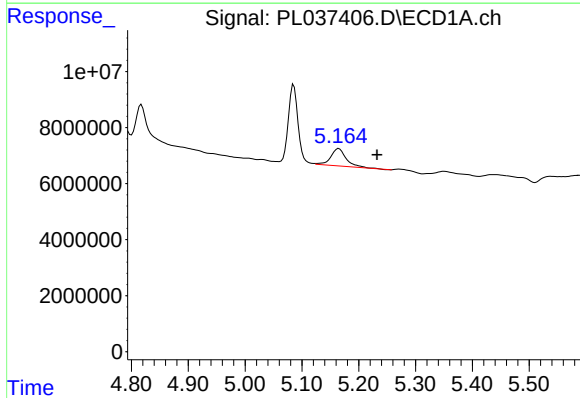


#10 gamma-Chlordane

R.T.: 5.165 min
Delta R.T.: -0.068 min
Response: 11757362
Conc: 1.26 ng/ml

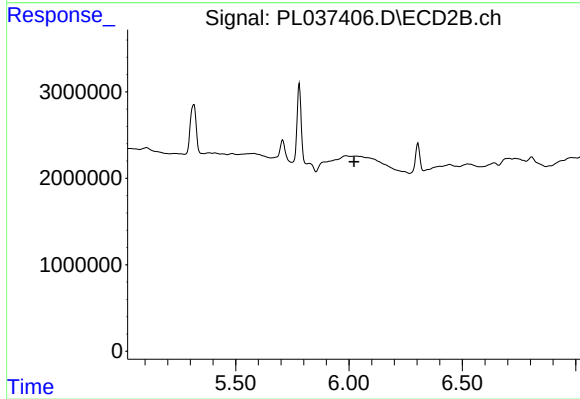

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

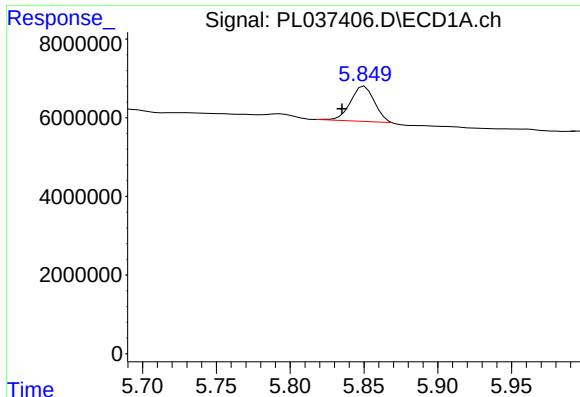

#14 Endrin


R.T.: 5.850 min
Delta R.T.: 0.015 min
Response: 9988077
Conc: 1.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

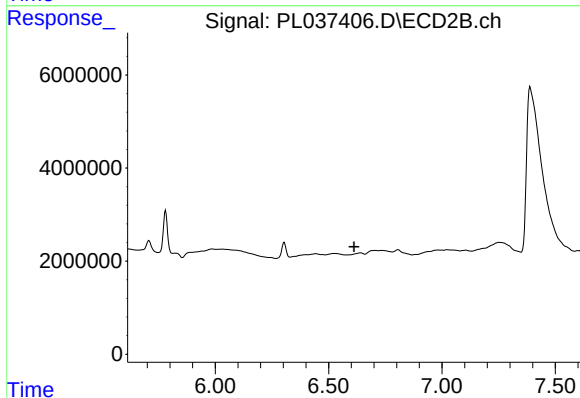


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

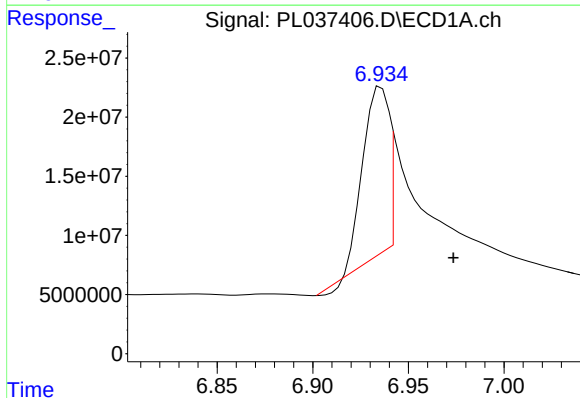


#21 Endrin ketone

R.T.: 6.936 min
Delta R.T.: -0.038 min
Response: 137849397
Conc: 19.38 ng/ml

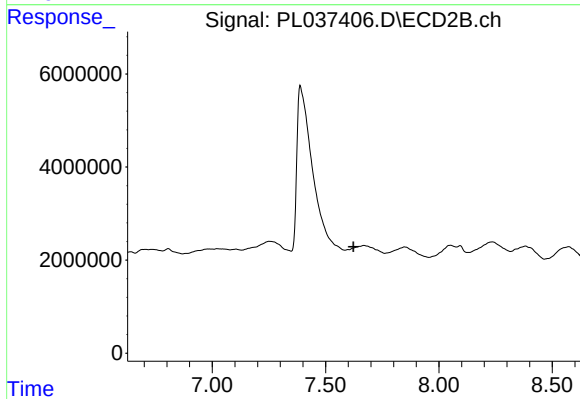

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.623 min
Response: 0
Conc: N.D.

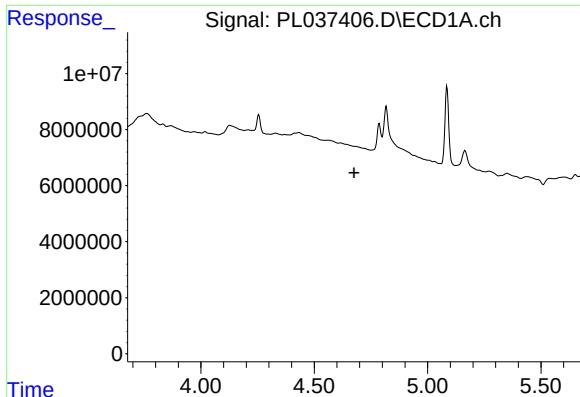

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.676 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

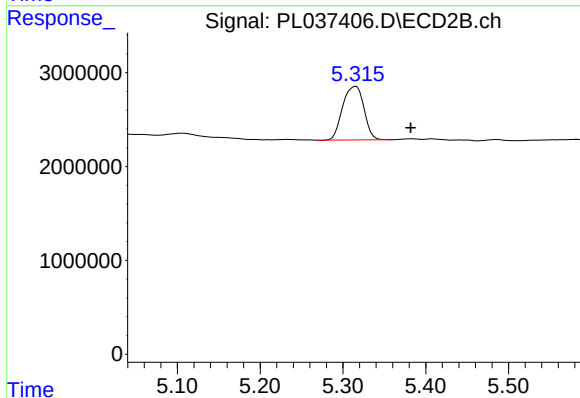


#24 Chlordane-2

R.T.: 5.316 min
Delta R.T.: -0.066 min
Response: 10203873
Conc: 80.63 ng/ml

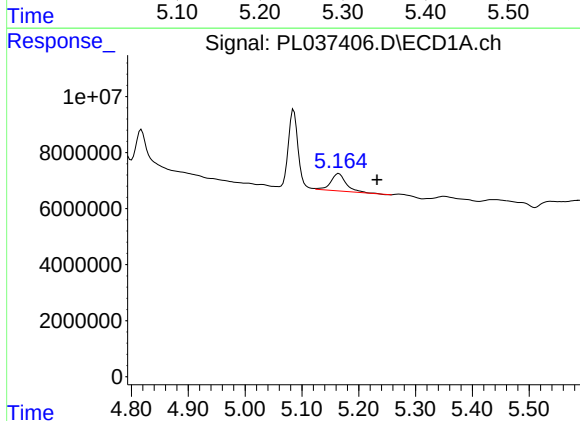


#25 Chlordane-3

R.T.: 5.165 min
Delta R.T.: -0.067 min
Response: 11757362
Conc: 11.06 ng/ml

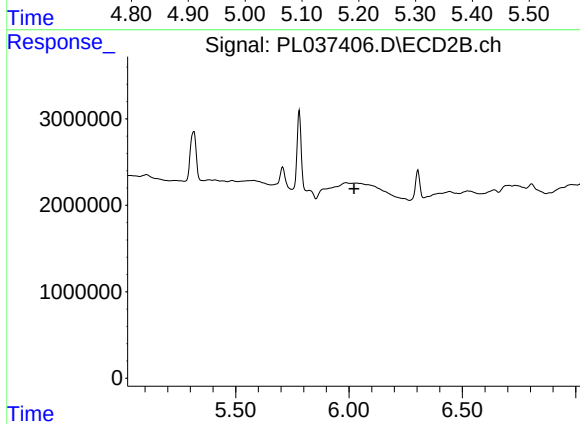

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.022 min
Response: 0
Conc: N.D.

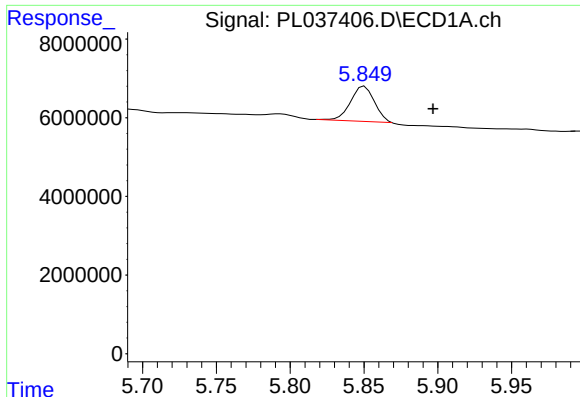

#27 Chlordane-5


R.T.: 5.850 min
Delta R.T.: -0.046 min
Response: 9988077
Conc: 76.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

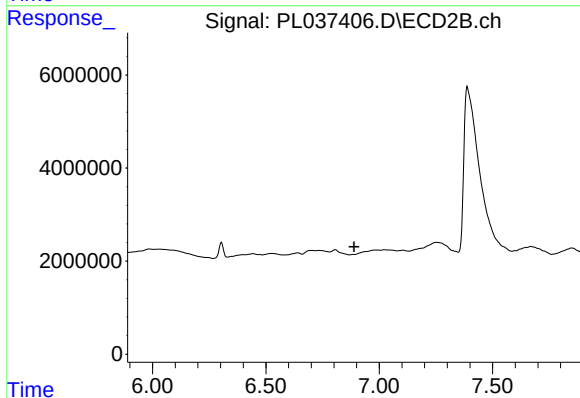


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.889 min
Response: 0
Conc: N.D.

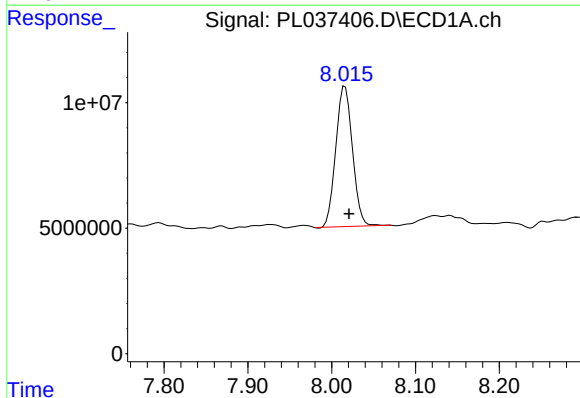

#28 Decachlorobiphenyl

R.T.: 8.016 min
Delta R.T.: -0.005 min
Response: 77319117
Conc: 12.81 ng/ml

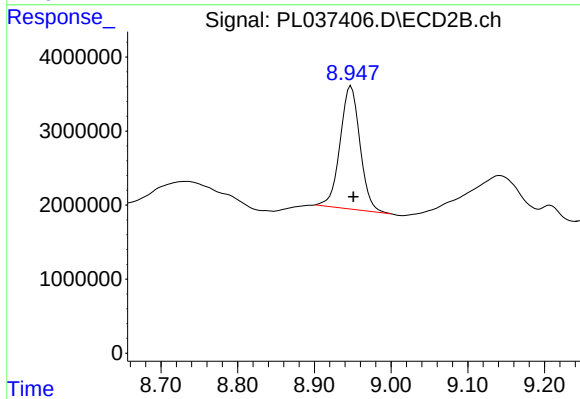

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 29870452
Conc: 15.06 ng/ml