

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
 Data File : PL037411.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2018 10:23
 Operator : UA\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 11:20:39 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.936	122.1E6	42988276	15.434	15.538
28)	SA Decachlor...	8.014	8.947	116.3E6	35167147	19.267	17.726
Target Compounds							
6)	B beta-BHC	4.253f	0.000	2908319	0	0.638	N.D. #
8)	B Heptachlo...	0.000	5.780	0	27630367	N.D.	9.693 #
12)	B 4,4'-DDE	0.000	6.304f	0	312206	N.D.	0.123 #
13)	MA Dieldrin	5.541f	0.000	1286849	0	0.145	N.D. #
14)	MA Endrin	5.849	0.000	24801083	0	3.148	N.D. #
21)	B Endrin ke...	6.936f	0.000	355.4E6	0	49.977	N.D. #
24)	Chlordane-2	0.000	5.316	0	26948744	N.D.	212.948 #
27)	Chlordane-5	5.849	0.000	24801083	0	191.322	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
Data File : PL037411.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2018 10:23
Operator : UA\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 11:20:39 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

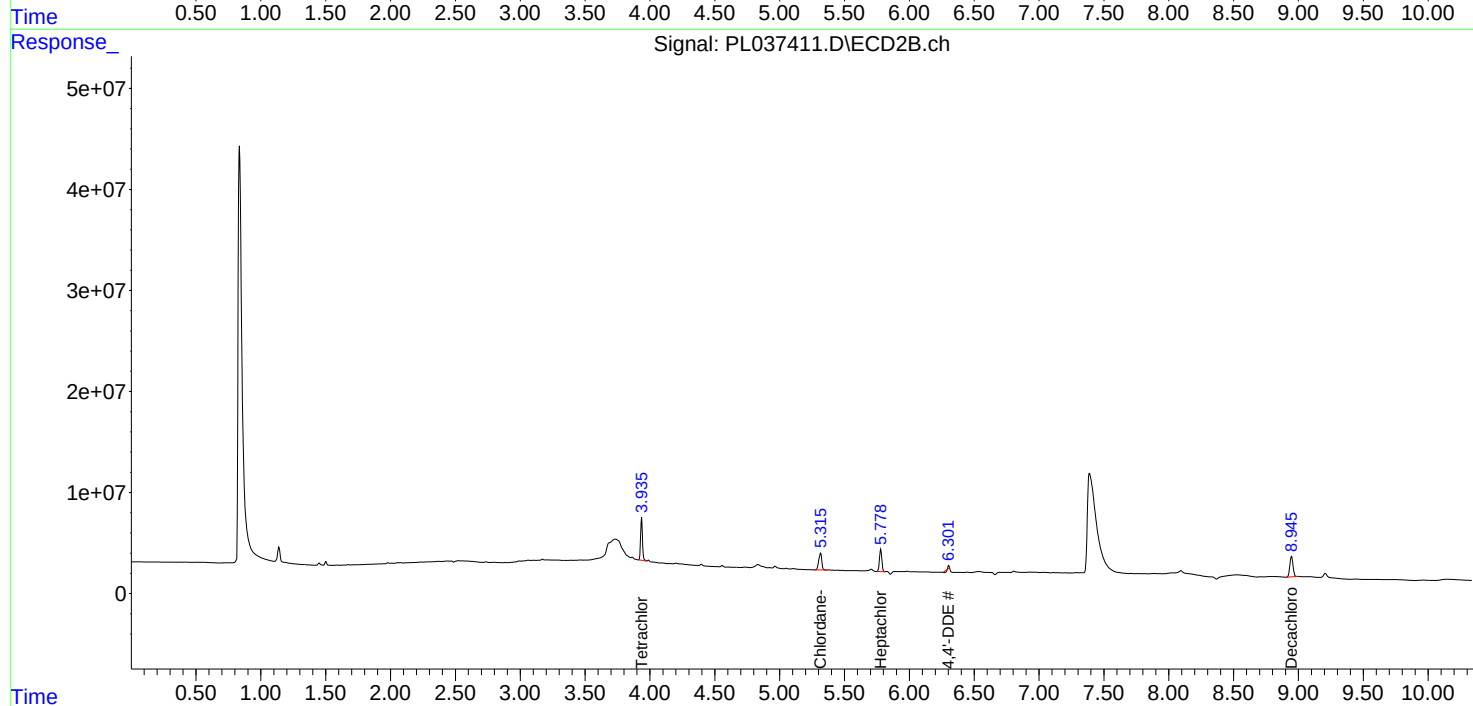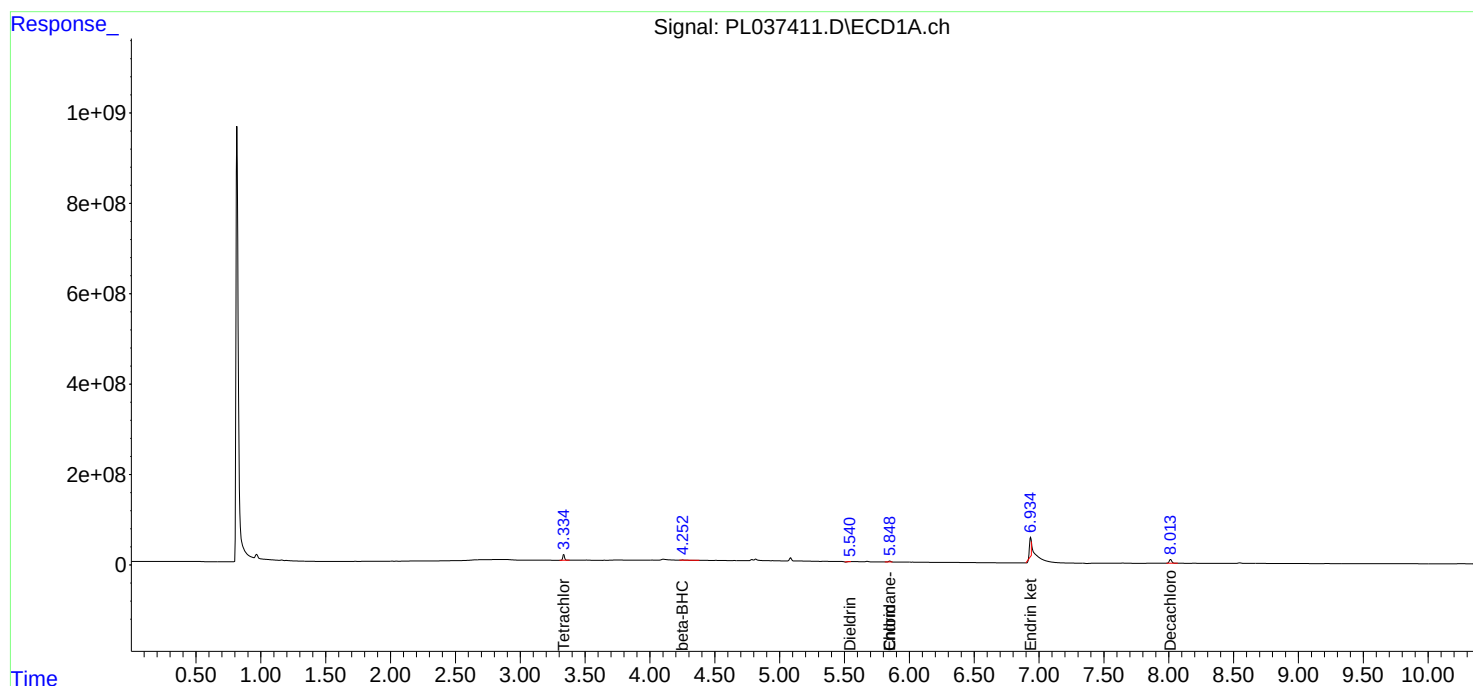


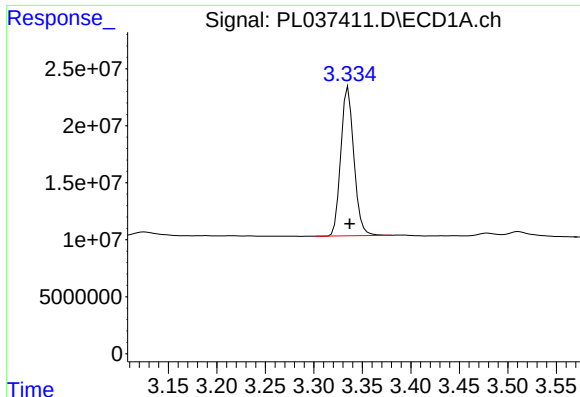

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: -0.002 min
Response: 122086716
Conc: 15.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

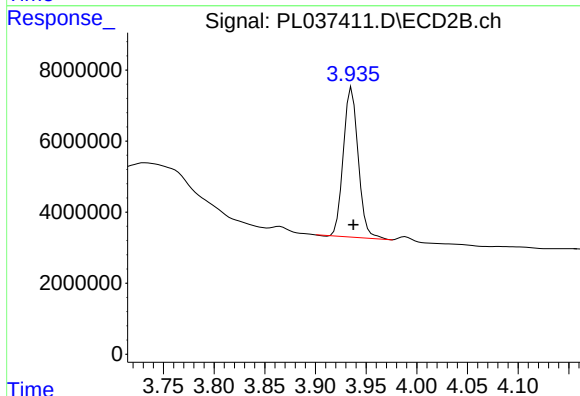


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 42988276
Conc: 15.54 ng/ml

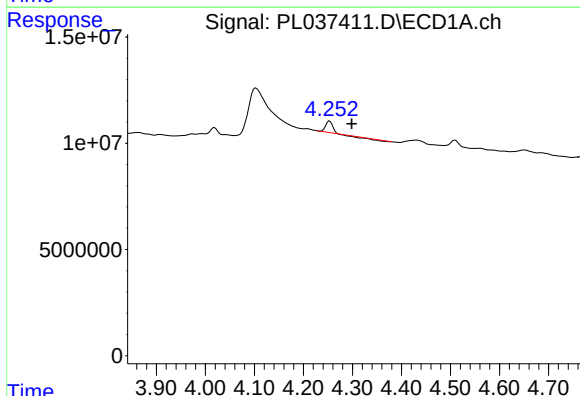


#6 beta-BHC

R.T.: 4.253 min
Delta R.T.: -0.045 min
Response: 2908319
Conc: 0.64 ng/ml

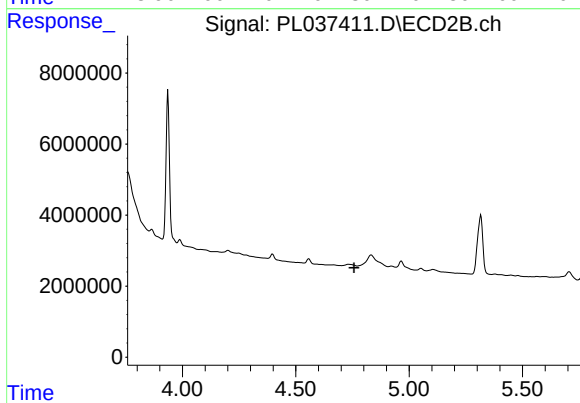

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.758 min
Response: 0
Conc: N.D.

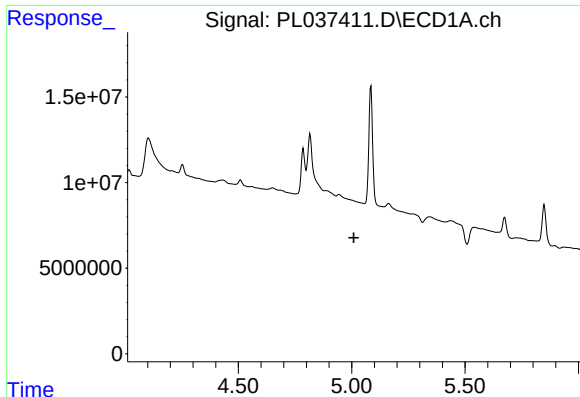

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.010 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

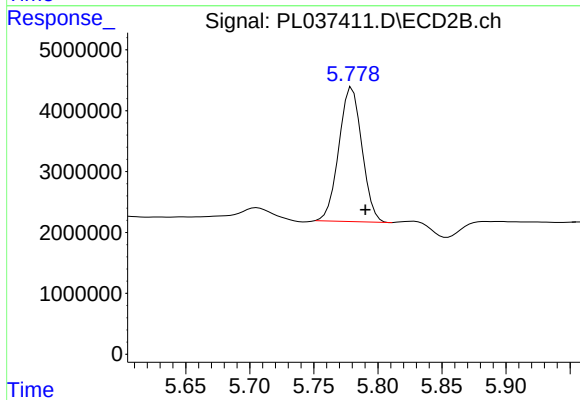


#8 Heptachlor epoxide

R.T.: 5.780 min
Delta R.T.: -0.011 min
Response: 27630367
Conc: 9.69 ng/ml

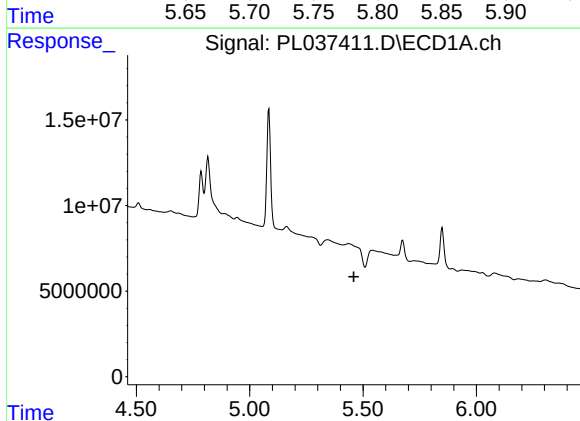


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

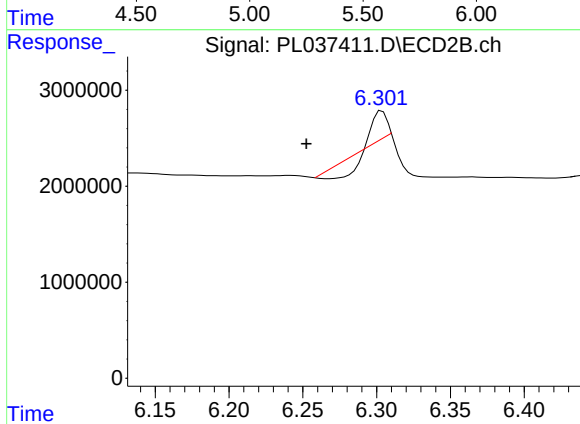

#12 4,4'-DDE


R.T.: 6.304 min
Delta R.T.: 0.051 min
Response: 312206
Conc: 0.12 ng/ml

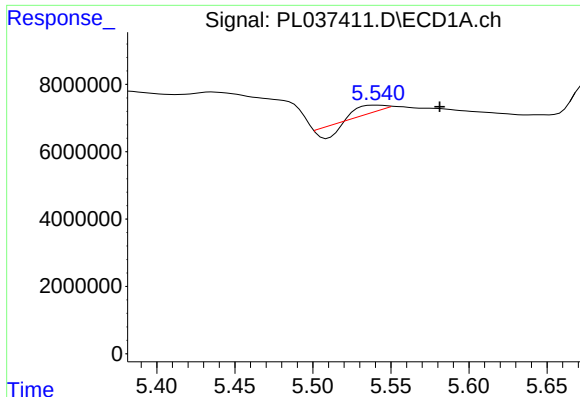

#13 Dieldrin


R.T.: 5.541 min
Delta R.T.: -0.040 min
Response: 1286849
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

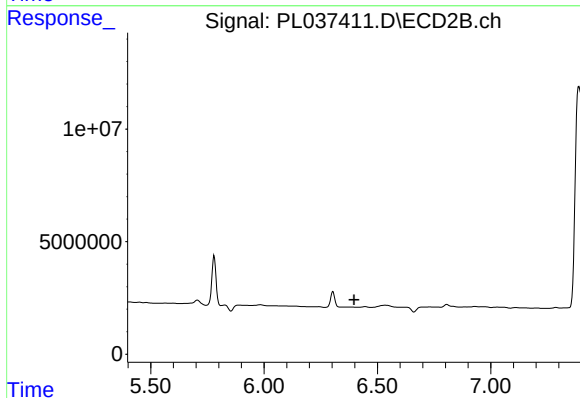


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.398 min
Response: 0
Conc: N.D.

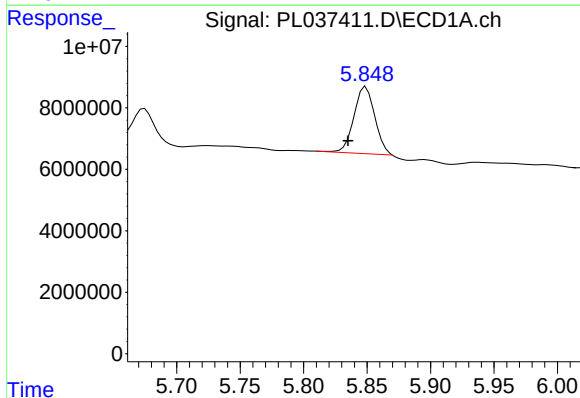


#14 Endrin

R.T.: 5.849 min
Delta R.T.: 0.014 min
Response: 24801083
Conc: 3.15 ng/ml

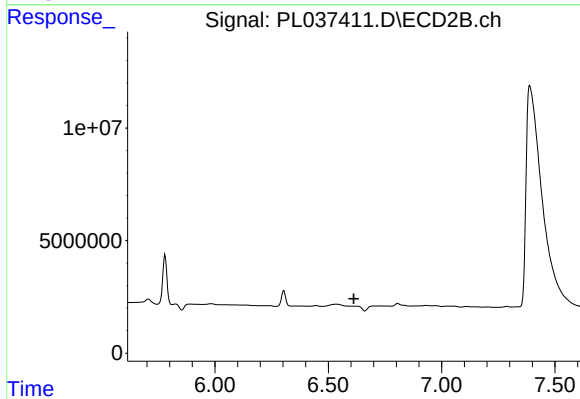

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

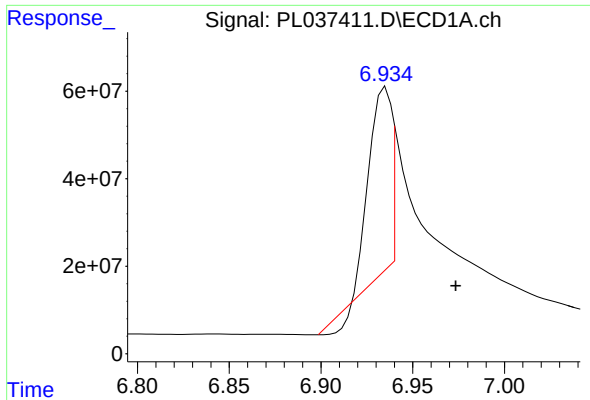

#21 Endrin ketone


R.T.: 6.936 min
Delta R.T.: -0.038 min
Response: 355421767
Conc: 49.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

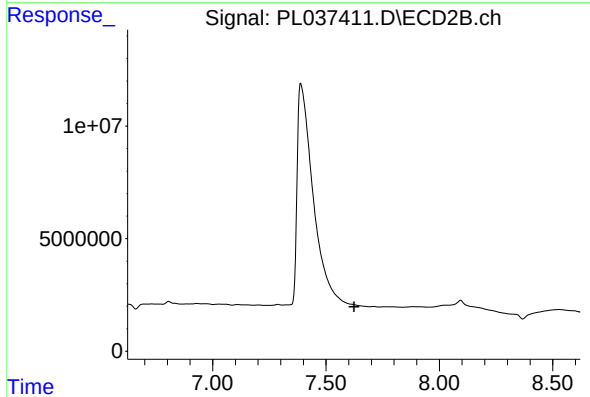


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.623 min
Response: 0
Conc: N.D.

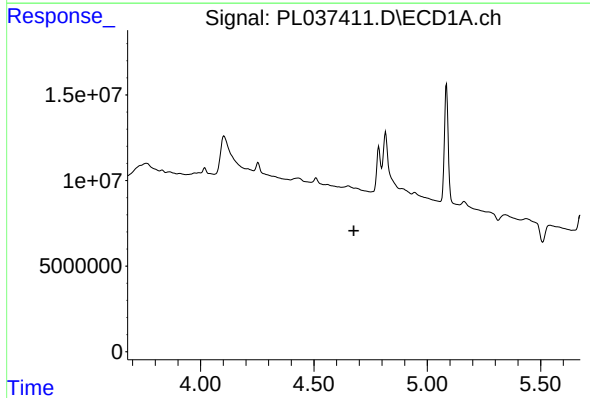


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.676 min
Response: 0
Conc: N.D.

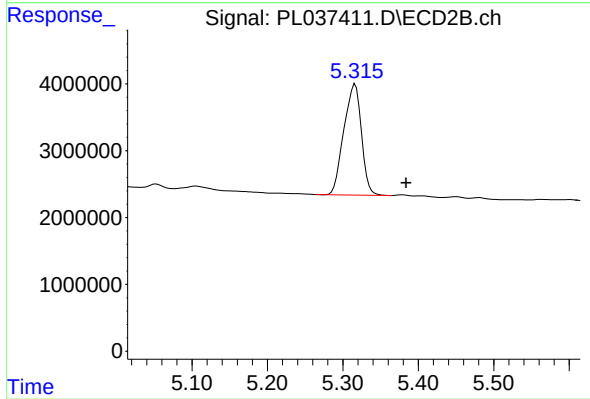

#24 Chlordane-2


R.T.: 5.316 min
Delta R.T.: -0.067 min
Response: 26948744
Conc: 212.95 ng/ml

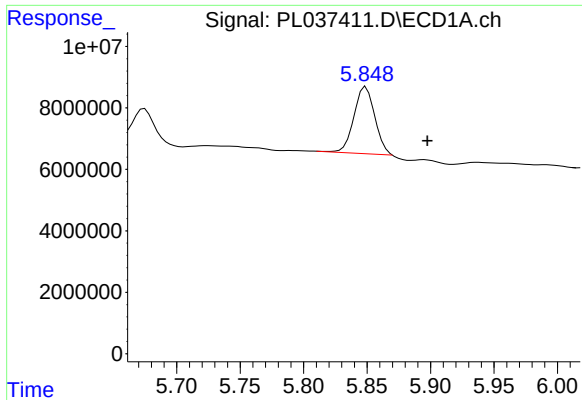

#27 Chlordane-5


R.T.: 5.849 min
Delta R.T.: -0.048 min
Response: 24801083
Conc: 191.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

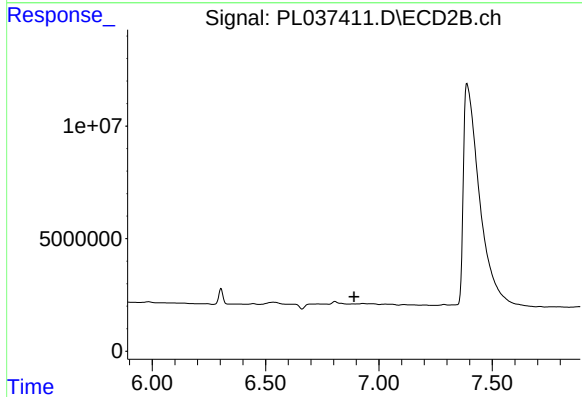


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.890 min
Response: 0
Conc: N.D.

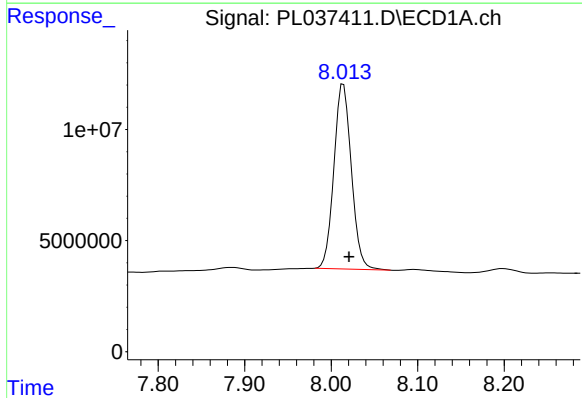

#28 Decachlorobiphenyl

R.T.: 8.014 min
Delta R.T.: -0.006 min
Response: 116258368
Conc: 19.27 ng/ml

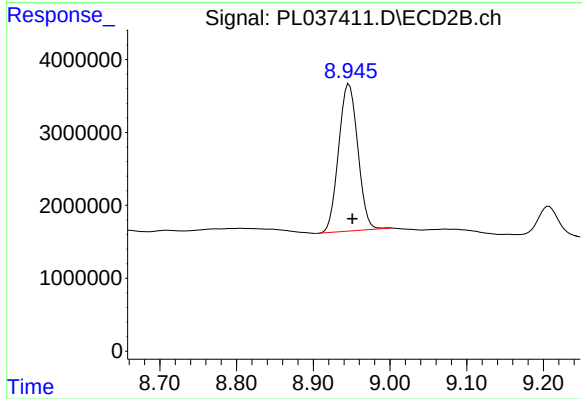

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 35167147
Conc: 17.73 ng/ml