

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
 Data File : PL037387.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2018 22:14
 Operator : UA\AJ
 Sample : J3667-01 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CS-PAINT-CHIP

Manual Integrations
 APPROVED

ugo
 6/26/2018 2:49:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 04:24:41 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	3.932	11235181	3496285	1.420m	1.264m
28)	SA Decachlor...	8.015	8.952	25330070	7796540	4.198m	3.930m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062518\
Data File : PL037387.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2018 22:14
Operator : UA\AJ
Sample : J3667-01 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CS-PAINT-CHIP


Manual Integrations
APPROVED

ugo
6/26/2018 2:49:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:24:41 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

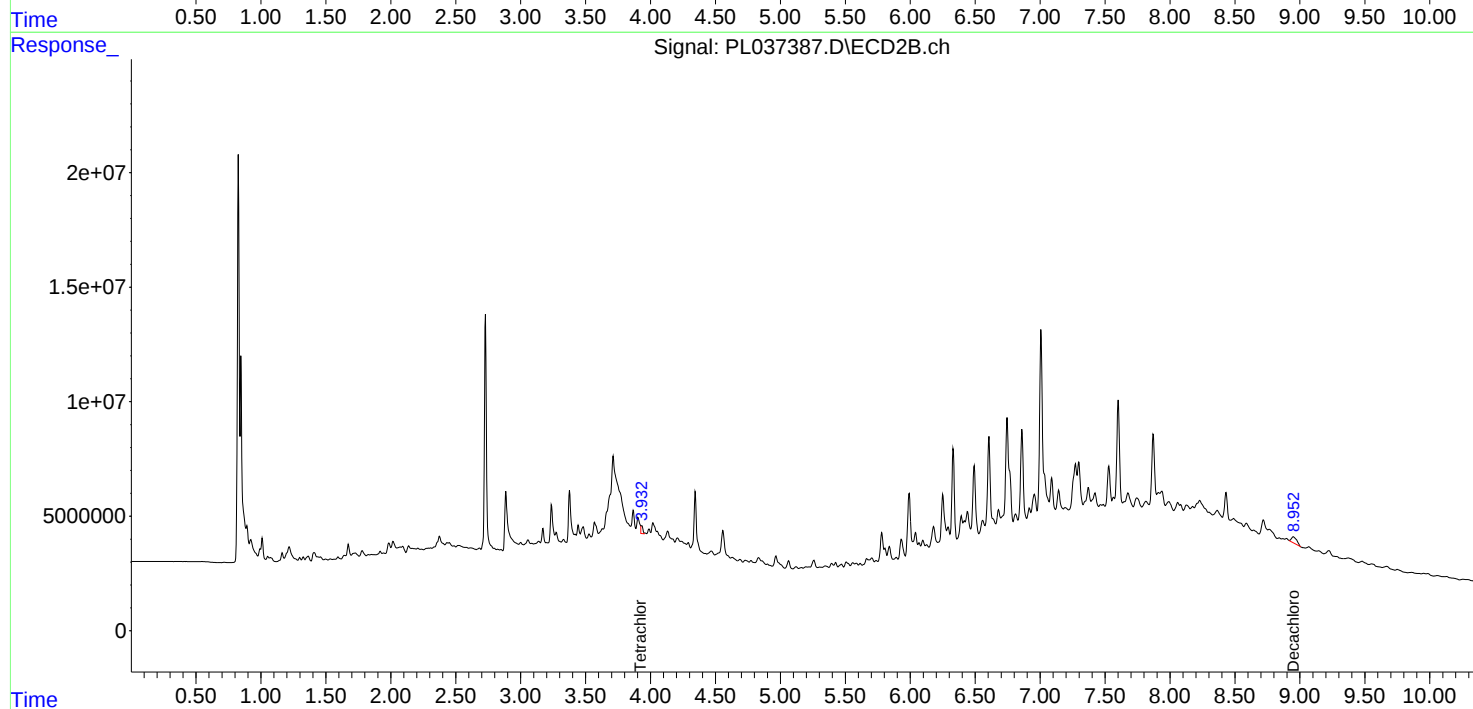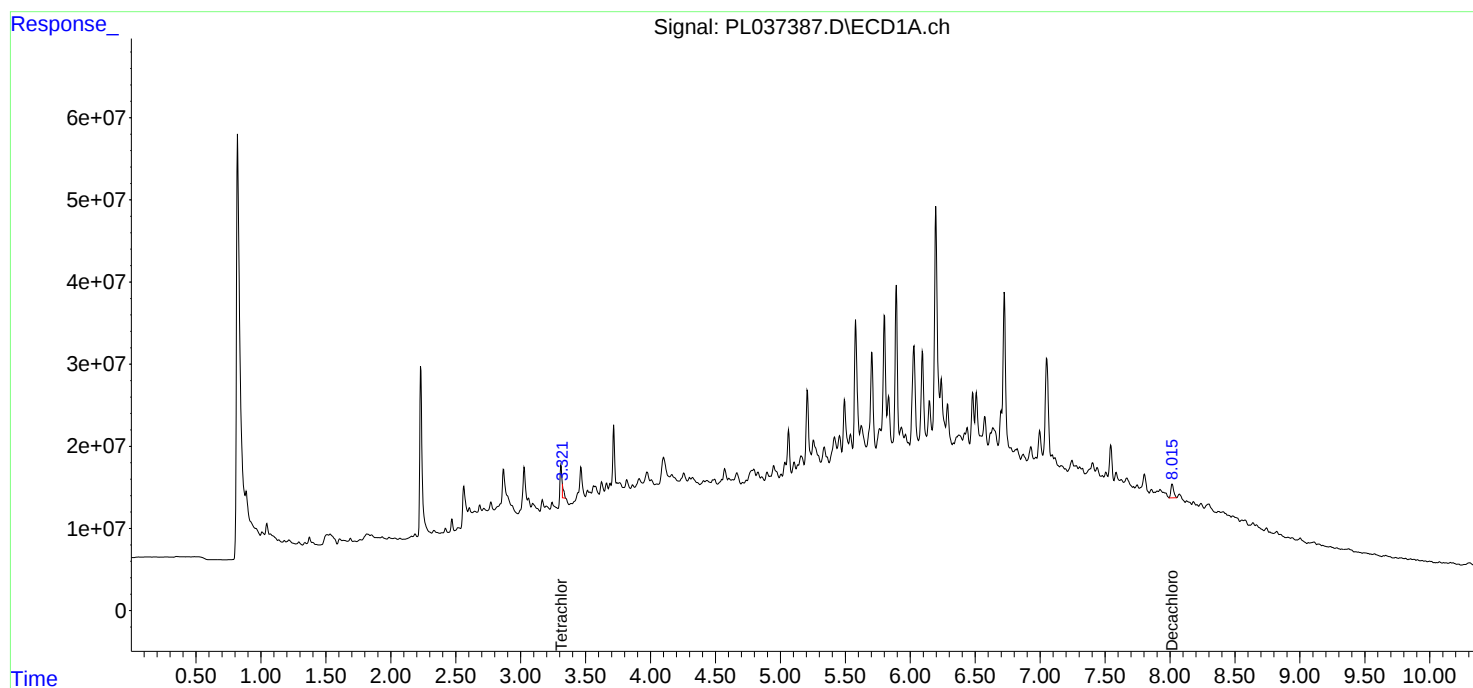

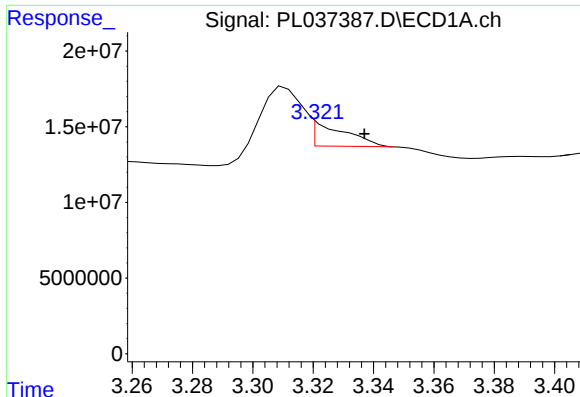


#1 Tetrachloro-m-xylene

R.T.: 3.321 min
Delta R.T.: -0.016 min
Response: 11235181
Conc: 1.42 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CS-PAINT-CHIP


Manual Integrations
APPROVED

ugo
6/26/2018 2:49:04 PM

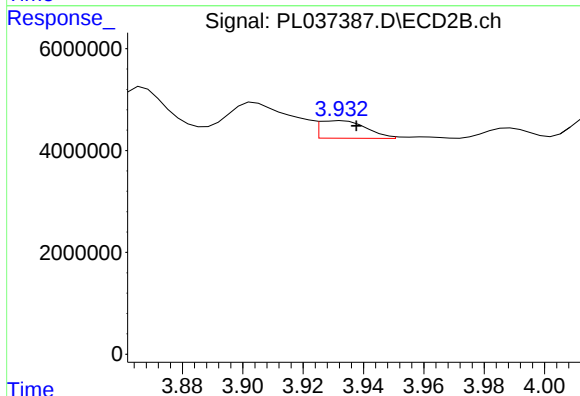


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.006 min
Response: 3496285
Conc: 1.26 ng/ml m

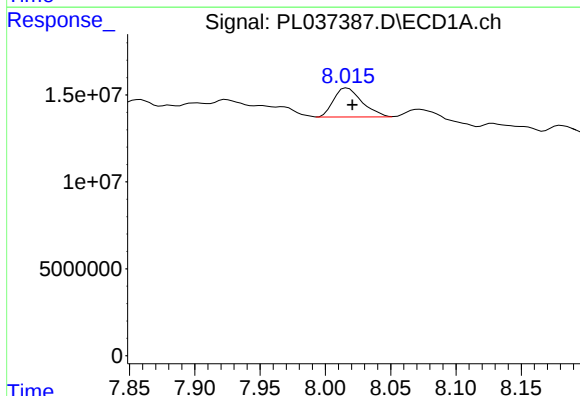

#28 Decachlorobiphenyl

R.T.: 8.015 min
Delta R.T.: -0.005 min
Response: 25330070
Conc: 4.20 ng/ml m

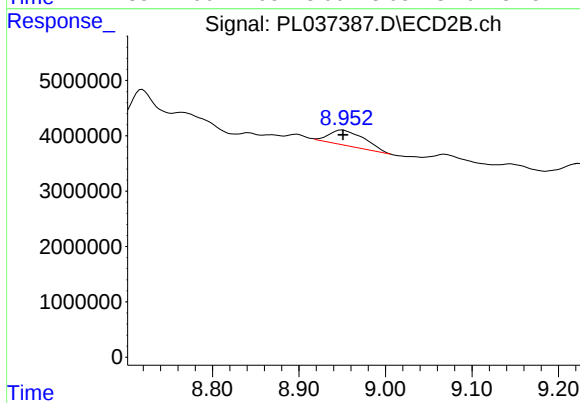

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: 0.000 min
Response: 7796540
Conc: 3.93 ng/ml m