

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062519\
 Data File : PL049822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2019 15:27
 Operator : SM\AJ
 Sample : K3155-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BAT-B11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:09:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.933	250.5E6	65058520	22.208	21.249
28)	SA Decachlor...	7.989	8.969	257.3E6	68894854	20.252	20.522
Target Compounds							
10)	B gamma-Chl...	5.187f	0.000	29636432	0	1.734	N.D. #
12)	B 4,4'-DDE	5.432	6.263	42989791	13575947	2.581	3.912 #
13)	MA Dieldrin	5.554	0.000	29161058	0	1.751	N.D. #
14)	MA Endrin	0.000	6.622	0	6594835	N.D.	2.089 #
17)	MA 4,4'-DDT	6.172	0.000	42360810	0	3.191	N.D. #
25)	Chlordane-3	5.187f	0.000	29636432	0	15.779	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062519\
Data File : PL049822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2019 15:27
Operator : SM\AJ
Sample : K3155-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BAT-B11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:09:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

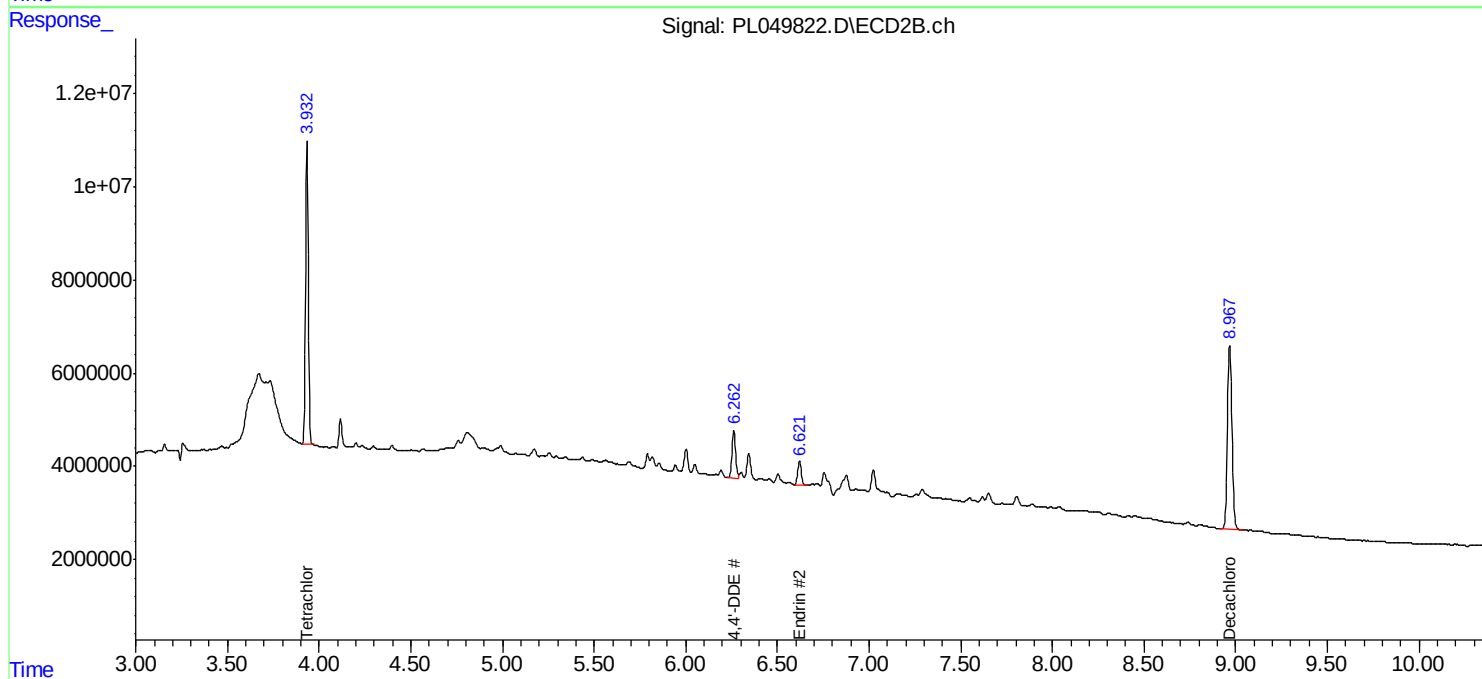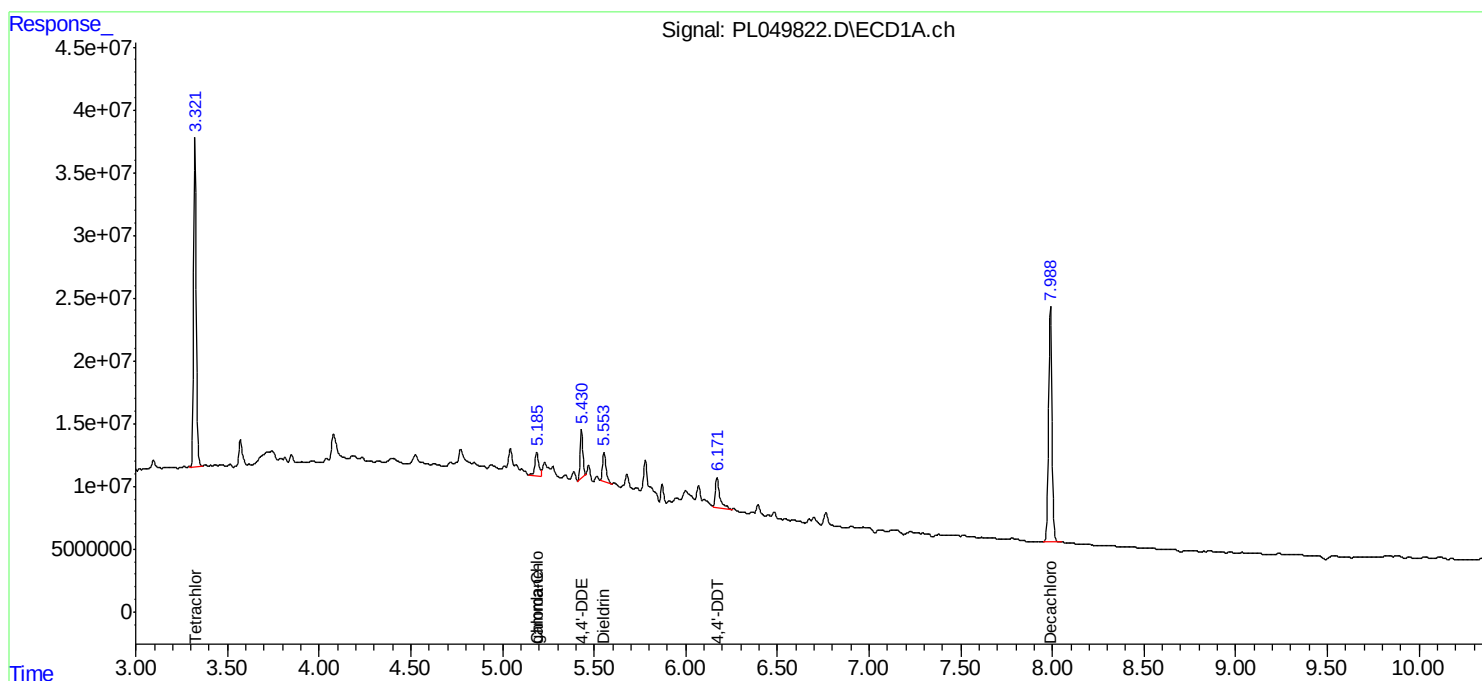


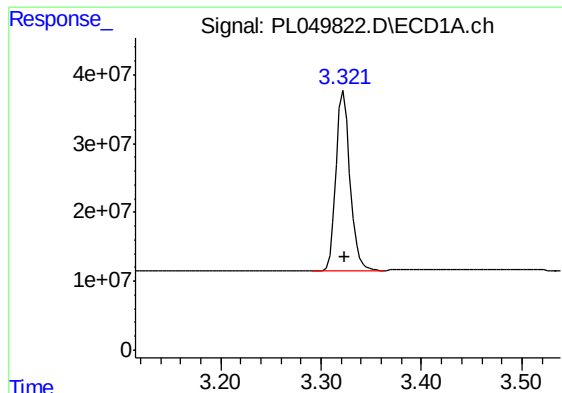

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: -0.001 min
Response: 250454068
Conc: 22.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B11

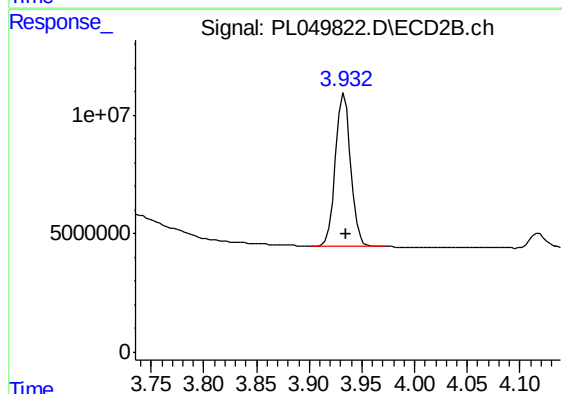


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.002 min
Response: 65058520
Conc: 21.25 ng/ml

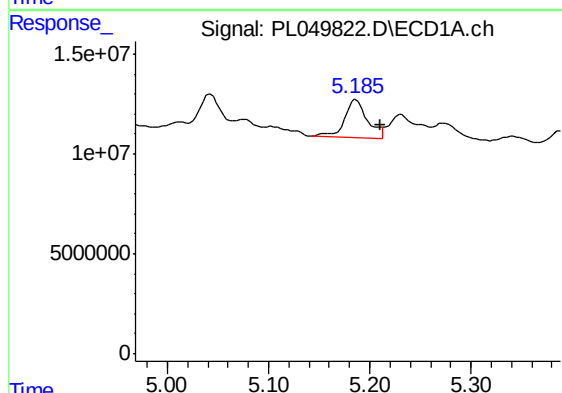


#10 gamma-Chlordane

R.T.: 5.187 min
Delta R.T.: -0.024 min
Response: 29636432
Conc: 1.73 ng/ml

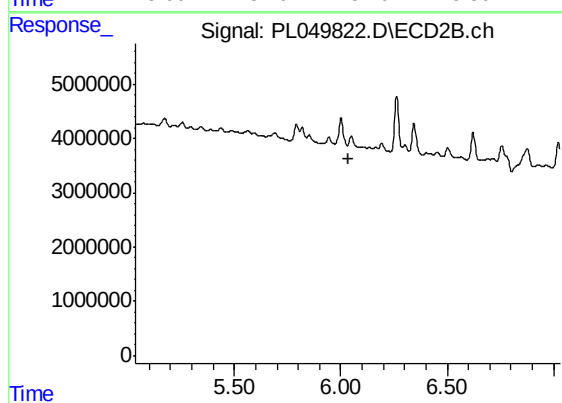

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.034 min
Response: 0
Conc: N.D.

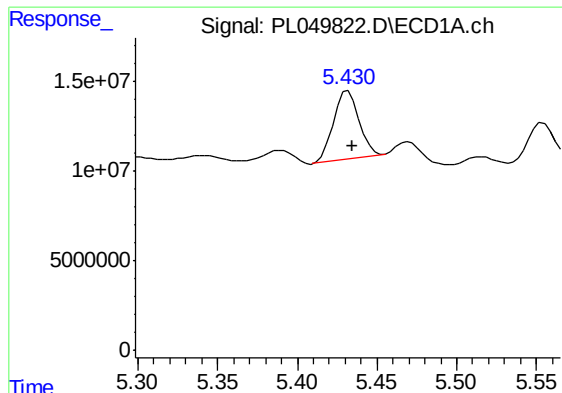

#12 4,4'-DDE


R.T.: 5.432 min
Delta R.T.: -0.002 min
Response: 42989791
Conc: 2.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B11

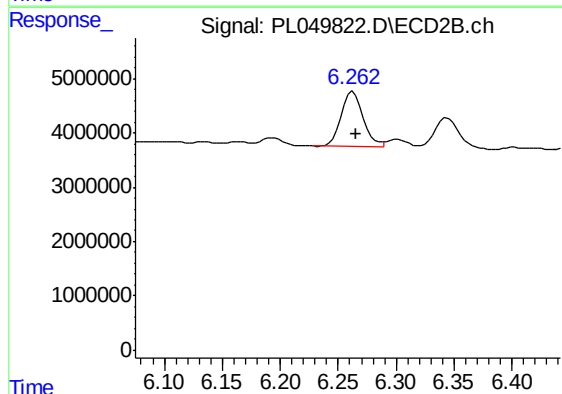


#12 4,4'-DDE

R.T.: 6.263 min
Delta R.T.: -0.003 min
Response: 13575947
Conc: 3.91 ng/ml

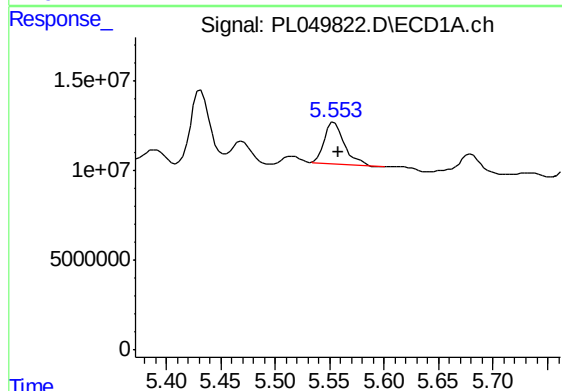


#13 Dieldrin

R.T.: 5.554 min
Delta R.T.: -0.003 min
Response: 29161058
Conc: 1.75 ng/ml

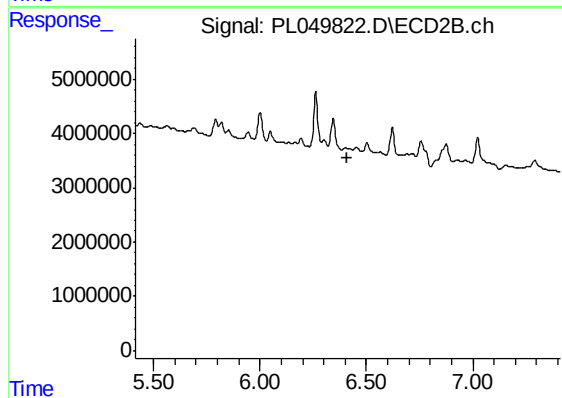

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.412 min
Response: 0
Conc: N.D.

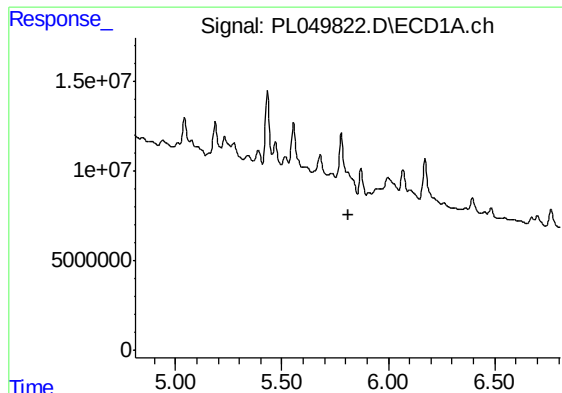

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.811 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BAT-B11

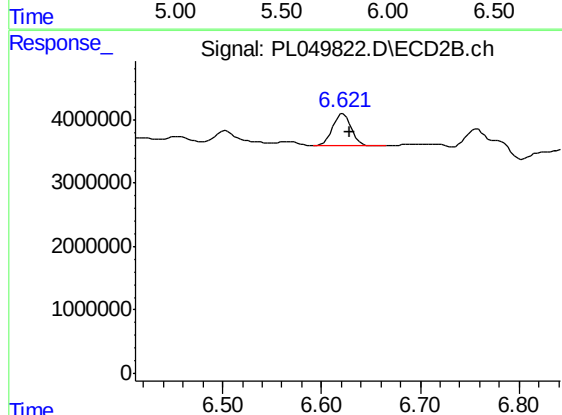


#14 Endrin

R.T.: 6.622 min
Delta R.T.: -0.007 min
Response: 6594835
Conc: 2.09 ng/ml

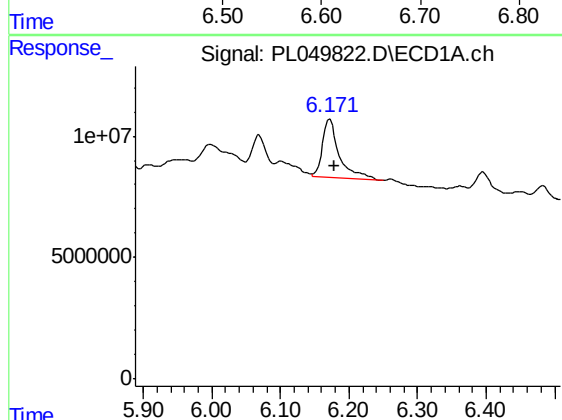


#17 4,4'-DDT

R.T.: 6.172 min
Delta R.T.: -0.008 min
Response: 42360810
Conc: 3.19 ng/ml

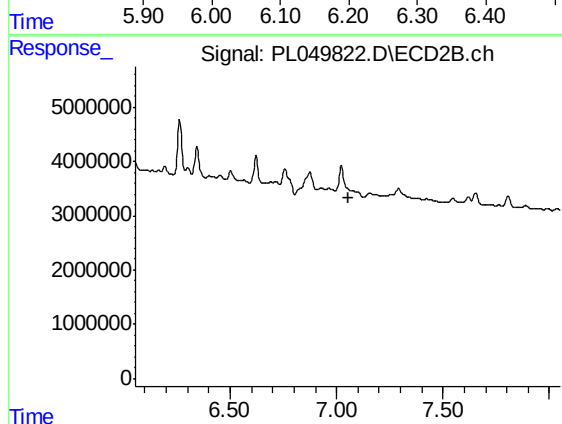

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.054 min
Response: 0
Conc: N.D.

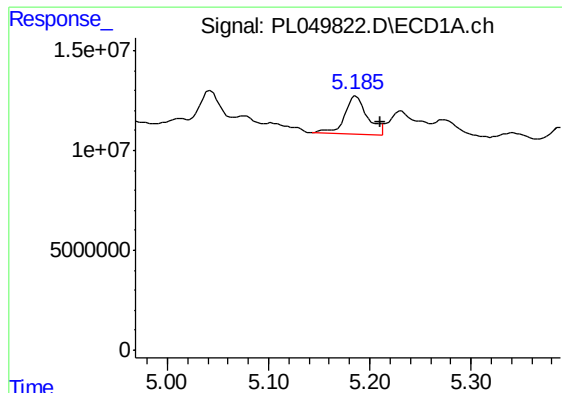

#25 Chlordane-3


R.T.: 5.187 min
Delta R.T.: -0.024 min
Response: 29636432
Conc: 15.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B11

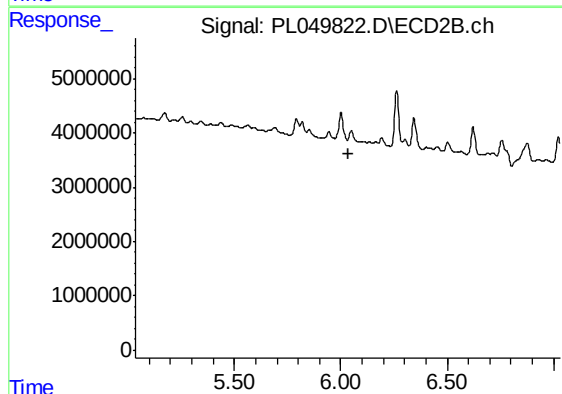


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.035 min
Response: 0
Conc: N.D.

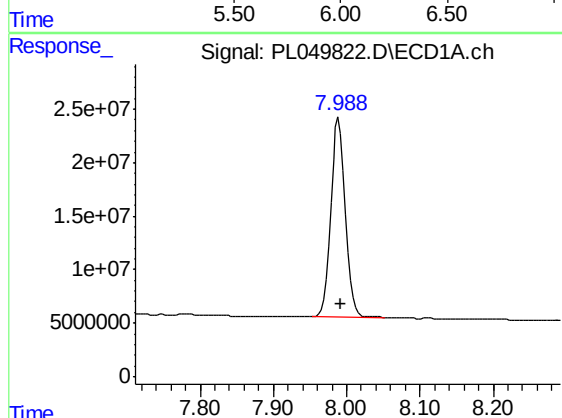

#28 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.003 min
Response: 257334717
Conc: 20.25 ng/ml

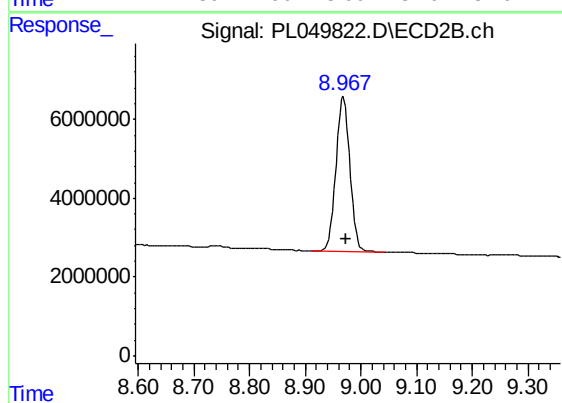

#28 Decachlorobiphenyl

R.T.: 8.969 min
Delta R.T.: -0.004 min
Response: 68894854
Conc: 20.52 ng/ml