

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062519\
 Data File : PL049856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2019 00:17
 Operator : SM\AJ
 Sample : K3510-02
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-04-062419

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:17:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.934	181.5E6	52682686	16.090	17.207
28)	SA Decachlor...	7.987	8.968	195.8E6	53930648	15.407	16.065
Target Compounds							
6)	B beta-BHC	4.278	0.000	33587931	0	4.592	N.D. #
7)	B delta-BHC	0.000	4.968f	0	7221162	N.D.	1.833 #
9)	A Endosulfan I	5.300f	6.135f	56408437	25460959	3.646	7.494 #
11)	B alpha-Chl...	0.000	6.135f	0	25460959	N.D.	6.884 #
23)	Chlordane-1	4.176	0.000	80938198	0	142.103	N.D. #
24)	Chlordane-2	4.661	0.000	122.1E6	0	209.120	N.D. #
26)	Chlordane-4	0.000	6.135f	0	25460959	N.D.	42.839 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062519\
Data File : PL049856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2019 00:17
Operator : SM\AJ
Sample : K3510-02
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TR-04-062419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:17:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

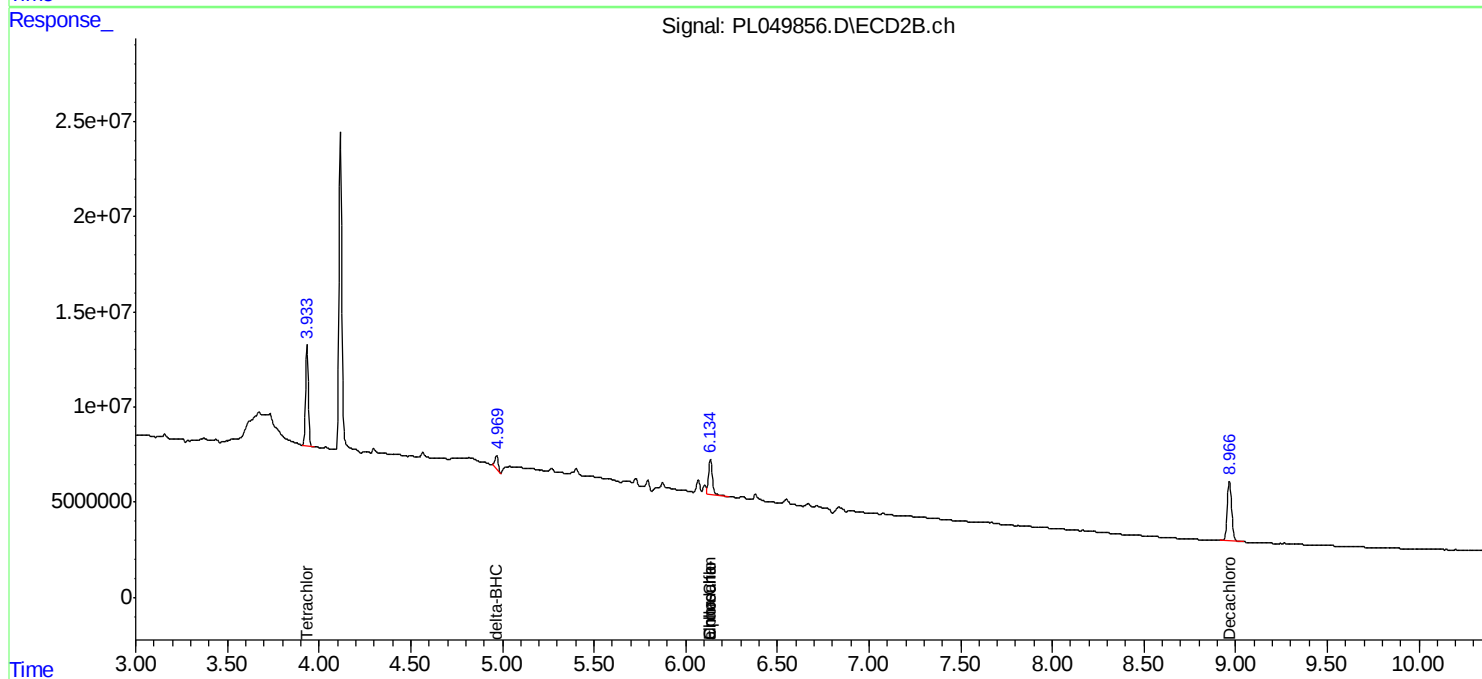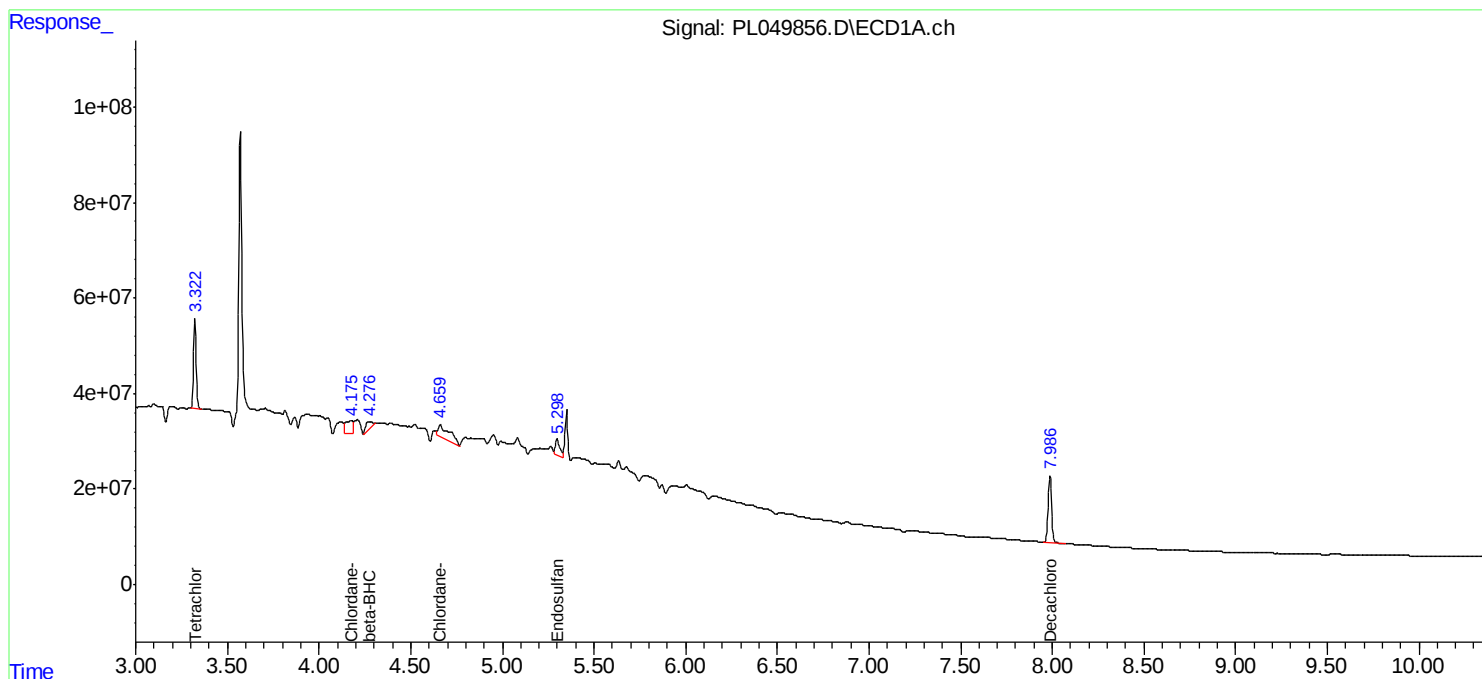


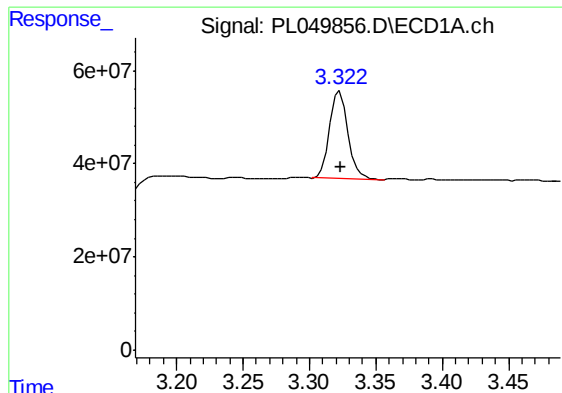

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: -0.001 min
Response: 181461214
Conc: 16.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-062419

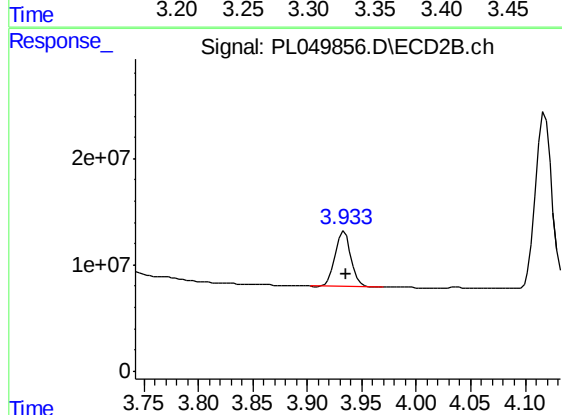


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.001 min
Response: 52682686
Conc: 17.21 ng/ml

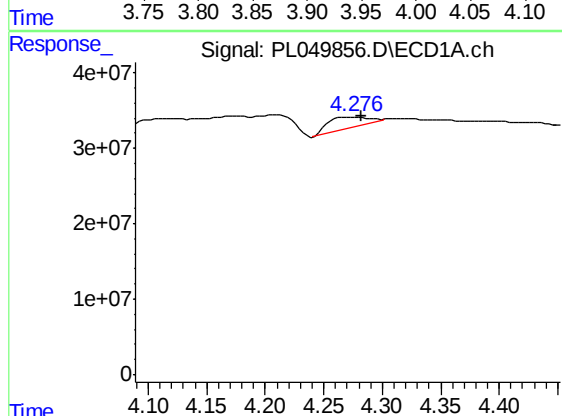


#6 beta-BHC

R.T.: 4.278 min
Delta R.T.: -0.004 min
Response: 33587931
Conc: 4.59 ng/ml

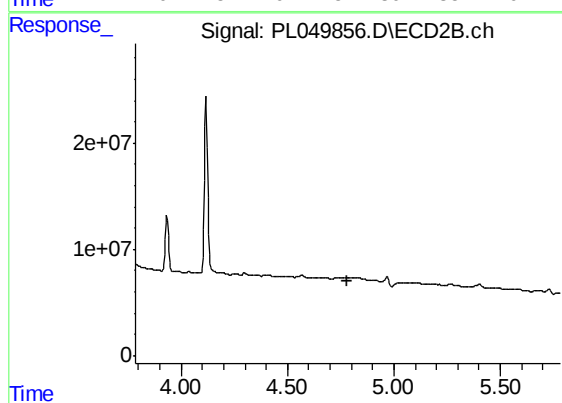

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.783 min
Response: 0
Conc: N.D.

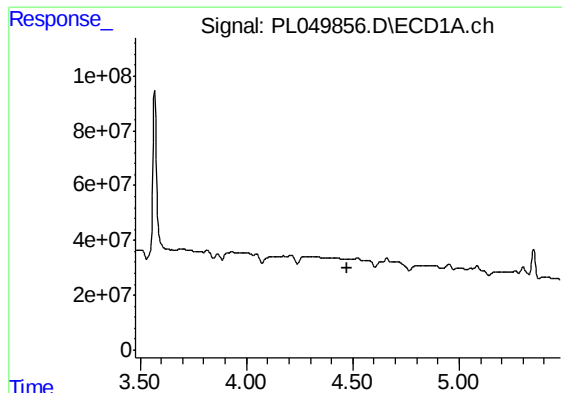

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TR-04-062419

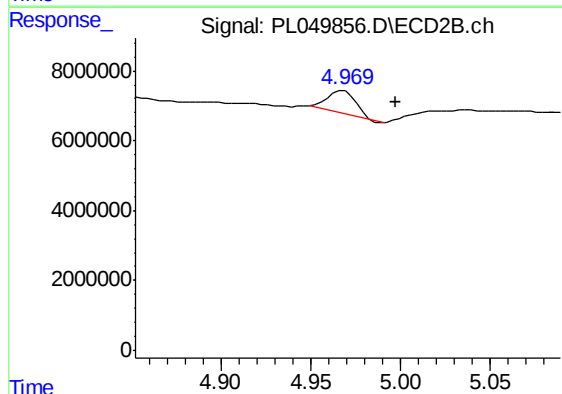


#7 delta-BHC

R.T.: 4.968 min
Delta R.T.: -0.029 min
Response: 7221162
Conc: 1.83 ng/ml

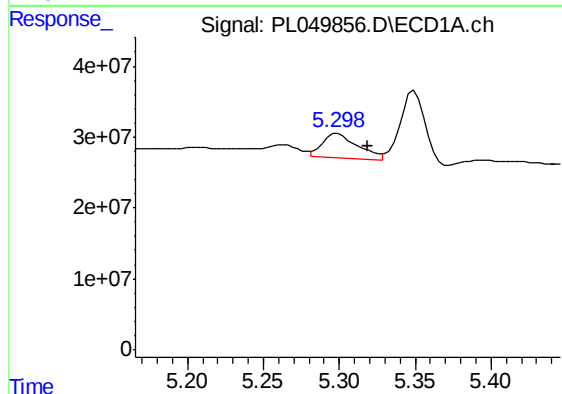


#9 Endosulfan I

R.T.: 5.300 min
Delta R.T.: -0.019 min
Response: 56408437
Conc: 3.65 ng/ml

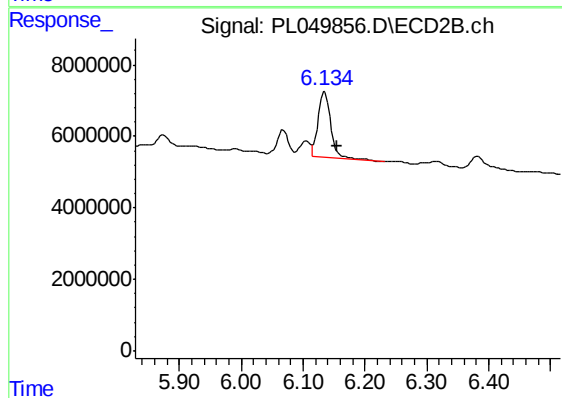

#9 Endosulfan I


R.T.: 6.135 min
Delta R.T.: -0.020 min
Response: 25460959
Conc: 7.49 ng/ml

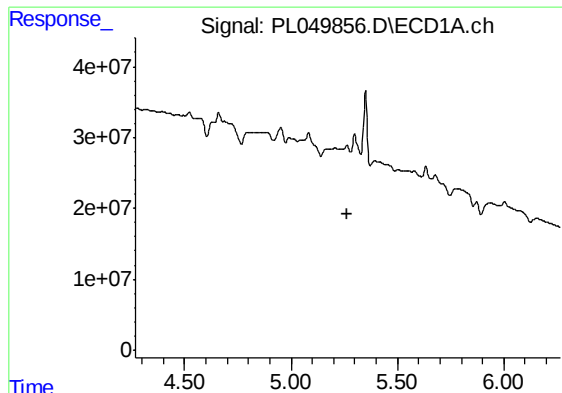

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TR-04-062419

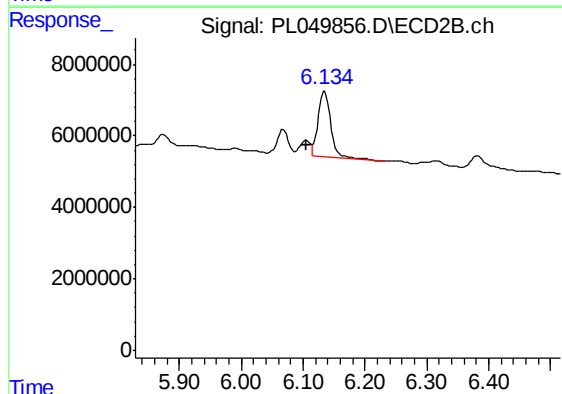


#11 alpha-Chlordane

R.T.: 6.135 min
Delta R.T.: 0.029 min
Response: 25460959
Conc: 6.88 ng/ml

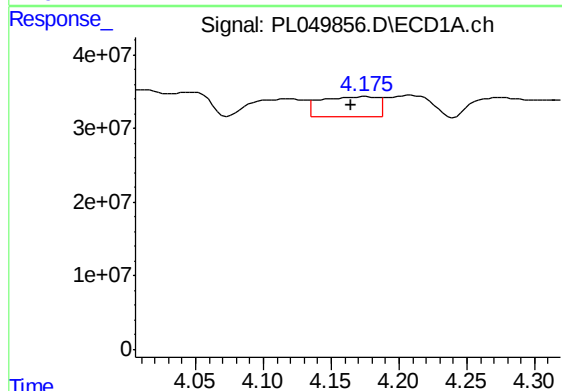


#23 Chlordane-1

R.T.: 4.176 min
Delta R.T.: 0.012 min
Response: 80938198
Conc: 142.10 ng/ml

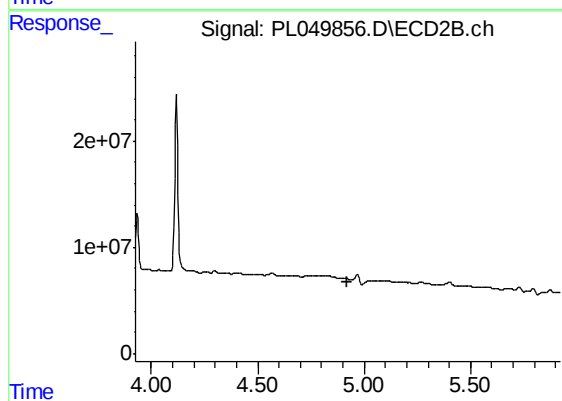

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.922 min
Response: 0
Conc: N.D.

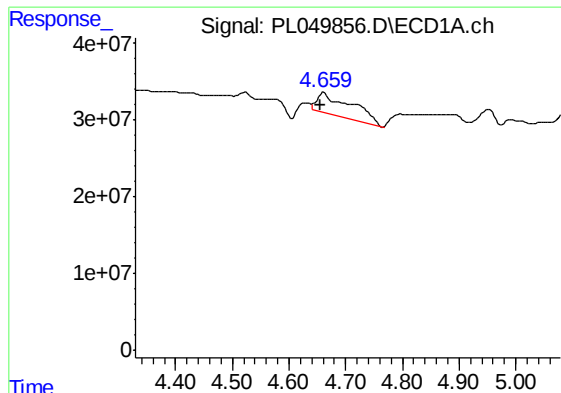

#24 Chlordane-2


R.T.: 4.661 min
Delta R.T.: 0.006 min
Response: 122133095
Conc: 209.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-062419

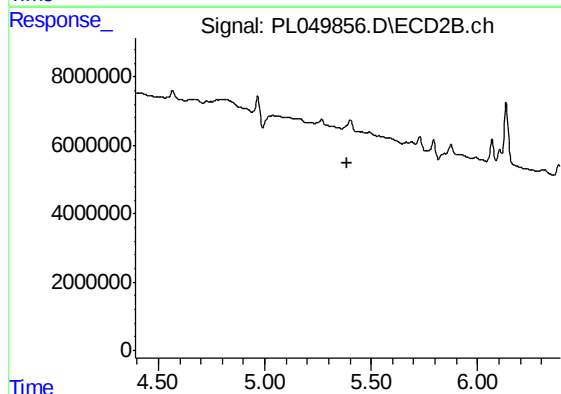


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.390 min
Response: 0
Conc: N.D.

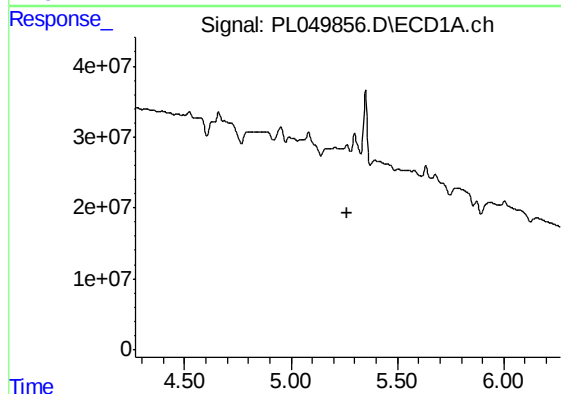


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.266 min
Response: 0
Conc: N.D.

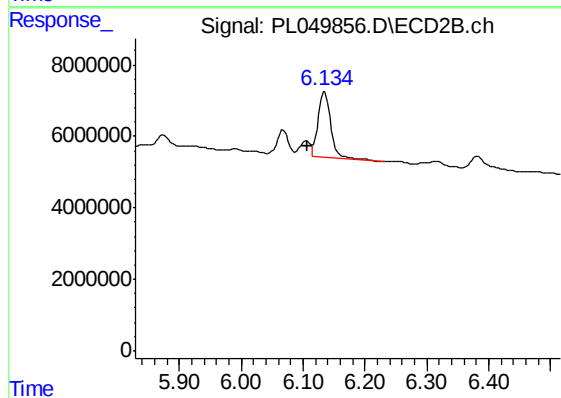

#26 Chlordane-4


R.T.: 6.135 min
Delta R.T.: 0.027 min
Response: 25460959
Conc: 42.84 ng/ml

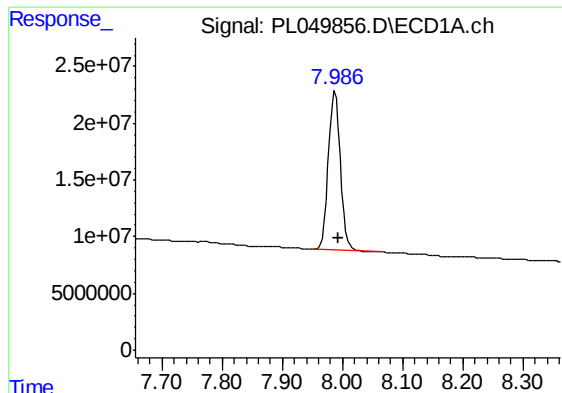

#28 Decachlorobiphenyl

R.T.: 7.987 min
Delta R.T.: -0.005 min
Response: 195764555
Conc: 15.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-062419

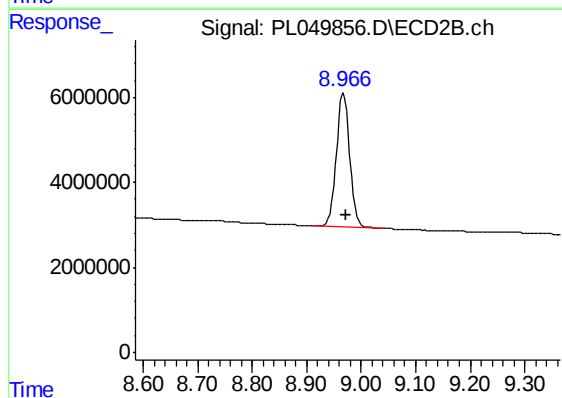

#28 Decachlorobiphenyl

R.T.: 8.968 min
Delta R.T.: -0.005 min
Response: 53930648
Conc: 16.06 ng/ml