

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062519\
 Data File : PL049846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2019 21:46
 Operator : SM\AJ
 Sample : K3511-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-2

Manual Integrations
 APPROVED

Ankita
 6/26/2019 8:28:41 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:15:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.322	3.934	225.0E6	60972336	19.950	19.914
2) SA Decachlor...	7.987	8.968	172.4E6	51415133	13.568	15.316
Target Compounds						
12) B 4,4'-DDE	5.427	6.263	13650506	2585602	0.819m	0.745m
16) A 4,4'-DDD	5.942	6.753	58999610	16089399	4.674	6.155 #
17) MA 4,4'-DDT	6.172	7.049	6624197	1295461	0.499m	0.442m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062519\
Data File : PL049846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2019 21:46
Operator : SM\AJ
Sample : K3511-03
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Ankita
6/26/2019 8:28:41 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:15:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

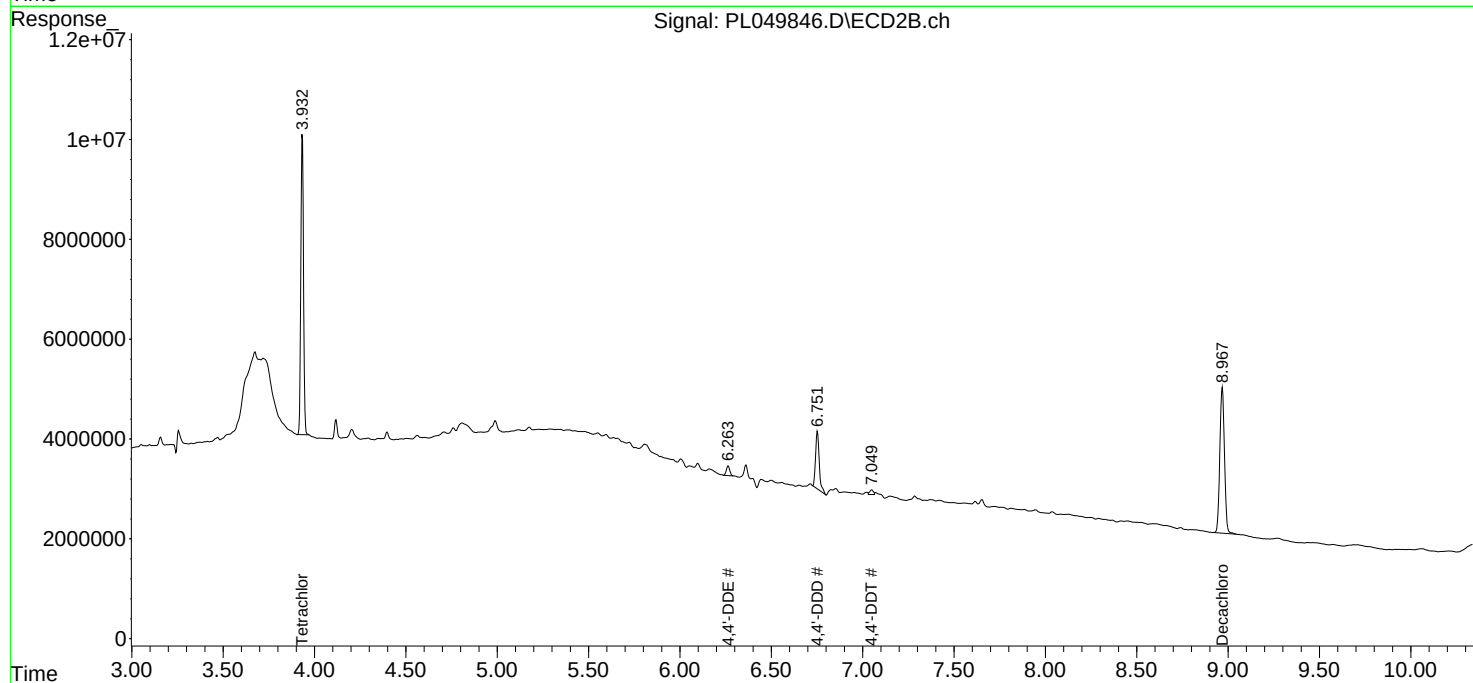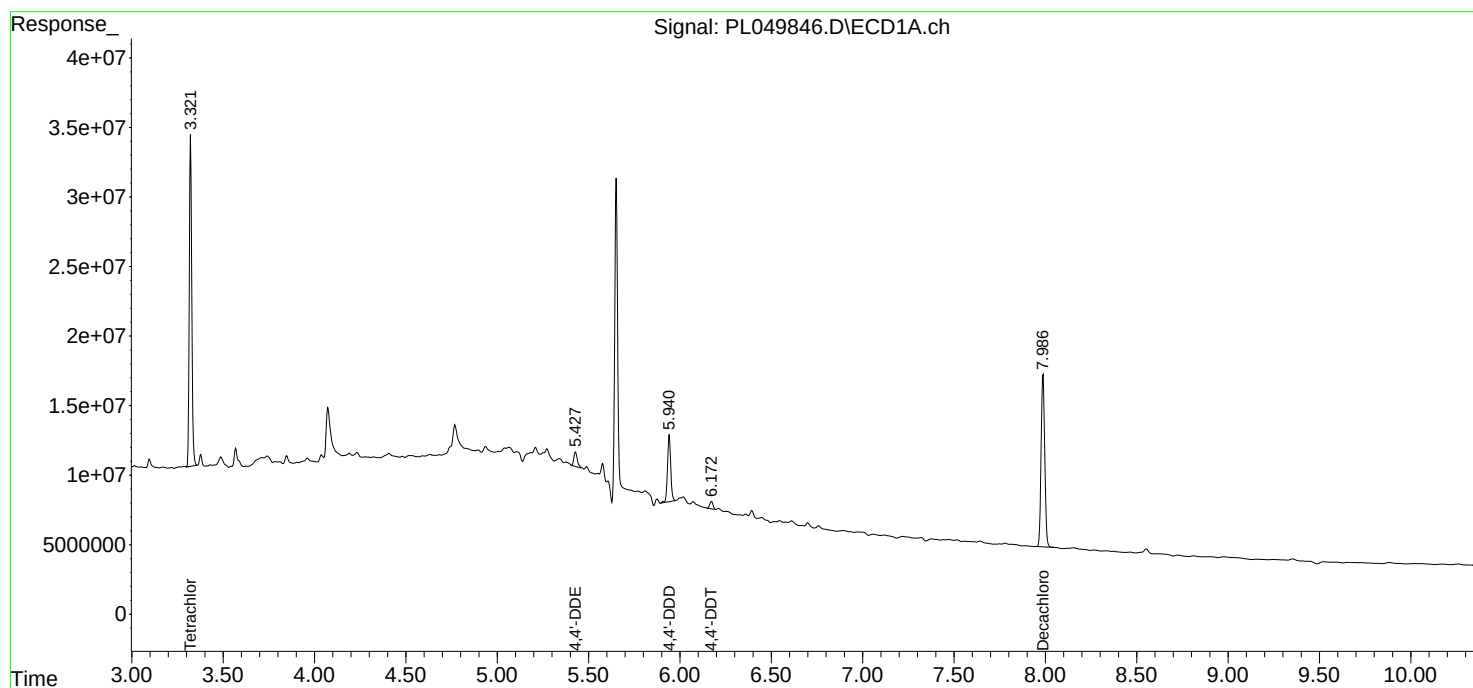

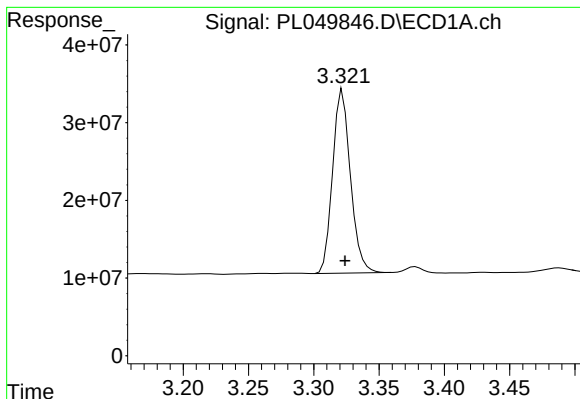


#1 Tetrachloro-m-xylene

R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 224987040
Conc: 19.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Ankita
6/26/2019 8:28:41 AM

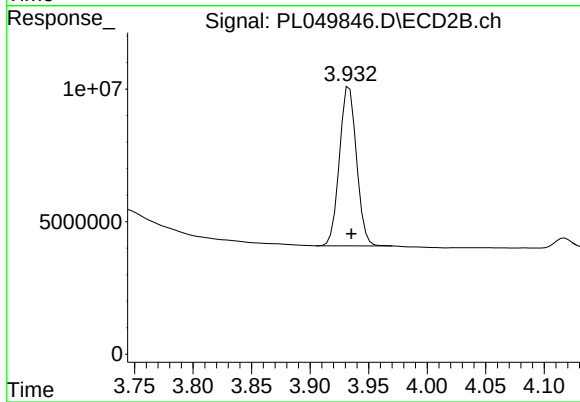


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.002 min
Response: 60972336
Conc: 19.91 ng/ml

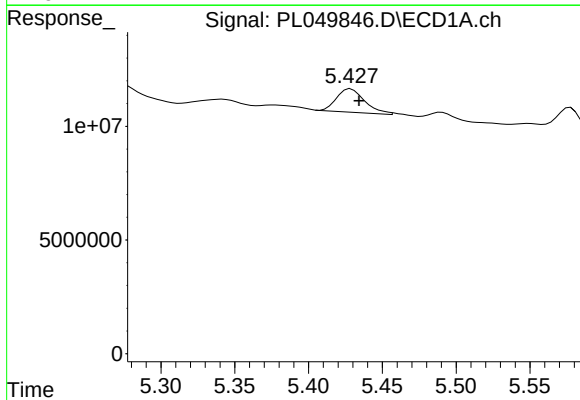


#12 4,4'-DDE

R.T.: 5.427 min
Delta R.T.: -0.007 min
Response: 13650506
Conc: 0.82 ng/ml m

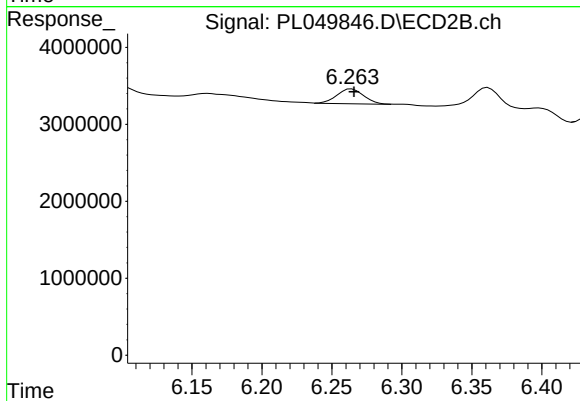

#12 4,4'-DDE

R.T.: 6.263 min
Delta R.T.: -0.003 min
Response: 2585602
Conc: 0.75 ng/ml m

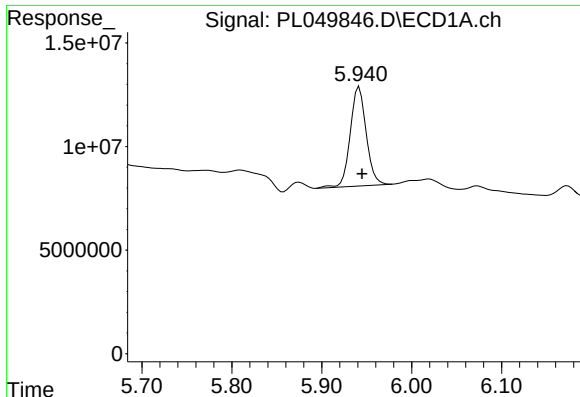


#16 4,4'-DDD

R.T.: 5.942 min
Delta R.T.: -0.003 min
Response: 58999610
Conc: 4.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Ankita
6/26/2019 8:28:41 AM

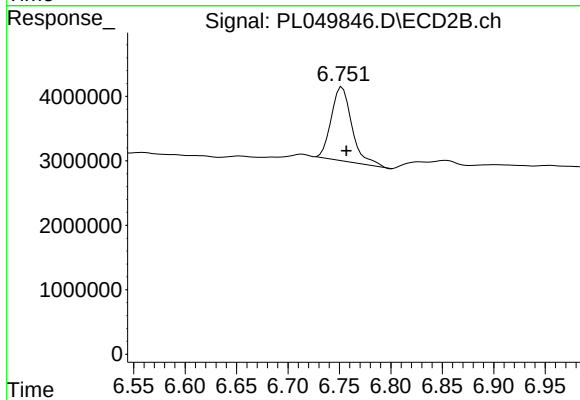


#16 4,4'-DDD

R.T.: 6.753 min
Delta R.T.: -0.004 min
Response: 16089399
Conc: 6.15 ng/ml

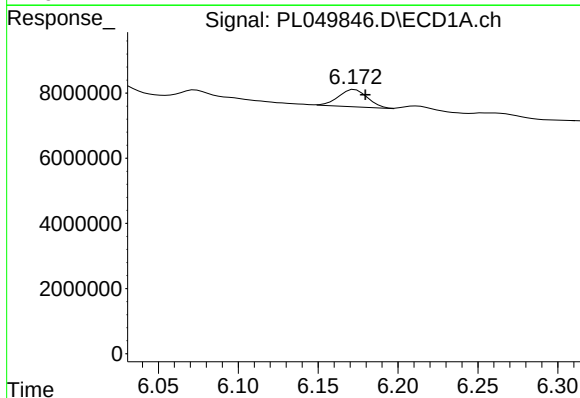


#17 4,4'-DDT

R.T.: 6.172 min
Delta R.T.: -0.008 min
Response: 6624197
Conc: 0.50 ng/ml m

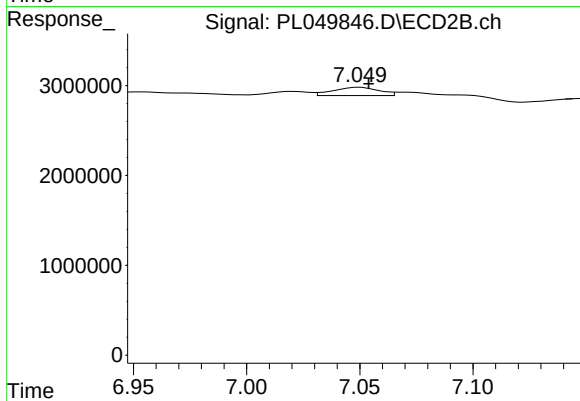

#17 4,4'-DDT

R.T.: 7.049 min
Delta R.T.: -0.005 min
Response: 1295461
Conc: 0.44 ng/ml m

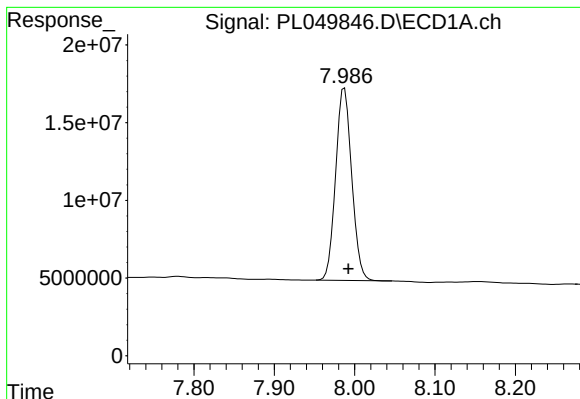

#28 Decachlorobiphenyl

R.T.: 7.987 min

Delta R.T.: -0.005 min


Response: 172406624

Conc: 13.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-2

Manual Integrations
APPROVED

Ankita
6/26/2019 8:28:41 AM

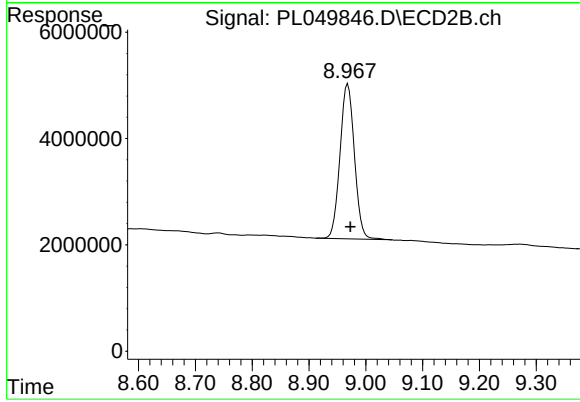

#28 Decachlorobiphenyl

R.T.: 8.968 min

Delta R.T.: -0.005 min

Response: 51415133

Conc: 15.32 ng/ml