

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062520\
 Data File : PL059507.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2020 15:49
 Operator : AJ\MA
 Sample : PB129762BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB129762BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 17:01:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 22 14:09:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.520	4.071	39015365	57441489	21.710	22.256
28)	SA Decachlor...	8.290	9.182	34669833	47575259	20.360	20.779
Target Compounds							
4)	MA Heptachlor	0.000	5.260	0	559424	N.D.	0.173 #
5)	MB Aldrin	0.000	5.571	0	100219	N.D.	0.033 #
8)	B Heptachlo...	0.000	5.936f	0	2864639	N.D.	1.141 #
9)	A Endosulfan I	0.000	6.315	0	135475	N.D.	0.050 #
14)	MA Endrin	0.000	6.819f	0	40924	N.D.	0.017 #
15)	B Endosulfa...	0.000	7.007	0	1975774	N.D.	0.779 #
18)	B Endrin al...	0.000	7.121	0	311356	N.D.	0.142 #
22)	Mirex	0.000	8.305f	0	253384	N.D.	0.128 #
23)	Chlordane-1	4.423f	0.000	692492	0	12.169	N.D. #
24)	Chlordane-2	0.000	5.571f	0	100219	N.D.	0.913 #
27)	Chlordane-5	0.000	7.069	0	913395	N.D.	10.549 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062520\
Data File : PL059507.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2020 15:49
Operator : AJ\MA
Sample : PB129762BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PB129762BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 17:01:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
Quant Title : GC Extractables
QLast Update : Mon Jun 22 14:09:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

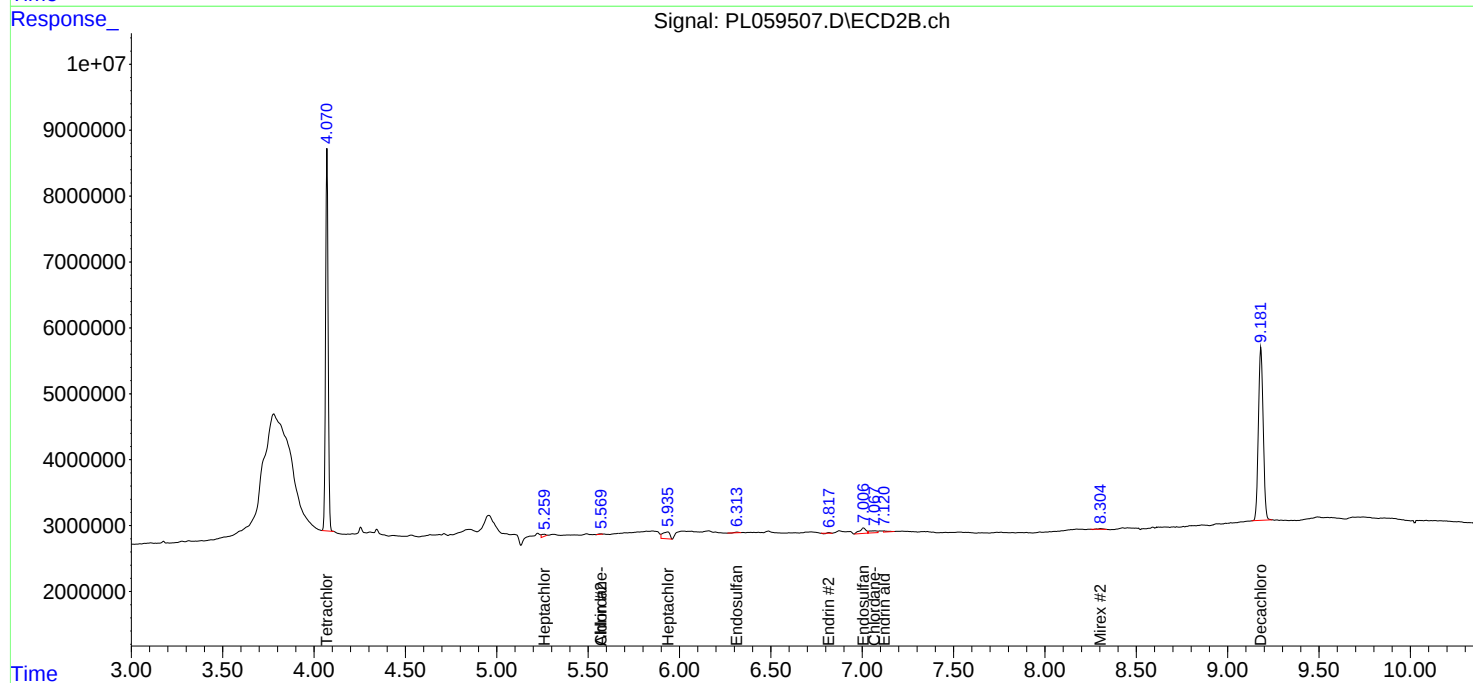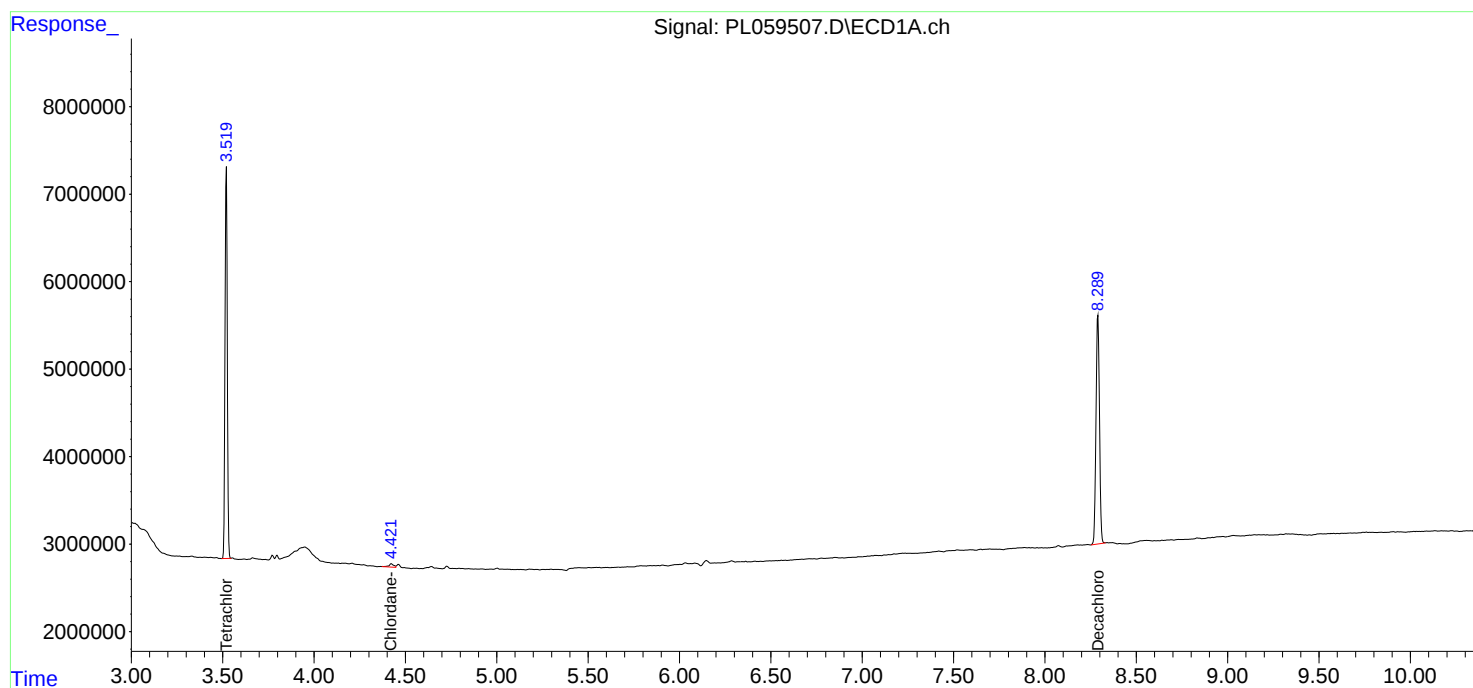


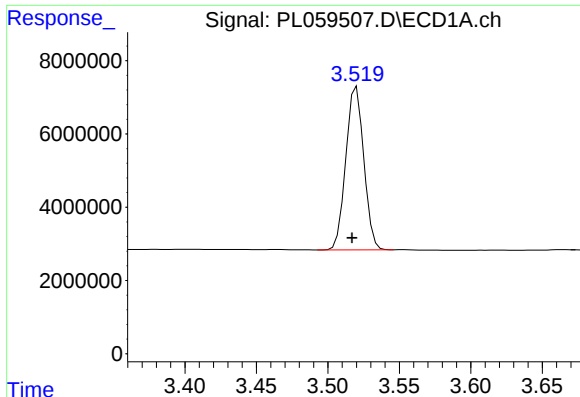

#1 Tetrachloro-m-xylene


R.T.: 3.520 min
Delta R.T.: 0.003 min
Response: 39015365
Conc: 21.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB129762BL

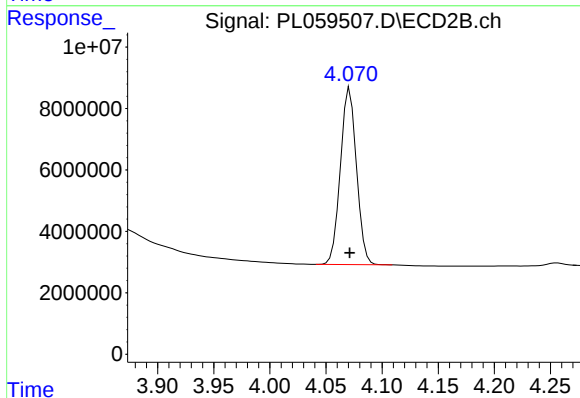


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: 0.000 min
Response: 57441489
Conc: 22.26 ng/ml

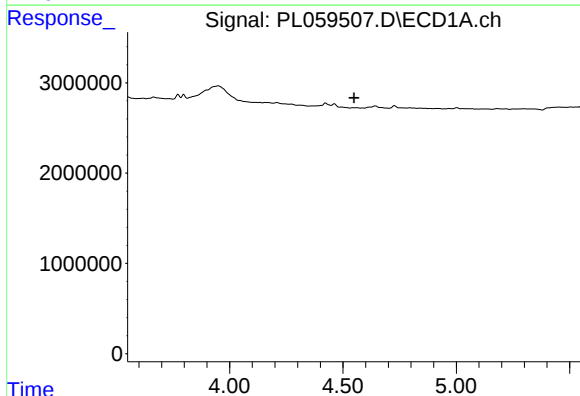


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.549 min
Response: 0
Conc: N.D.

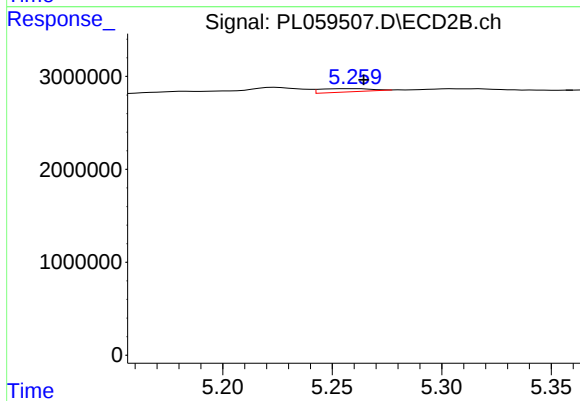

#4 Heptachlor


R.T.: 5.260 min
Delta R.T.: -0.004 min
Response: 559424
Conc: 0.17 ng/ml

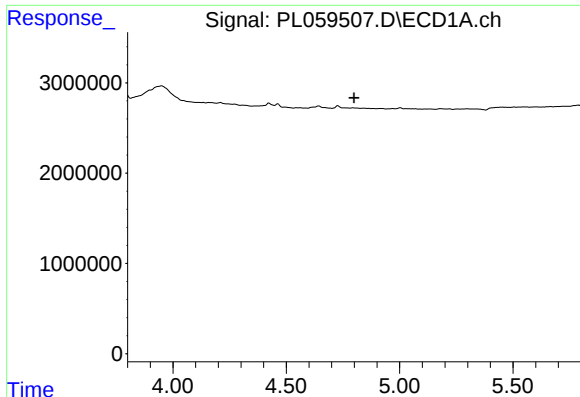

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 4.799 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB129762BL

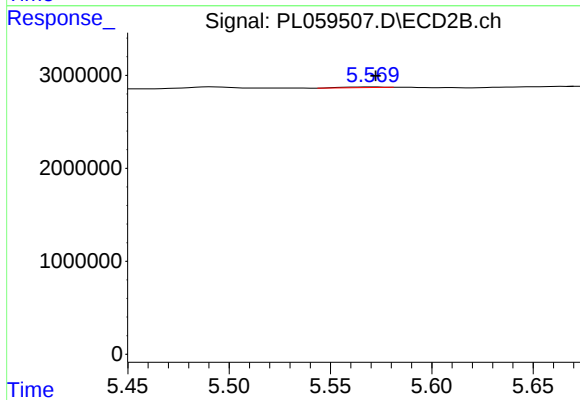


#5 Aldrin

R.T.: 5.571 min
Delta R.T.: -0.001 min
Response: 100219
Conc: 0.03 ng/ml

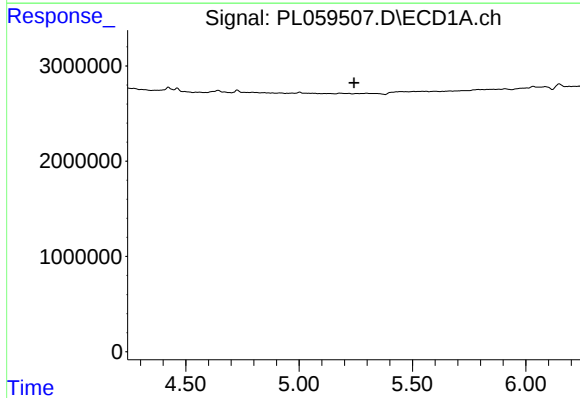


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.243 min
Response: 0
Conc: N.D.

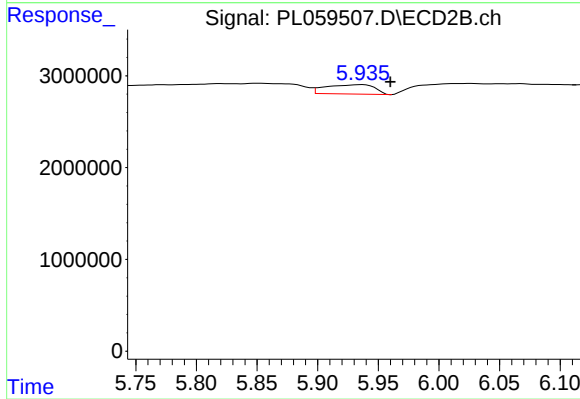

#8 Heptachlor epoxide


R.T.: 5.936 min
Delta R.T.: -0.024 min
Response: 2864639
Conc: 1.14 ng/ml

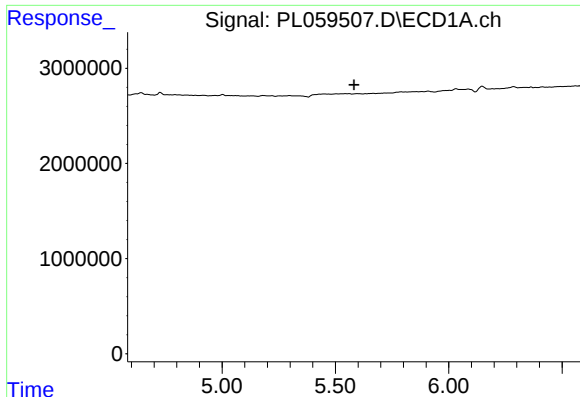

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB129762BL

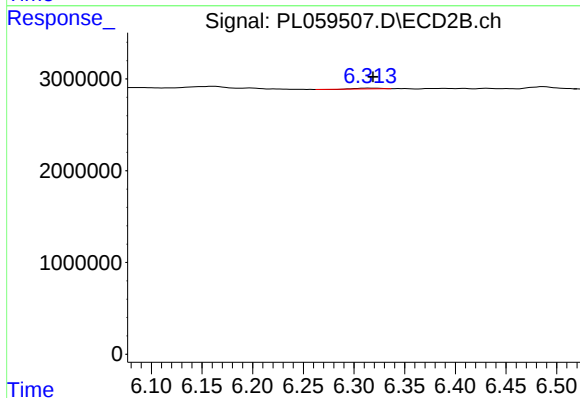


#9 Endosulfan I

R.T.: 6.315 min
Delta R.T.: -0.004 min
Response: 135475
Conc: 0.05 ng/ml

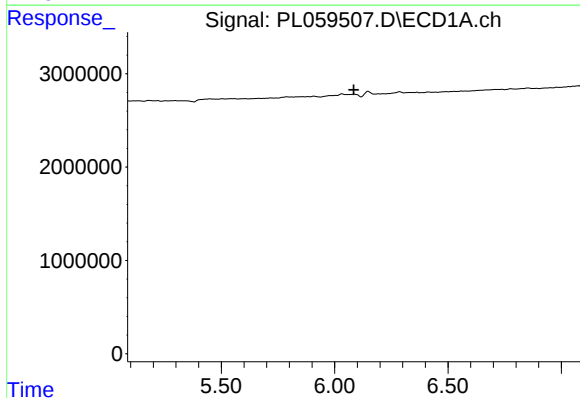


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.085 min
Response: 0
Conc: N.D.

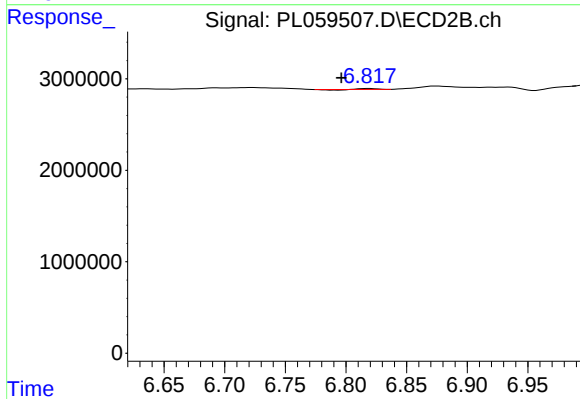

#14 Endrin


R.T.: 6.819 min
Delta R.T.: 0.023 min
Response: 40924
Conc: 0.02 ng/ml

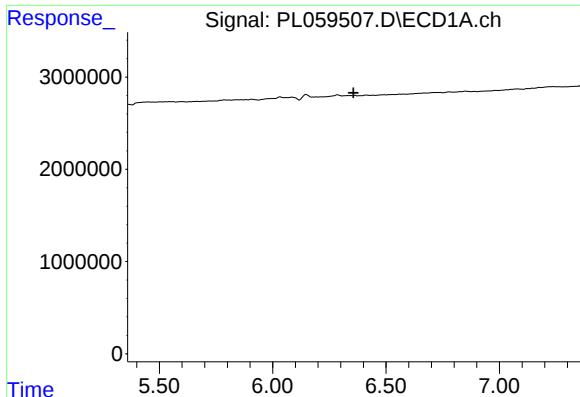

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB129762BL

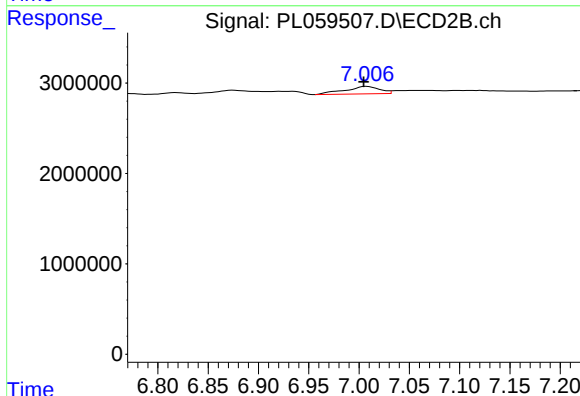


#15 Endosulfan II

R.T.: 7.007 min
Delta R.T.: 0.002 min
Response: 1975774
Conc: 0.78 ng/ml

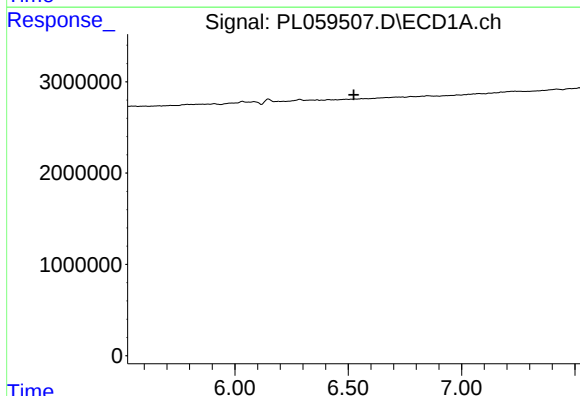


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.525 min
Response: 0
Conc: N.D.

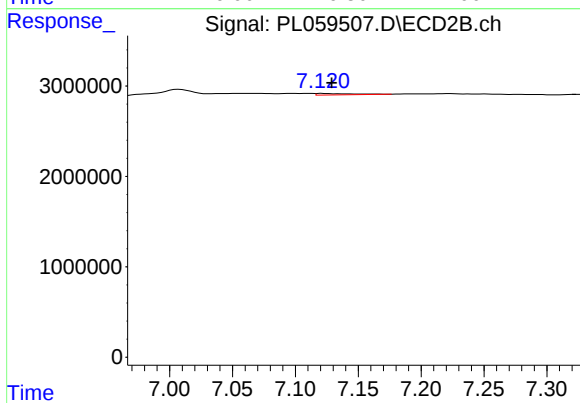

#18 Endrin aldehyde


R.T.: 7.121 min
Delta R.T.: -0.008 min
Response: 311356
Conc: 0.14 ng/ml

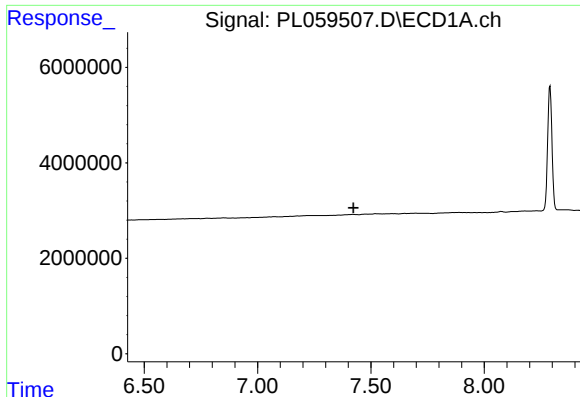

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.423 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB129762BL

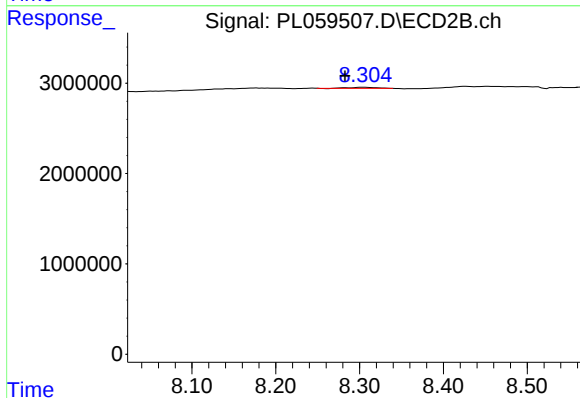


#22 Mirex

R.T.: 8.305 min
Delta R.T.: 0.022 min
Response: 253384
Conc: 0.13 ng/ml

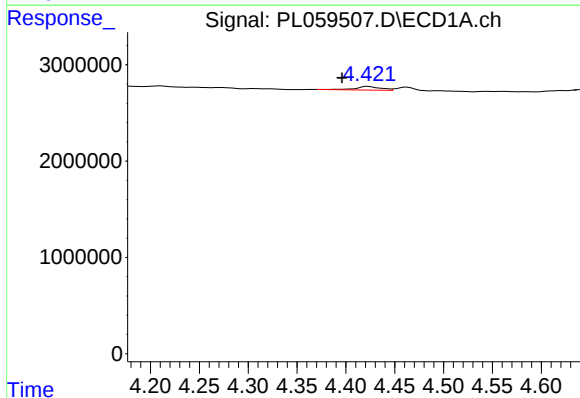


#23 Chlordane-1

R.T.: 4.423 min
Delta R.T.: 0.027 min
Response: 692492
Conc: 12.17 ng/ml

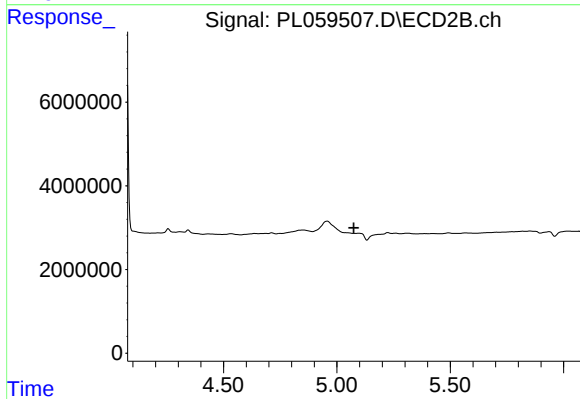

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.075 min
Response: 0
Conc: N.D.

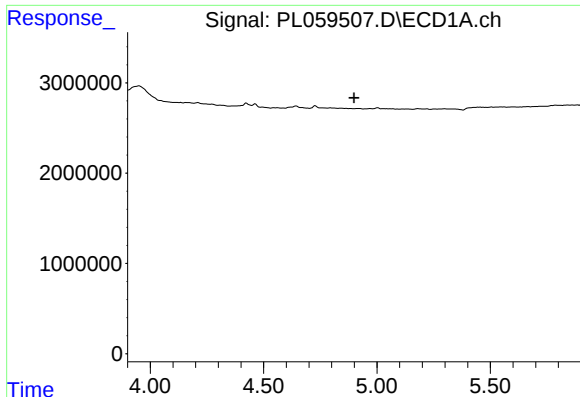

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.900 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB129762BL

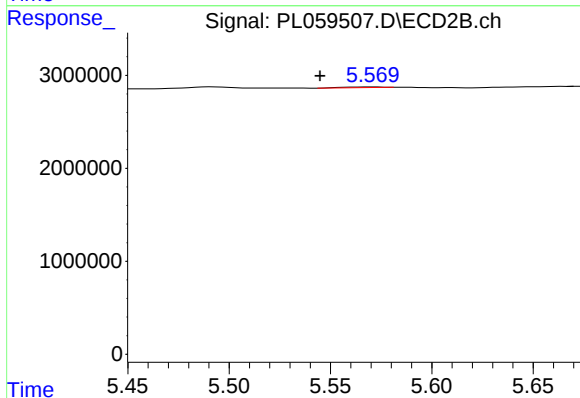


#24 Chlordane-2

R.T.: 5.571 min
Delta R.T.: 0.026 min
Response: 100219
Conc: 0.91 ng/ml

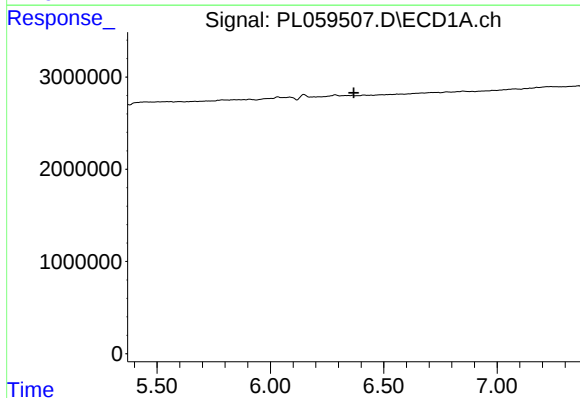


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.367 min
Response: 0
Conc: N.D.

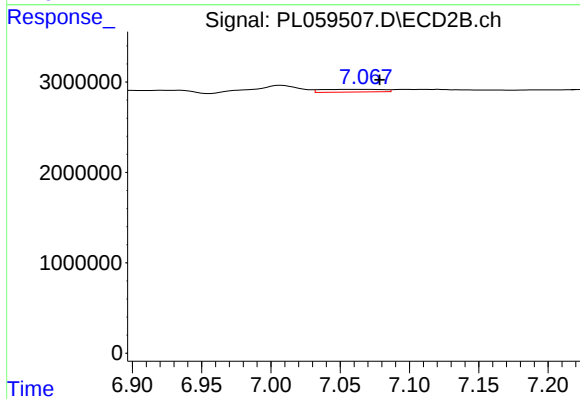

#27 Chlordane-5


R.T.: 7.069 min
Delta R.T.: -0.010 min
Response: 913395
Conc: 10.55 ng/ml

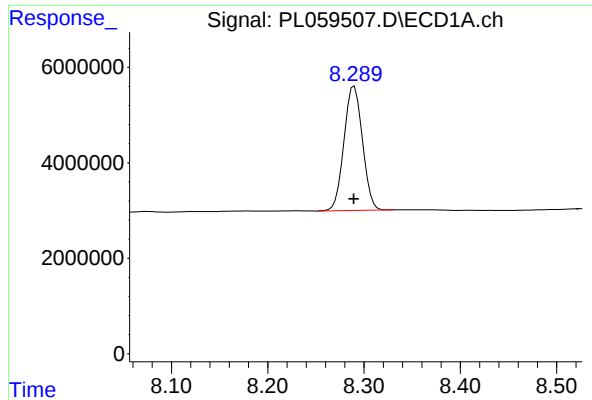

#28 Decachlorobiphenyl

R.T.: 8.290 min
Delta R.T.: 0.000 min
Response: 34669833
Conc: 20.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB129762BL

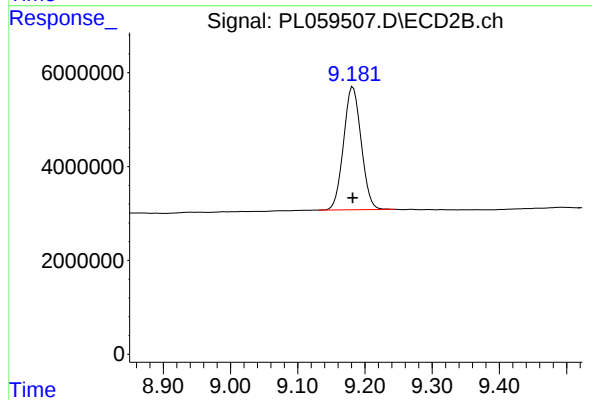

#28 Decachlorobiphenyl

R.T.: 9.182 min
Delta R.T.: 0.000 min
Response: 47575259
Conc: 20.78 ng/ml