

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062520\
 Data File : PL059512.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2020 17:04
 Operator : AJ\MA
 Sample : L3111-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 17:39:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 22 14:09:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.517	4.071	11403729	16759754	6.346	6.494
28)	SA Decachlor...	8.288	9.182	11115381	16195485	6.528	7.073
Target Compounds							
2)	A alpha-BHC	3.966	4.493f	721598	75793	0.280	0.022 #
4)	MA Heptachlor	0.000	5.265	0	566614	N.D.	0.175 #
6)	B beta-BHC	4.497	0.000	2495725	0	2.621	N.D. #
8)	B Heptachlo...	5.252	0.000	267370	0	0.178	N.D. #
15)	B Endosulfa...	6.367	7.007	59699	1744724	0.039	0.688 #
18)	B Endrin al...	0.000	7.153f	0	1348651	N.D.	0.615 #
22)	Mirex	0.000	8.282	0	152821	N.D.	0.077 #
27)	Chlordane-5	6.367	7.099f	59699	641309	1.064	7.406 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062520\
Data File : PL059512.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2020 17:04
Operator : AJ\MA
Sample : L3111-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-6-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 17:39:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
Quant Title : GC Extractables
QLast Update : Mon Jun 22 14:09:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

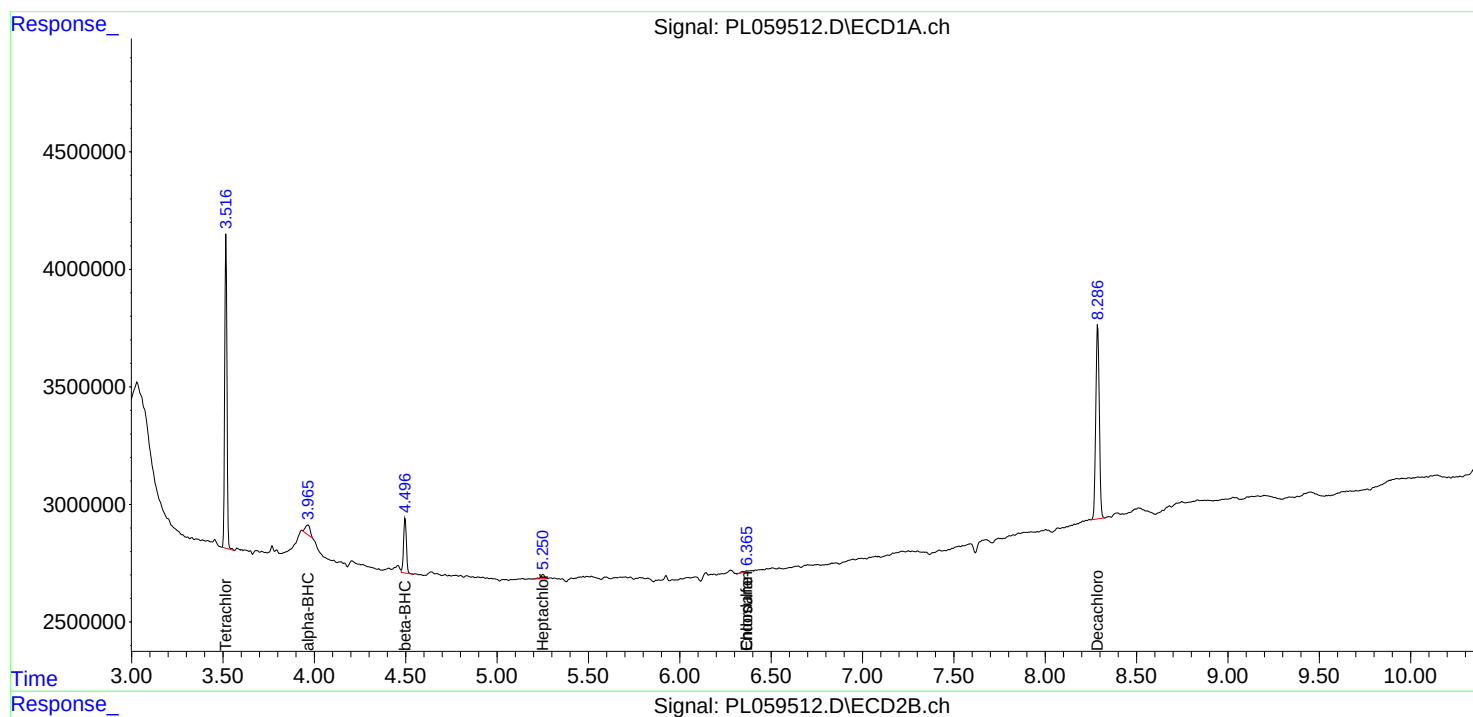


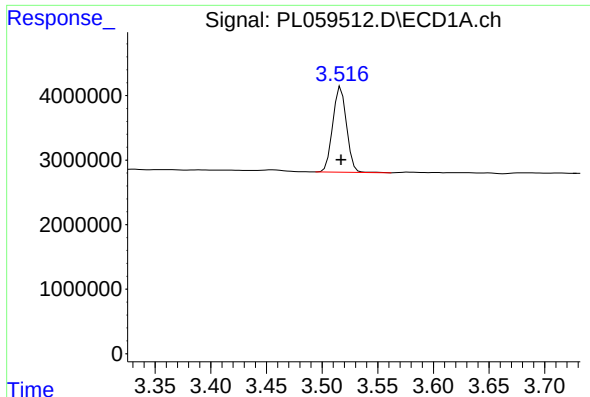

#1 Tetrachloro-m-xylene


R.T.: 3.517 min
Delta R.T.: 0.000 min
Response: 11403729
Conc: 6.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-S

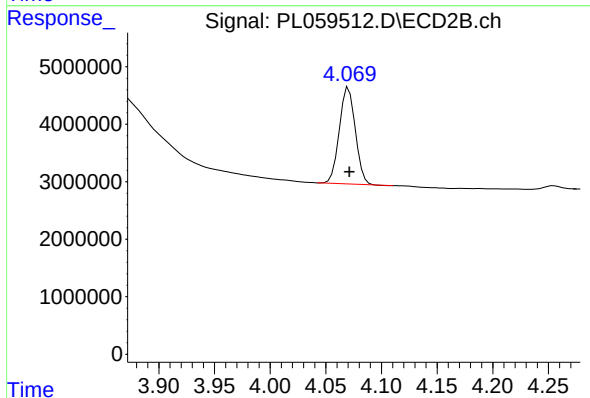


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: 0.000 min
Response: 16759754
Conc: 6.49 ng/ml

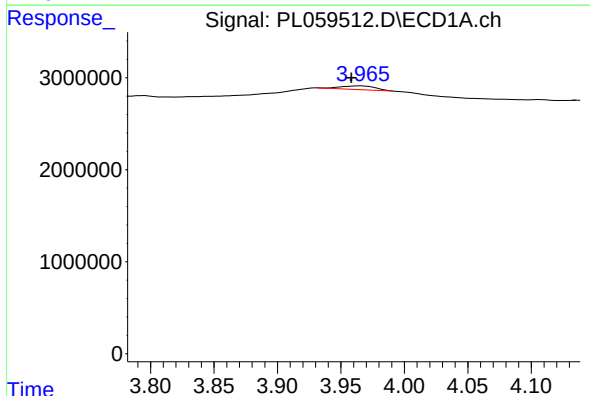


#2 alpha-BHC

R.T.: 3.966 min
Delta R.T.: 0.008 min
Response: 721598
Conc: 0.28 ng/ml

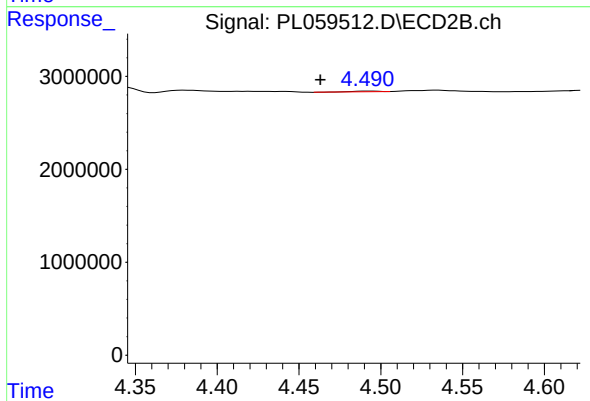

#2 alpha-BHC


R.T.: 4.493 min
Delta R.T.: 0.030 min
Response: 75793
Conc: 0.02 ng/ml

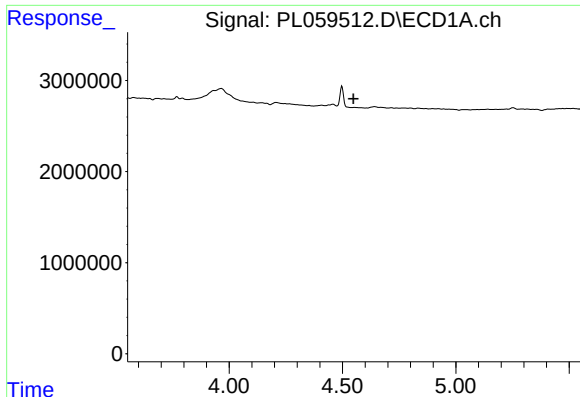

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-6-S

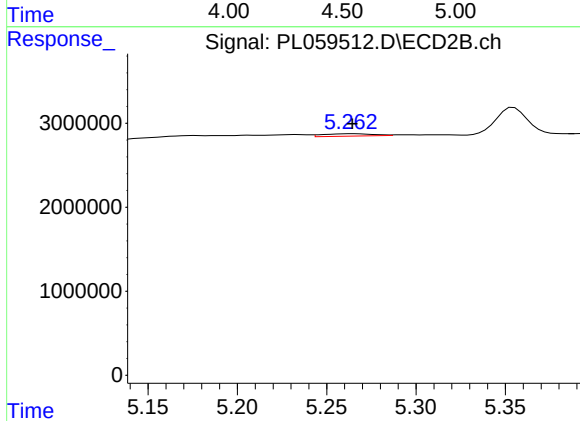


#4 Heptachlor

R.T.: 5.265 min
Delta R.T.: 0.000 min
Response: 566614
Conc: 0.17 ng/ml

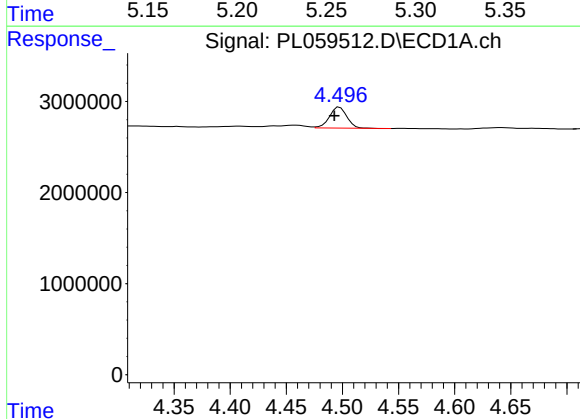


#6 beta-BHC

R.T.: 4.497 min
Delta R.T.: 0.005 min
Response: 2495725
Conc: 2.62 ng/ml

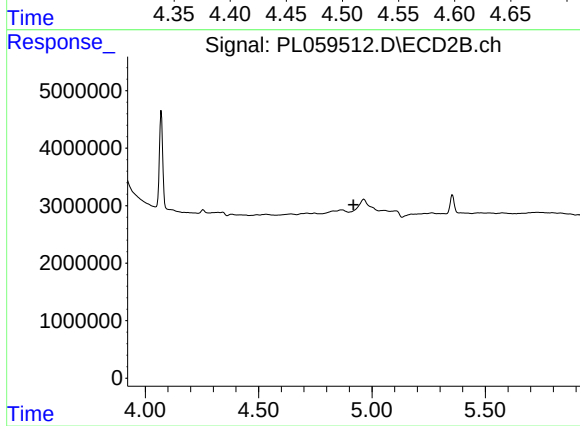

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.919 min
Response: 0
Conc: N.D.

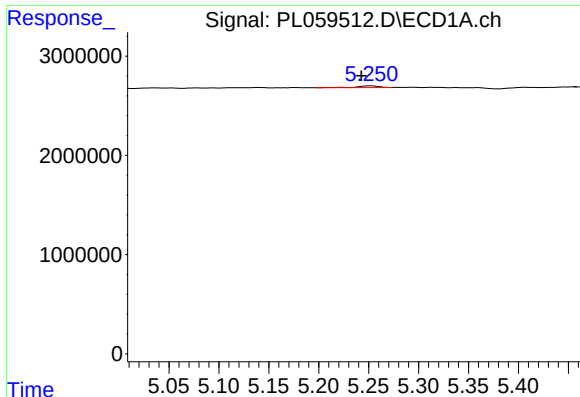

#8 Heptachlor epoxide


R.T.: 5.252 min
Delta R.T.: 0.009 min
Response: 267370
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-S

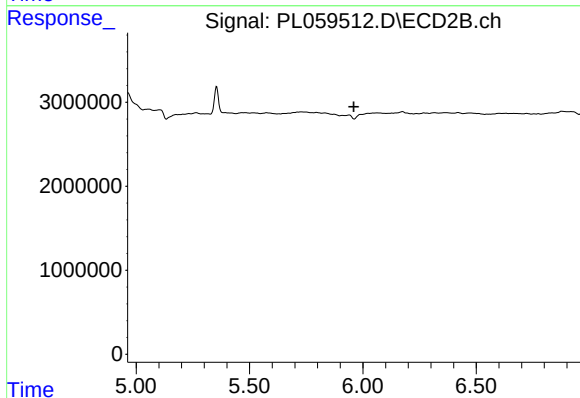


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

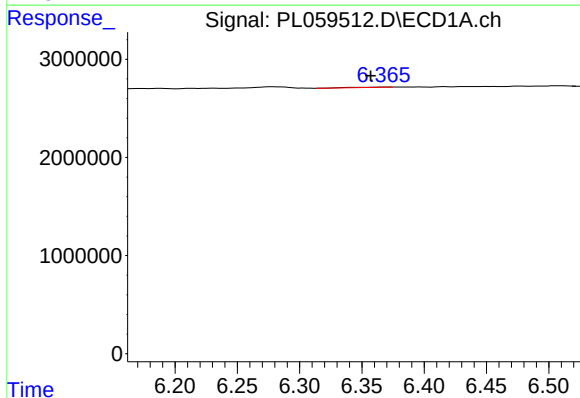


#15 Endosulfan II

R.T.: 6.367 min
Delta R.T.: 0.010 min
Response: 59699
Conc: 0.04 ng/ml

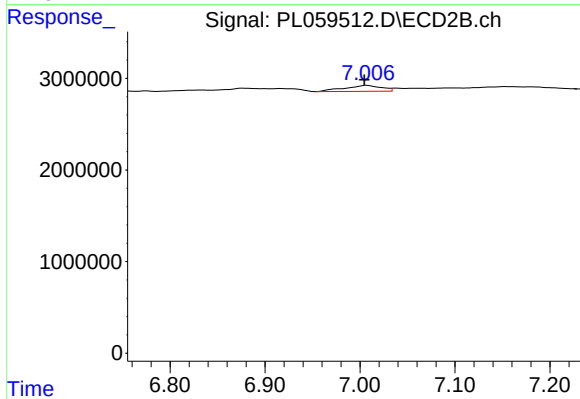

#15 Endosulfan II


R.T.: 7.007 min
Delta R.T.: 0.002 min
Response: 1744724
Conc: 0.69 ng/ml

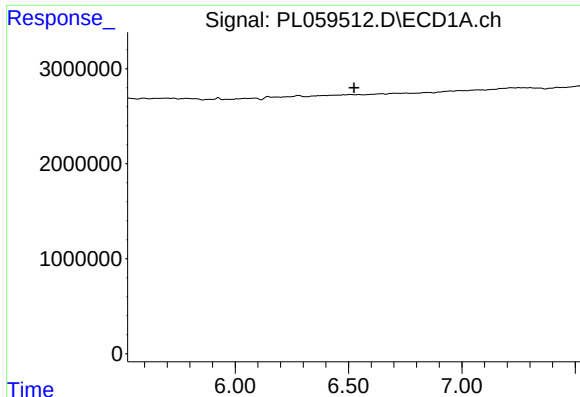

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-6-S

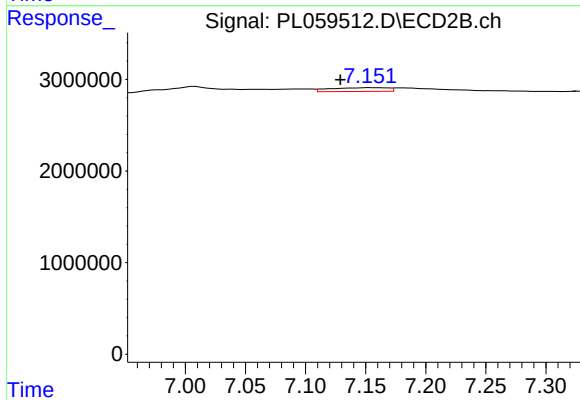


#18 Endrin aldehyde

R.T.: 7.153 min
Delta R.T.: 0.024 min
Response: 1348651
Conc: 0.61 ng/ml

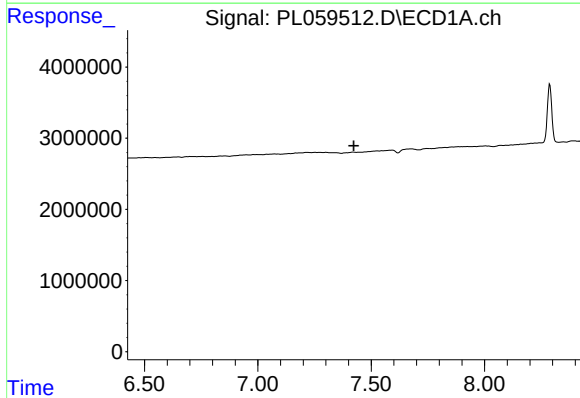


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.423 min
Response: 0
Conc: N.D.

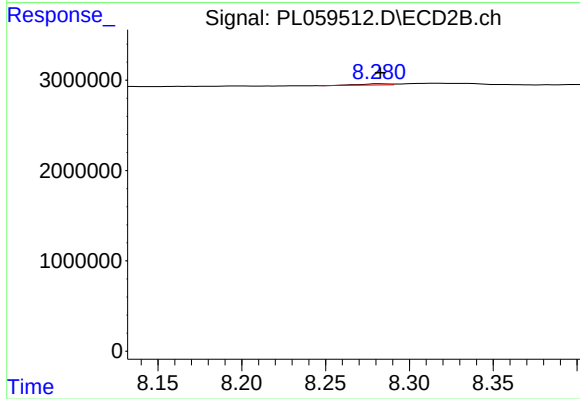

#22 Mirex


R.T.: 8.282 min
Delta R.T.: 0.000 min
Response: 152821
Conc: 0.08 ng/ml

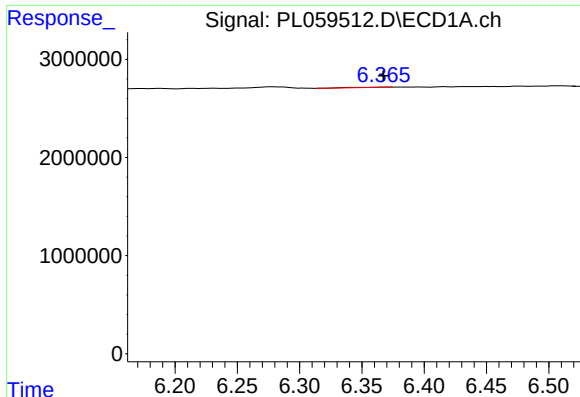

#27 Chlordane-5


R.T.: 6.367 min
Delta R.T.: 0.000 min
Response: 59699
Conc: 1.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-S

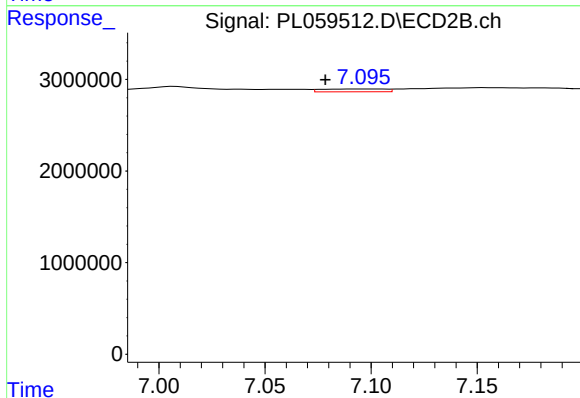


#27 Chlordane-5

R.T.: 7.099 min
Delta R.T.: 0.020 min
Response: 641309
Conc: 7.41 ng/ml

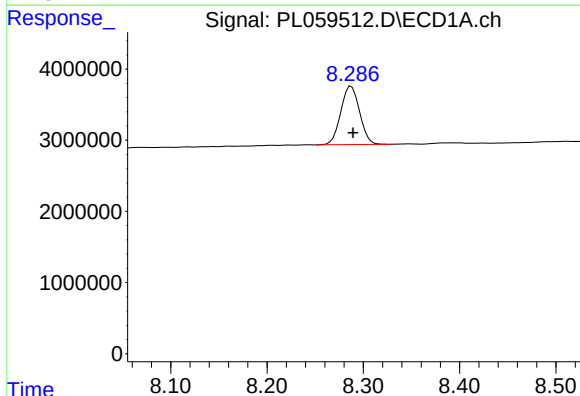

#28 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: -0.002 min
Response: 11115381
Conc: 6.53 ng/ml

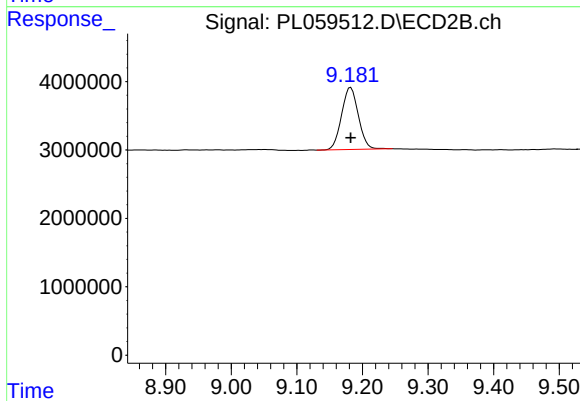

#28 Decachlorobiphenyl

R.T.: 9.182 min
Delta R.T.: 0.000 min
Response: 16195485
Conc: 7.07 ng/ml