

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062520\
 Data File : PL059514.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2020 17:32
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 18:21:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 22 14:09:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.518	4.072	31141946	45105507	17.329	17.476
28)	SA Decachlor...	8.289	9.182	27544184	38423758	16.176	16.782
Target Compounds							
2)	A alpha-BHC	3.966	0.000	854955	0	0.331	N.D. #
4)	MA Heptachlor	0.000	5.266	0	594413	N.D.	0.184 #
7)	B delta-BHC	0.000	5.112f	0	1801130	N.D.	0.647 #
8)	B Heptachlo...	0.000	5.949	0	2087460	N.D.	0.832 #
15)	B Endosulfa...	6.367	7.007	103902	526340	0.067	0.208 #
18)	B Endrin al...	6.552f	0.000	113844	0	0.086	N.D. #
23)	Chlordane-1	4.423f	0.000	317295	0	5.576	N.D. #
27)	Chlordane-5	6.367	0.000	103902	0	1.851	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062520\
Data File : PL059514.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2020 17:32
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 18:21:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
Quant Title : GC Extractables
QLast Update : Mon Jun 22 14:09:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

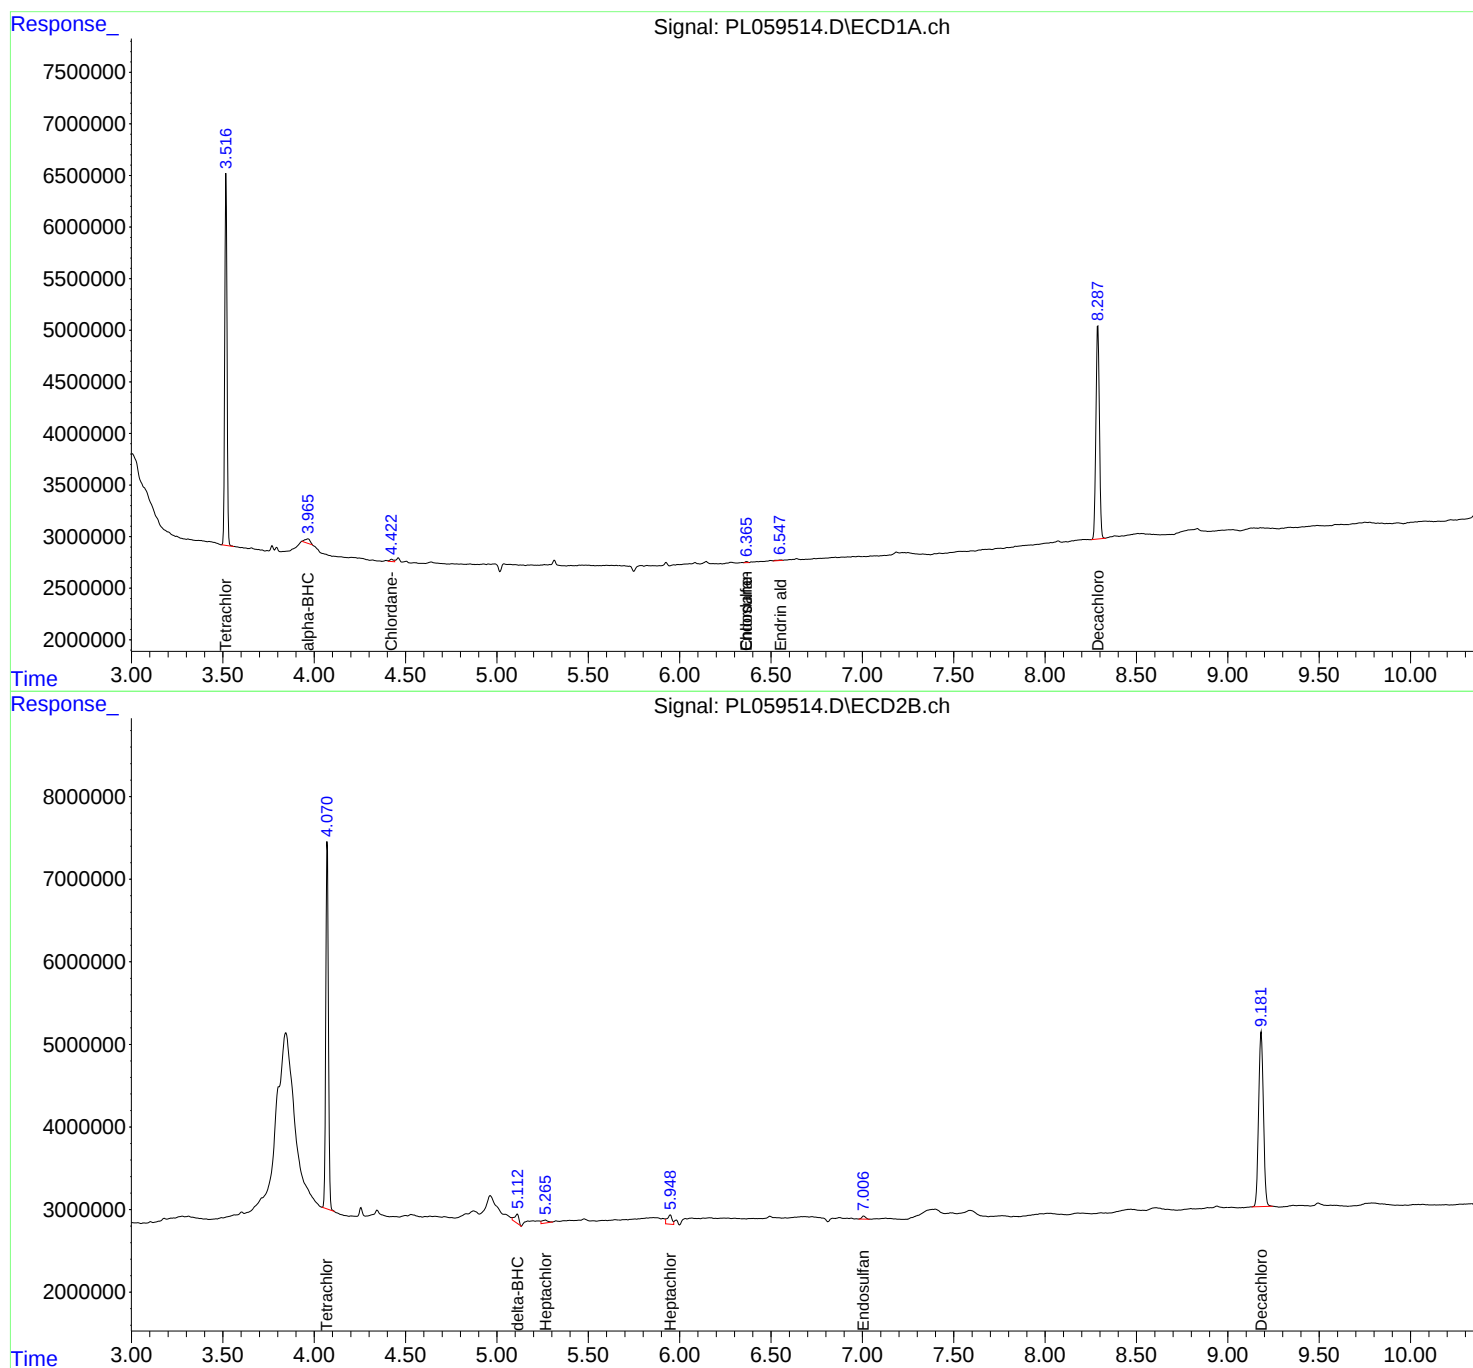


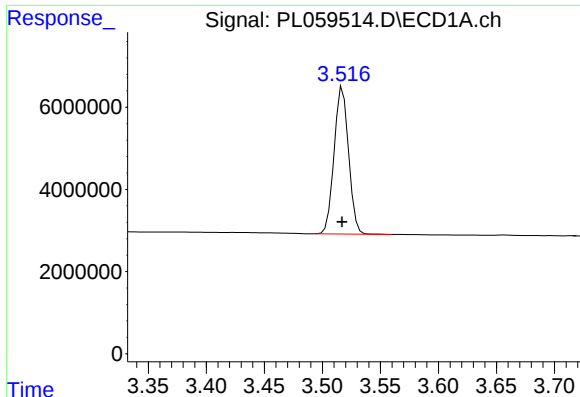

#1 Tetrachloro-m-xylene


R.T.: 3.518 min
Delta R.T.: 0.000 min
Response: 31141946
Conc: 17.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

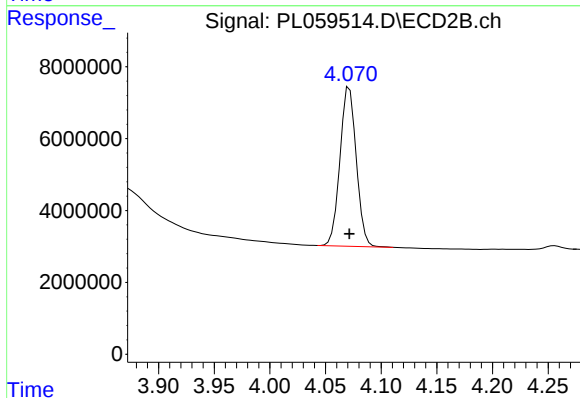


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 45105507
Conc: 17.48 ng/ml

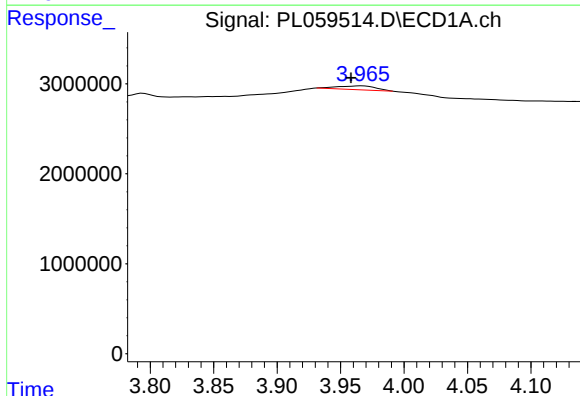


#2 alpha-BHC

R.T.: 3.966 min
Delta R.T.: 0.008 min
Response: 854955
Conc: 0.33 ng/ml

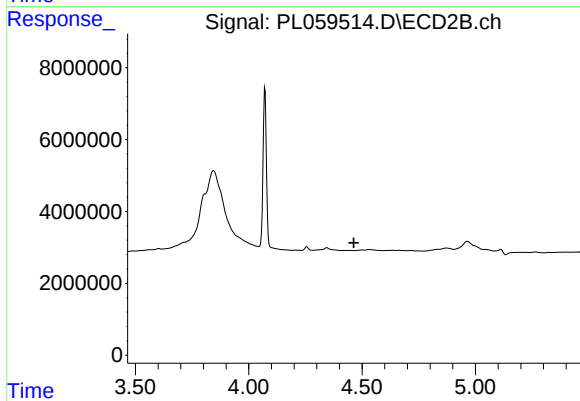

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.463 min
Response: 0
Conc: N.D.

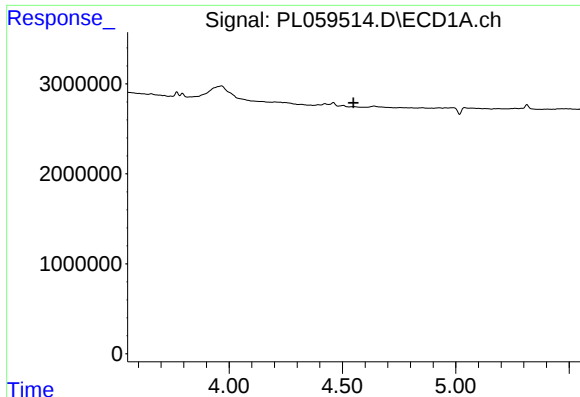

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

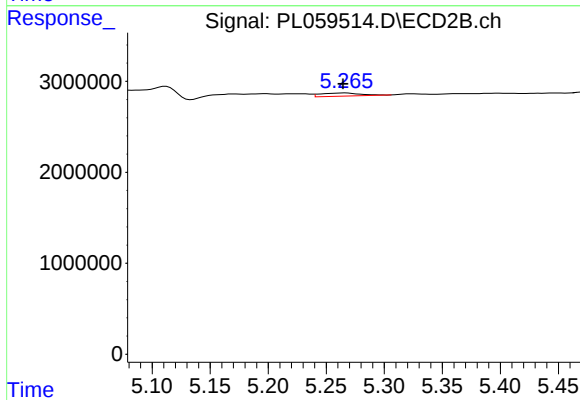


#4 Heptachlor

R.T.: 5.266 min
Delta R.T.: 0.002 min
Response: 594413
Conc: 0.18 ng/ml

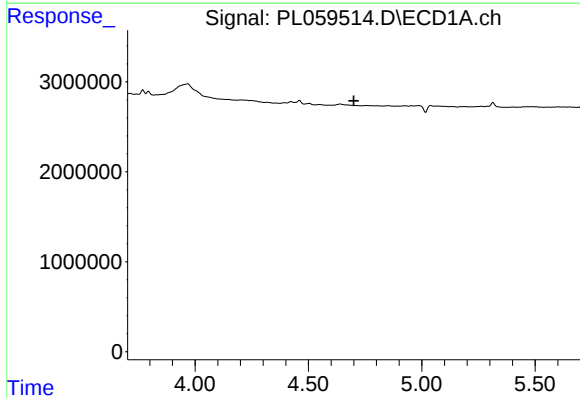


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.700 min
Response: 0
Conc: N.D.

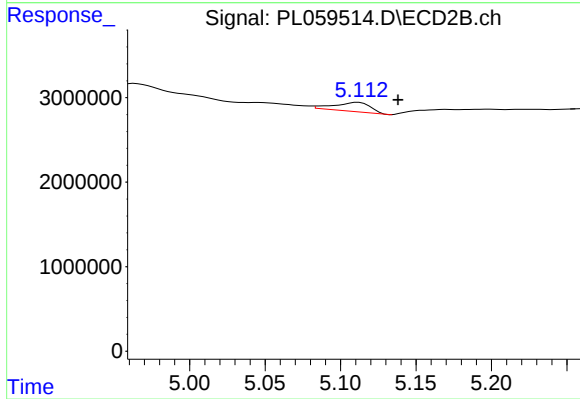

#7 delta-BHC


R.T.: 5.112 min
Delta R.T.: -0.026 min
Response: 1801130
Conc: 0.65 ng/ml

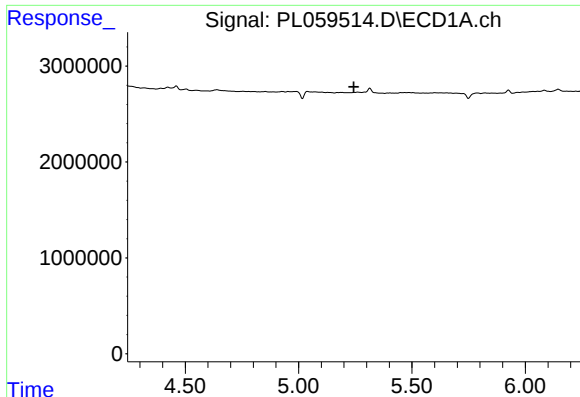

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.243 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

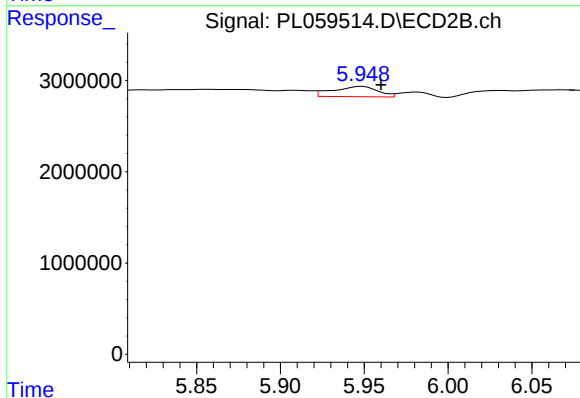


#8 Heptachlor epoxide

R.T.: 5.949 min
Delta R.T.: -0.011 min
Response: 2087460
Conc: 0.83 ng/ml

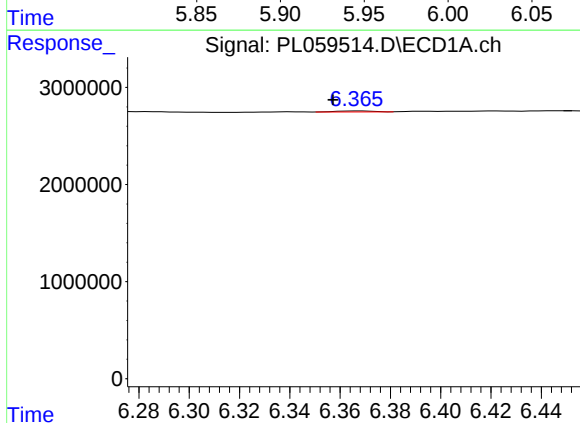


#15 Endosulfan II

R.T.: 6.367 min
Delta R.T.: 0.010 min
Response: 103902
Conc: 0.07 ng/ml

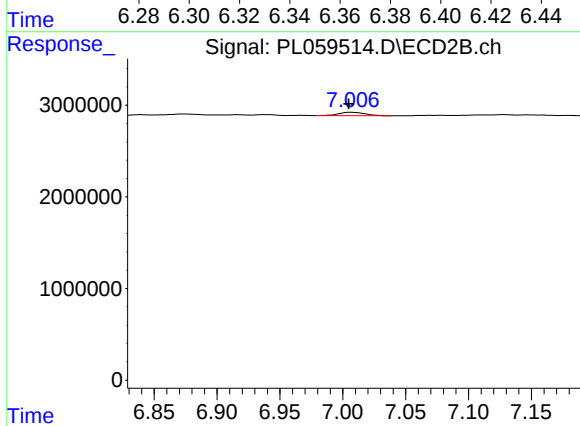

#15 Endosulfan II


R.T.: 7.007 min
Delta R.T.: 0.003 min
Response: 526340
Conc: 0.21 ng/ml

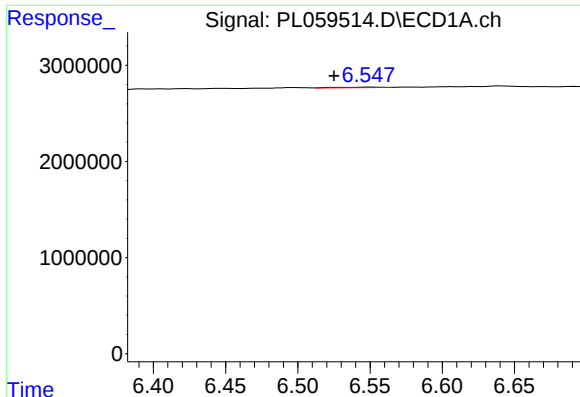

#18 Endrin aldehyde


R.T.: 6.552 min
Delta R.T.: 0.027 min
Response: 113844
Conc: 0.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

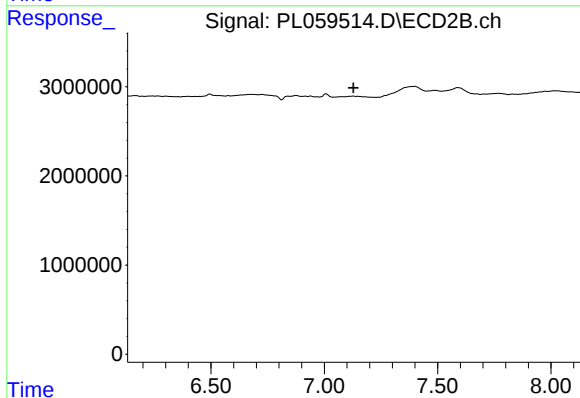


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.129 min
Response: 0
Conc: N.D.

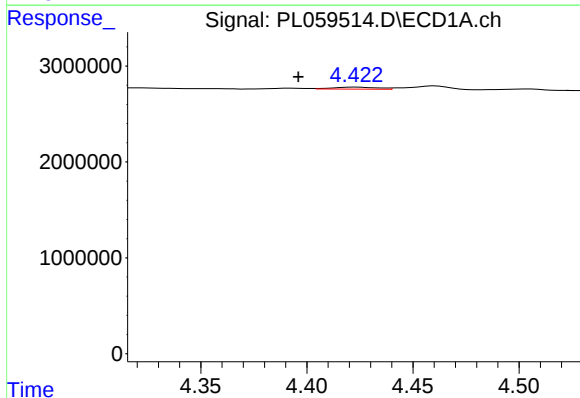


#23 Chlordane-1

R.T.: 4.423 min
Delta R.T.: 0.027 min
Response: 317295
Conc: 5.58 ng/ml

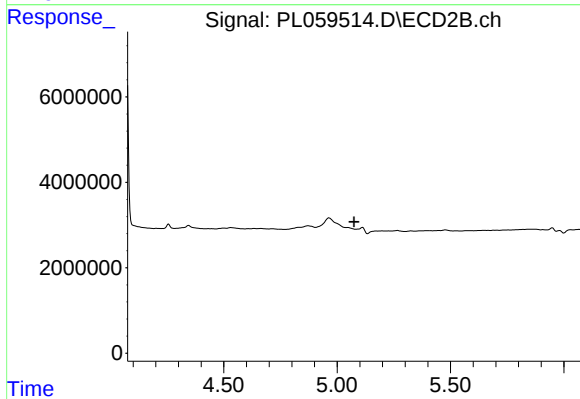

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.075 min
Response: 0
Conc: N.D.

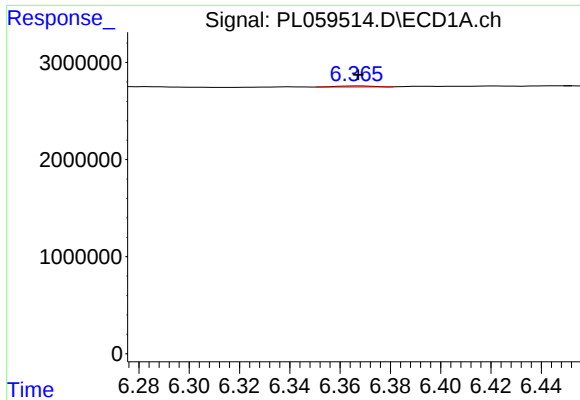

#27 Chlordane-5


R.T.: 6.367 min
Delta R.T.: 0.000 min
Response: 103902
Conc: 1.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

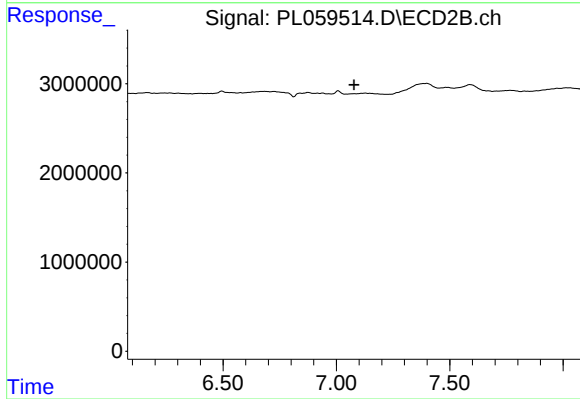


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

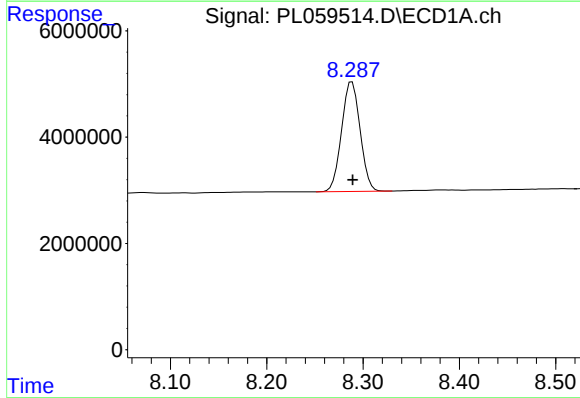

#28 Decachlorobiphenyl

R.T.: 8.289 min
Delta R.T.: 0.000 min
Response: 27544184
Conc: 16.18 ng/ml

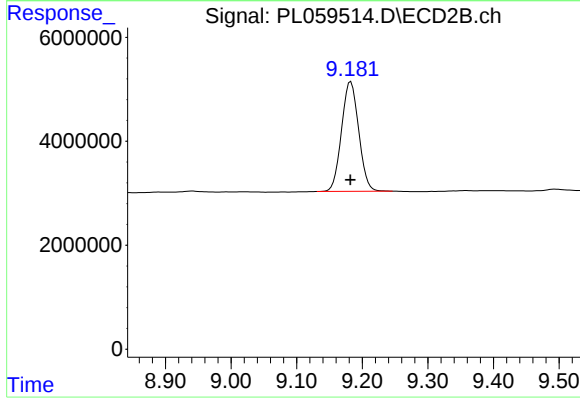

#28 Decachlorobiphenyl

R.T.: 9.182 min
Delta R.T.: 0.000 min
Response: 38423758
Conc: 16.78 ng/ml