

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062520\
 Data File : PL059519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2020 18:43
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 00:46:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 22 14:09:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.518	4.072	30426308	43562876	16.931	16.878
28)	SA Decachlor...	8.289	9.183	24013713	35089630	14.102	15.326
Target Compounds							
2)	A alpha-BHC	3.964	0.000	859093	0	0.333	N.D. #
4)	MA Heptachlor	0.000	5.261	0	290161	N.D.	0.090 #
5)	MB Aldrin	0.000	5.581	0	704390	N.D.	0.229 #
7)	B delta-BHC	0.000	5.113f	0	1397758	N.D.	0.502 #
8)	B Heptachlo...	5.237	5.950	224509	2660631	0.149	1.060 #
15)	B Endosulfa...	0.000	7.007	0	612751	N.D.	0.242 #
18)	B Endrin al...	6.497f	7.103f	126147	158718	0.095	0.072
23)	Chlordane-1	4.421f	0.000	543187	0	9.545	N.D. #
27)	Chlordane-5	0.000	7.103f	0	158718	N.D.	1.833 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062520\
Data File : PL059519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2020 18:43
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 00:46:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
Quant Title : GC Extractables
QLast Update : Mon Jun 22 14:09:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

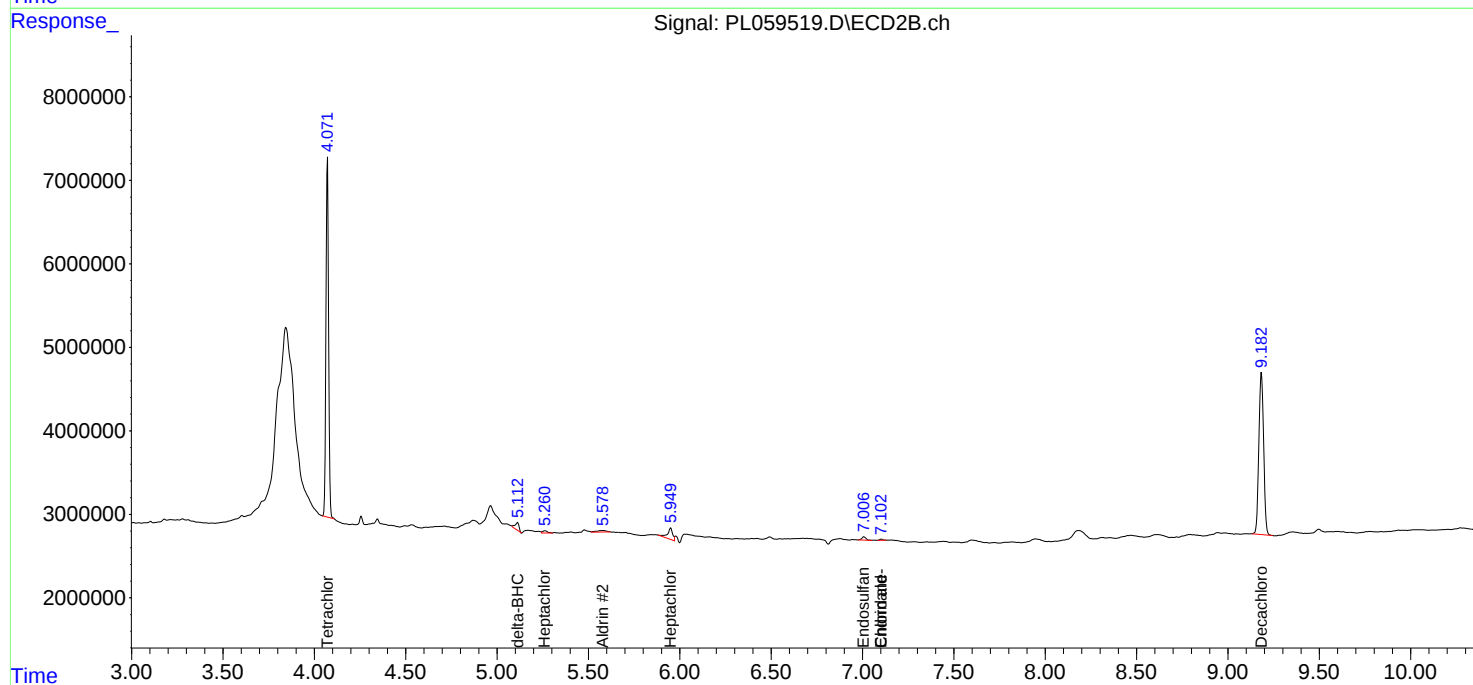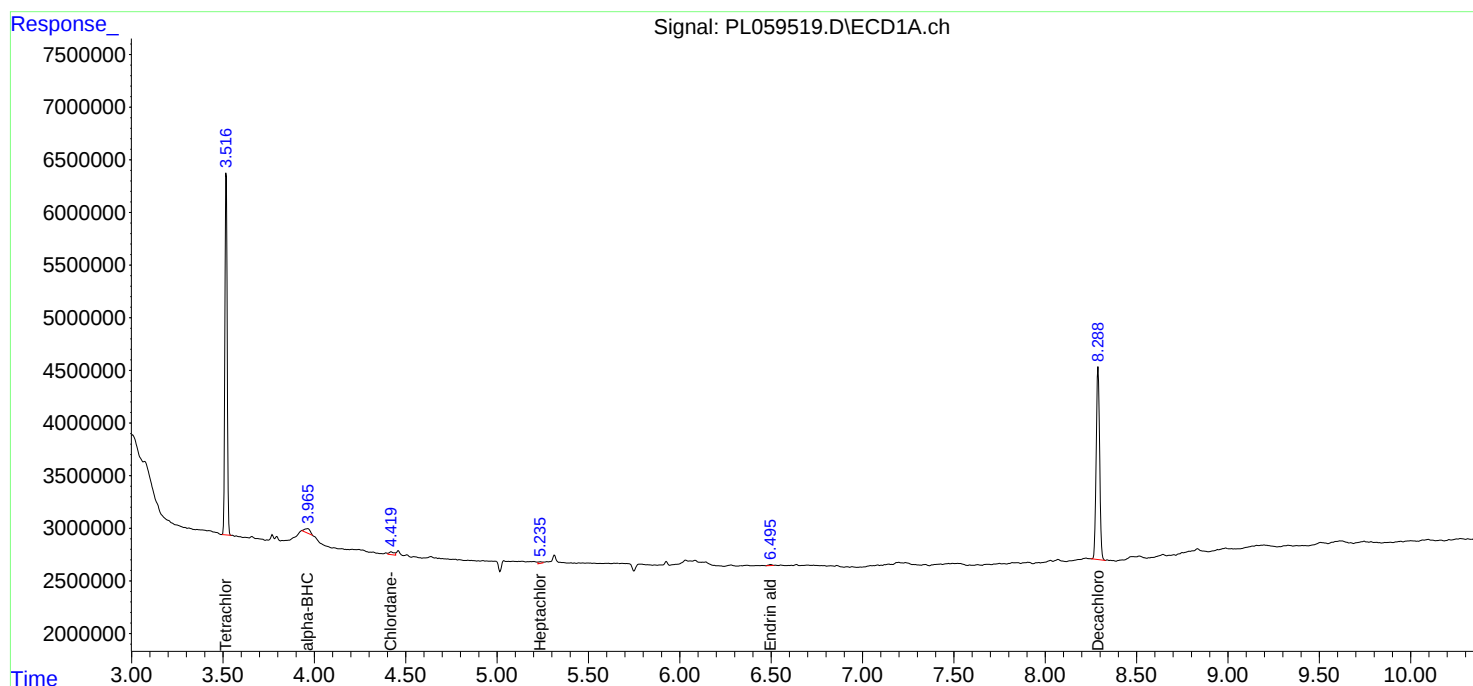


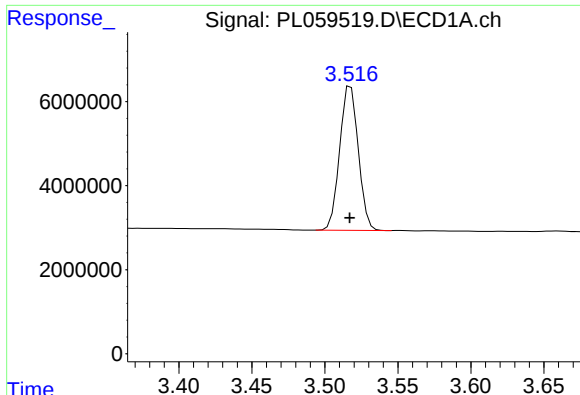

#1 Tetrachloro-m-xylene


R.T.: 3.518 min
Delta R.T.: 0.000 min
Response: 30426308
Conc: 16.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

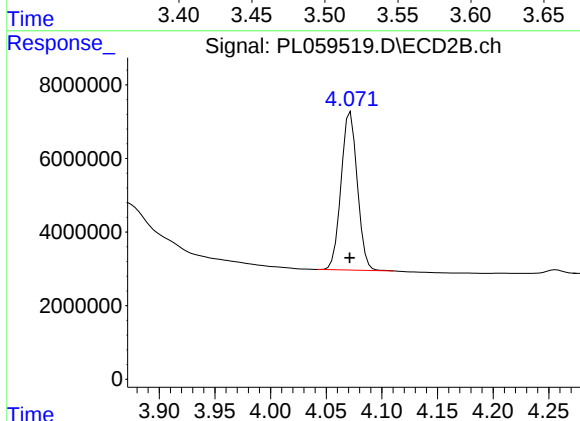


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 43562876
Conc: 16.88 ng/ml

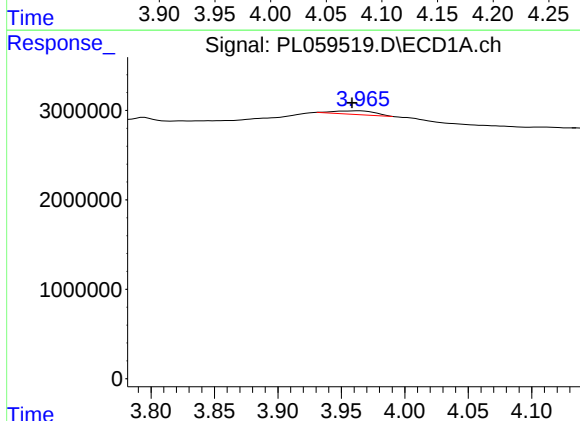


#2 alpha-BHC

R.T.: 3.964 min
Delta R.T.: 0.005 min
Response: 859093
Conc: 0.33 ng/ml

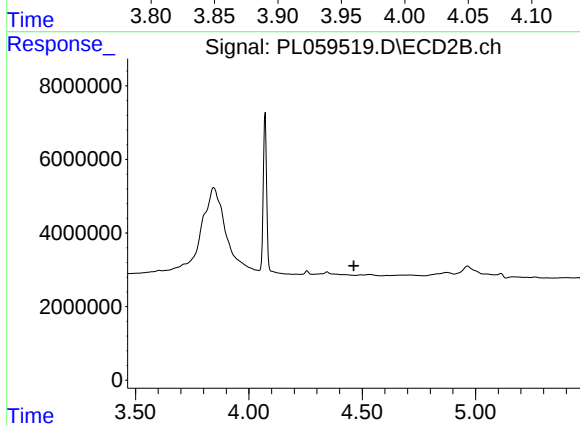

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.463 min
Response: 0
Conc: N.D.

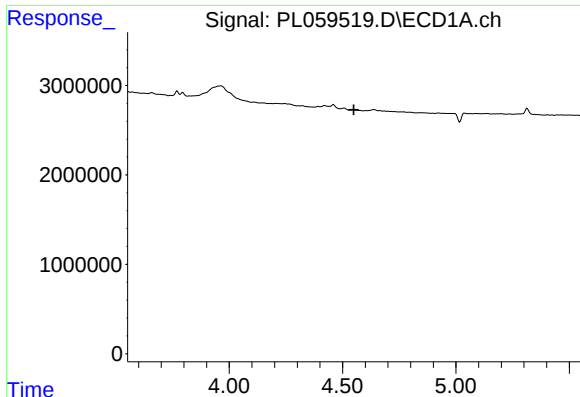

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

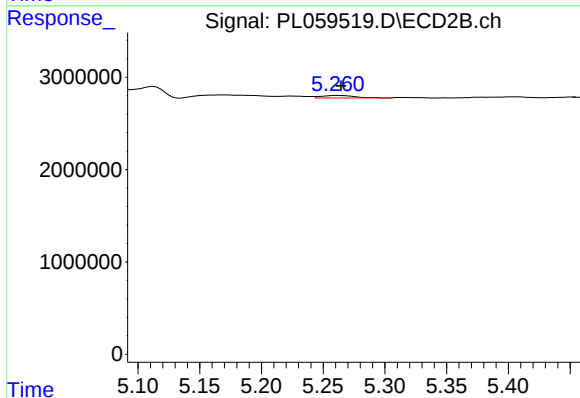


#4 Heptachlor

R.T.: 5.261 min
Delta R.T.: -0.003 min
Response: 290161
Conc: 0.09 ng/ml

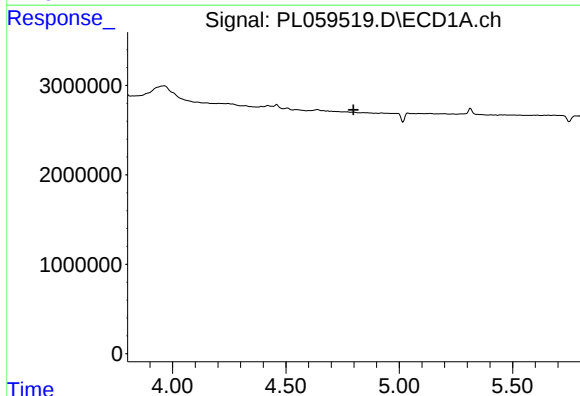


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.799 min
Response: 0
Conc: N.D.

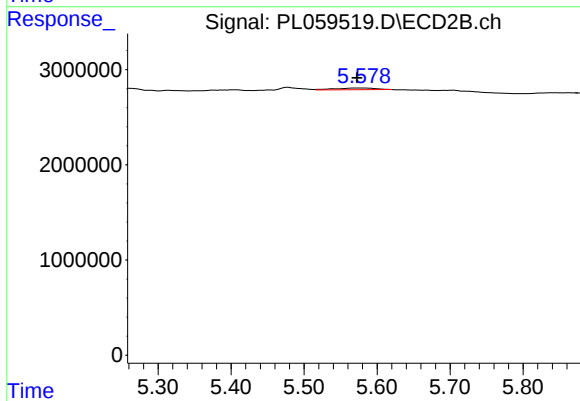

#5 Aldrin


R.T.: 5.581 min
Delta R.T.: 0.008 min
Response: 704390
Conc: 0.23 ng/ml

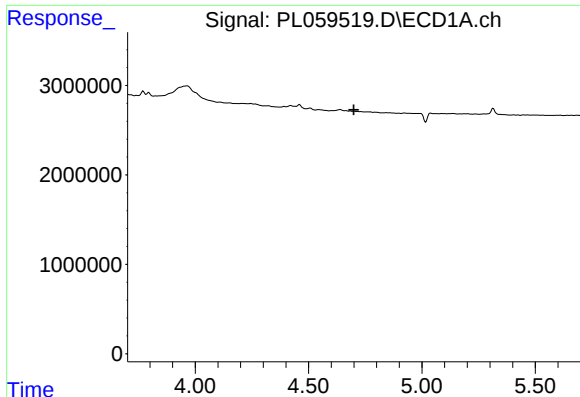

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.700 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

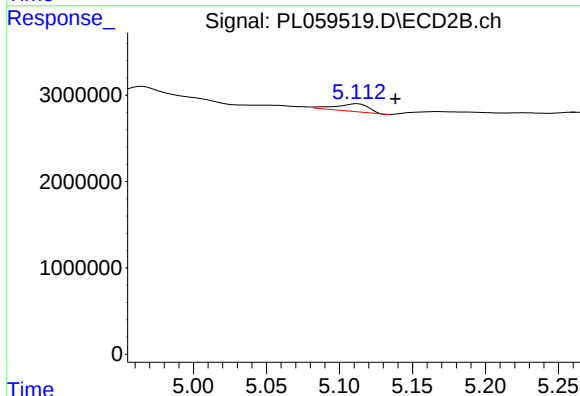


#7 delta-BHC

R.T.: 5.113 min
Delta R.T.: -0.026 min
Response: 1397758
Conc: 0.50 ng/ml

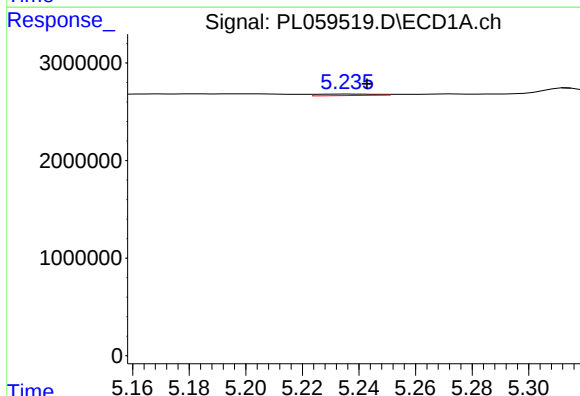


#8 Heptachlor epoxide

R.T.: 5.237 min
Delta R.T.: -0.006 min
Response: 224509
Conc: 0.15 ng/ml

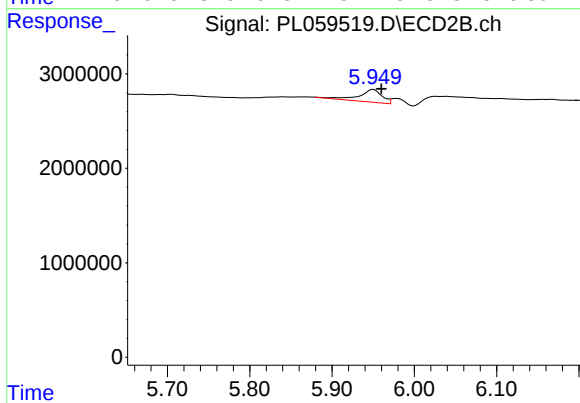

#8 Heptachlor epoxide


R.T.: 5.950 min
Delta R.T.: -0.010 min
Response: 2660631
Conc: 1.06 ng/ml

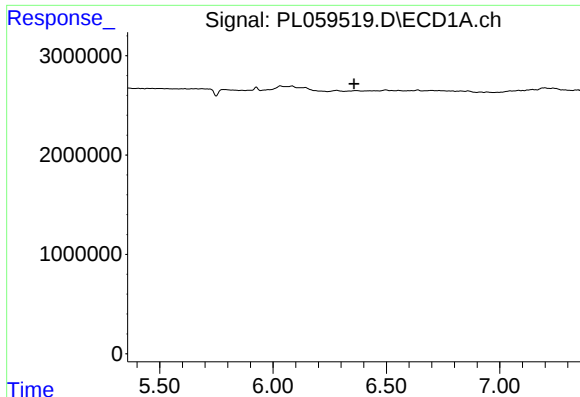

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

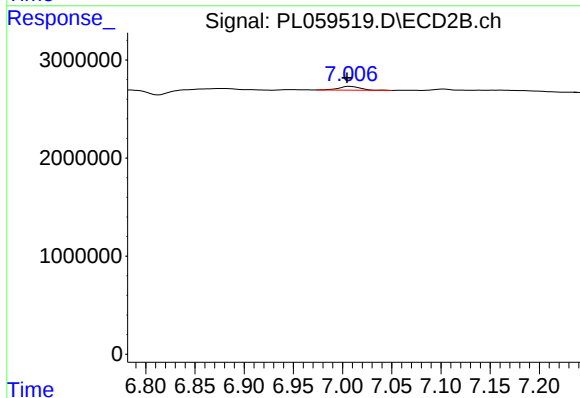


#15 Endosulfan II

R.T.: 7.007 min
Delta R.T.: 0.003 min
Response: 612751
Conc: 0.24 ng/ml

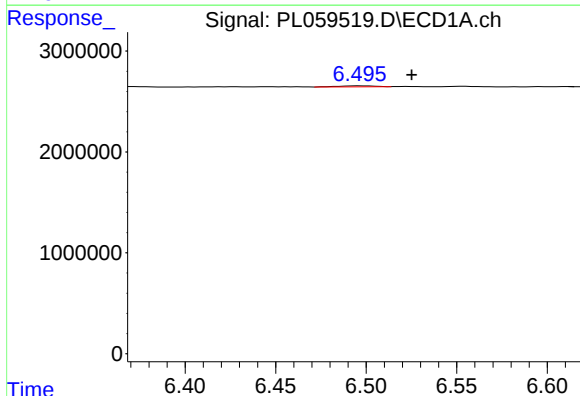


#18 Endrin aldehyde

R.T.: 6.497 min
Delta R.T.: -0.029 min
Response: 126147
Conc: 0.10 ng/ml

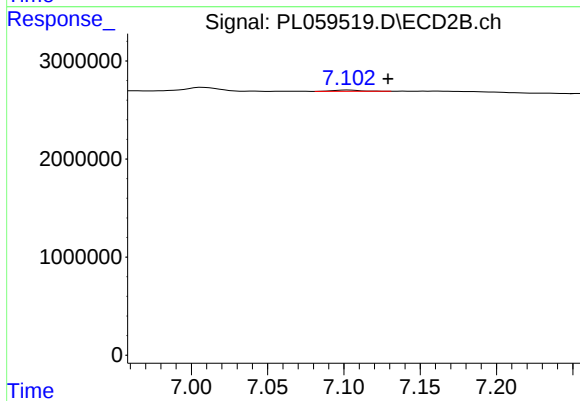

#18 Endrin aldehyde


R.T.: 7.103 min
Delta R.T.: -0.026 min
Response: 158718
Conc: 0.07 ng/ml

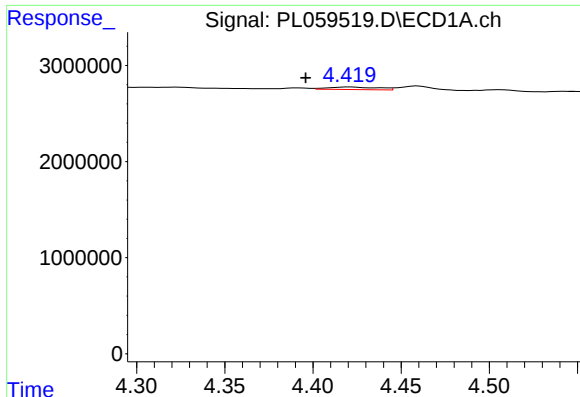

#23 Chlordane-1


R.T.: 4.421 min
Delta R.T.: 0.025 min
Response: 543187
Conc: 9.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

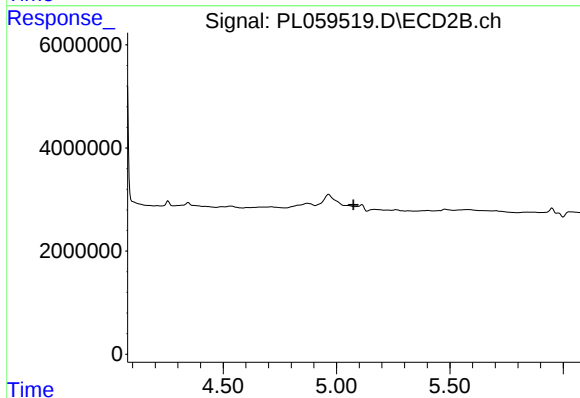


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.075 min
Response: 0
Conc: N.D.

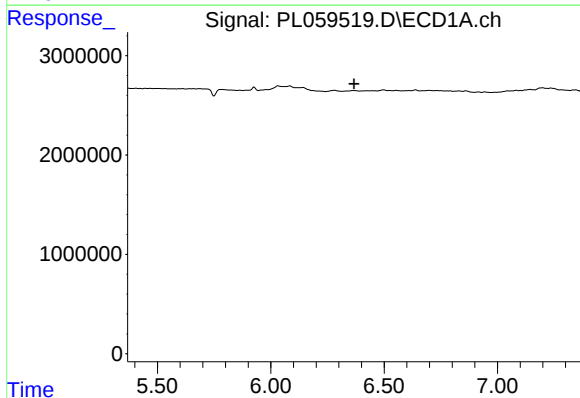


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.367 min
Response: 0
Conc: N.D.

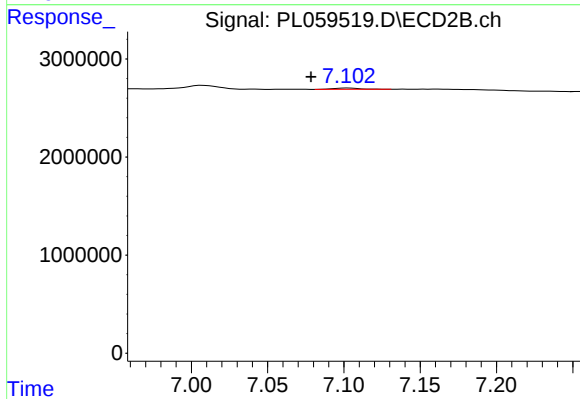

#27 Chlordane-5


R.T.: 7.103 min
Delta R.T.: 0.024 min
Response: 158718
Conc: 1.83 ng/ml

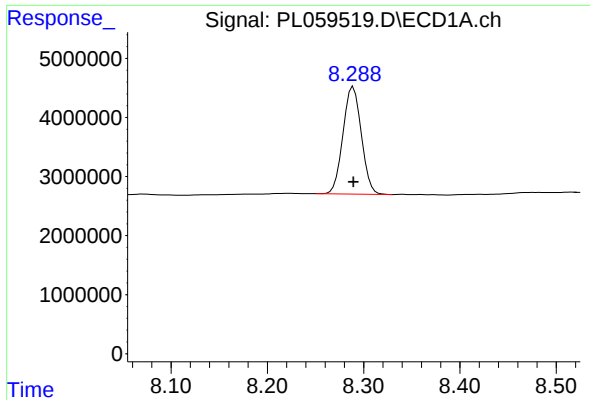

#28 Decachlorobiphenyl

R.T.: 8.289 min
Delta R.T.: 0.000 min
Response: 24013713
Conc: 14.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

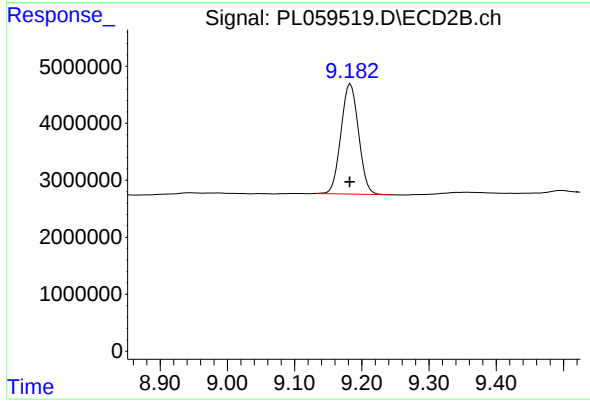

#28 Decachlorobiphenyl

R.T.: 9.183 min
Delta R.T.: 0.000 min
Response: 35089630
Conc: 15.33 ng/ml