

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062520\
 Data File : PL059518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2020 18:29
 Operator : AJ\MA
 Sample : L2810-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-01-062420

Manual Integrations
 APPROVED

Ankita
 6/26/2020 11:48:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 00:46:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 22 14:09:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.518	4.072	23820641	33162538	13.255	12.849
28) SA Decachlor...	8.289	9.182	20902015	30299423	12.275	13.233m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062520\
Data File : PL059518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2020 18:29
Operator : AJ\MA
Sample : L2810-09
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CL-01-062420


Manual Integrations
APPROVED

Ankita
6/26/2020 11:48:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 00:46:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
Quant Title : GC Extractables
QLast Update : Mon Jun 22 14:09:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

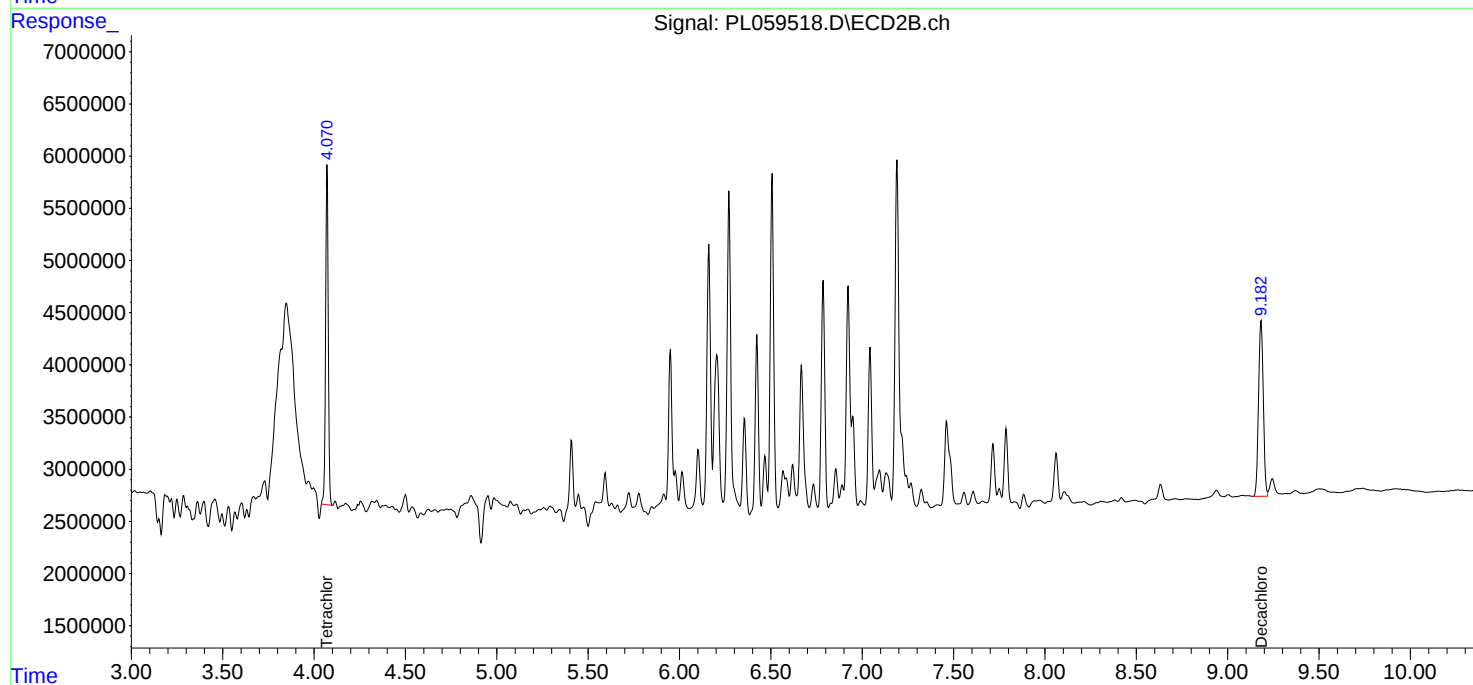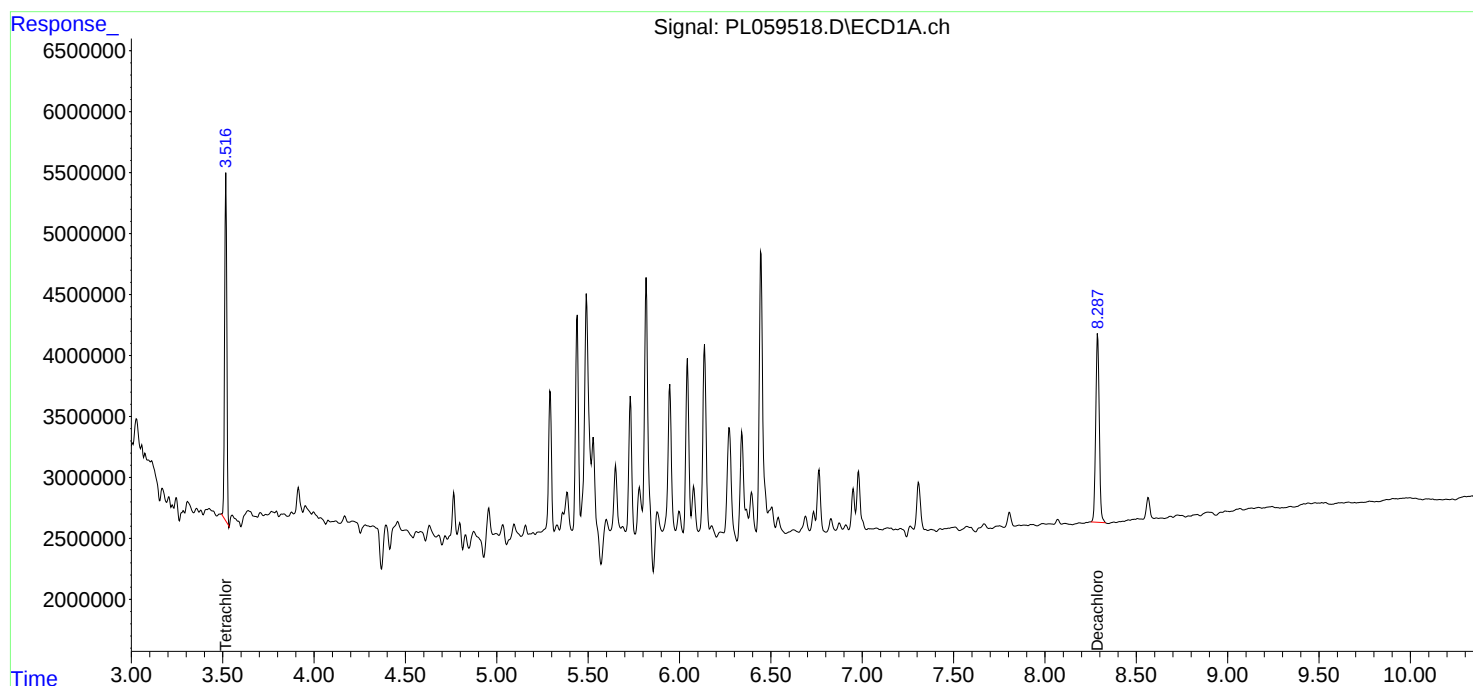

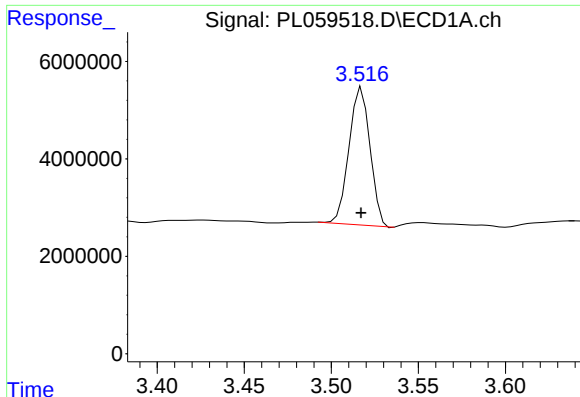


#1 Tetrachloro-m-xylene

R.T.: 3.518 min
Delta R.T.: 0.000 min
Response: 23820641
Conc: 13.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-062420


Manual Integrations
APPROVED

Ankita
6/26/2020 11:48:01 AM

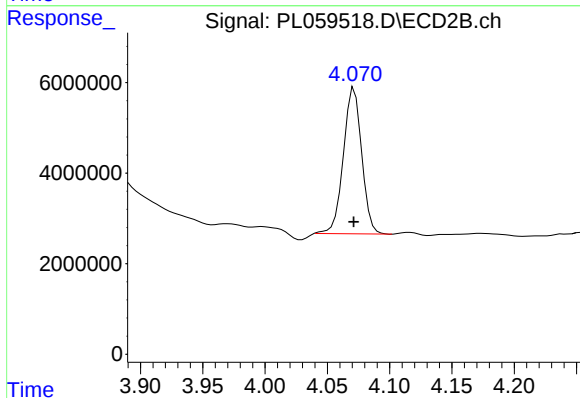


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 33162538
Conc: 12.85 ng/ml

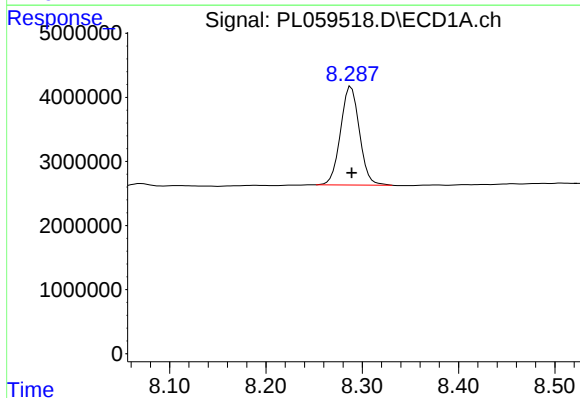

#28 Decachlorobiphenyl

R.T.: 8.289 min
Delta R.T.: 0.000 min
Response: 20902015
Conc: 12.27 ng/ml

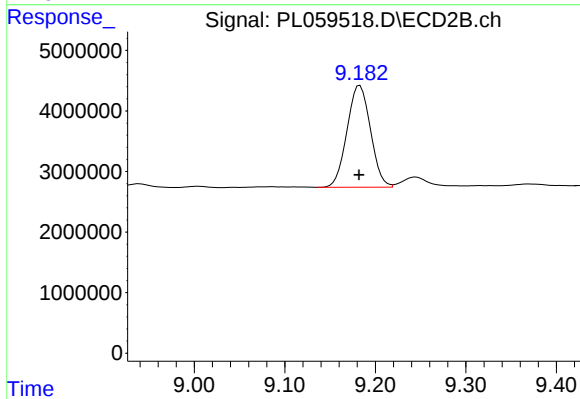

#28 Decachlorobiphenyl

R.T.: 9.182 min
Delta R.T.: 0.000 min
Response: 30299423
Conc: 13.23 ng/ml m