

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
 Data File : PL067788.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2021 08:14
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 05:44:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	5.989f	0.000	1357167	0	1.799	N.D.	#
6) B	beta-BHC	5.989	0.000	1357167	0	3.793	N.D.	#
7) B	delta-BHC	0.000	7.046f	0	446557	N.D.	0.380	#
15) B	Endosulfa...	8.176	0.000	389195	0	0.632	N.D.	#
21) B	Endrin ke...	0.000	10.047f	0	82180	N.D.	0.091	#
22)	Mirex	9.304	0.000	471041	0	0.748	N.D.	#
24)	Chlordane-2	6.488	0.000	1142365	0	42.660	N.D.	#
27)	Chlordane-5	8.176f	0.000	389195	0	17.788	N.D.	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
Data File : PL067788.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2021 08:14
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 05:44:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

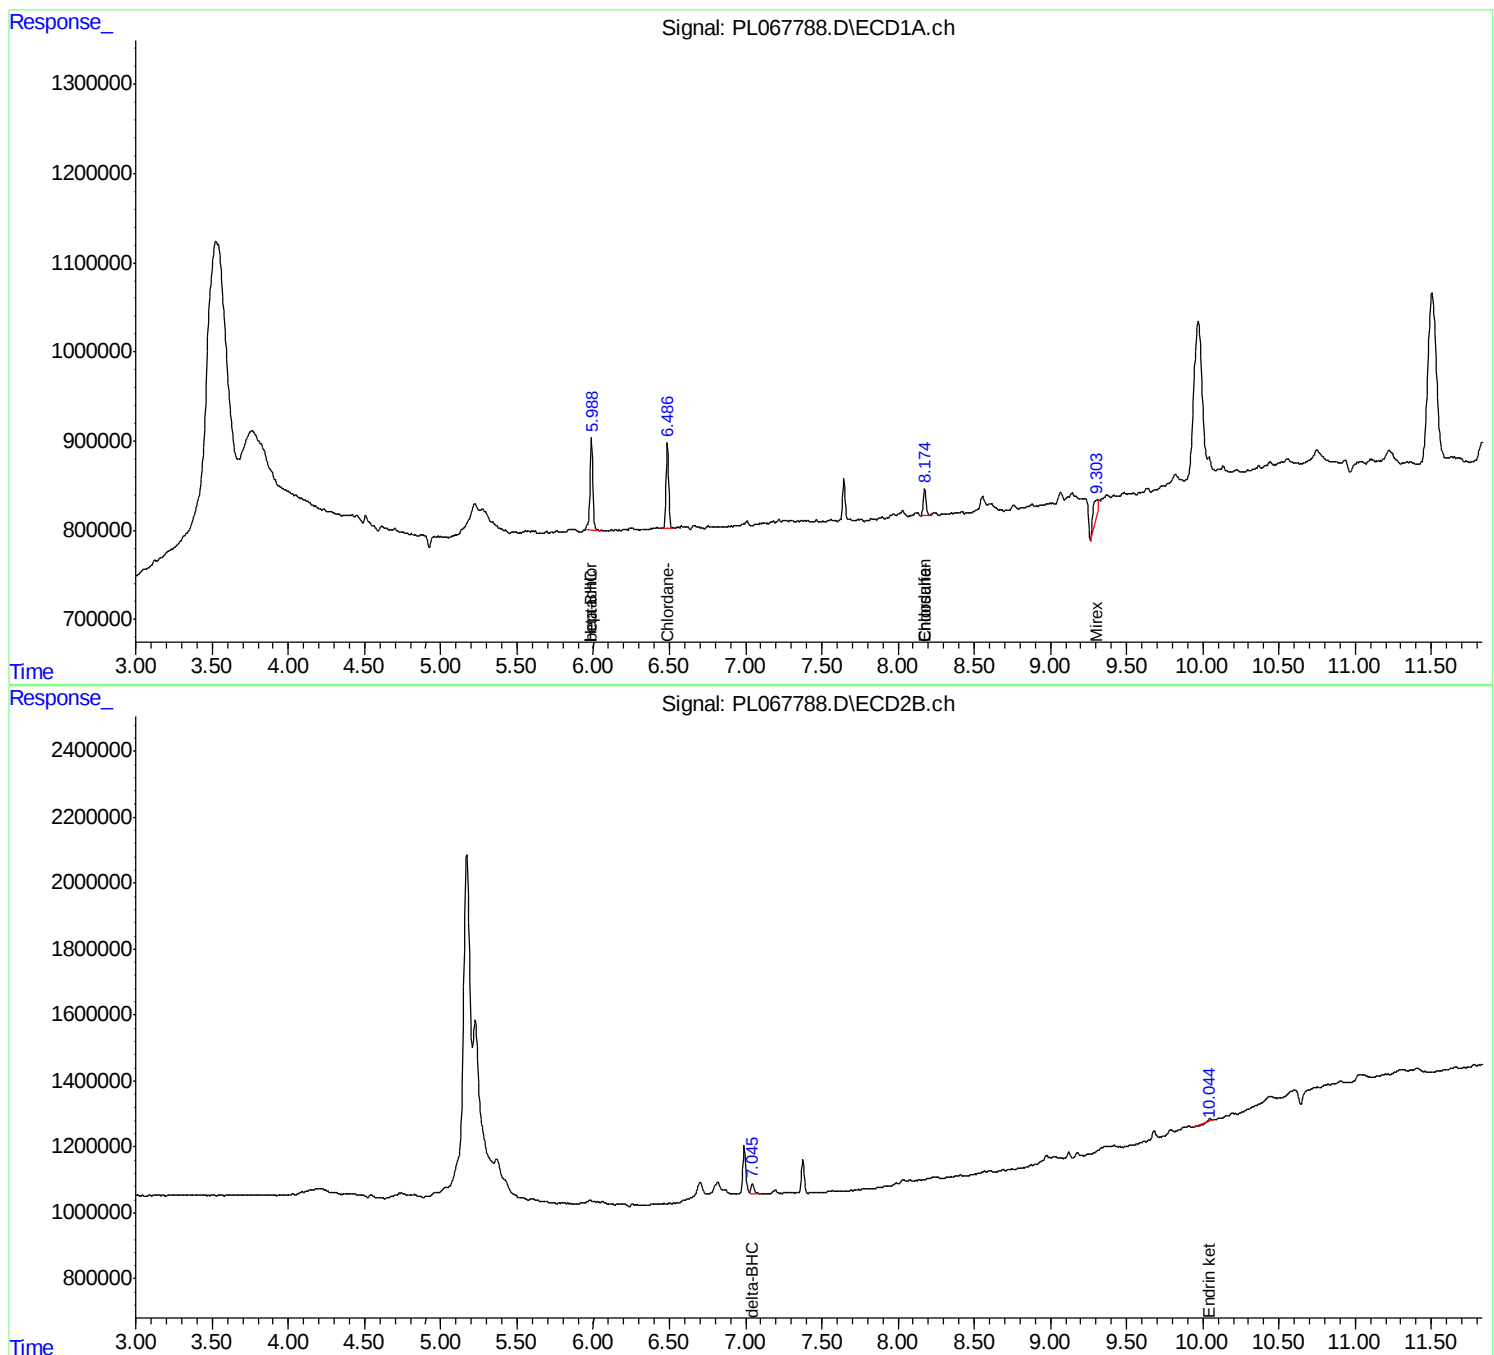


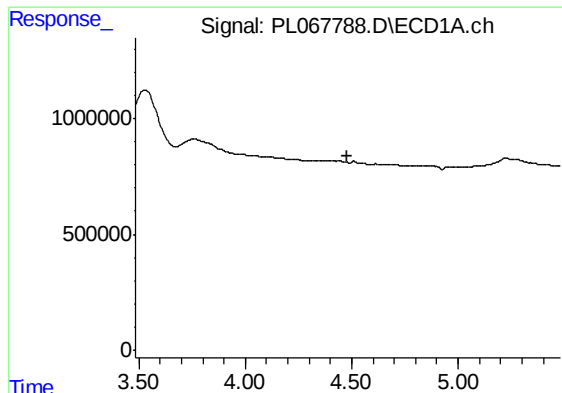

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

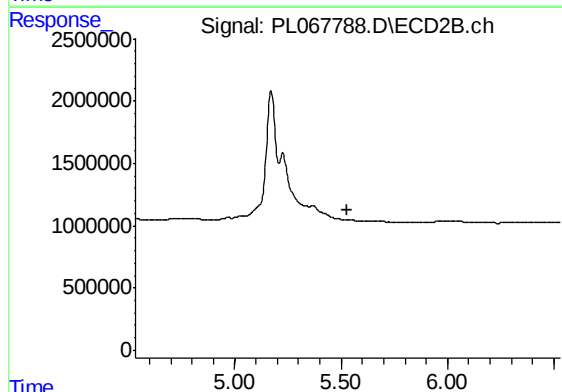


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.531 min
Response: 0
Conc: N.D.

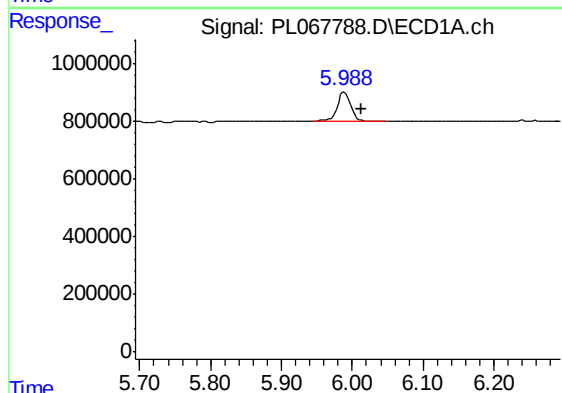


#4 Heptachlor

R.T.: 5.989 min
Delta R.T.: -0.023 min
Response: 1357167
Conc: 1.80 ng/ml

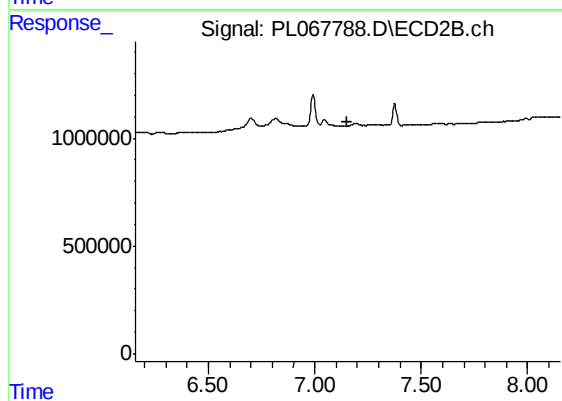

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

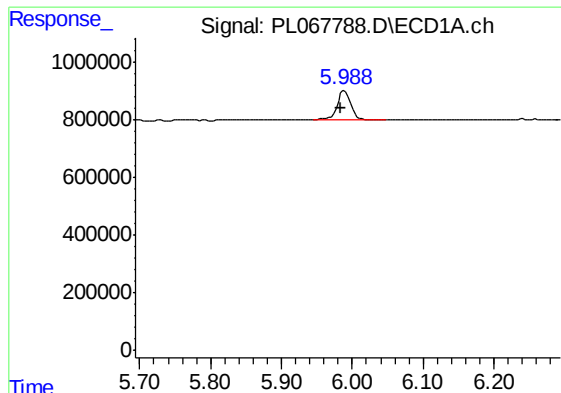

#6 beta-BHC


R.T.: 5.989 min
Delta R.T.: 0.006 min
Response: 1357167
Conc: 3.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

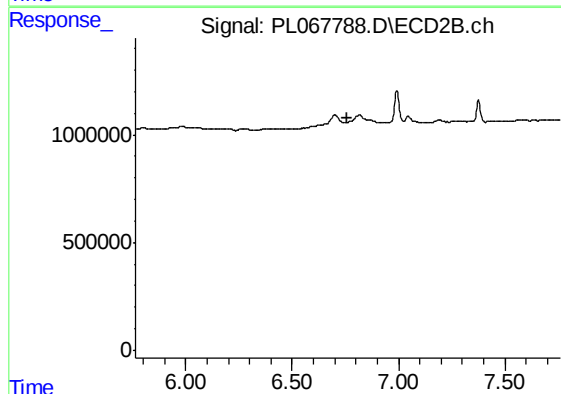


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

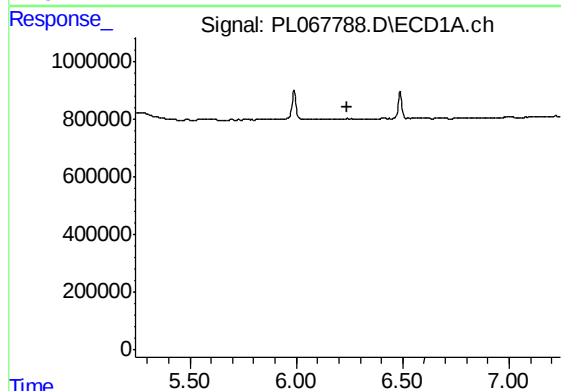


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

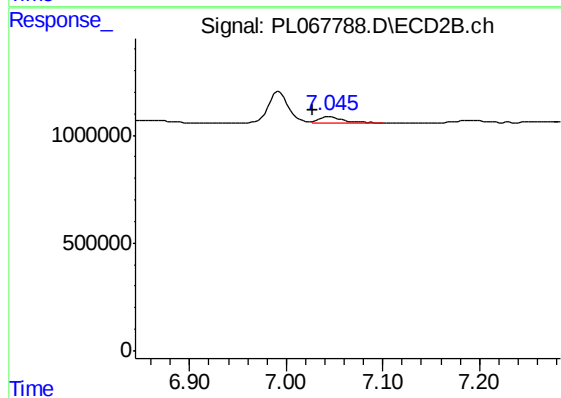

#7 delta-BHC


R.T.: 7.046 min
Delta R.T.: 0.018 min
Response: 446557
Conc: 0.38 ng/ml

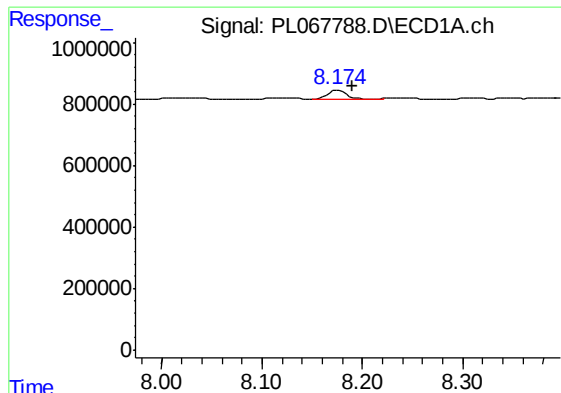

#15 Endosulfan II


R.T.: 8.176 min
Delta R.T.: -0.014 min
Response: 389195
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

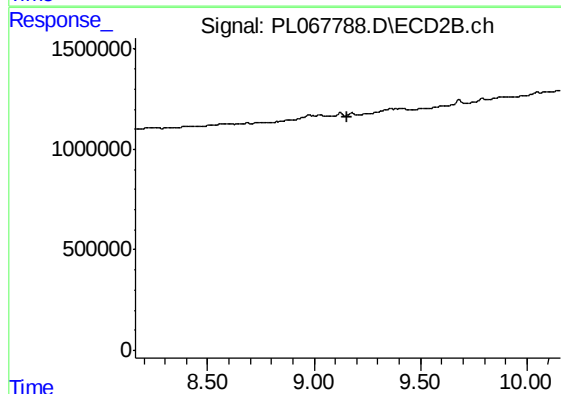


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.158 min
Response: 0
Conc: N.D.

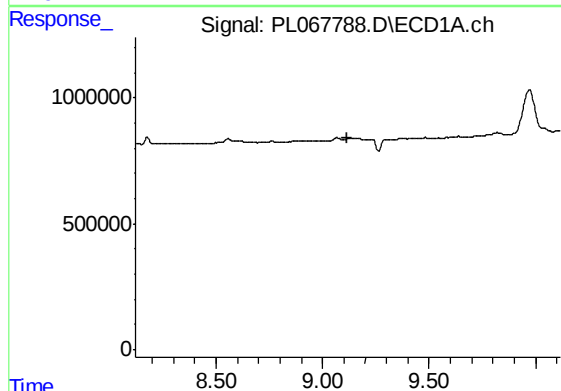


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.118 min
Response: 0
Conc: N.D.

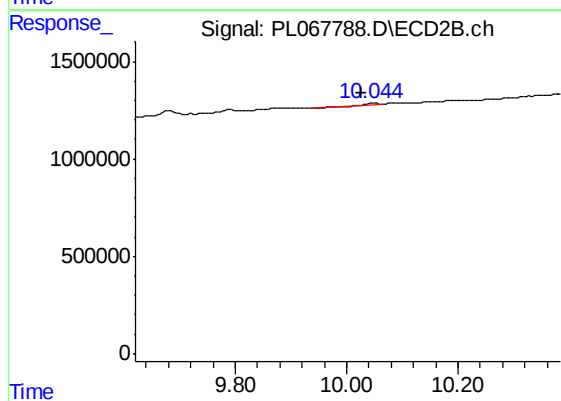

#21 Endrin ketone


R.T.: 10.047 min
Delta R.T.: 0.020 min
Response: 82180
Conc: 0.09 ng/ml

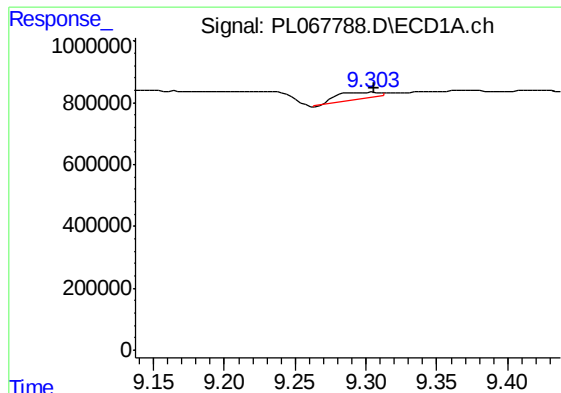

#22 Mirex


R.T.: 9.304 min
Delta R.T.: -0.001 min
Response: 471041
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

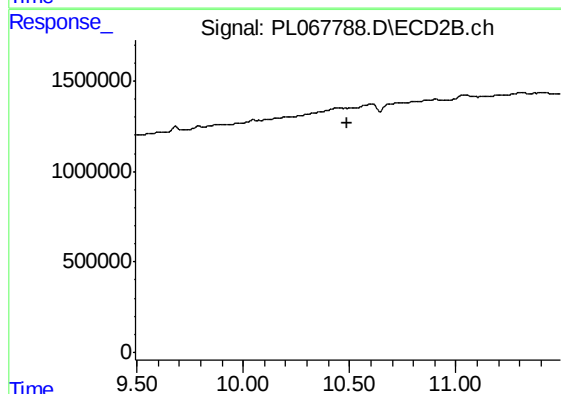


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 10.492 min
Response: 0
Conc: N.D.

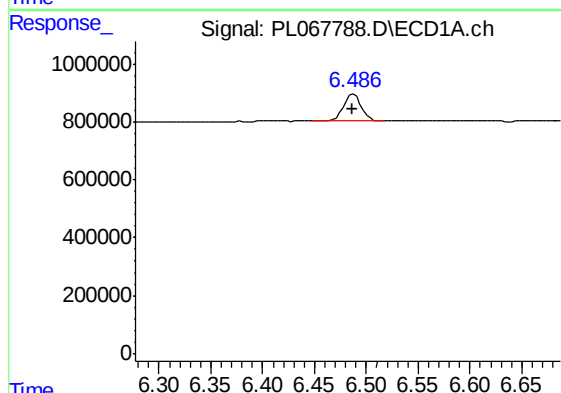


#24 Chlordane-2

R.T.: 6.488 min
Delta R.T.: 0.001 min
Response: 1142365
Conc: 42.66 ng/ml

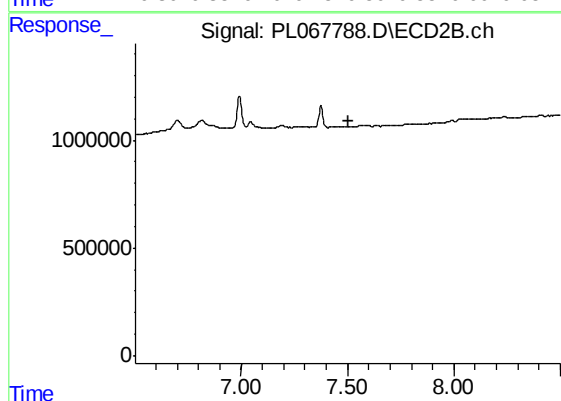

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

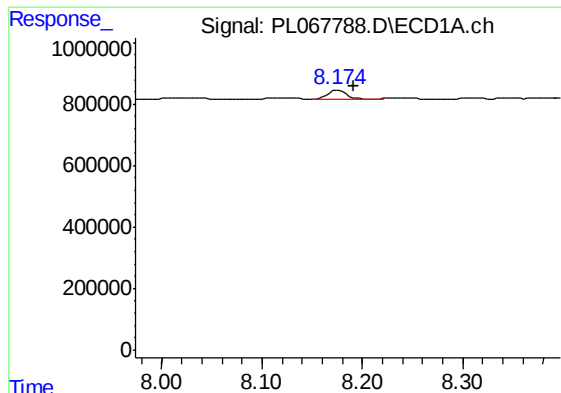

#27 Chlordane-5


R.T.: 8.176 min
Delta R.T.: -0.015 min
Response: 389195
Conc: 17.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

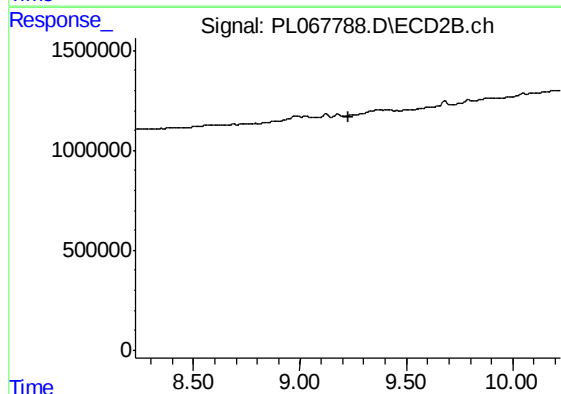


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

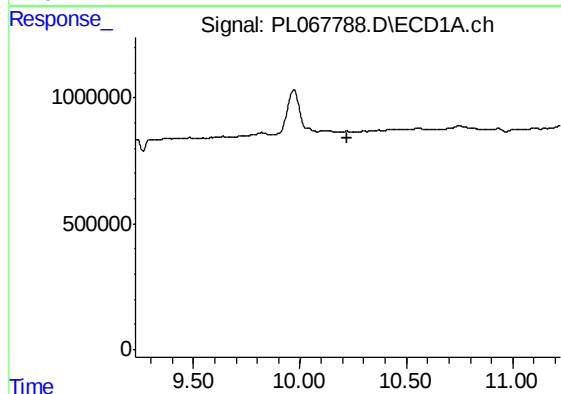

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.224 min
Response: 0
Conc: N.D.

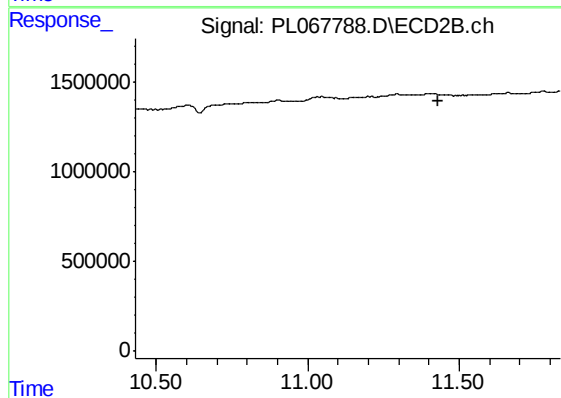

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.429 min
Response: 0
Conc: N.D.