

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
 Data File : PL067797.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2021 14:54
 Operator : AR\AJ
 Sample : M2852-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MANHOLE-WC-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 05:47:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.498f	5.529	10769794	19545990	19.589	20.733
28)	SA Decachlor...	10.240f	11.426	14431262	20345228	20.363	20.426
Target Compounds							
15)	B Endosulfa...	8.196	9.177f	300748	581930	0.488	0.730 #
16)	A 4,4'-DDD	8.053	0.000	1290649	0	2.220	N.D. #
20)	A Methoxychlor	8.892f	0.000	172156	0	0.484	N.D. #
27)	Chlordane-5	8.196	0.000	300748	0	13.746	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
Data File : PL067797.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2021 14:54
Operator : AR\AJ
Sample : M2852-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MANHOLE-WC-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 05:47:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

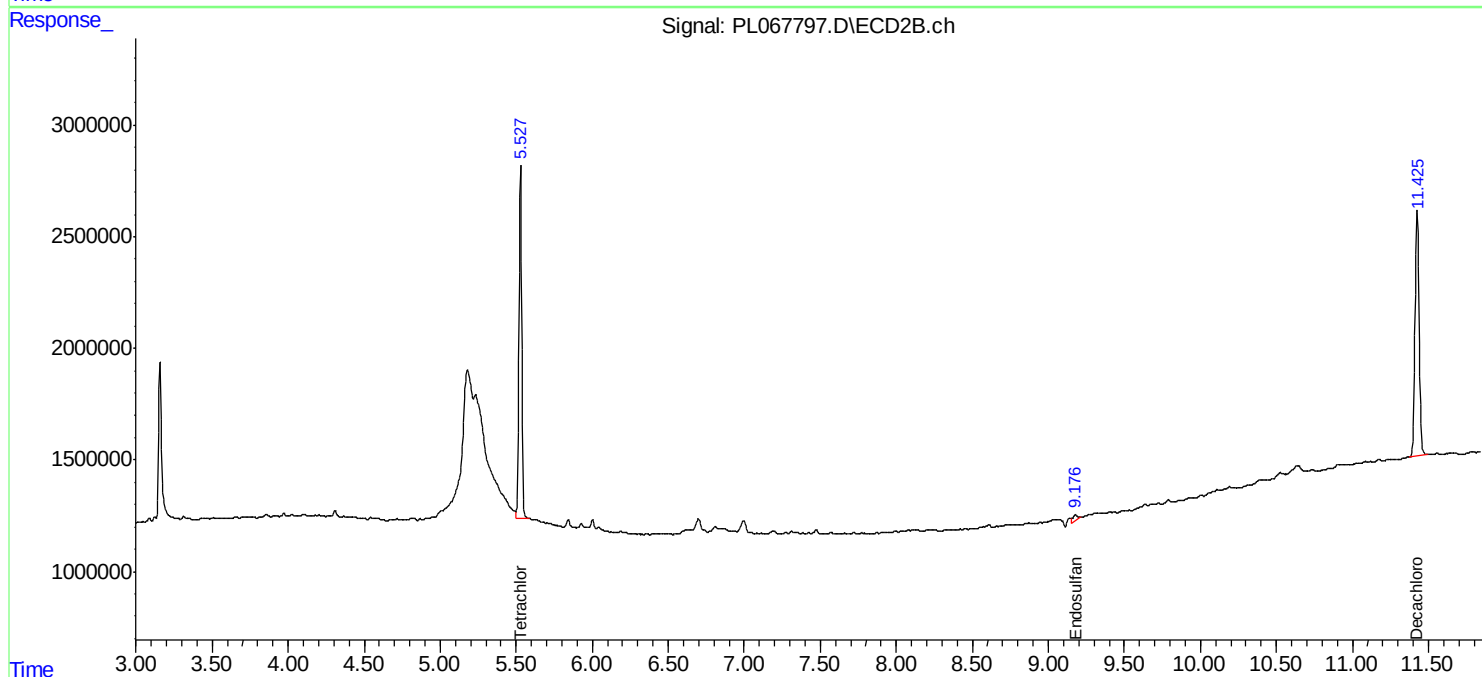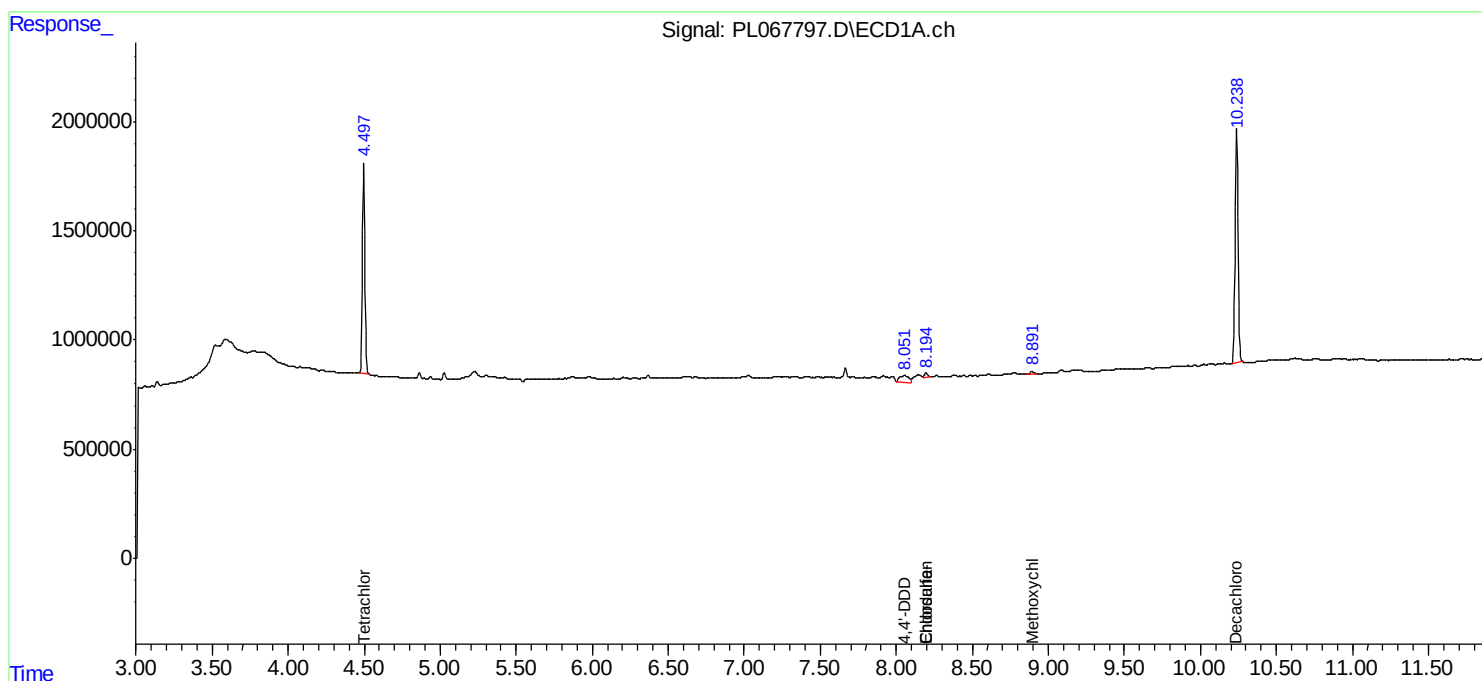


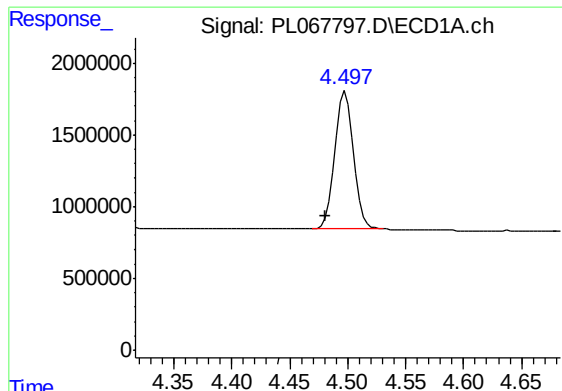

#1 Tetrachloro-m-xylene


R.T.: 4.498 min
Delta R.T.: 0.017 min
Response: 10769794
Conc: 19.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
MANHOLE-WC-D

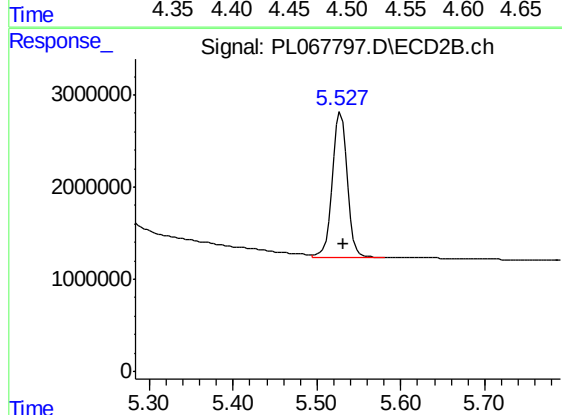


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.003 min
Response: 19545990
Conc: 20.73 ng/ml

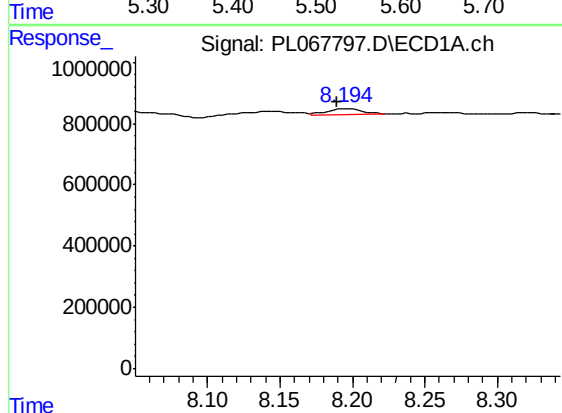


#15 Endosulfan II

R.T.: 8.196 min
Delta R.T.: 0.006 min
Response: 300748
Conc: 0.49 ng/ml

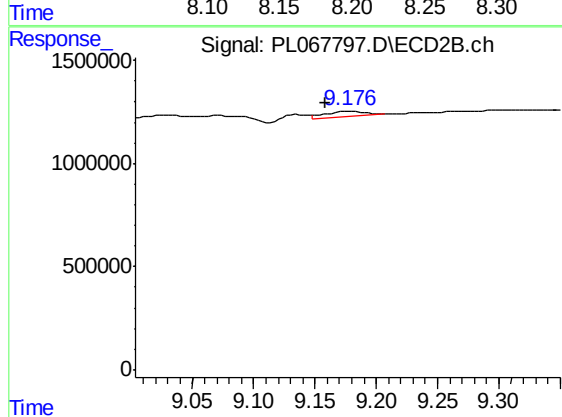

#15 Endosulfan II


R.T.: 9.177 min
Delta R.T.: 0.019 min
Response: 581930
Conc: 0.73 ng/ml

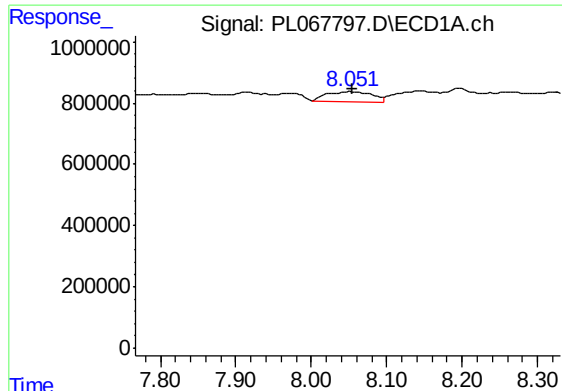

#16 4,4'-DDD


R.T.: 8.053 min
Delta R.T.: -0.002 min
Response: 1290649
Conc: 2.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
MANHOLE-WC-D

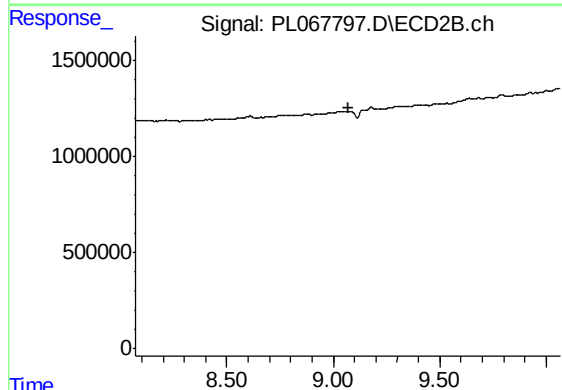


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 9.069 min
Response: 0
Conc: N.D.

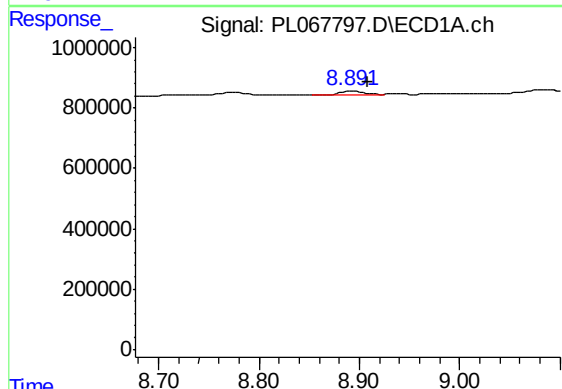


#20 Methoxychlor

R.T.: 8.892 min
Delta R.T.: -0.015 min
Response: 172156
Conc: 0.48 ng/ml

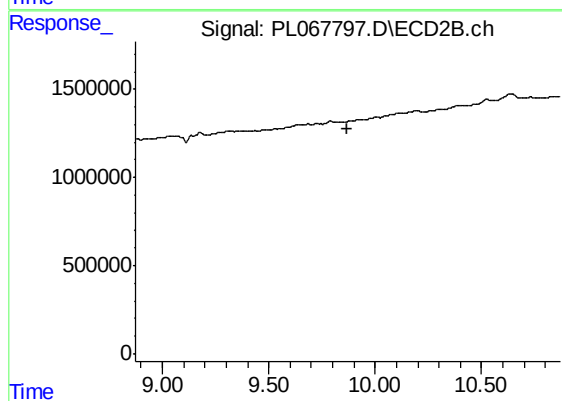

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 9.872 min
Response: 0
Conc: N.D.

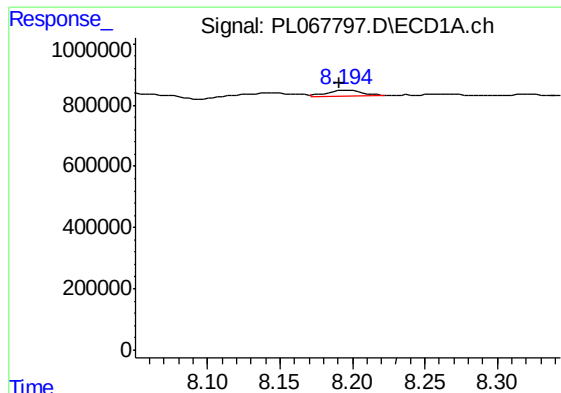

#27 Chlordane-5


R.T.: 8.196 min
Delta R.T.: 0.005 min
Response: 300748
Conc: 13.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
MANHOLE-WC-D

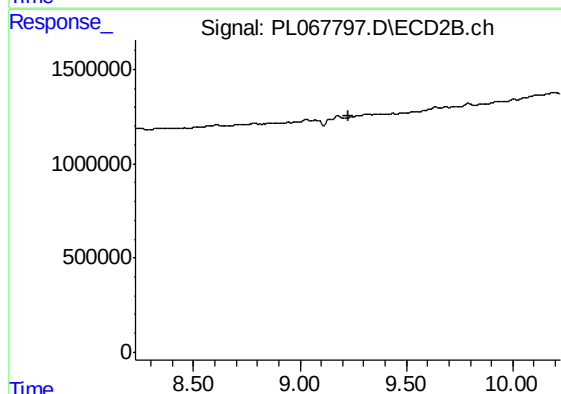


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

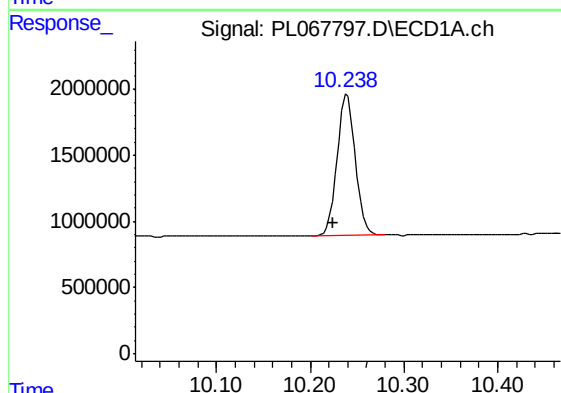

#28 Decachlorobiphenyl

R.T.: 10.240 min
Delta R.T.: 0.015 min
Response: 14431262
Conc: 20.36 ng/ml

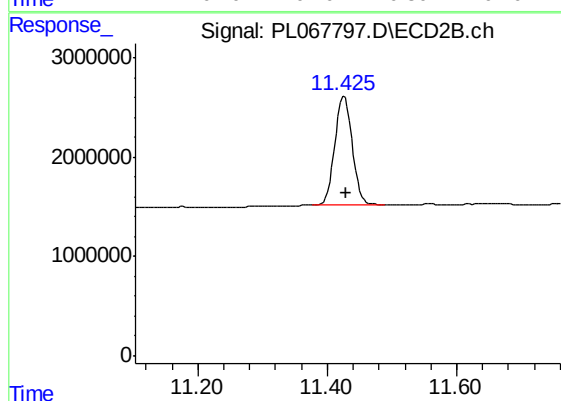

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 20345228
Conc: 20.43 ng/ml