

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
 Data File : PL067814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2021 19:36
 Operator : AR\AJ
 Sample : M2829-12
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 15B-DUP-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 05:53:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.476	5.527	10232169	19813785	18.611	21.017
28)	SA Decachlor...	10.216	11.420	11555088	17308641	16.305	17.377
Target Compounds							
2)	A alpha-BHC	0.000	6.085f	0	560156	N.D.	0.453 #
5)	MB Aldrin	6.334	0.000	761760	0	1.035	N.D. #
6)	B beta-BHC	5.959f	0.000	255153	0	0.713	N.D. #
7)	B delta-BHC	0.000	7.002f	0	1881842	N.D.	1.601 #
8)	B Heptachlo...	0.000	7.967f	0	250565	N.D.	0.250 #
11)	B alpha-Chl...	7.248	0.000	130684	0	0.179	N.D. #
15)	B Endosulfa...	0.000	9.175f	0	696365	N.D.	0.873 #
16)	A 4,4'-DDD	8.026f	0.000	251060	0	0.432	N.D. #
18)	B Endrin al...	0.000	9.307	0	140068	N.D.	0.219 #
26)	Chlordane-4	7.248	0.000	130684	0	1.788	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
Data File : PL067814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2021 19:36
Operator : AR\AJ
Sample : M2829-12
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
15B-DUP-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 05:53:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

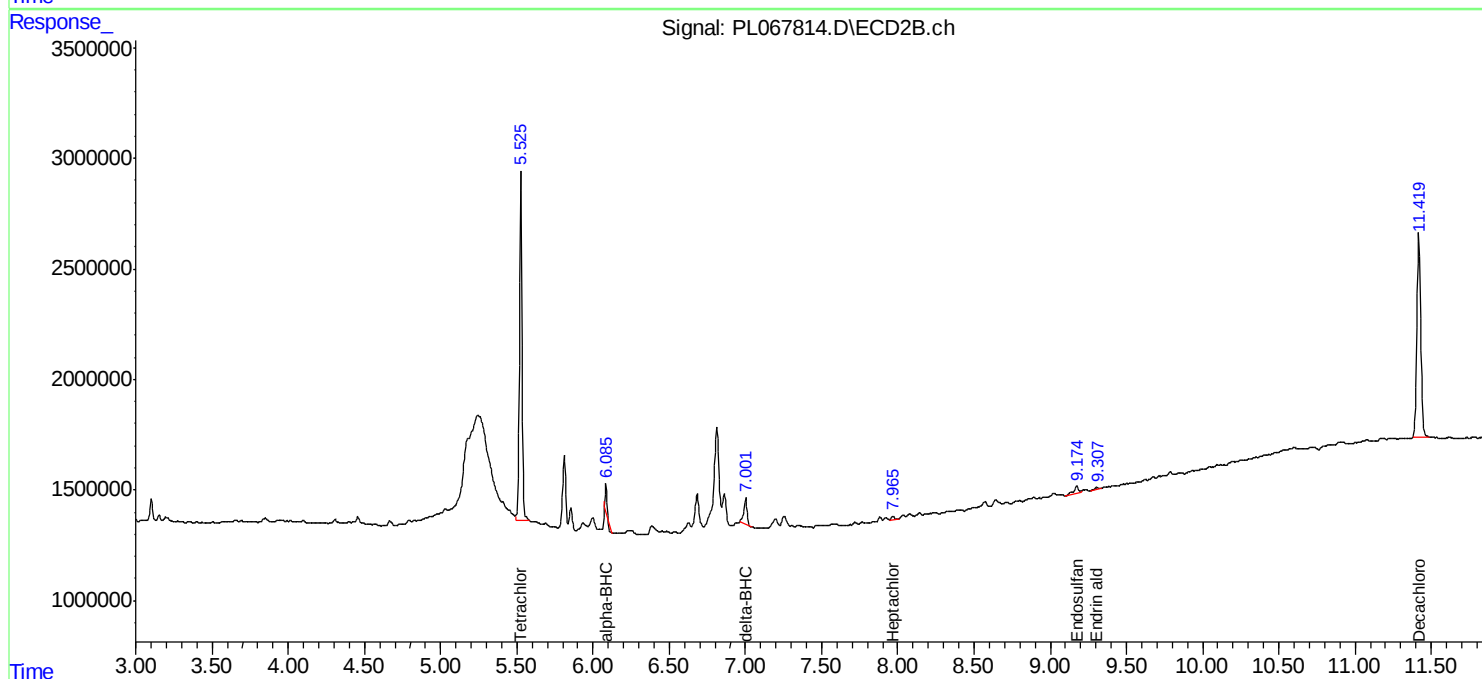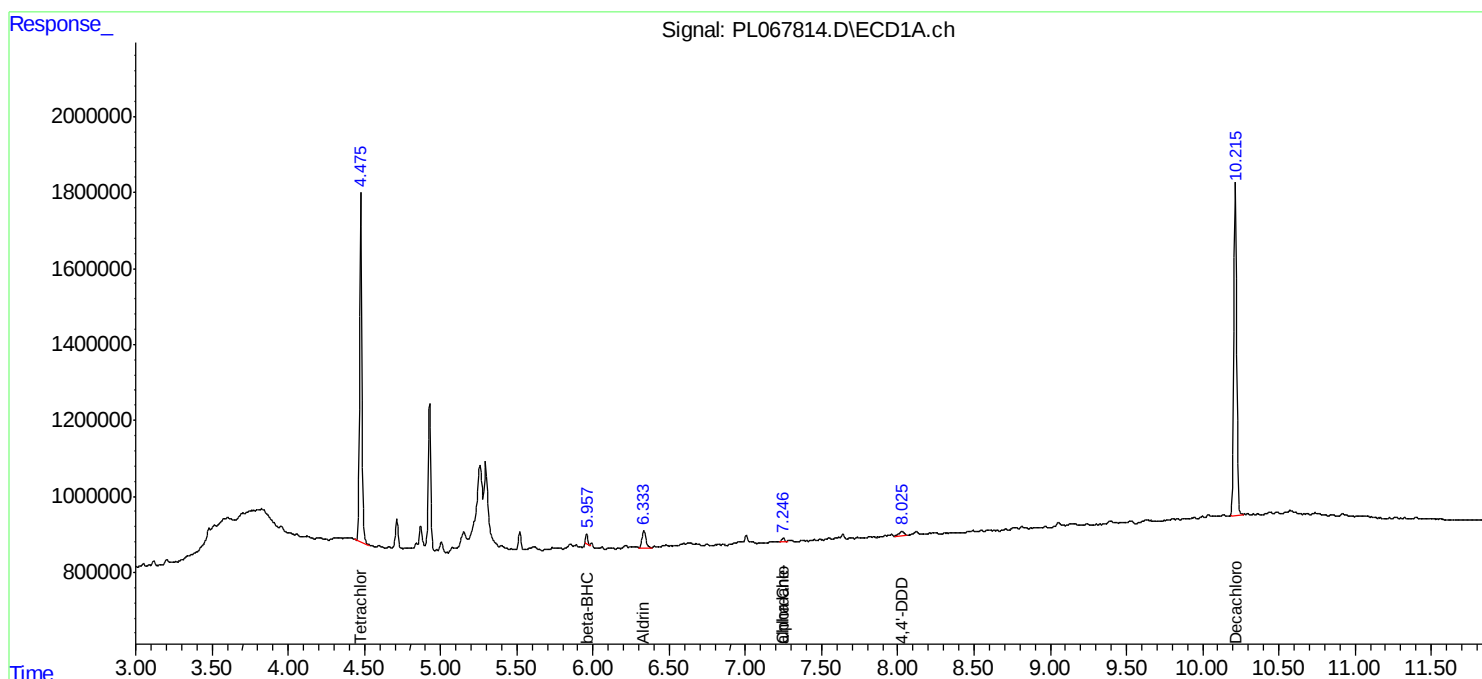


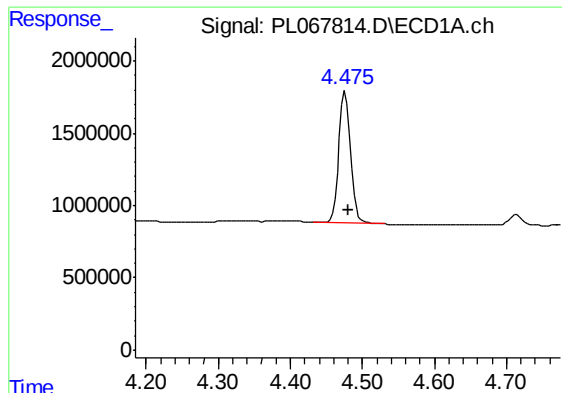

#1 Tetrachloro-m-xylene


R.T.: 4.476 min
Delta R.T.: -0.005 min
Response: 10232169
Conc: 18.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
15B-DUP-01

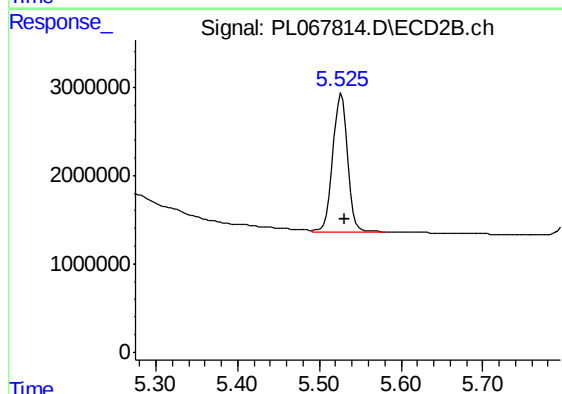


#1 Tetrachloro-m-xylene

R.T.: 5.527 min
Delta R.T.: -0.004 min
Response: 19813785
Conc: 21.02 ng/ml

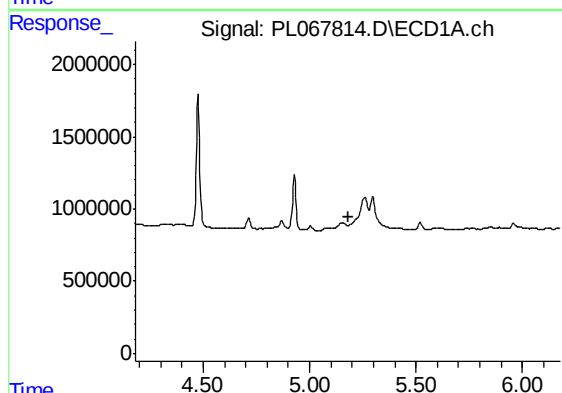


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.181 min
Response: 0
Conc: N.D.

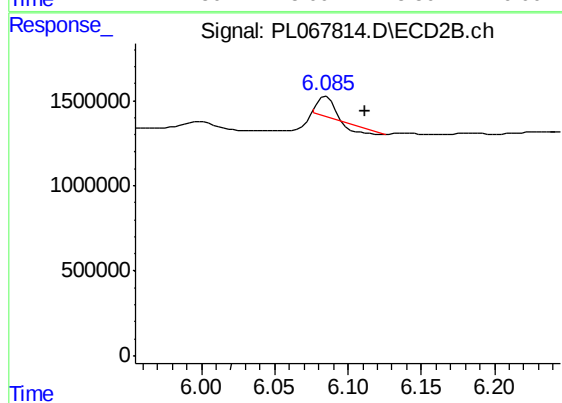

#2 alpha-BHC


R.T.: 6.085 min
Delta R.T.: -0.026 min
Response: 560156
Conc: 0.45 ng/ml

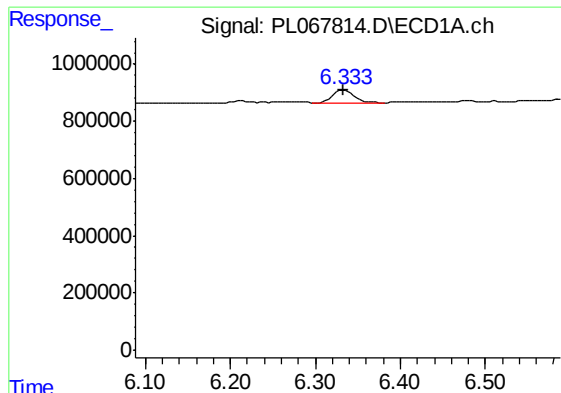

#5 Aldrin


R.T.: 6.334 min
Delta R.T.: 0.000 min
Response: 761760
Conc: 1.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
15B-DUP-01

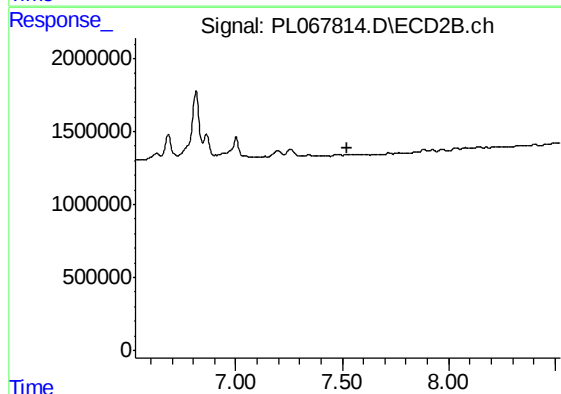


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.525 min
Response: 0
Conc: N.D.

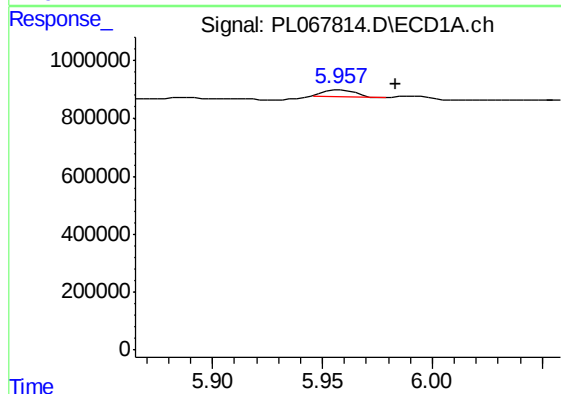


#6 beta-BHC

R.T.: 5.959 min
Delta R.T.: -0.025 min
Response: 255153
Conc: 0.71 ng/ml

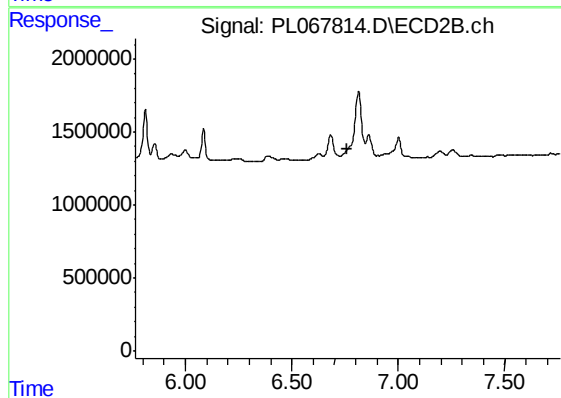

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

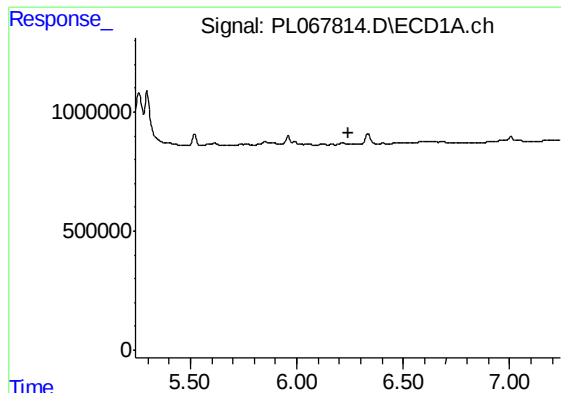

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
15B-DUP-01

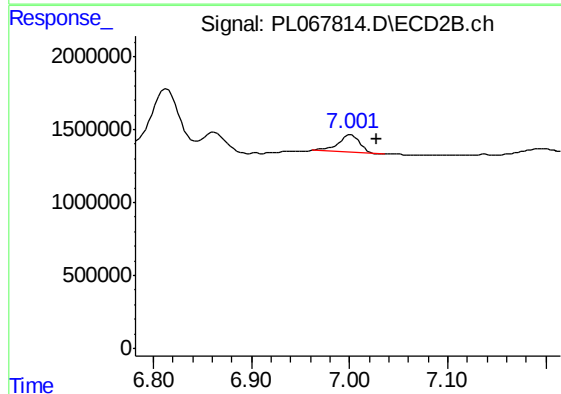


#7 delta-BHC

R.T.: 7.002 min
Delta R.T.: -0.026 min
Response: 1881842
Conc: 1.60 ng/ml

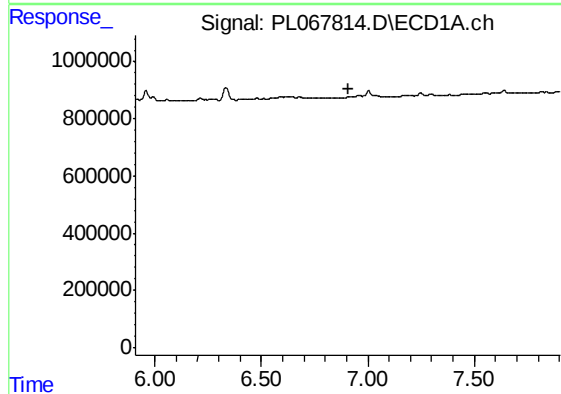


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

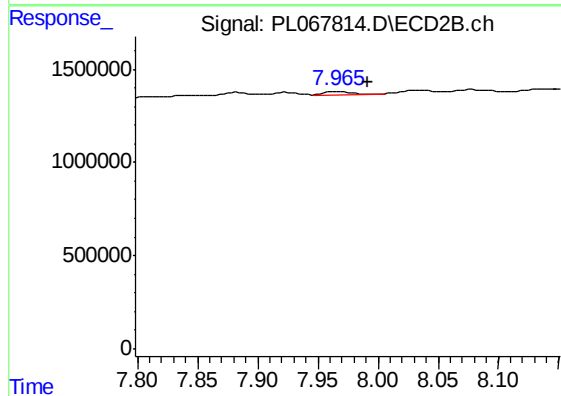

#8 Heptachlor epoxide


R.T.: 7.967 min
Delta R.T.: -0.025 min
Response: 250565
Conc: 0.25 ng/ml

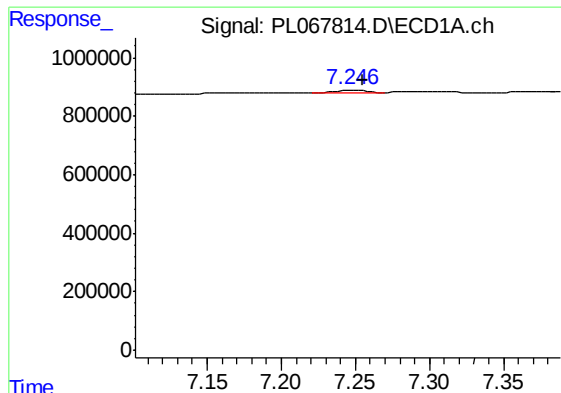

#11 alpha-Chlordane


R.T.: 7.248 min
Delta R.T.: -0.006 min
Response: 130684
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
15B-DUP-01

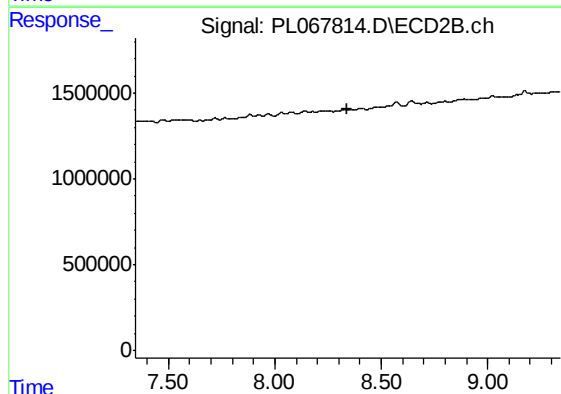


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

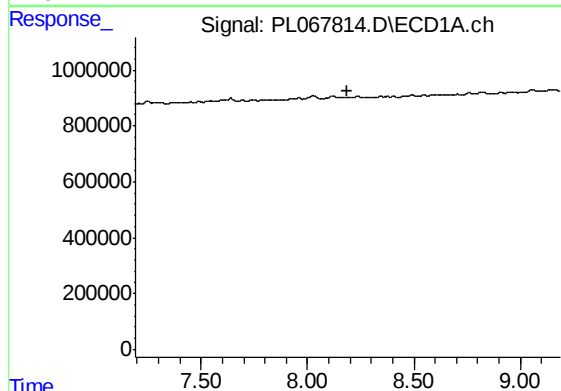


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

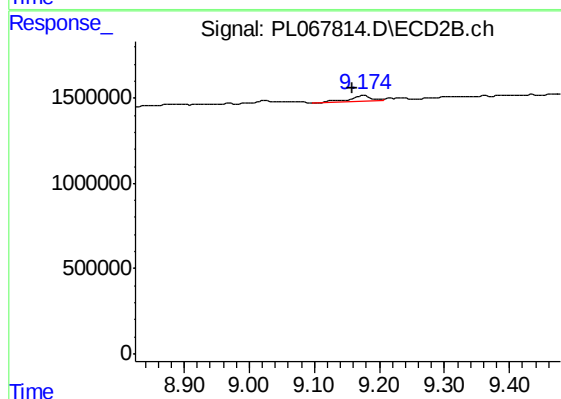

#15 Endosulfan II


R.T.: 9.175 min
Delta R.T.: 0.017 min
Response: 696365
Conc: 0.87 ng/ml

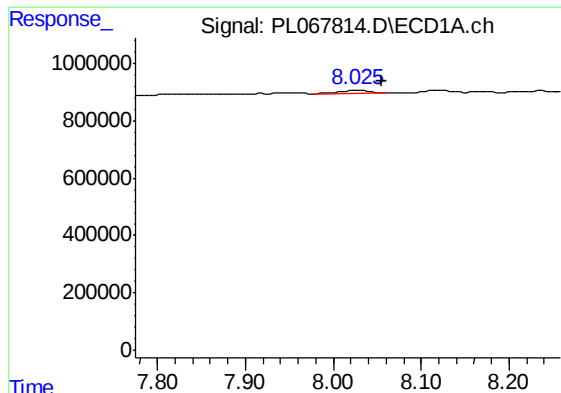

#16 4,4'-DDD


R.T.: 8.026 min
Delta R.T.: -0.029 min
Response: 251060
Conc: 0.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
15B-DUP-01

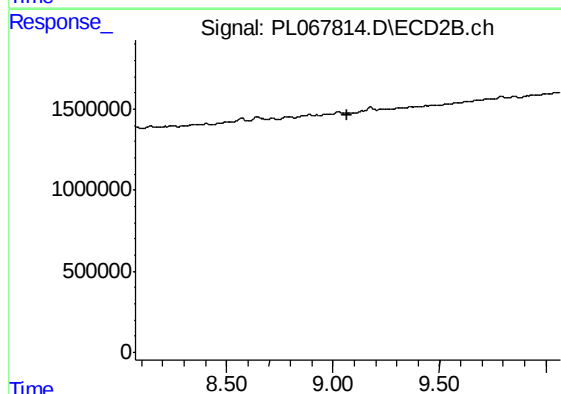


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 9.069 min
Response: 0
Conc: N.D.

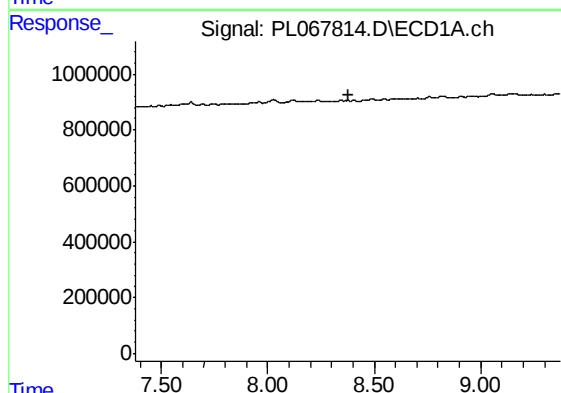


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 8.377 min
Response: 0
Conc: N.D.

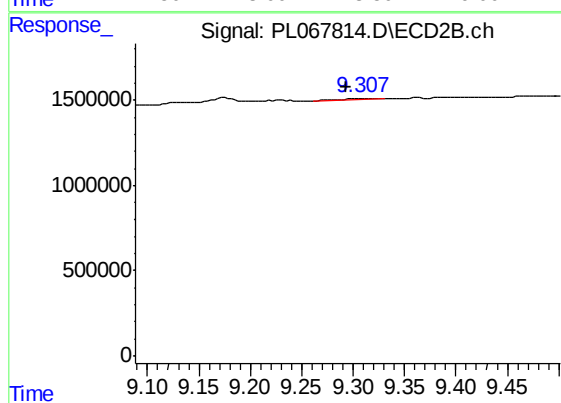

#18 Endrin aldehyde


R.T.: 9.307 min
Delta R.T.: 0.014 min
Response: 140068
Conc: 0.22 ng/ml

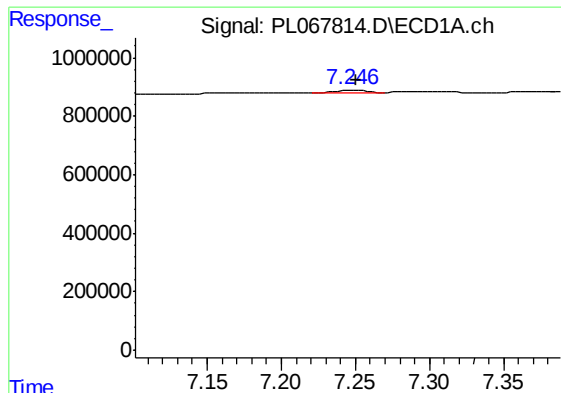

#26 Chlordane-4


R.T.: 7.248 min
Delta R.T.: -0.002 min
Response: 130684
Conc: 1.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
15B-DUP-01

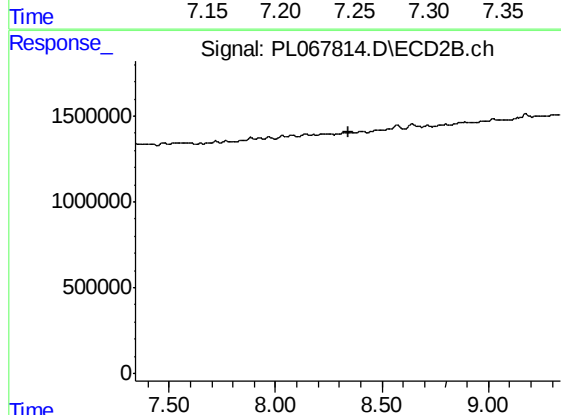


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.341 min
Response: 0
Conc: N.D.

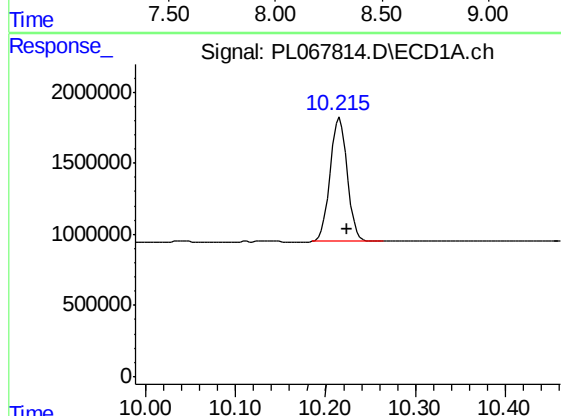

#28 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: -0.009 min
Response: 11555088
Conc: 16.30 ng/ml

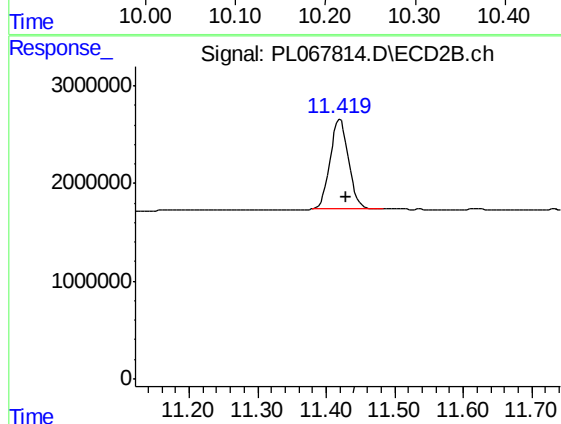

#28 Decachlorobiphenyl

R.T.: 11.420 min
Delta R.T.: -0.008 min
Response: 17308641
Conc: 17.38 ng/ml