

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
 Data File : PL067824.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2021 22:22
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 05:56:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.477	5.527	10923778	20713161	19.869	21.971
28)	SA Decachlor...	10.215	11.420	13640423	20789853	19.248	20.872
Target Compounds							
4)	MA Heptachlor	5.985f	0.000	649107	0	0.861	N.D. #
6)	B beta-BHC	5.985	0.000	649107	0	1.814	N.D. #
14)	MA Endrin	7.891	0.000	281466	0	0.429	N.D. #
15)	B Endosulfa...	0.000	9.175f	0	407086	N.D.	0.511 #
16)	A 4,4'-DDD	8.027f	0.000	278062	0	0.478	N.D. #
24)	Chlordane-2	6.483	0.000	641410	0	23.953	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
Data File : PL067824.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2021 22:22
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 05:56:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

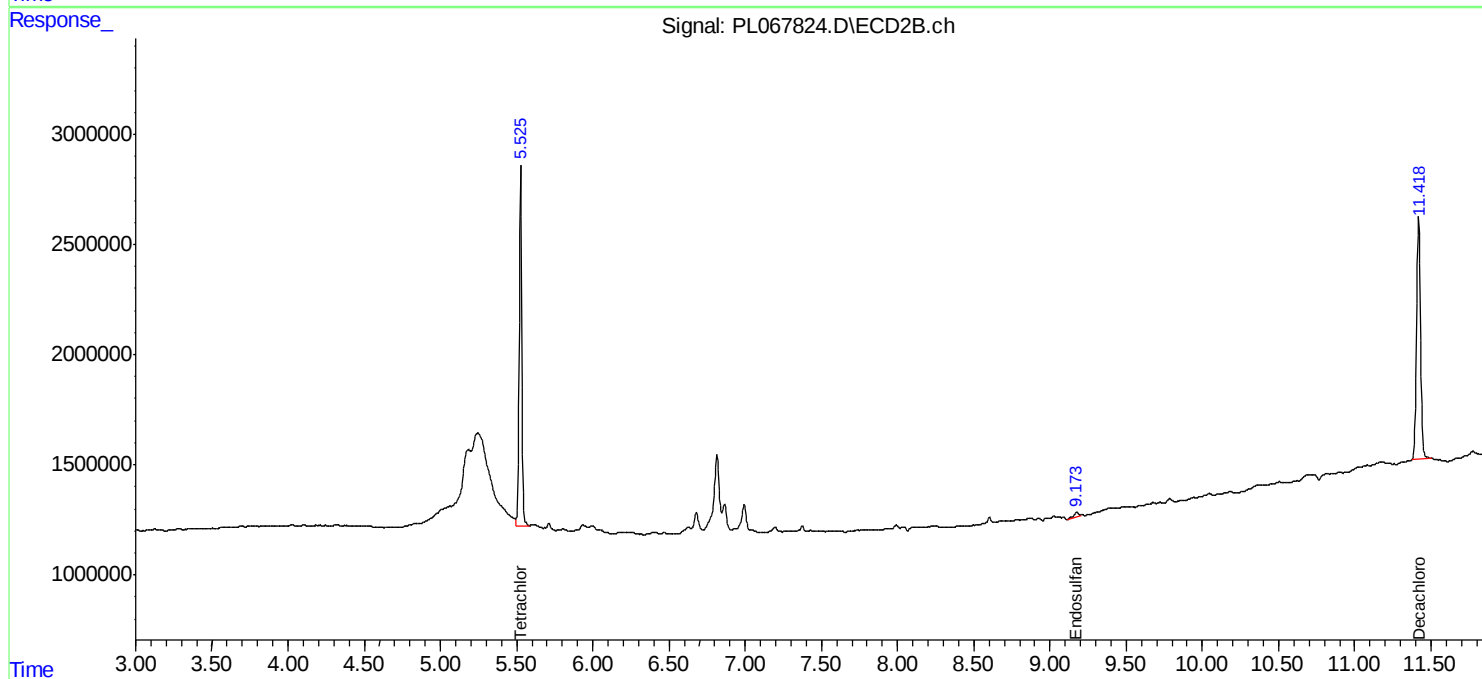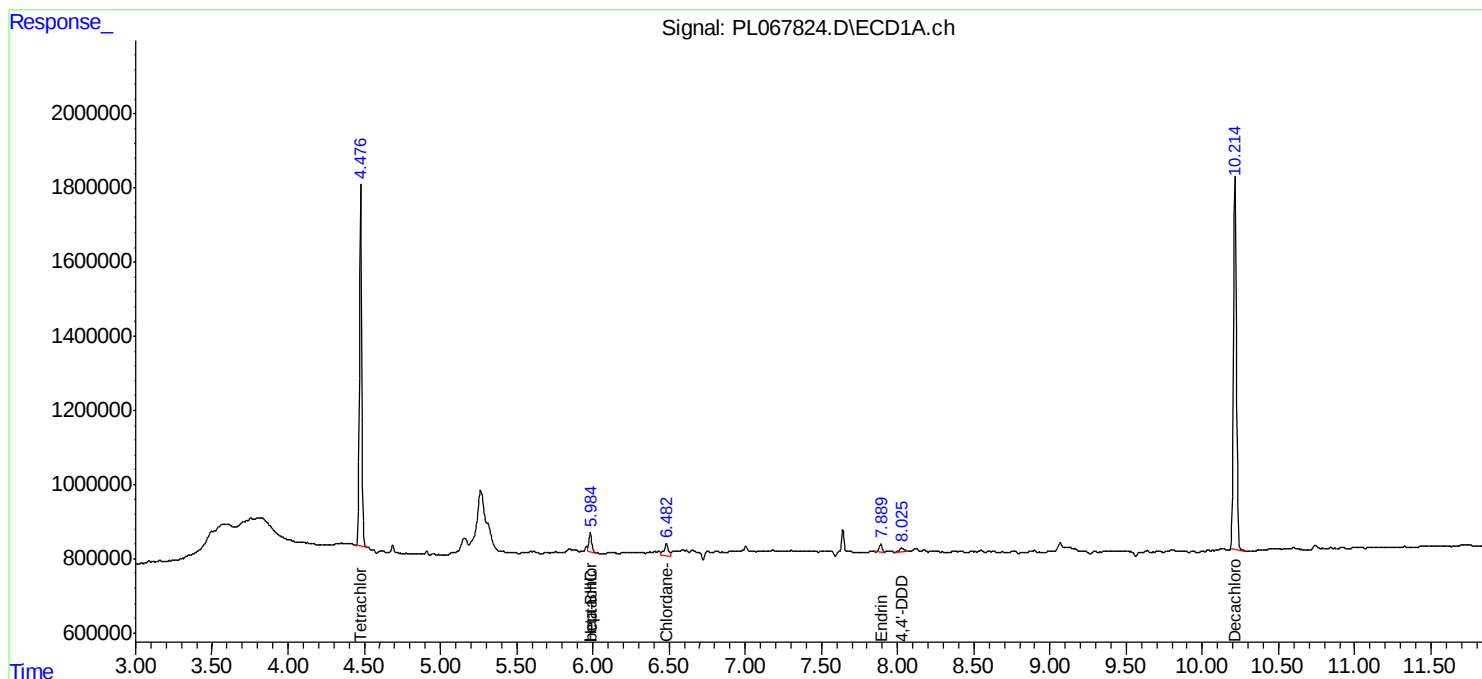


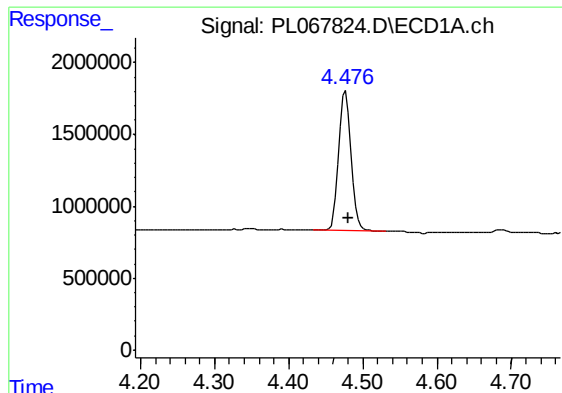

#1 Tetrachloro-m-xylene


R.T.: 4.477 min
Delta R.T.: -0.004 min
Response: 10923778
Conc: 19.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

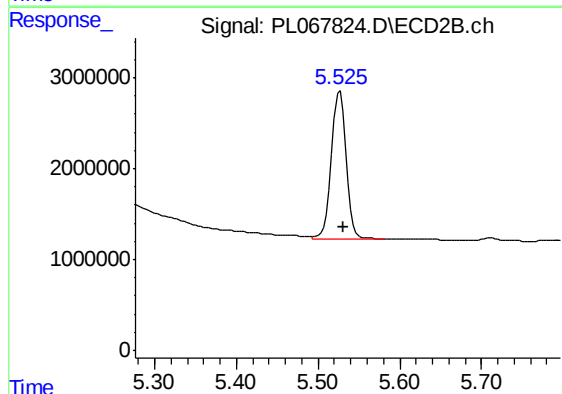


#1 Tetrachloro-m-xylene

R.T.: 5.527 min
Delta R.T.: -0.004 min
Response: 20713161
Conc: 21.97 ng/ml

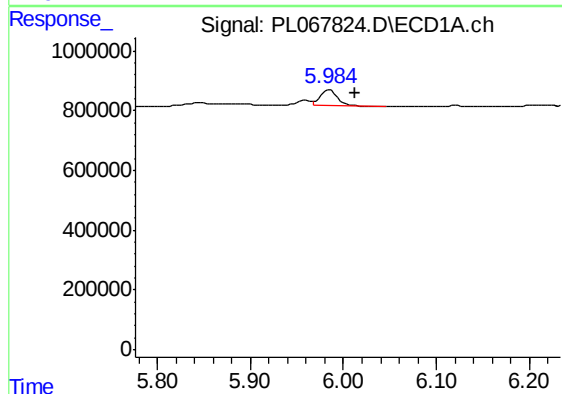


#4 Heptachlor

R.T.: 5.985 min
Delta R.T.: -0.027 min
Response: 649107
Conc: 0.86 ng/ml

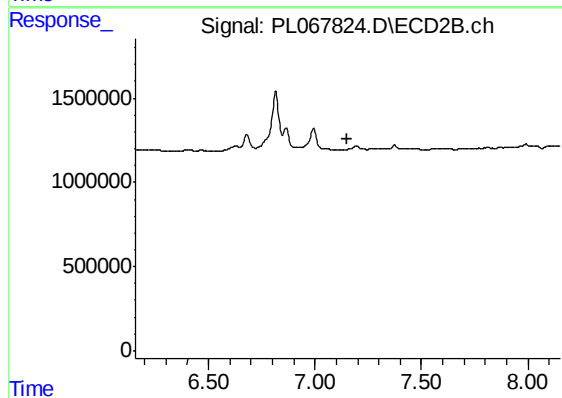

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

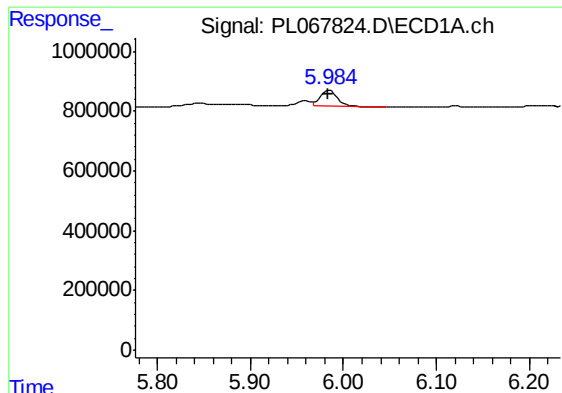

#6 beta-BHC


R.T.: 5.985 min
Delta R.T.: 0.002 min
Response: 649107
Conc: 1.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

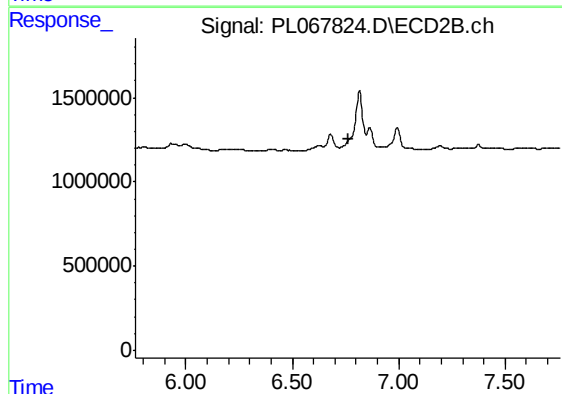


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

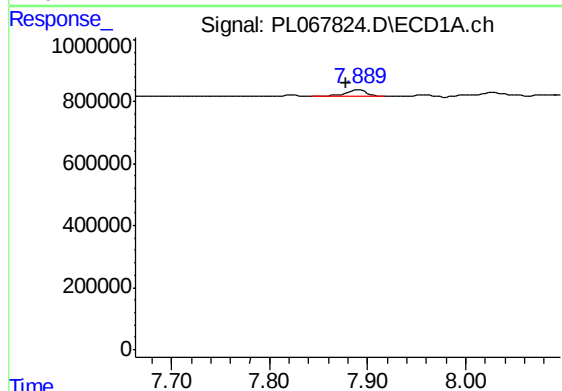


#14 Endrin

R.T.: 7.891 min
Delta R.T.: 0.012 min
Response: 281466
Conc: 0.43 ng/ml

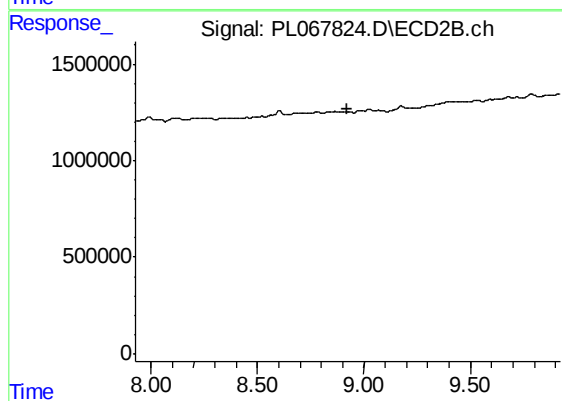

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

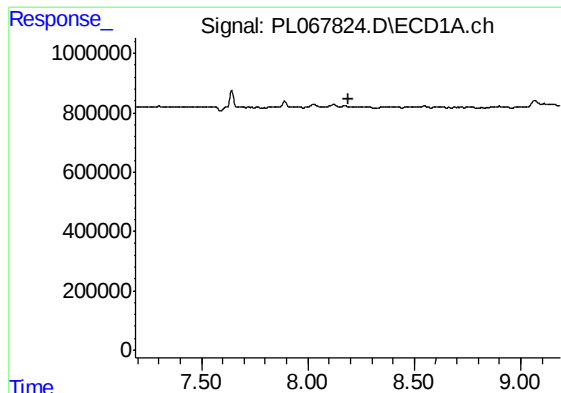

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

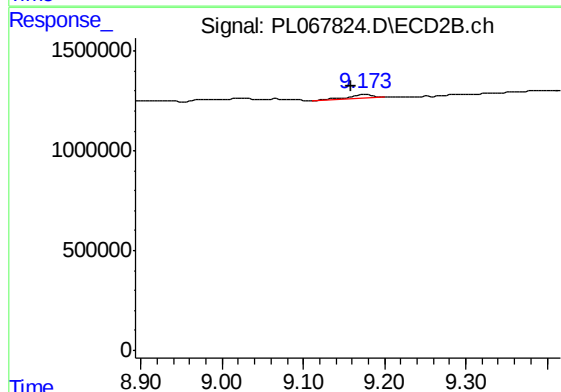


#15 Endosulfan II

R.T.: 9.175 min
Delta R.T.: 0.017 min
Response: 407086
Conc: 0.51 ng/ml

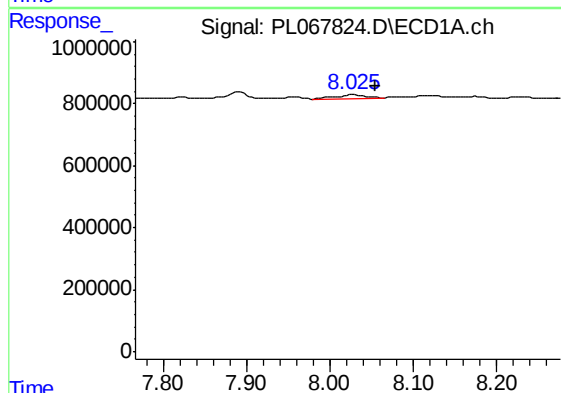


#16 4,4'-DDD

R.T.: 8.027 min
Delta R.T.: -0.028 min
Response: 278062
Conc: 0.48 ng/ml

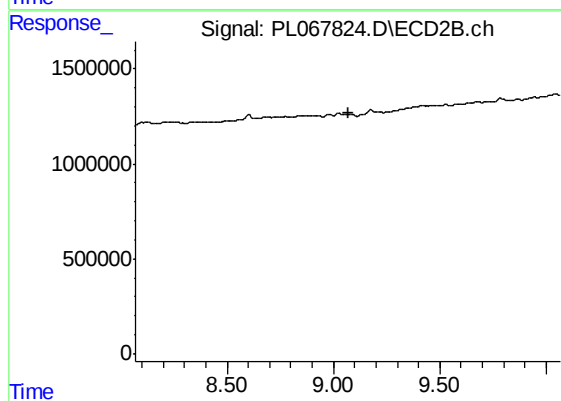

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 9.069 min
Response: 0
Conc: N.D.

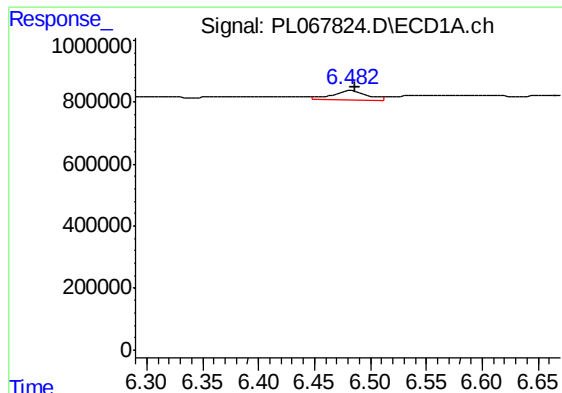

#24 Chlordane-2


R.T.: 6.483 min
Delta R.T.: -0.003 min
Response: 641410
Conc: 23.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

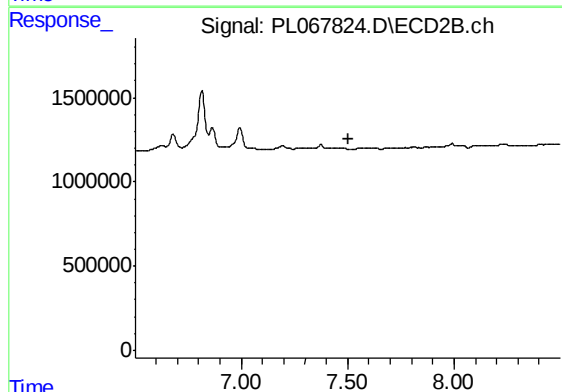


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

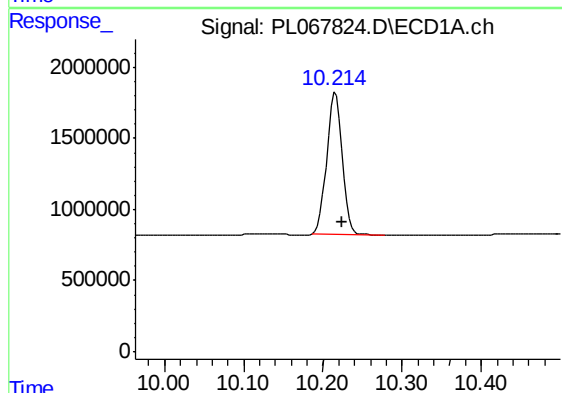

#28 Decachlorobiphenyl

R.T.: 10.215 min
Delta R.T.: -0.009 min
Response: 13640423
Conc: 19.25 ng/ml

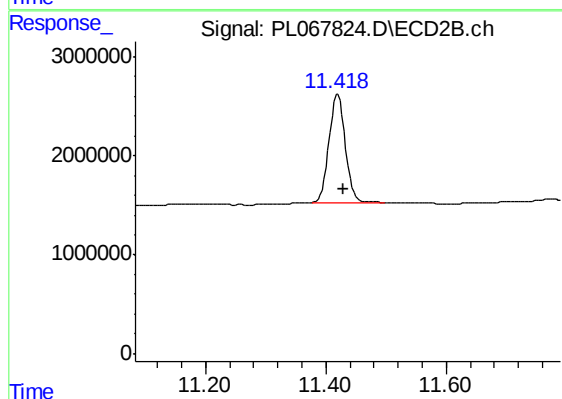

#28 Decachlorobiphenyl

R.T.: 11.420 min
Delta R.T.: -0.009 min
Response: 20789853
Conc: 20.87 ng/ml