

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
 Data File : PL067798.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2021 15:11
 Operator : AR\AJ
 Sample : M2852-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MANHOLE-WC-S

Manual Integrations
 APPROVED

Ankita
 6/28/2021 9:29:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 05:48:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	6706323	11897687	12.198m	12.620
28)	SA Decachlor...	10.220	11.427	11493081	16106925	16.217	16.171

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
Data File : PL067798.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2021 15:11
Operator : AR\AJ
Sample : M2852-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
MANHOLE-WC-S


Manual Integrations
APPROVED

Ankita
6/28/2021 9:29:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 05:48:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

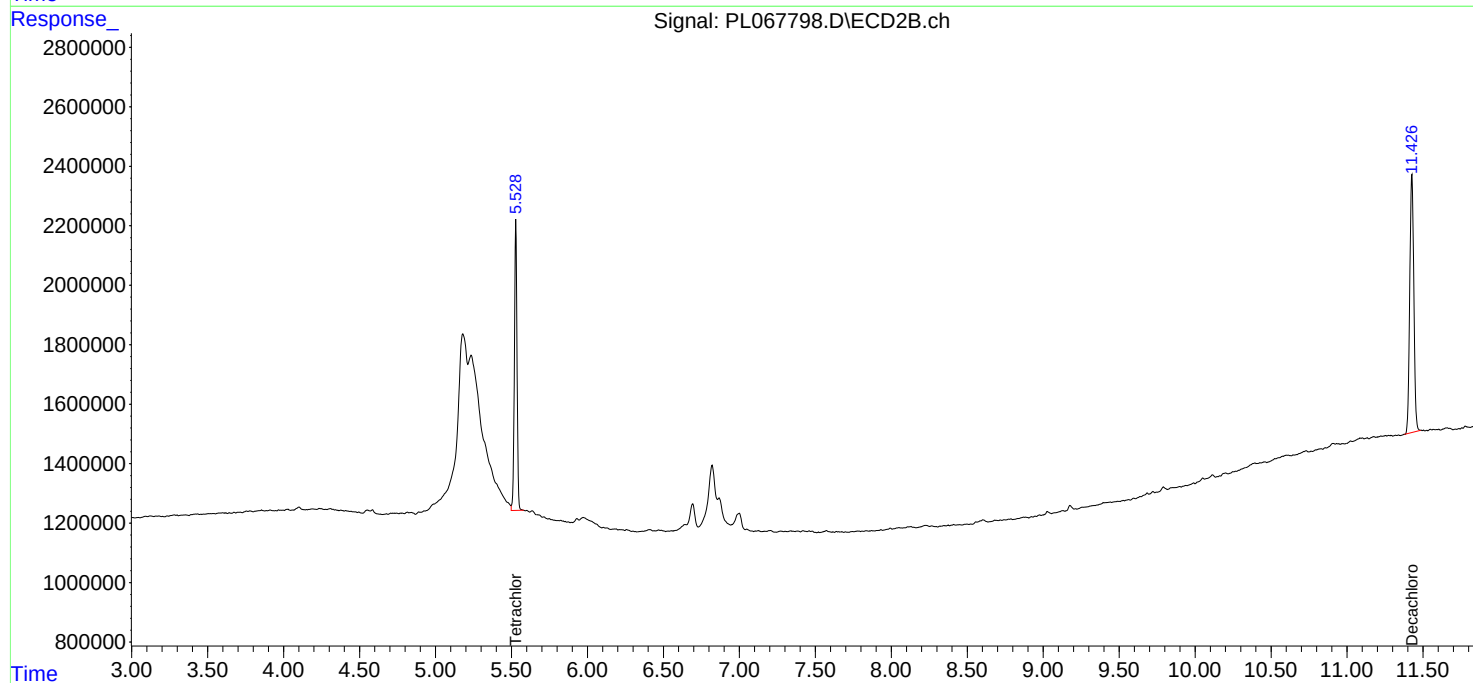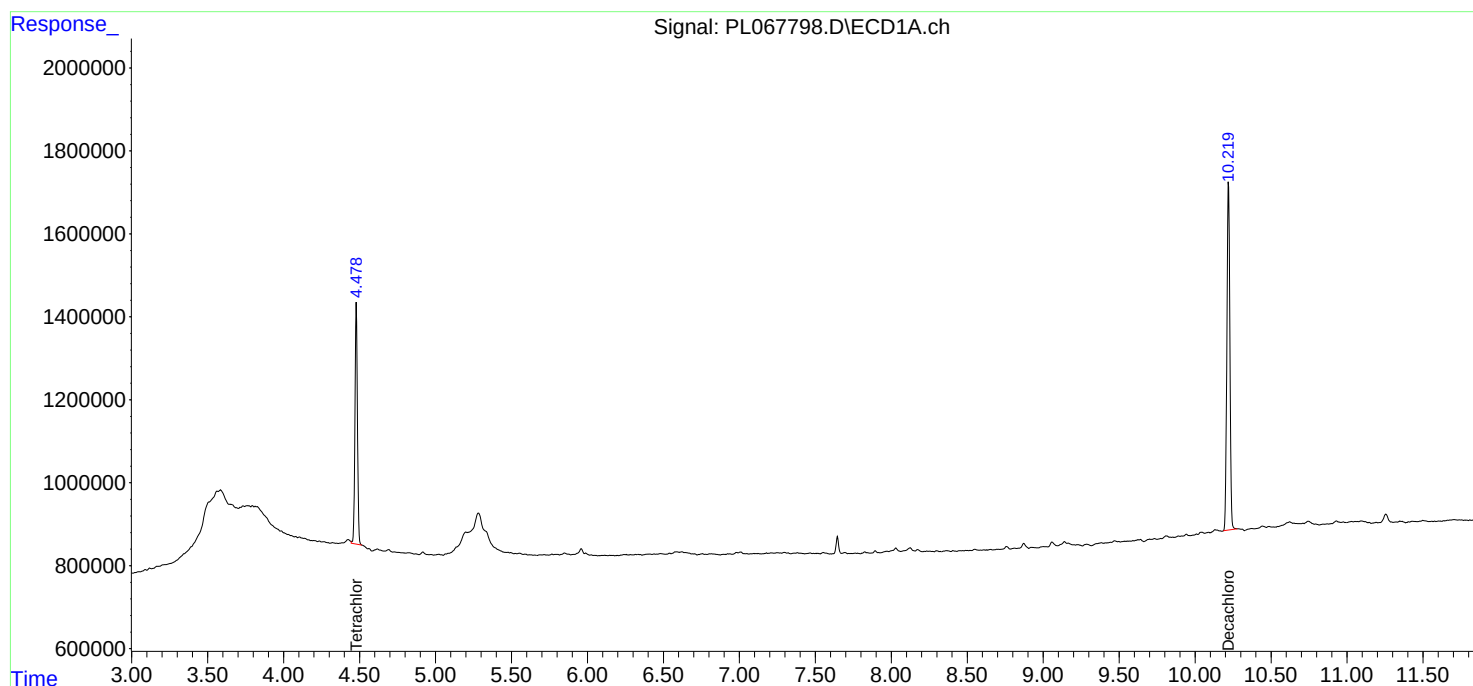

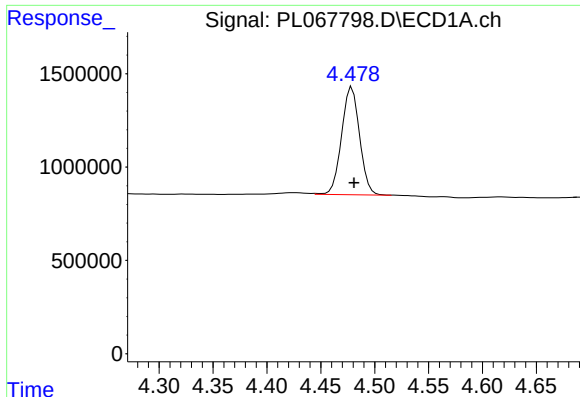


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 6706323
Conc: 12.20 ng/ml m

Instrument :
ECD_L
ClientSampleId :
MANHOLE-WC-S


Manual Integrations
APPROVED

Ankita
6/28/2021 9:29:05 AM

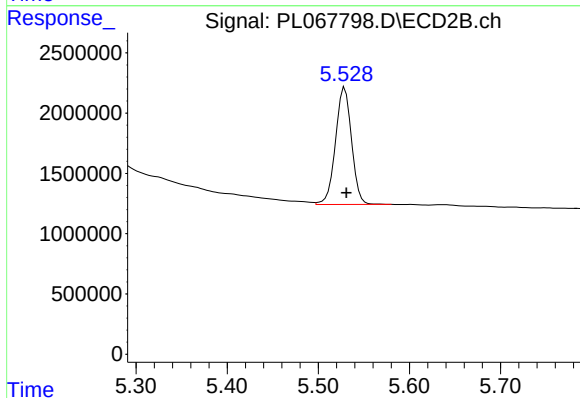


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 11897687
Conc: 12.62 ng/ml

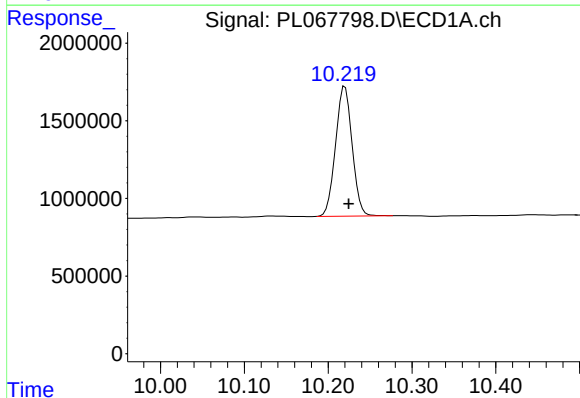

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 11493081
Conc: 16.22 ng/ml

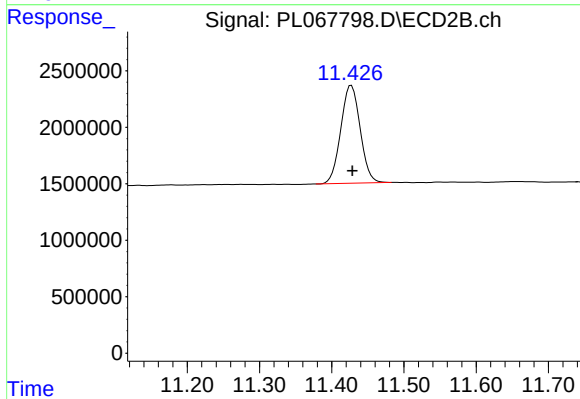

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.001 min
Response: 16106925
Conc: 16.17 ng/ml